



SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2980B 2/3 10m 800C 1h A 0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

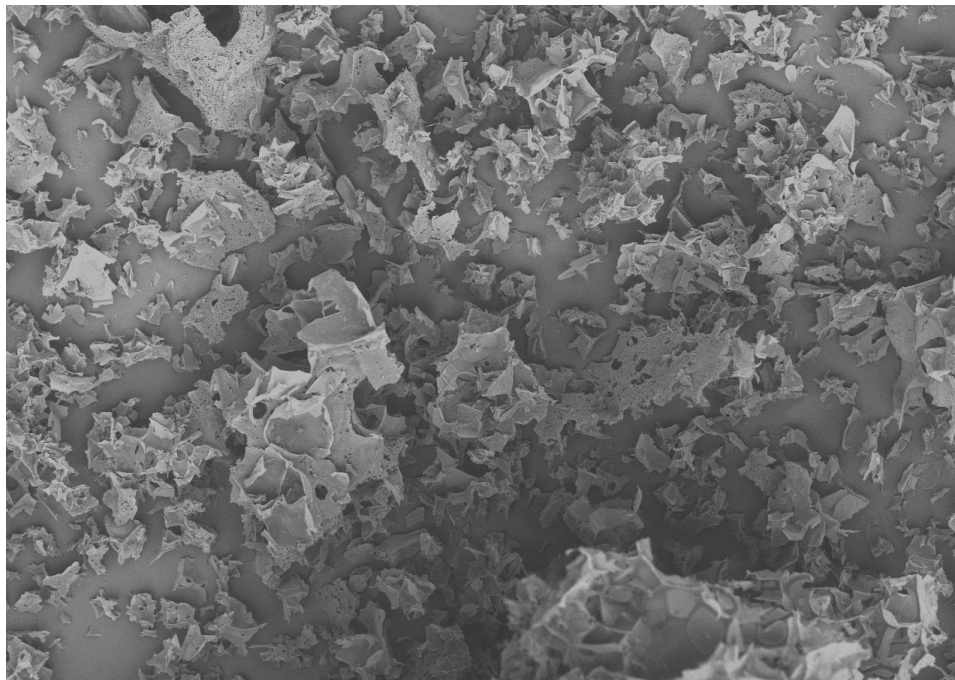

Clariant SU7000 5.00kV 6.0mm x100 UD+LD+MD 08/26/2024 500µm

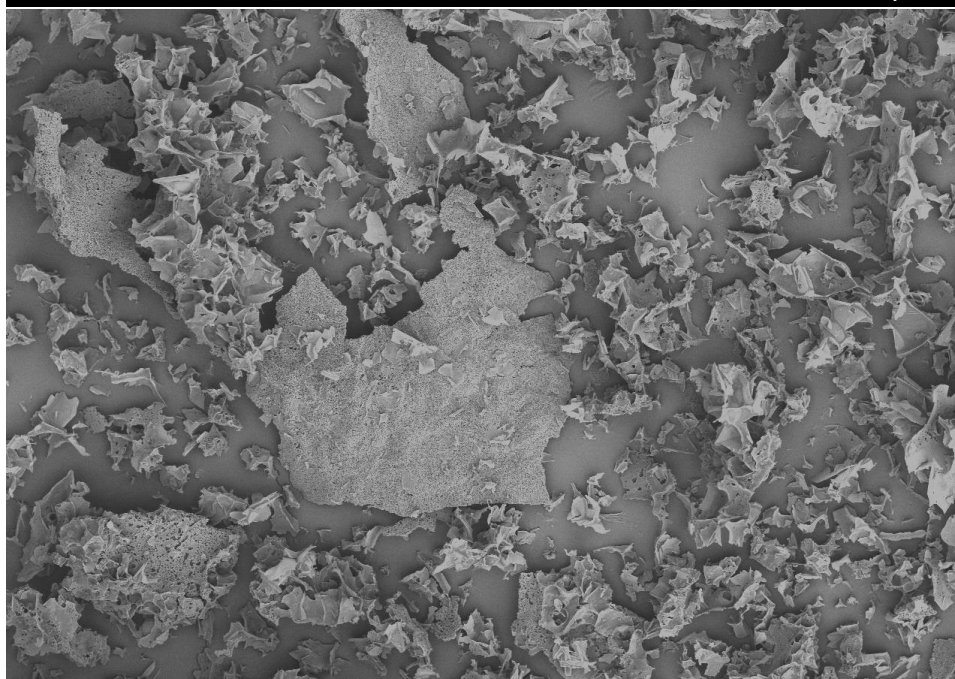

Clariant SU7000 5.00kV 6.0mm x100 UD+LD+MD 08/26/2024 500µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980B 2/3 10m 800C 1h A 0.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

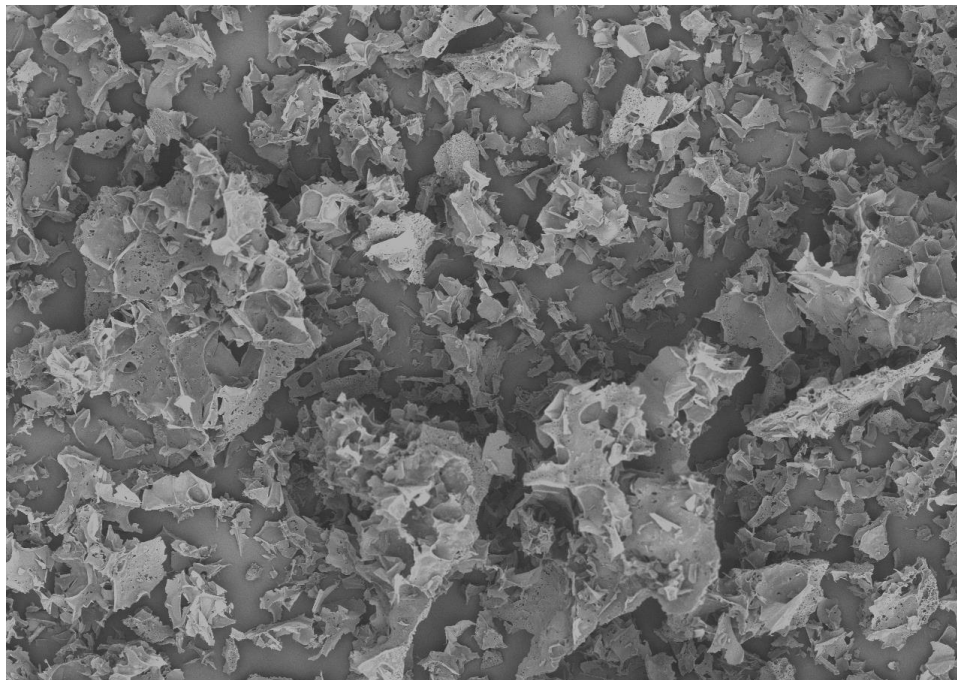

Clariant SU7000 5.00kV 6.0mm x100 UD+LD+MD 08/26/2024 500µm

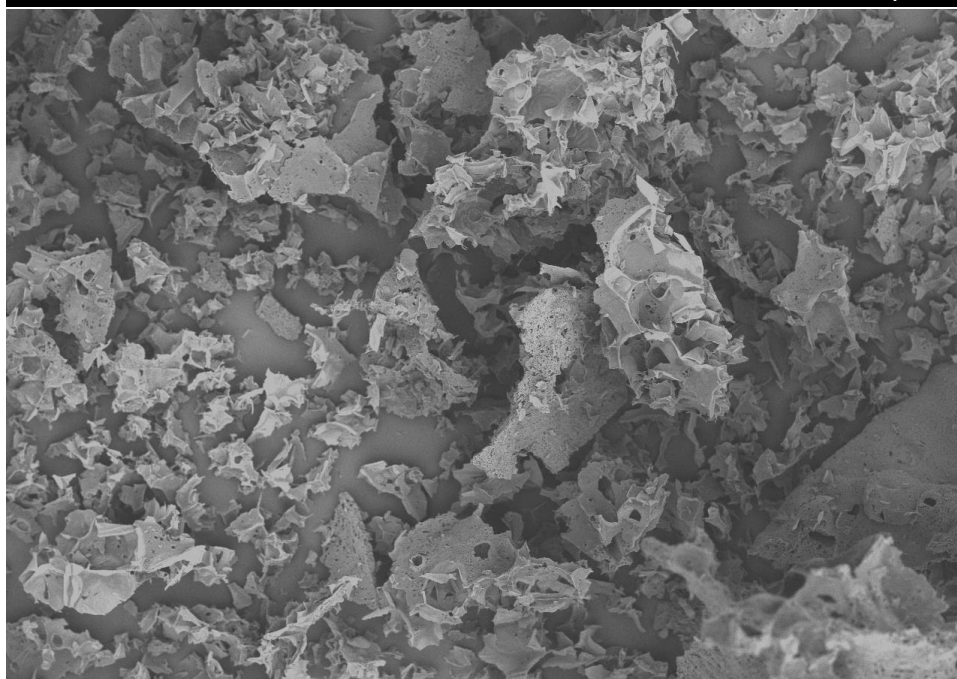


Clariant SU7000 5.00kV 5.8mm x100 UD+LD+MD 08/26/2024 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2980B 2/3 10m 800C 1h A 0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

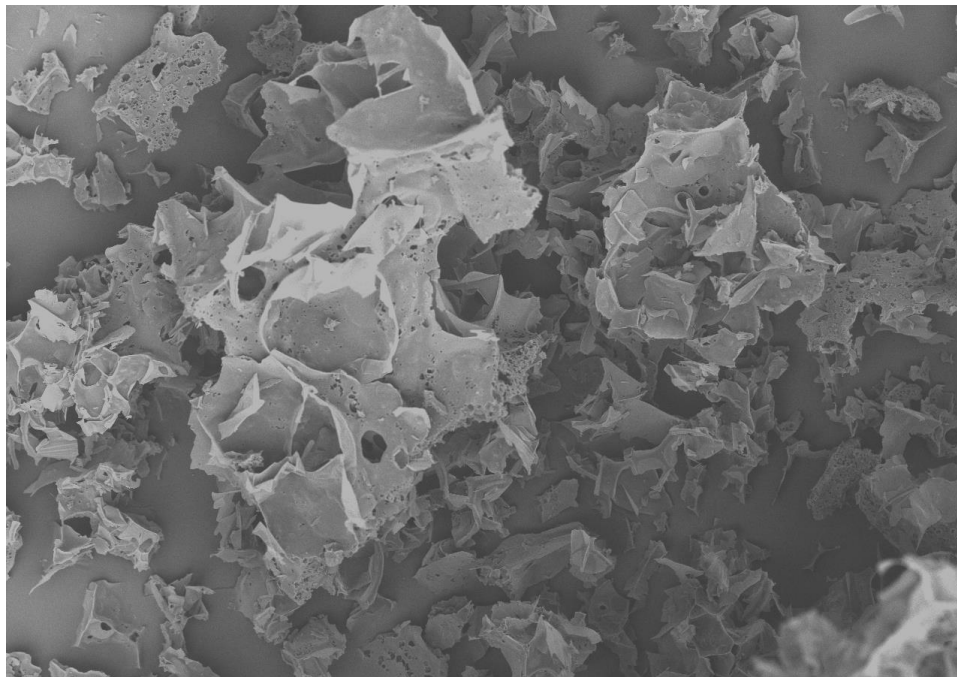

Clariant SU7000 5.00kV 6.0mm x200 UD+LD+MD 08/26/2024 200µm

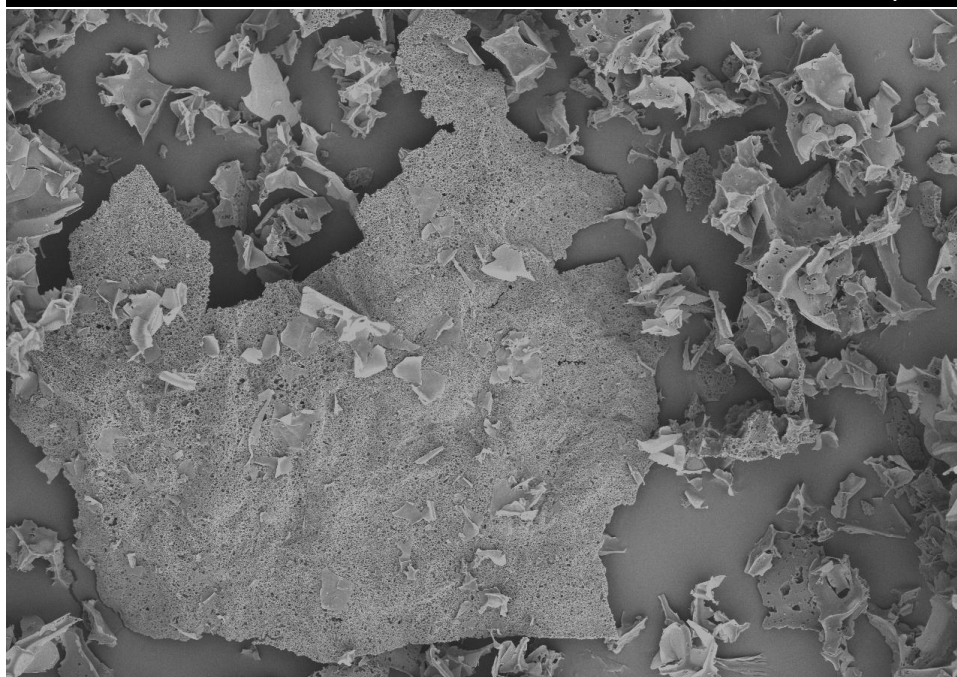

Clariant SU7000 5.00kV 6.0mm x200 UD+LD+MD 08/26/2024 200µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980B 2/3 10m 800C 1h A 0.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

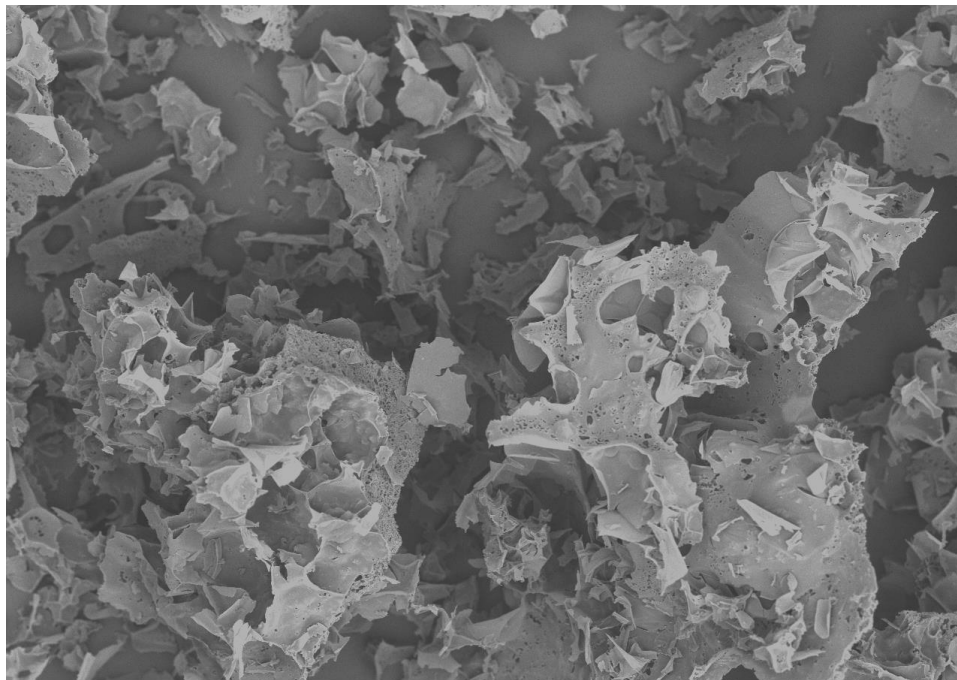

Clariant SU7000 5.00kV 5.8mm x200 UD+LD+MD 08/26/2024 200µm

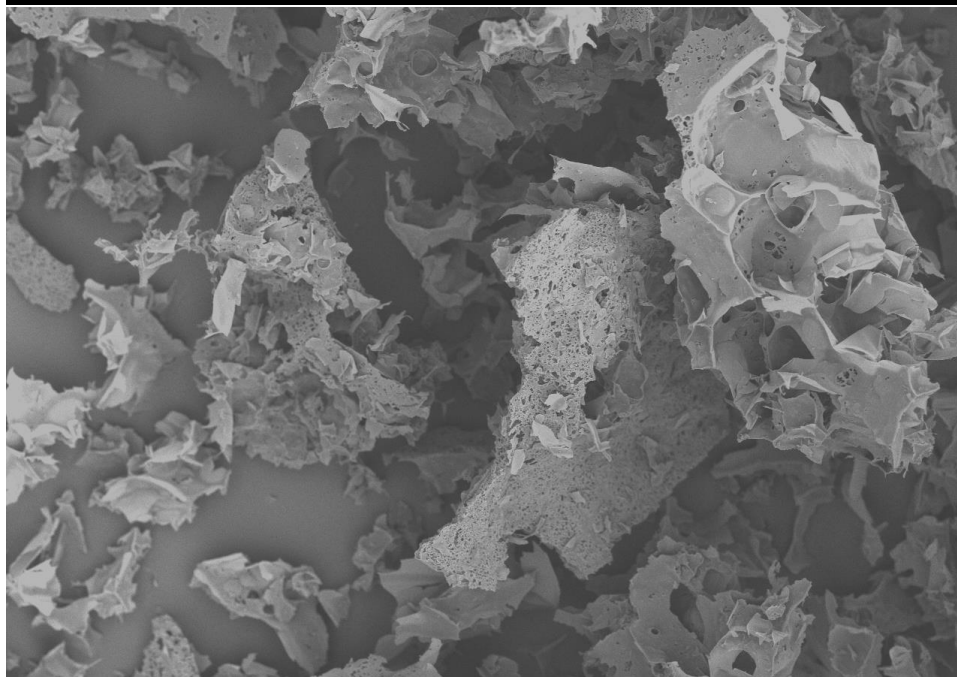

Clariant SU7000 5.00kV 5.8mm x200 UD+LD+MD 08/26/2024 200µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980B 2/3 10m 800C 1h A 0.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

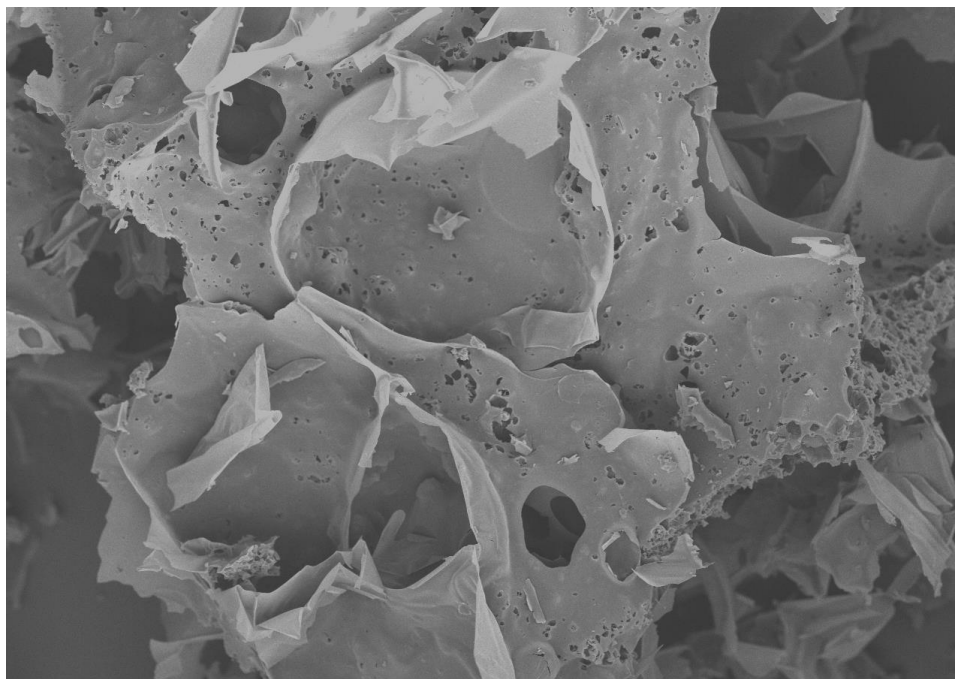

Clariant SU7000 5.00kV 5.9mm x500 UD+LD+MD 08/26/2024 100µm

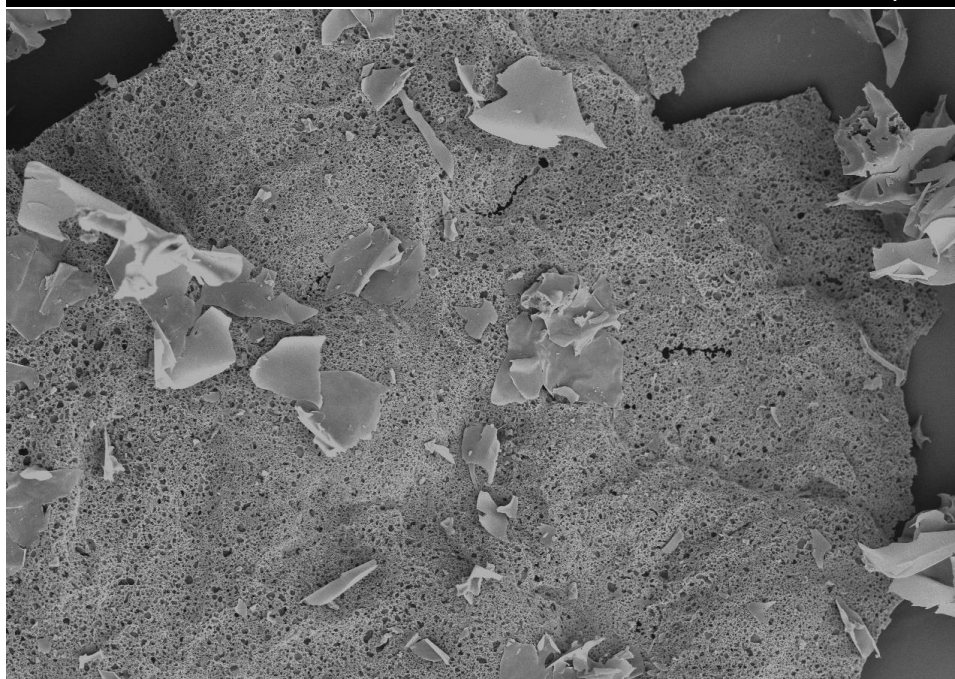


Clariant SU7000 5.00kV 6.0mm x500 UD+LD+MD 08/26/2024 100µm

SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2980B 2/3 10m 800C 1h A 0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

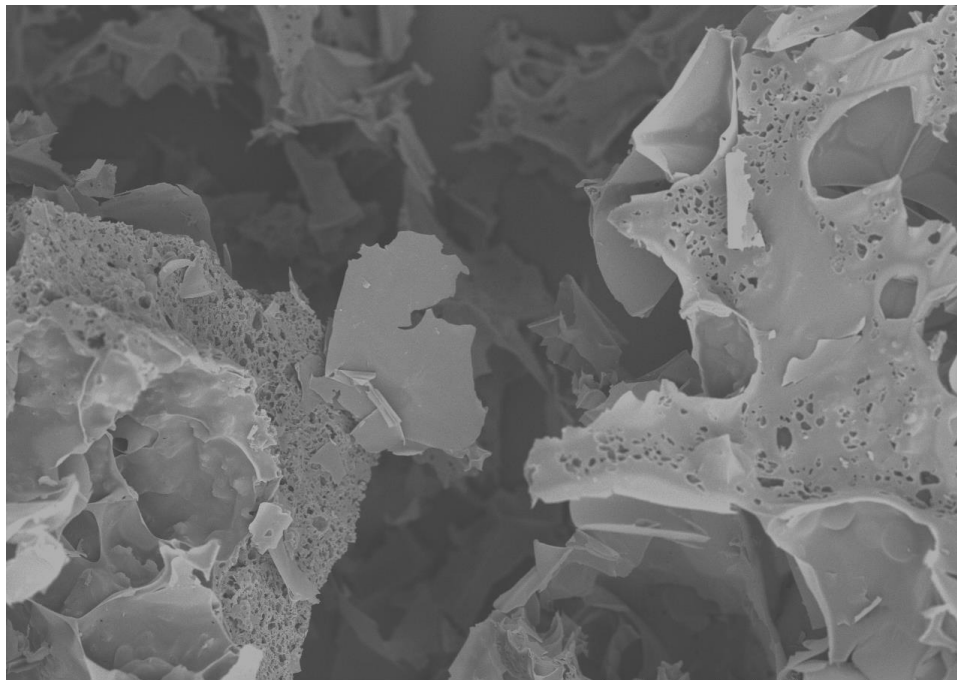

Clariant SU7000 5.00kV 5.8mm x500 UD+LD+MD 08/26/2024 100µm



Clariant SU7000 5.00kV 5.8mm x500 UD+LD+MD 08/26/2024 100µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980B 2/3 10m 800C 1h A 0.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

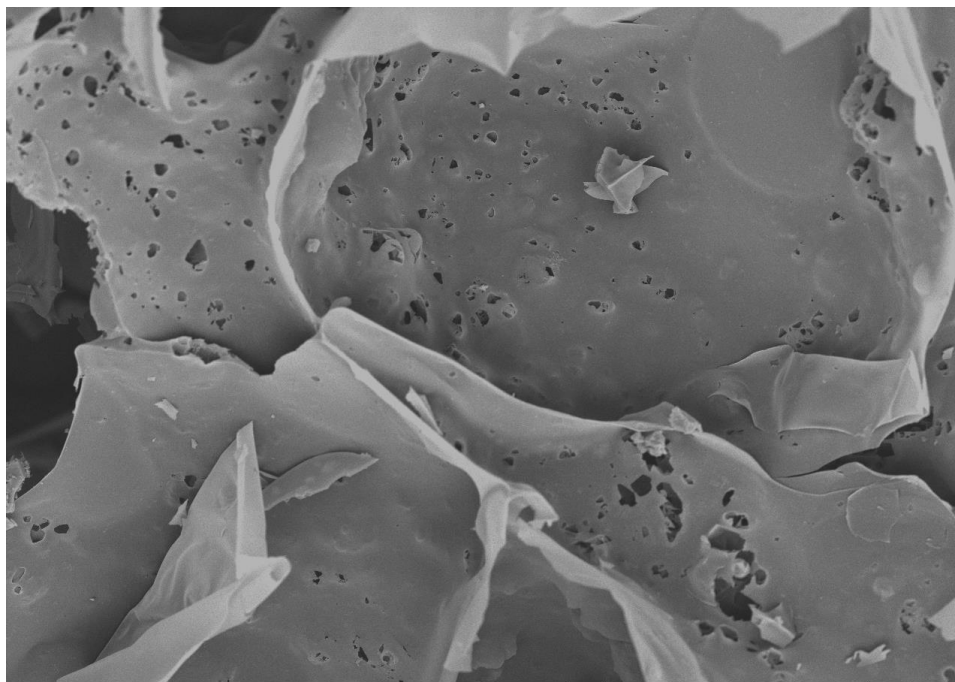

Clariant SU7000 5.00kV 5.9mm x1.00k UD+LD+MD 08/26/2024 50.0μm

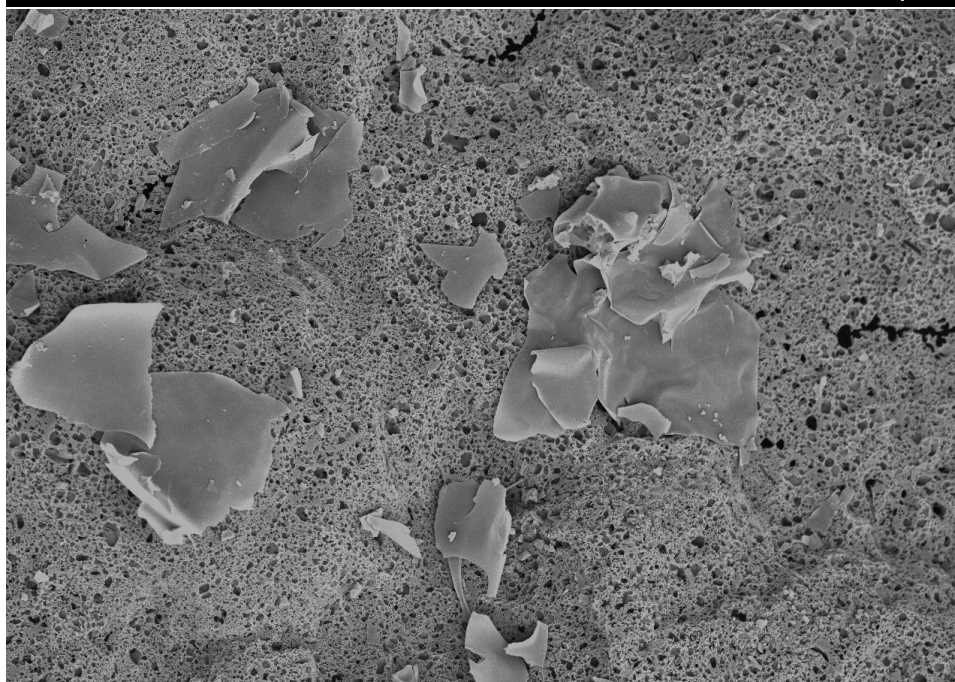

Clariant SU7000 5.00kV 6.0mm x1.00k UD+LD+MD 08/26/2024 50.0μm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980B 2/3 10m 800C 1h A 0.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

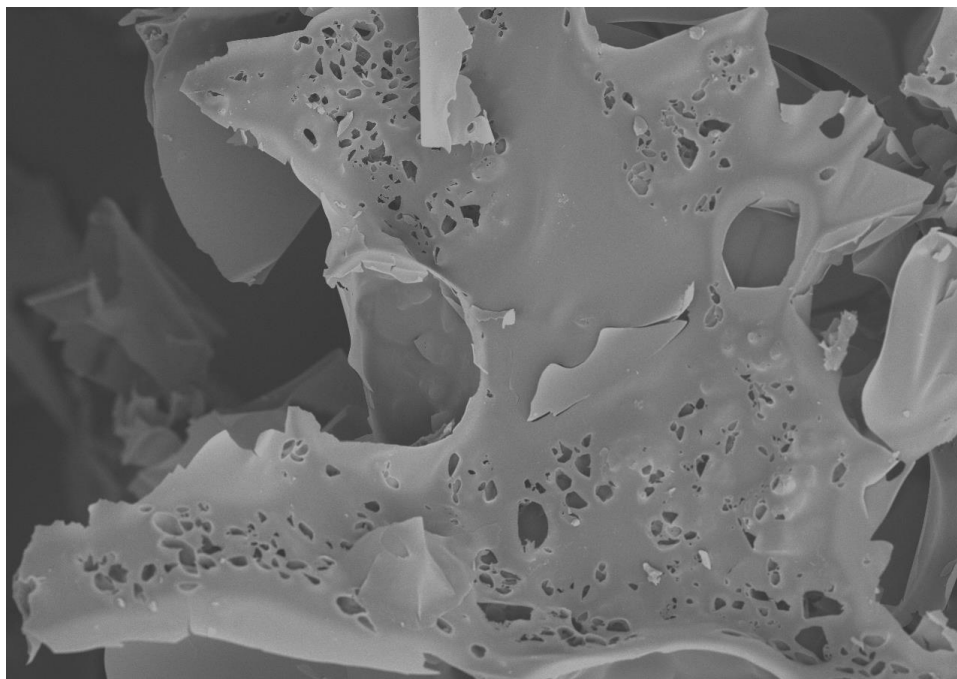

Clariant SU7000 5.00kV 5.8mm x1.00k UD+LD+MD 08/26/2024 50.0µm

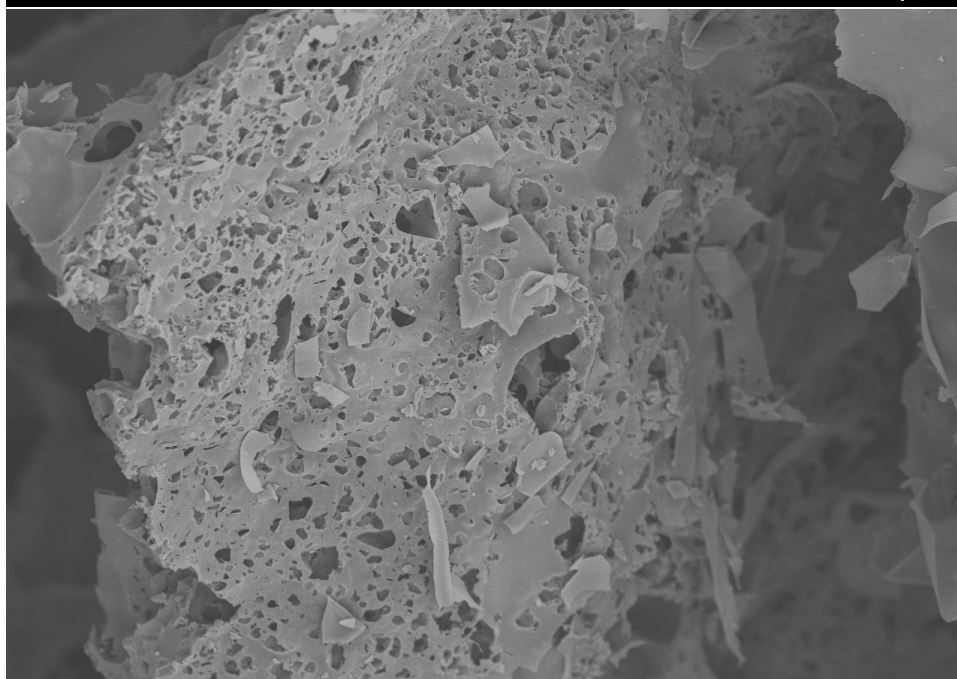


Clariant SU7000 5.00kV 5.8mm x1.00k UD+LD+MD 08/26/2024 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2980B 2/3 10m 800C 1h A 0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

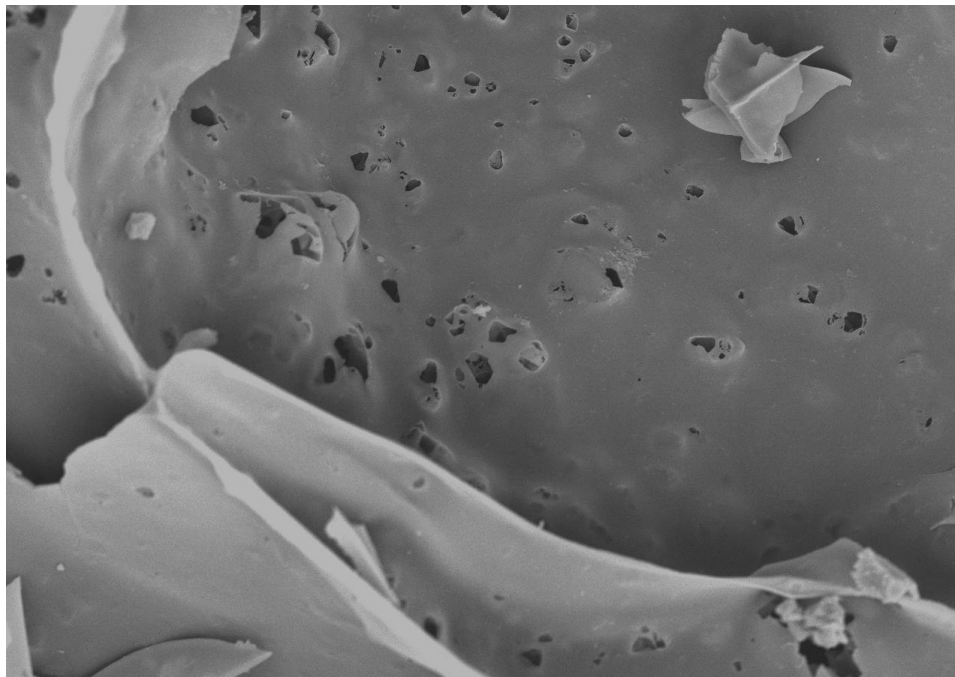

Clariant SU7000 5.00kV 5.9mm x2.00k UD+LD+MD 08/26/2024 20.0µm

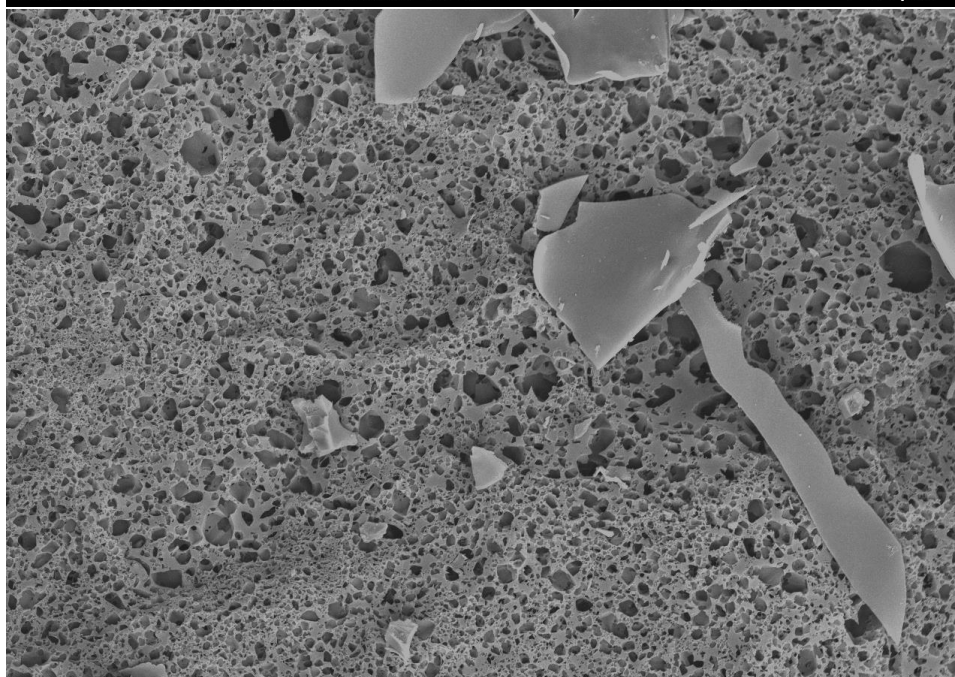


Clariant SU7000 5.00kV 6.0mm x2.00k UD+LD+MD 08/26/2024 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2980B 2/3 10m 800C 1h A 0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

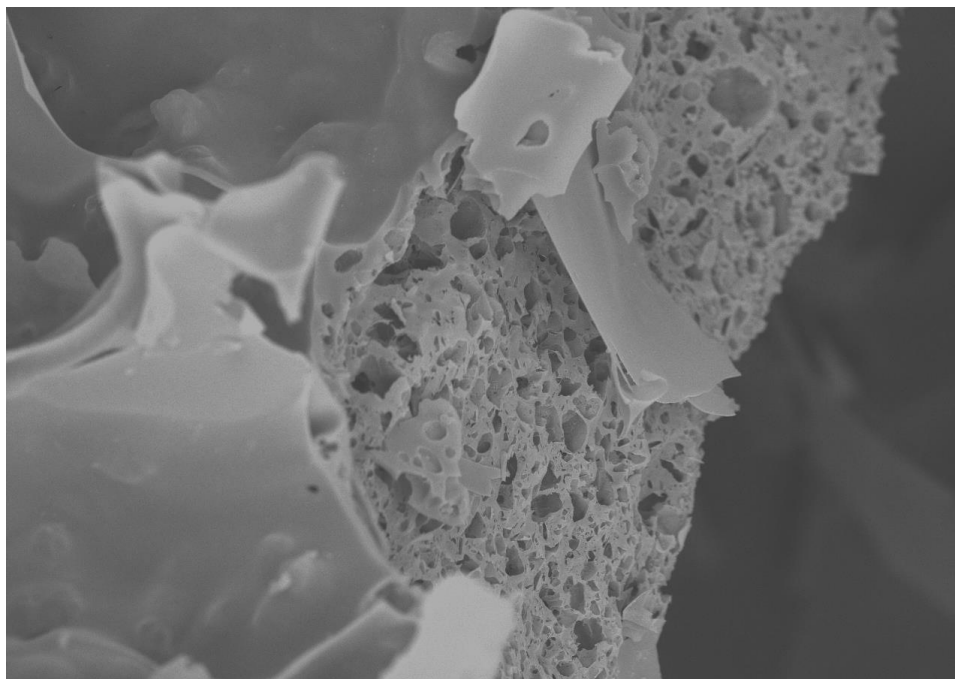

Clariant SU7000 5.00kV 5.8mm x2.00k UD+LD+MD 08/26/2024 20.0µm

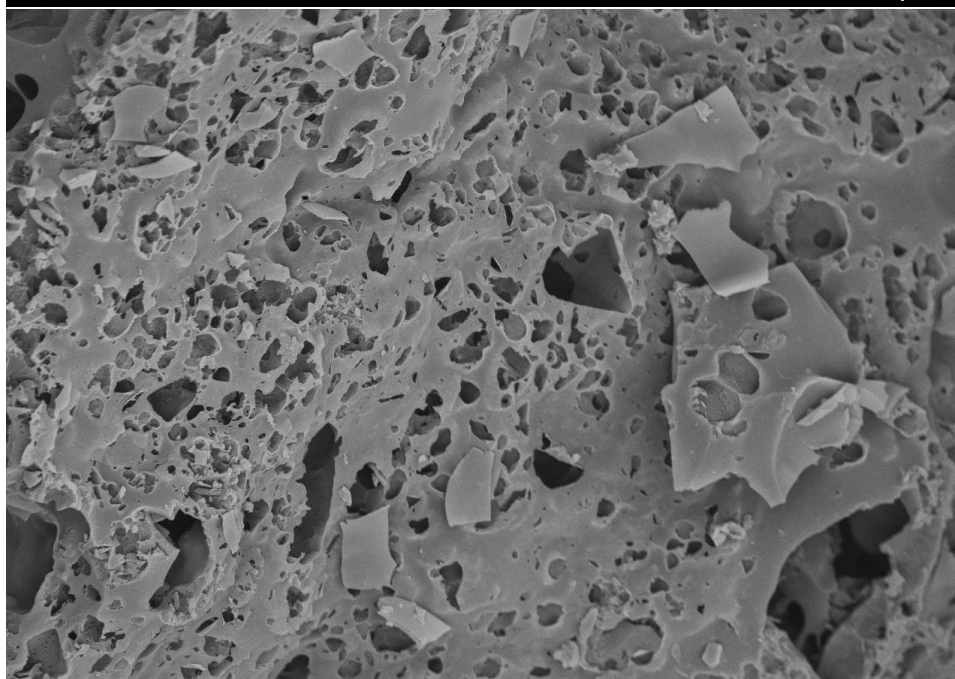


Clariant SU7000 5.00kV 5.8mm x2.00k UD+LD+MD 08/26/2024 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2980B 2/3 10m 800C 1h A 0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

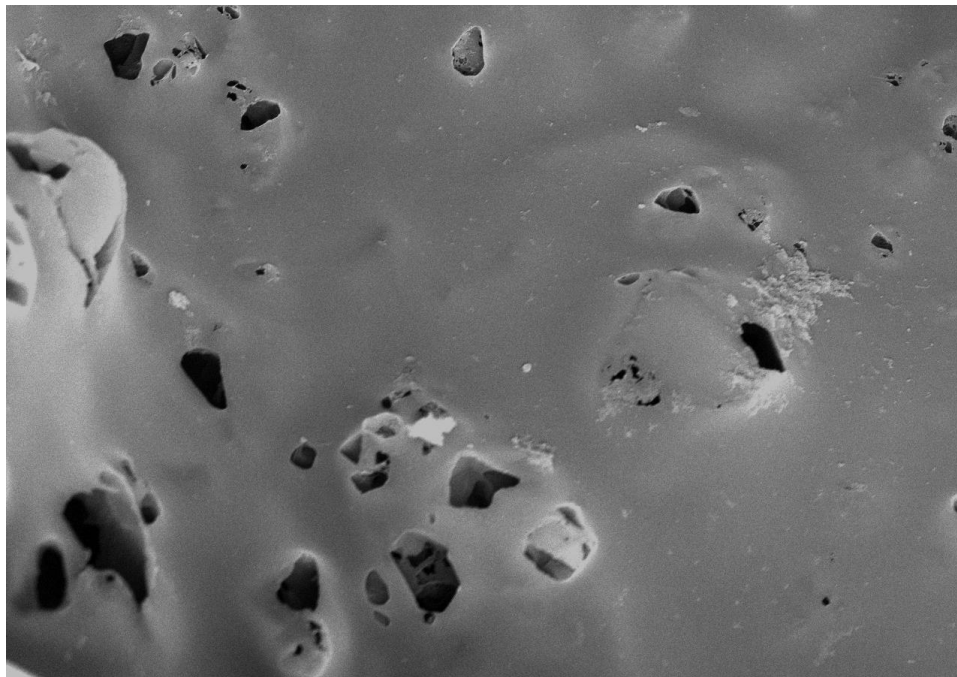

Clariant SU7000 5.00kV 5.9mm x5.00k UD+LD+MD 08/26/2024 10.0µm

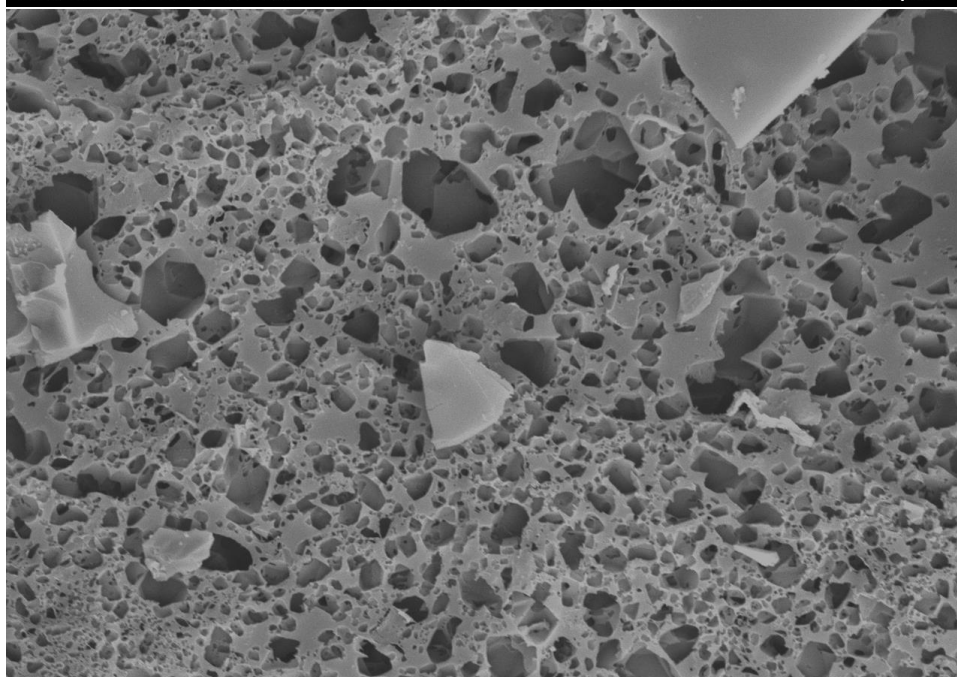


Clariant SU7000 5.00kV 6.0mm x5.00k UD+LD+MD 08/26/2024 10.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2980B 2/3 10m 800C 1h A 0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

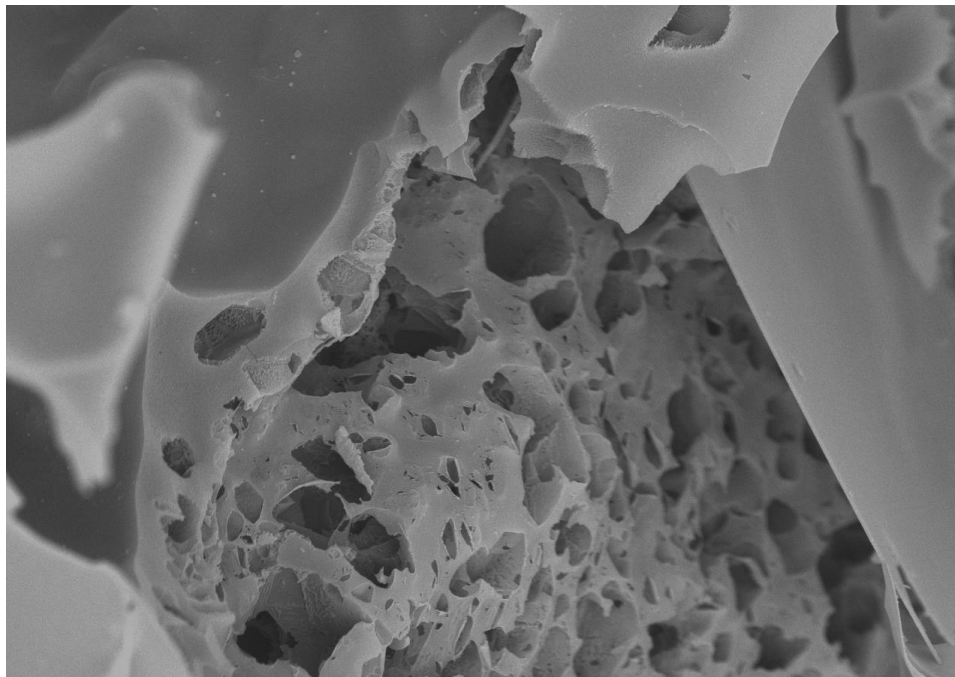

Clariant SU7000 5.00kV 5.8mm x5.00k UD+LD+MD 08/26/2024 10.0µm

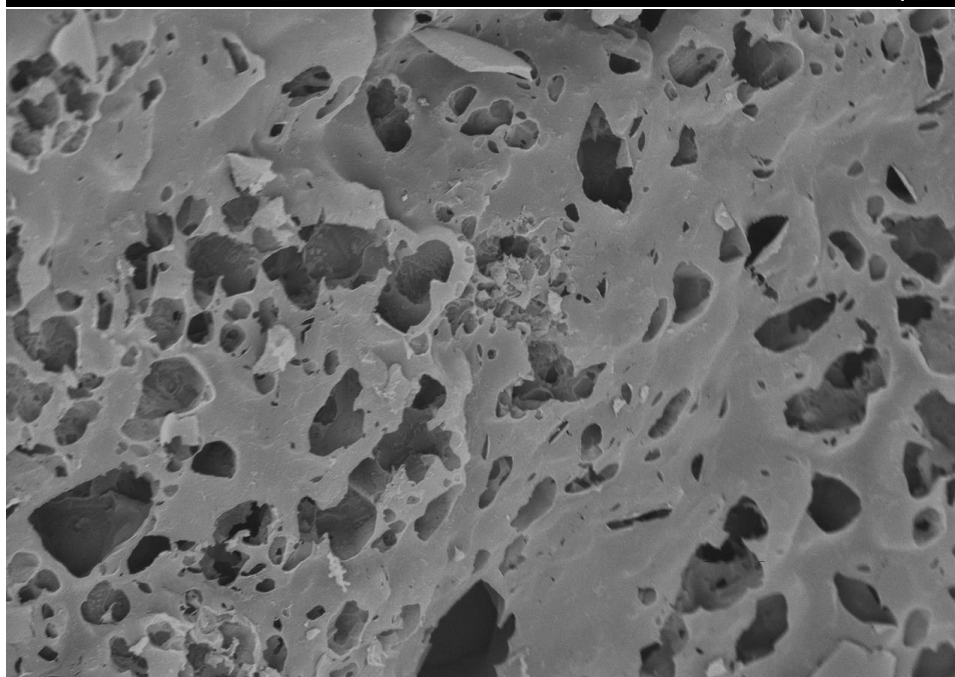


Clariant SU7000 5.00kV 5.8mm x5.00k UD+LD+MD 08/26/2024 10.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2980B 2/3 10m 800C 1h A 0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

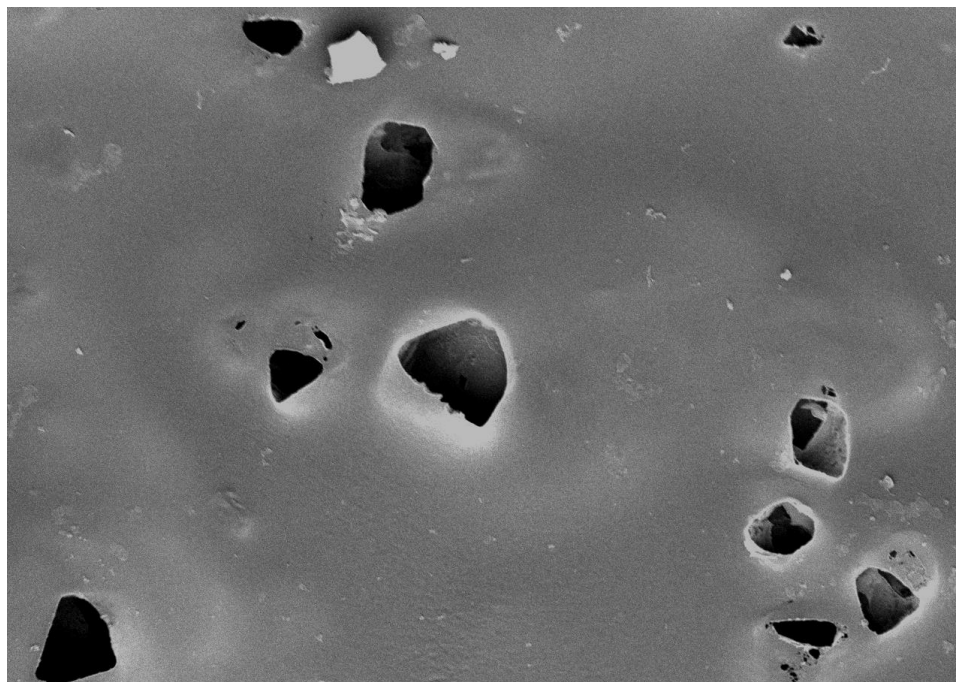

Clariant SU7000 5.00kV 5.9mm x10.0k UD+LD+MD 08/26/2024 5.00µm

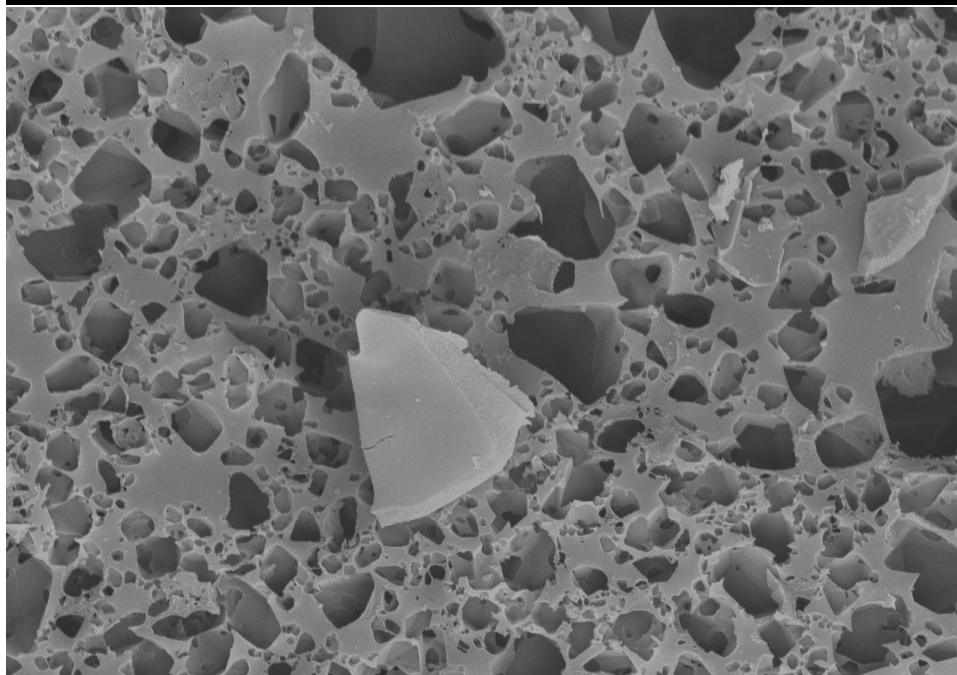

Clariant SU7000 5.00kV 6.0mm x10.0k UD+LD+MD 08/26/2024 5.00µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980B 2/3 10m 800C 1h A 0.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

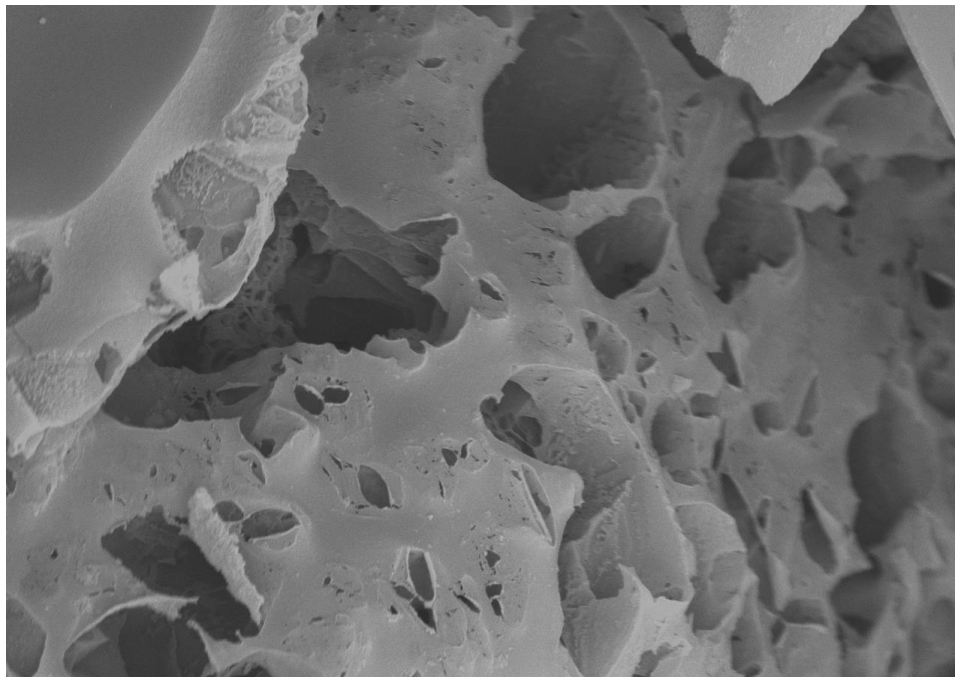

Clariant SU7000 5.00kV 5.8mm x10.0k UD+LD+MD 08/26/2024 5.00µm

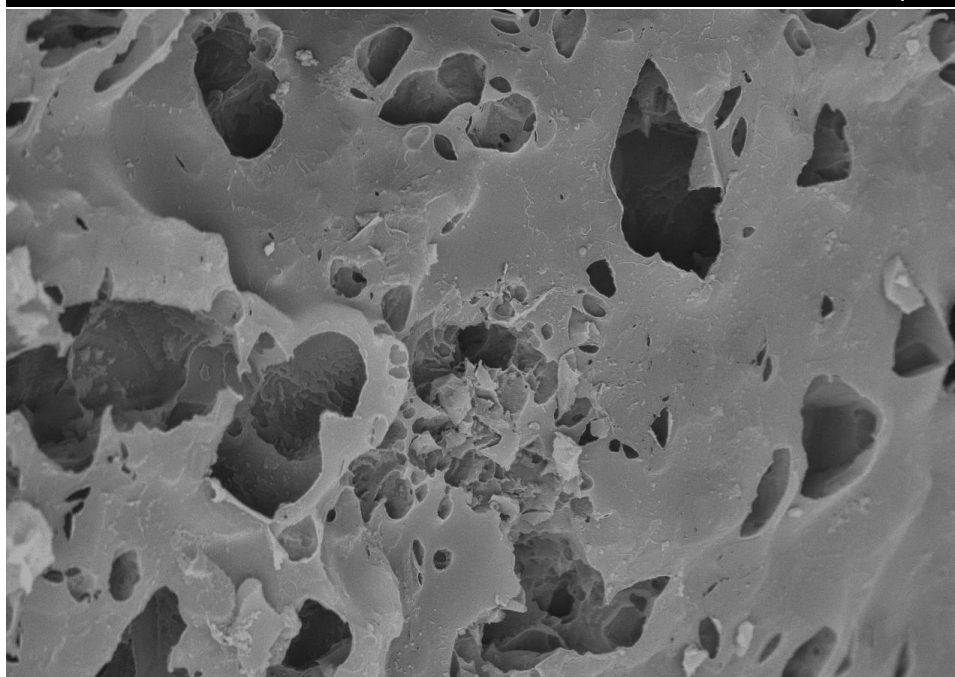

Clariant SU7000 5.00kV 5.8mm x10.0k UD+LD+MD 08/26/2024 5.00µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980B 2/3 10m 800C 1h A 0.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

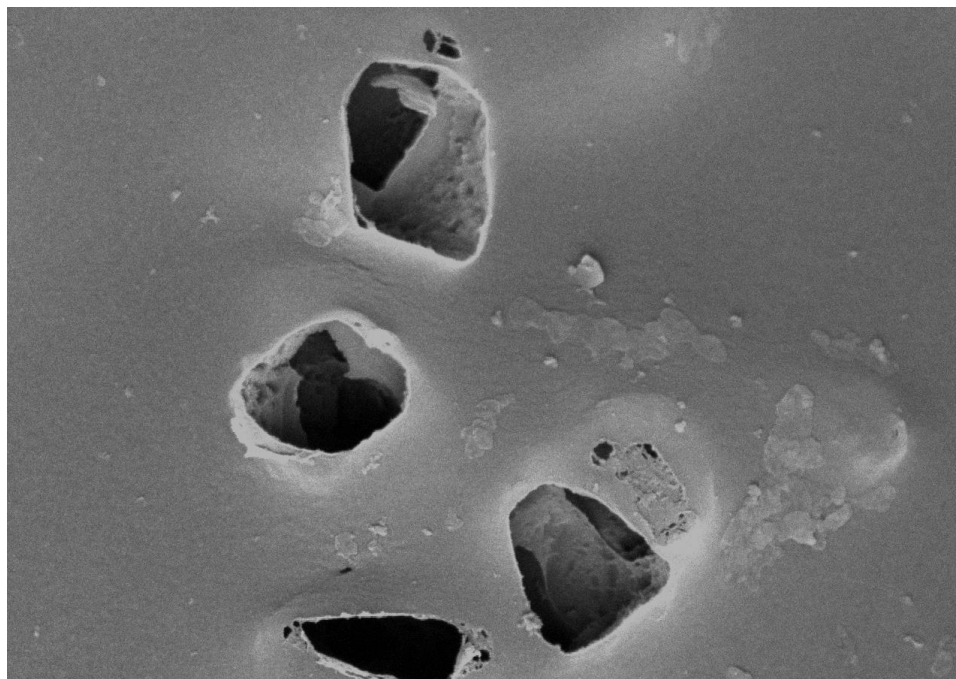

Clariant SU7000 5.00kV 5.9mm x25.0k UD+LD+MD 08/26/2024 2.00µm

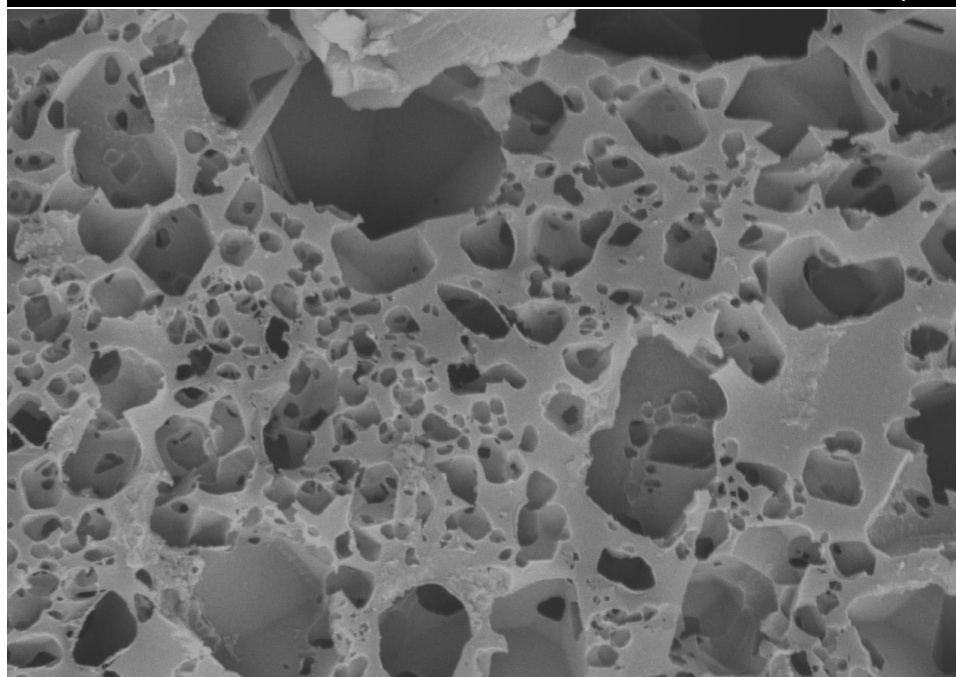

Clariant SU7000 5.00kV 6.0mm x25.0k UD+LD+MD 08/26/2024 2.00µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980B 2/3 10m 800C 1h A 0.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047658-24

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

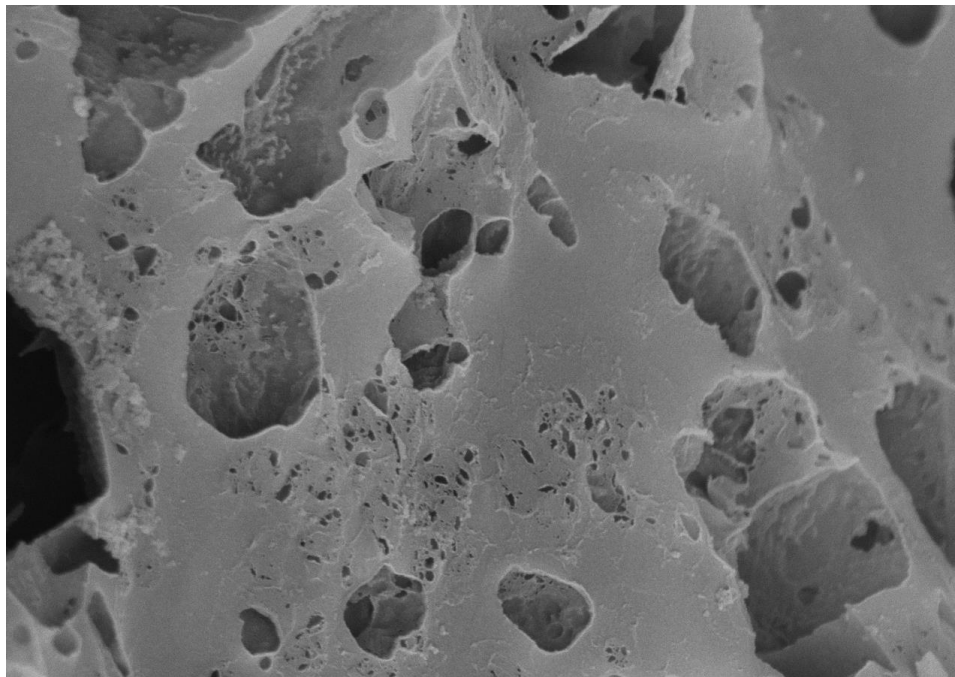

Clariant SU7000 5.00kV 5.8mm x25.0k UD+LD+MD 08/26/2024 2.00µm

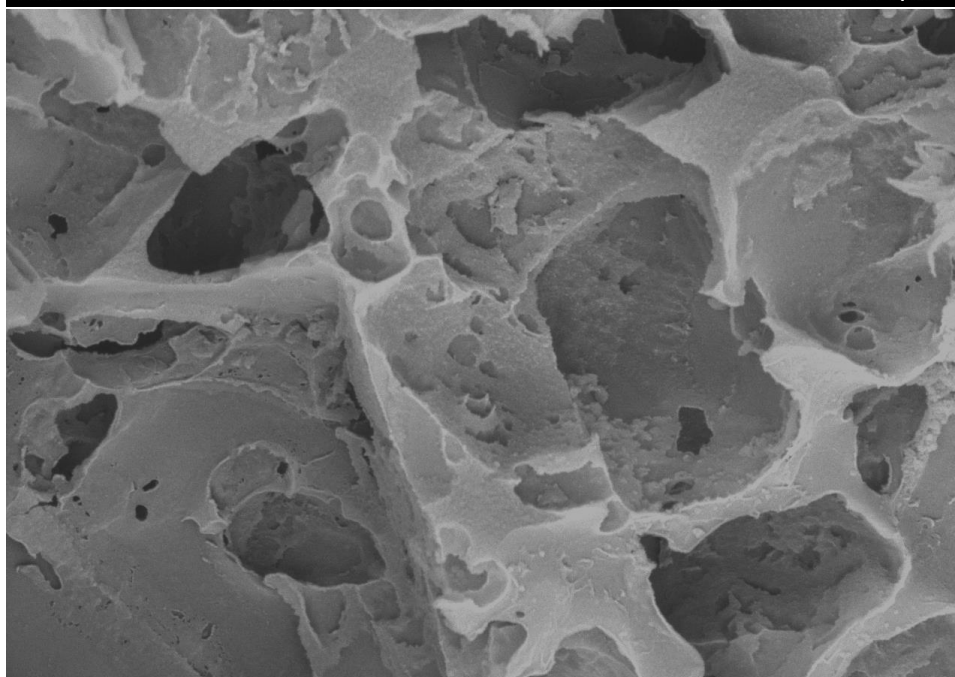

Clariant SU7000 5.00kV 5.8mm x25.0k UD+LD+MD 08/26/2024 2.00µm