

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

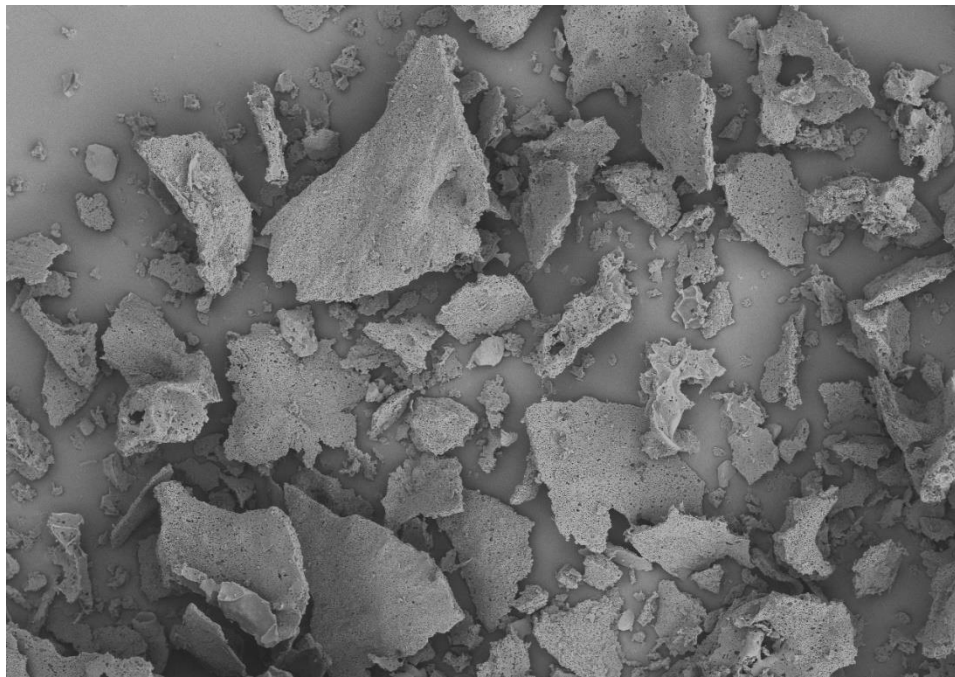

Clariant SU7000 5.00kV 5.7mm x100 UD+LD+MD 08/28/2024 500µm

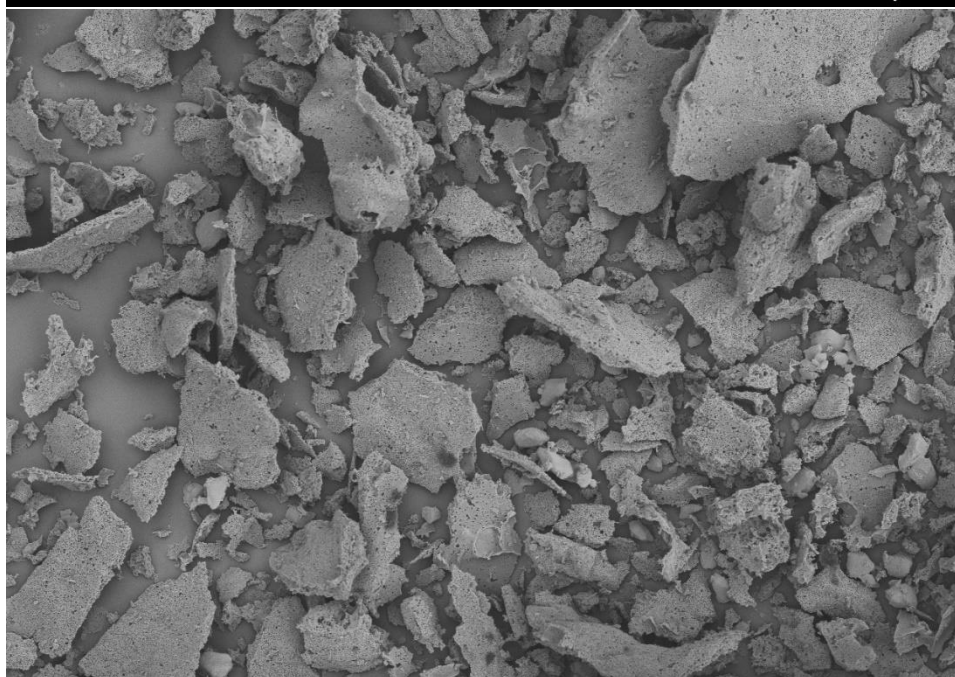

Clariant SU7000 5.00kV 5.9mm x100 UD+LD+MD 08/28/2024 500µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch

Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

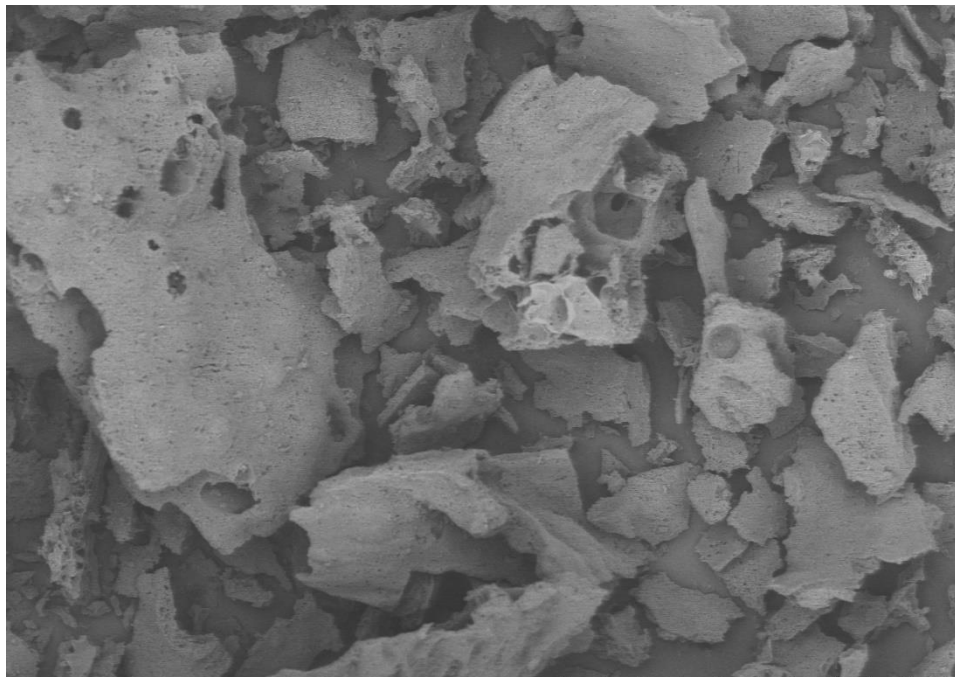

Clariant SU7000 5.00kV 5.8mm x100 UD+LD+MD 08/28/2024 500µm



Clariant SU7000 5.00kV 5.9mm x100 UD+LD+MD 08/28/2024 500µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

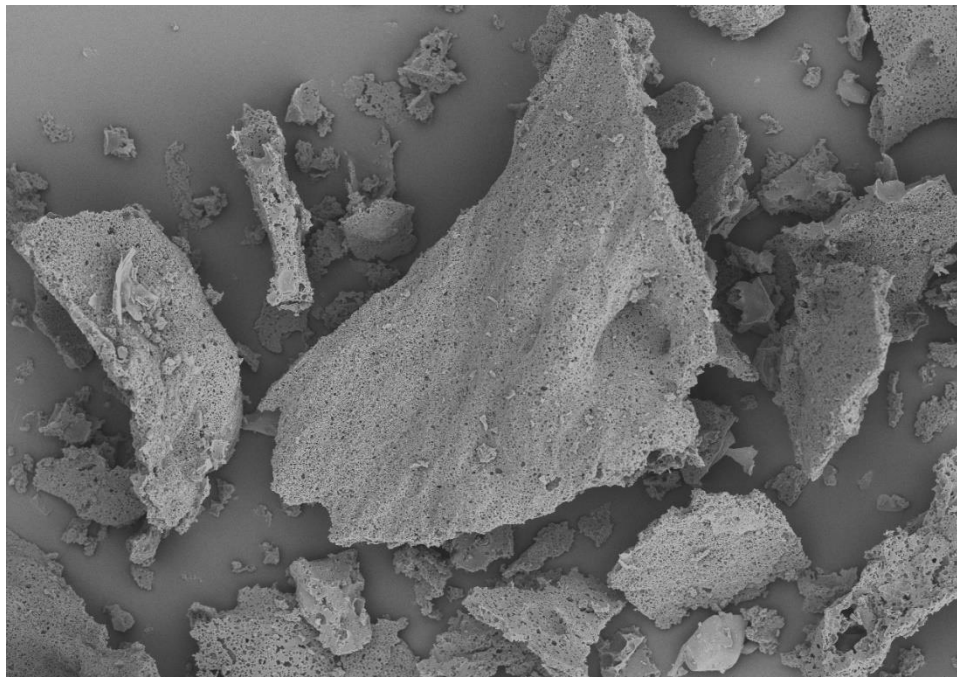

Clariant SU7000 5.00kV 5.7mm x200 UD+LD+MD 08/28/2024 200µm

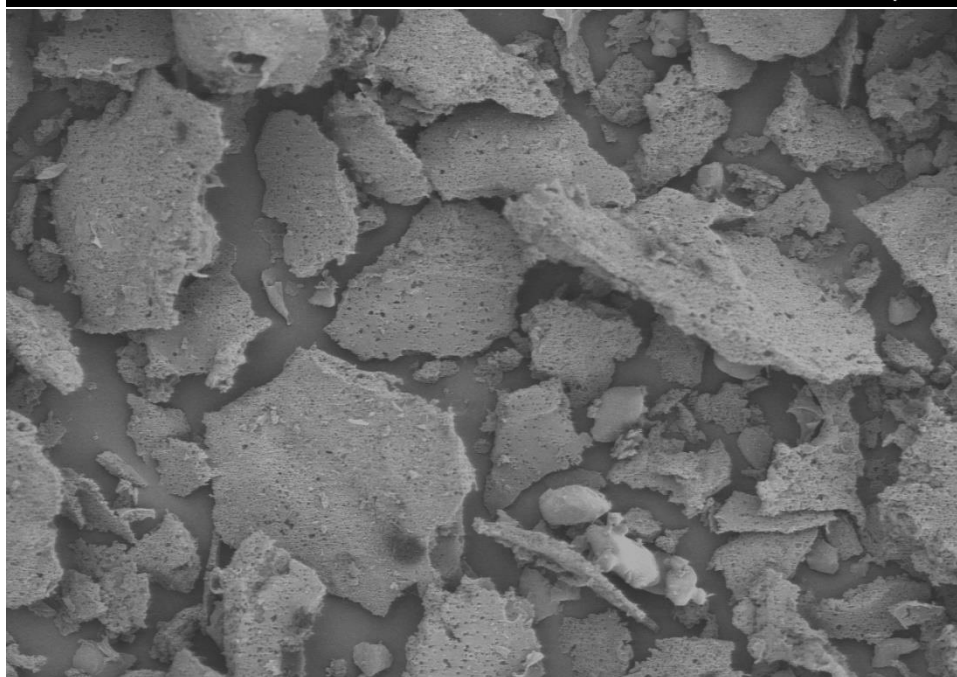

Clariant SU7000 5.00kV 5.9mm x200 UD+LD+MD 08/28/2024 200µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

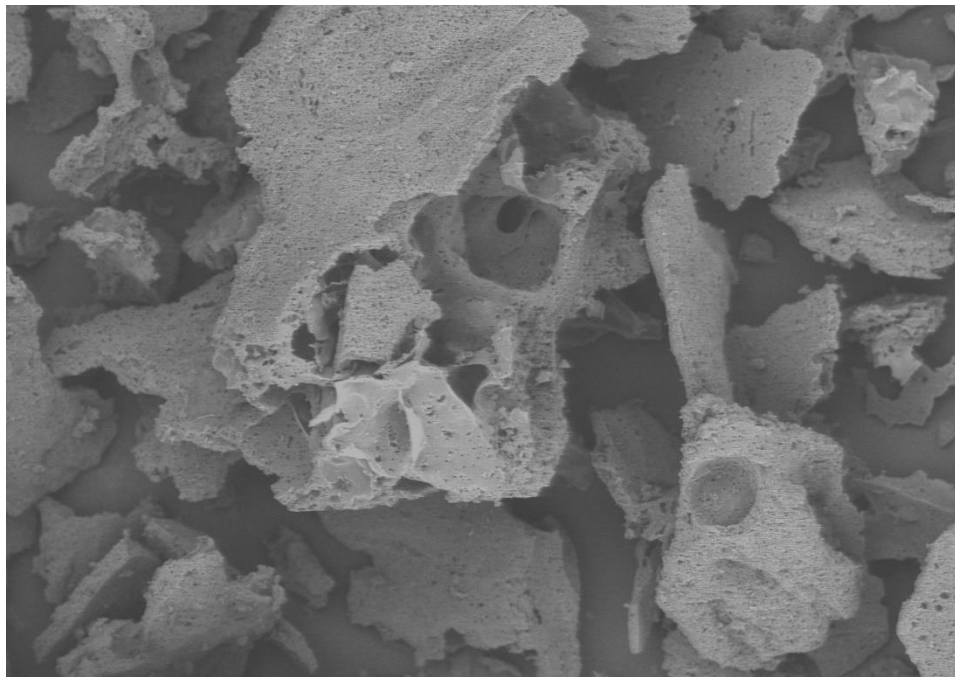

Clariant SU7000 5.00kV 5.6mm x200 UD+LD+MD 08/28/2024 200µm

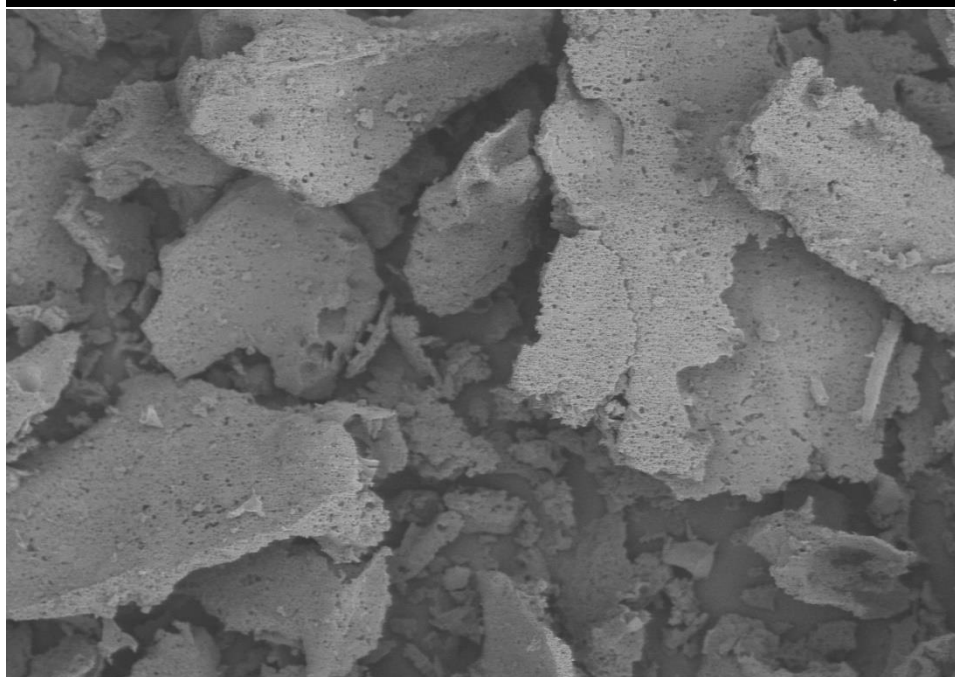

Clariant SU7000 5.00kV 5.7mm x200 UD+LD+MD 08/28/2024 200µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

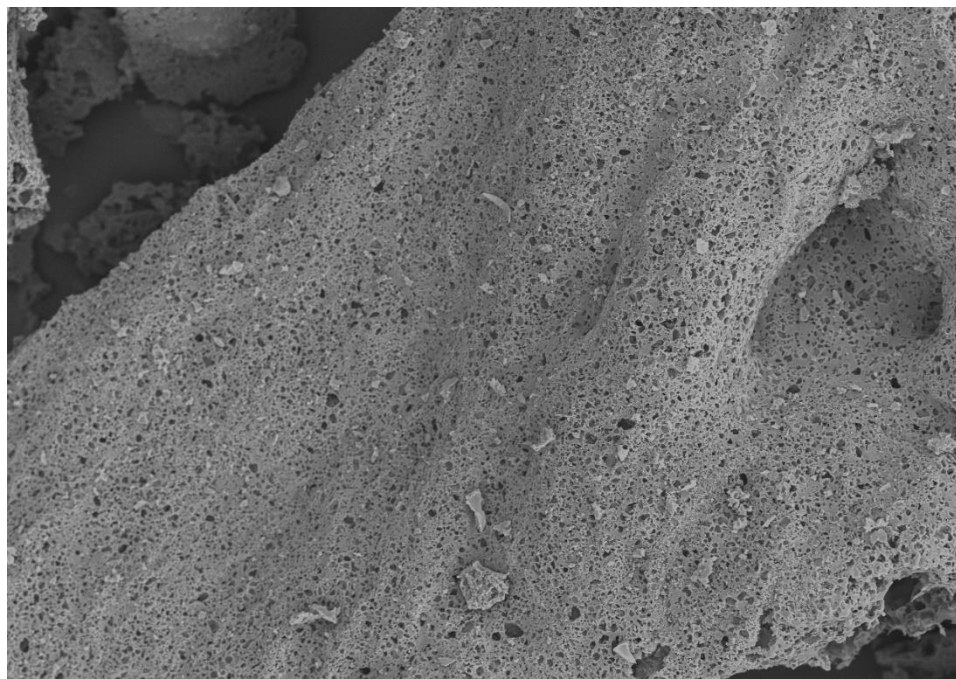

Clariant SU7000 5.00kV 5.7mm x500 UD+LD+MD 08/28/2024 100μm

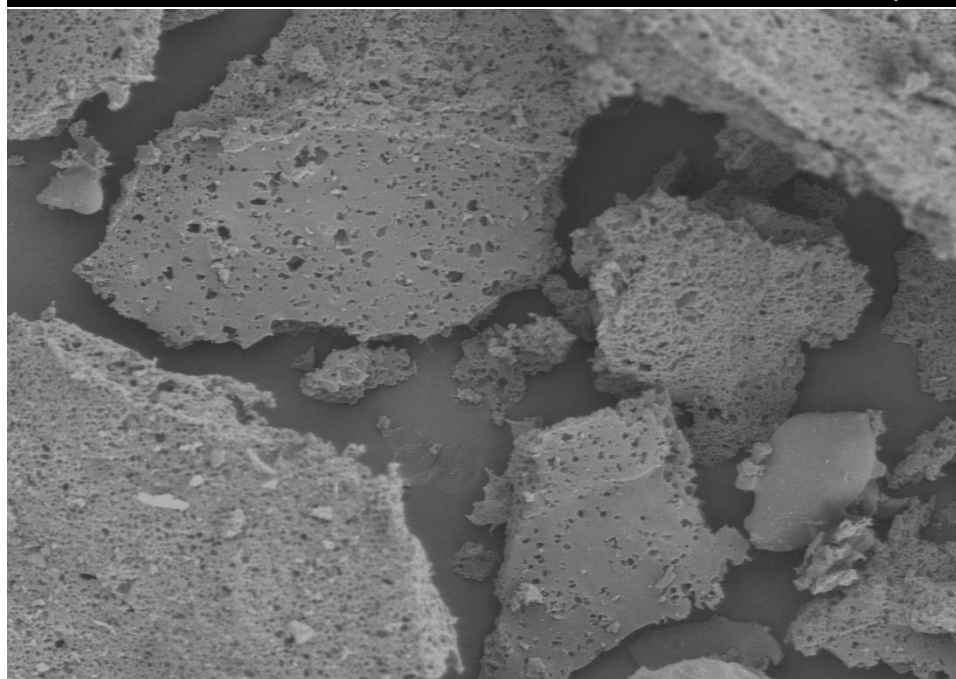

Clariant SU7000 5.00kV 5.9mm x500 UD+LD+MD 08/28/2024 100μm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

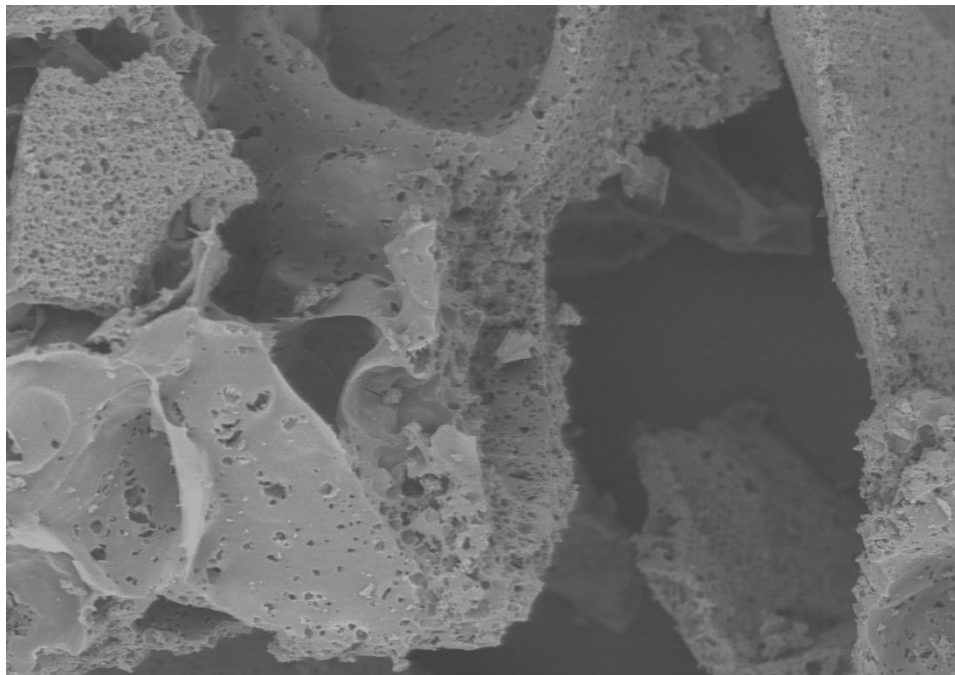

Clariant SU7000 5.00kV 5.6mm x500 UD+LD+MD 08/28/2024 100µm

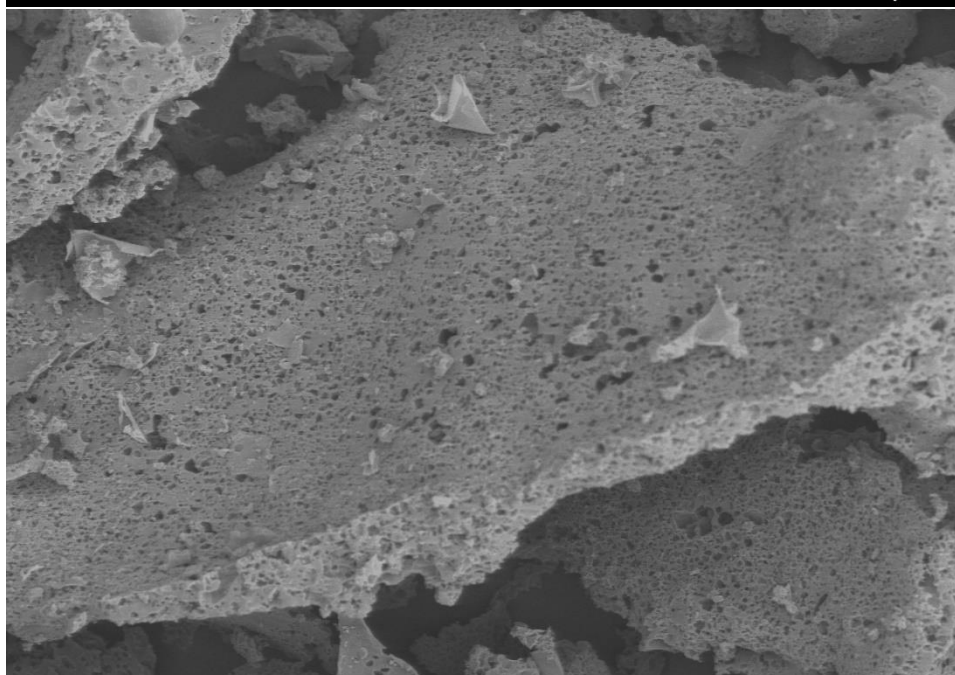

Clariant SU7000 5.00kV 5.9mm x500 UD+LD+MD 08/28/2024 100µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

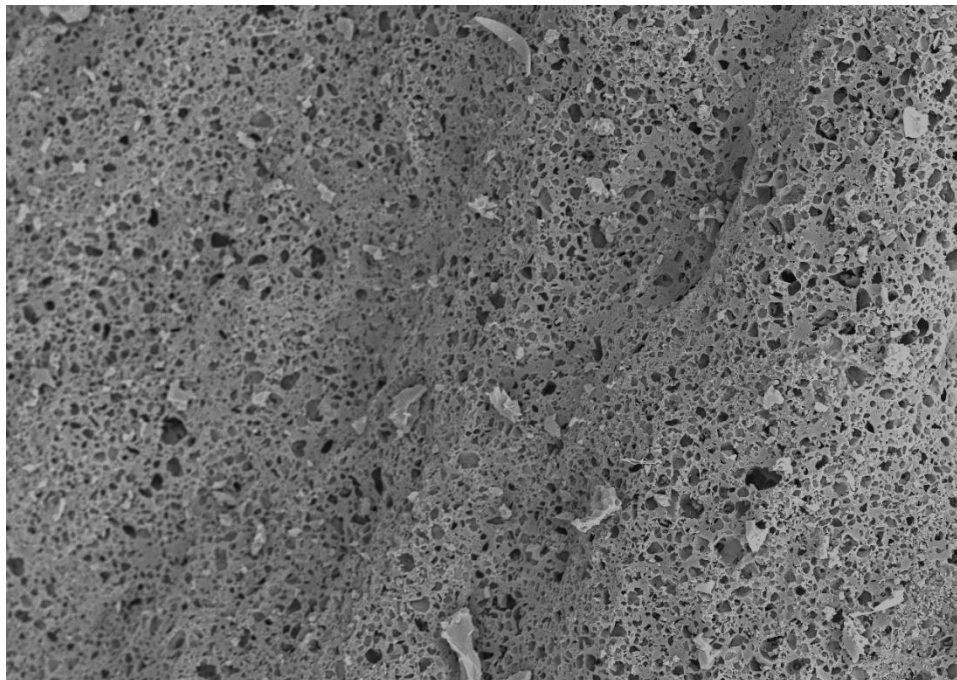

Clariant SU7000 5.00kV 5.7mm x1.00k UD+LD+MD 08/28/2024 50.0µm

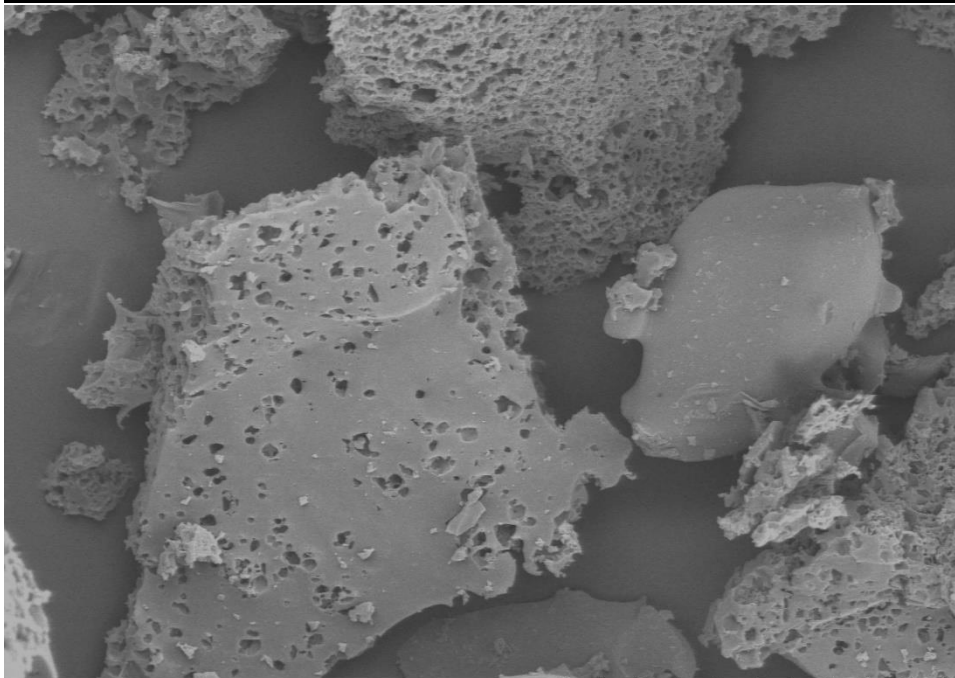

Clariant SU7000 5.00kV 5.9mm x1.00k UD+LD+MD 08/28/2024 50.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

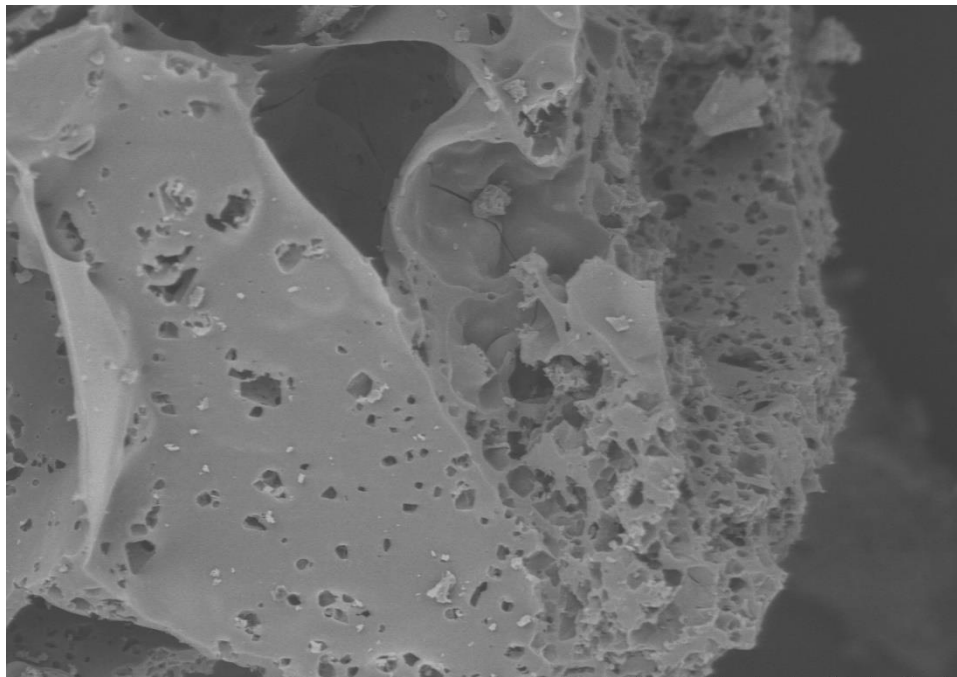

Clariant SU7000 5.00kV 5.5mm x1.00k UD+LD+MD 08/28/2024 50.0µm

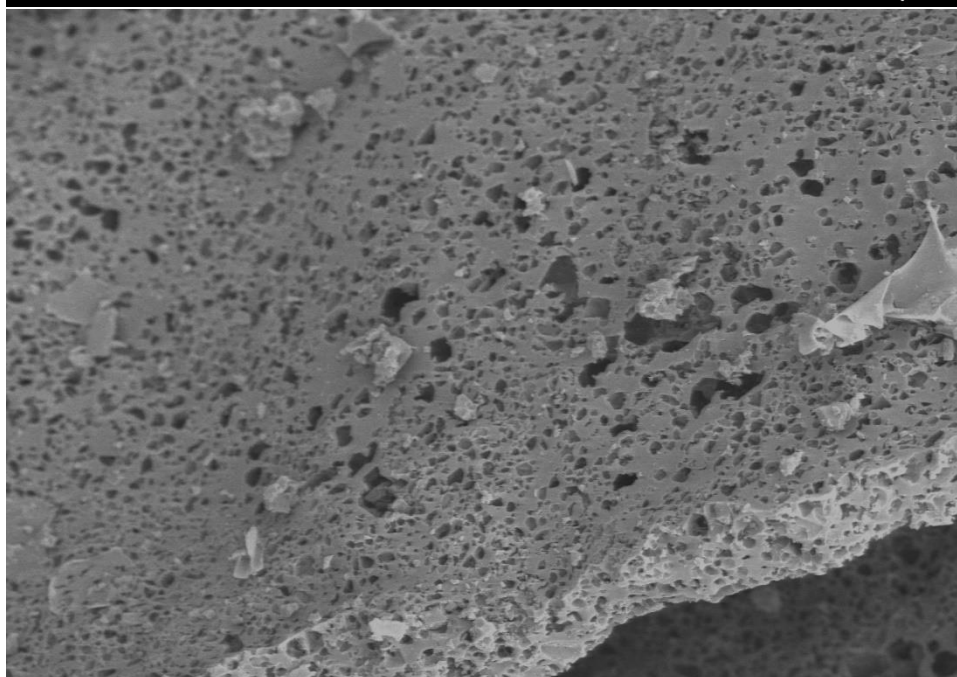

Clariant SU7000 5.00kV 5.8mm x1.00k UD+LD+MD 08/28/2024 50.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

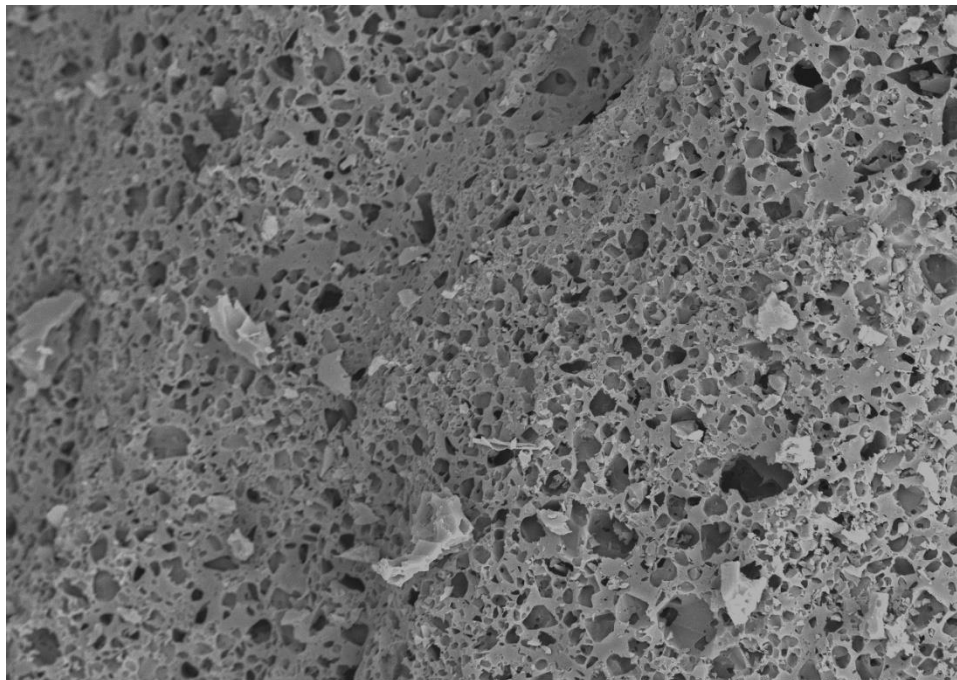

Clariant SU7000 5.00kV 5.7mm x2.00k UD+LD+MD 08/28/2024 20.0µm

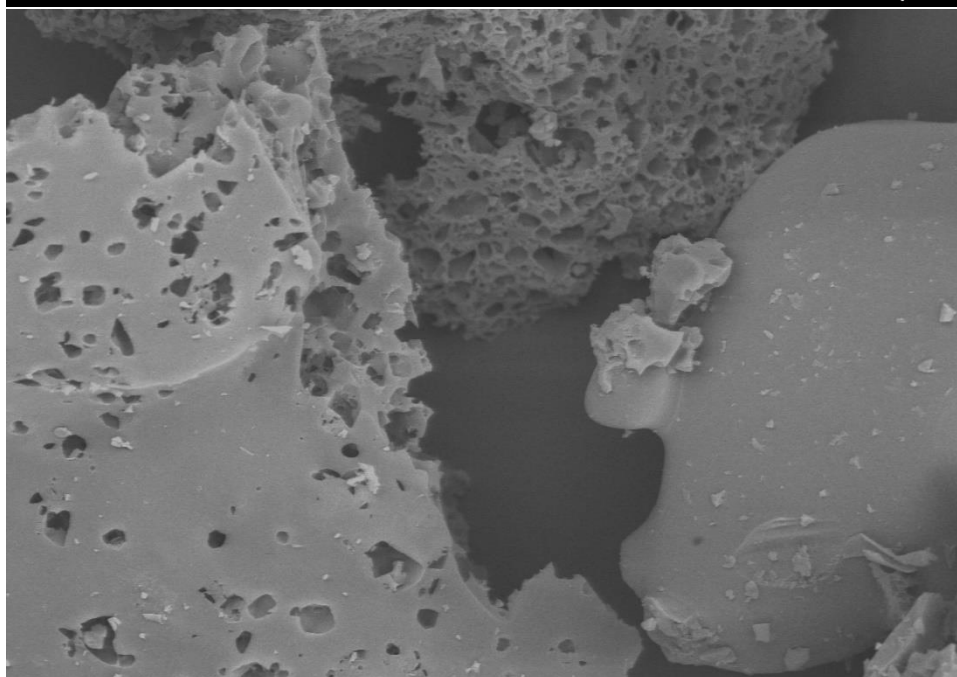

Clariant SU7000 5.00kV 5.9mm x2.00k UD+LD+MD 08/28/2024 20.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

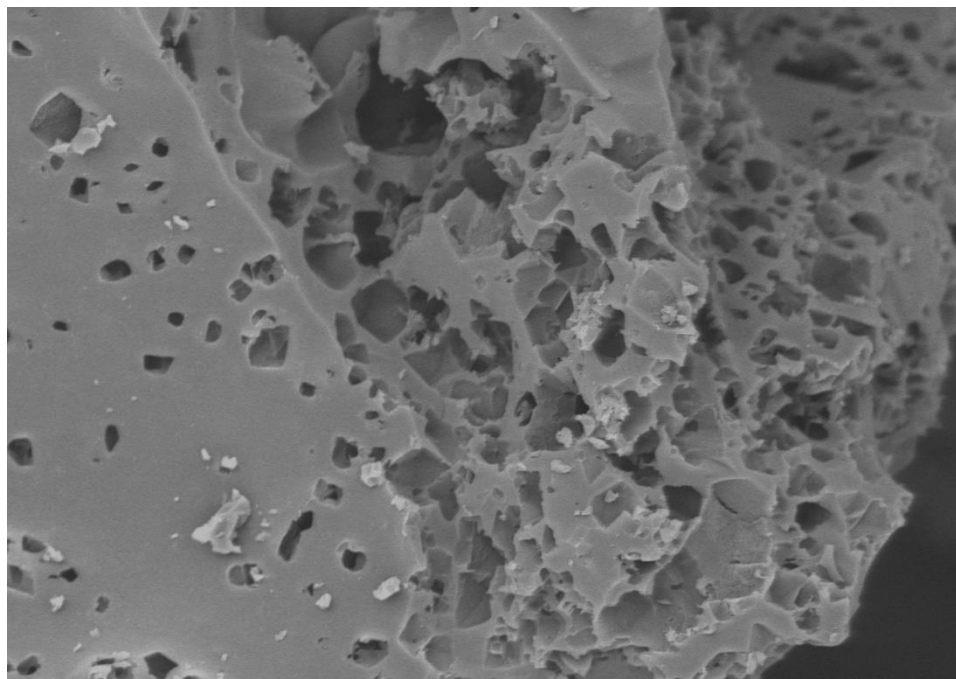

Clariant SU7000 5.00kV 5.5mm x2.00k UD+LD+MD 08/28/2024 20.0µm

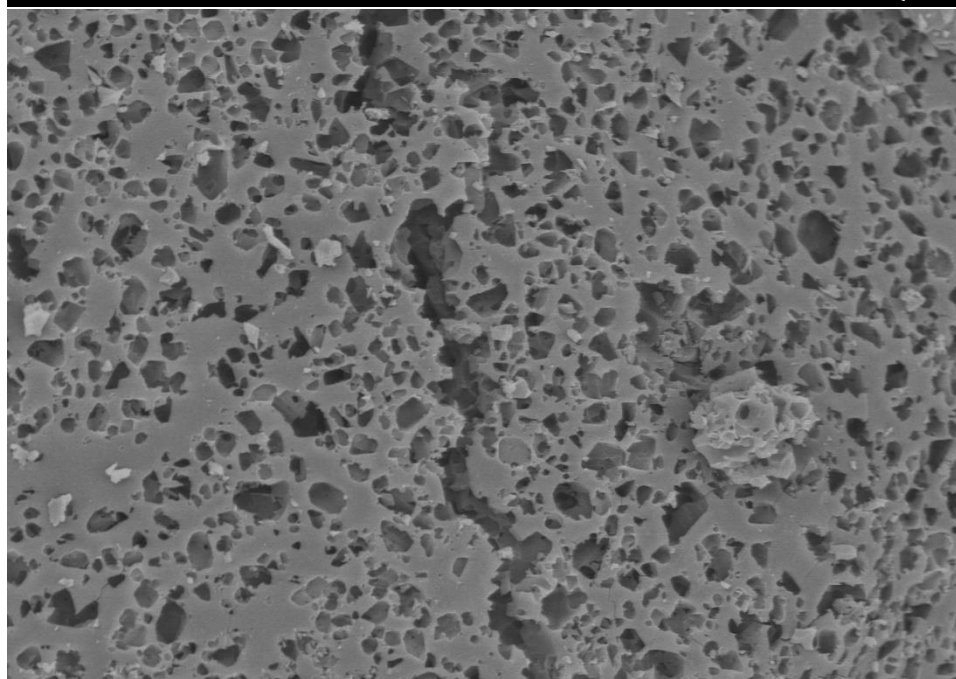

Clariant SU7000 5.00kV 5.7mm x2.00k UD+LD+MD 08/28/2024 20.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

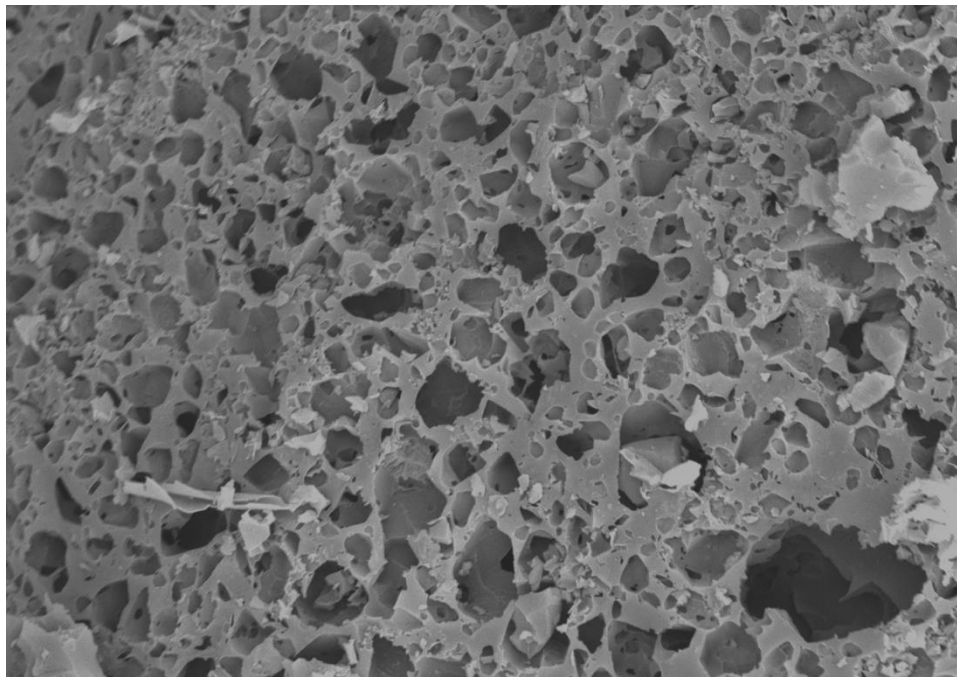

Clariant SU7000 5.00kV 5.7mm x5.00k UD+LD+MD 08/28/2024 10.0µm

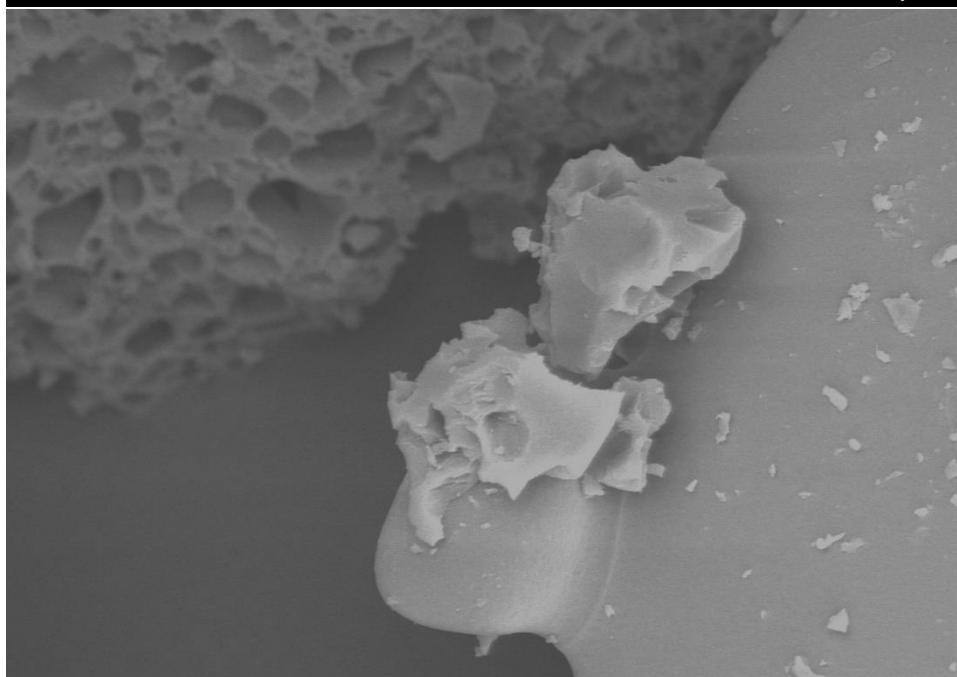

Clariant SU7000 5.00kV 5.9mm x5.00k UD+LD+MD 08/28/2024 10.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

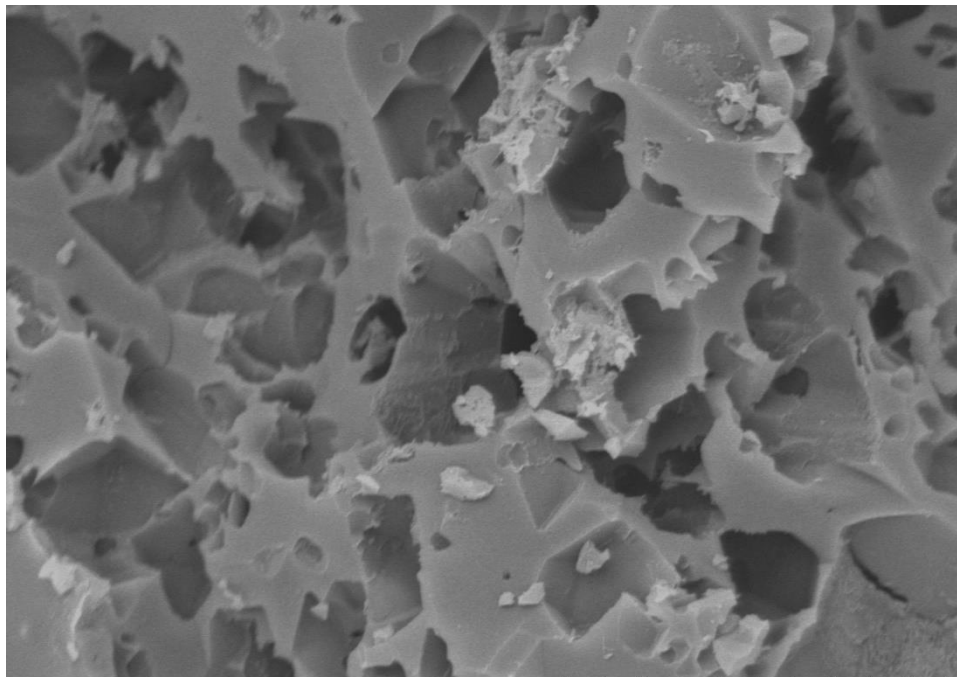

Clariant SU7000 5.00kV 5.5mm x5.00k UD+LD+MD 08/28/2024 10.0µm

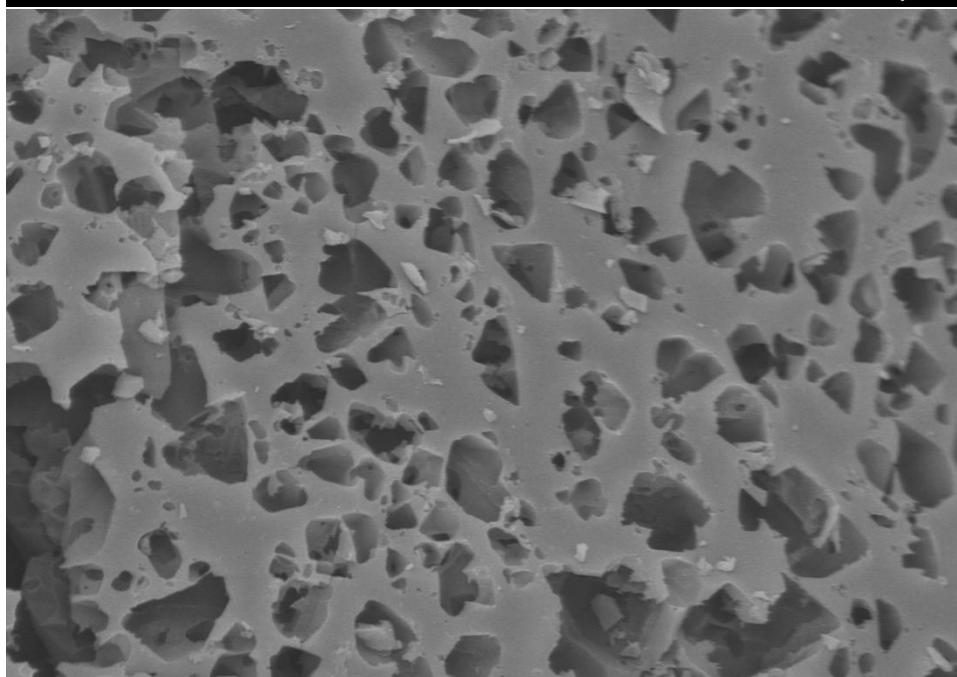

Clariant SU7000 5.00kV 5.7mm x5.00k UD+LD+MD 08/28/2024 10.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

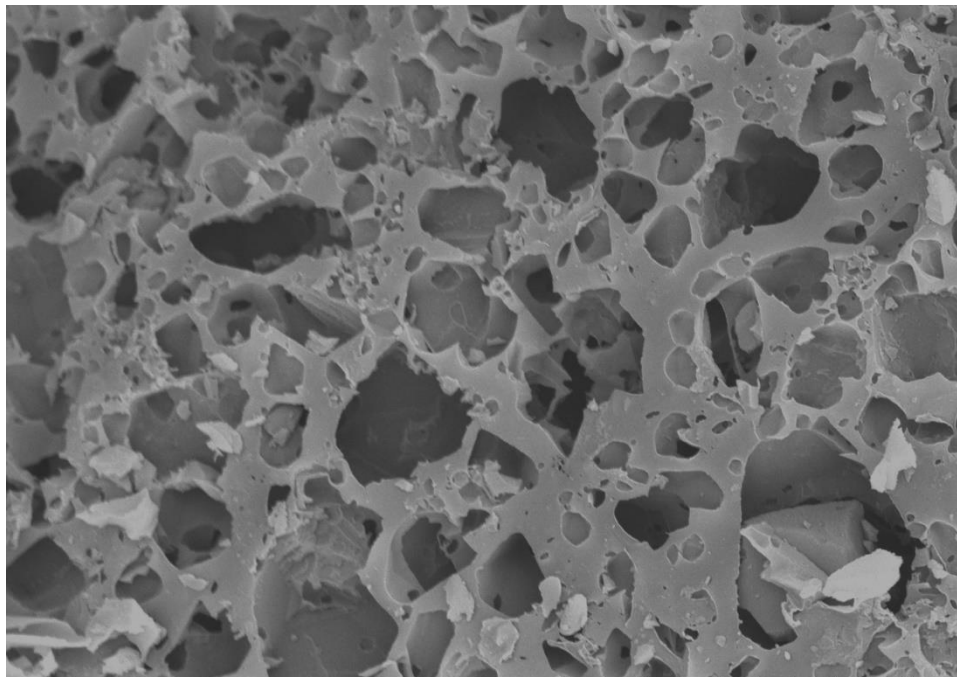

Clariant SU7000 5.00kV 5.7mm x10.0k UD+LD+MD 08/28/2024 5.00µm

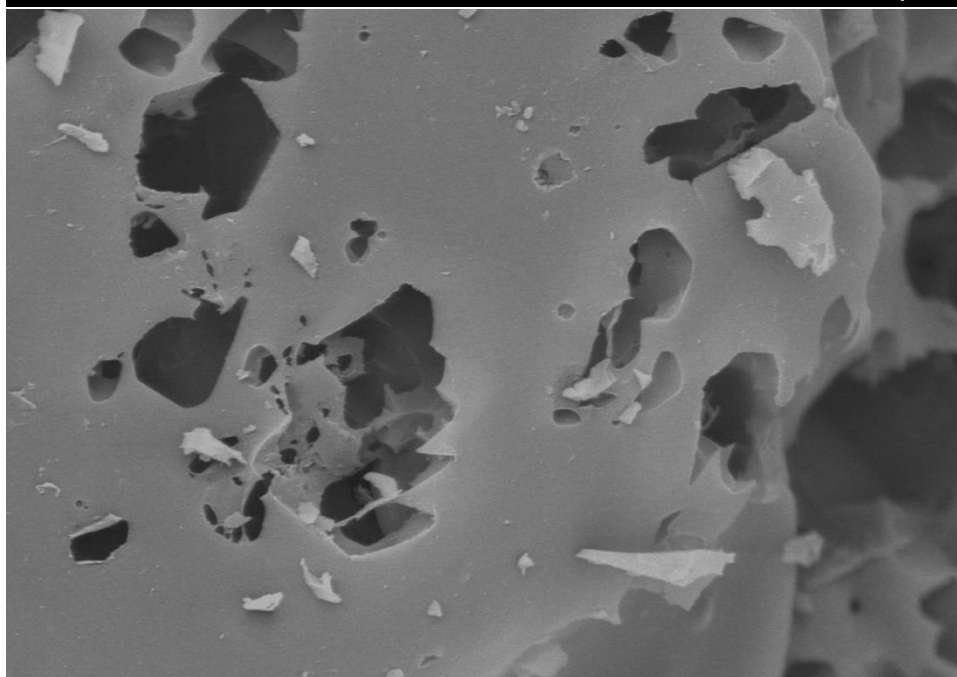

Clariant SU7000 5.00kV 5.9mm x10.0k UD+LD+MD 08/28/2024 5.00µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

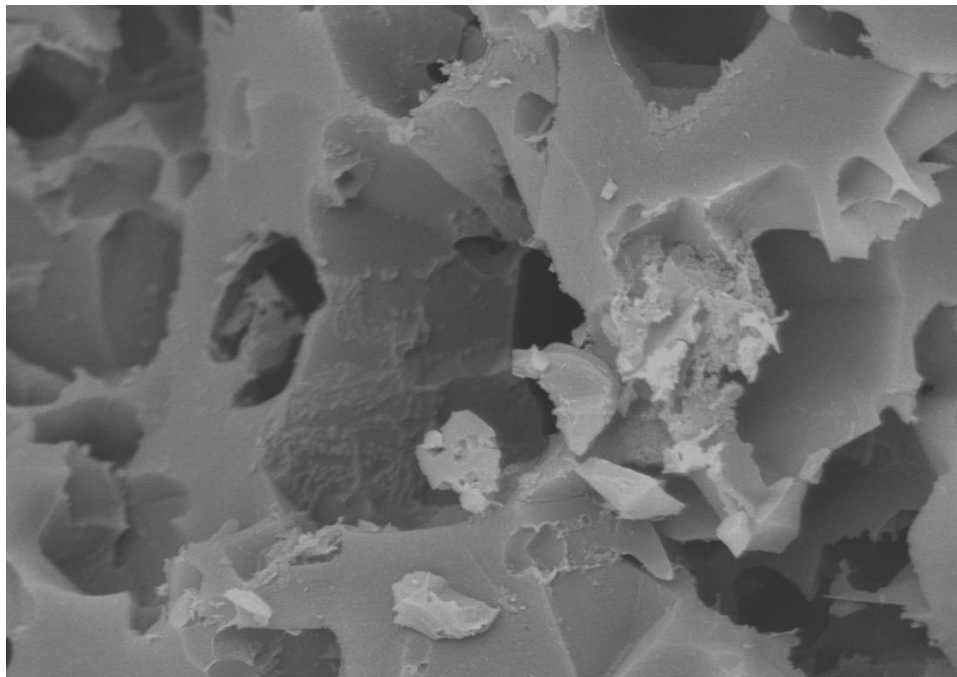

Clariant SU7000 5.00kV 5.5mm x10.0k UD+LD+MD 08/28/2024 5.00µm

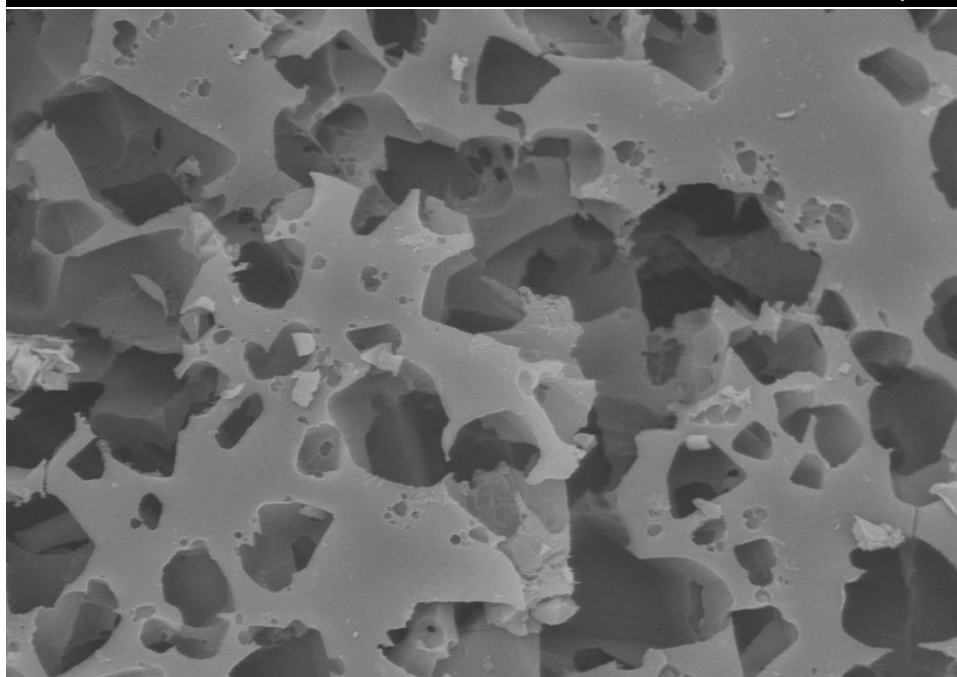

Clariant SU7000 5.00kV 5.7mm x10.0k UD+LD+MD 08/28/2024 5.00µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

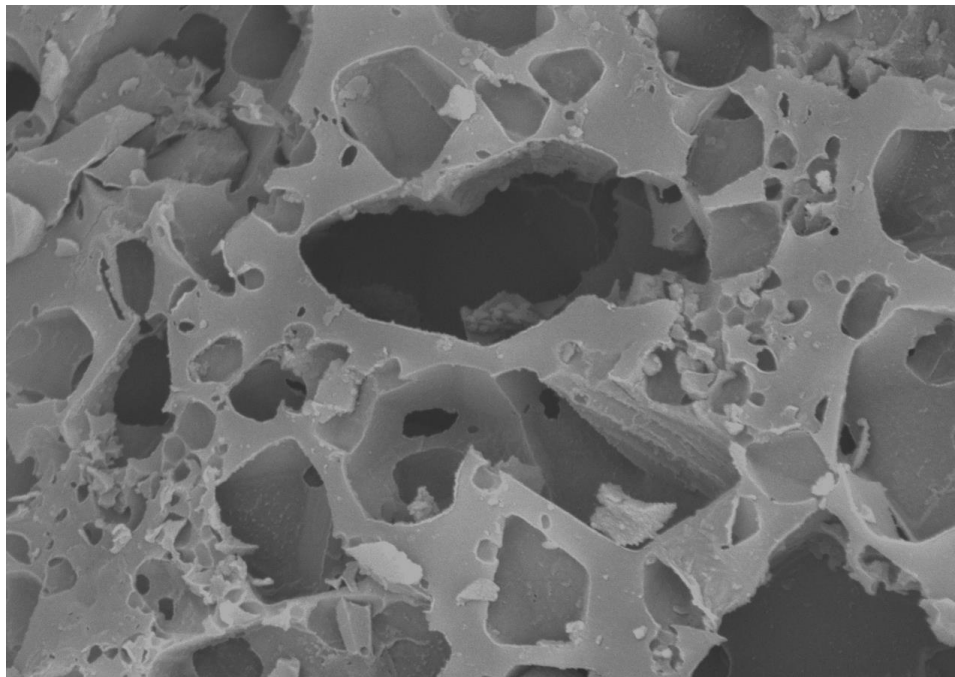

Clariant SU7000 5.00kV 5.7mm x25.0k UD+LD+MD 08/28/2024 2.00µm

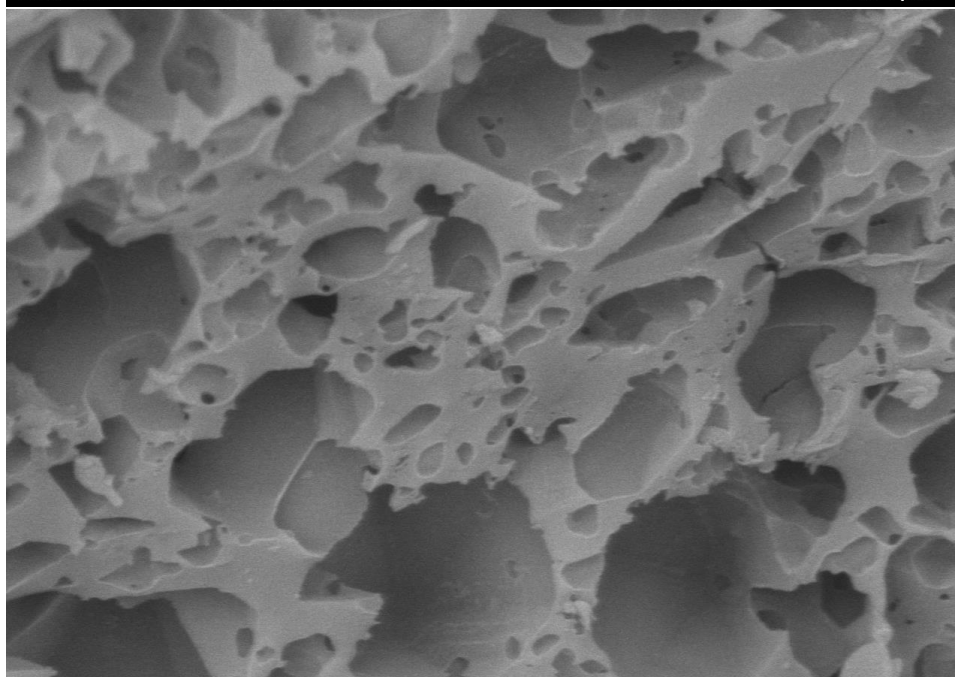

Clariant SU7000 5.00kV 5.9mm x25.0k UD+LD+MD 08/28/2024 2.00µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB2980C 2/3 20m 800C 1h B 1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047909-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

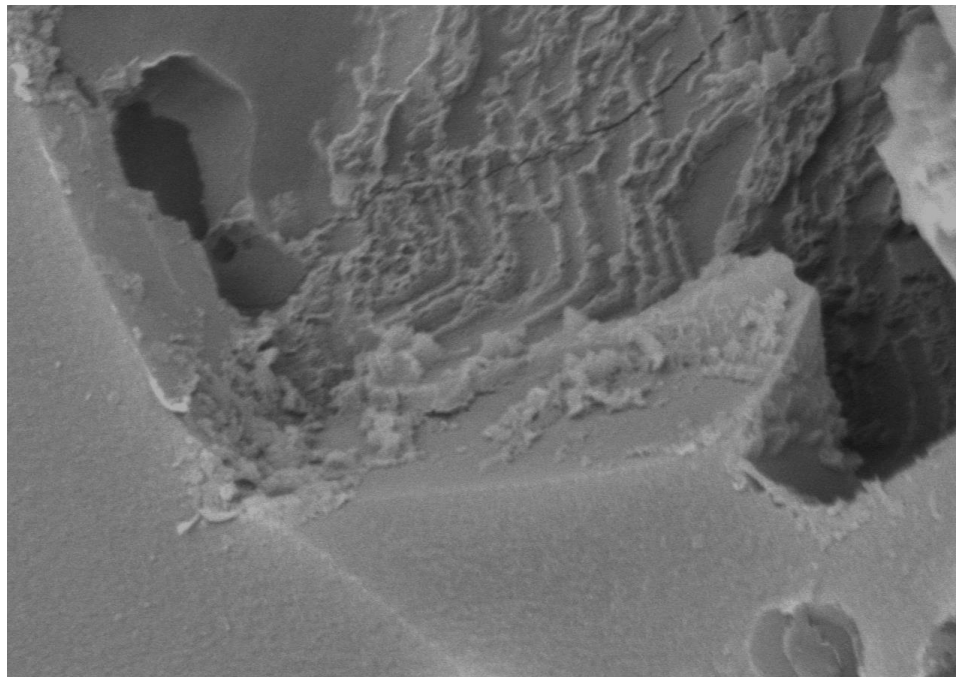

Clariant SU7000 5.00kV 5.5mm x25.0k UD+LD+MD 08/28/2024 2.00µm

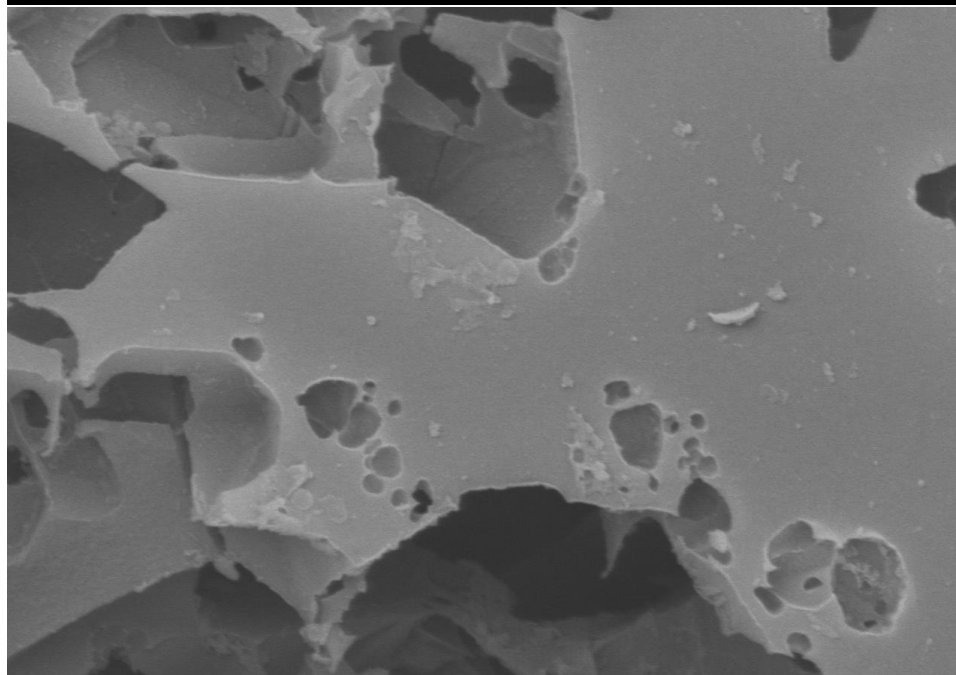

Clariant SU7000 5.00kV 5.7mm x25.0k UD+LD+MD 08/28/2024 2.00µm