
SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

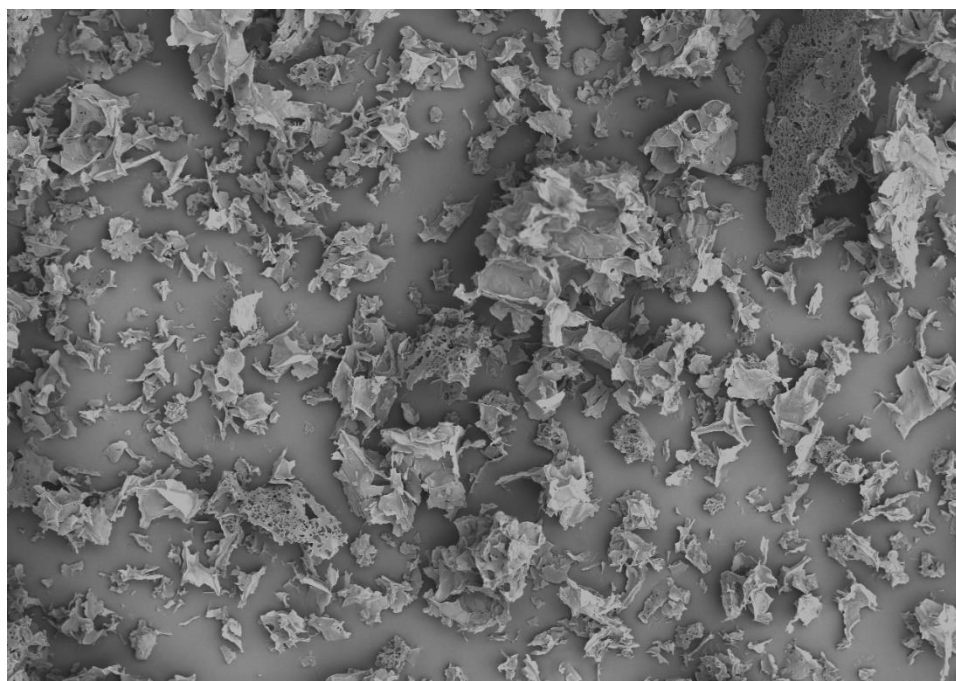

Clariant SU7000 5.00kV 5.7mm x100 UD+LD+MD 09/02/2024 500µm

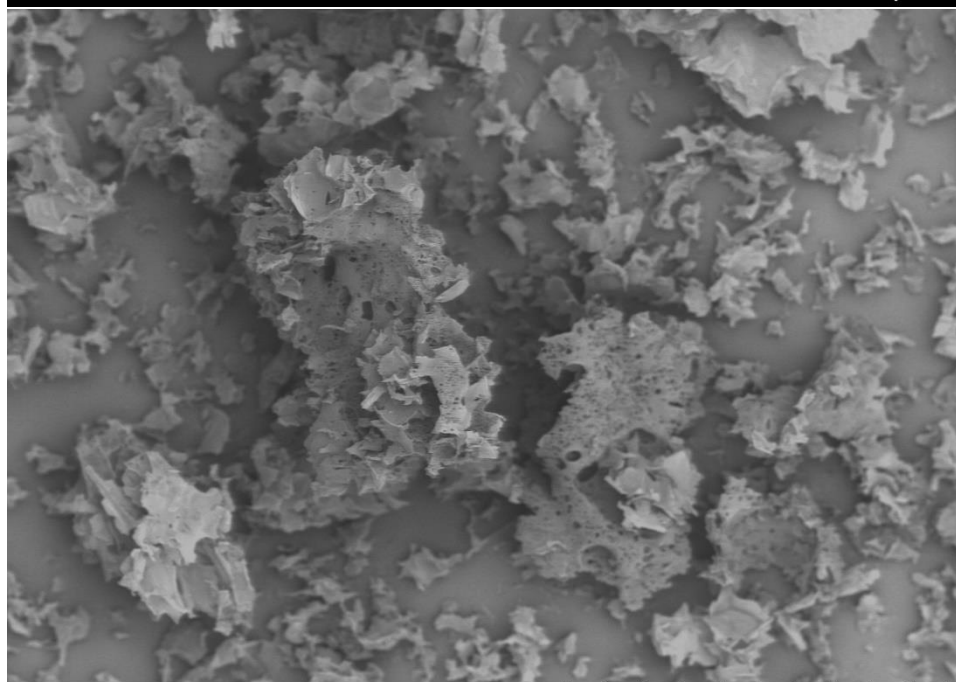


Clariant SU7000 5.00kV 5.5mm x100 UD+LD+MD 09/02/2024 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

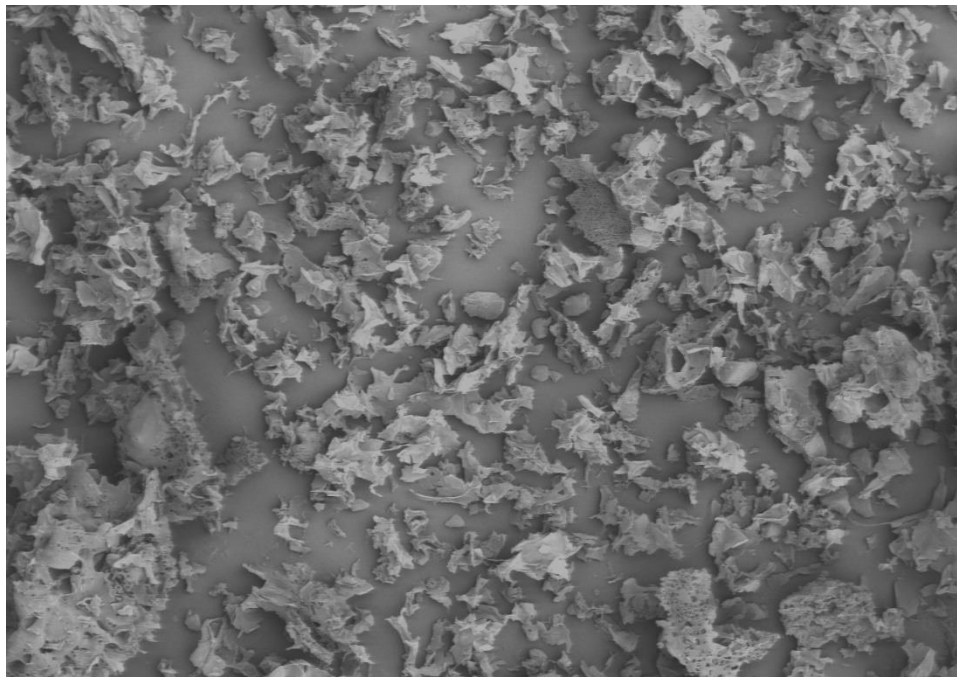

Clariant SU7000 5.00kV 5.8mm x100 UD+LD+MD 09/02/2024 500µm

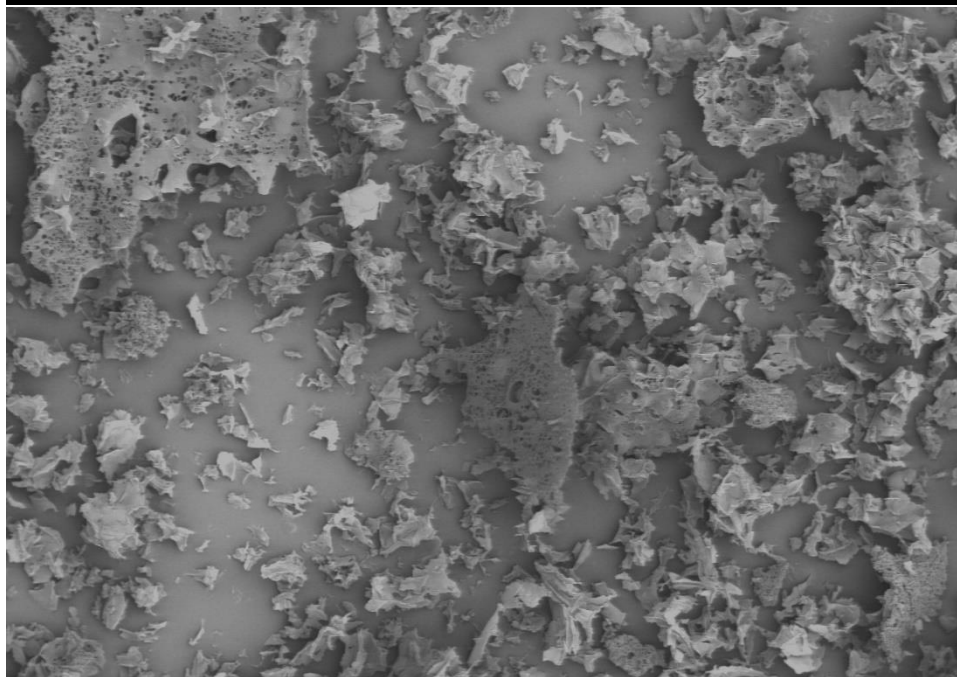


Clariant SU7000 5.00kV 5.8mm x100 UD+LD+MD 09/02/2024 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

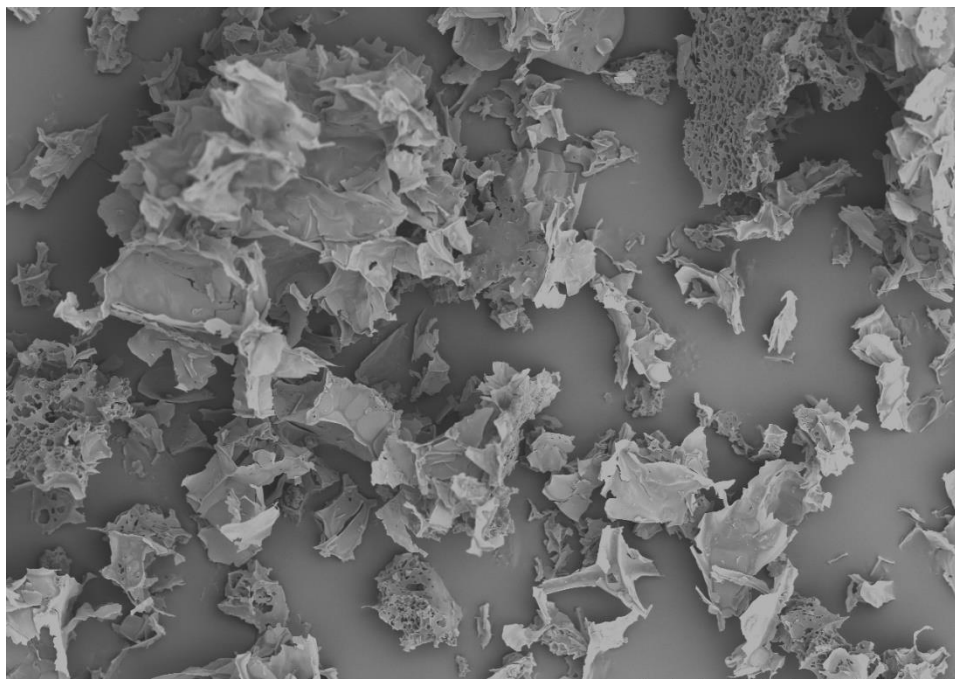

Clariant SU7000 5.00kV 5.7mm x200 UD+LD+MD 09/02/2024 200µm

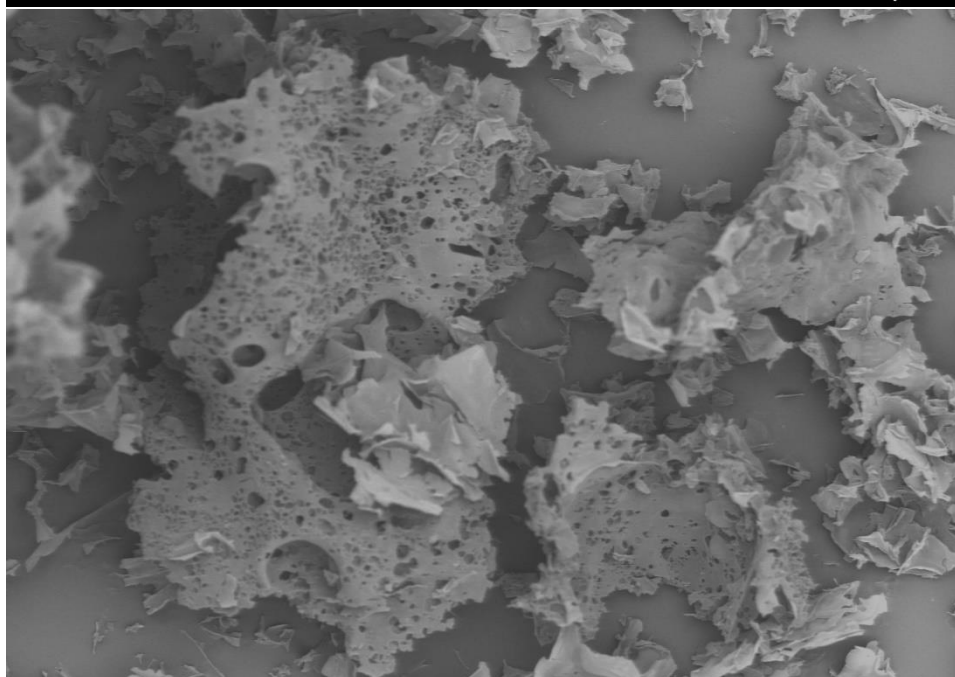


Clariant SU7000 5.00kV 6.0mm x200 UD+LD+MD 09/02/2024 200µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

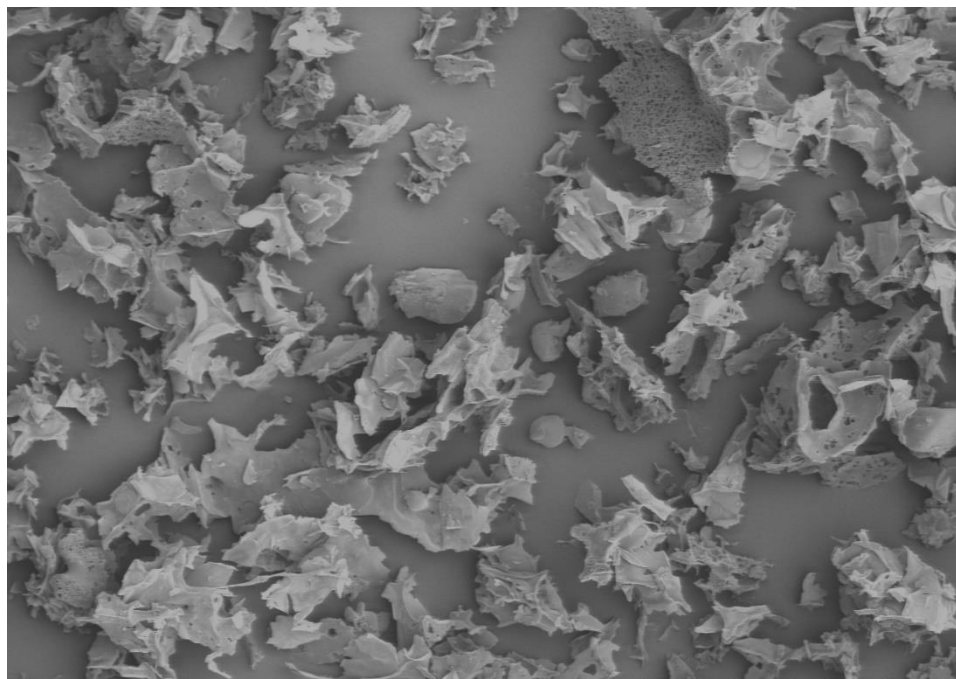

Clariant SU7000 5.00kV 5.8mm x200 UD+LD+MD 09/02/2024 200μm

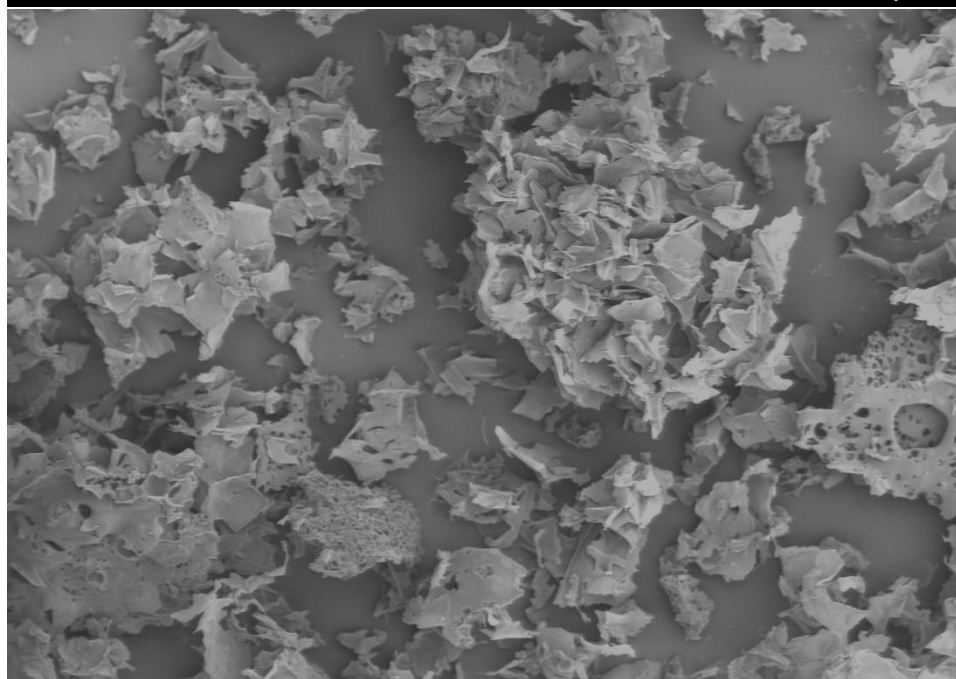


Clariant SU7000 5.00kV 5.8mm x200 UD+LD+MD 09/02/2024 200μm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

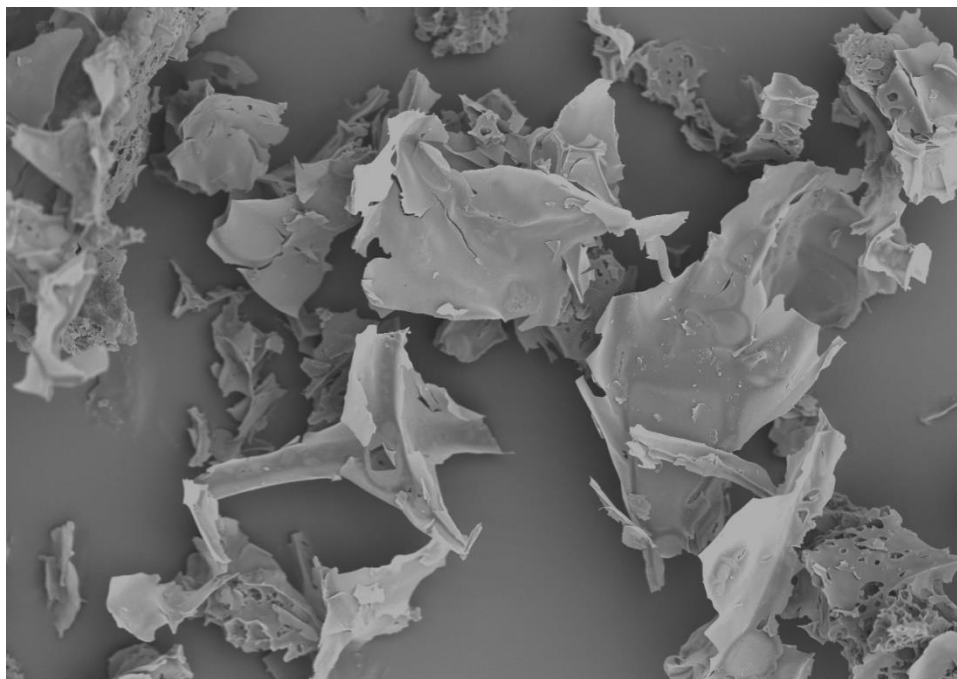

Clariant SU7000 5.00kV 5.7mm x500 UD+LD+MD 09/02/2024 100µm

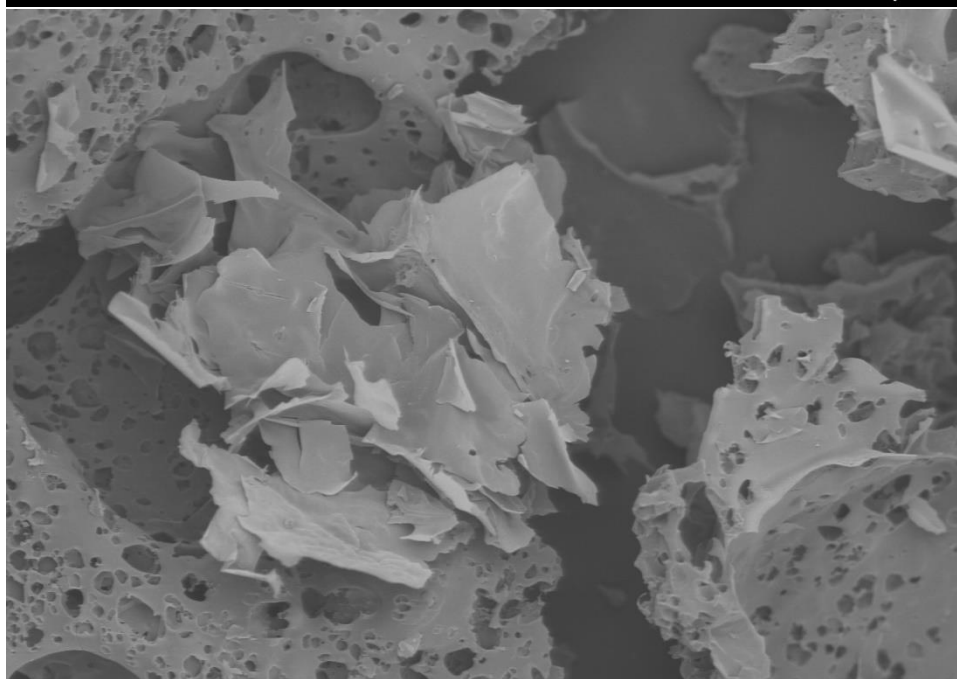


Clariant SU7000 5.00kV 5.9mm x500 UD+LD+MD 09/02/2024 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

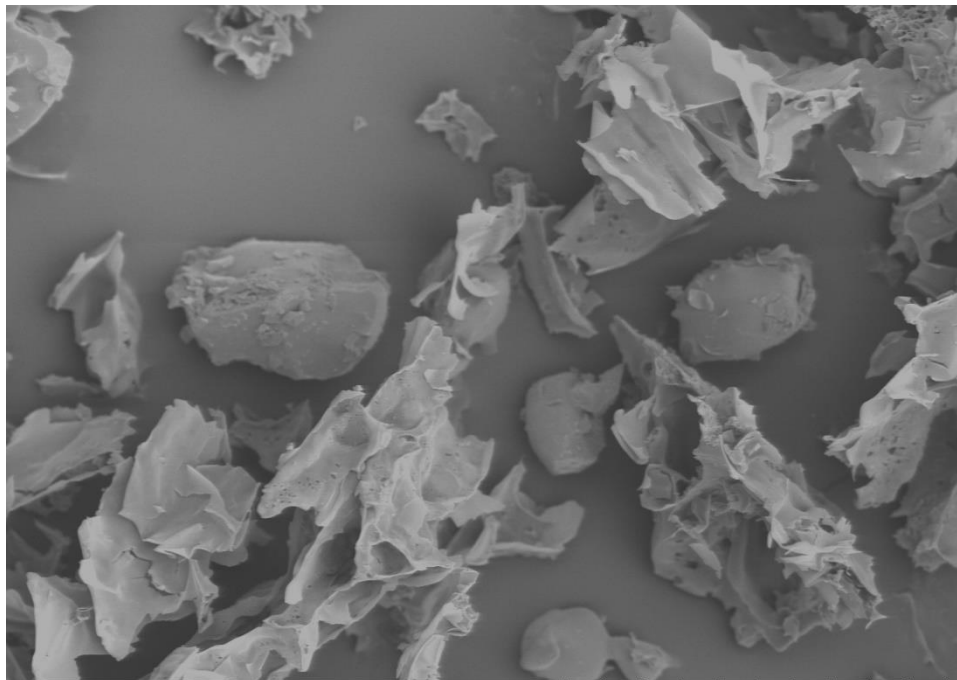

Clariant SU7000 5.00kV 5.8mm x500 UD+LD+MD 09/02/2024 100µm

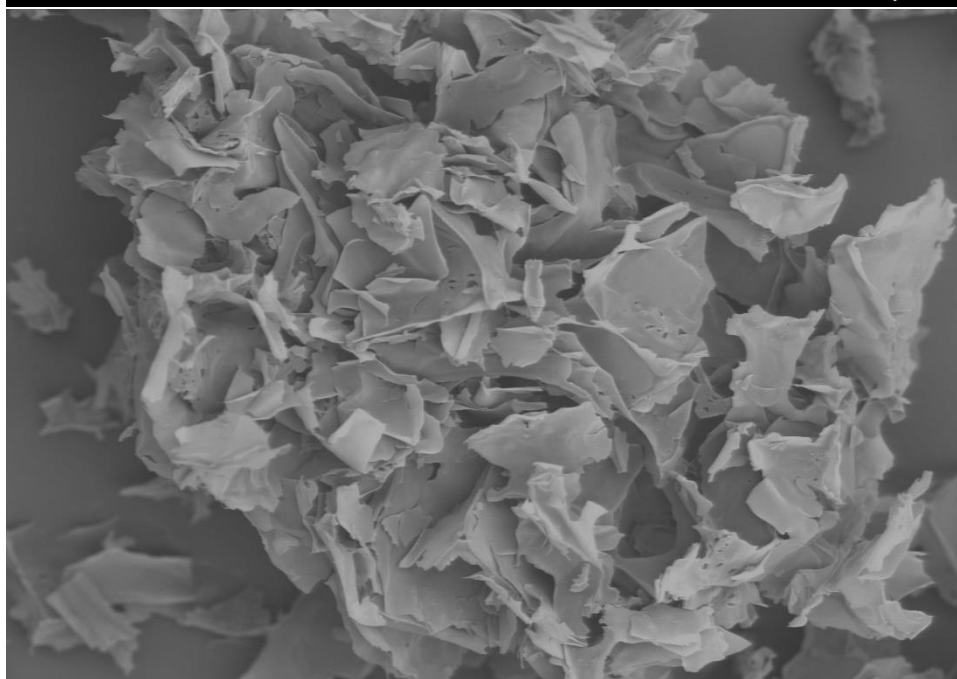


Clariant SU7000 5.00kV 5.8mm x500 UD+LD+MD 09/02/2024 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

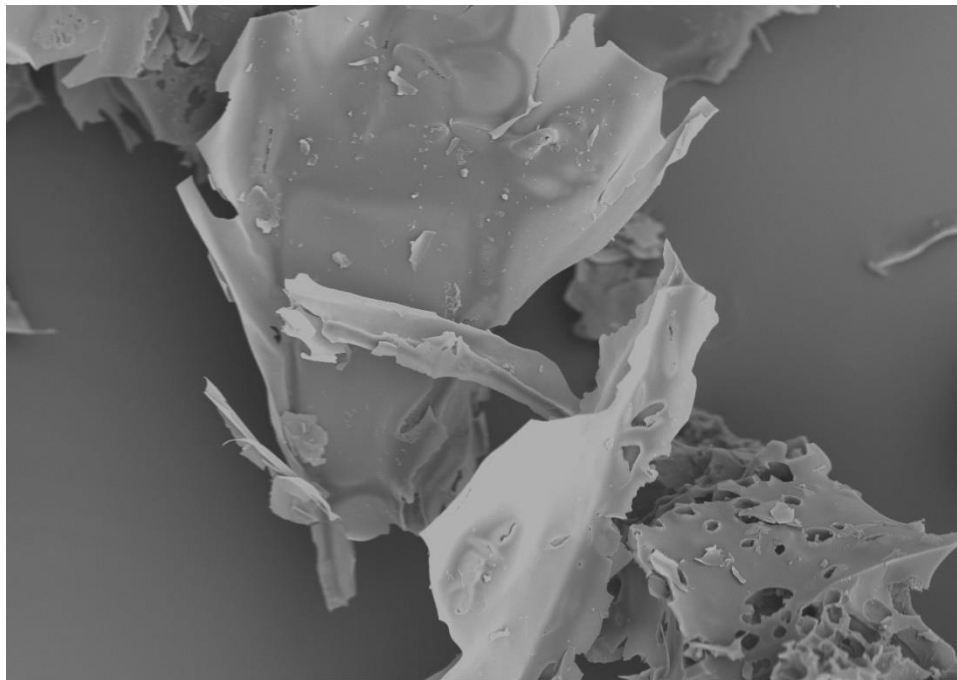

Clariant SU7000 5.00kV 5.7mm x1.00k UD+LD+MD 09/02/2024 50.0µm

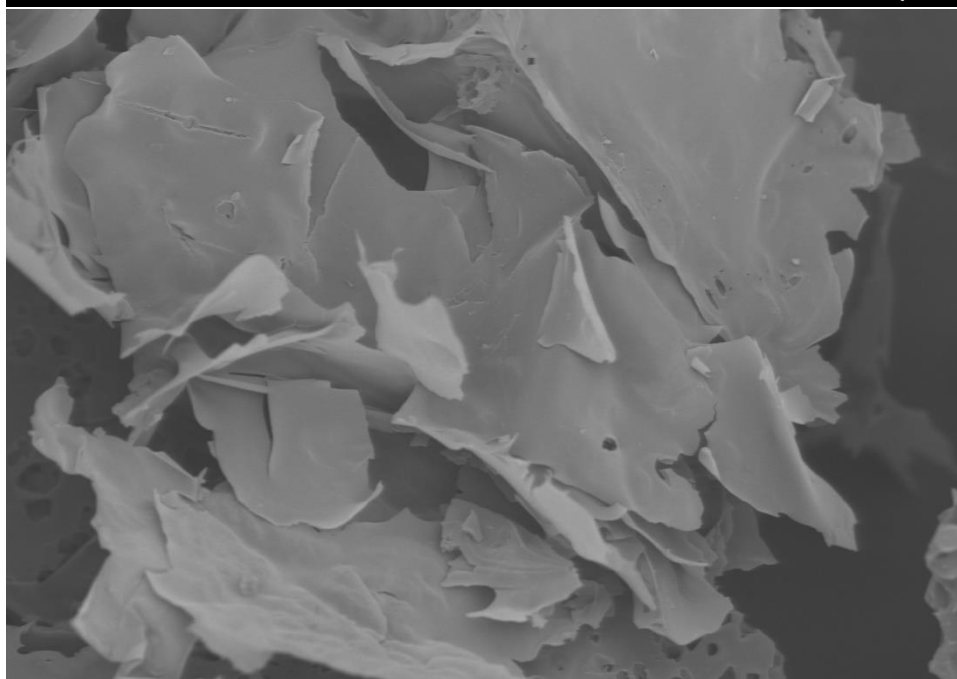


Clariant SU7000 5.00kV 5.9mm x1.00k UD+LD+MD 09/02/2024 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

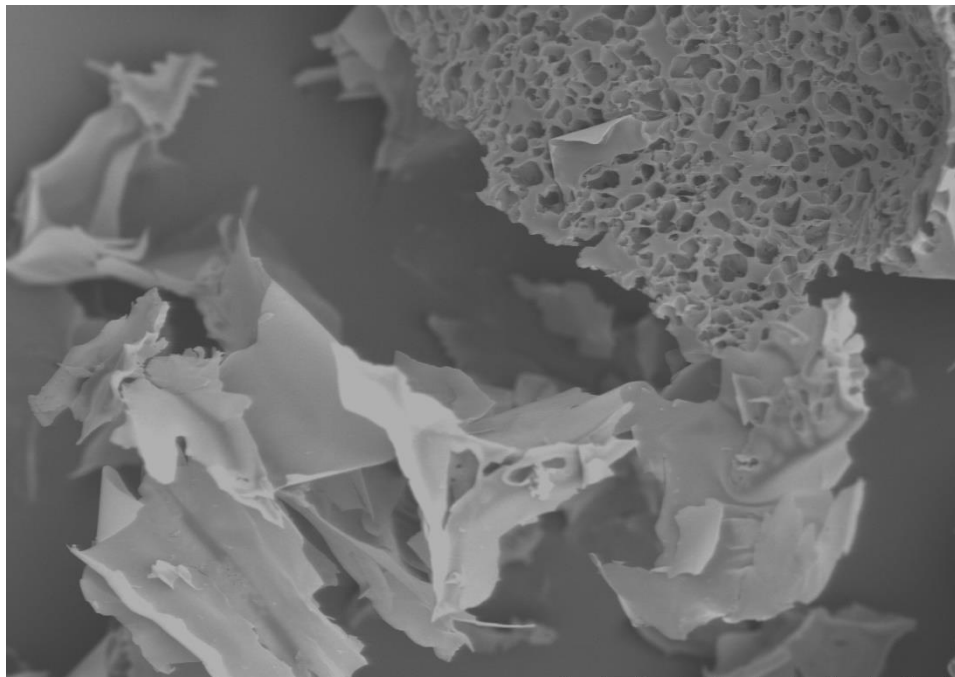

Clariant SU7000 5.00kV 5.8mm x1.00k UD+LD+MD 09/02/2024 50.0µm

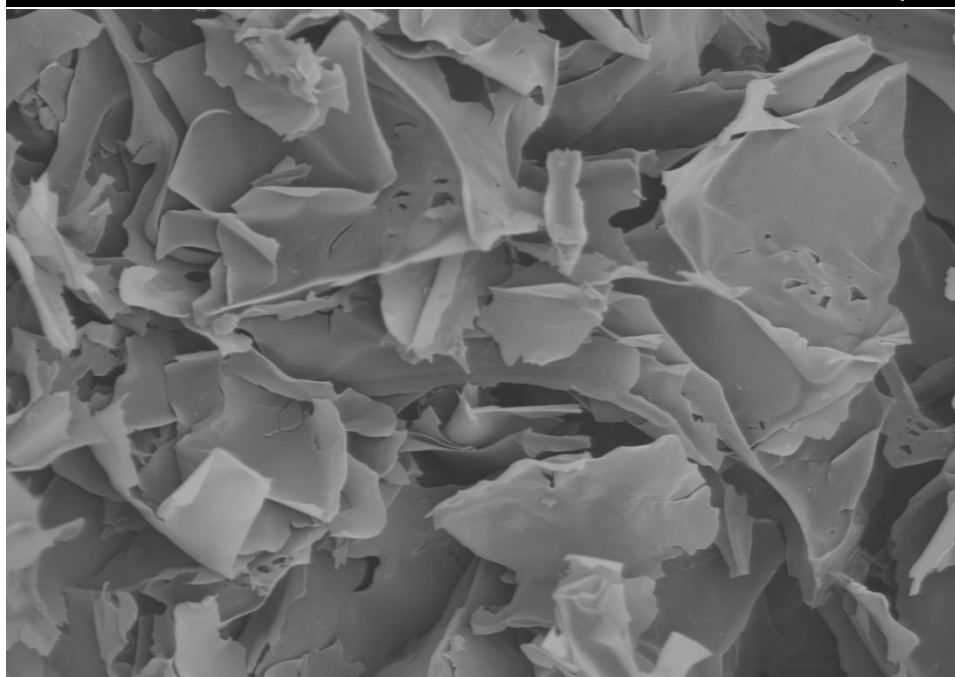


Clariant SU7000 5.00kV 5.8mm x1.00k UD+LD+MD 09/02/2024 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

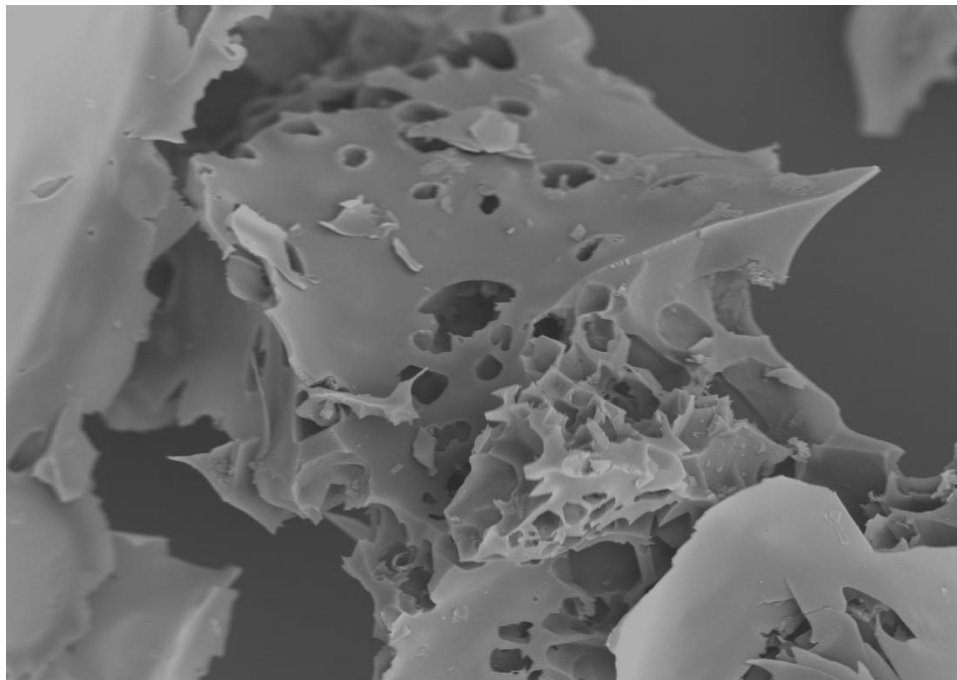

Clariant SU7000 5.00kV 5.7mm x2.00k UD+LD+MD 09/02/2024 20.0µm

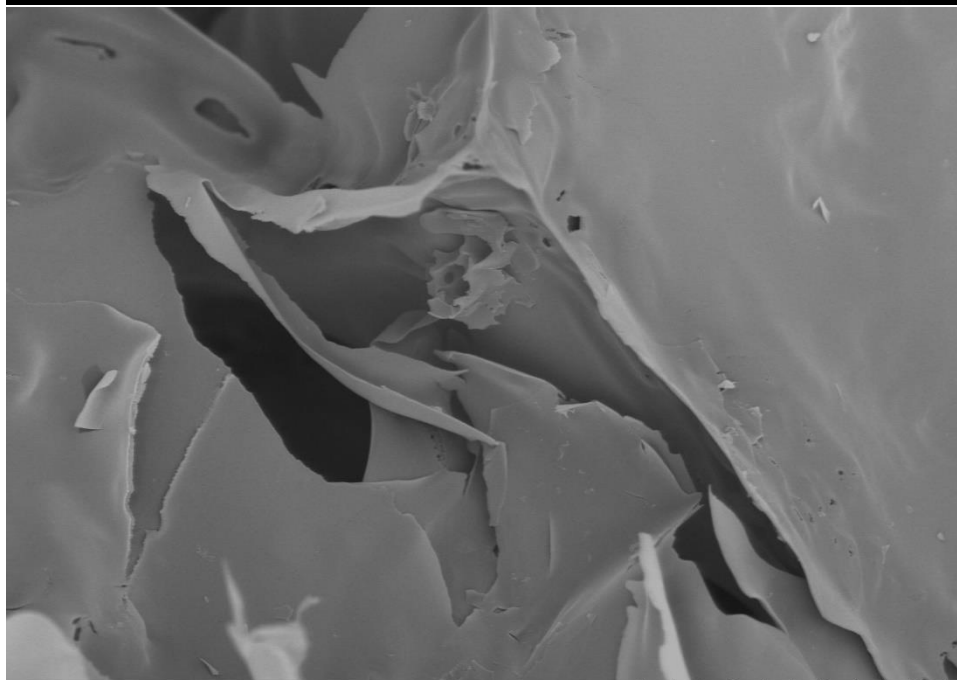


Clariant SU7000 5.00kV 5.9mm x2.00k UD+LD+MD 09/02/2024 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

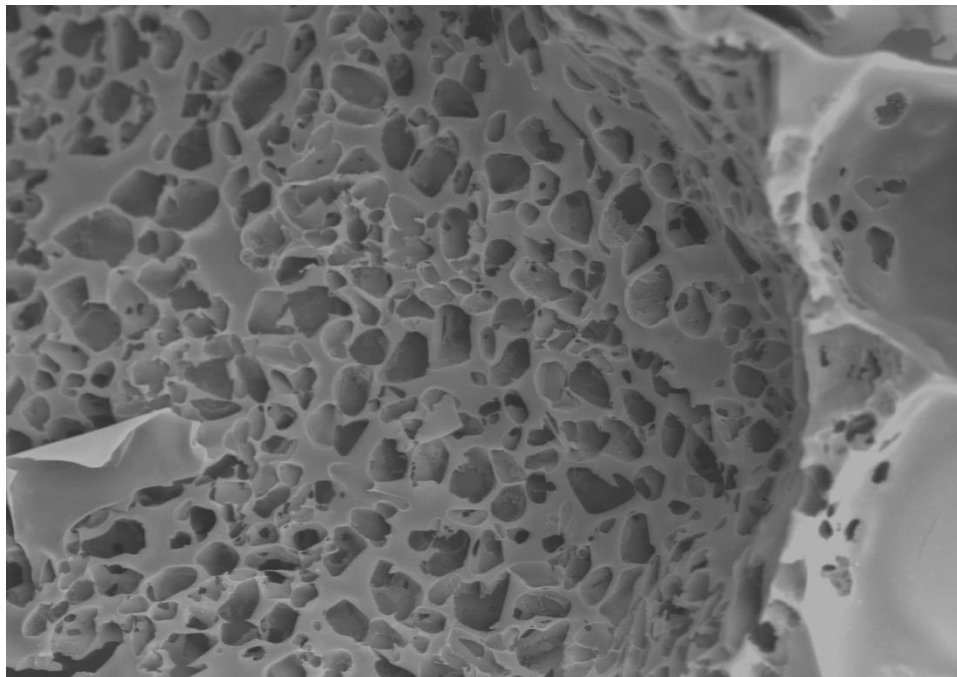

Clariant SU7000 5.00kV 5.8mm x2.00k UD+LD+MD 09/02/2024 20.0μm

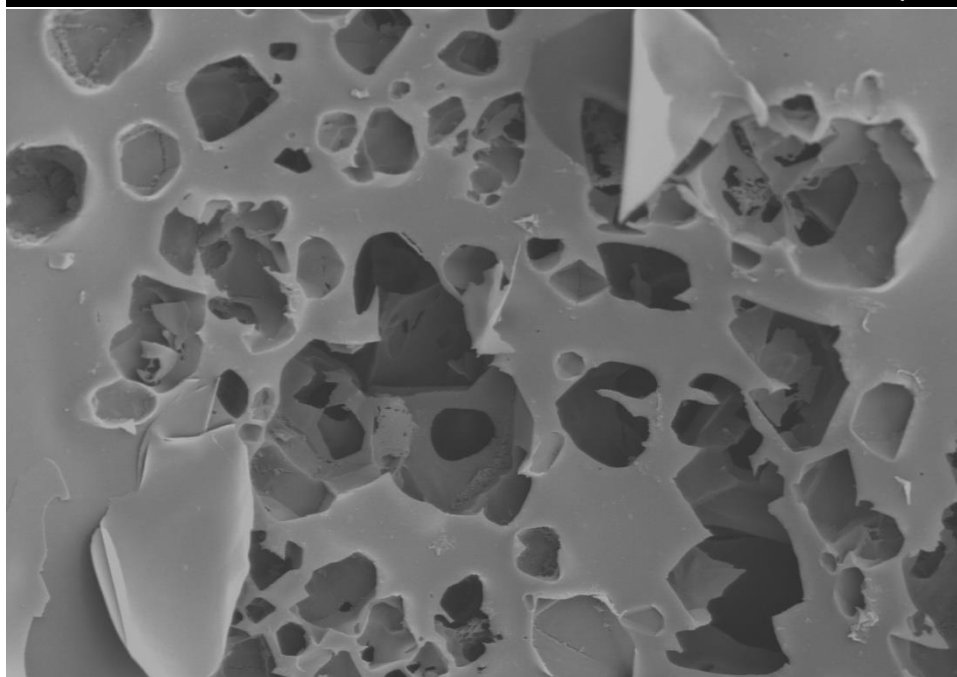


Clariant SU7000 5.00kV 5.8mm x2.00k UD+LD+MD 09/02/2024 20.0μm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

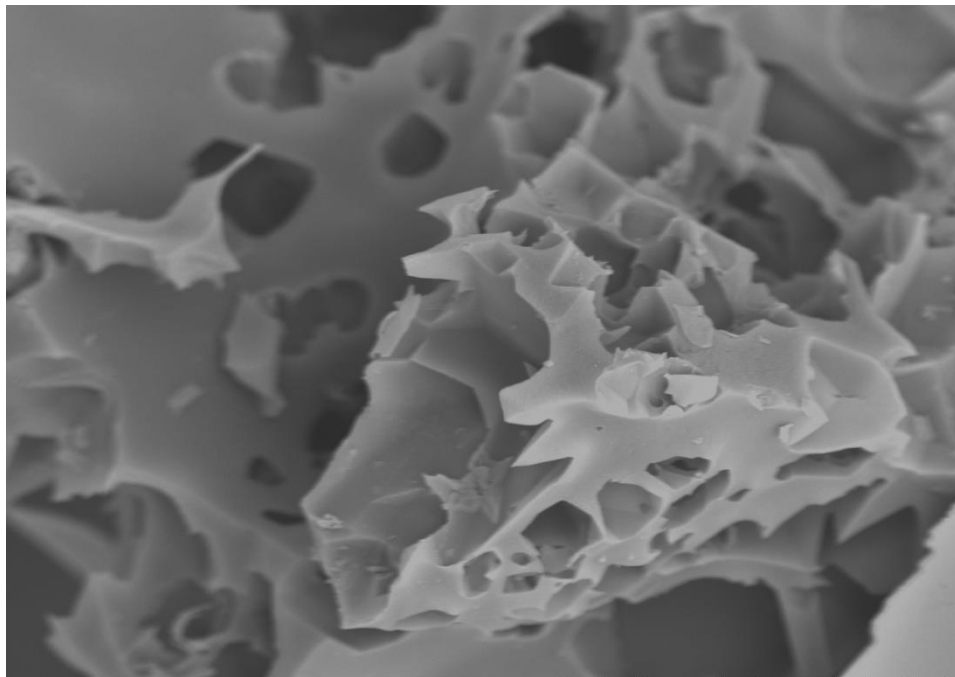

Clariant SU7000 5.00kV 5.7mm x5.00k UD+LD+MD 09/02/2024 10.0μm

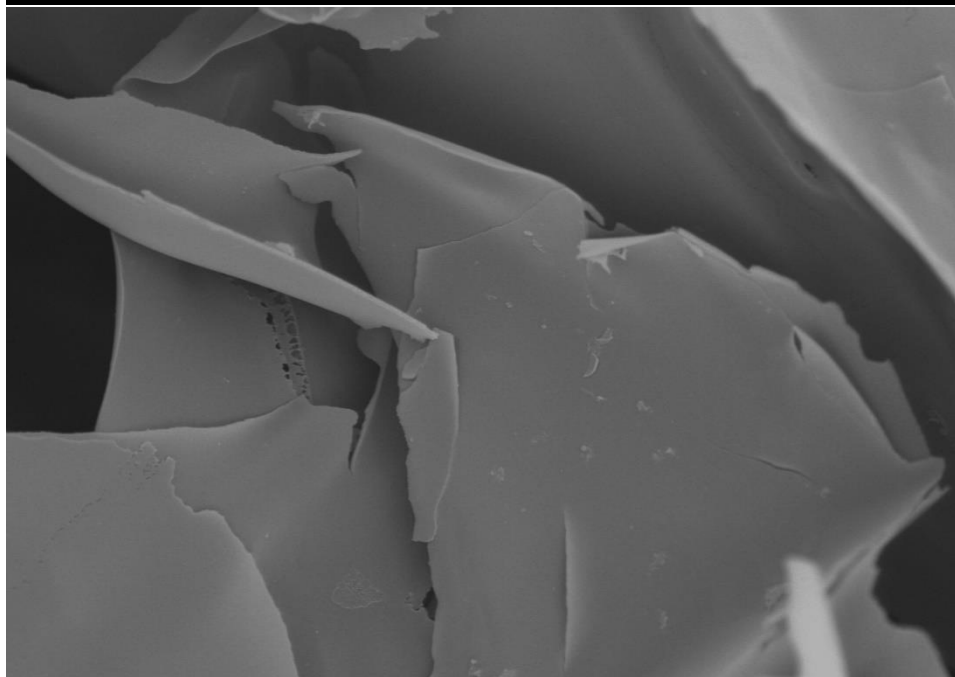


Clariant SU7000 5.00kV 5.9mm x5.00k UD+LD+MD 09/02/2024 10.0μm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

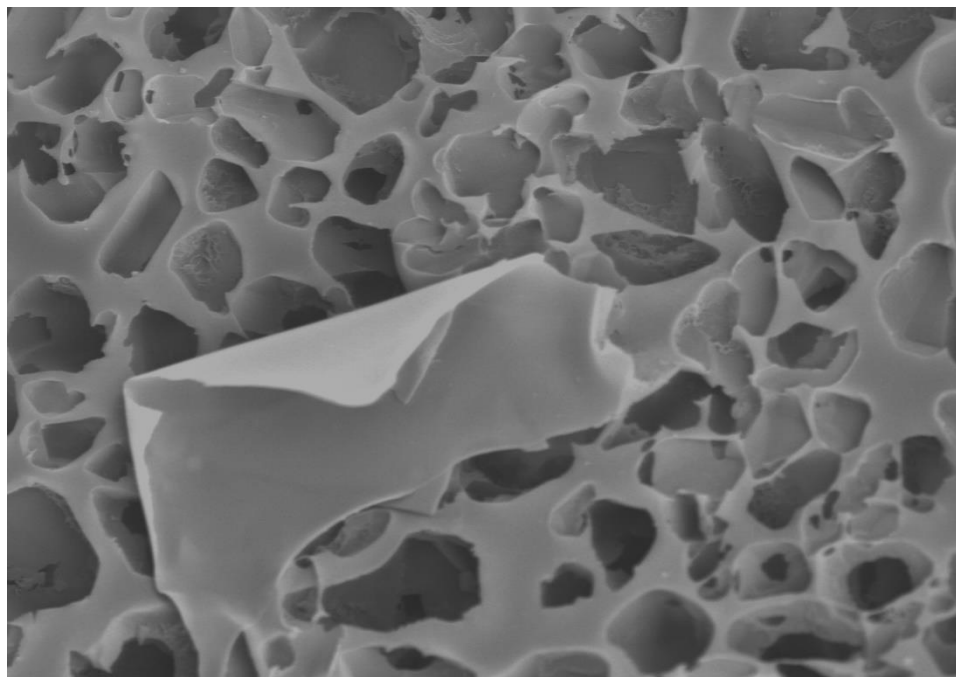

Clariant SU7000 5.00kV 5.9mm x5.00k UD+LD+MD 09/02/2024 10.0µm

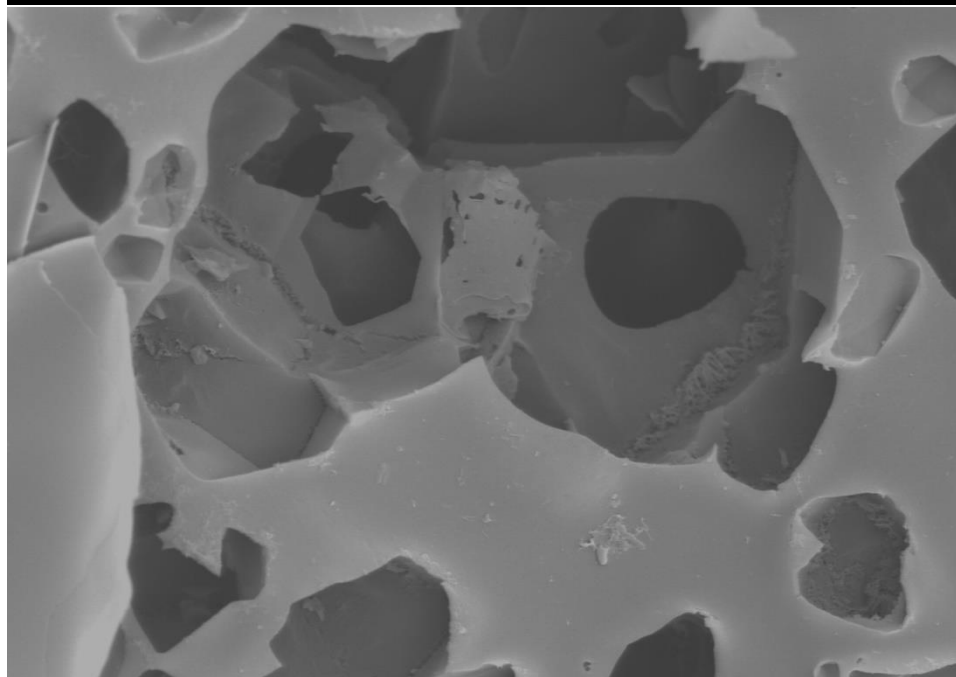


Clariant SU7000 5.00kV 5.8mm x5.00k UD+LD+MD 09/02/2024 10.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

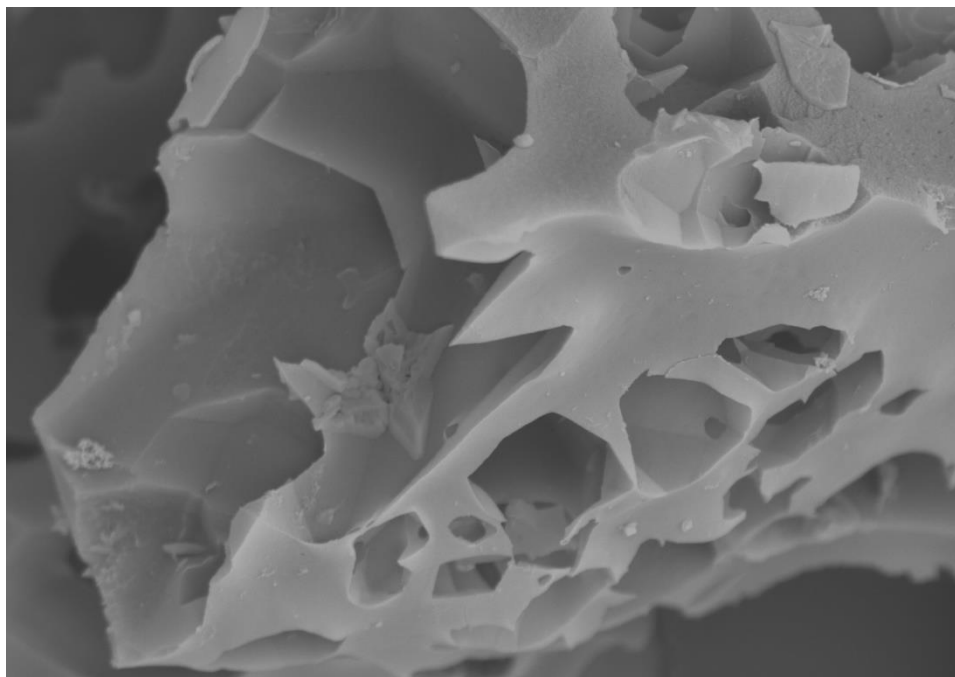

Clariant SU7000 5.00kV 5.7mm x10.0k UD+LD+MD 09/02/2024 5.00µm

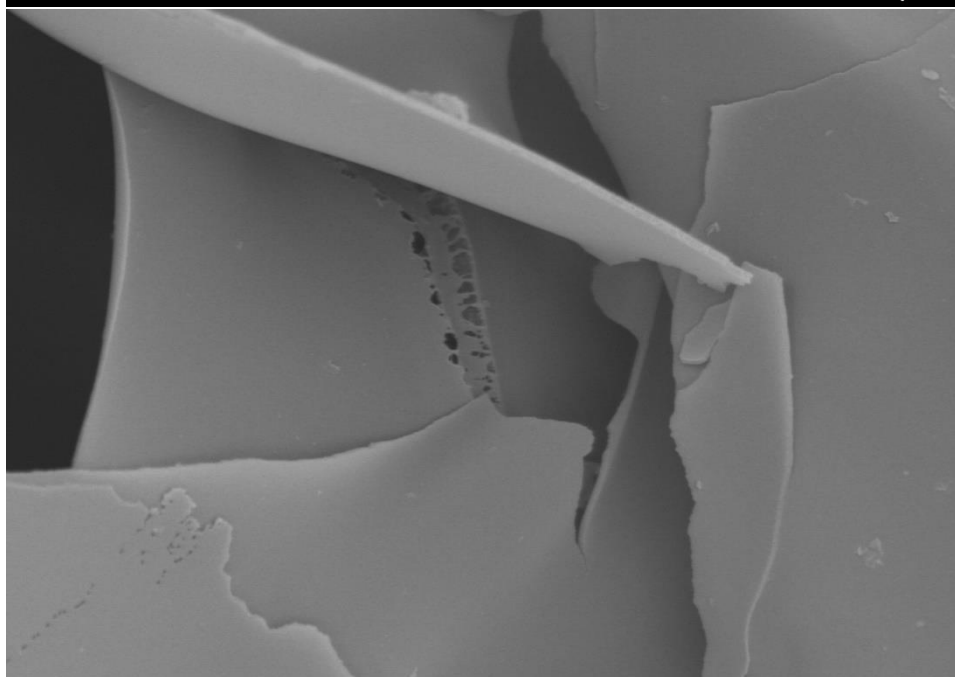


Clariant SU7000 5.00kV 5.9mm x10.0k UD+LD+MD 09/02/2024 5.00µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

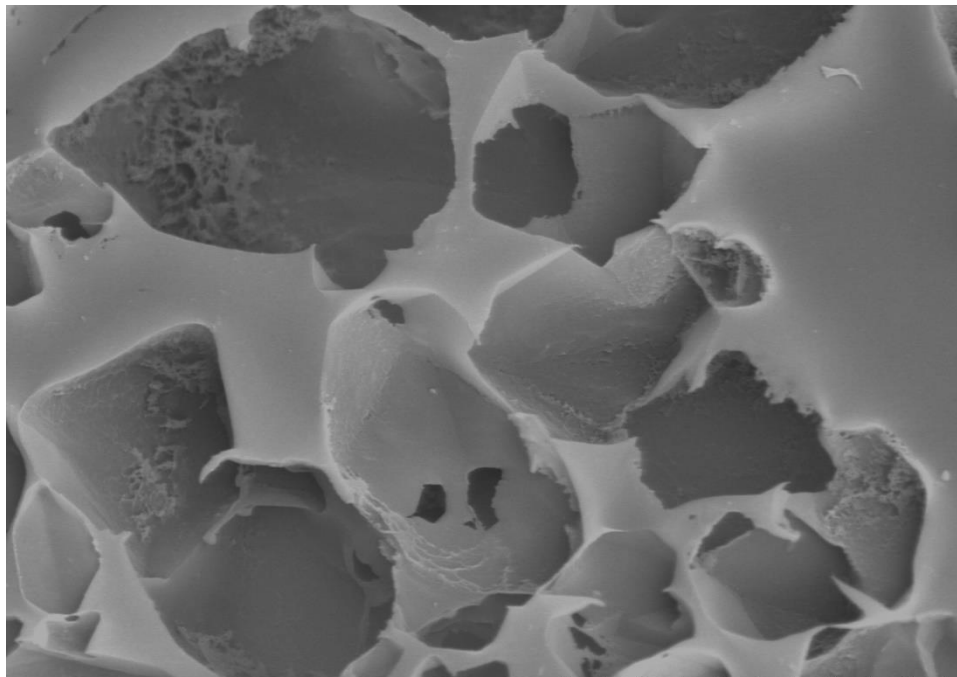

Clariant SU7000 5.00kV 5.9mm x10.0k UD+LD+MD 09/02/2024 5.00µm

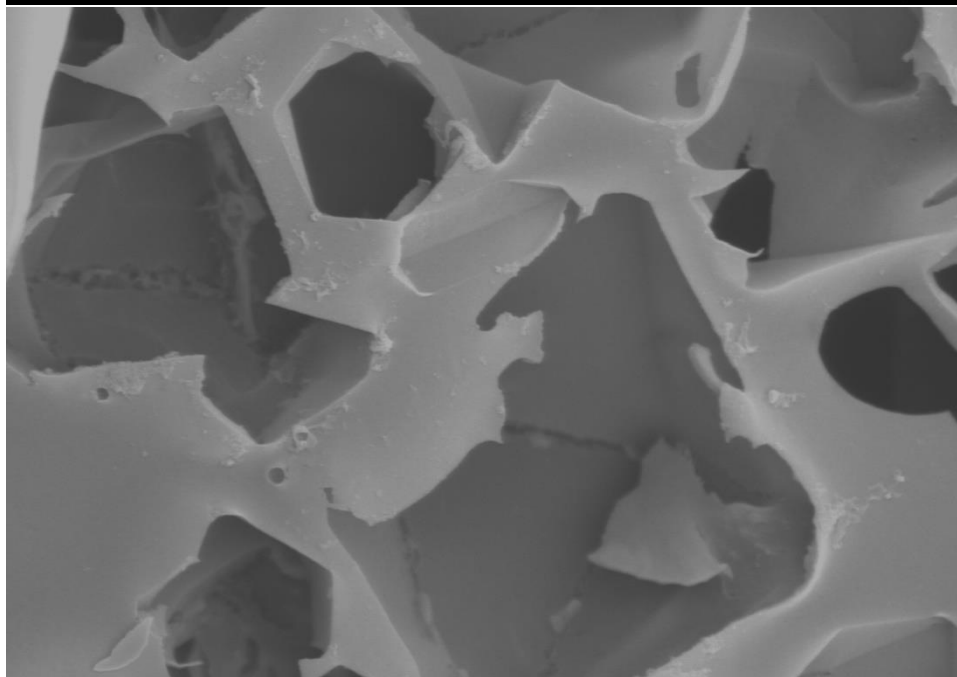


Clariant SU7000 5.00kV 5.8mm x10.0k UD+LD+MD 09/02/2024 5.00µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

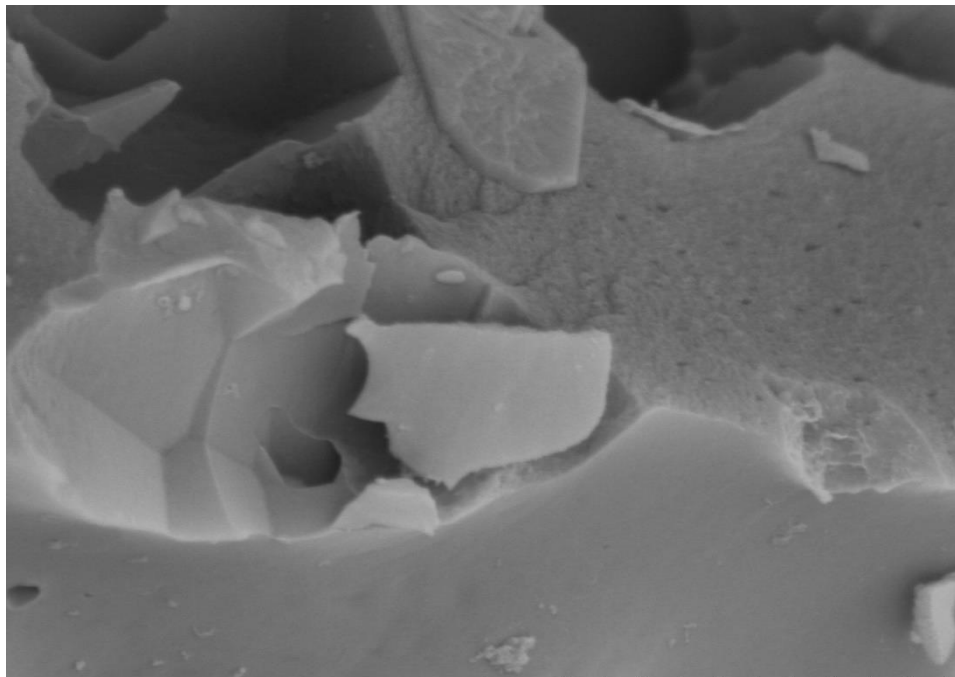

Clariant SU7000 5.00kV 5.7mm x25.0k UD+LD+MD 09/02/2024 2.00μm

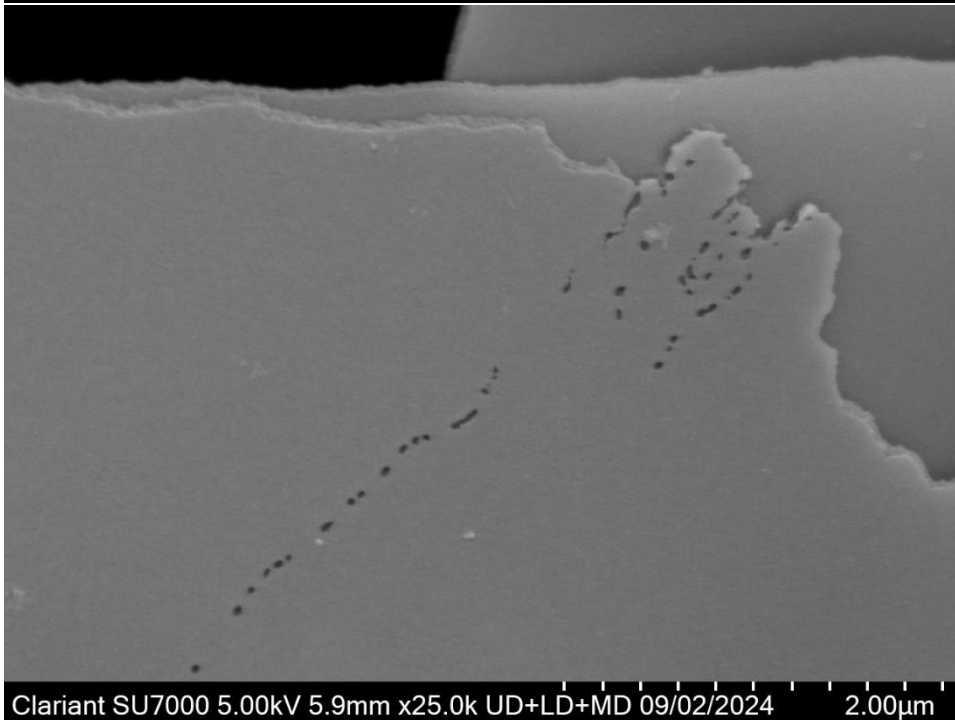


Clariant SU7000 5.00kV 5.9mm x25.0k UD+LD+MD 09/02/2024 2.00μm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0166A 2/3 10m 800C 10C/m 1h A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047917-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

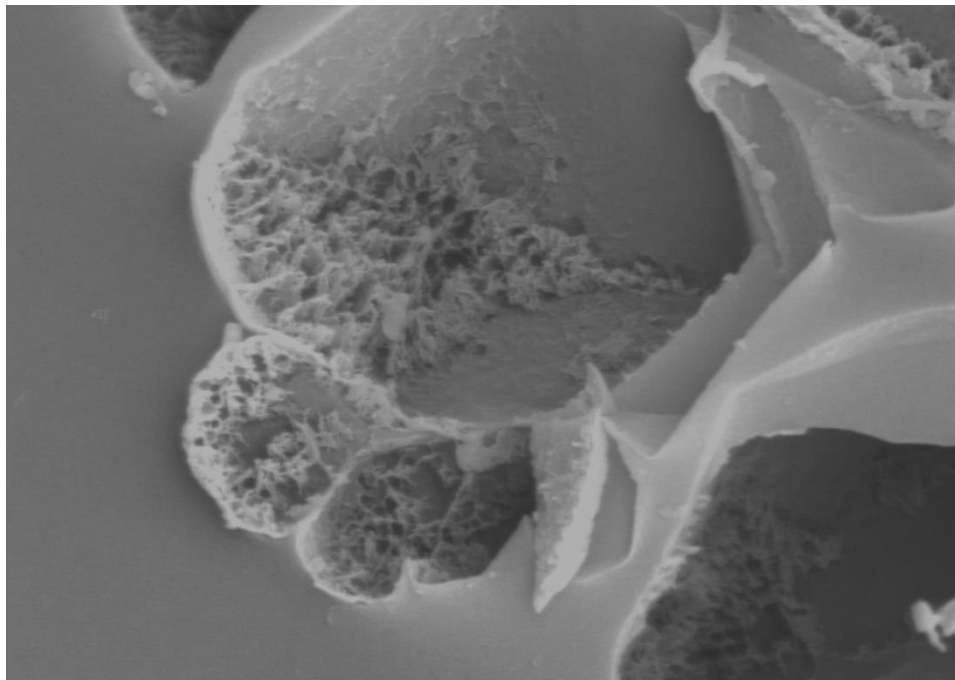

Clariant SU7000 5.00kV 5.8mm x25.0k UD+LD+MD 09/02/2024 2.00μm

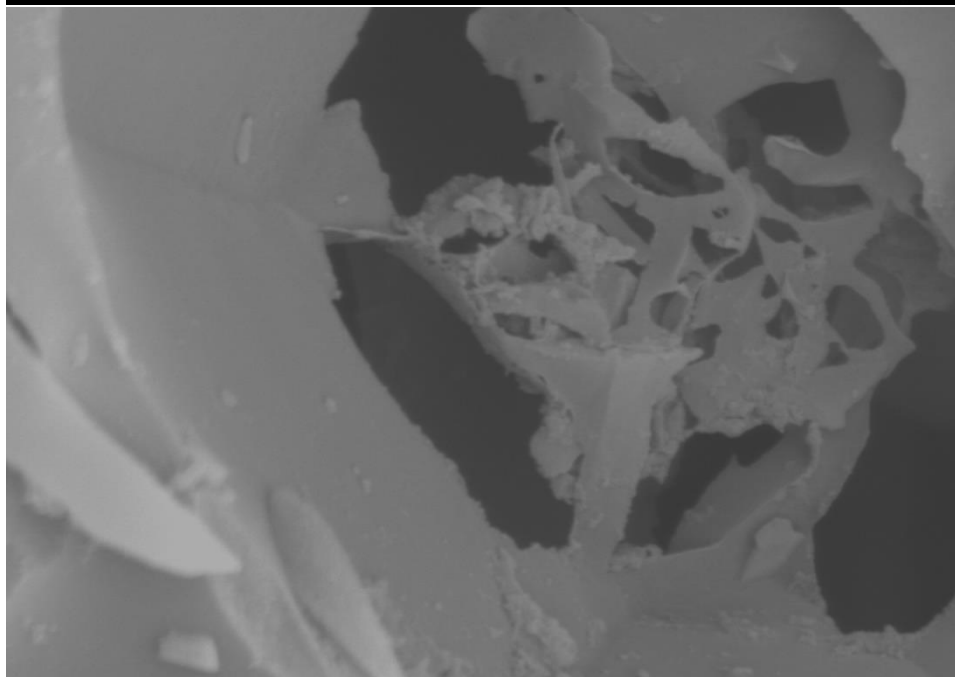

Clariant SU7000 5.00kV 5.8mm x25.0k UD+LD+MD 09/02/2024 2.00μm