


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

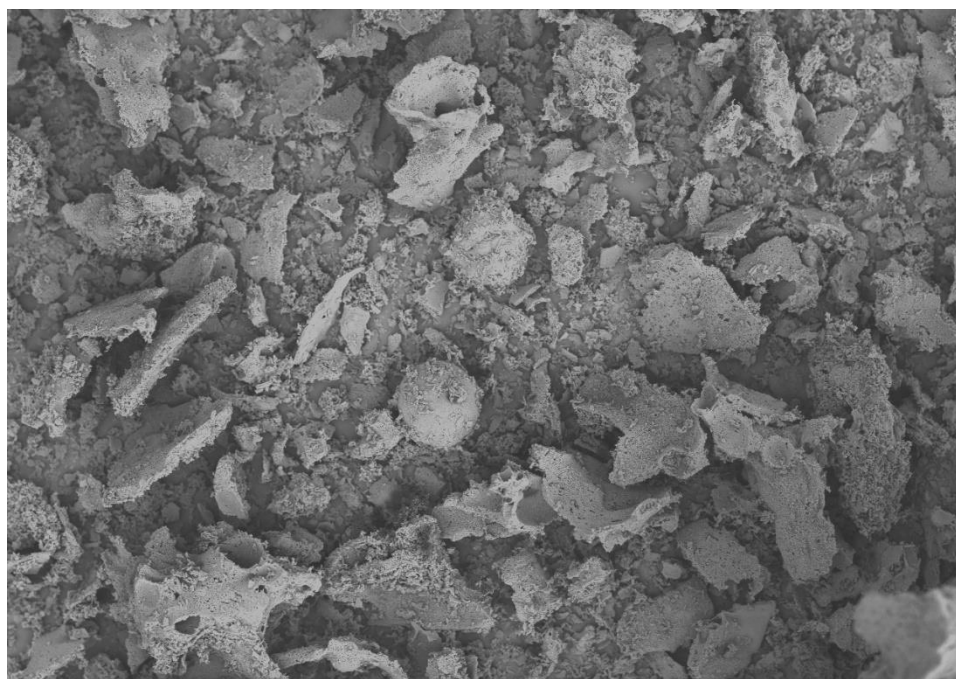

Clariant SU7000 5.00kV 6.4mm x100 UD+LD+MD 02/24/2025 500µm




Clariant SU7000 5.00kV 6.6mm x100 UD+LD+MD 02/24/2025 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

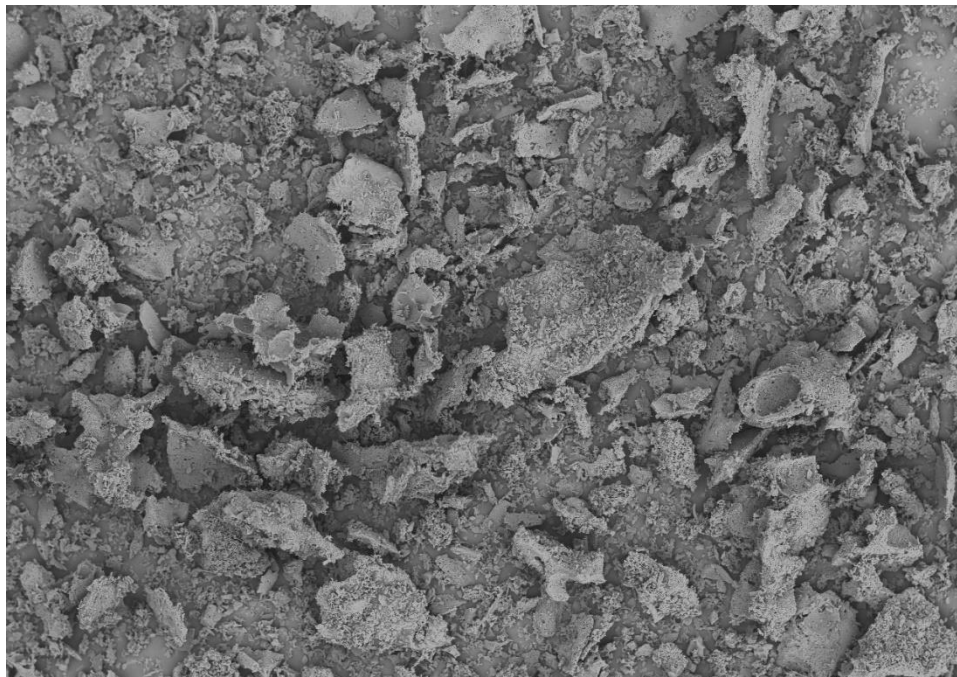

Clariant SU7000 5.00kV 6.5mm x100 UD+LD+MD 02/24/2025 500µm

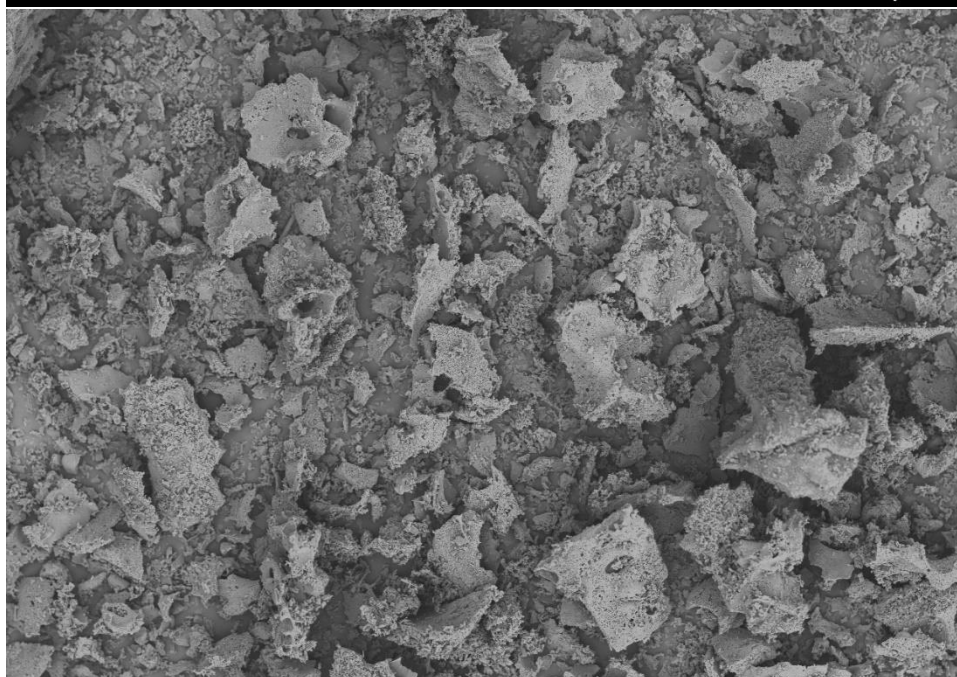


Clariant SU7000 5.00kV 6.5mm x100 UD+LD+MD 02/24/2025 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

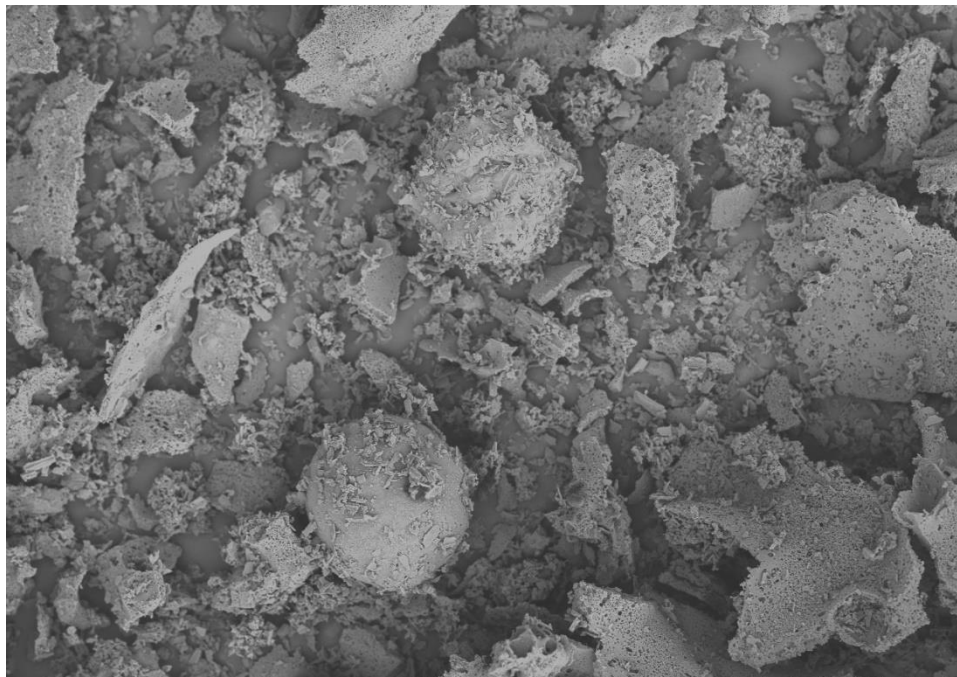

Clariant SU7000 5.00kV 6.4mm x200 UD+LD+MD 02/24/2025 200µm

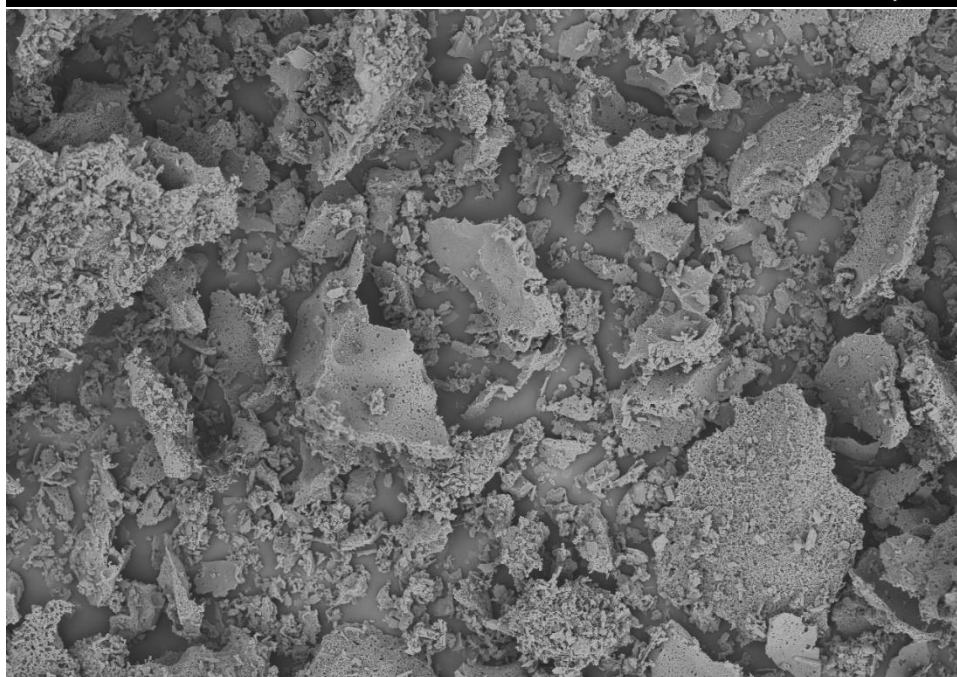


Clariant SU7000 5.00kV 6.6mm x200 UD+LD+MD 02/24/2025 200µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

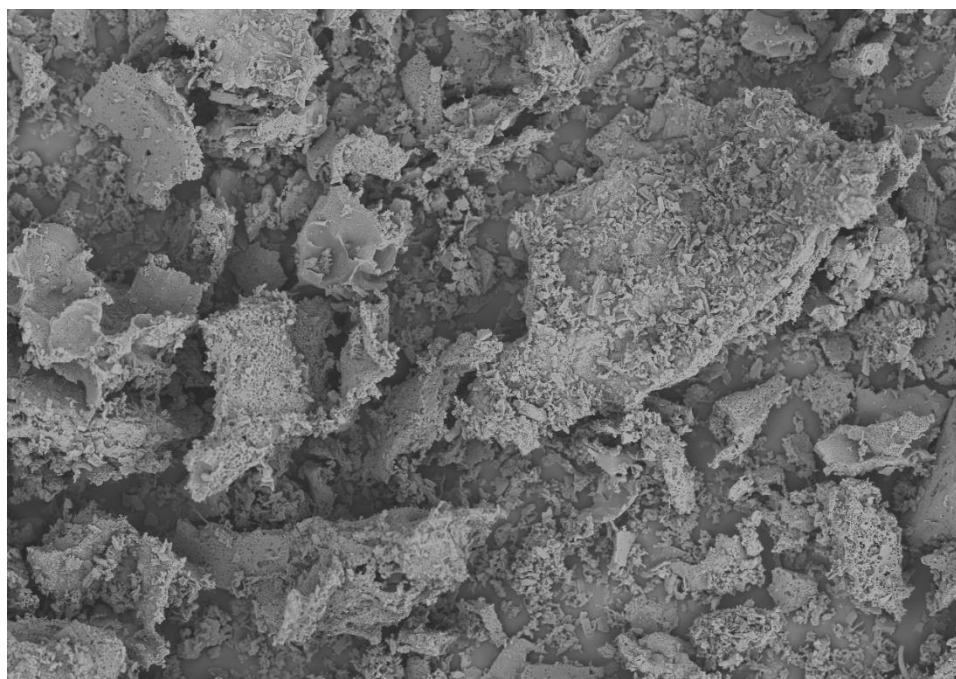

Clariant SU7000 5.00kV 6.5mm x200 UD+LD+MD 02/24/2025 200µm

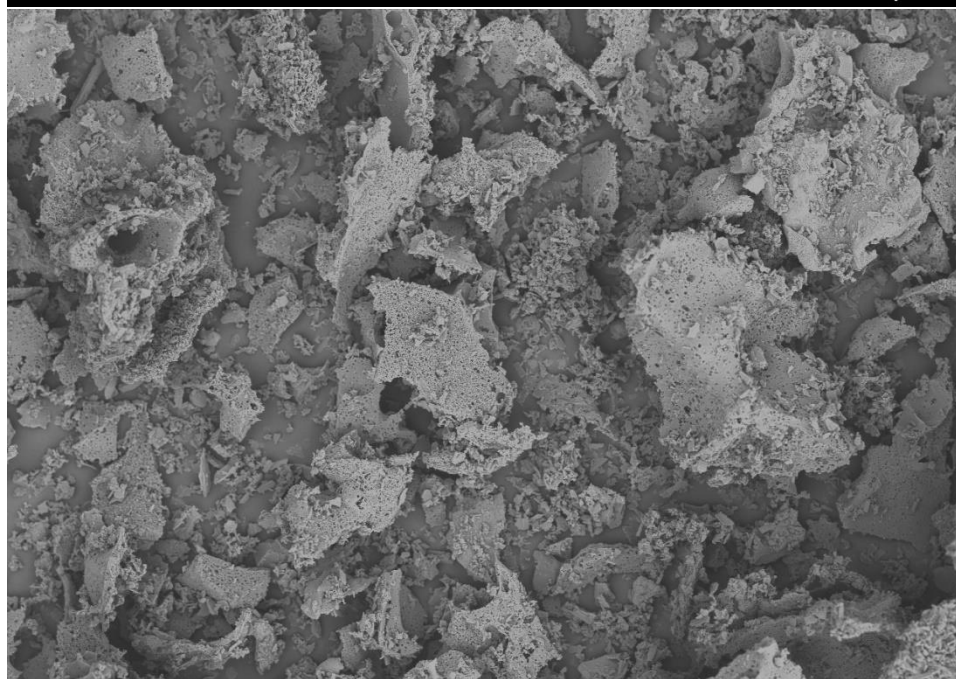

Clariant SU7000 5.00kV 6.5mm x200 UD+LD+MD 02/24/2025 200µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

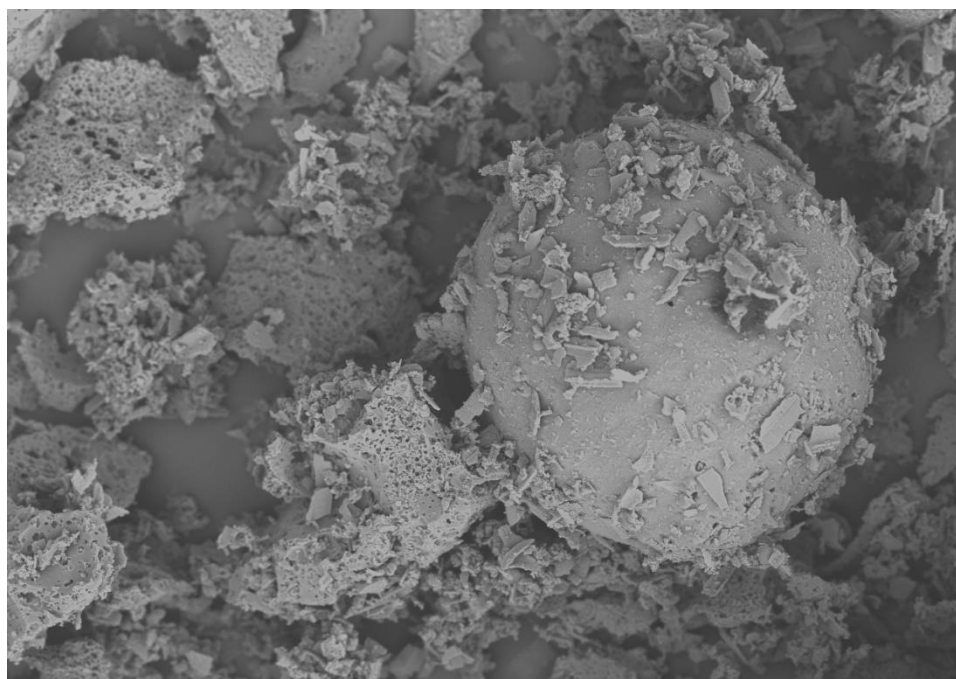

Clariant SU7000 5.00kV 6.4mm x500 UD+LD+MD 02/24/2025 100µm

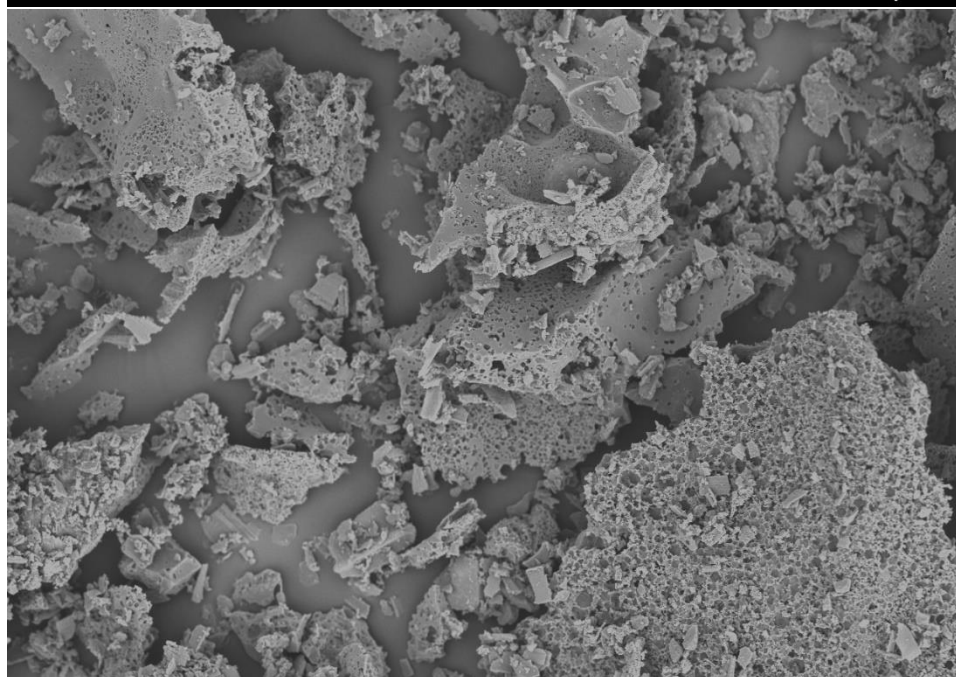


Clariant SU7000 5.00kV 6.5mm x500 UD+LD+MD 02/24/2025 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

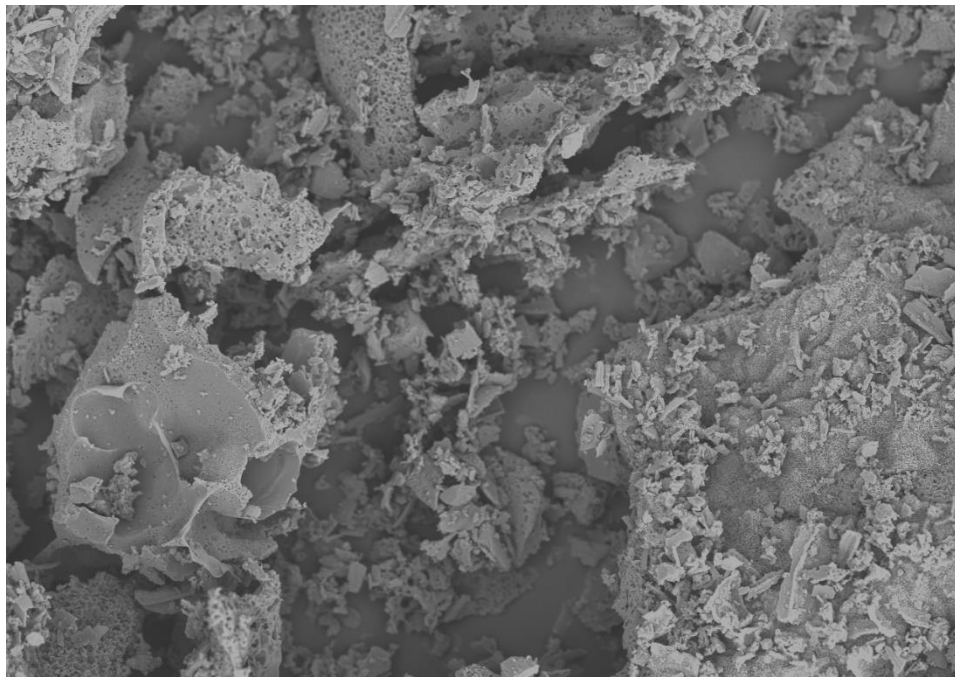

Clariant SU7000 5.00kV 6.5mm x500 UD+LD+MD 02/24/2025 100µm

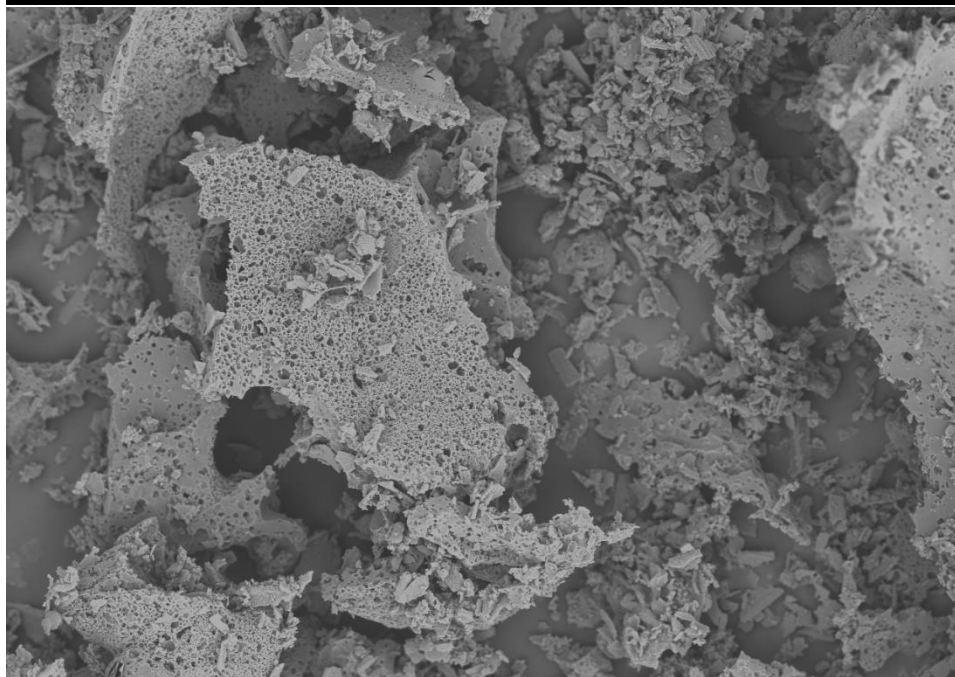


Clariant SU7000 5.00kV 6.5mm x500 UD+LD+MD 02/24/2025 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

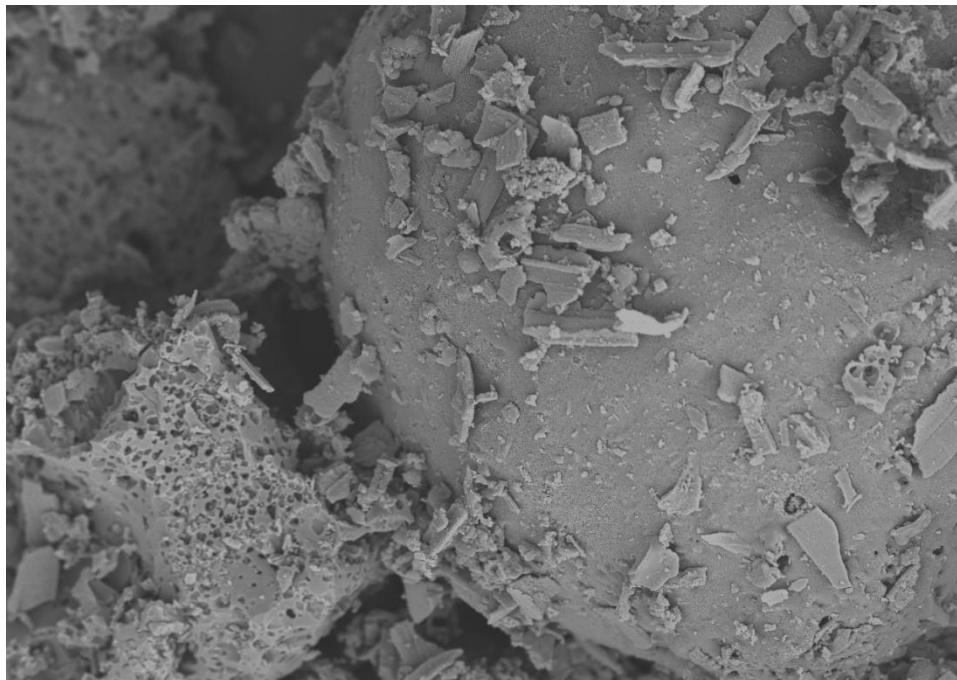

Clariant SU7000 5.00kV 6.4mm x1.00k UD+LD+MD 02/24/2025 50.0µm

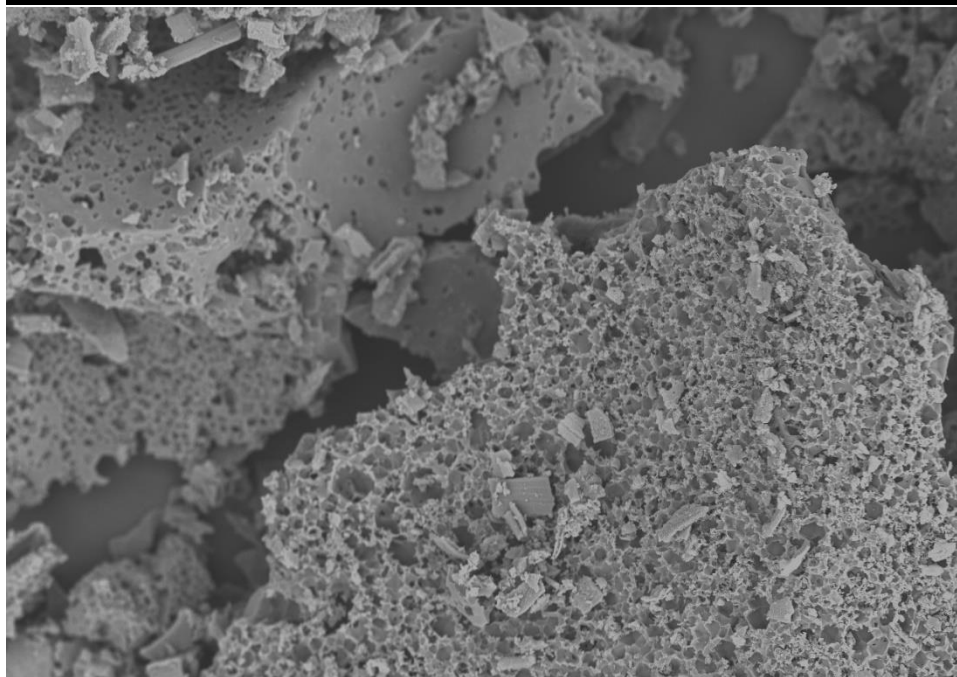


Clariant SU7000 5.00kV 6.5mm x1.00k UD+LD+MD 02/24/2025 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

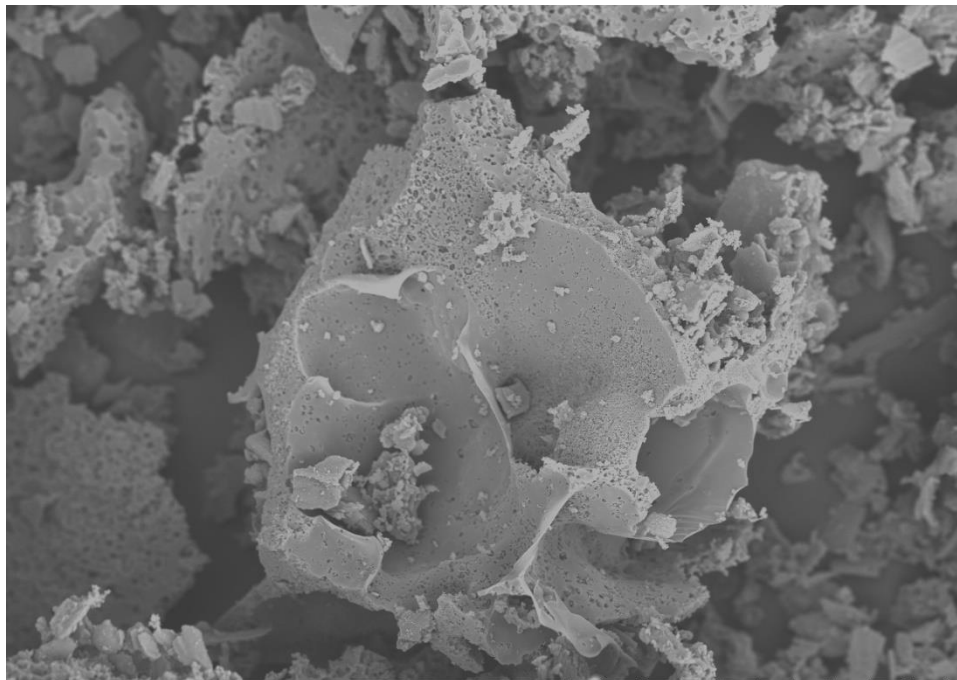

Clariant SU7000 5.00kV 6.5mm x1.00k UD+LD+MD 02/24/2025 50.0µm

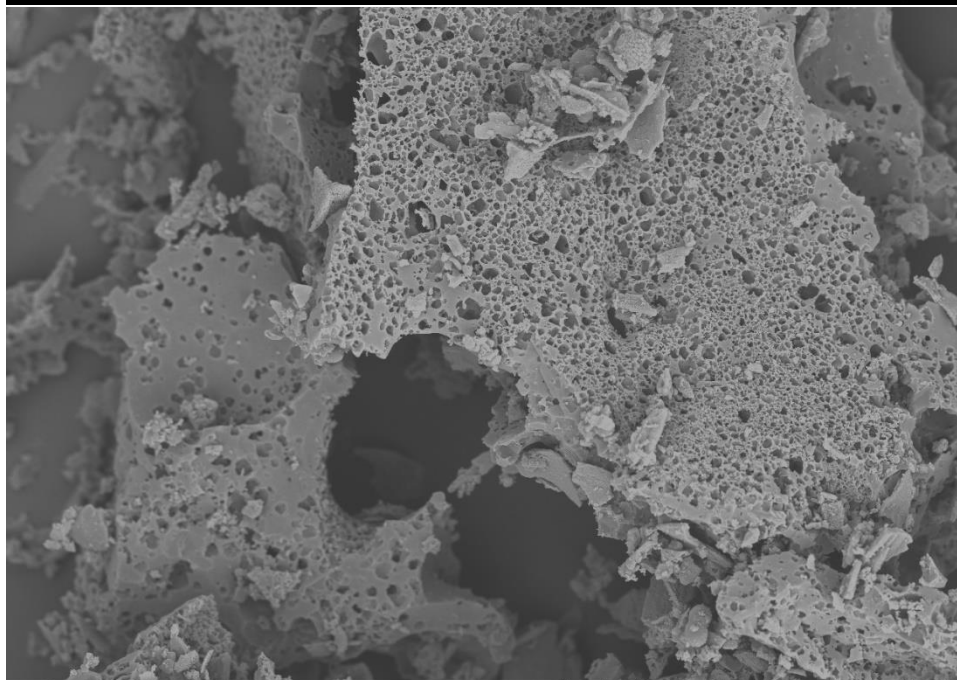


Clariant SU7000 5.00kV 6.5mm x1.00k UD+LD+MD 02/24/2025 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

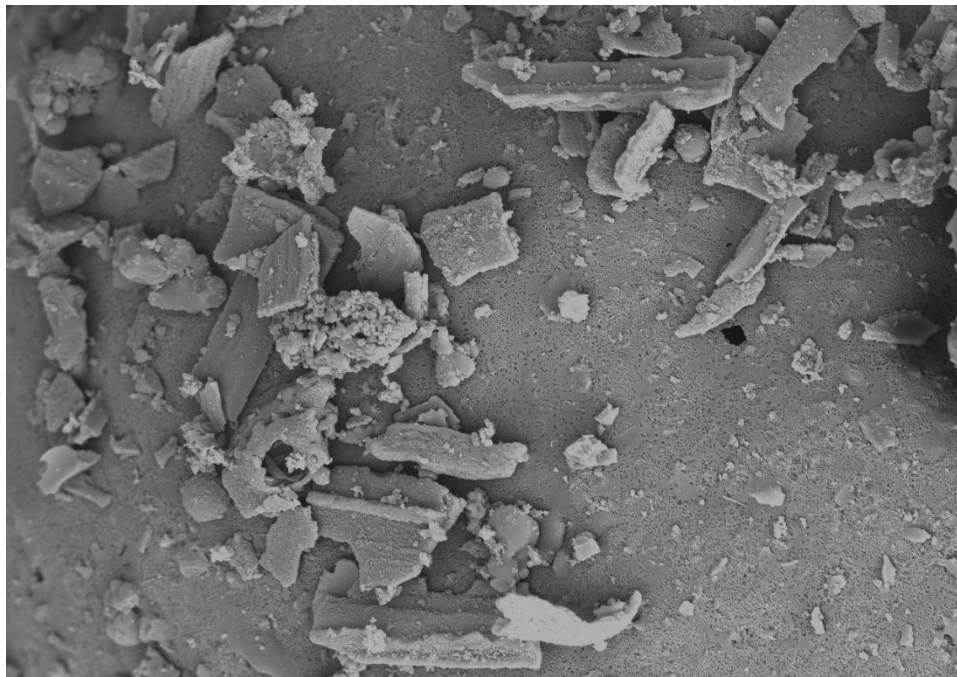

Clariant SU7000 5.00kV 6.4mm x2.00k UD+LD+MD 02/24/2025 20.0µm

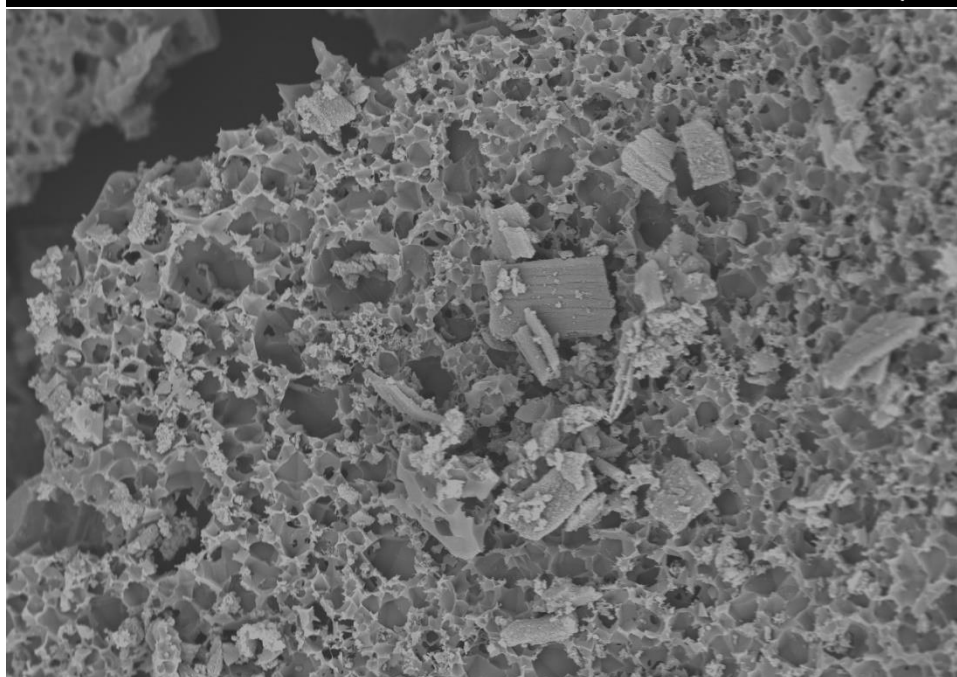


Clariant SU7000 5.00kV 6.6mm x2.00k UD+LD+MD 02/24/2025 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

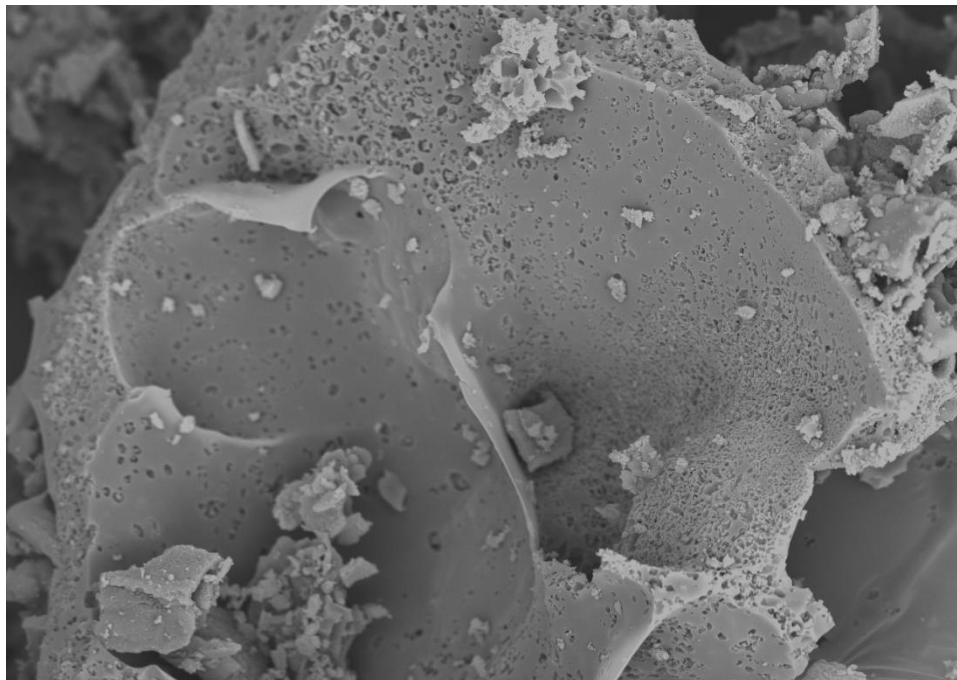

Clariant SU7000 5.00kV 6.5mm x2.00k UD+LD+MD 02/24/2025 20.0µm

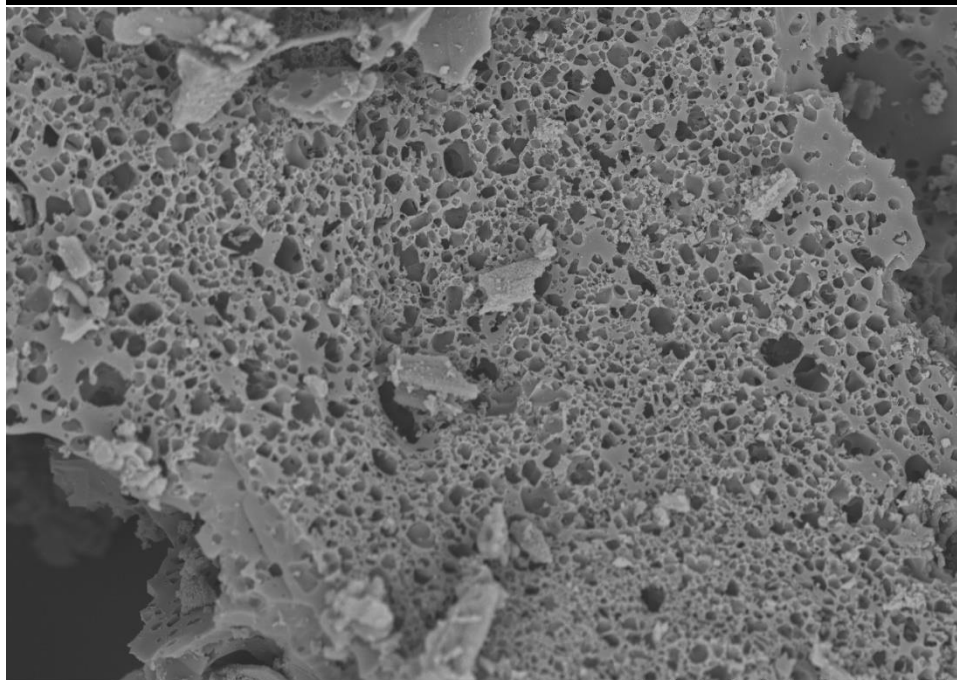


Clariant SU7000 5.00kV 6.5mm x2.00k UD+LD+MD 02/24/2025 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

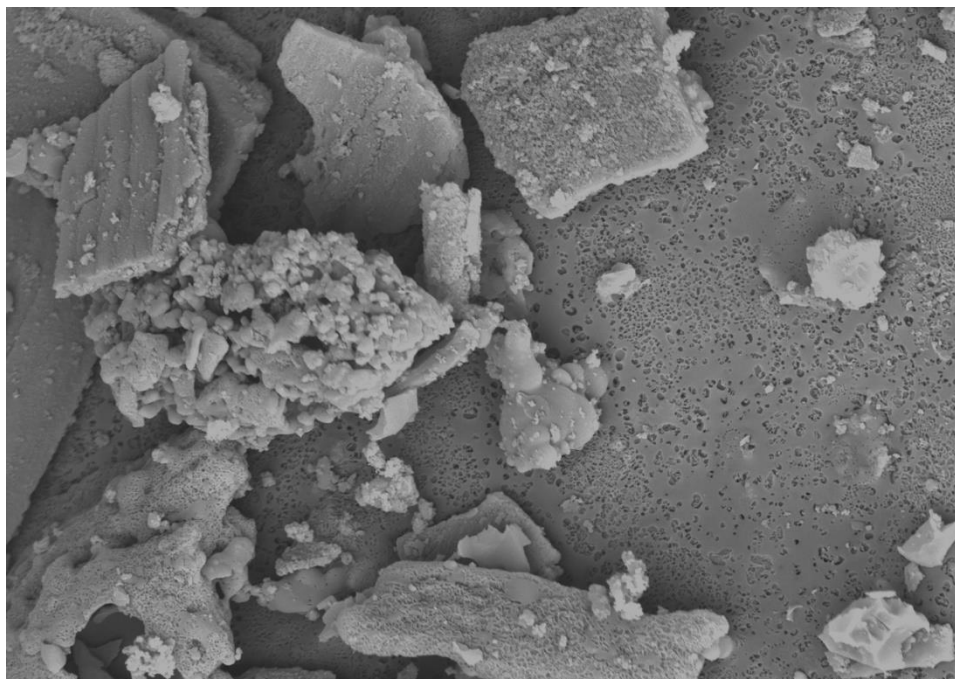

Clariant SU7000 5.00kV 6.4mm x5.00k UD+LD+MD 02/24/2025 10.0μm

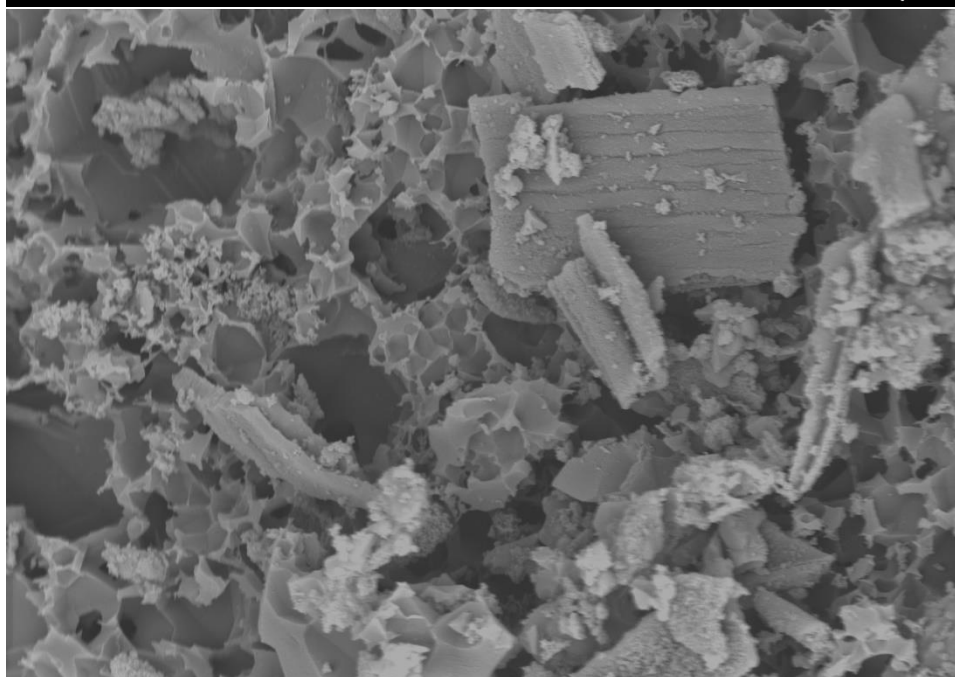


Clariant SU7000 5.00kV 6.6mm x5.00k UD+LD+MD 02/24/2025 10.0μm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

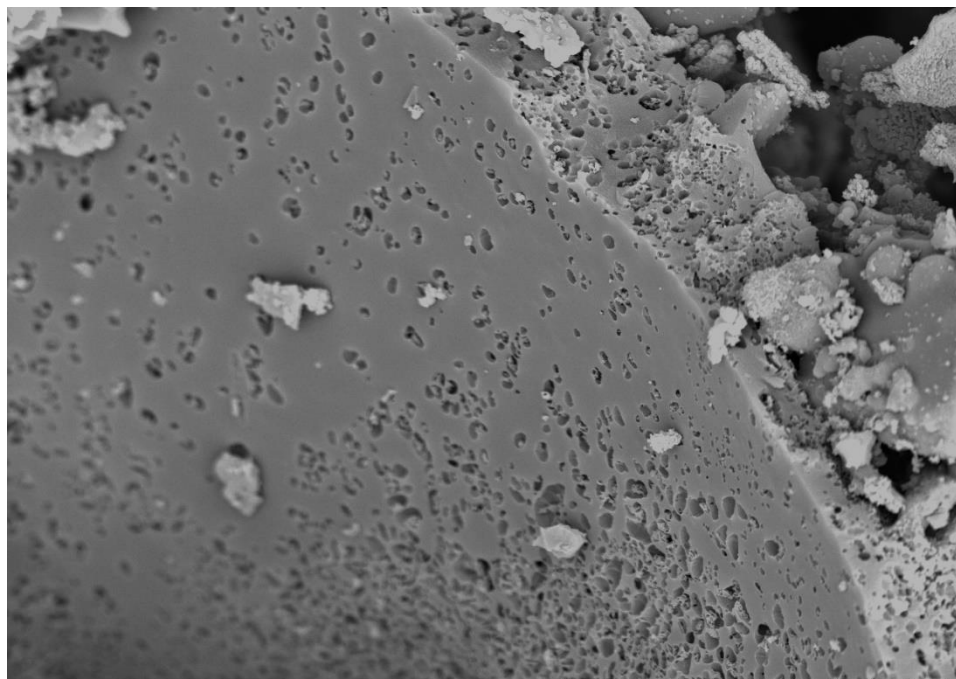

Clariant SU7000 5.00kV 6.5mm x5.00k UD+LD+MD 02/24/2025 10.0µm

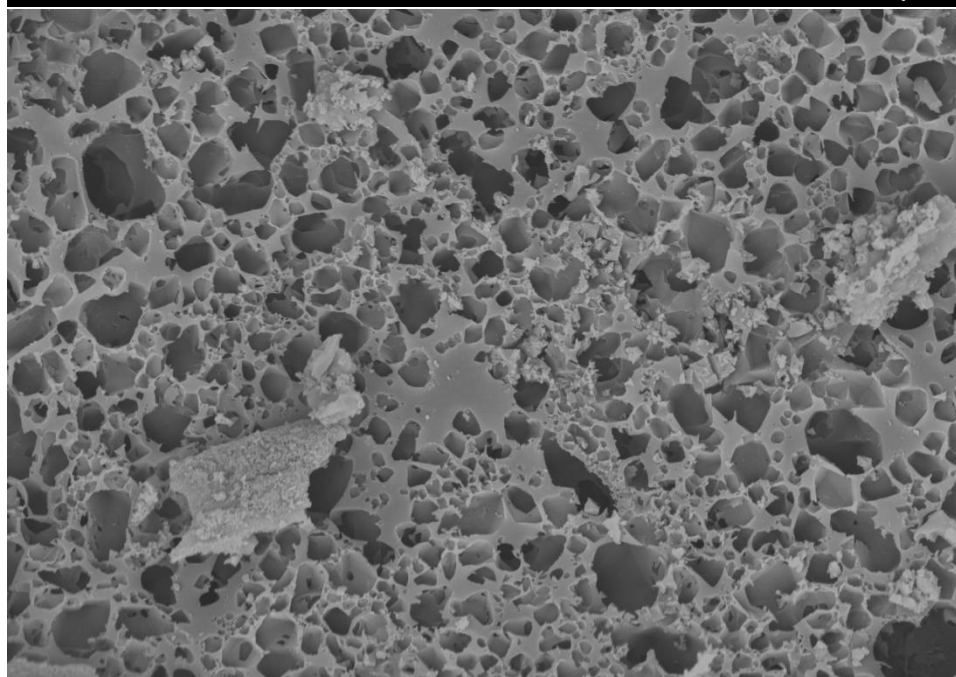


Clariant SU7000 5.00kV 6.5mm x5.00k UD+LD+MD 02/24/2025 10.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

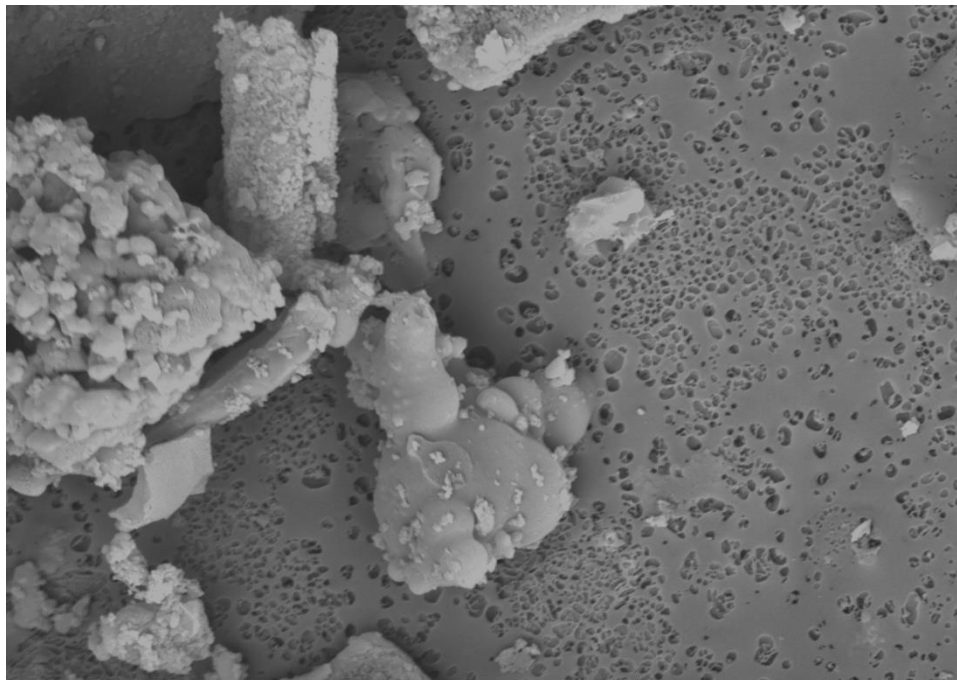

Clariant SU7000 5.00kV 6.4mm x10.0k UD+LD+MD 02/24/2025 5.00µm

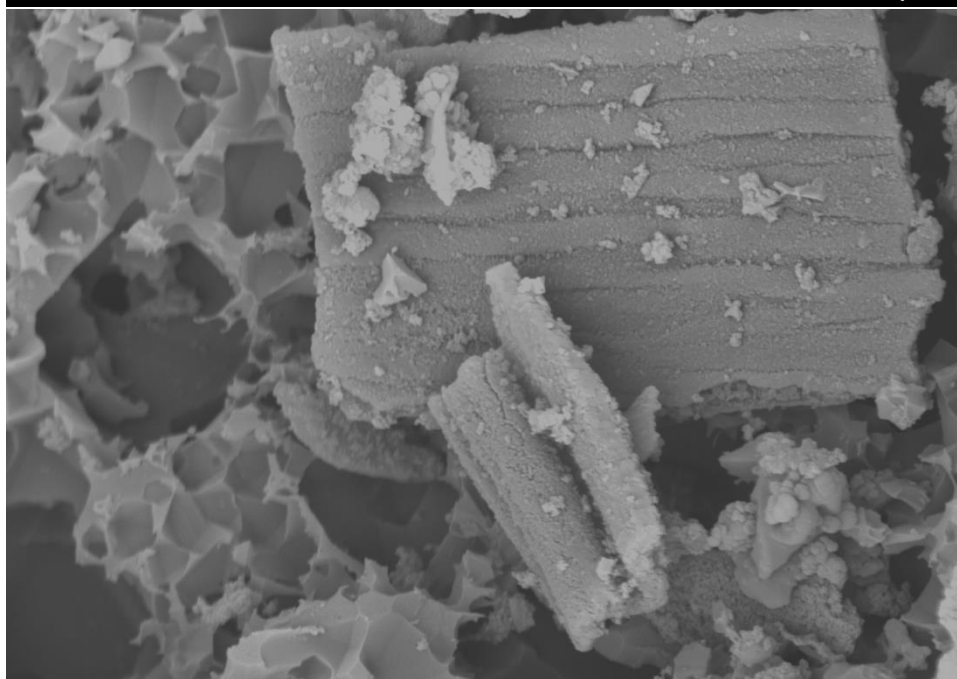


Clariant SU7000 5.00kV 6.5mm x10.0k UD+LD+MD 02/24/2025 5.00µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

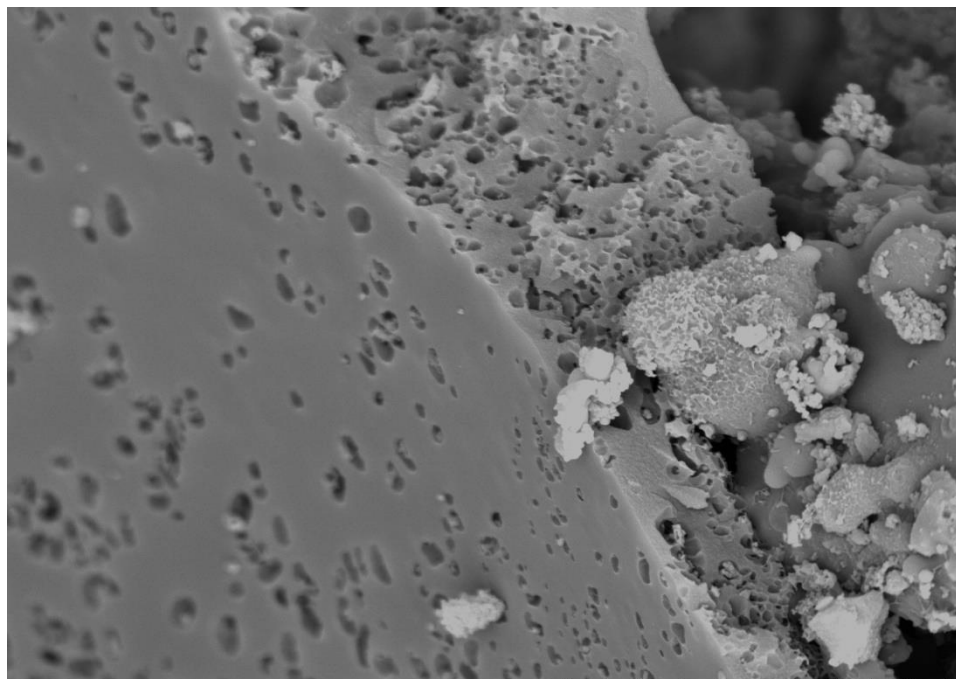

Clariant SU7000 5.00kV 6.4mm x10.0k UD+LD+MD 02/24/2025 5.00μm

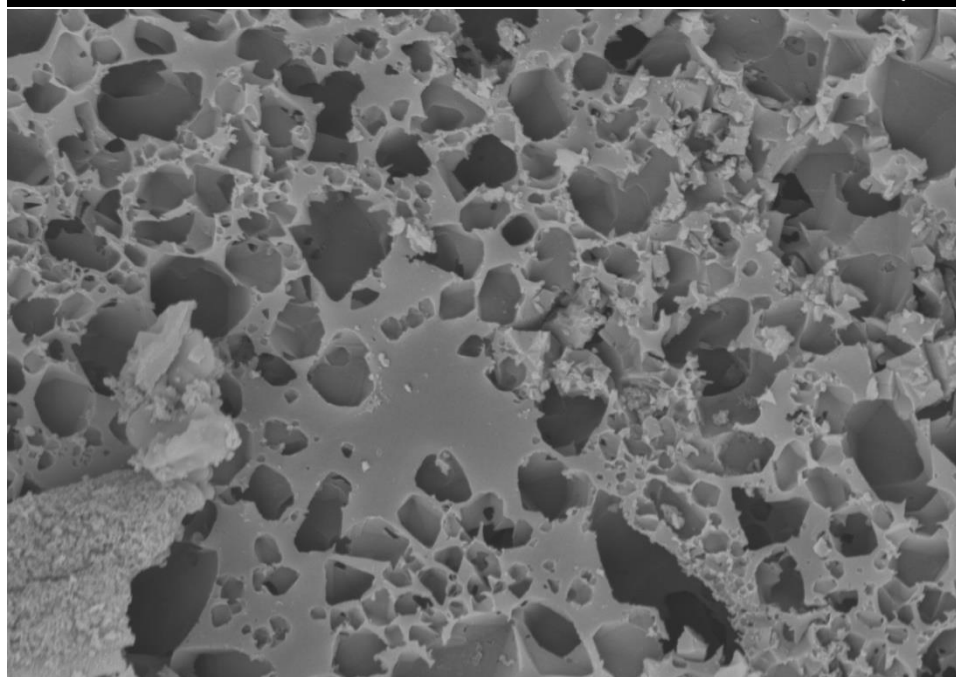

Clariant SU7000 5.00kV 6.5mm x10.0k UD+LD+MD 02/24/2025 5.00μm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

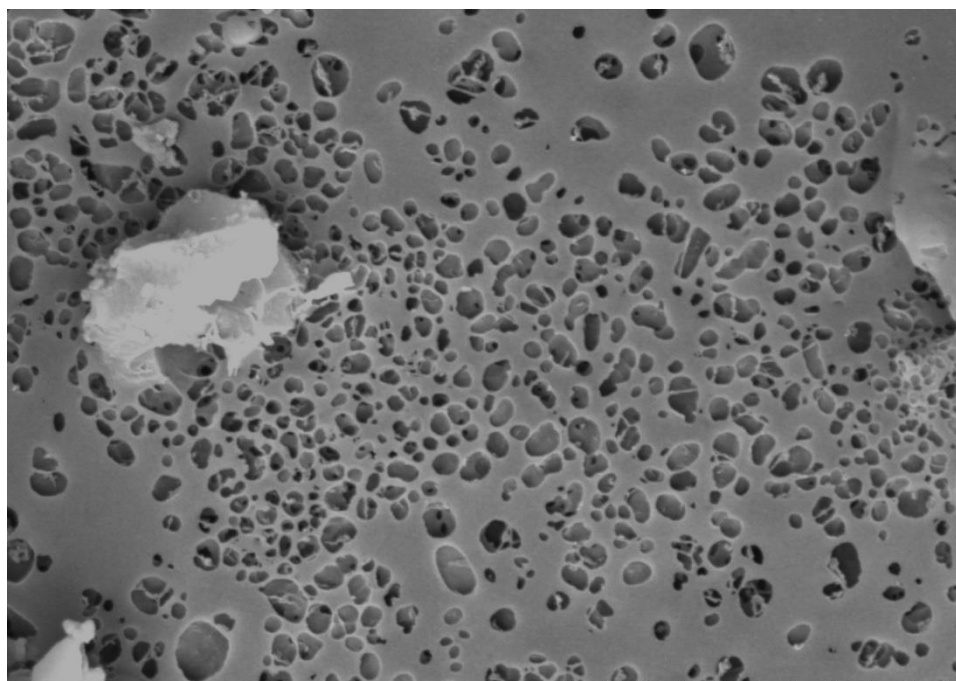

Clariant SU7000 5.00kV 6.4mm x25.0k UD+LD+MD 02/24/2025 2.00µm

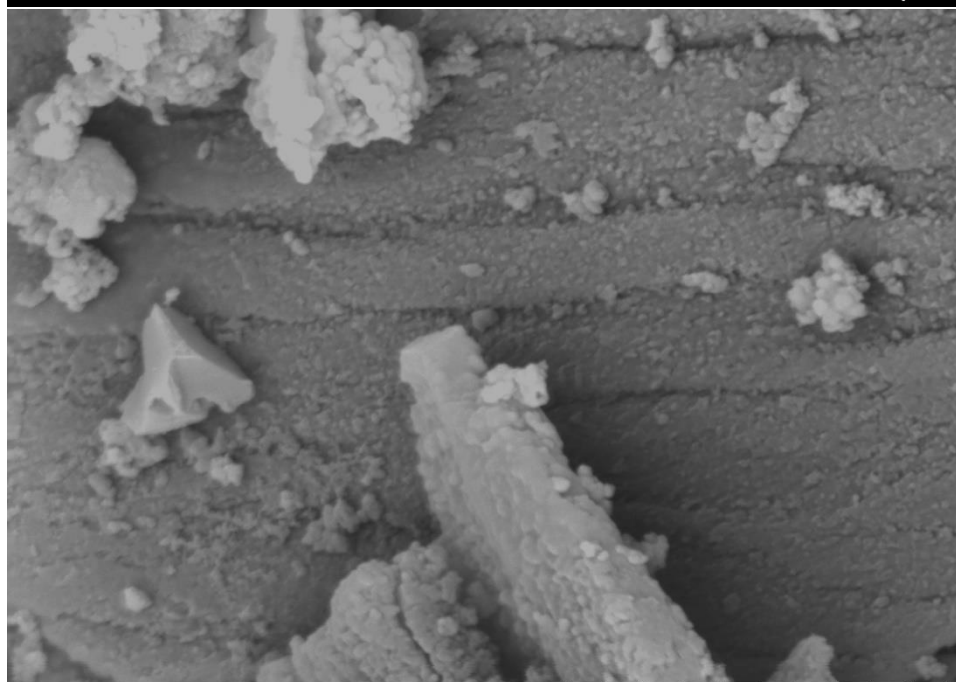


Clariant SU7000 5.00kV 6.5mm x25.0k UD+LD+MD 02/24/2025 2.00µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3054 1/1 2% 90sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049341-3

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

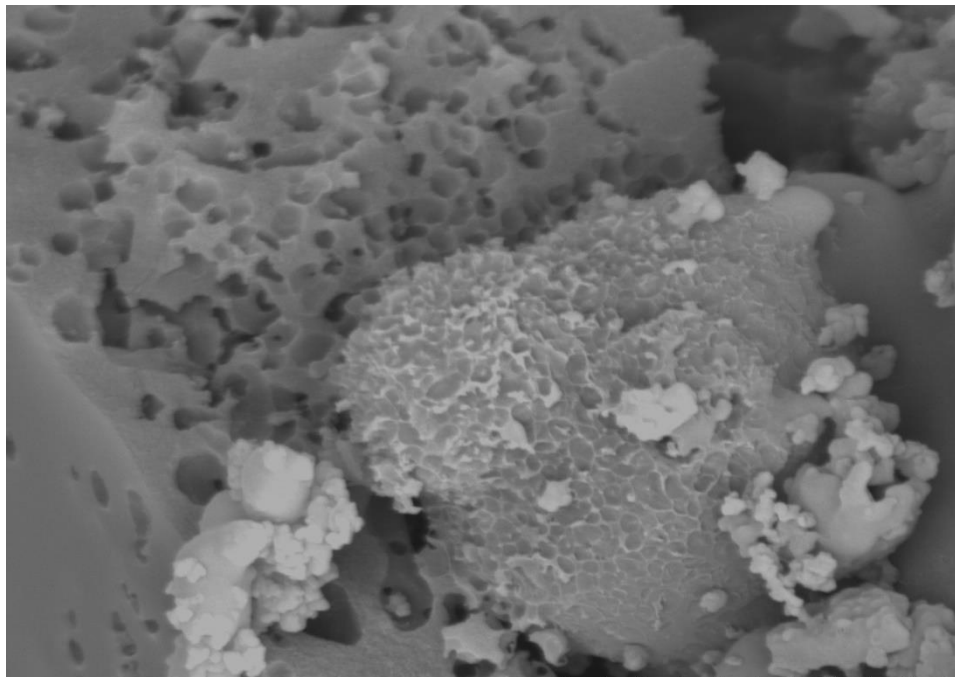

Clariant SU7000 5.00kV 6.4mm x25.0k UD+LD+MD 02/24/2025 2.00µm

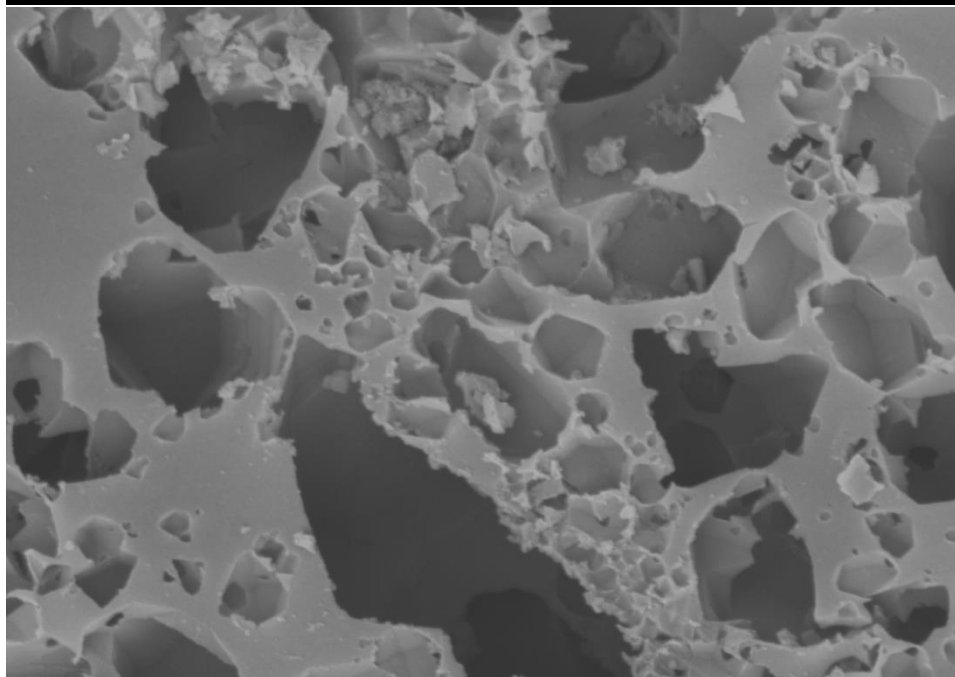

Clariant SU7000 5.00kV 6.5mm x25.0k UD+LD+MD 02/24/2025 2.00µm