

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa406 2/3 3min 800C 3C/m 1h A 2x1.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049538-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

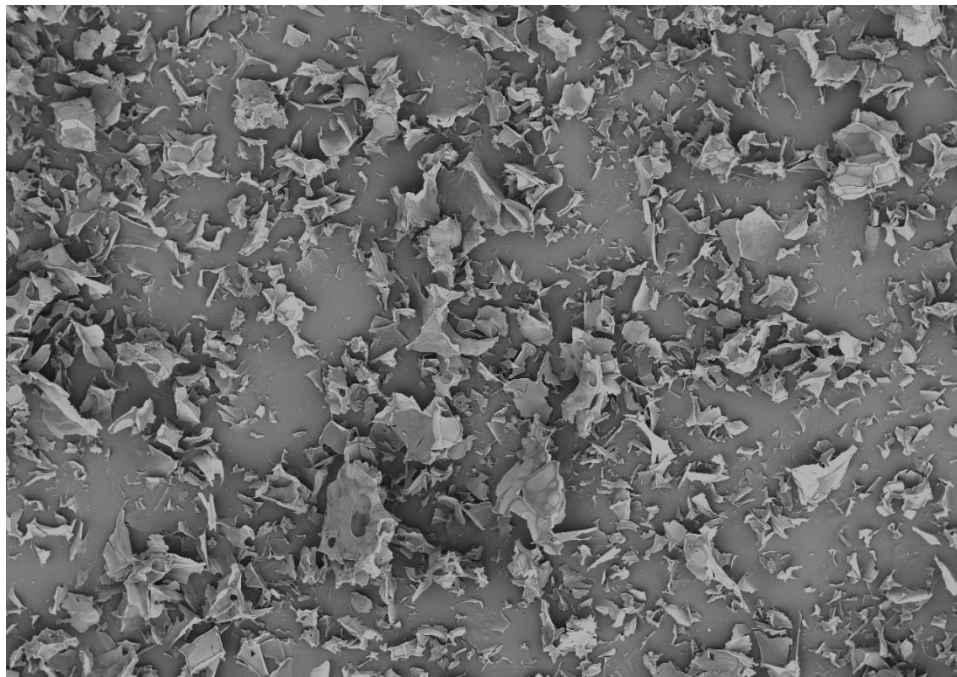

Clariant SU7000 5.00kV 4.5mm x100 UD+LD+MD 03/17/2025 500µm

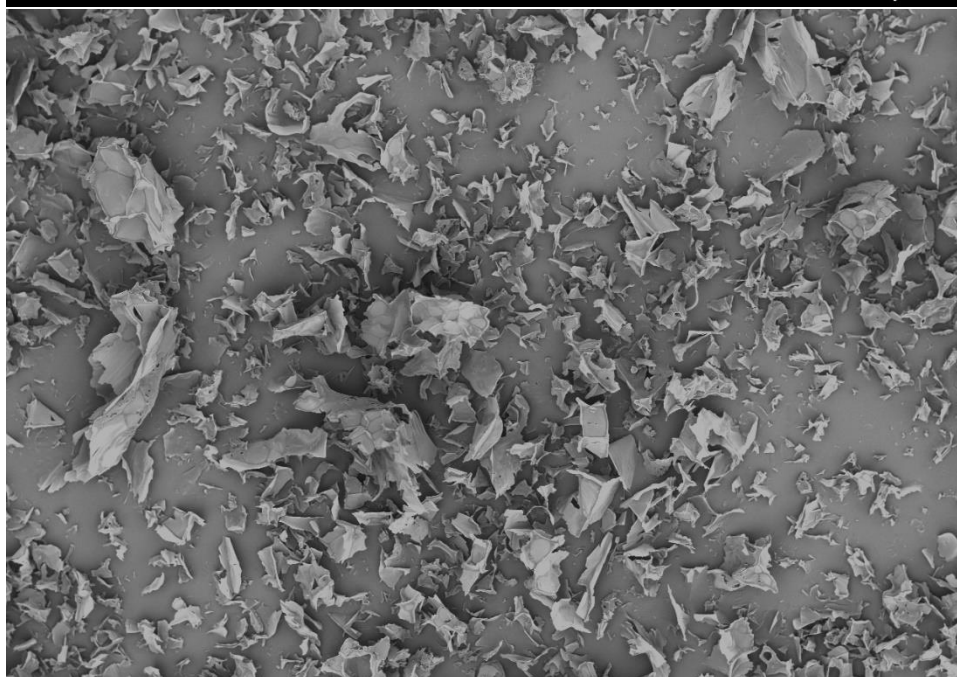

Clariant SU7000 5.00kV 4.5mm x100 UD+LD+MD 03/17/2025 500µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa406 2/3 3min 800C 3C/m 1h A 2x1.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049538-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

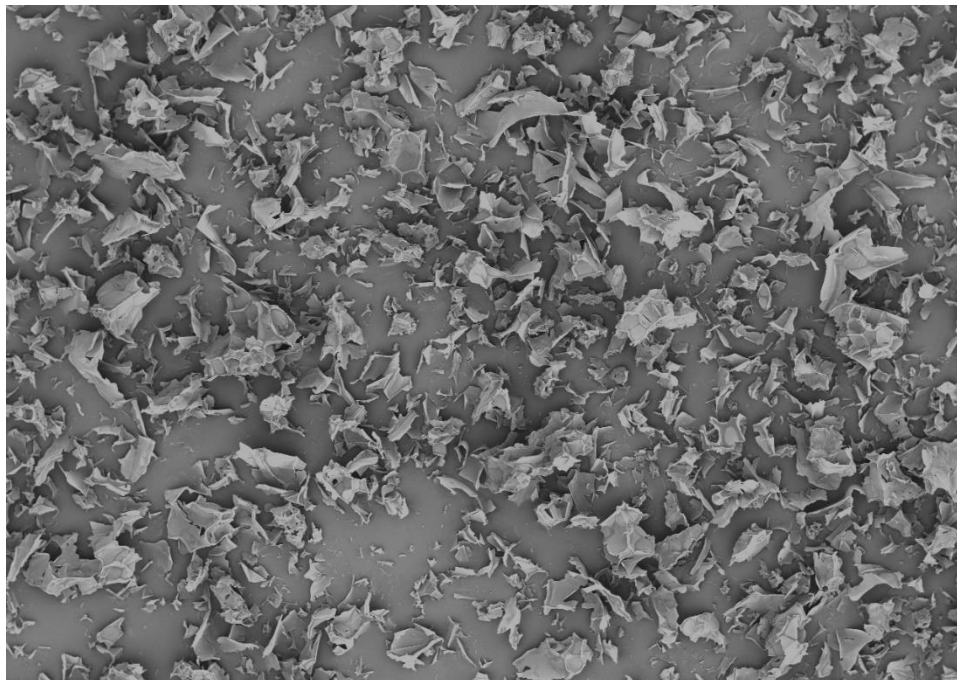

Clariant SU7000 5.00kV 4.5mm x100 UD+LD+MD 03/17/2025 500µm

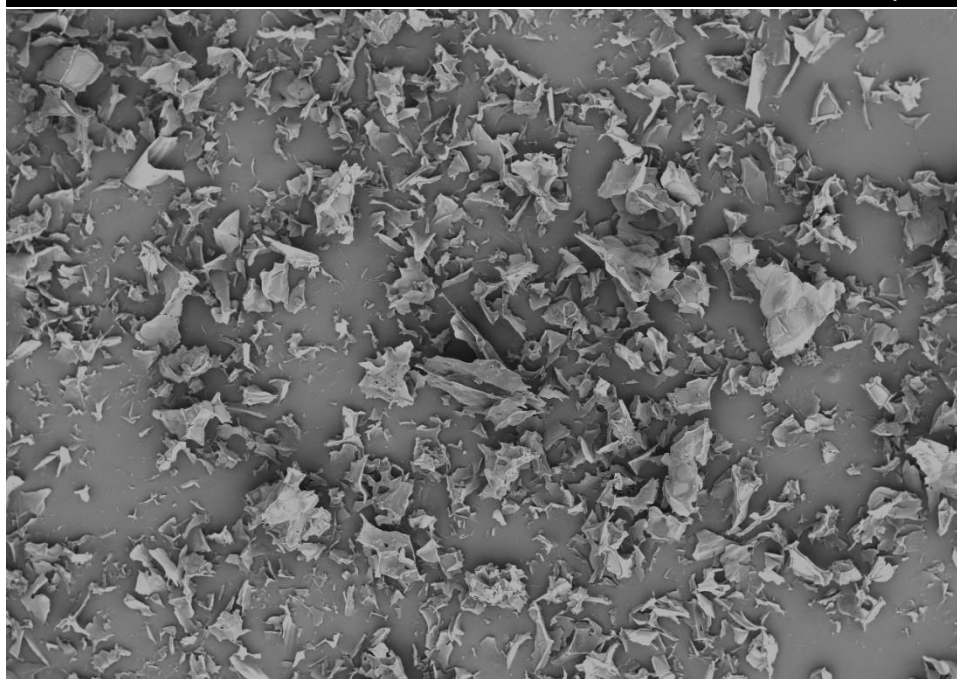

Clariant SU7000 5.00kV 4.4mm x100 UD+LD+MD 03/17/2025 500µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa406 2/3 3min 800C 3C/m 1h A 2x1.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049538-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

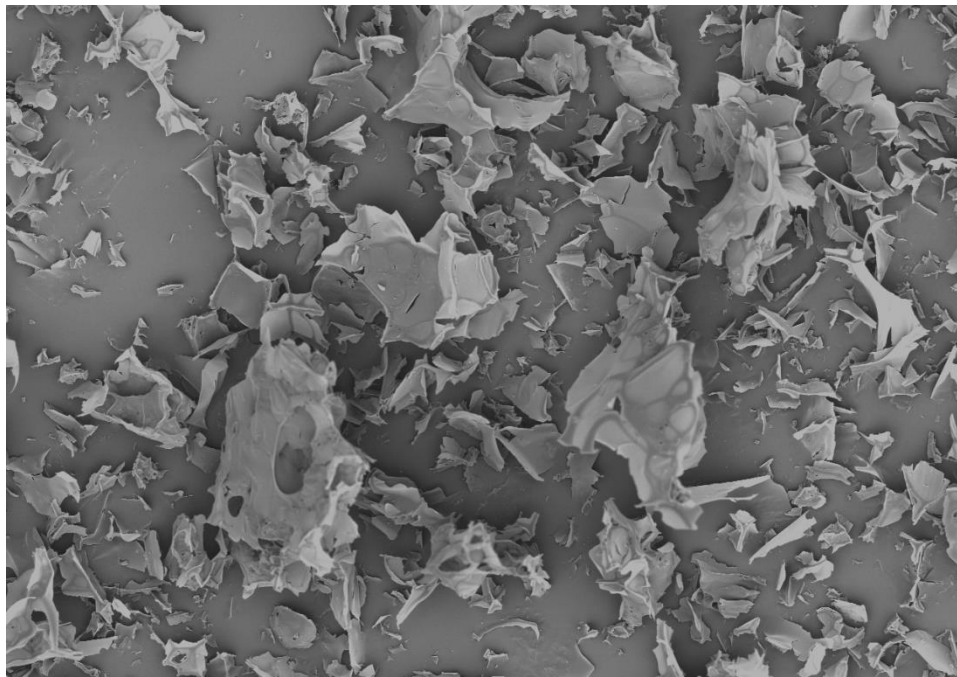

Clariant SU7000 5.00kV 4.6mm x200 UD+LD+MD 03/17/2025 200µm

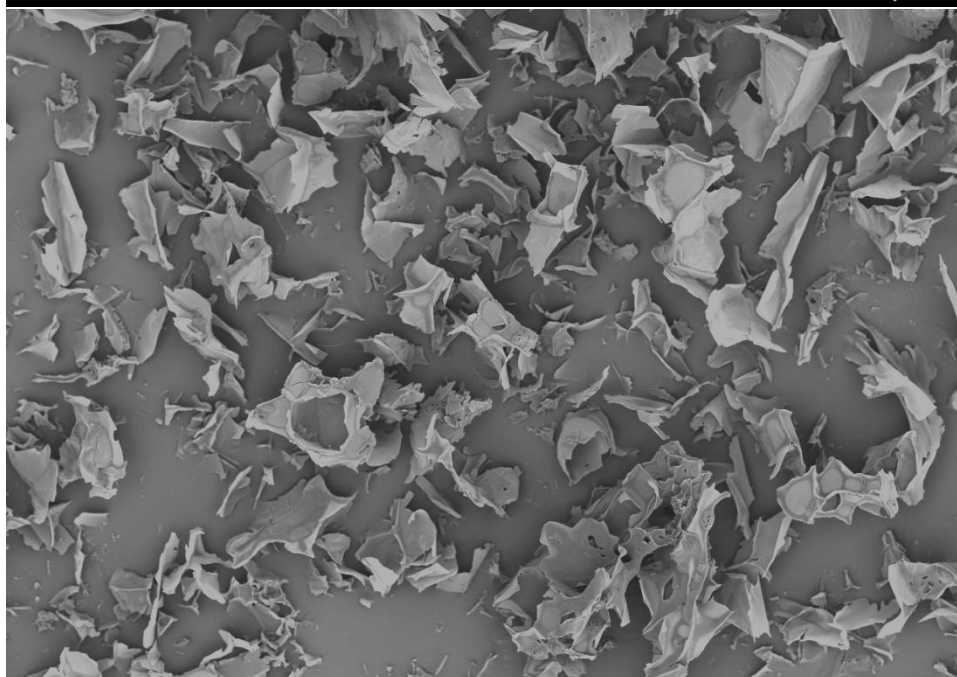

Clariant SU7000 5.00kV 4.5mm x200 UD+LD+MD 03/17/2025 200µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa406 2/3 3min 800C 3C/m 1h A 2x1.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049538-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

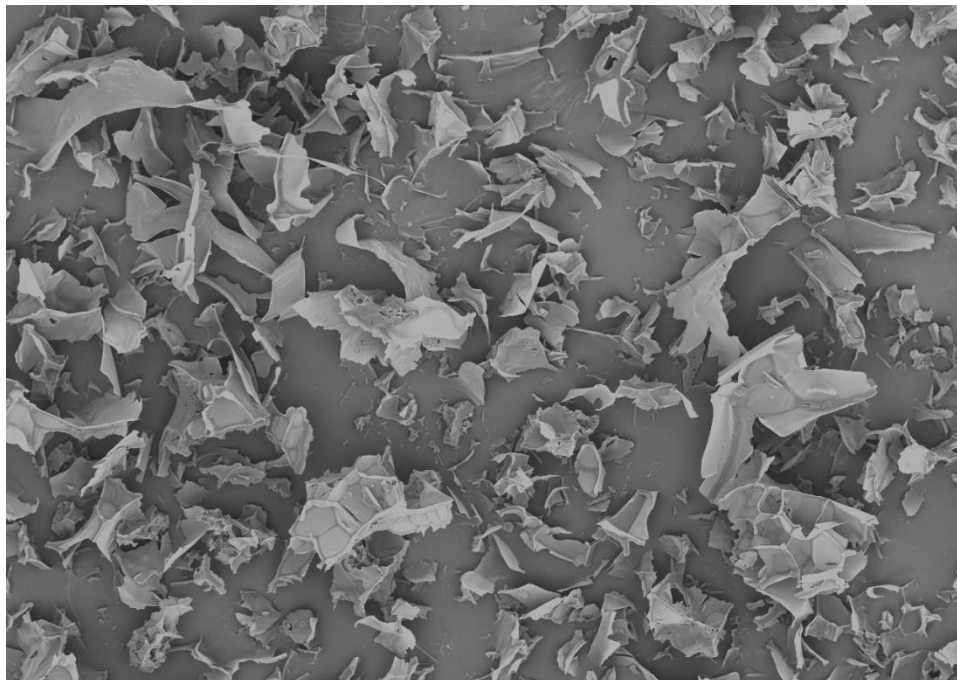

Clariant SU7000 5.00kV 4.5mm x200 UD+LD+MD 03/17/2025 200µm

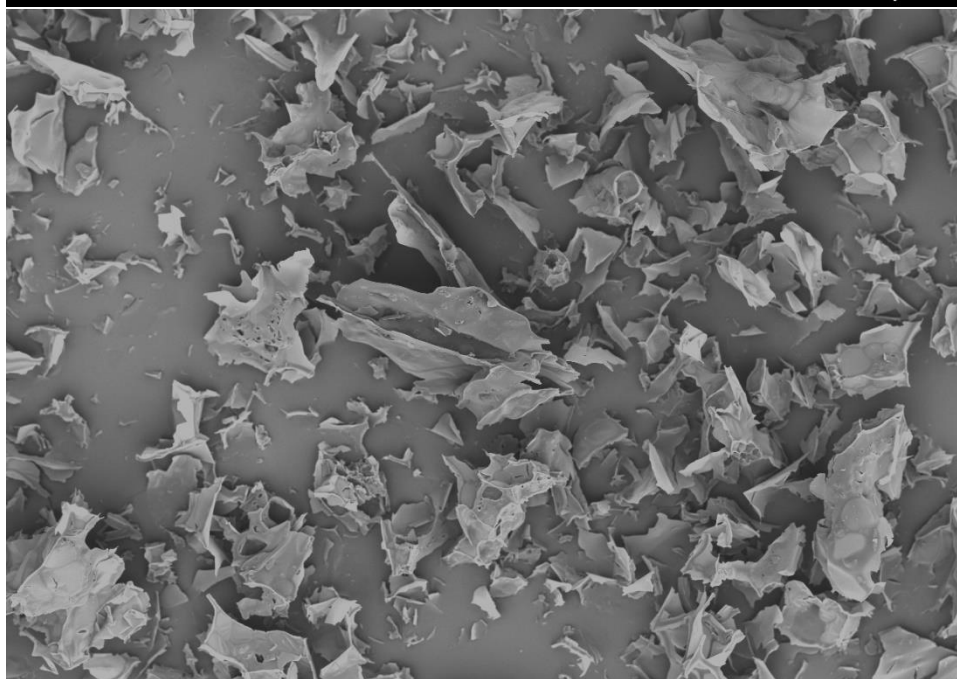

Clariant SU7000 5.00kV 4.4mm x200 UD+LD+MD 03/17/2025 200µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa406 2/3 3min 800C 3C/m 1h A 2x1.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049538-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

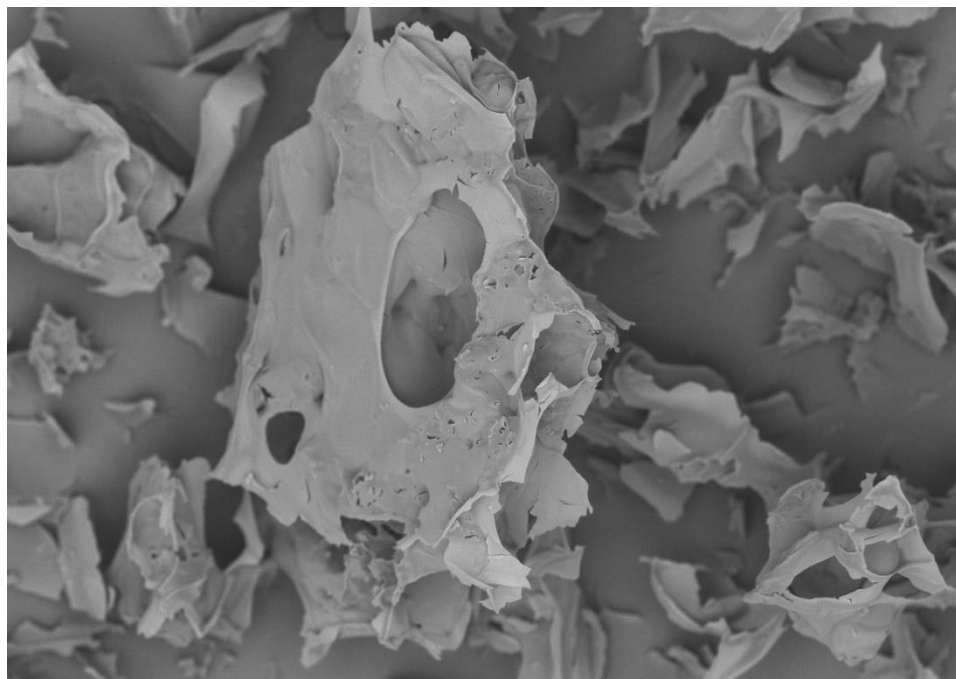

Clariant SU7000 5.00kV 4.4mm x500 MD 03/17/2025 100µm

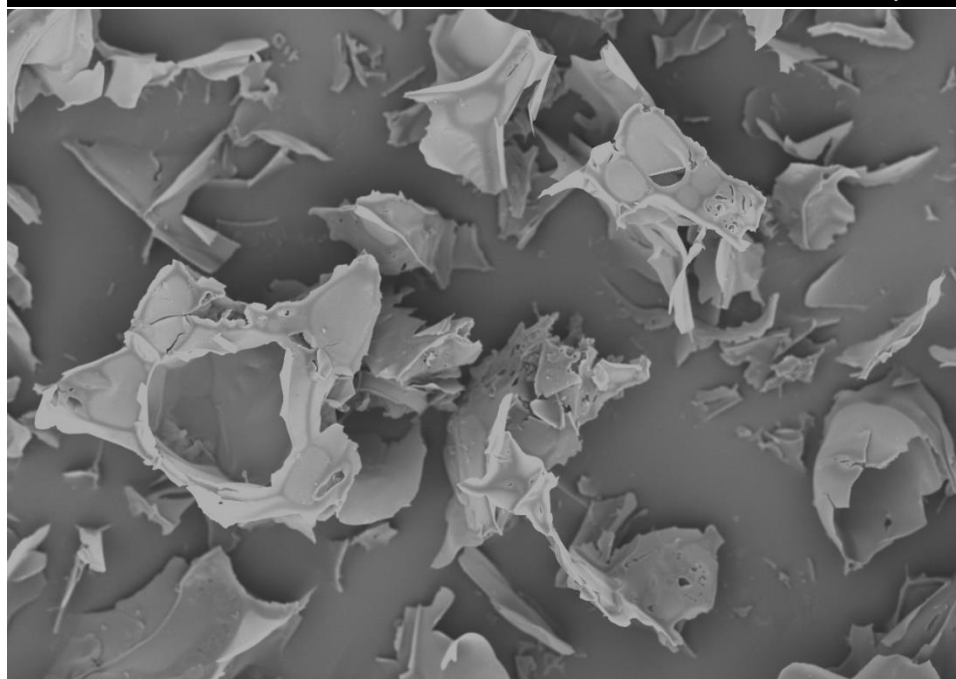

Clariant SU7000 5.00kV 4.5mm x500 UD+LD+MD 03/17/2025 100µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa406 2/3 3min 800C 3C/m 1h A 2x1.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049538-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

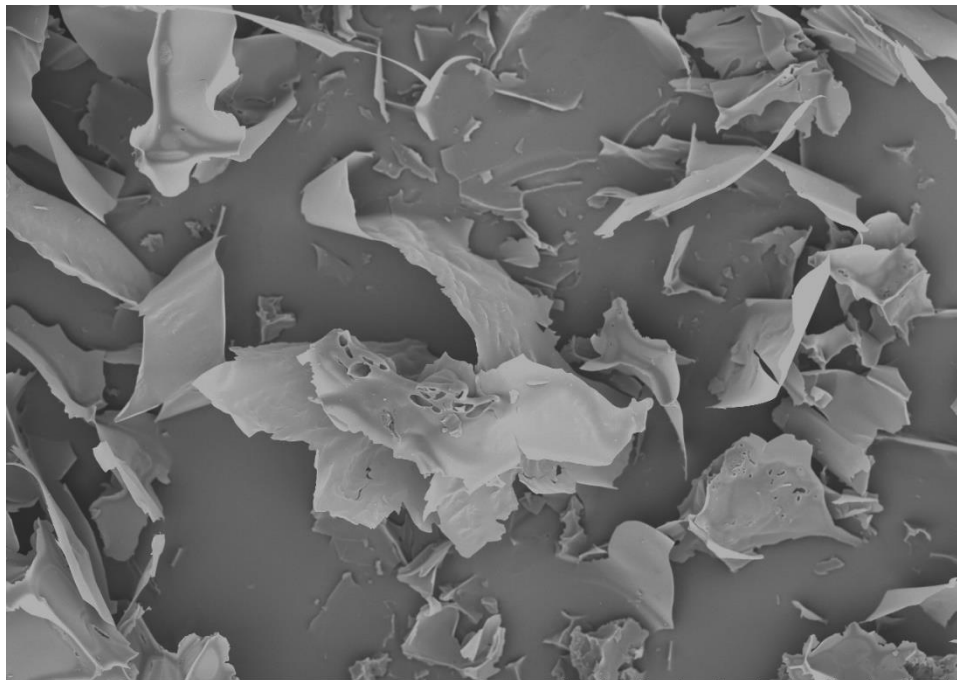

Clariant SU7000 5.00kV 4.5mm x500 UD+LD+MD 03/17/2025 100µm

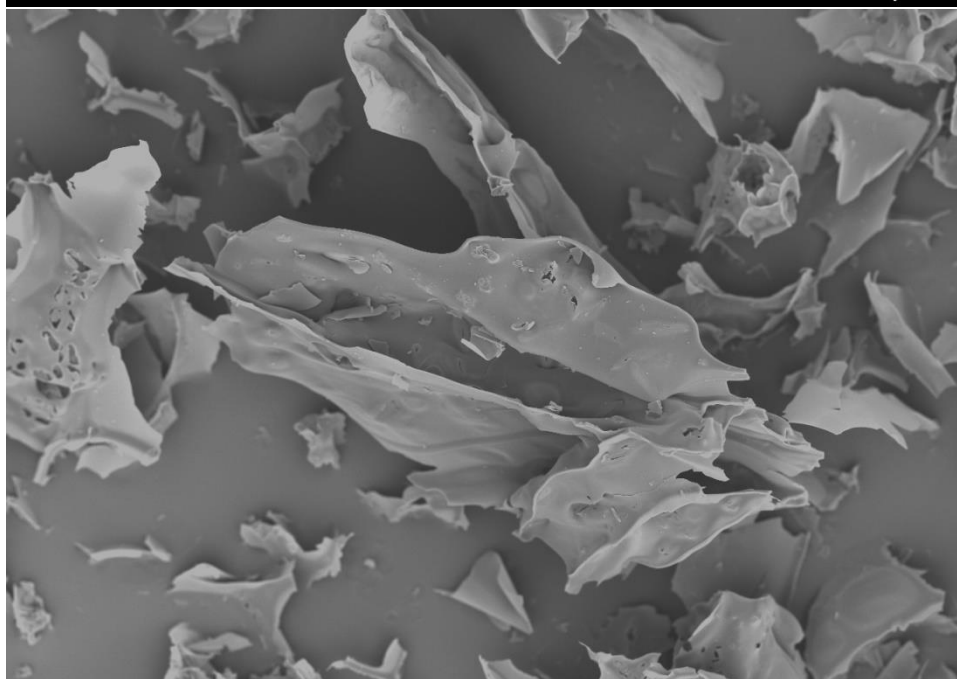

Clariant SU7000 5.00kV 4.4mm x500 UD+LD+MD 03/17/2025 100µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa406 2/3 3min 800C 3C/m 1h A 2x1.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049538-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

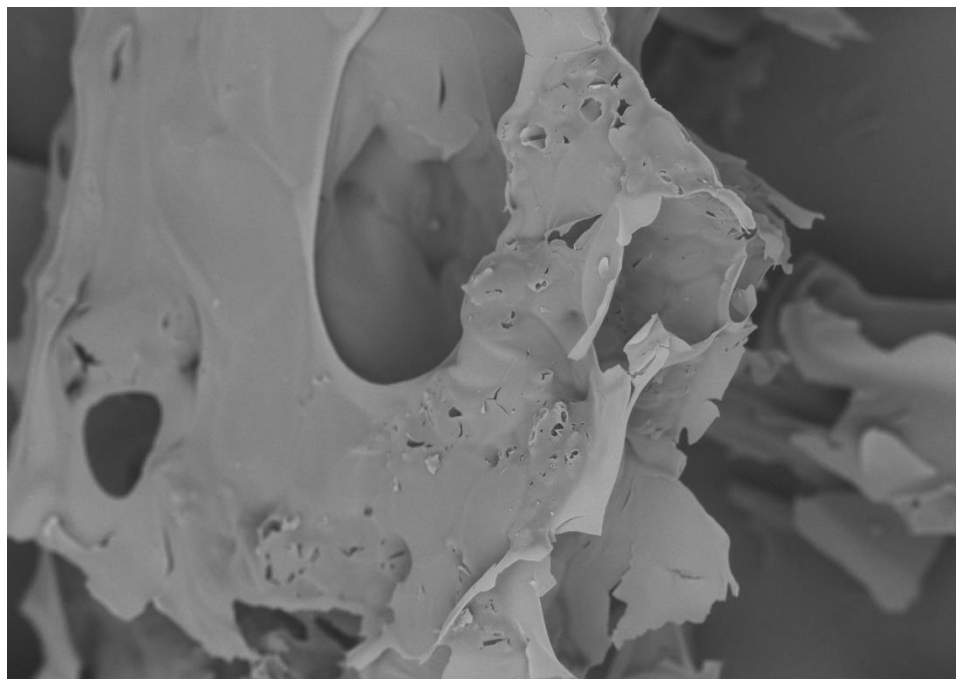

Clariant SU7000 5.00kV 4.4mm x1.00k MD 03/17/2025 50.0µm

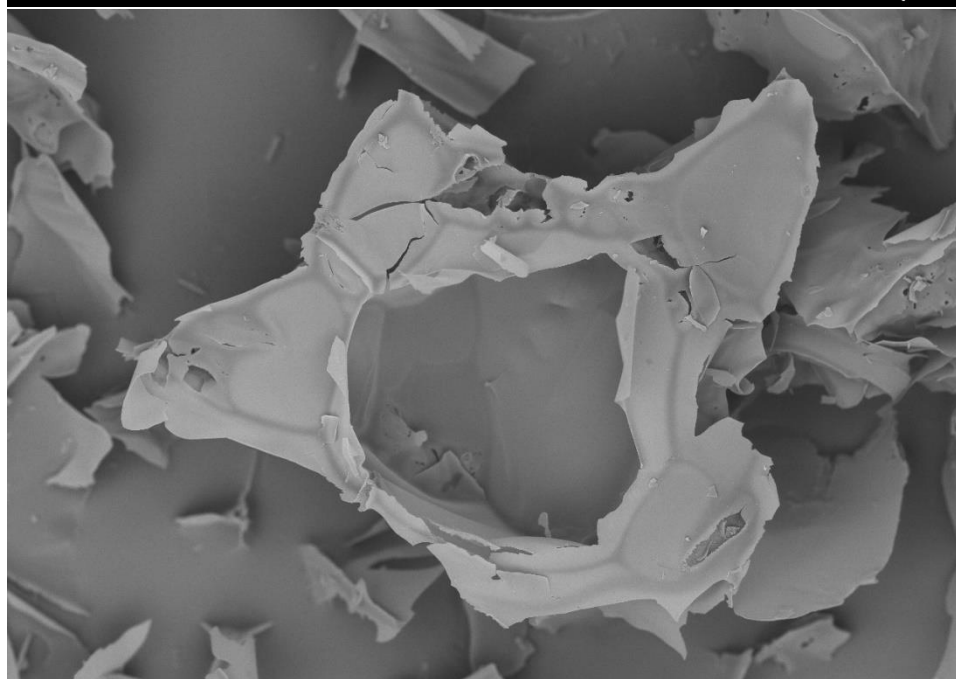

Clariant SU7000 5.00kV 4.5mm x1.00k MD 03/17/2025 50.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa406 2/3 3min 800C 3C/m 1h A 2x1.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049538-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

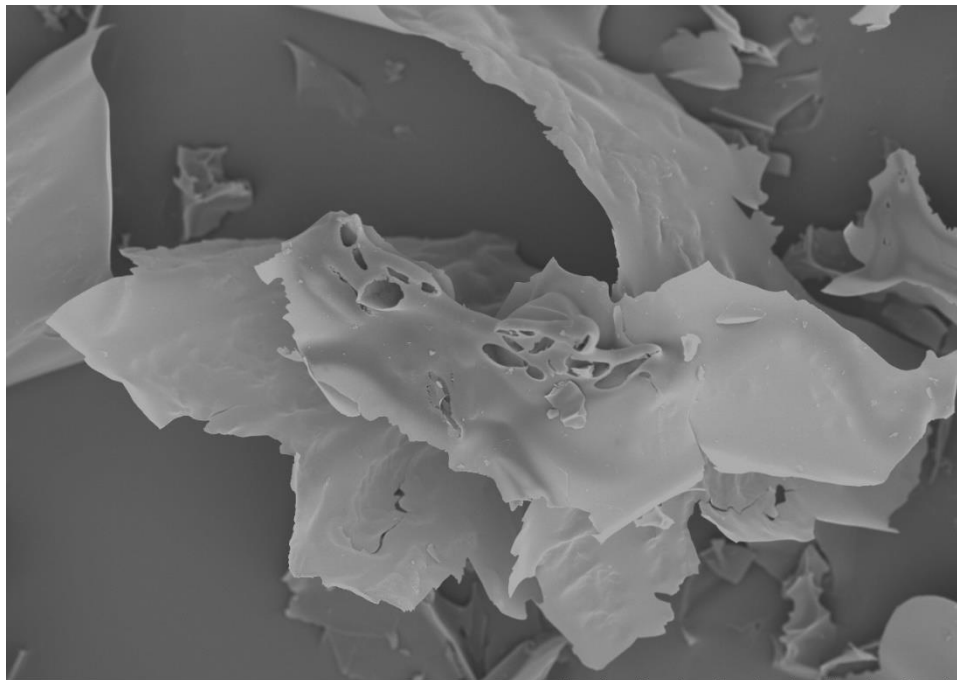

Clariant SU7000 5.00kV 4.5mm x1.00k UD+LD+MD 03/17/2025 50.0µm

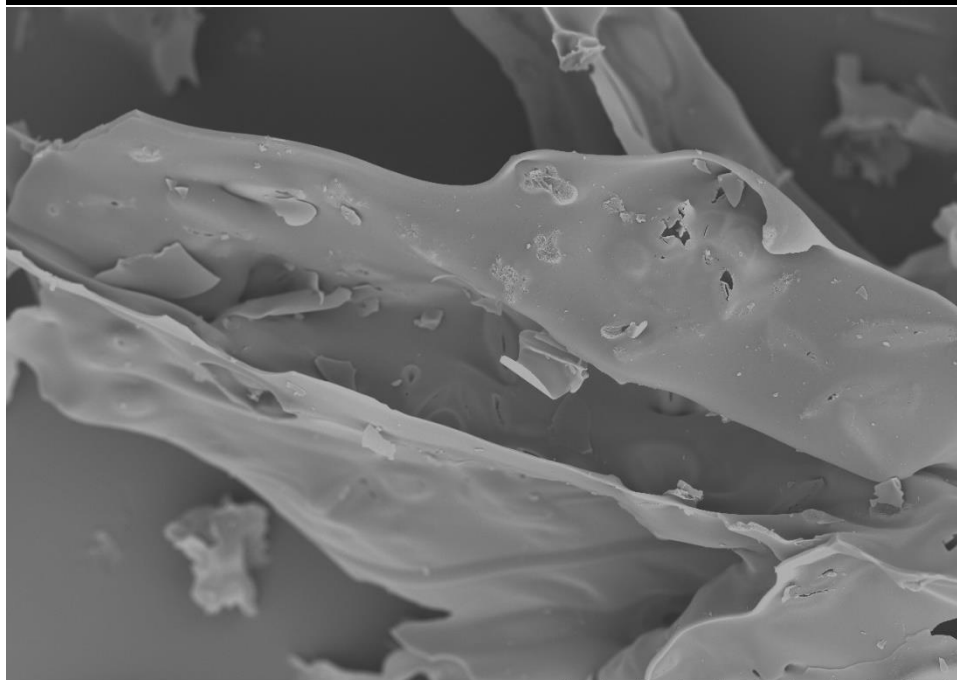

Clariant SU7000 5.00kV 4.4mm x1.00k UD+LD+MD 03/17/2025 50.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa406 2/3 3min 800C 3C/m 1h A 2x1.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049538-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

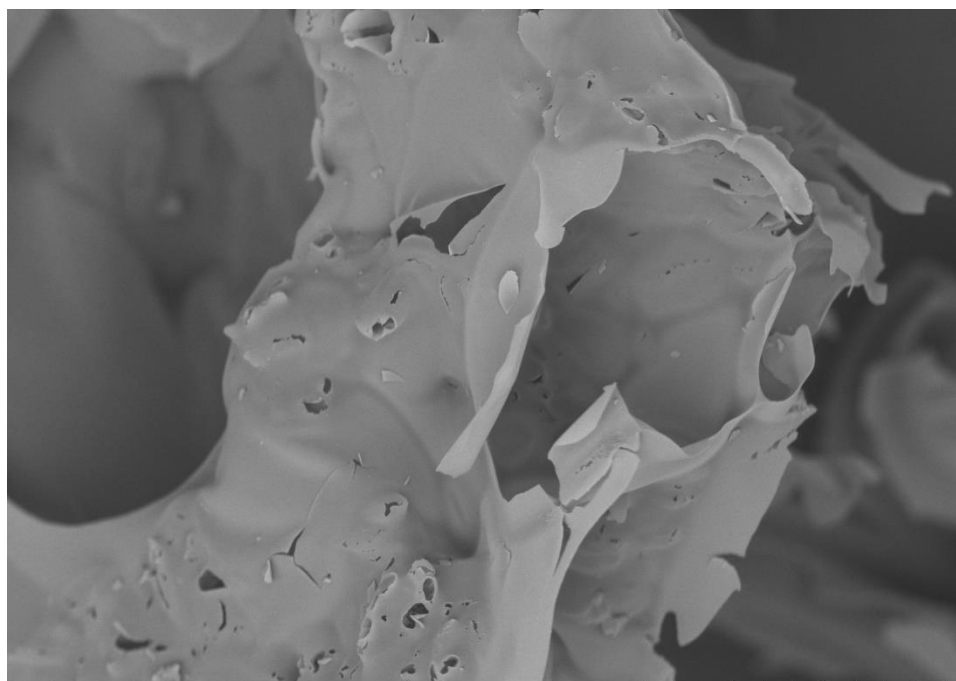

Clariant SU7000 5.00kV 4.4mm x2.00k MD 03/17/2025 20.0µm

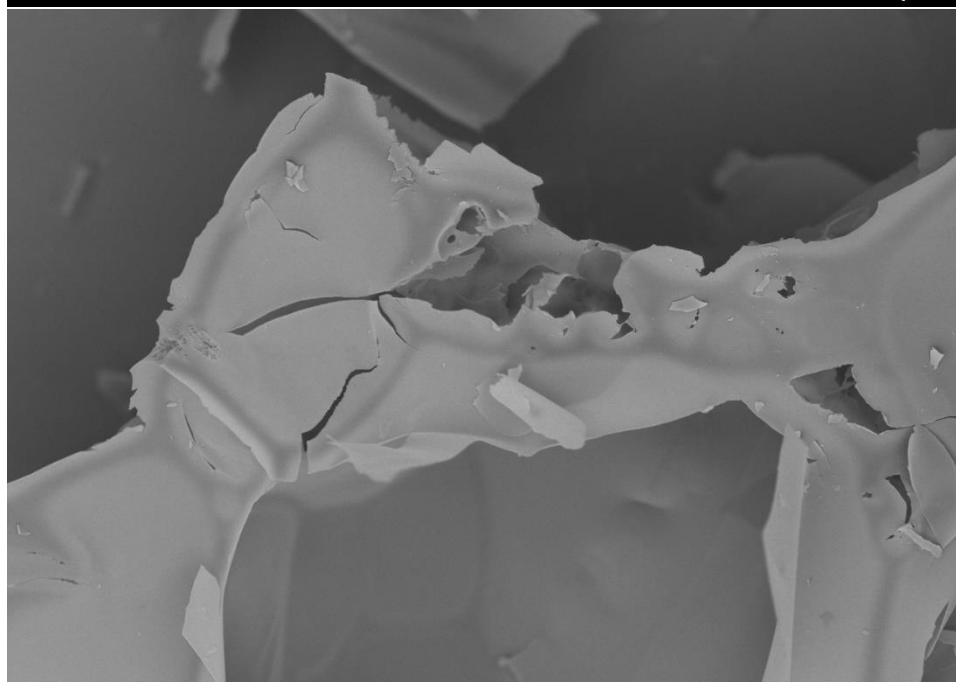

Clariant SU7000 5.00kV 4.5mm x2.00k MD 03/17/2025 20.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa406 2/3 3min 800C 3C/m 1h A 2x1.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049538-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

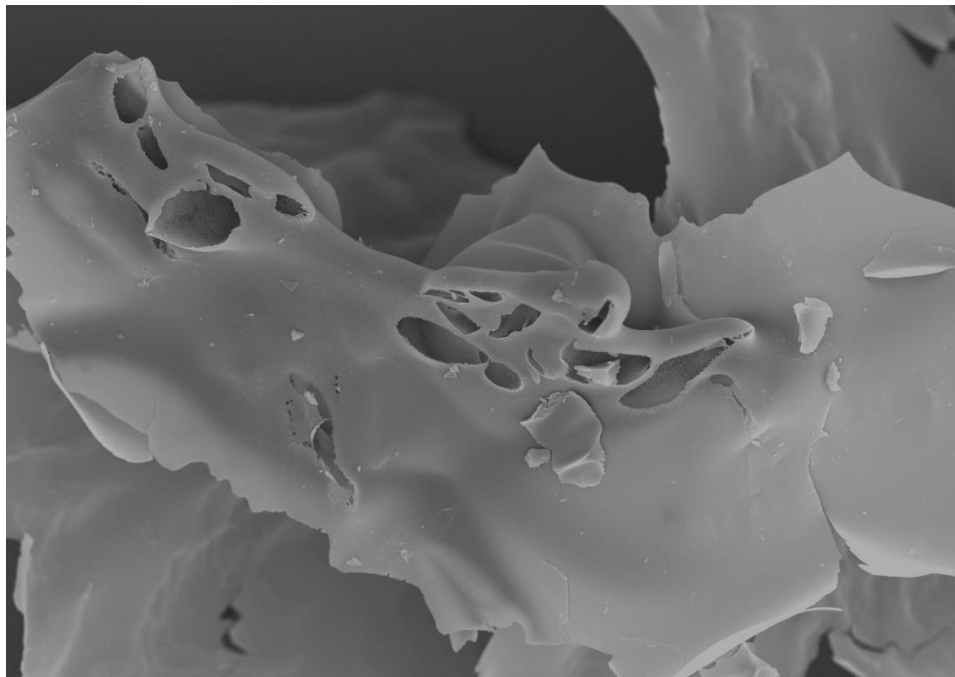

Clariant SU7000 5.00kV 4.5mm x2.00k UD+LD+MD 03/17/2025 20.0µm

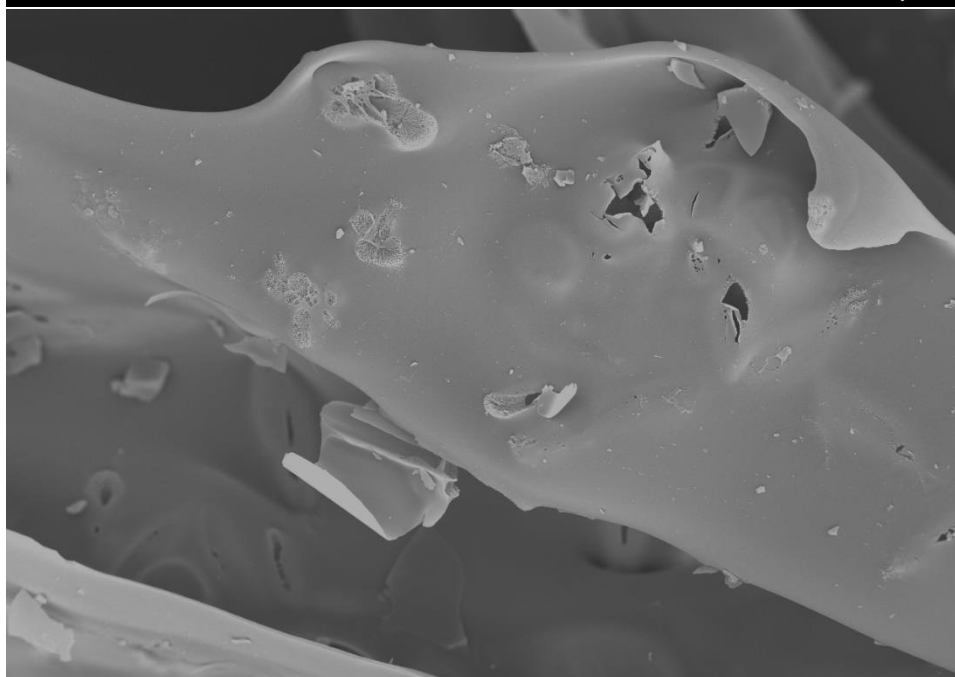

Clariant SU7000 5.00kV 4.4mm x2.00k UD+LD+MD 03/17/2025 20.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa406 2/3 3min 800C 3C/m 1h A 2x1.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049538-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

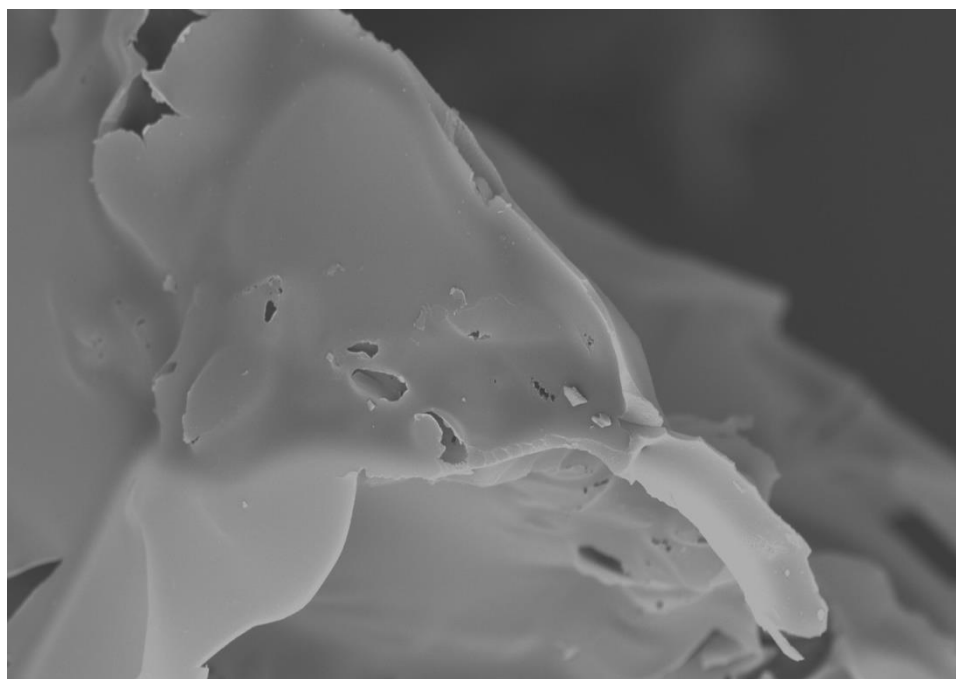

Clariant SU7000 5.00kV 4.4mm x5.00k UD+LD+MD 03/17/2025 10.0µm

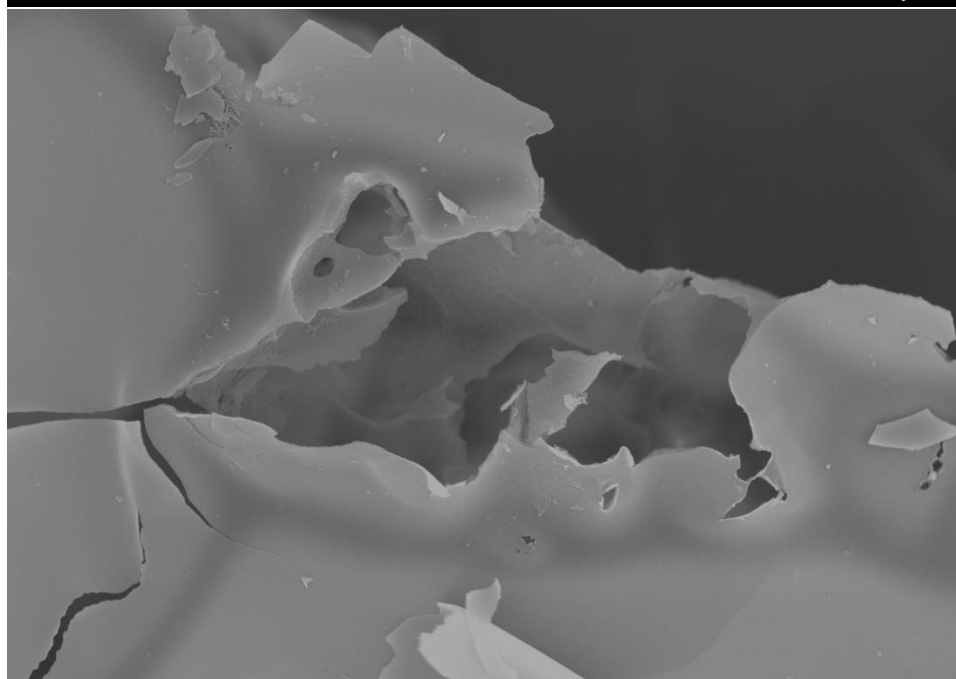

Clariant SU7000 5.00kV 4.5mm x5.00k UD+LD+MD 03/17/2025 10.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa406 2/3 3min 800C 3C/m 1h A 2x1.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049538-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

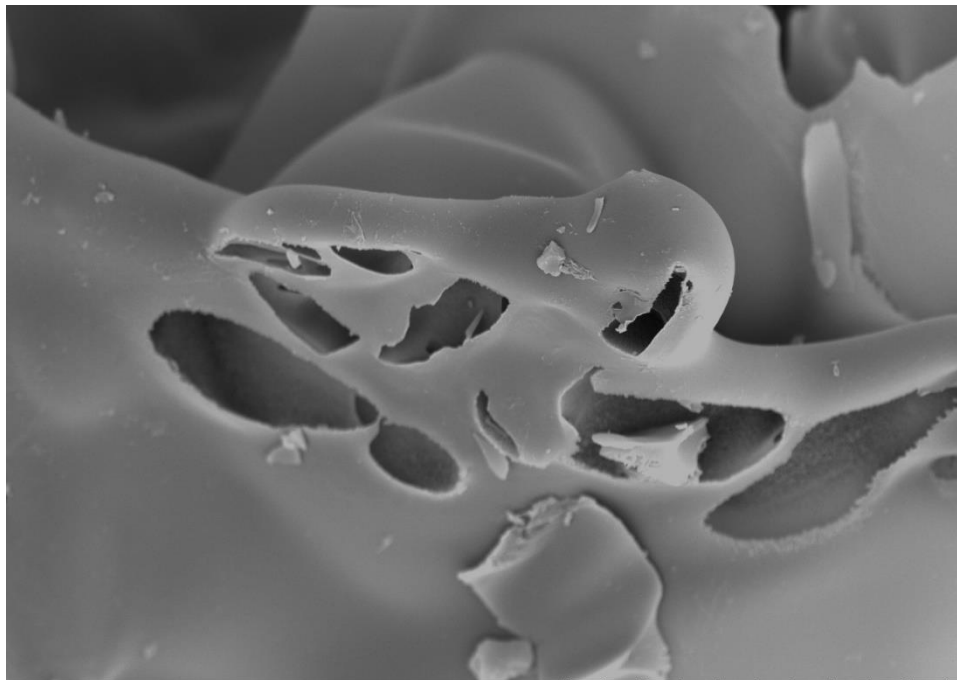

Clariant SU7000 5.00kV 4.4mm x5.00k UD+LD+MD 03/17/2025 10.0µm

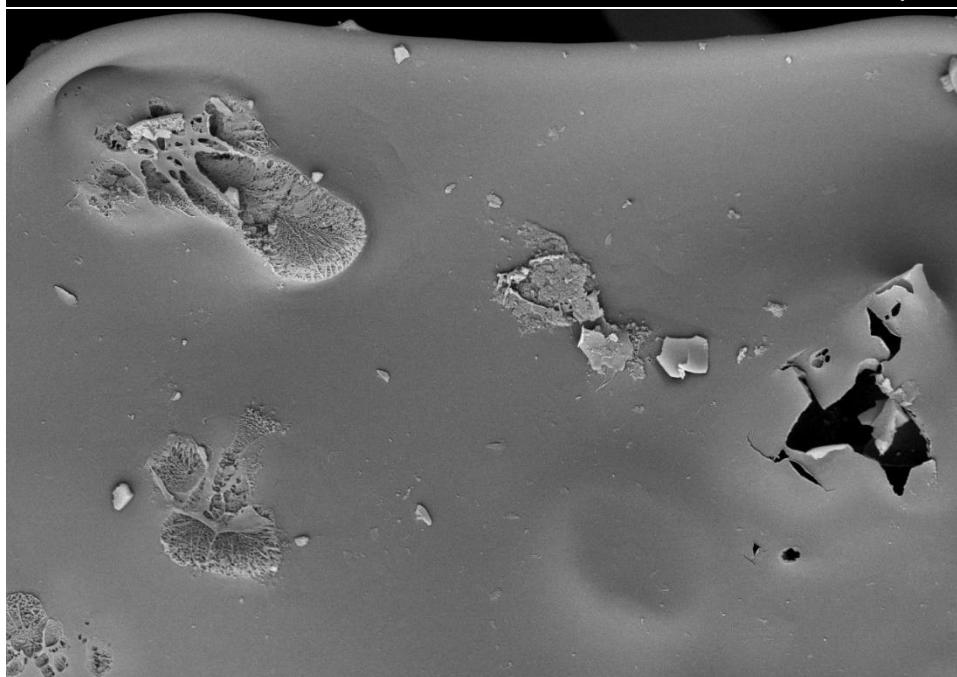

Clariant SU7000 5.00kV 4.4mm x5.00k MD 03/17/2025 10.0µm