



SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3063/MB3064/MB3066/MRa420 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-10

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

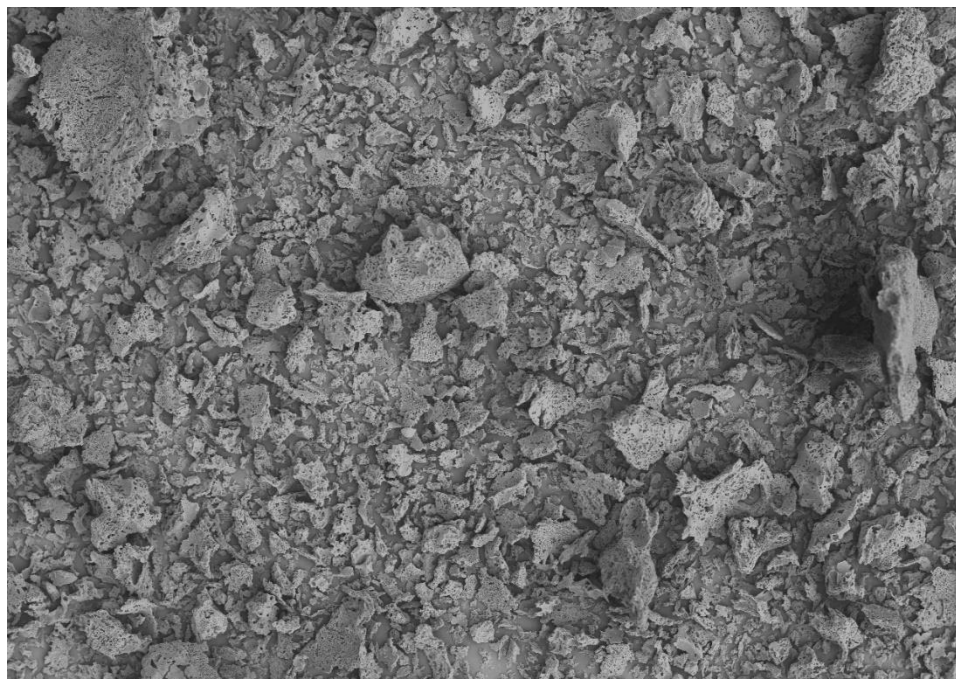

Clariant SU7000 5.00kV 6.3mm x100 UD+LD+MD 04/10/2025 500µm

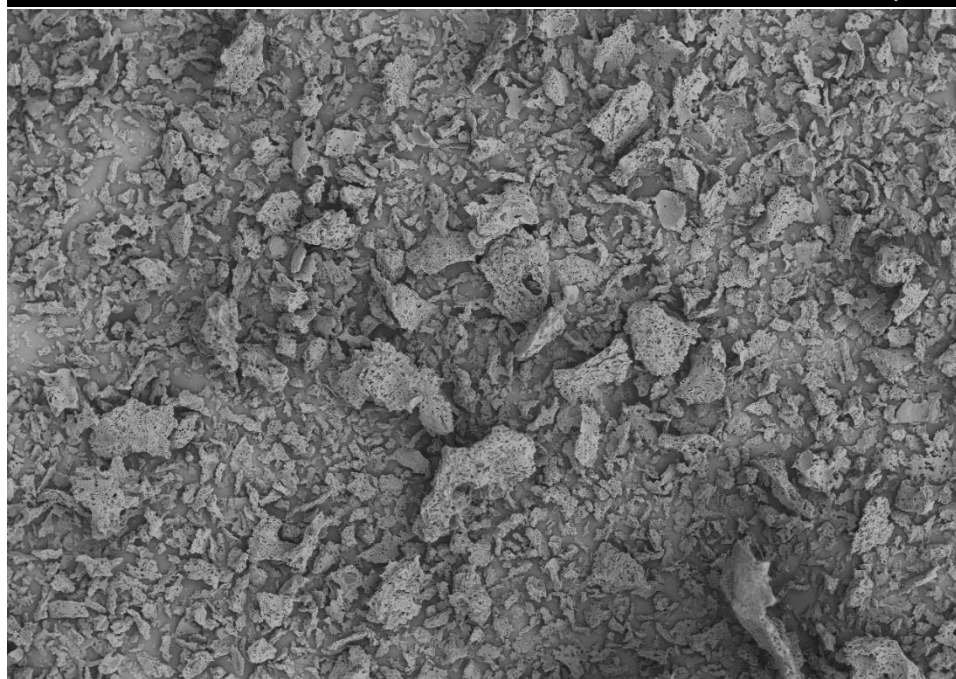


Clariant SU7000 5.00kV 6.2mm x100 UD+LD+MD 04/10/2025 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3063/MB3064/MB3066/MRa420 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-10

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

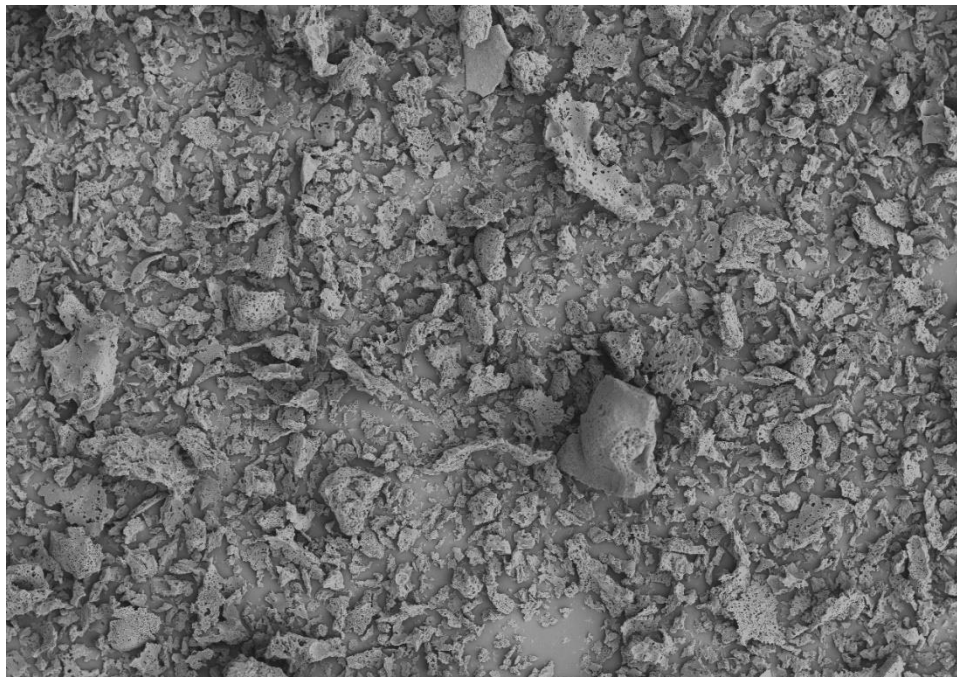

Clariant SU7000 5.00kV 6.2mm x100 UD+LD+MD 04/10/2025 500µm

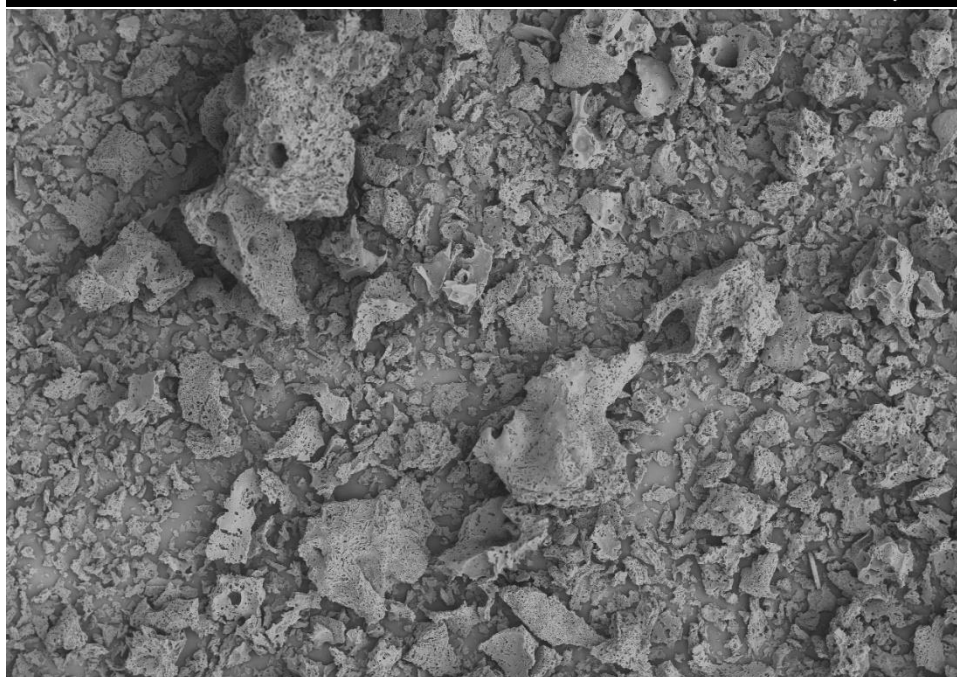


Clariant SU7000 5.00kV 6.2mm x100 UD+LD+MD 04/10/2025 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3063/MB3064/MB3066/MRa420 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-10

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

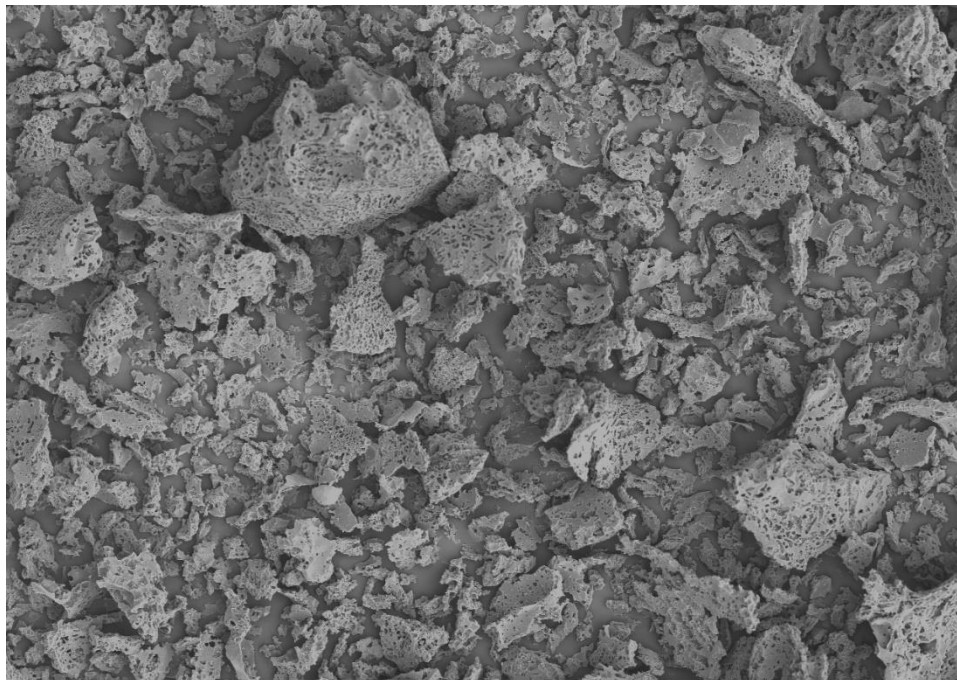

Clariant SU7000 5.00kV 6.3mm x200 UD+LD+MD 04/10/2025 200µm

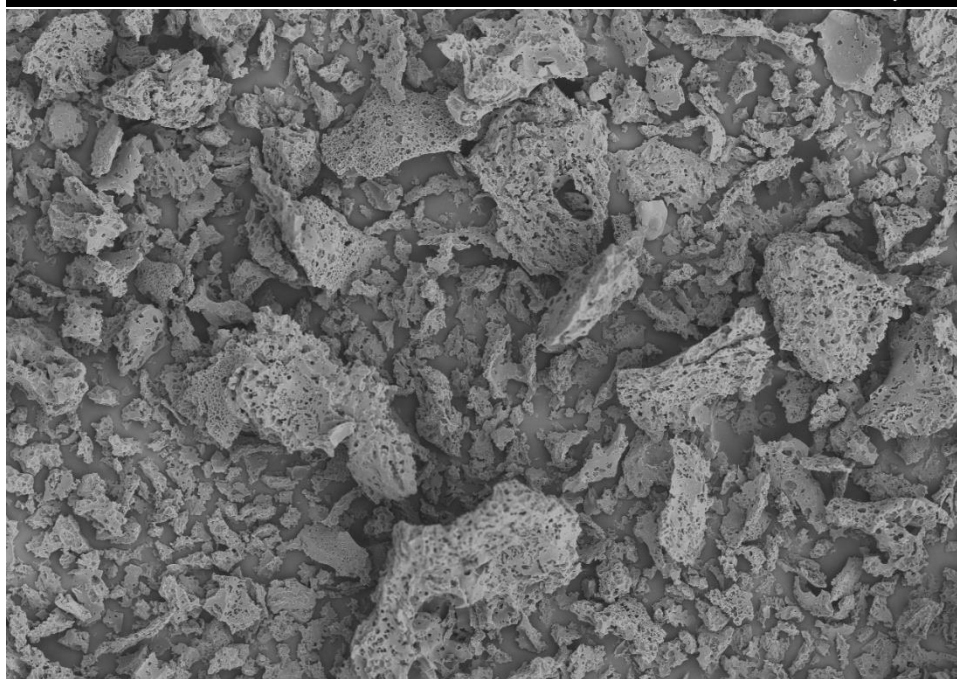


Clariant SU7000 5.00kV 6.2mm x200 UD+LD+MD 04/10/2025 200µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3063/MB3064/MB3066/MRa420 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-10

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

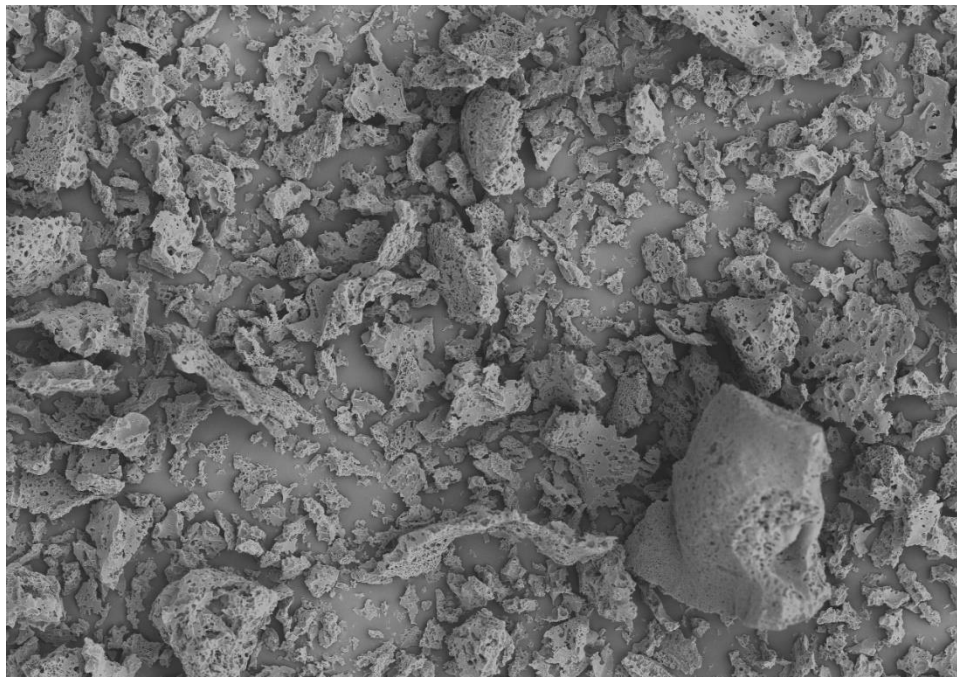

Clariant SU7000 5.00kV 6.2mm x200 UD+LD+MD 04/10/2025 200µm

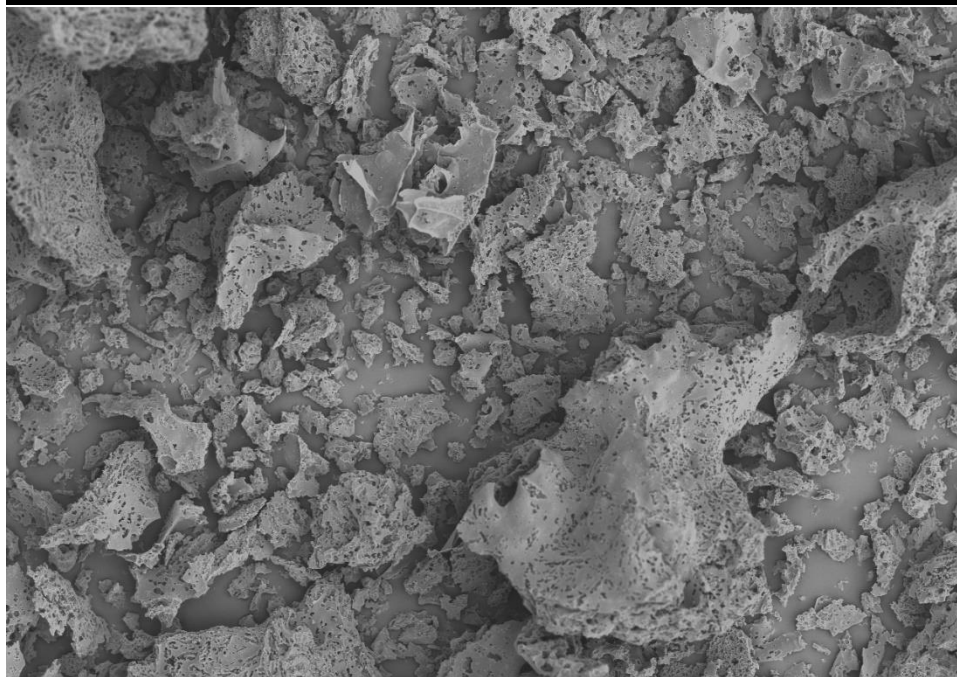


Clariant SU7000 5.00kV 6.2mm x200 UD+LD+MD 04/10/2025 200µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3063/MB3064/MB3066/MRa420 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-10

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

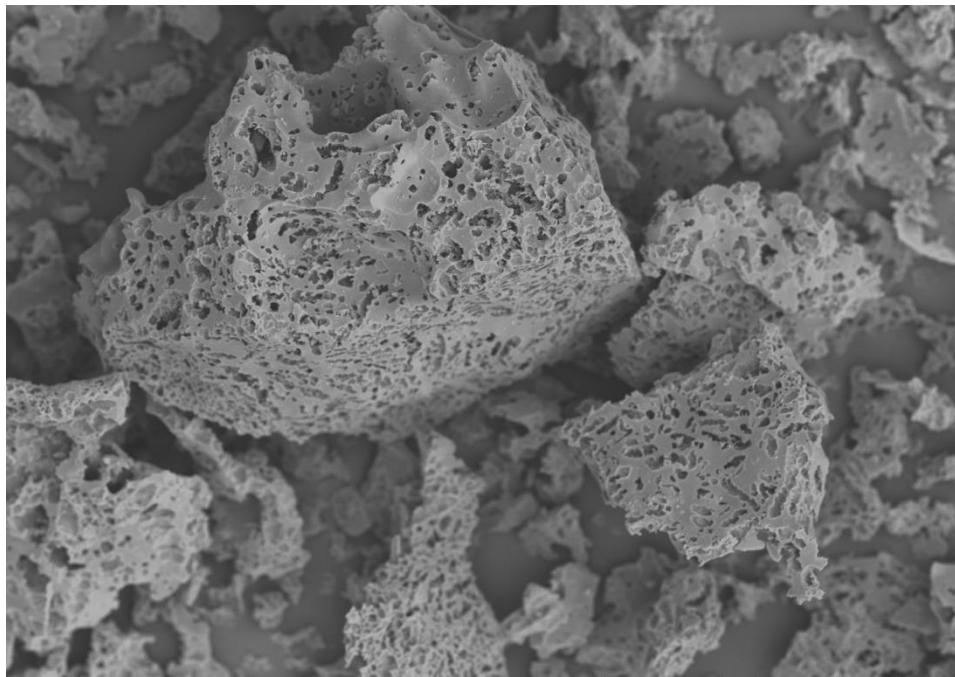

Clariant SU7000 5.00kV 6.1mm x500 UD+LD+MD 04/10/2025 100µm

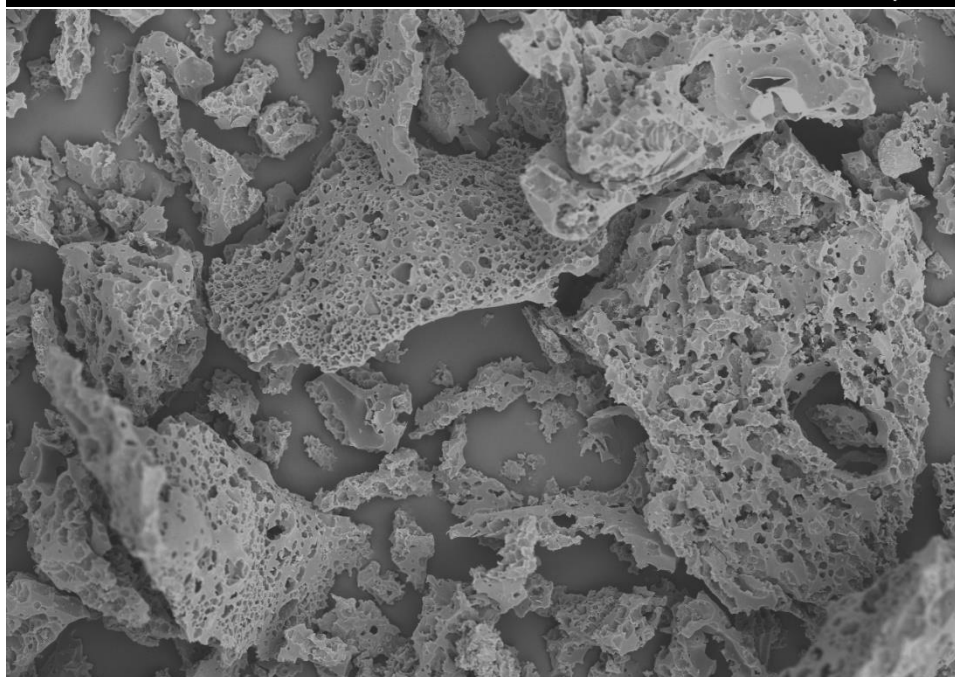


Clariant SU7000 5.00kV 6.2mm x500 UD+LD+MD 04/10/2025 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3063/MB3064/MB3066/MRa420 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-10

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

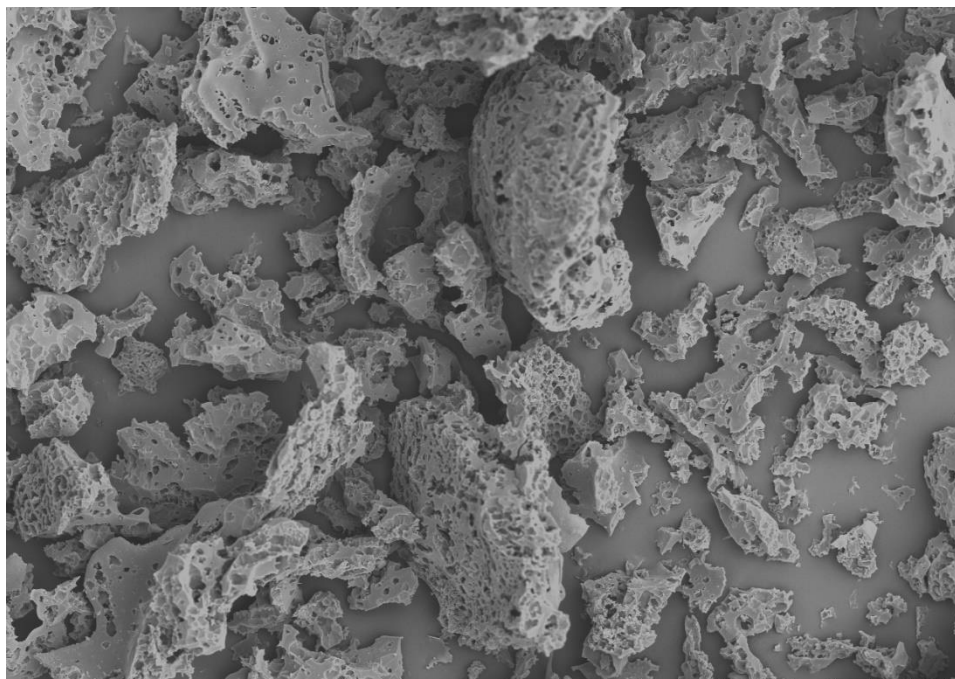

Clariant SU7000 5.00kV 6.2mm x500 UD+LD+MD 04/10/2025 100µm

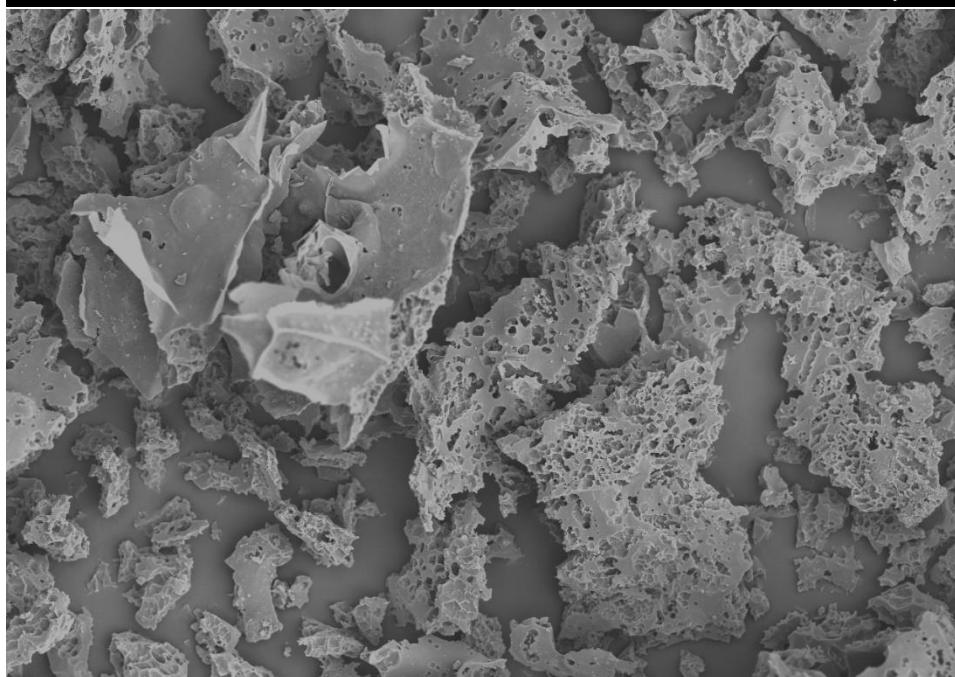


Clariant SU7000 5.00kV 6.2mm x500 UD+LD+MD 04/10/2025 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3063/MB3064/MB3066/MRa420 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-10

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

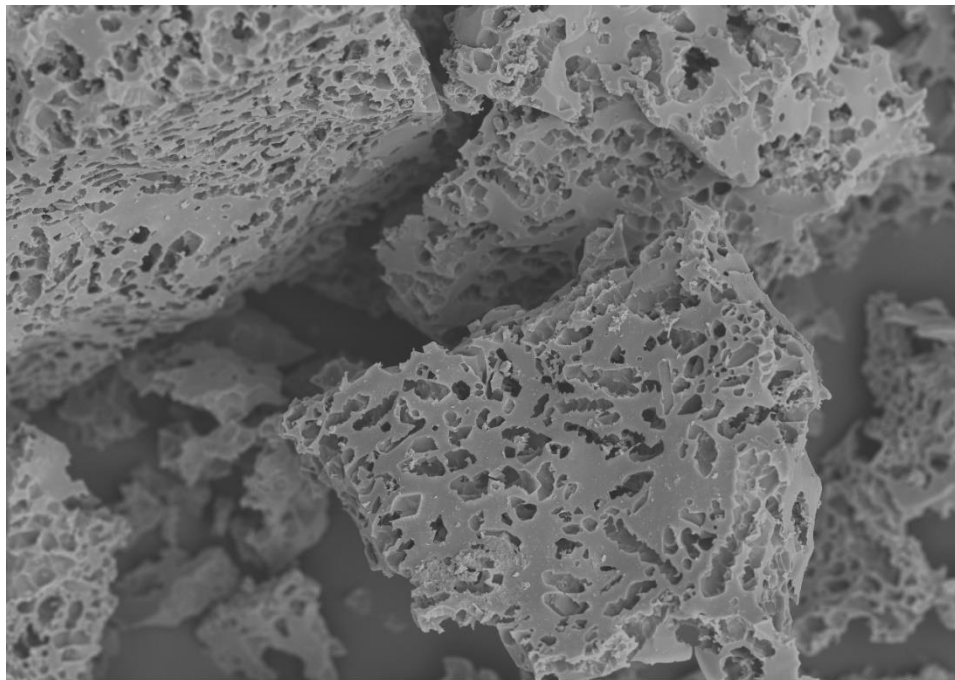

Clariant SU7000 5.00kV 6.2mm x1.00k UD+LD+MD 04/10/2025 50.0µm

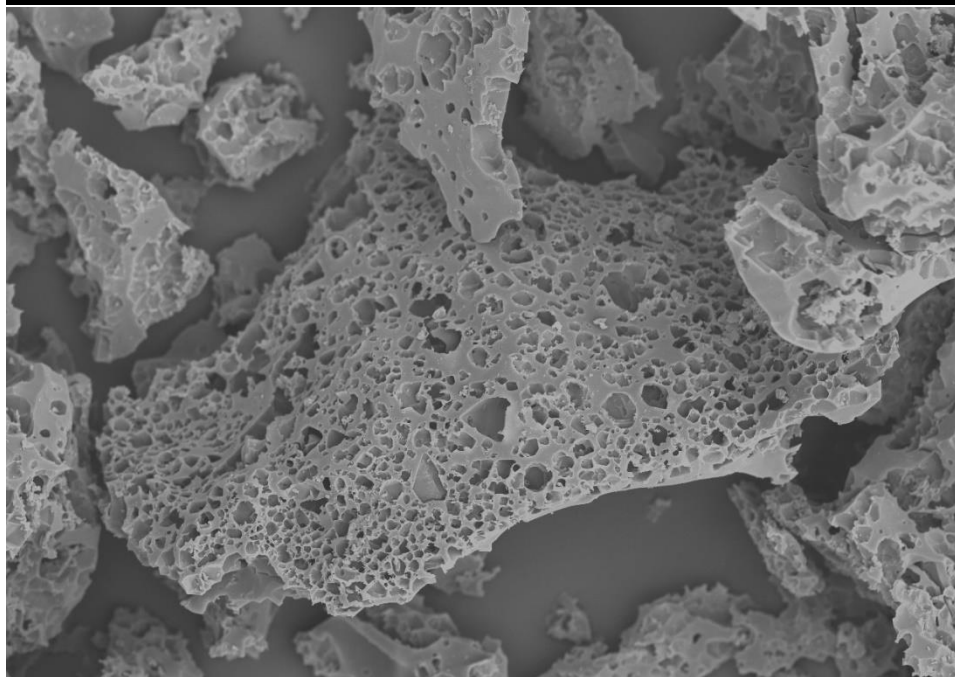


Clariant SU7000 5.00kV 6.2mm x1.00k UD+LD+MD 04/10/2025 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3063/MB3064/MB3066/MRa420 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-10

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

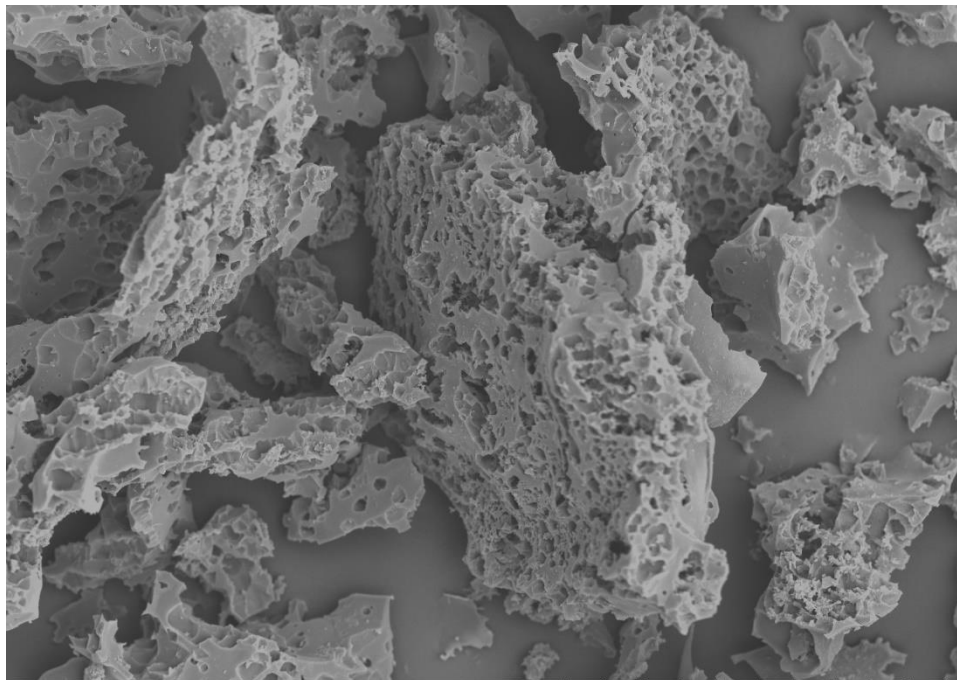

Clariant SU7000 5.00kV 6.2mm x1.00k UD+LD+MD 04/10/2025 50.0µm

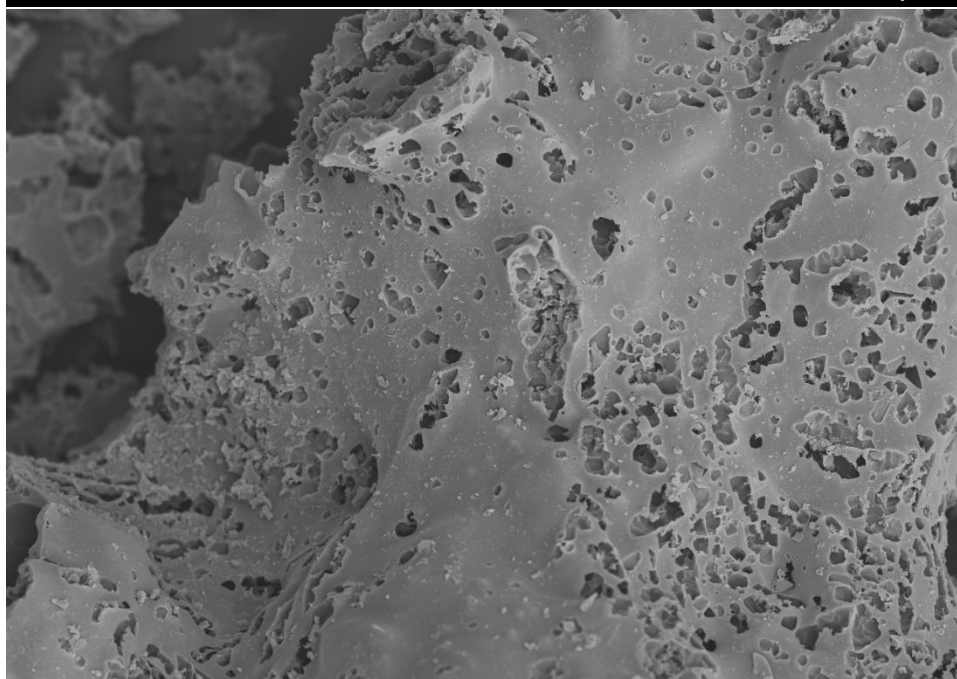


Clariant SU7000 5.00kV 6.1mm x1.00k UD+LD+MD 04/10/2025 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3063/MB3064/MB3066/MRa420 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-10

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

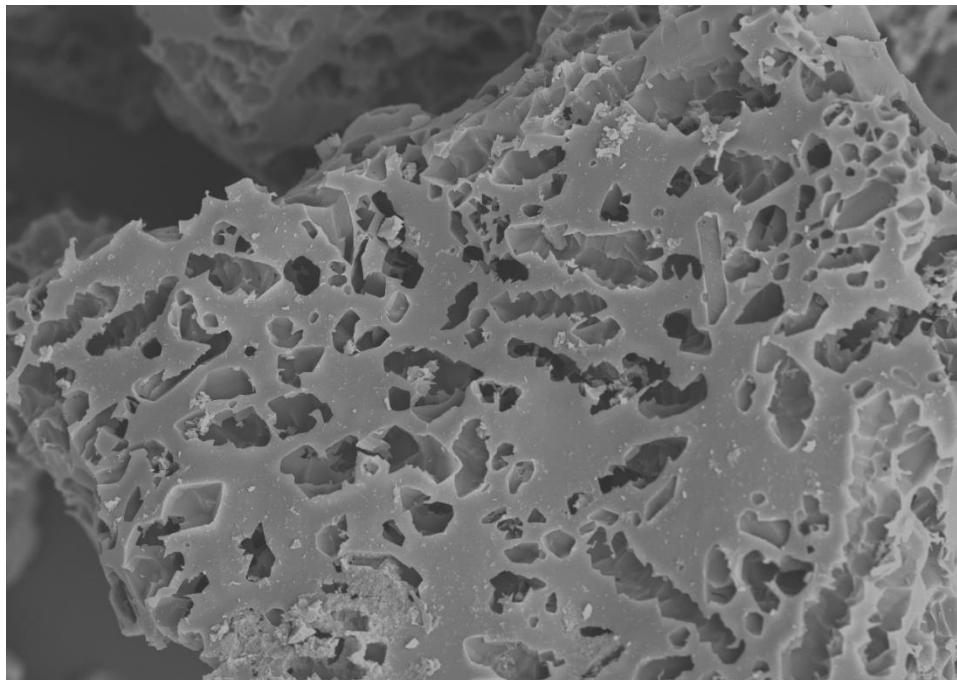

Clariant SU7000 5.00kV 6.2mm x2.00k UD+LD+MD 04/10/2025 20.0µm

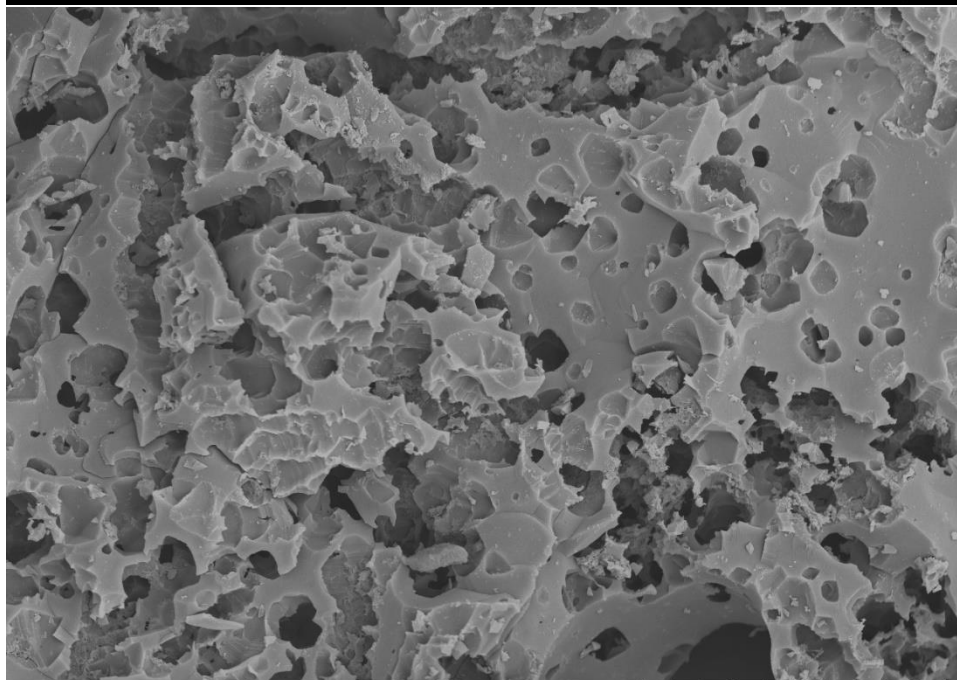


Clariant SU7000 5.00kV 6.2mm x2.00k UD+LD+MD 04/10/2025 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3063/MB3064/MB3066/MRa420 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-10

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

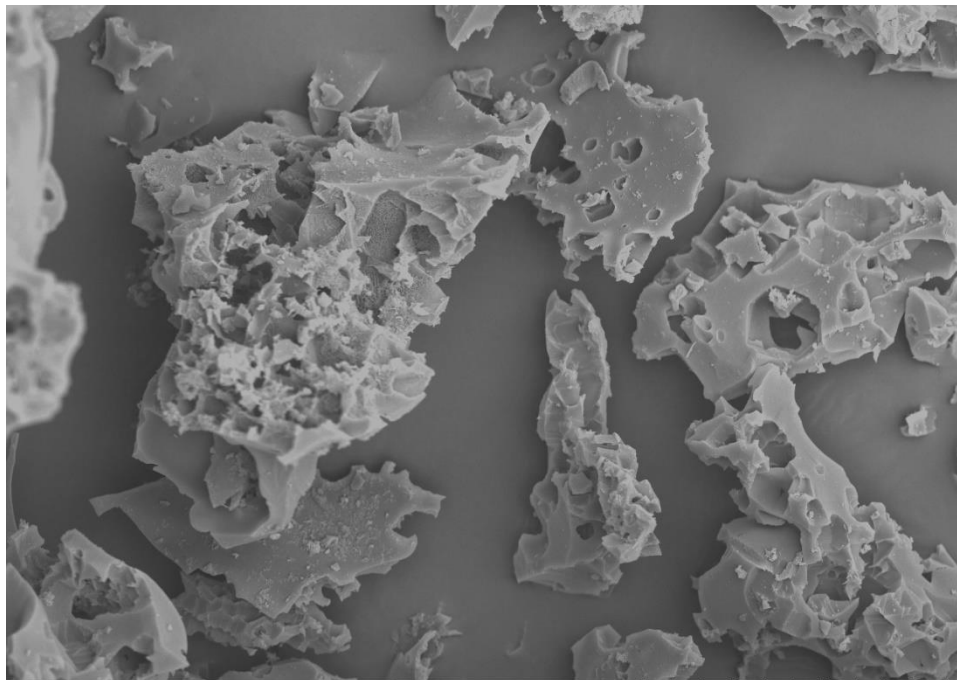

Clariant SU7000 5.00kV 6.2mm x2.00k UD+LD+MD 04/10/2025 20.0µm

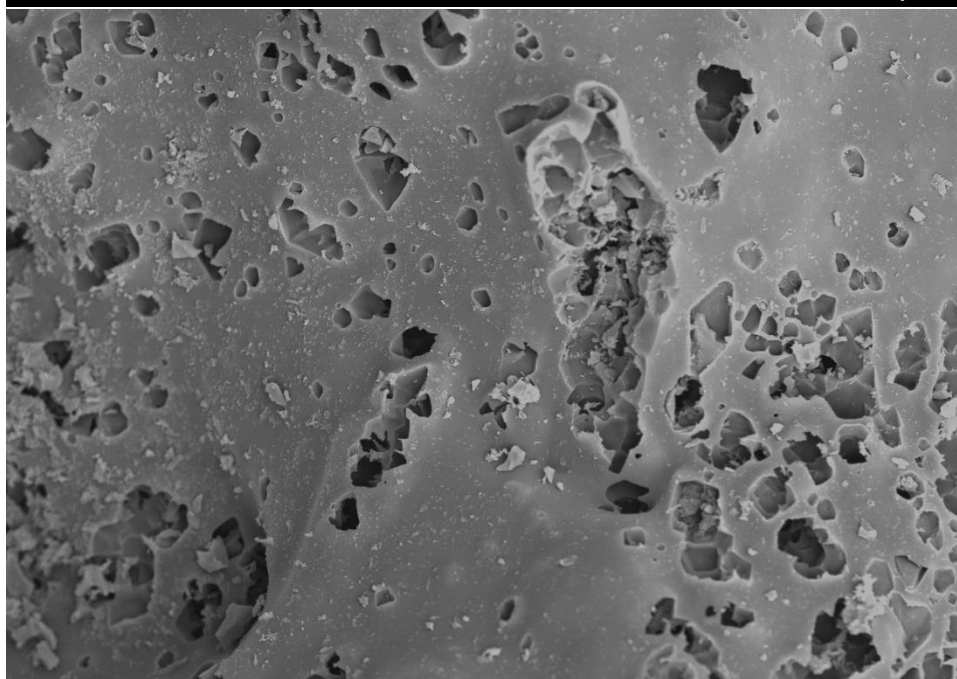


Clariant SU7000 5.00kV 6.1mm x2.00k UD+LD+MD 04/10/2025 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3063/MB3064/MB3066/MRa420 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-10

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

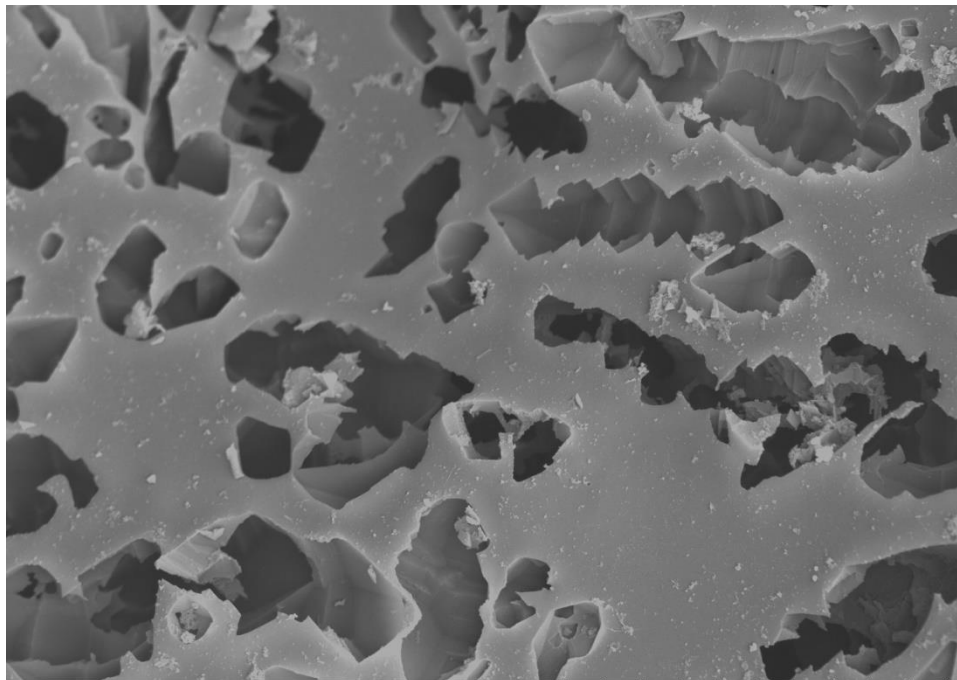

Clariant SU7000 5.00kV 6.2mm x5.00k UD+LD+MD 04/10/2025 10.0µm

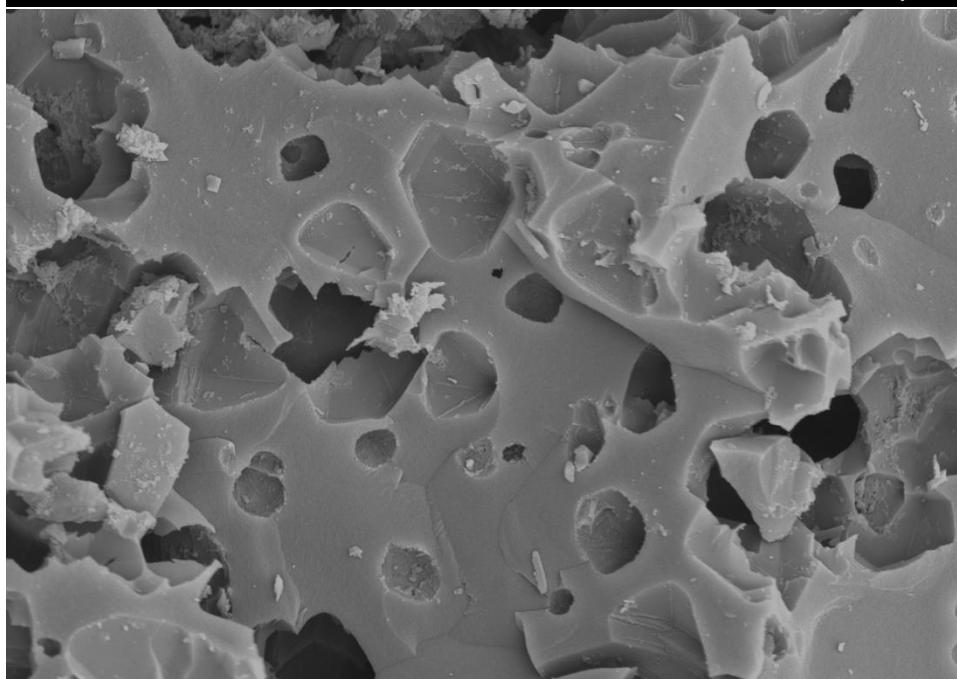


Clariant SU7000 5.00kV 6.2mm x5.00k UD+LD+MD 04/10/2025 10.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3063/MB3064/MB3066/MRa420 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-10

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

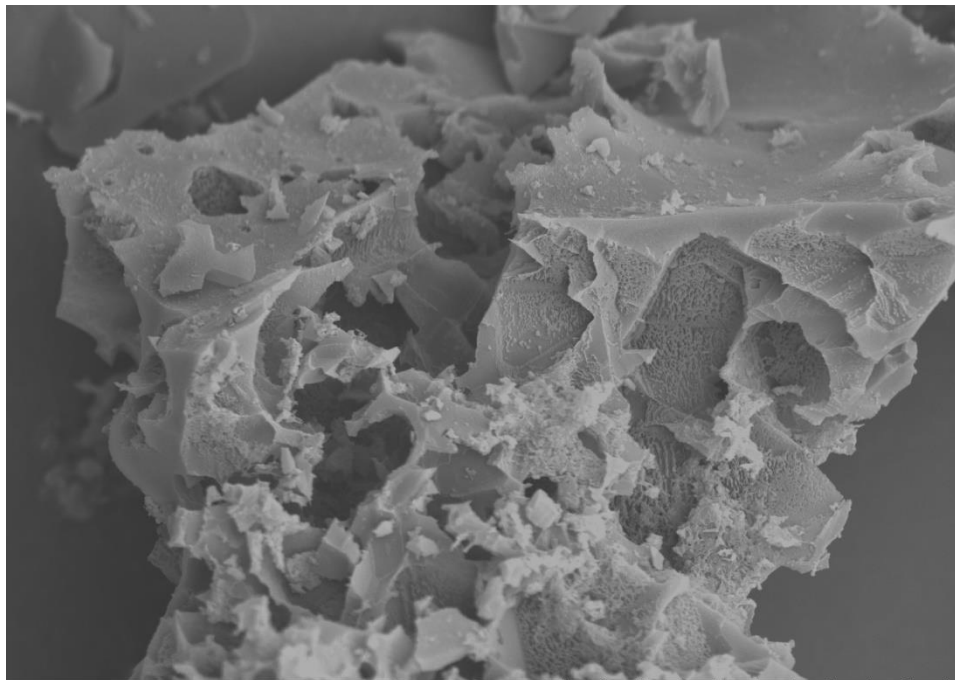

Clariant SU7000 5.00kV 6.2mm x5.00k UD+LD+MD 04/10/2025 10.0µm

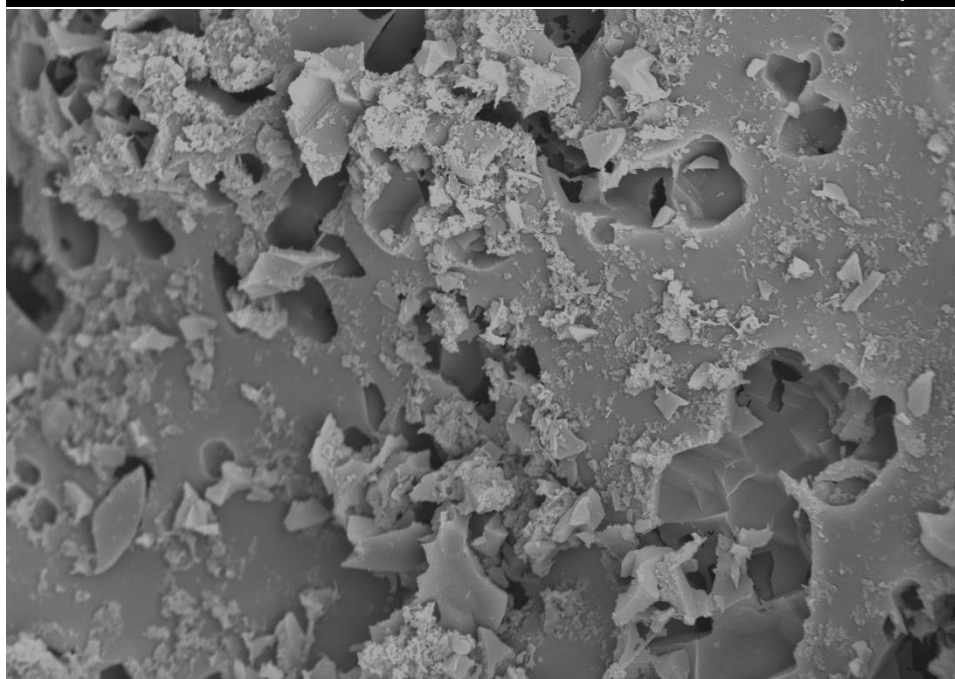

Clariant SU7000 5.00kV 6.2mm x5.00k UD+LD+MD 04/10/2025 10.0µm