

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa419A 2/3 1+3min 800C 3C/m 1h A 2x0.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049736-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

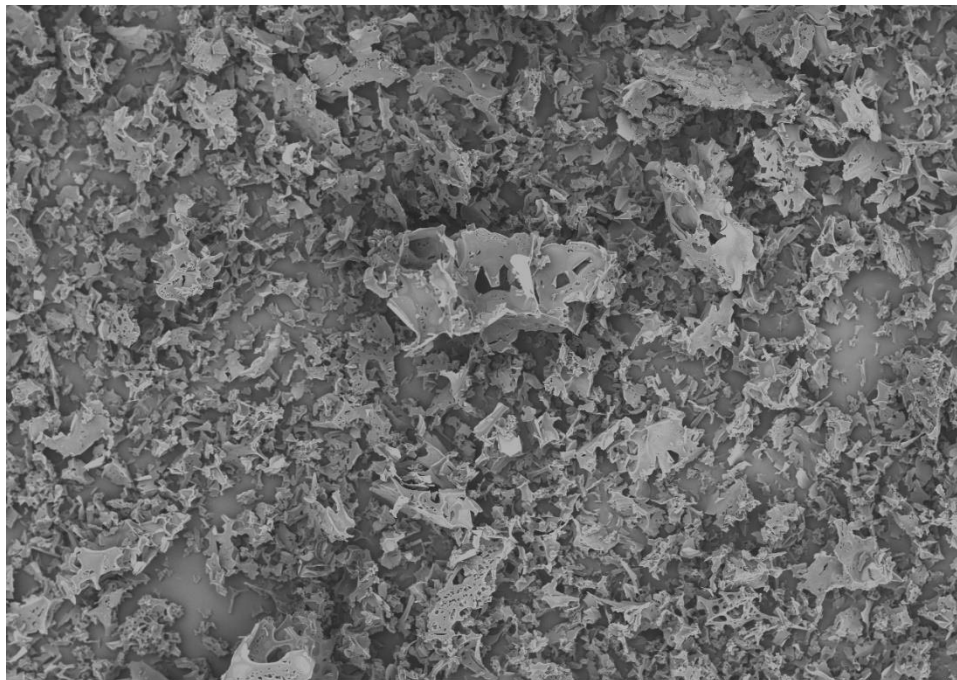

Clariant SU7000 5.00kV 6.2mm x100 UD+LD+MD 04/08/2025 500µm

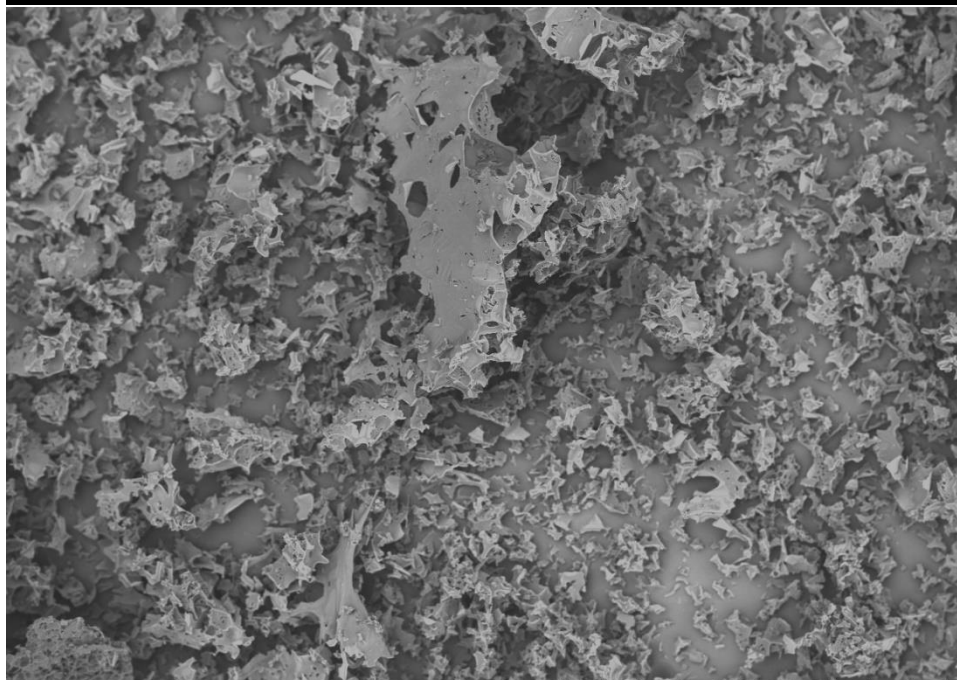


Clariant SU7000 5.00kV 6.1mm x100 UD+LD+MD 04/08/2025 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa419A 2/3 1+3min 800C 3C/m 1h A 2x0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

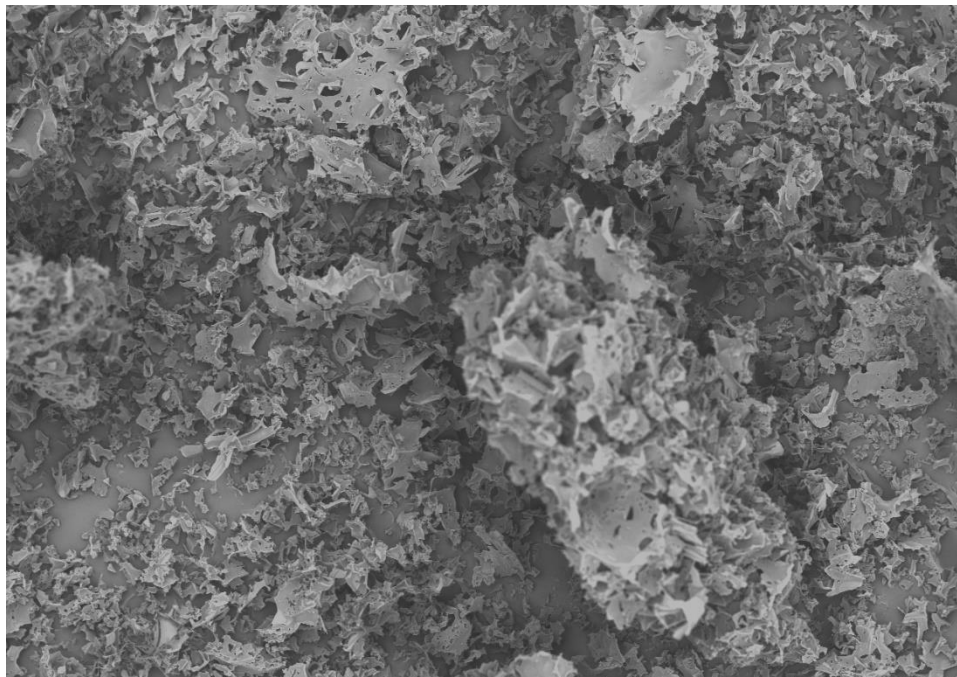

Clariant SU7000 5.00kV 6.4mm x100 UD+LD+MD 04/08/2025 500µm

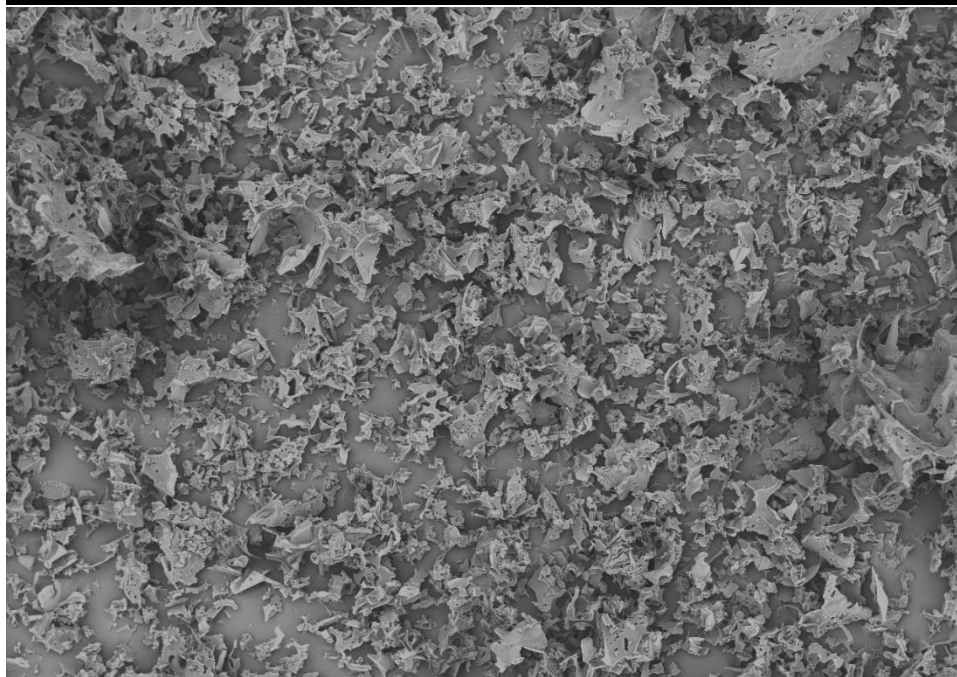


Clariant SU7000 5.00kV 6.4mm x100 UD+LD+MD 04/08/2025 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa419A 2/3 1+3min 800C 3C/m 1h A 2x0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

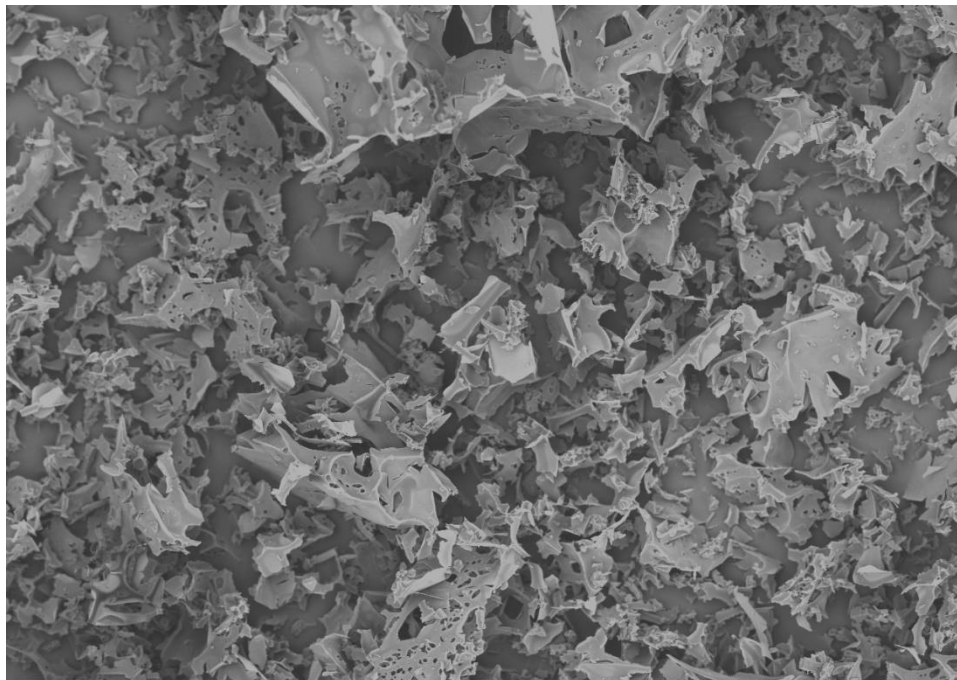

Clariant SU7000 5.00kV 6.2mm x200 UD+LD+MD 04/08/2025 200µm

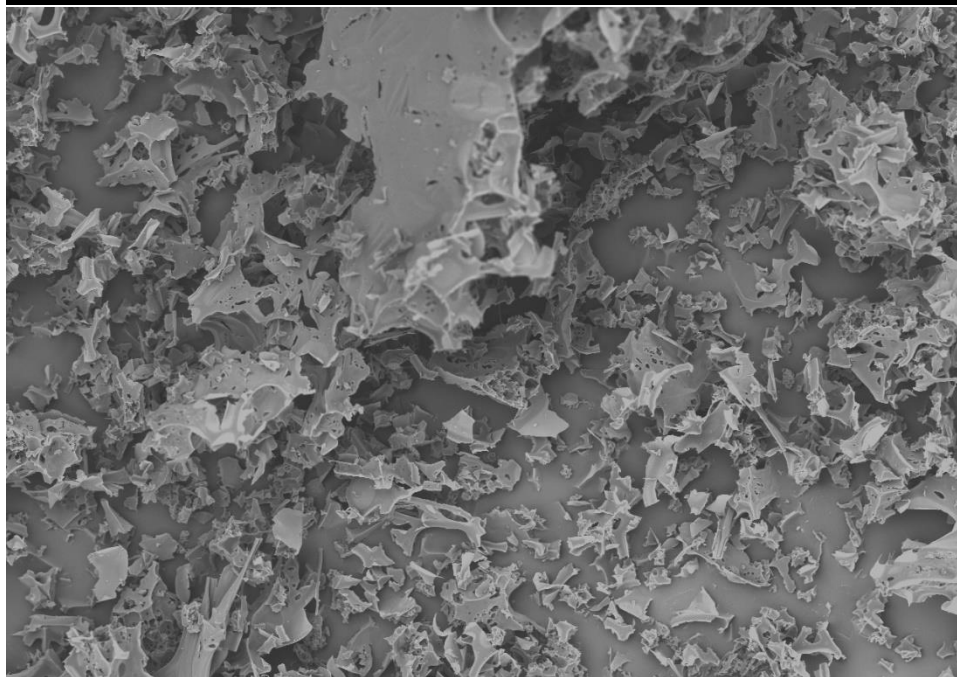


Clariant SU7000 5.00kV 6.3mm x200 UD+LD+MD 04/08/2025 200µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa419A 2/3 1+3min 800C 3C/m 1h A 2x0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

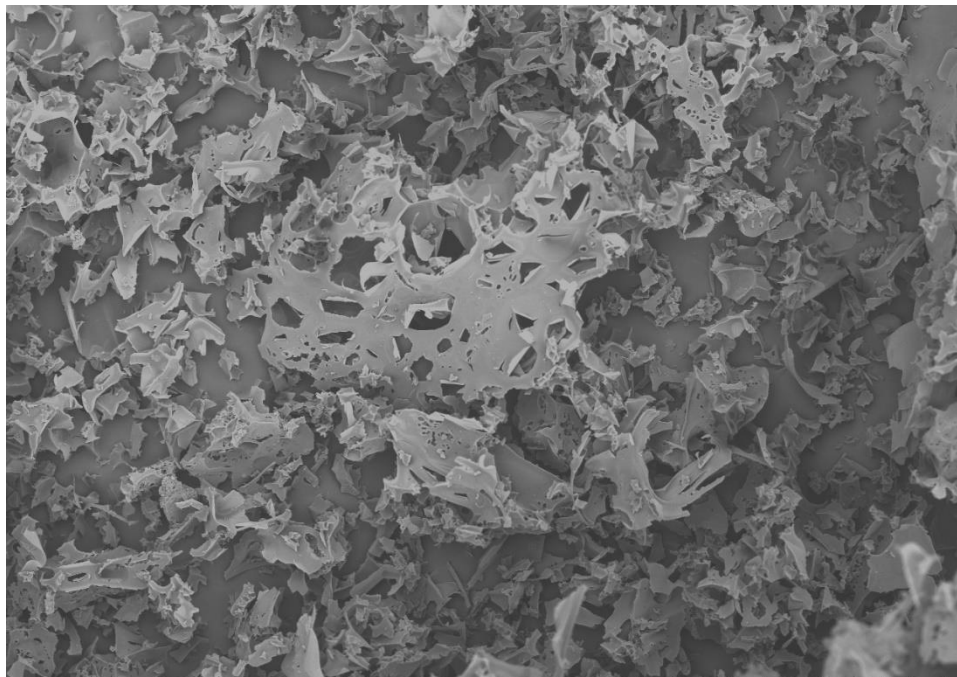

Clariant SU7000 5.00kV 6.4mm x200 UD+LD+MD 04/08/2025 200µm

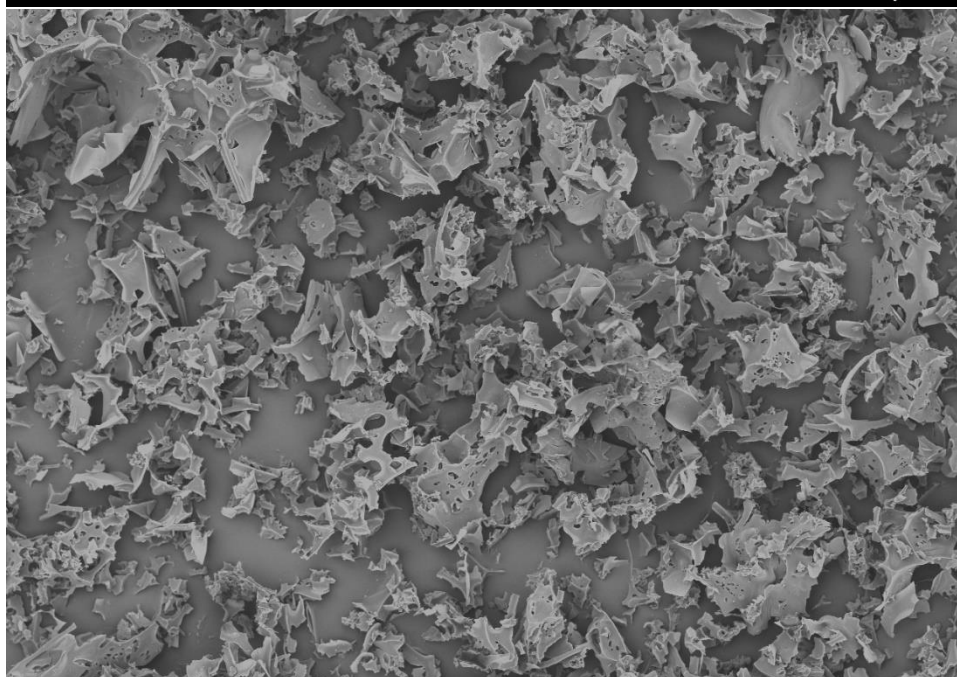


Clariant SU7000 5.00kV 6.4mm x200 UD+LD+MD 04/08/2025 200µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa419A 2/3 1+3min 800C 3C/m 1h A 2x0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

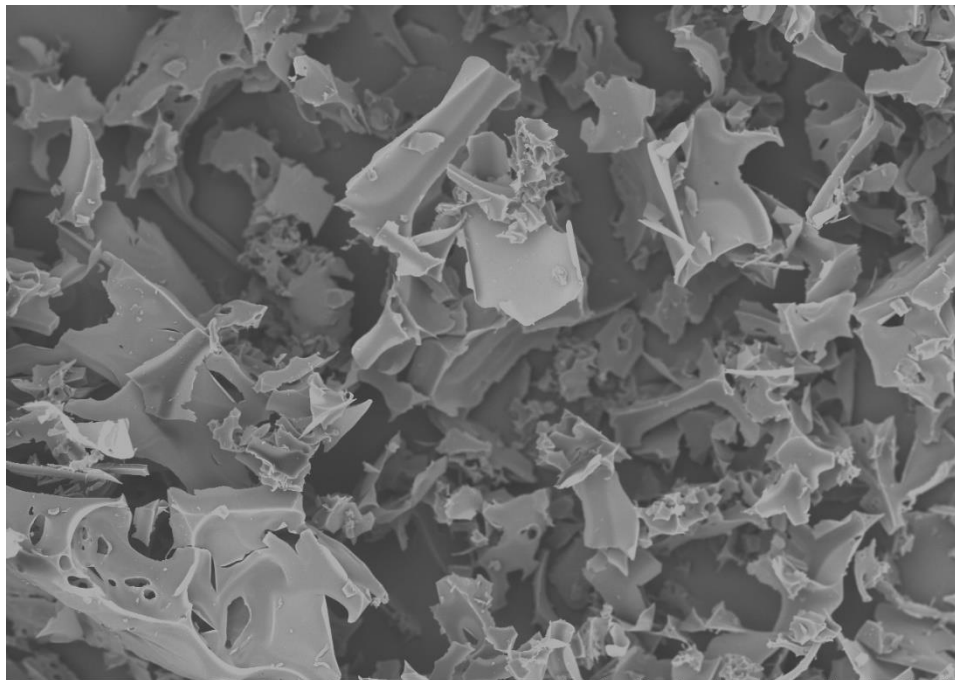

Clariant SU7000 5.00kV 6.2mm x500 UD+LD+MD 04/08/2025 100µm

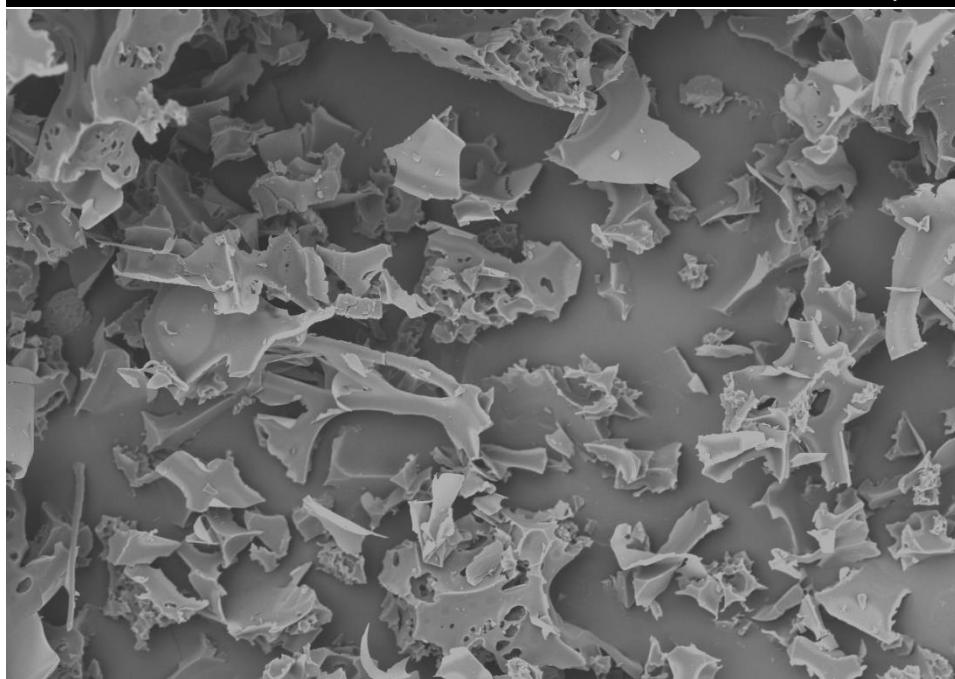


Clariant SU7000 5.00kV 6.3mm x500 UD+LD+MD 04/08/2025 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa419A 2/3 1+3min 800C 3C/m 1h A 2x0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

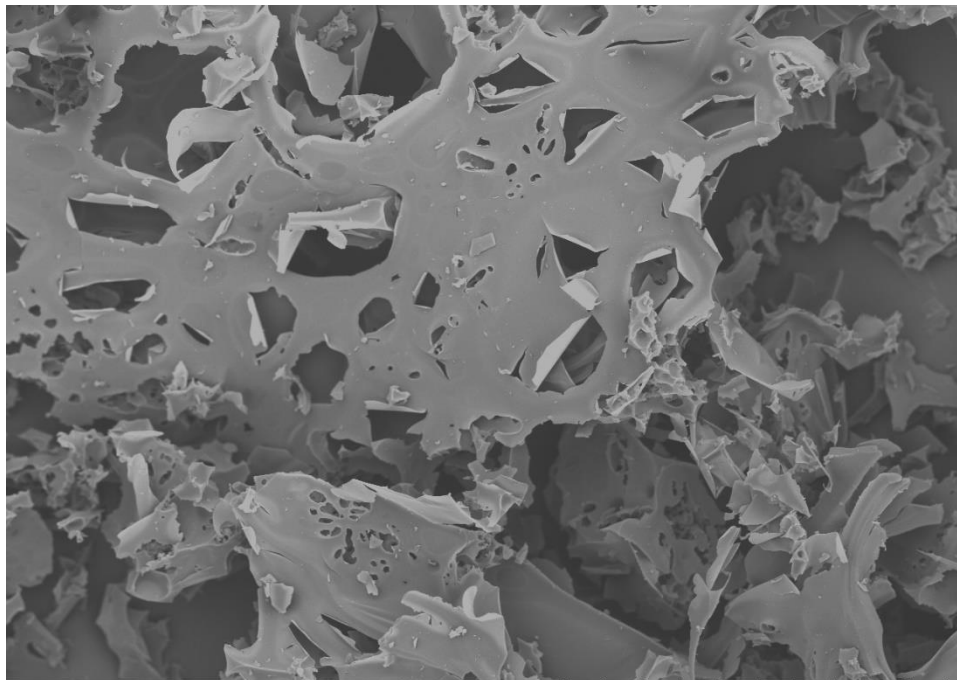

Clariant SU7000 5.00kV 6.3mm x500 UD+LD+MD 04/08/2025 100µm

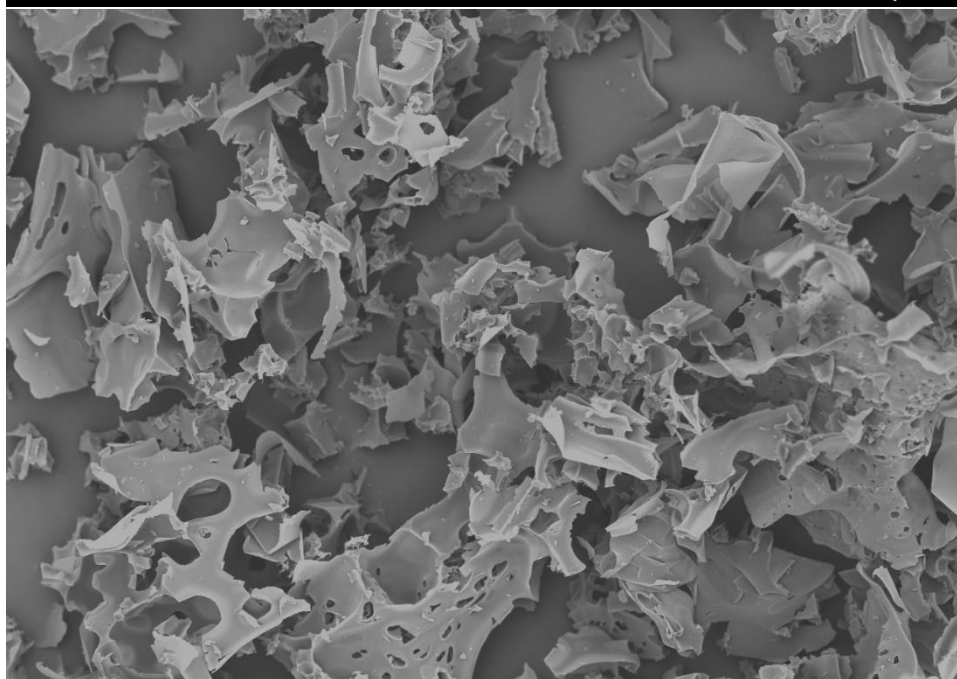

Clariant SU7000 5.00kV 6.4mm x500 UD+LD+MD 04/08/2025 100µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa419A 2/3 1+3min 800C 3C/m 1h A 2x0.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049736-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

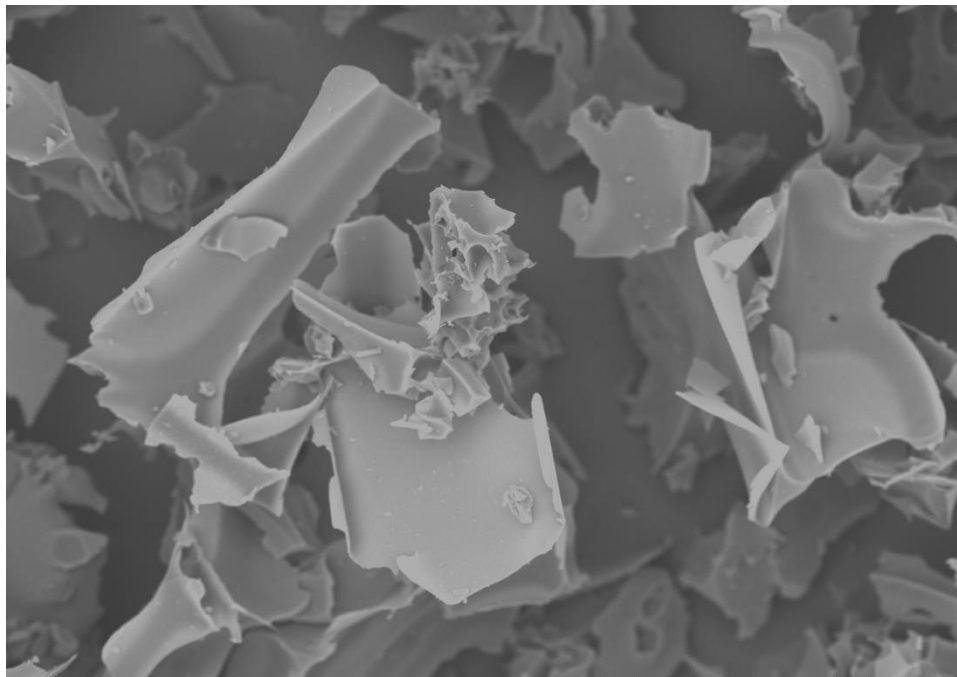

Clariant SU7000 5.00kV 6.2mm x1.00k UD+LD+MD 04/08/2025 50.0µm

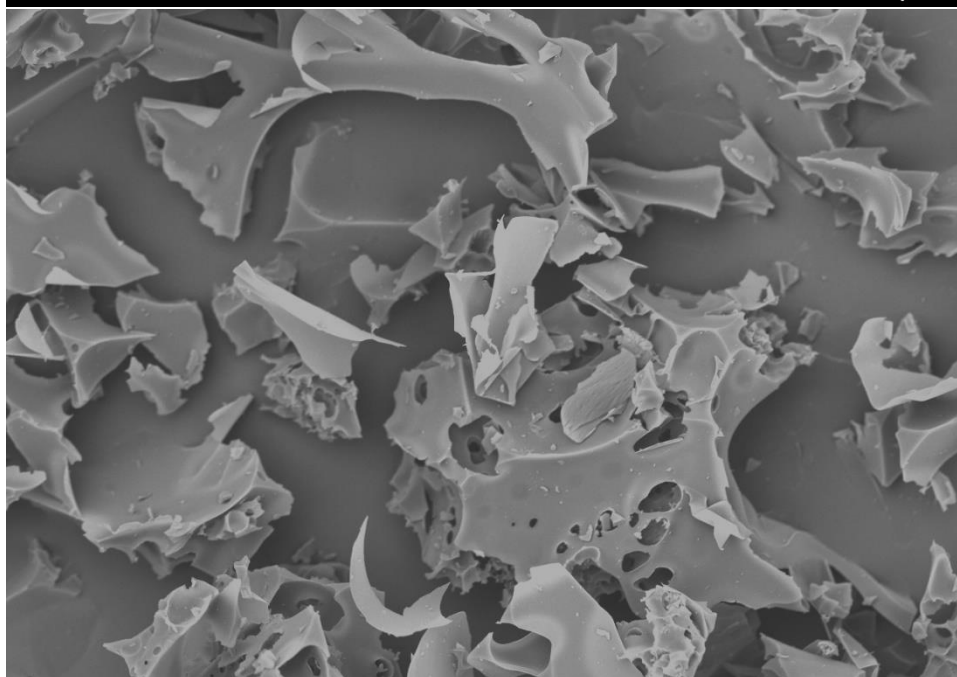


Clariant SU7000 5.00kV 6.3mm x1.00k UD+LD+MD 04/08/2025 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa419A 2/3 1+3min 800C 3C/m 1h A 2x0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

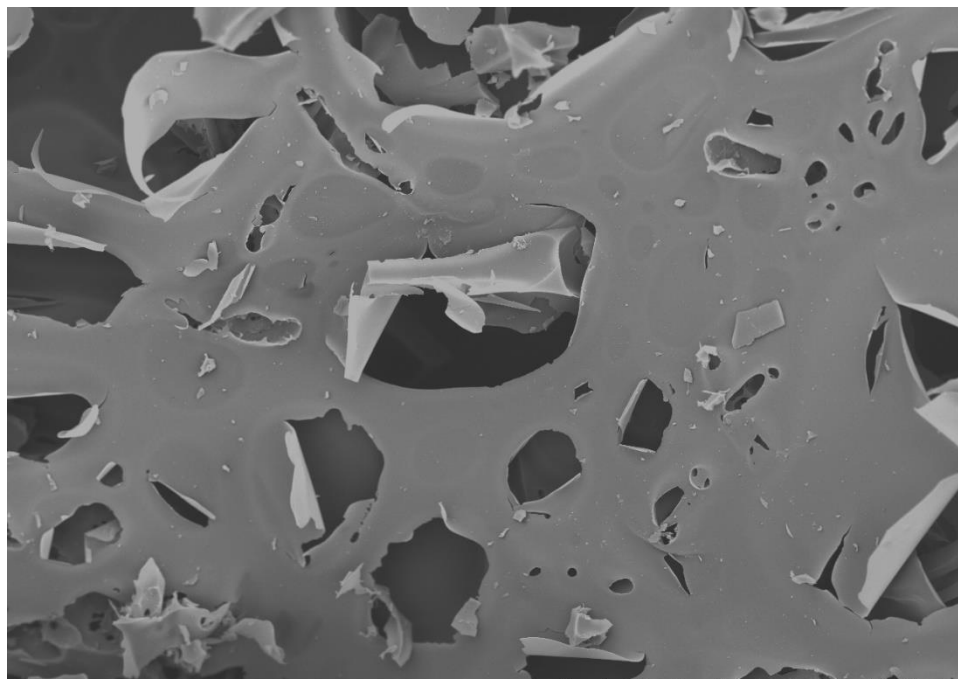

Clariant SU7000 5.00kV 6.3mm x1.00k UD+LD+MD 04/08/2025 50.0µm

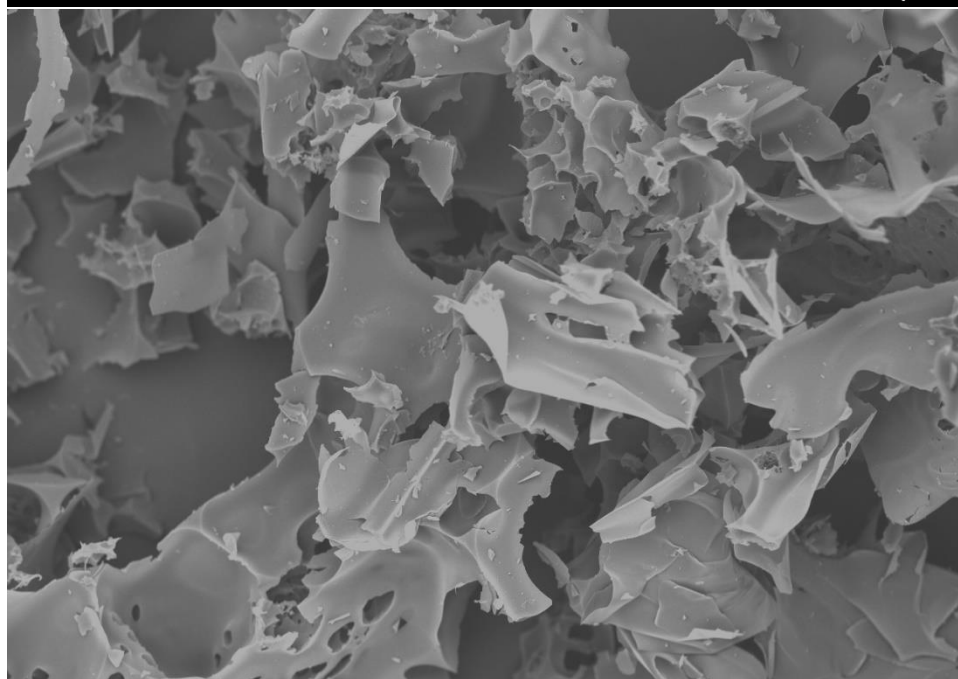

Clariant SU7000 5.00kV 6.4mm x1.00k UD+LD+MD 04/08/2025 50.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa419A 2/3 1+3min 800C 3C/m 1h A 2x0.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049736-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

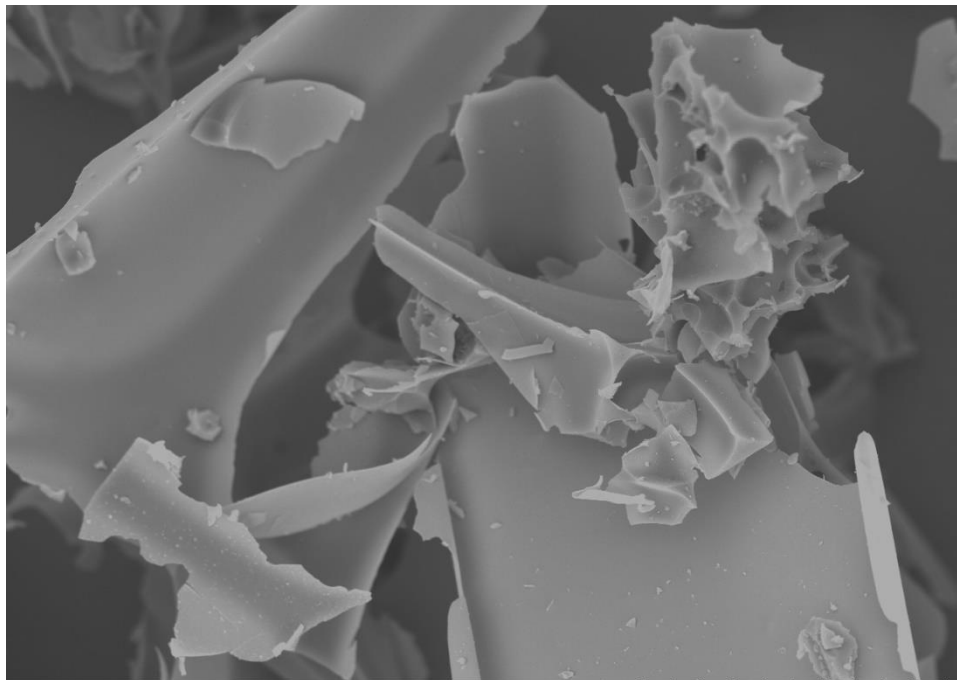

Clariant SU7000 5.00kV 6.3mm x2.00k UD+LD+MD 04/08/2025 20.0µm

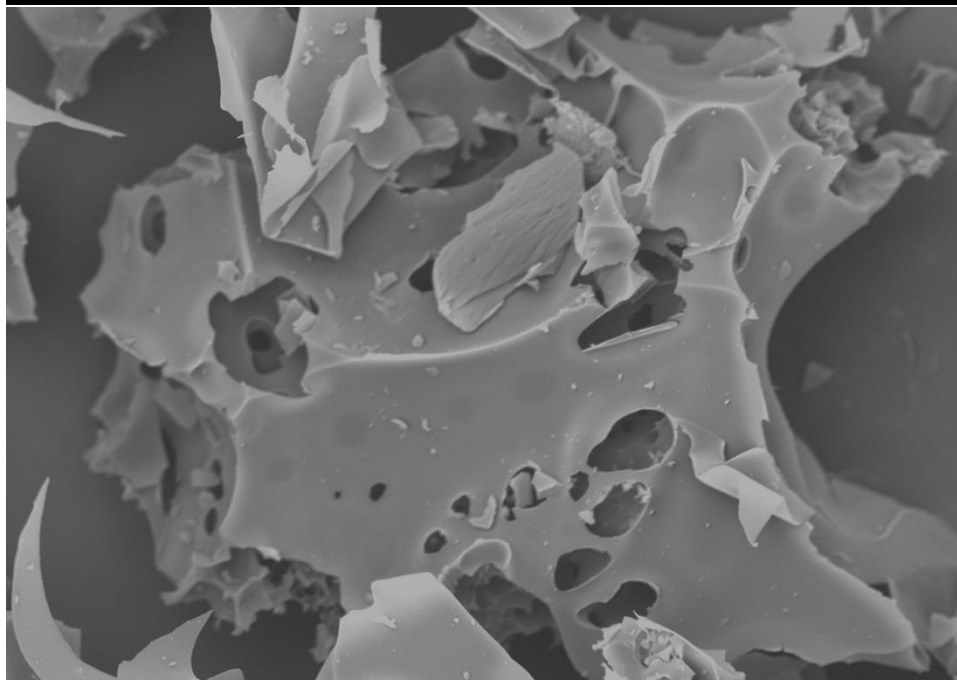


Clariant SU7000 5.00kV 6.3mm x2.00k UD+LD+MD 04/08/2025 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa419A 2/3 1+3min 800C 3C/m 1h A 2x0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

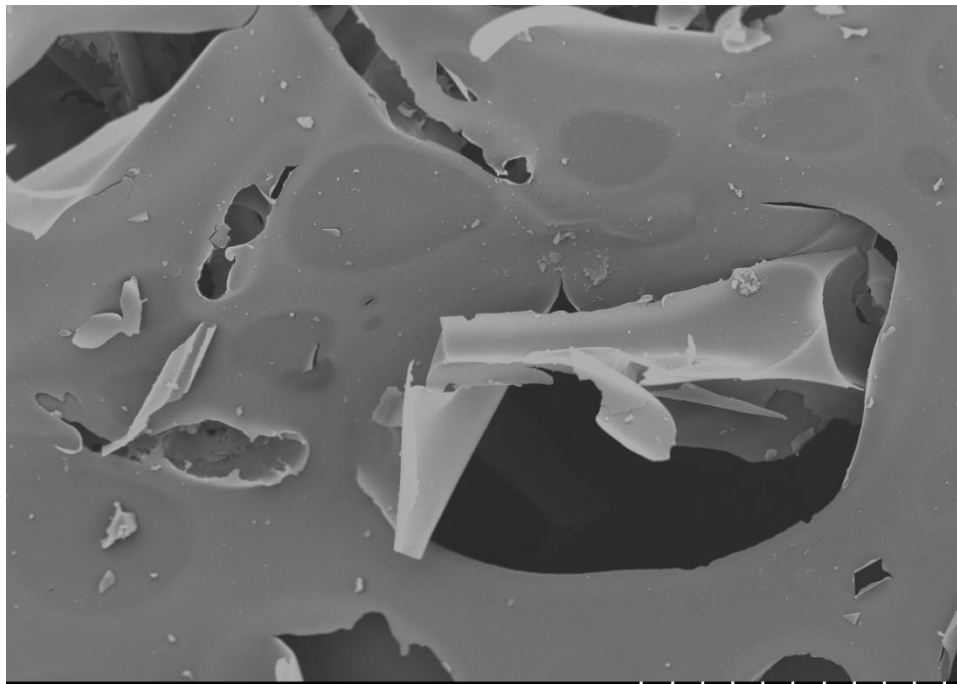

Clariant SU7000 5.00kV 6.3mm x2.00k UD+LD+MD 04/08/2025 20.0µm

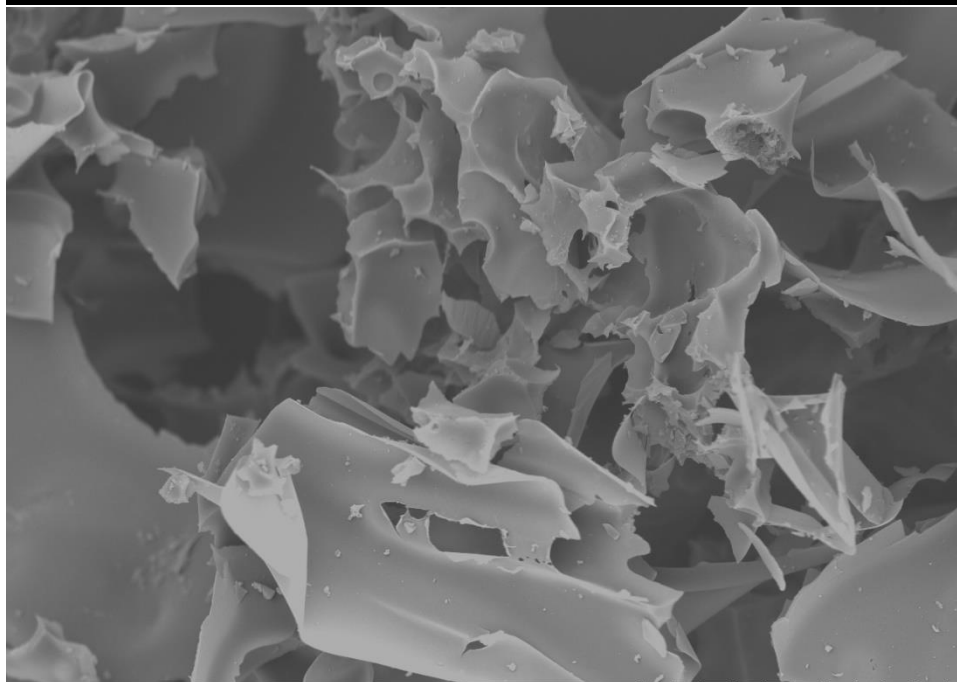


Clariant SU7000 5.00kV 6.3mm x2.00k UD+LD+MD 04/08/2025 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa419A 2/3 1+3min 800C 3C/m 1h A 2x0.6P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049736-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

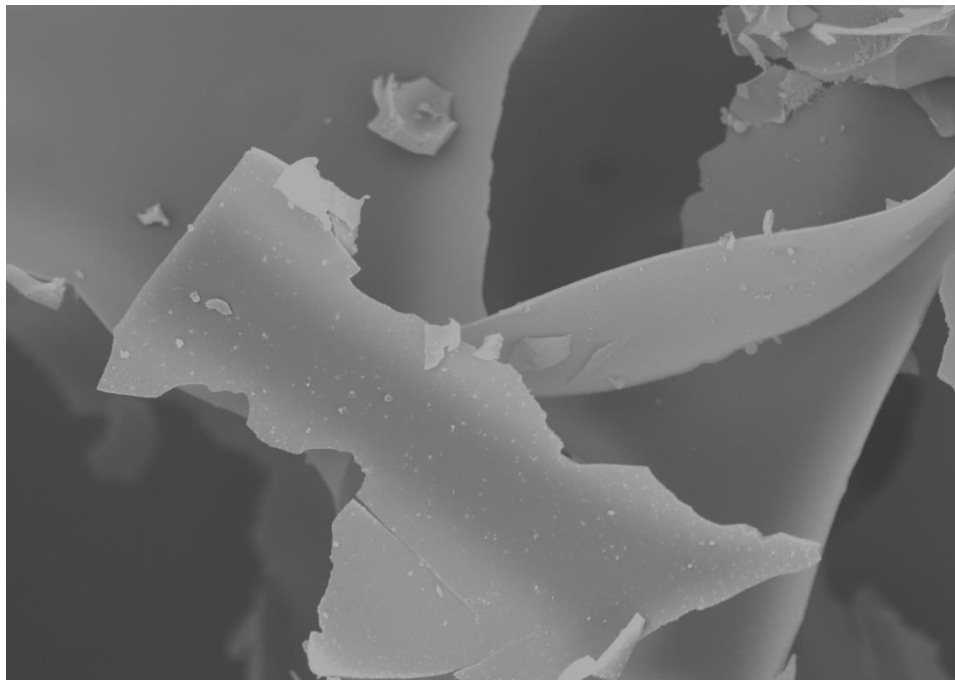

Clariant SU7000 5.00kV 6.3mm x5.00k UD+LD+MD 04/08/2025 10.0µm

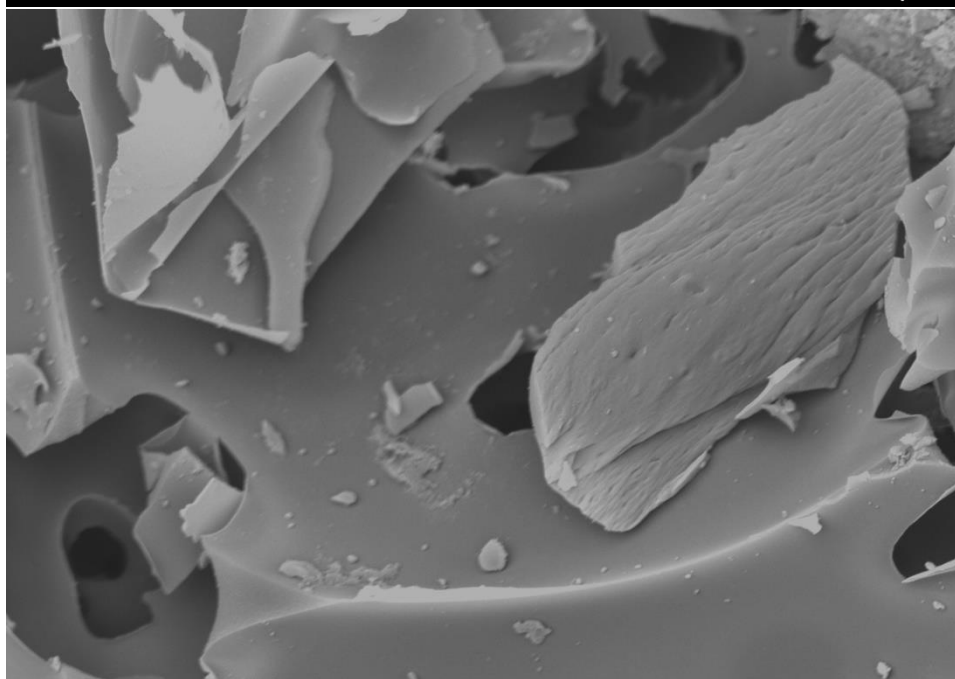

Clariant SU7000 5.00kV 6.4mm x5.00k UD+LD+MD 04/08/2025 10.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MRa419A 2/3 1+3min 800C 3C/m 1h A 2x0.6P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-049736-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

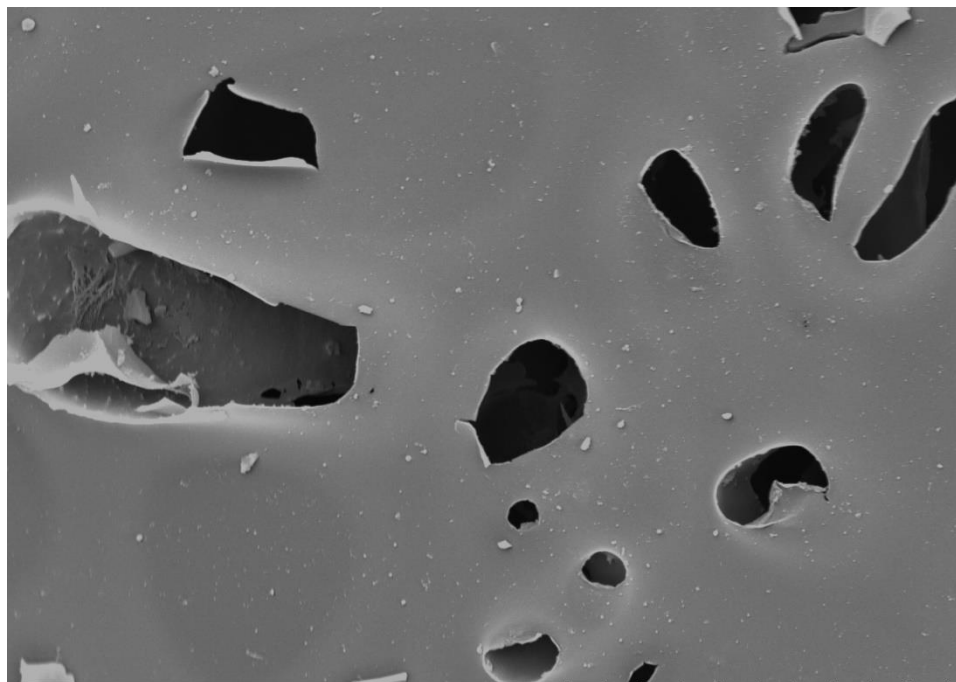

Clariant SU7000 5.00kV 6.3mm x5.00k UD+LD+MD 04/08/2025 10.0µm

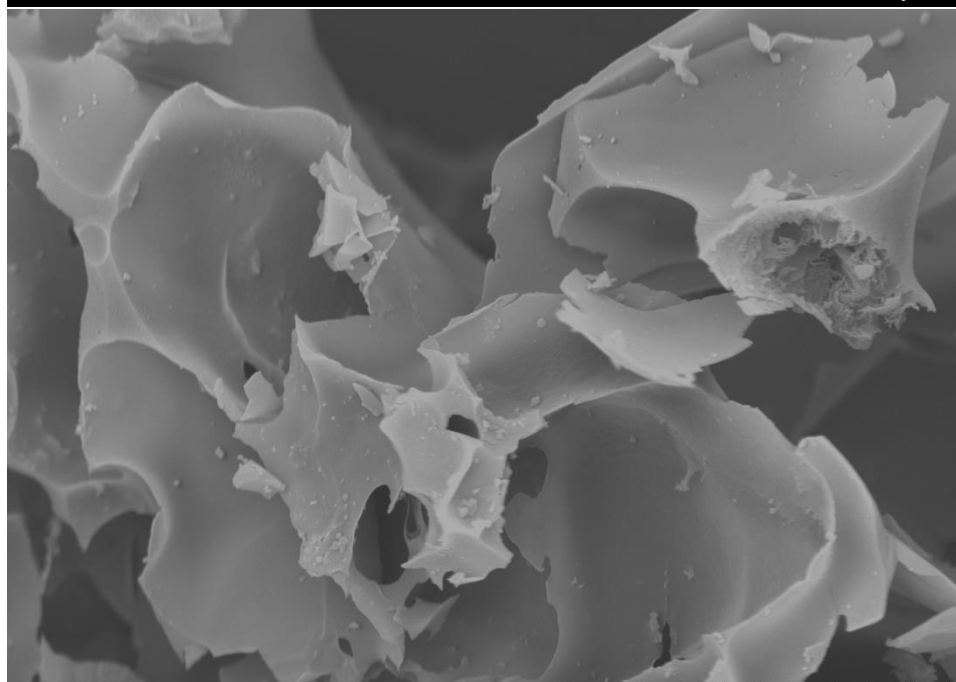

Clariant SU7000 5.00kV 6.3mm x5.00k UD+LD+MD 04/08/2025 10.0µm