



SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3074/MB3076 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049970-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

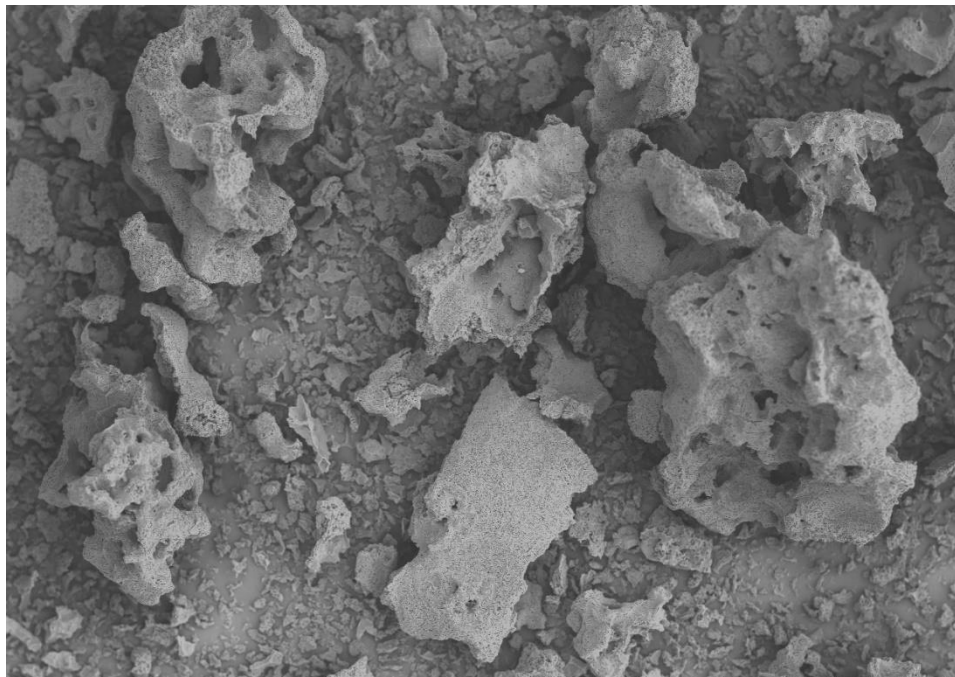

Clariant SU7000 5.00kV 4.2mm x100 UD+LD+MD 05/12/2025 500µm

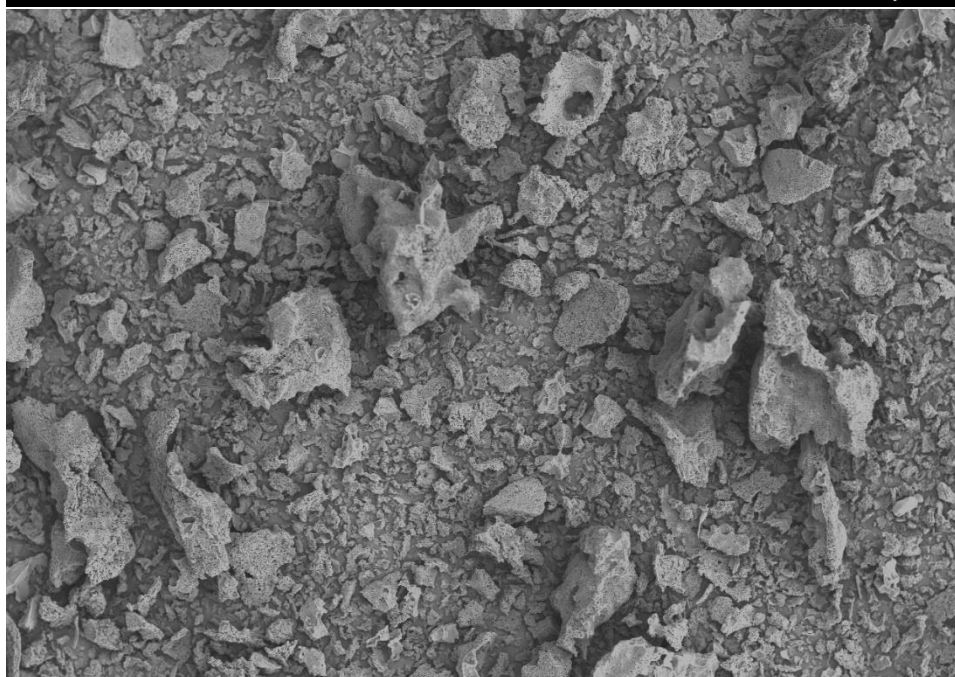


Clariant SU7000 5.00kV 4.3mm x100 UD+LD+MD 05/12/2025 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3074/MB3076 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049970-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

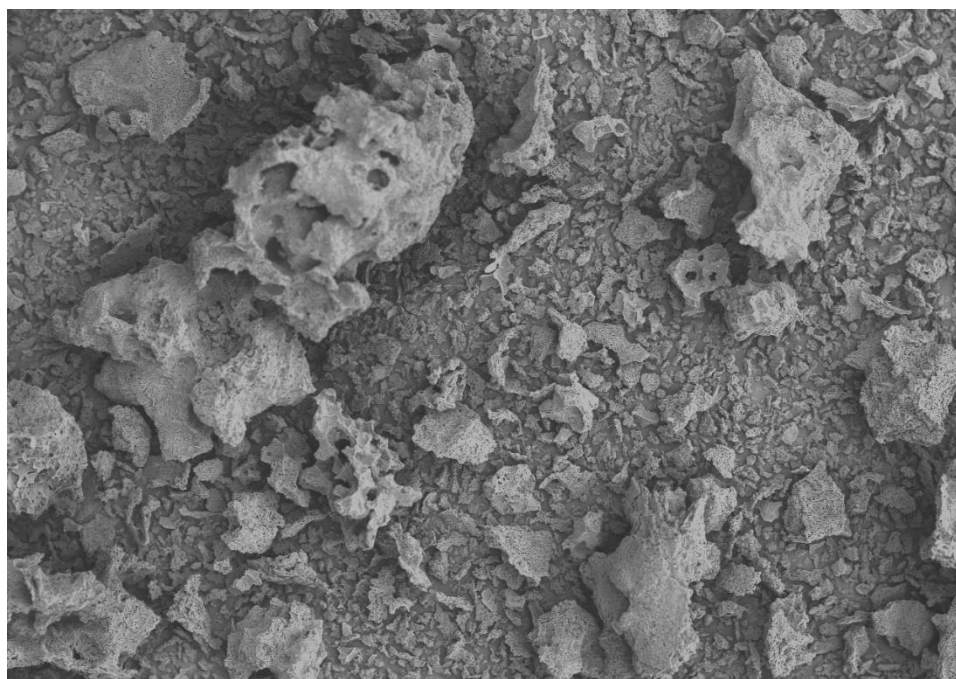

Clariant SU7000 5.00kV 4.3mm x100 UD+LD+MD 05/12/2025 500µm

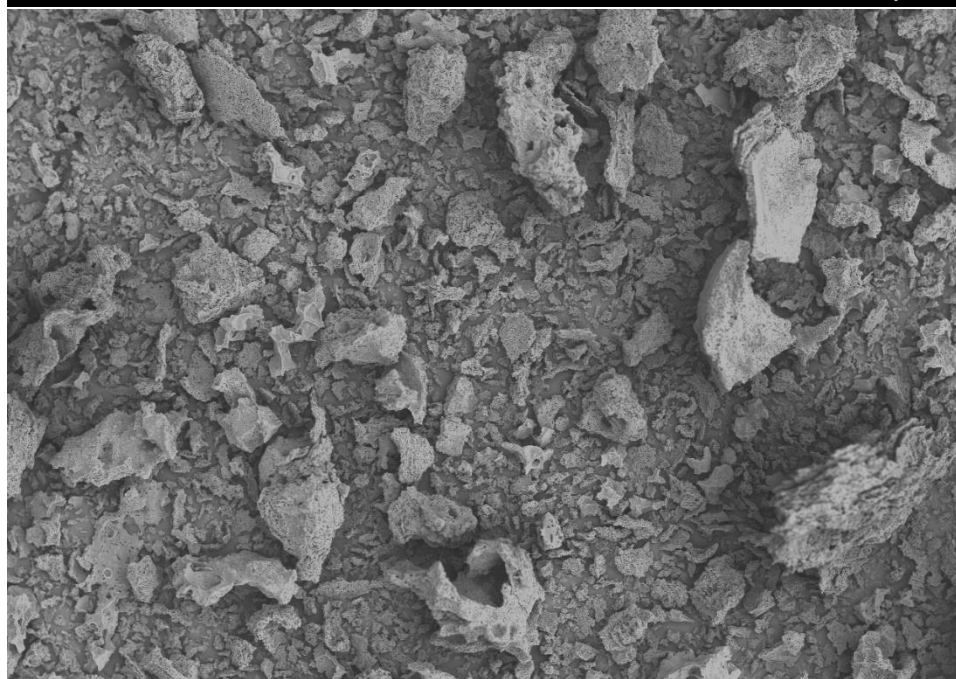


Clariant SU7000 5.00kV 4.4mm x100 UD+LD+MD 05/12/2025 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3074/MB3076 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049970-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

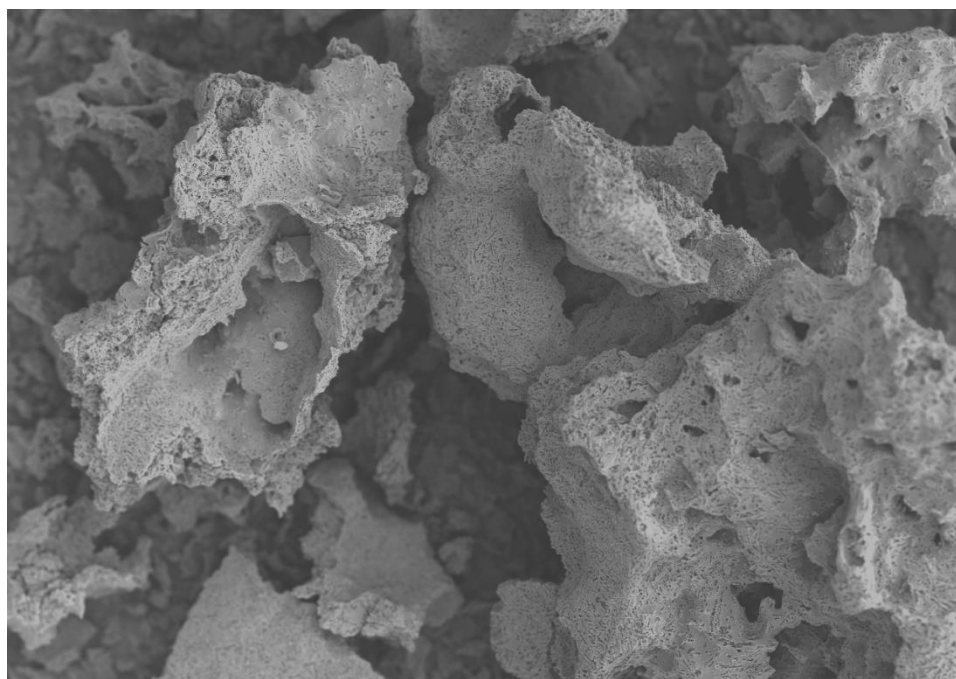

Clariant SU7000 5.00kV 4.1mm x200 UD+LD+MD 05/12/2025 200µm

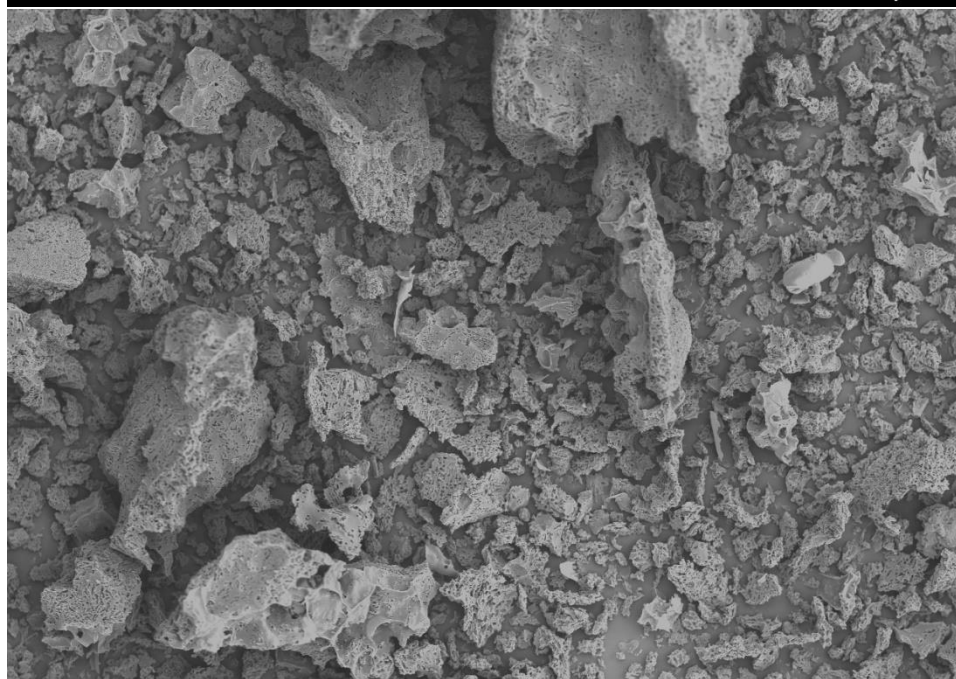


Clariant SU7000 5.00kV 4.3mm x200 UD+LD+MD 05/12/2025 200µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3074/MB3076 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049970-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

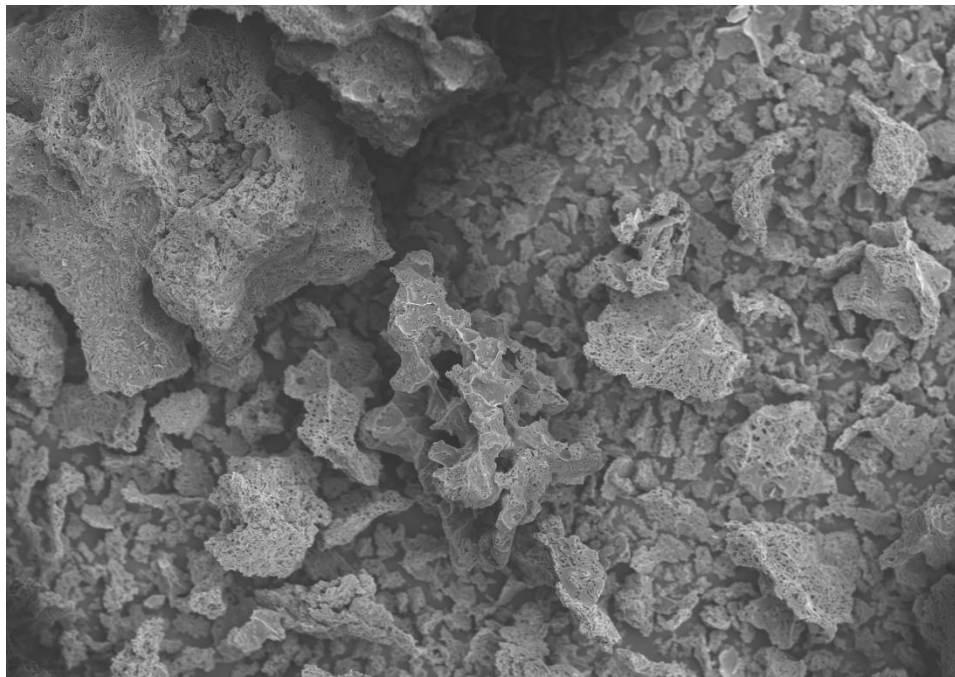

Clariant SU7000 5.00kV 4.2mm x200 UD 05/12/2025 200µm

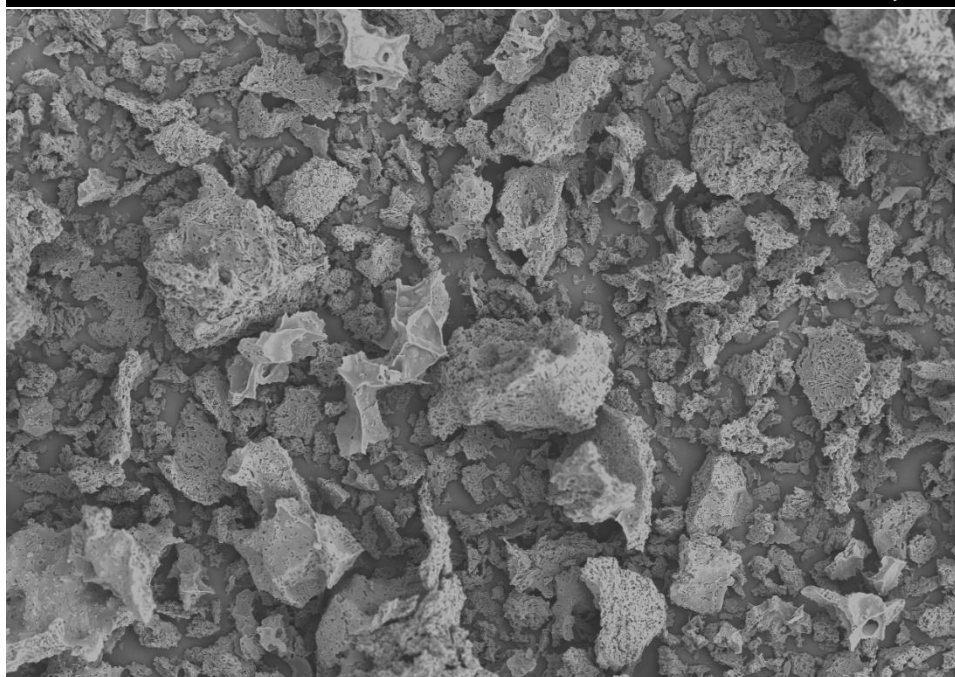


Clariant SU7000 5.00kV 4.4mm x200 UD+LD+MD 05/12/2025 200µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3074/MB3076 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049970-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

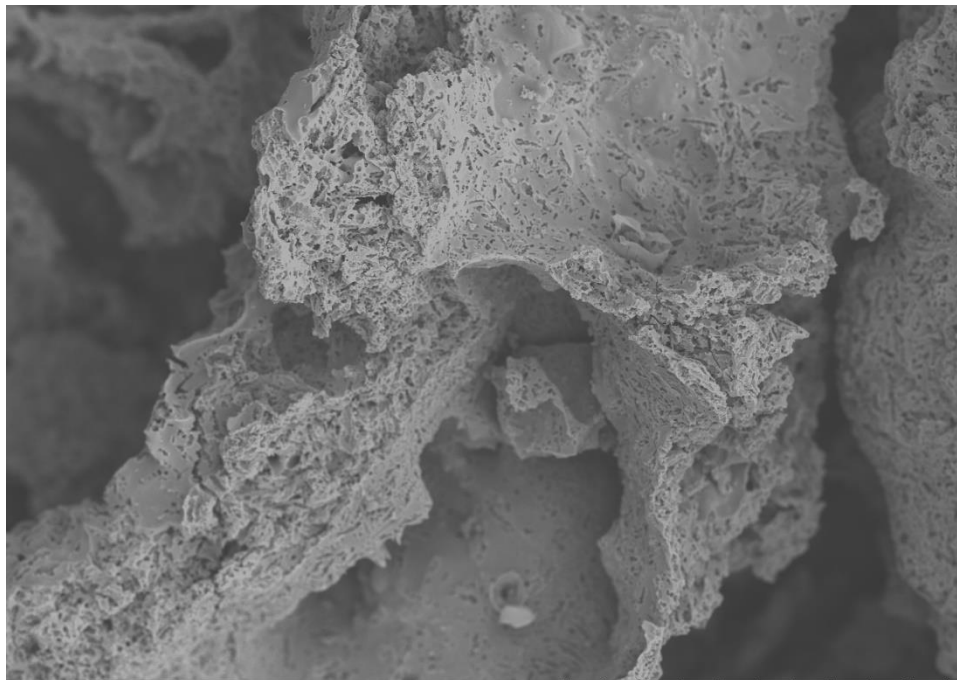

Clariant SU7000 5.00kV 4.0mm x500 UD+LD+MD 05/12/2025 100µm

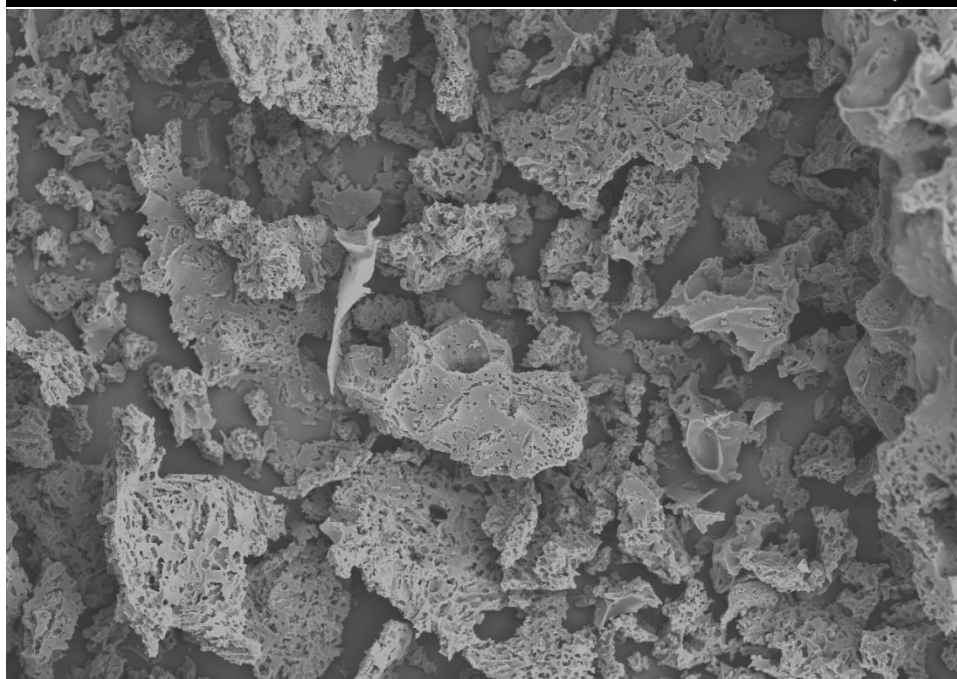


Clariant SU7000 5.00kV 4.3mm x500 UD+LD+MD 05/12/2025 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3074/MB3076 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049970-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

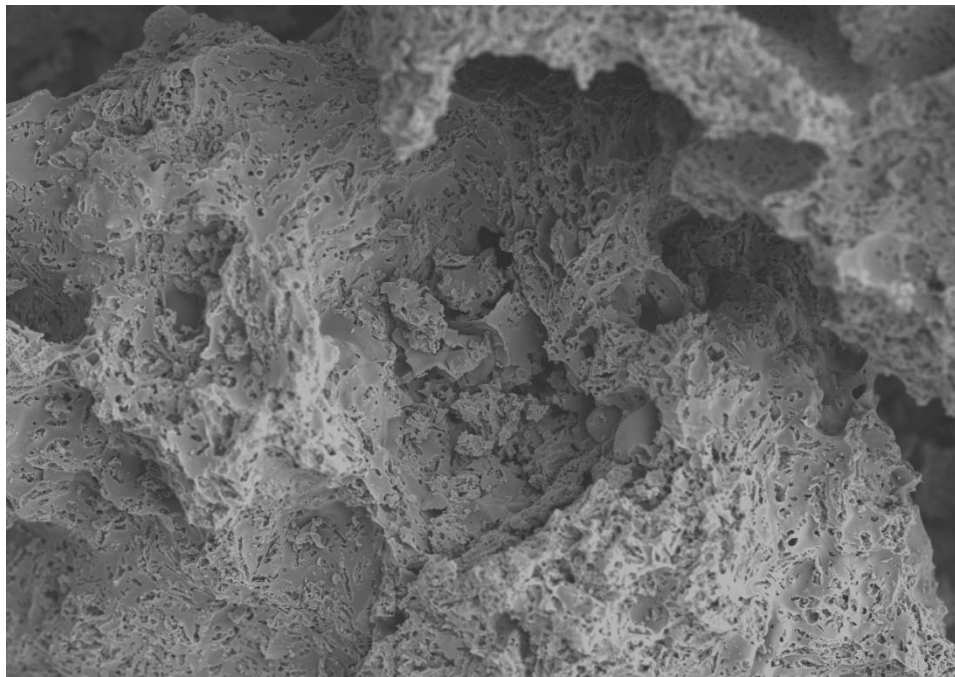

Clariant SU7000 5.00kV 4.2mm x500 UD+LD+MD 05/12/2025 100µm

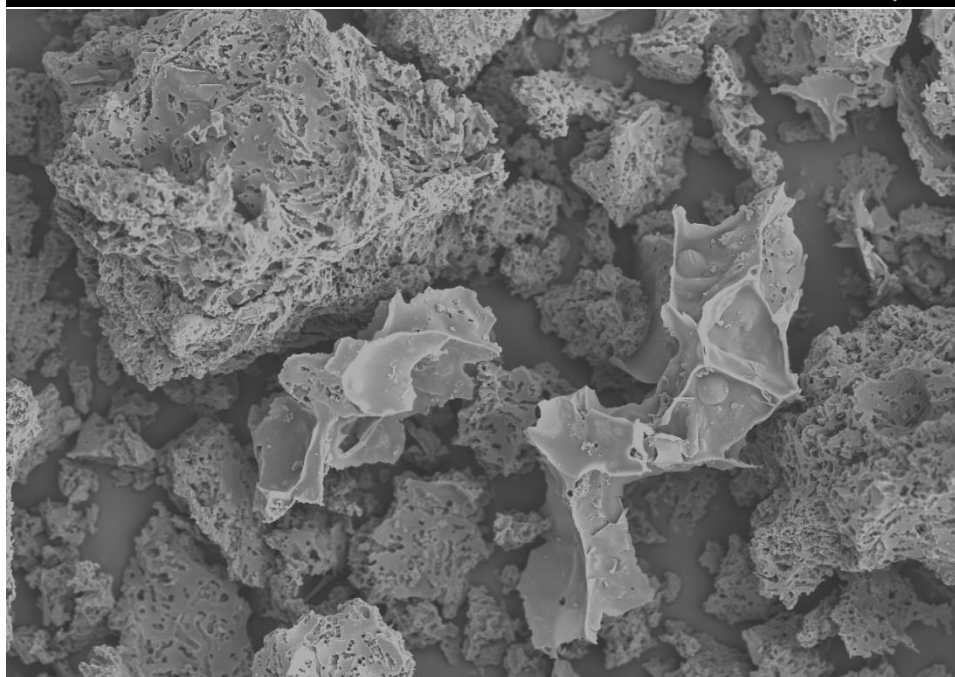


Clariant SU7000 5.00kV 4.3mm x500 UD+LD+MD 05/12/2025 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3074/MB3076 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049970-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

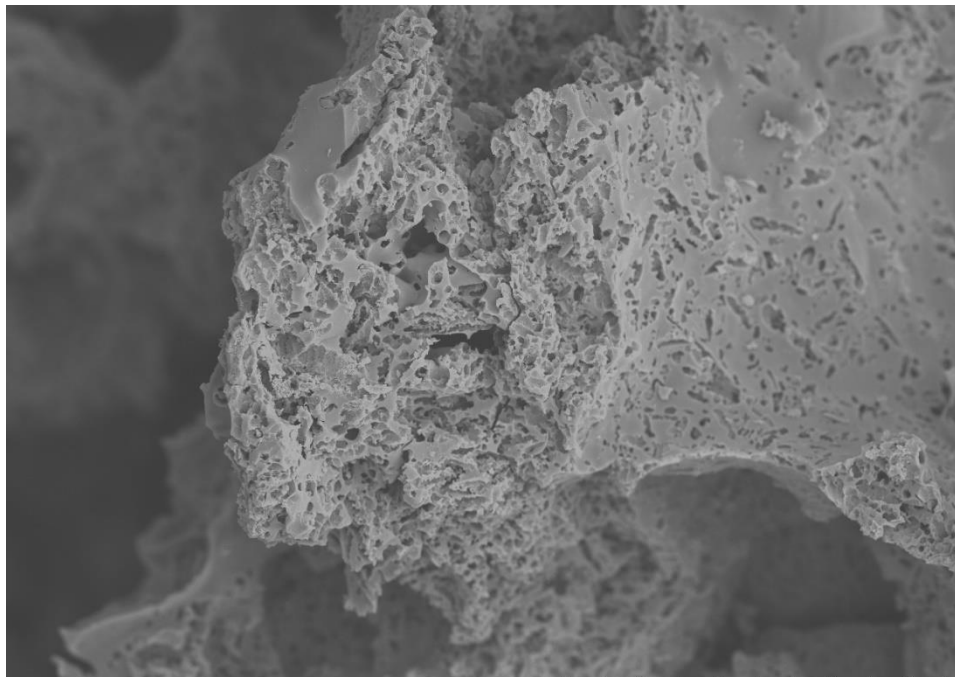

Clariant SU7000 5.00kV 4.0mm x1.00k UD+LD+MD 05/12/2025 50.0µm

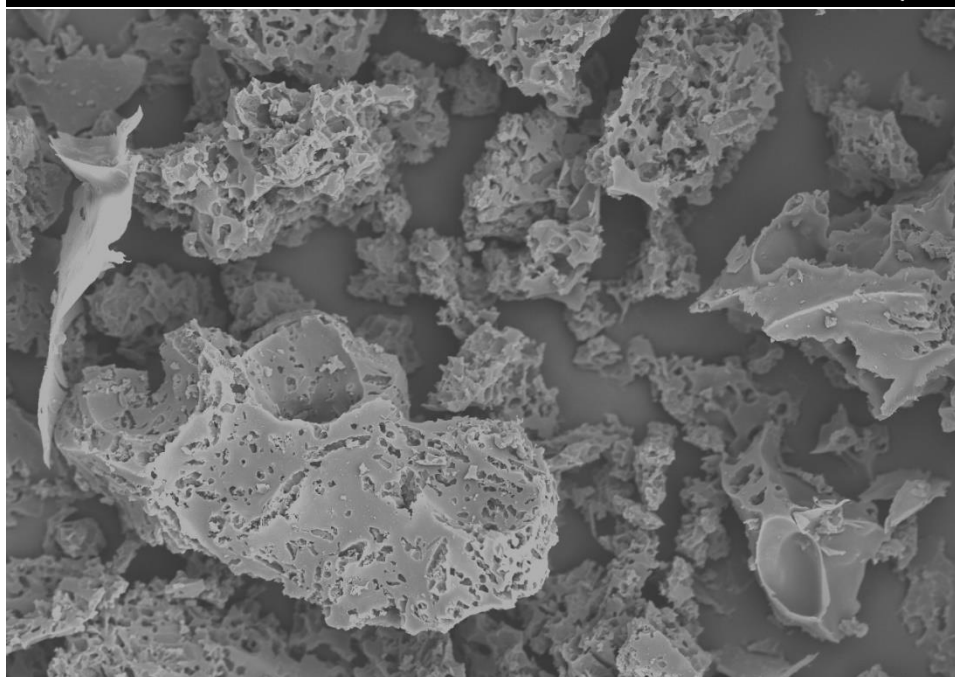


Clariant SU7000 5.00kV 4.3mm x1.00k UD+LD+MD 05/12/2025 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3074/MB3076 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049970-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

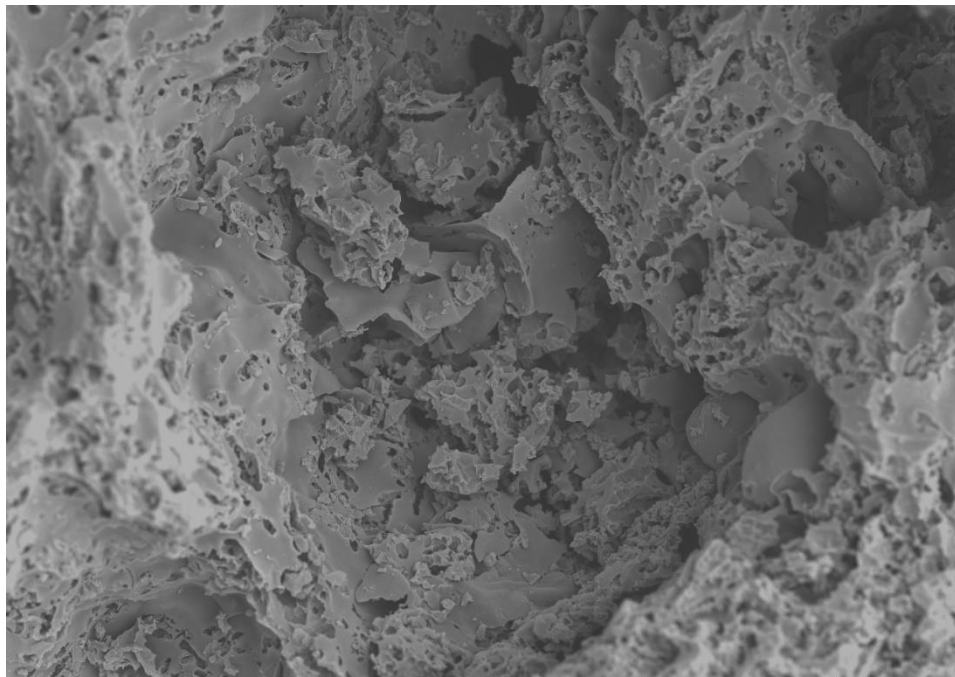

Clariant SU7000 5.00kV 4.2mm x1.00k UD+LD+MD 05/12/2025 50.0µm

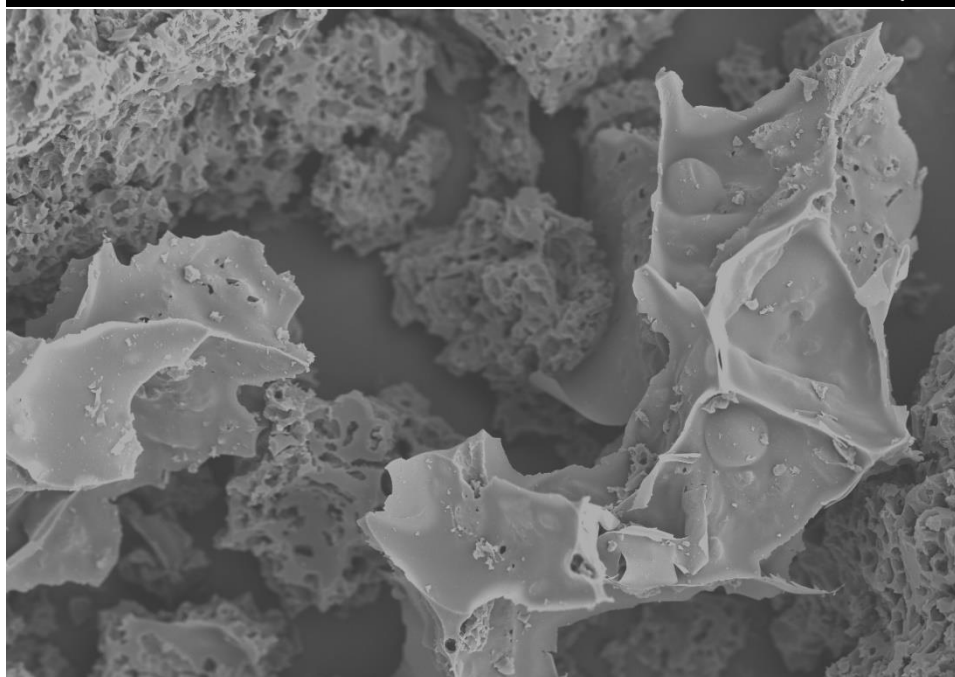


Clariant SU7000 5.00kV 4.3mm x1.00k UD+LD+MD 05/12/2025 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3074/MB3076 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049970-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

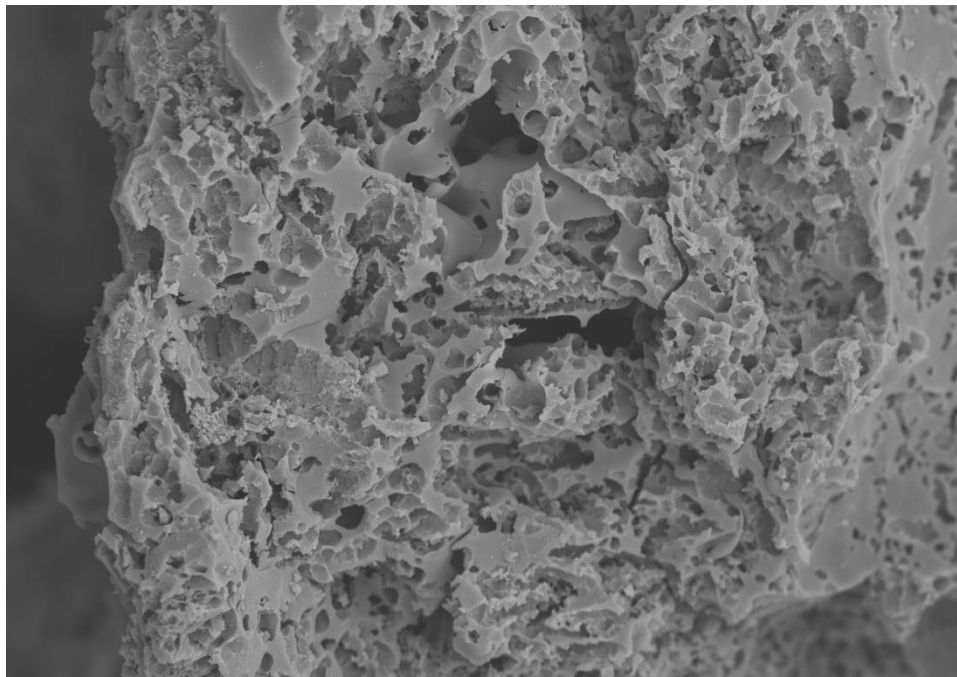

Clariant SU7000 5.00kV 4.0mm x2.00k UD+LD+MD 05/12/2025 20.0µm

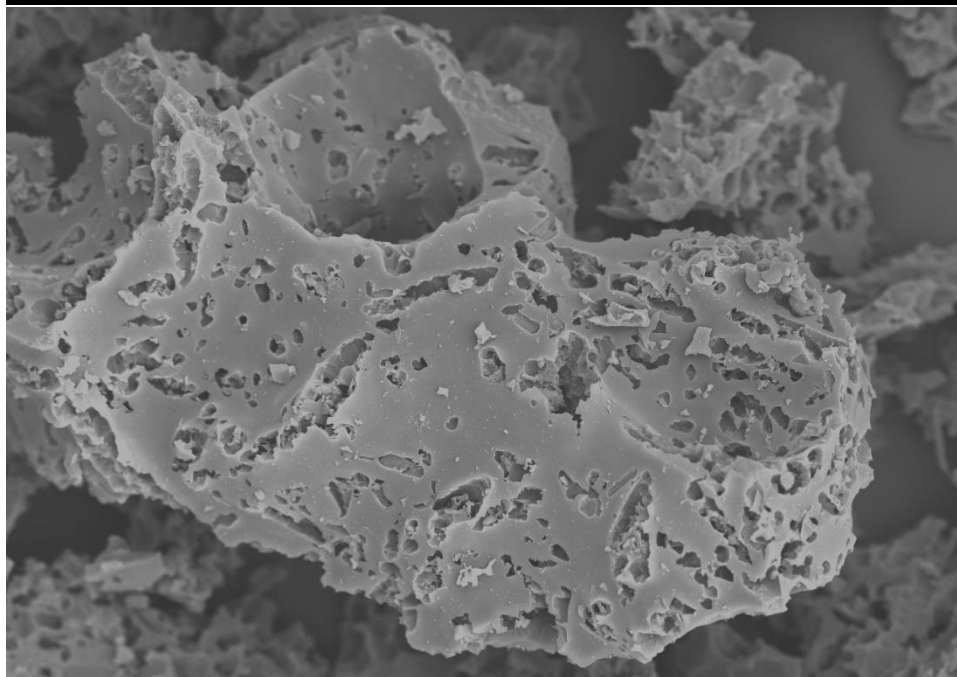


Clariant SU7000 5.00kV 4.3mm x2.00k UD+LD+MD 05/12/2025 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3074/MB3076 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049970-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

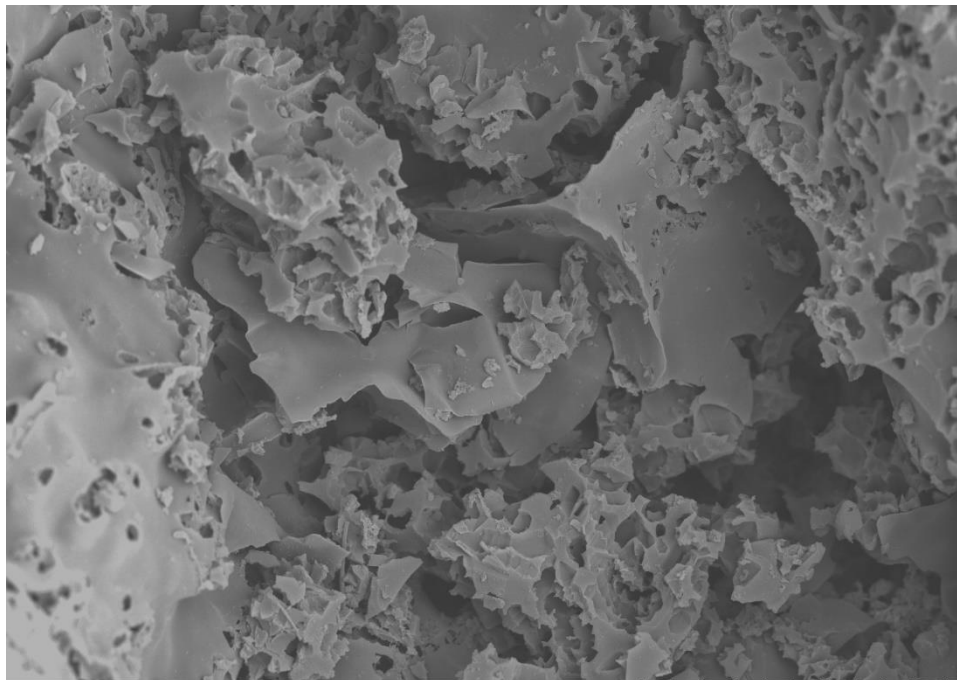

Clariant SU7000 5.00kV 4.2mm x2.00k UD+LD+MD 05/12/2025 20.0μm

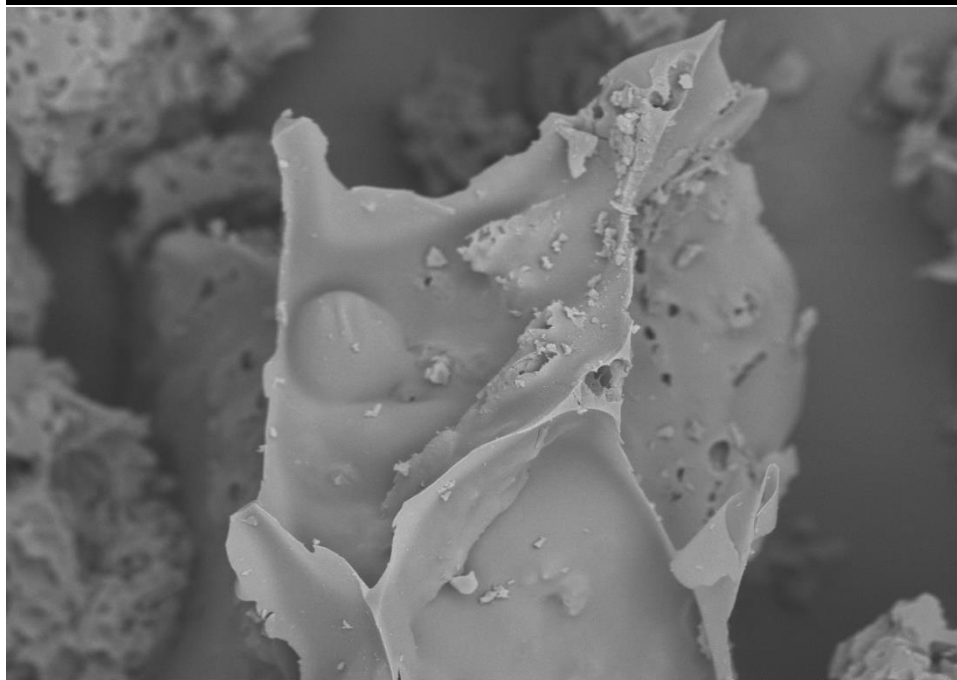


Clariant SU7000 5.00kV 4.3mm x2.00k MD 05/12/2025 20.0μm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3074/MB3076 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049970-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

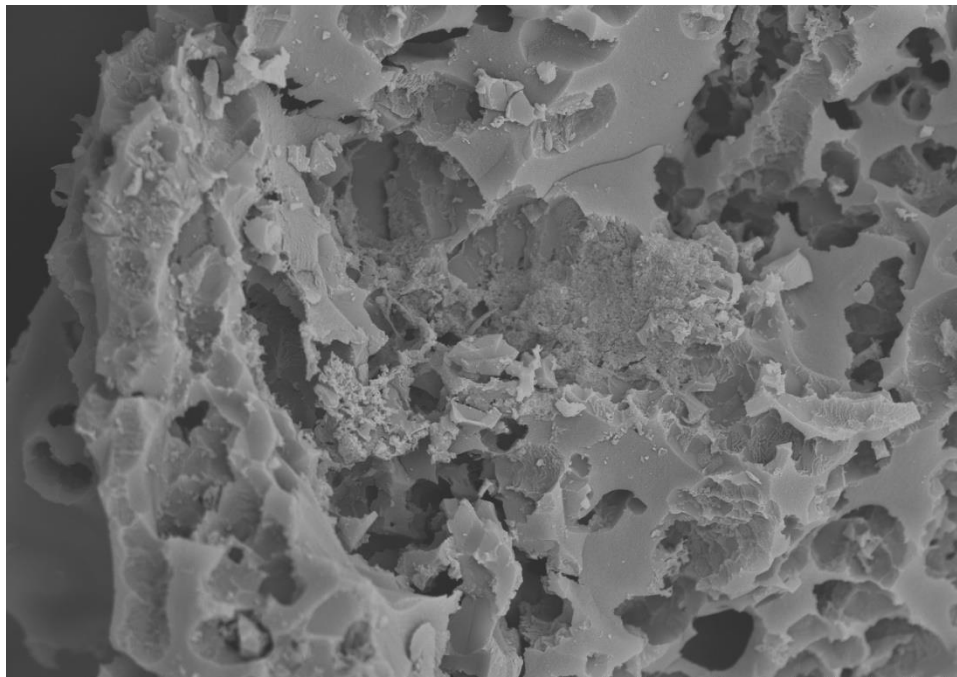

Clariant SU7000 5.00kV 4.0mm x5.00k UD+LD+MD 05/12/2025 10.0µm

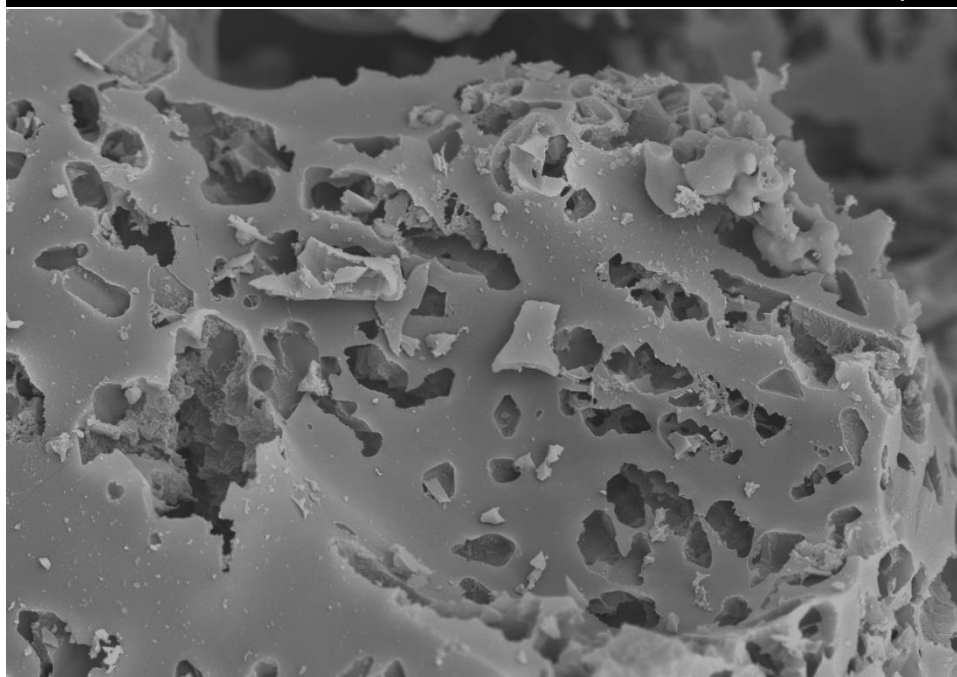

Clariant SU7000 5.00kV 4.3mm x5.00k UD+LD+MD 05/12/2025 10.0µm

SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3074/MB3076 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-049970-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

