
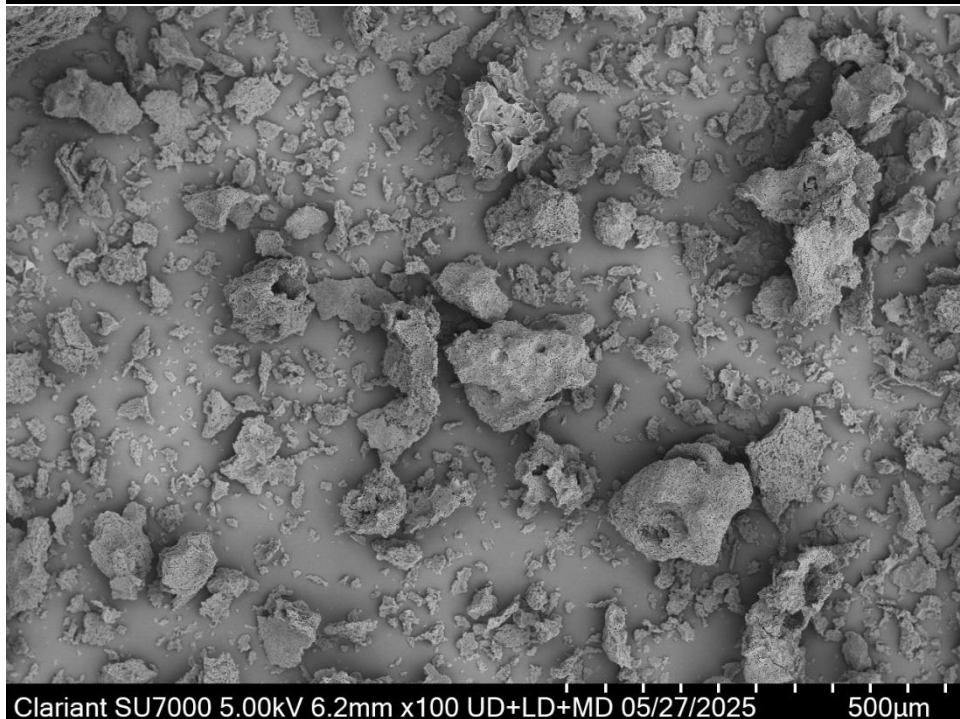


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa430/MRa431/MRa432/MRa433/ 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-050103-1


Sample treatment: The sample was subjected to platinum sputter coating and then measured.

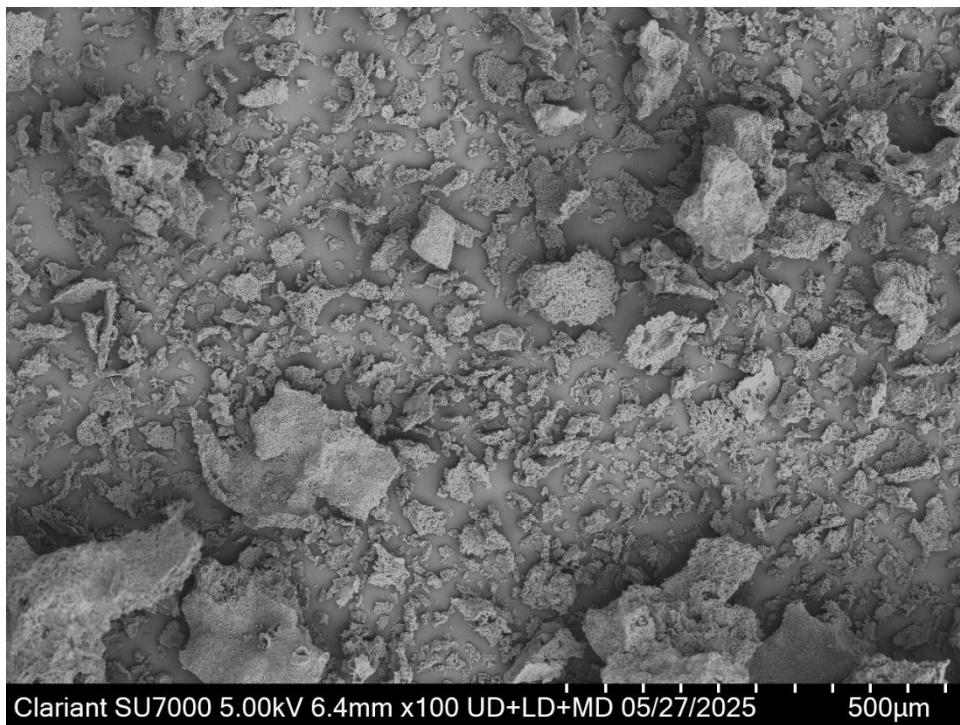

SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa430/MRa431/MRa432/MRa433/ 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-050103-1


Sample treatment: The sample was subjected to platinum sputter coating and then measured.

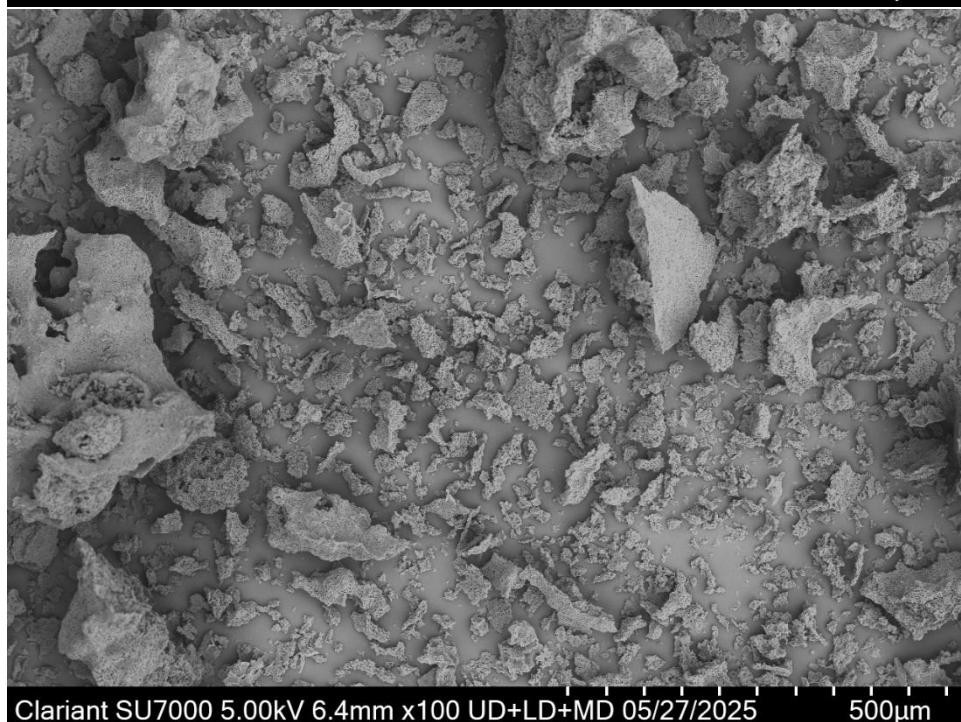


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa430/MRa431/MRa432/MRa433/ 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-050103-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

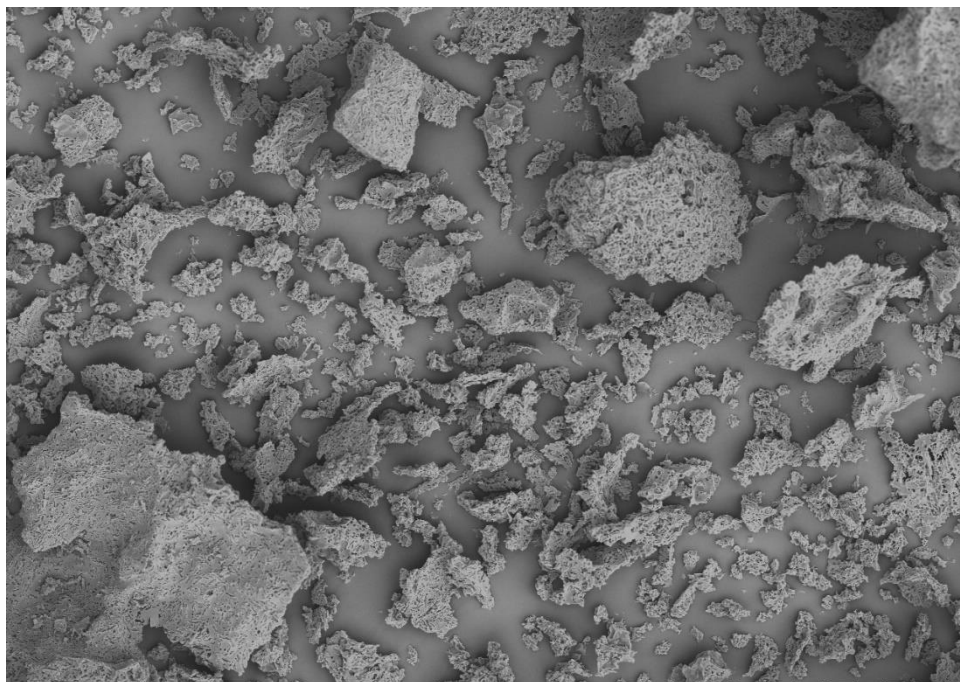

Clariant SU7000 5.00kV 6.4mm x200 UD+LD+MD 05/27/2025 200µm


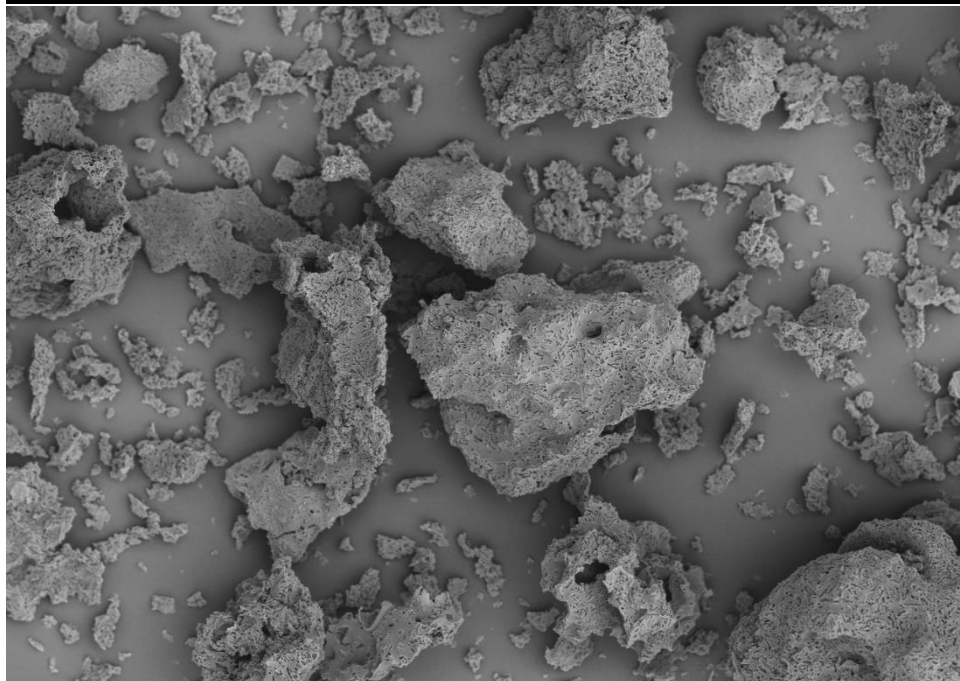


Clariant SU7000 5.00kV 6.2mm x200 UD+LD+MD 05/27/2025 200µm

SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa430/MRa431/MRa432/MRa433/ 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-050103-1


Sample treatment: The sample was subjected to platinum sputter coating and then measured.

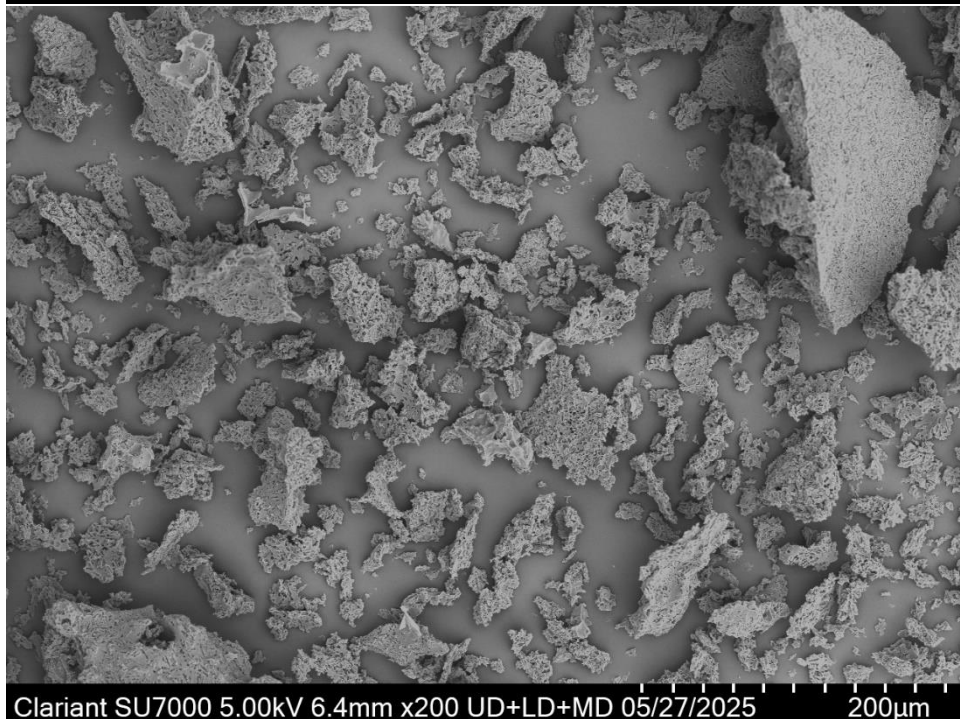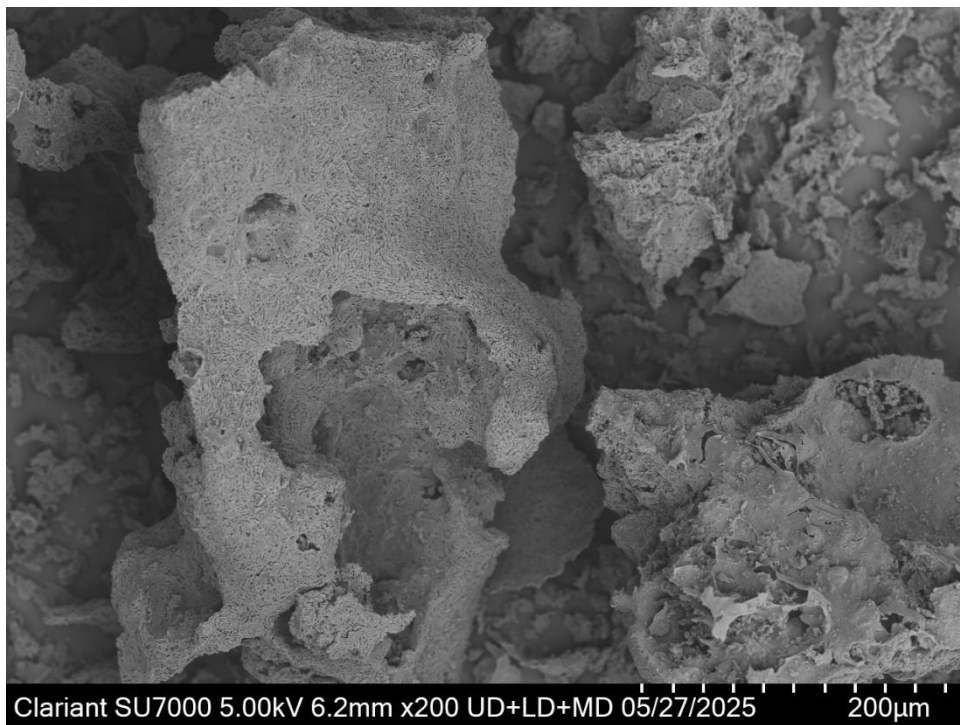


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa430/MRa431/MRa432/MRa433/ 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-050103-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

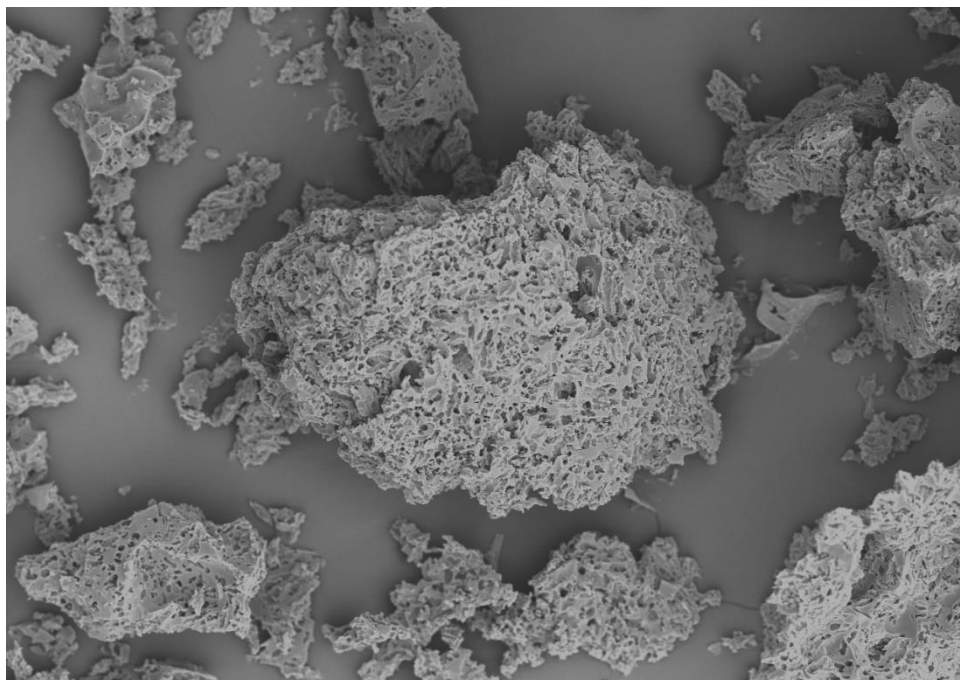

Clariant SU7000 5.00kV 6.3mm x500 UD+LD+MD 05/27/2025 100µm


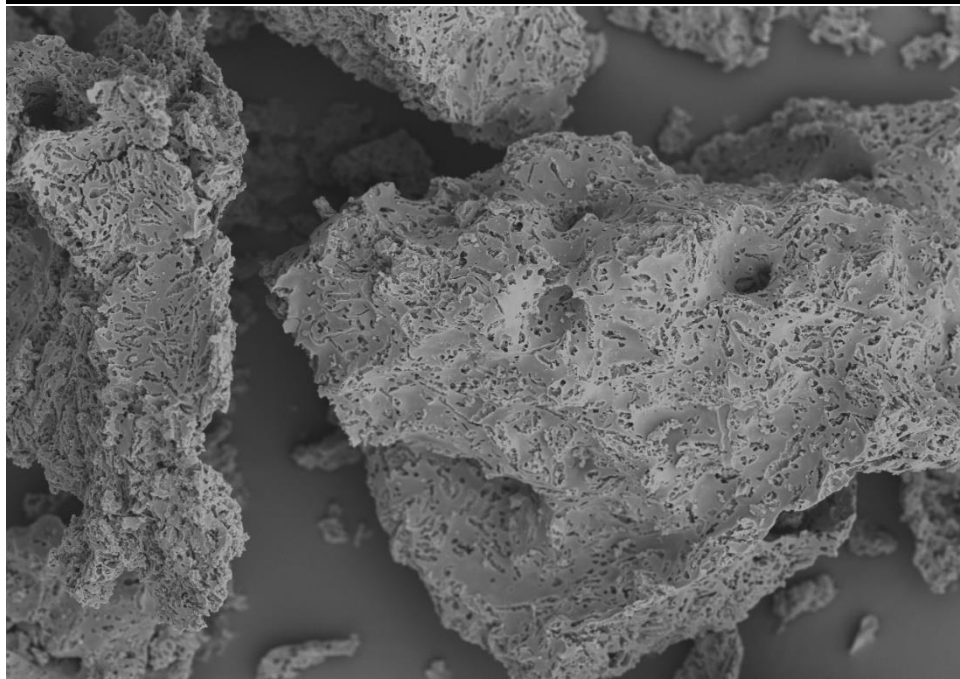


Clariant SU7000 5.00kV 6.2mm x500 UD+LD+MD 05/27/2025 100µm

SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa430/MRa431/MRa432/MRa433/ 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-050103-1


Sample treatment: The sample was subjected to platinum sputter coating and then measured.

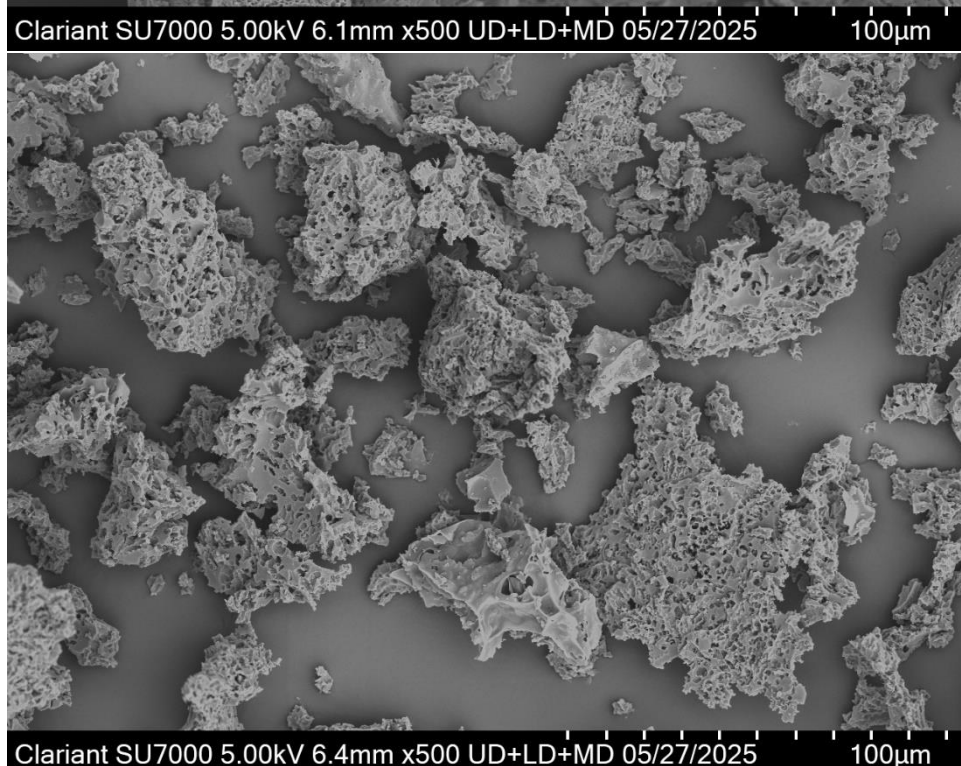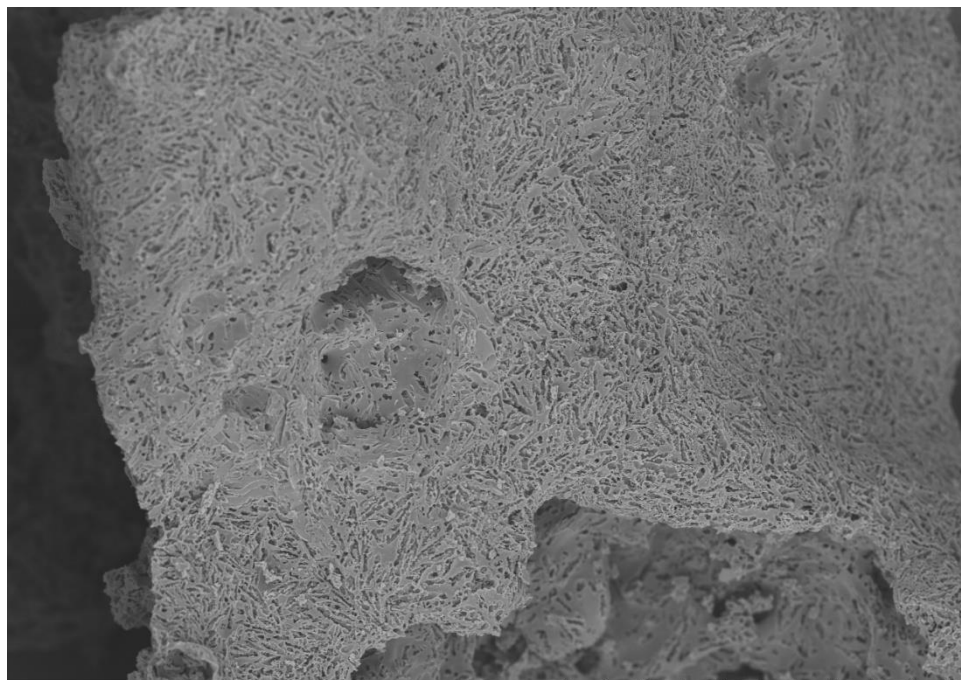


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa430/MRa431/MRa432/MRa433/ 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-050103-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

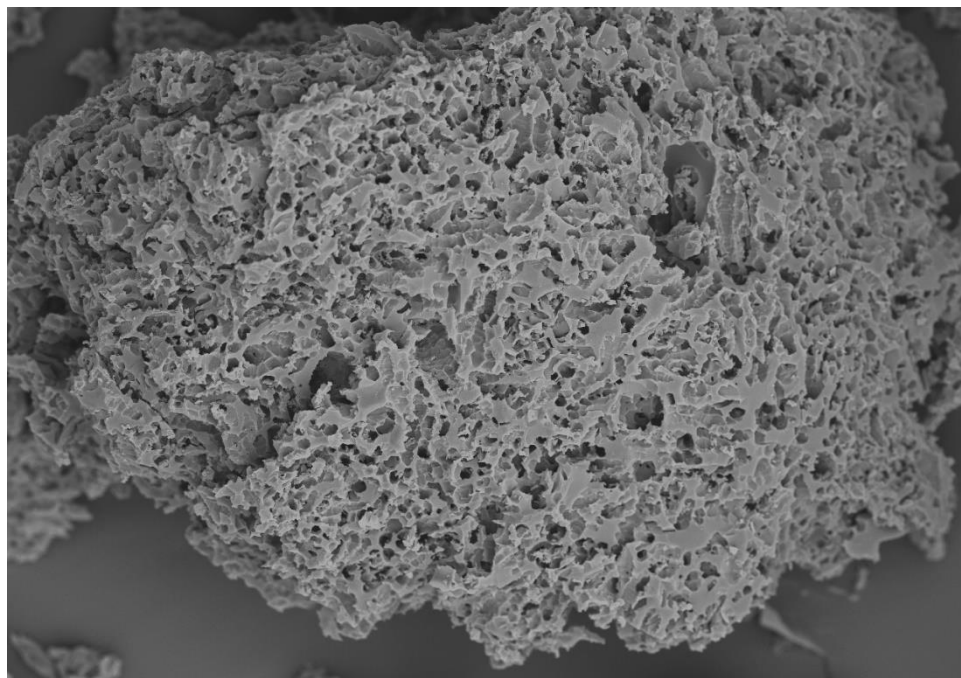

Clariant SU7000 5.00kV 6.3mm x1.00k UD+LD+MD 05/27/2025 50.0µm

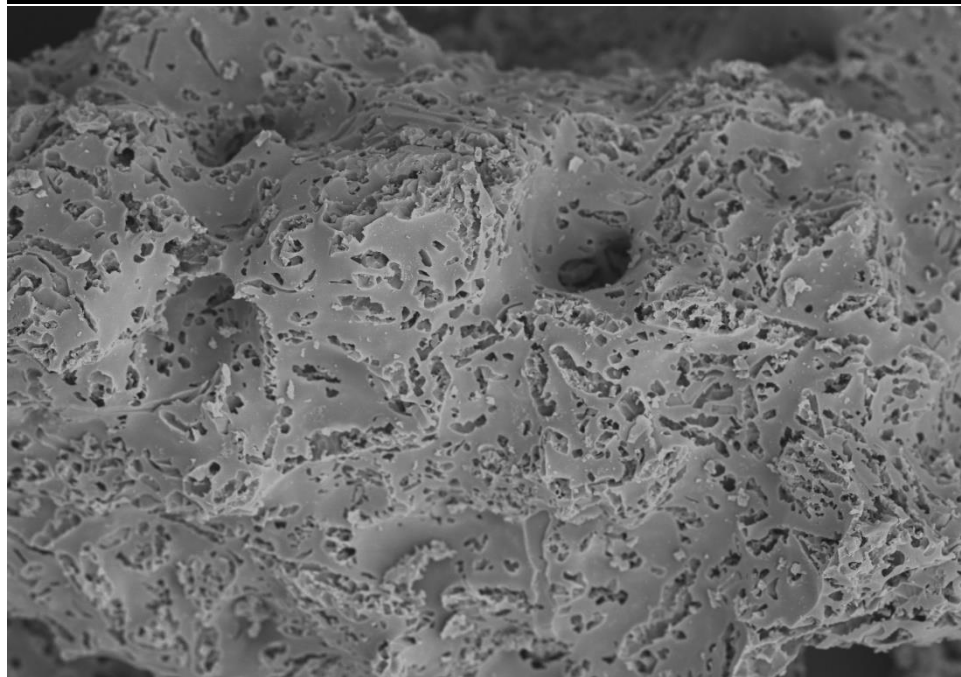


Clariant SU7000 5.00kV 6.2mm x1.00k UD+LD+MD 05/27/2025 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa430/MRa431/MRa432/MRa433/ 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-050103-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

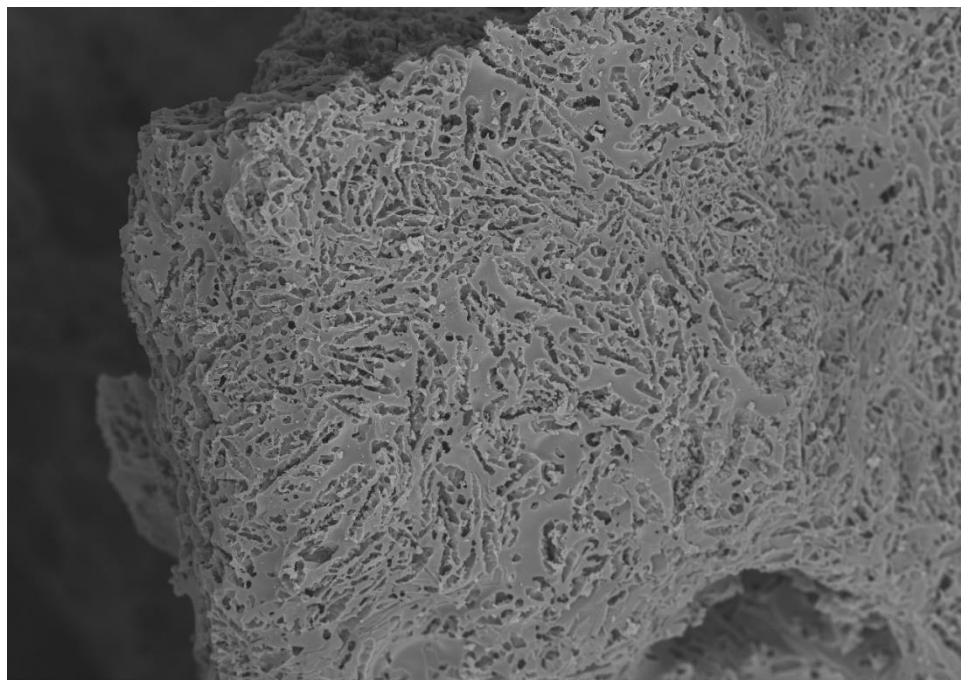

Clariant SU7000 5.00kV 6.0mm x1.00k UD+LD+MD 05/27/2025 50.0µm


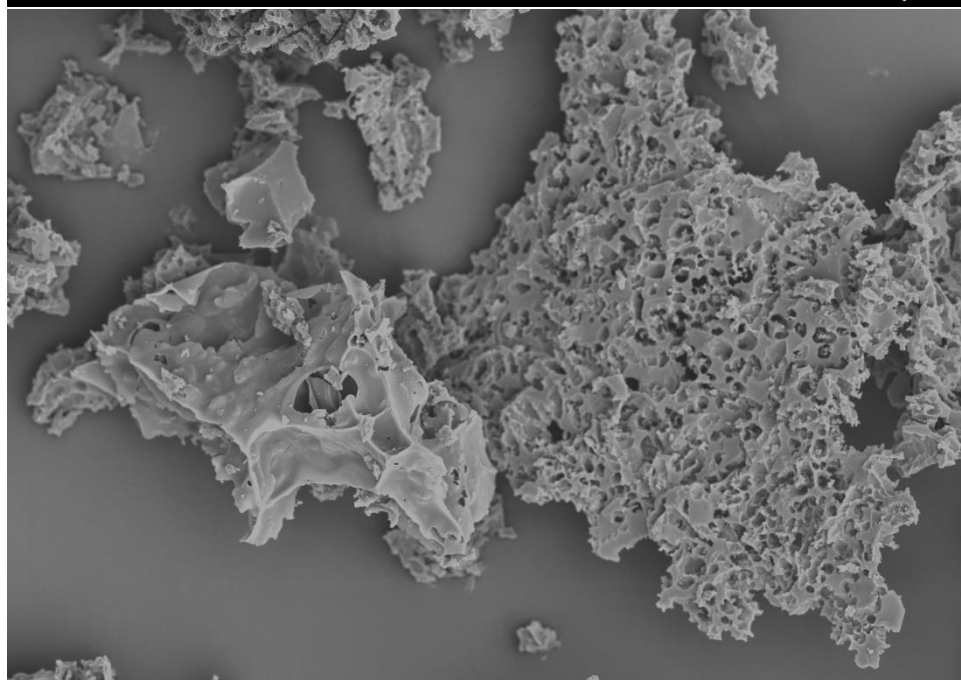


Clariant SU7000 5.00kV 6.3mm x1.00k UD+LD+MD 05/27/2025 50.0µm

SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa430/MRa431/MRa432/MRa433/ 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-050103-1



Sample treatment: The sample was subjected to platinum sputter coating and then measured.

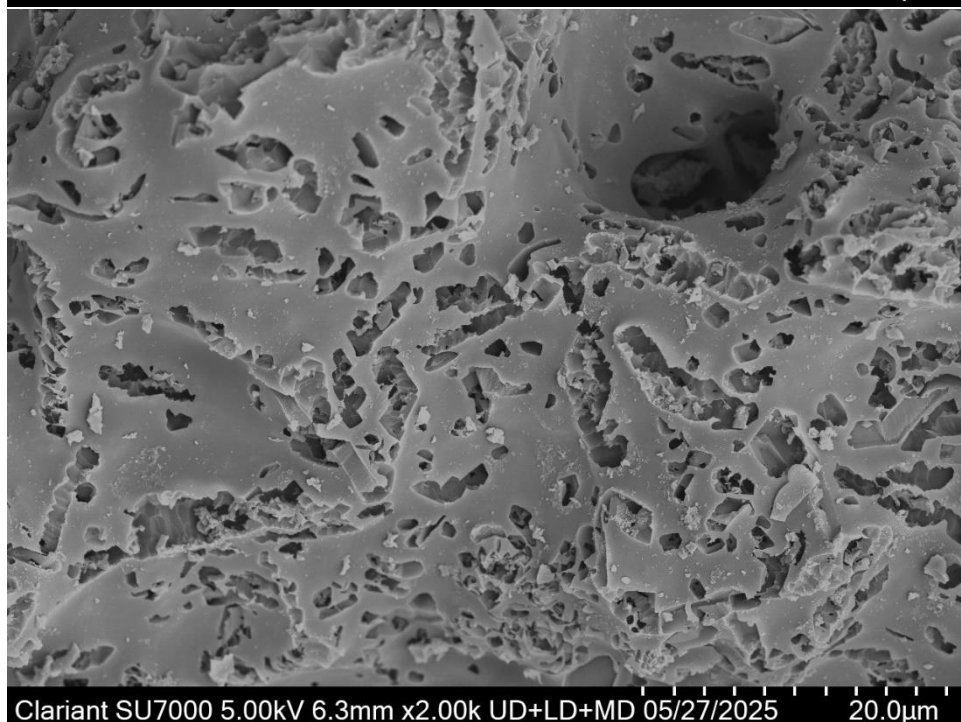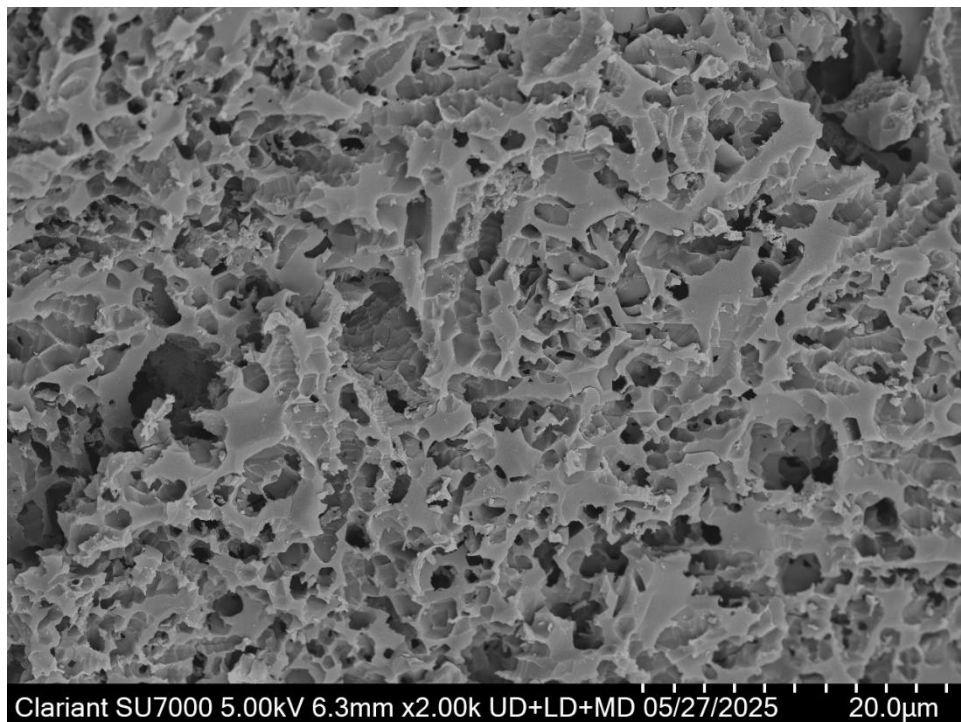

SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa430/MRa431/MRa432/MRa433/ 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-050103-1


Sample treatment: The sample was subjected to platinum sputter coating and then measured.

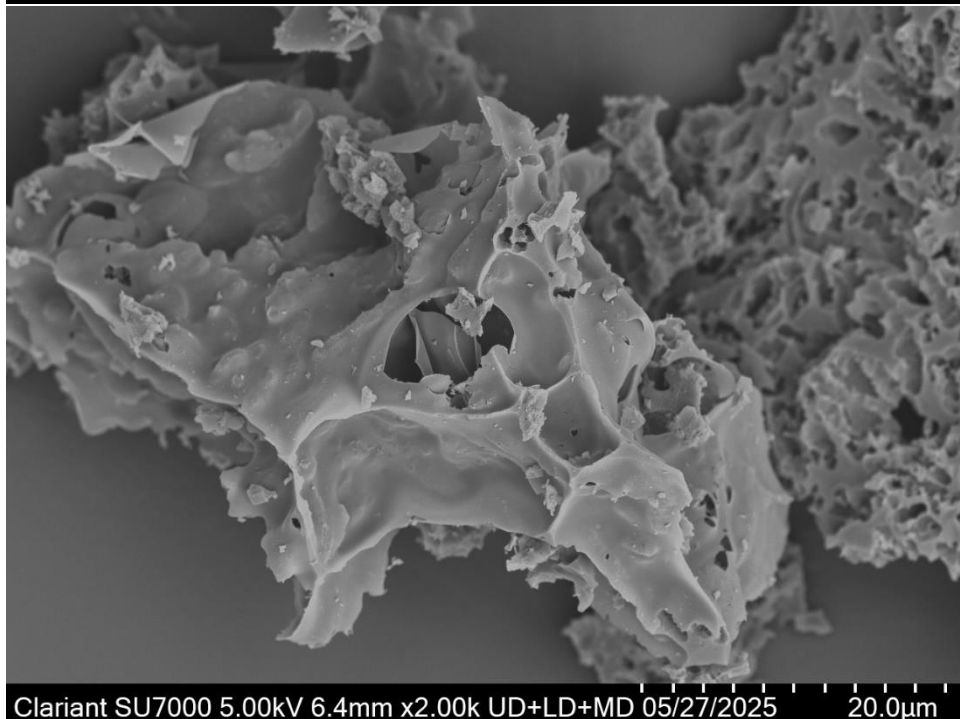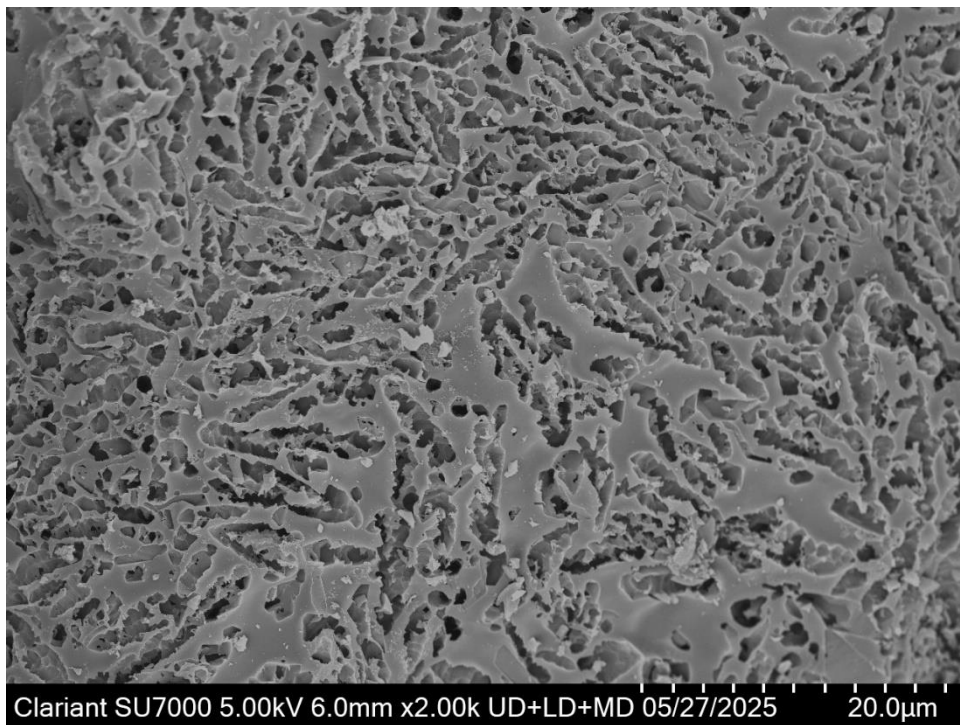


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa430/MRa431/MRa432/MRa433/ 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-050103-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

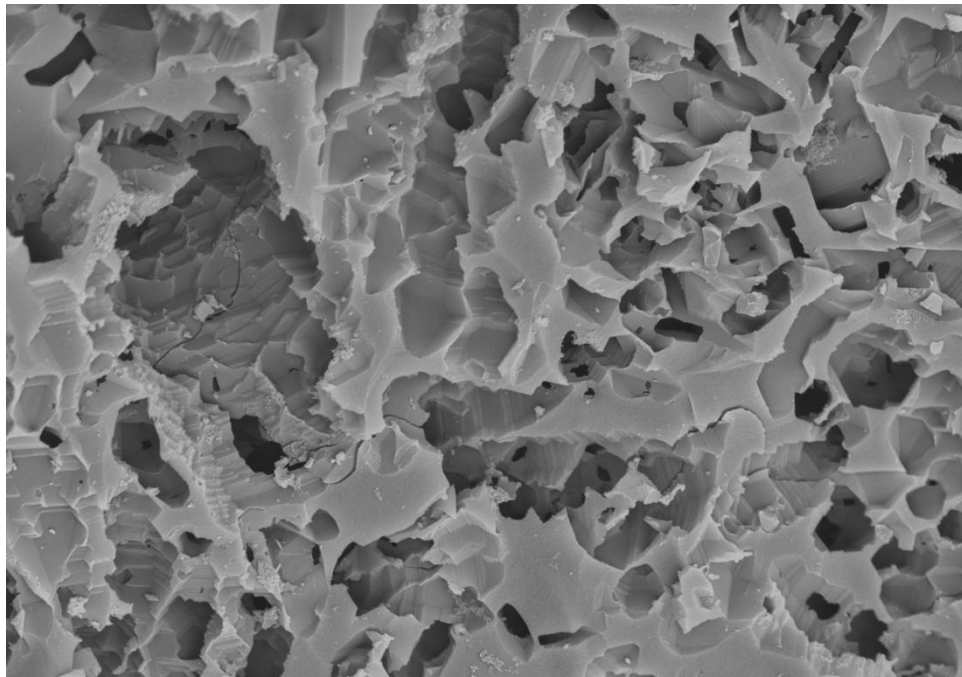

Clariant SU7000 5.00kV 6.3mm x5.00k UD+LD+MD 05/27/2025 10.0µm

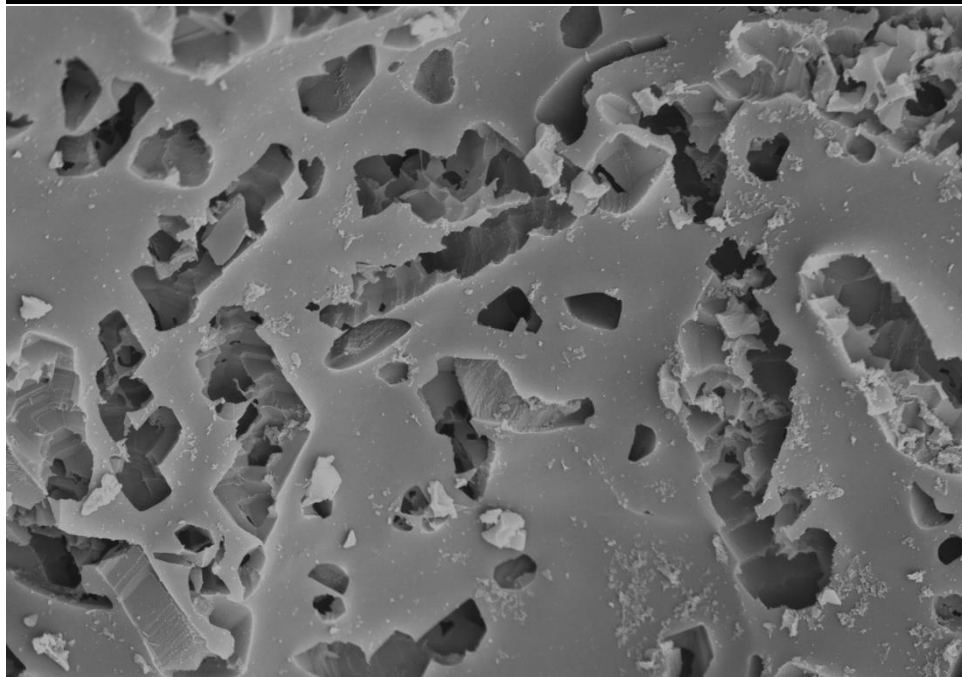


Clariant SU7000 5.00kV 6.3mm x5.00k UD+LD+MD 05/27/2025 10.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MRa430/MRa431/MRa432/MRa433/ 2/3 3x30sec 800C 3C/m 1h Rot
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-050103-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

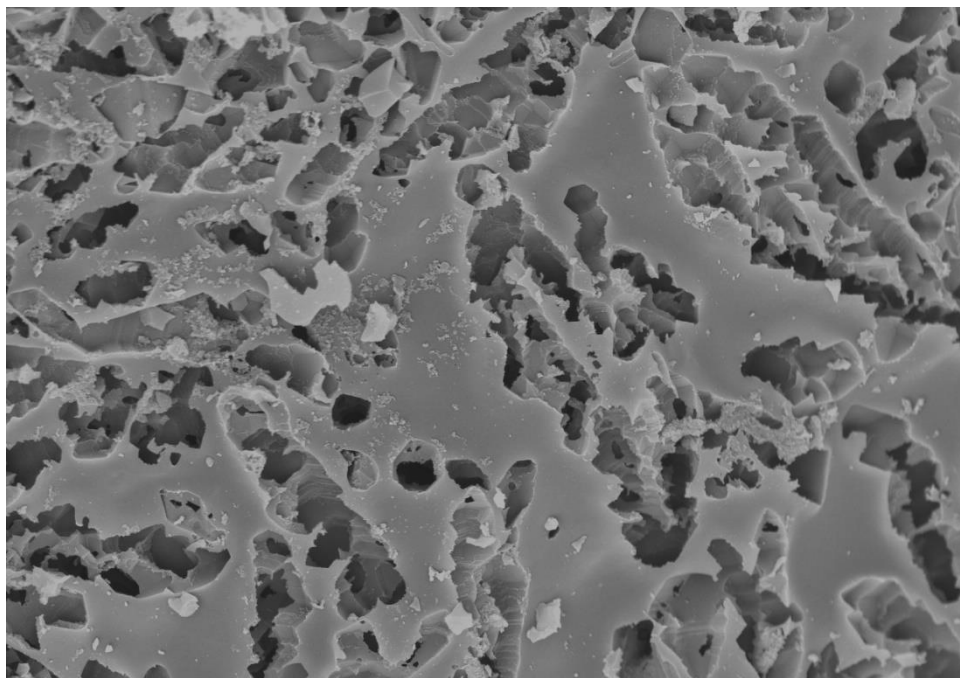

Clariant SU7000 5.00kV 6.0mm x5.00k UD+LD+MD 05/27/2025 10.0µm

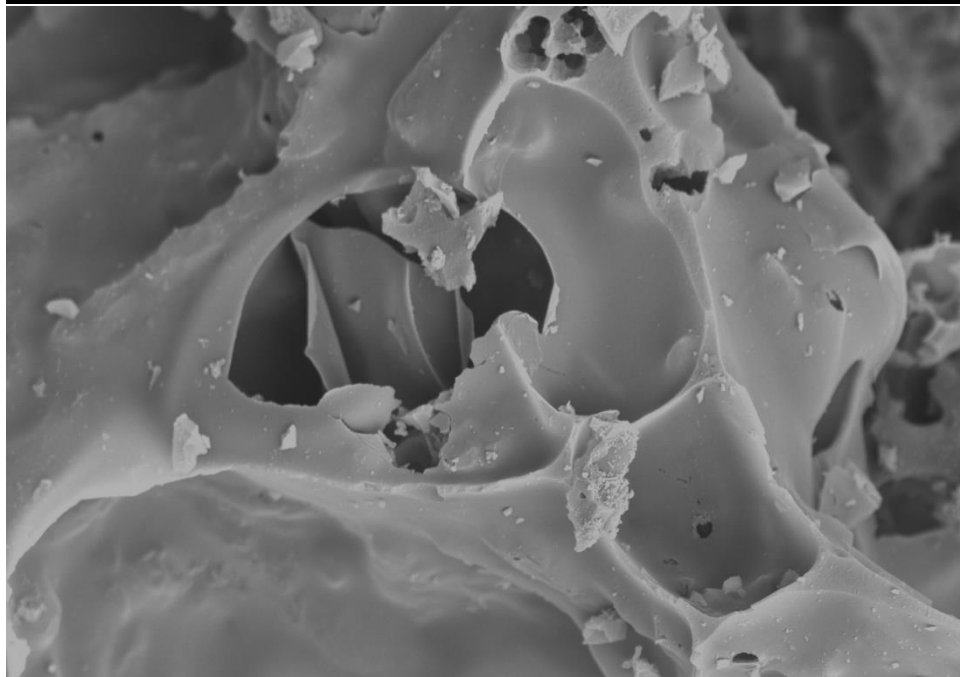

Clariant SU7000 5.00kV 6.4mm x5.00k UD+LD+MD 05/27/2025 10.0µm