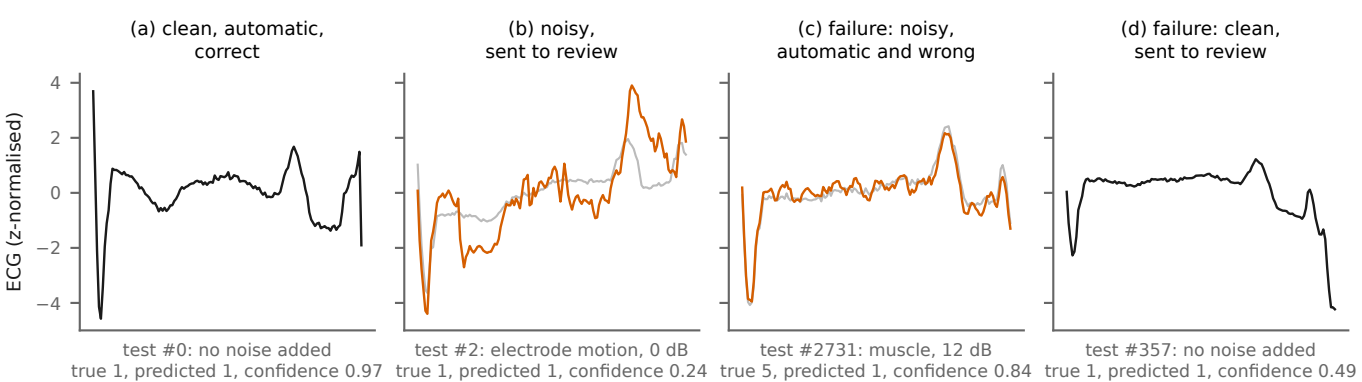
(a) clean, automatic, correct
(b) noisy, sent to review
(c) failure: noisy, automatic and wrong
(d) failure: clean, sent to review
ECG (z-normalised)
4
2
0
−2
−4
test #0: no noise added
true 1, predicted 1, confidence 0.97
test #2: electrode motion, 0 dB
true 1, predicted 1, confidence 0.24
test #2731: muscle, 12 dB
true 5, predicted 1, confidence 0.84
test #357: no noise added
true 1, predicted 1, confidence 0.49