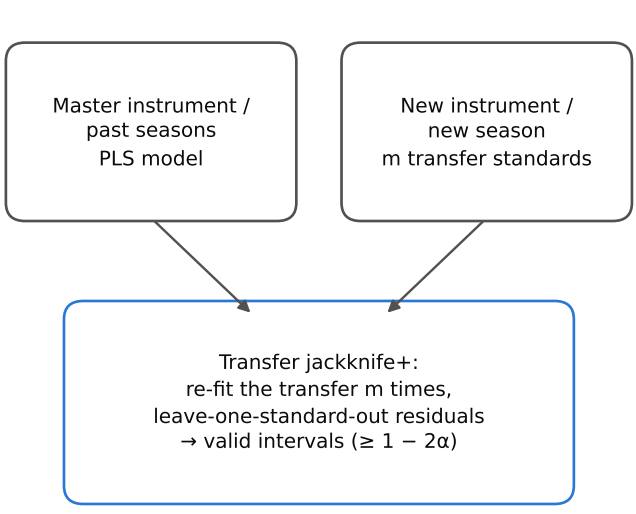
Master instrument /
past seasons
PLS model
New instrument /
new season
m transfer standards
Transfer jackknife+:
re-fit the transfer m times,
leave-one-standard-out residuals
→ valid intervals (≥ 1 − 2α)

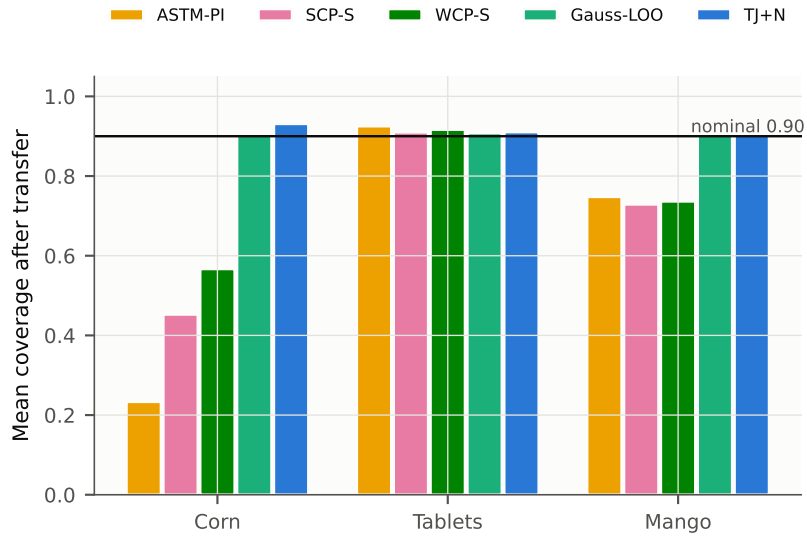
ASTM-PI
SCP-S
WCP-S
Gauss-LOO
TJ+N
Mean coverage after transfer
1.0
0.8
0.6
0.4
0.2
0.0
nominal 0.90
Corn
Tablets
Mango