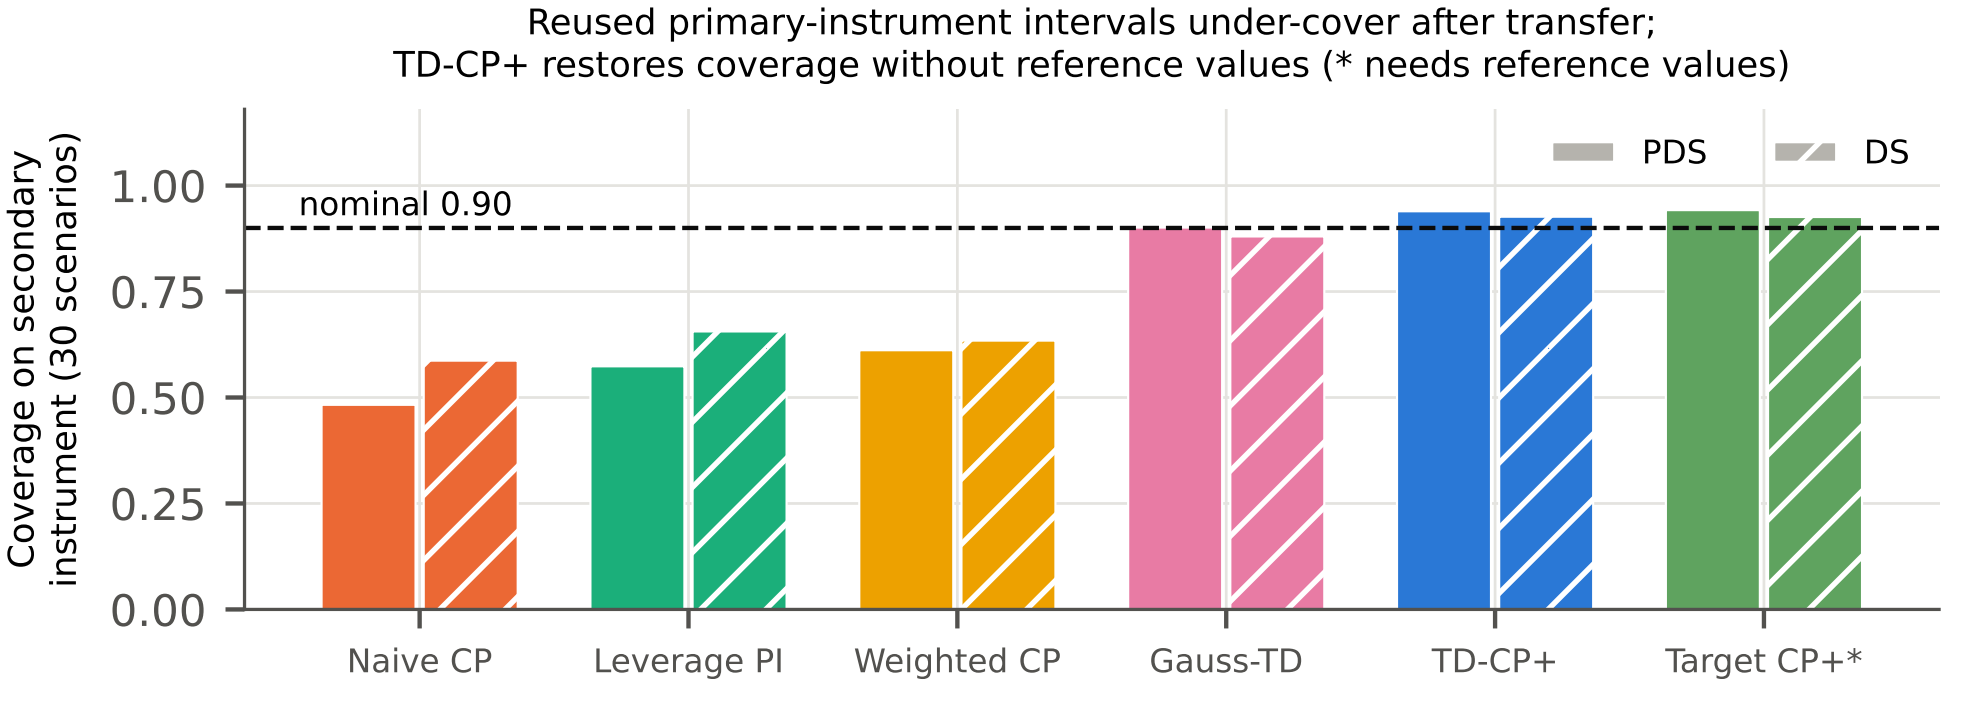
Reused primary-instrument intervals under-cover after transfer;
TD-CP+ restores coverage without reference values (* needs reference values)
Coverage on secondary instrument (30 scenarios)
1.00
0.75
0.50
0.25
0.00
nominal 0.90
PDS
DS
Naive CP
Leverage PI
Weighted CP
Gauss-TD
TD-CP+
Target CP+*