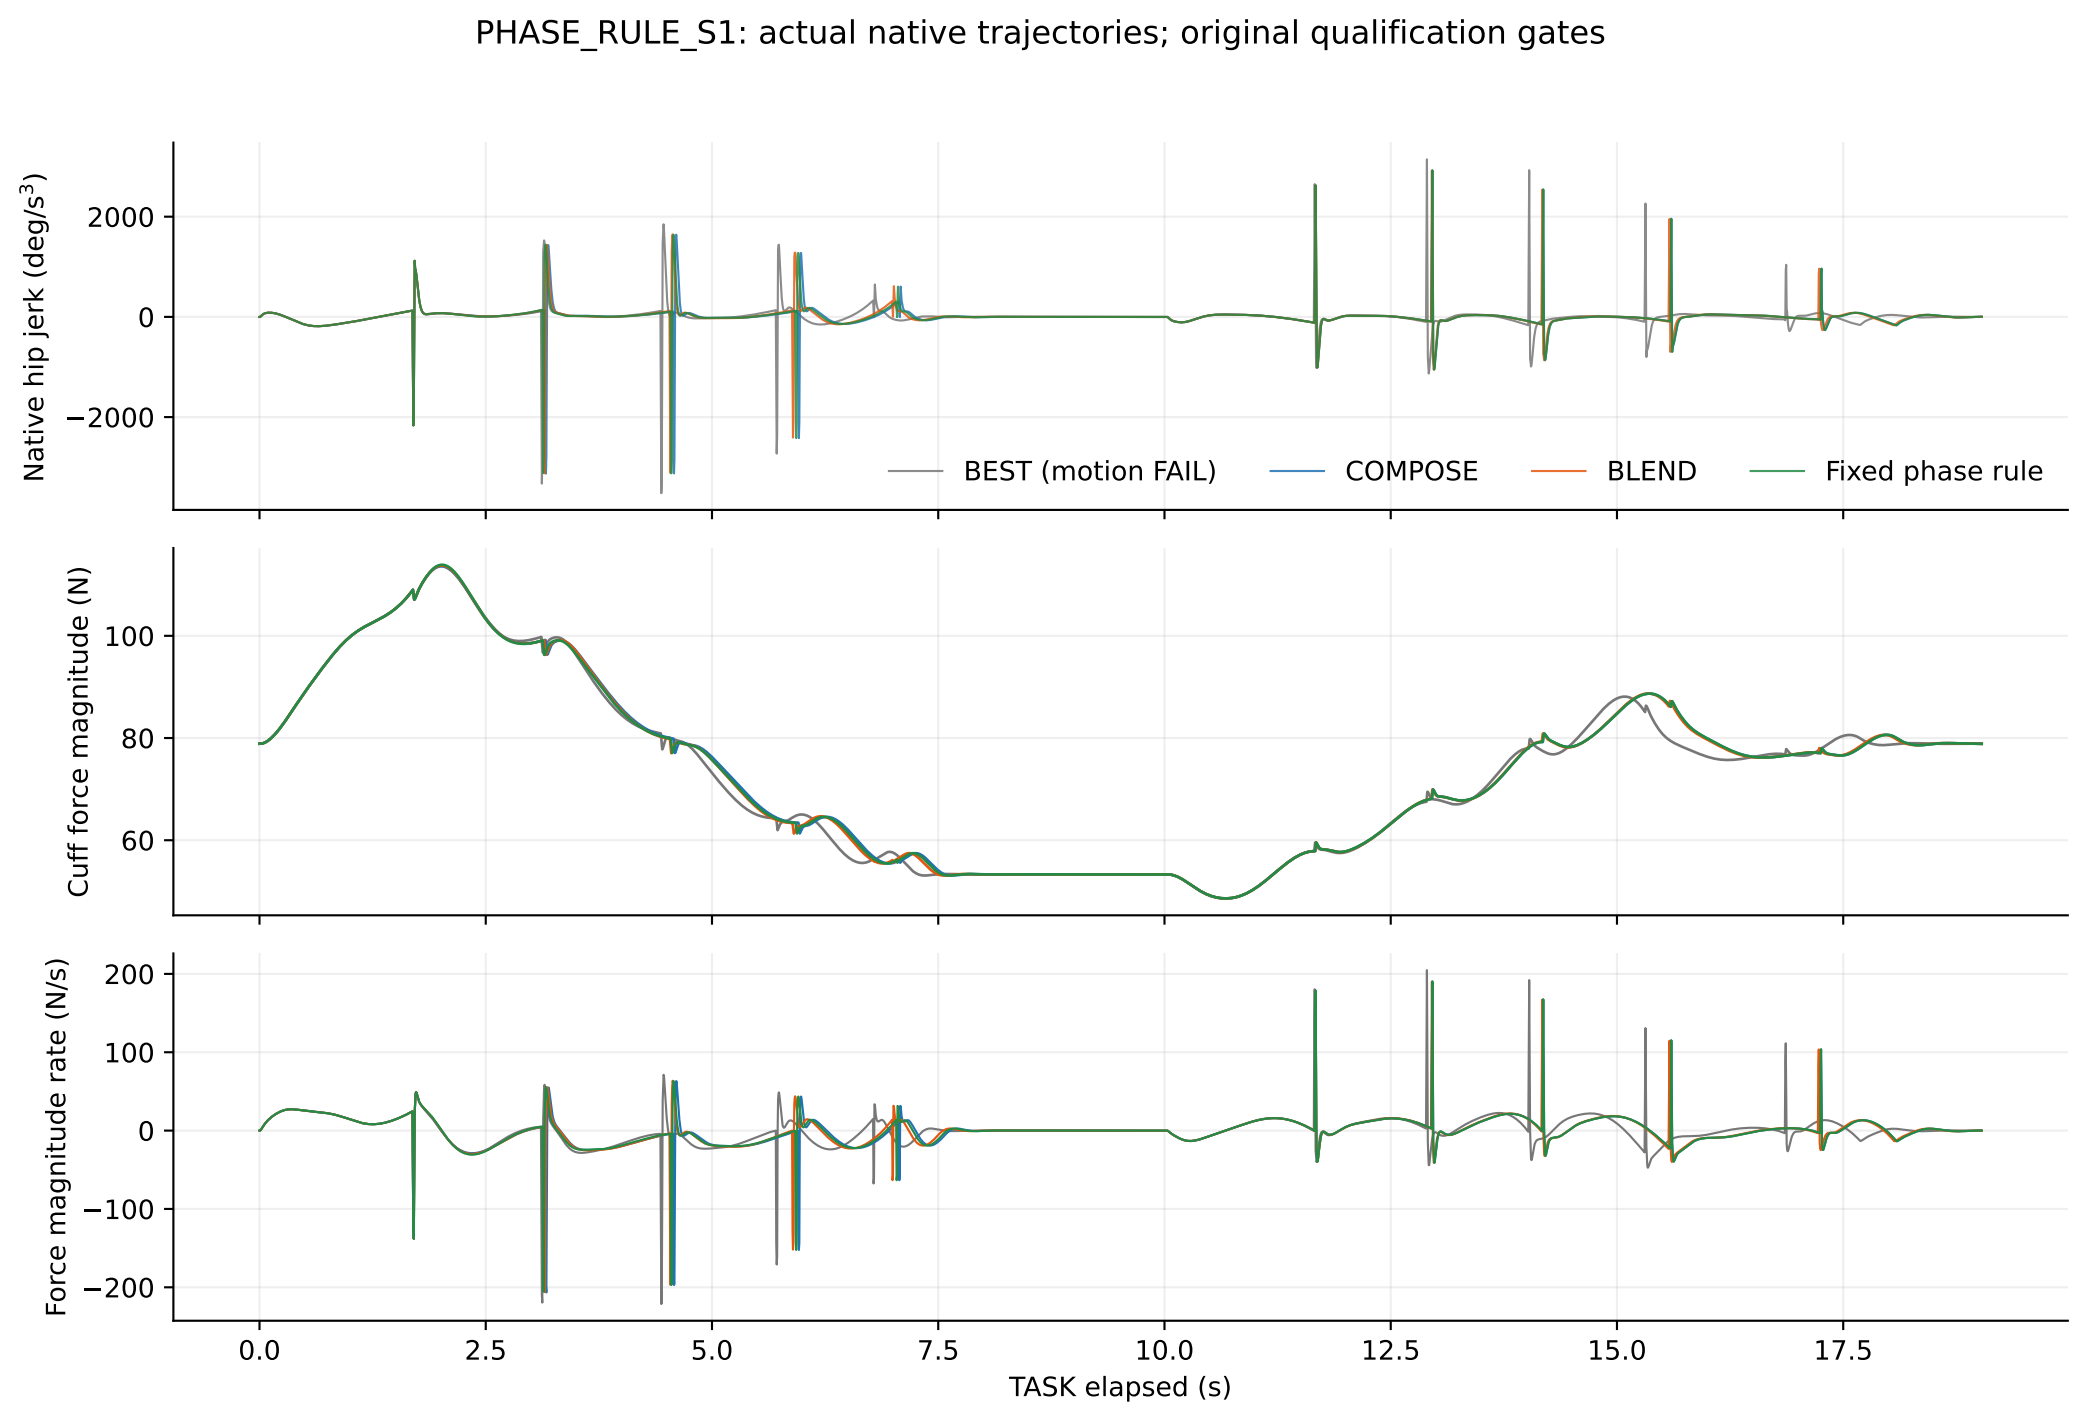

Display: every 20th native sample (5 ms); reported RMS uses every unfiltered 0.25 ms sample.
JF/JM retain the original 5 ms left integral. Lower jerk/rate does not establish patient comfort.