


val/reconstruction_mse

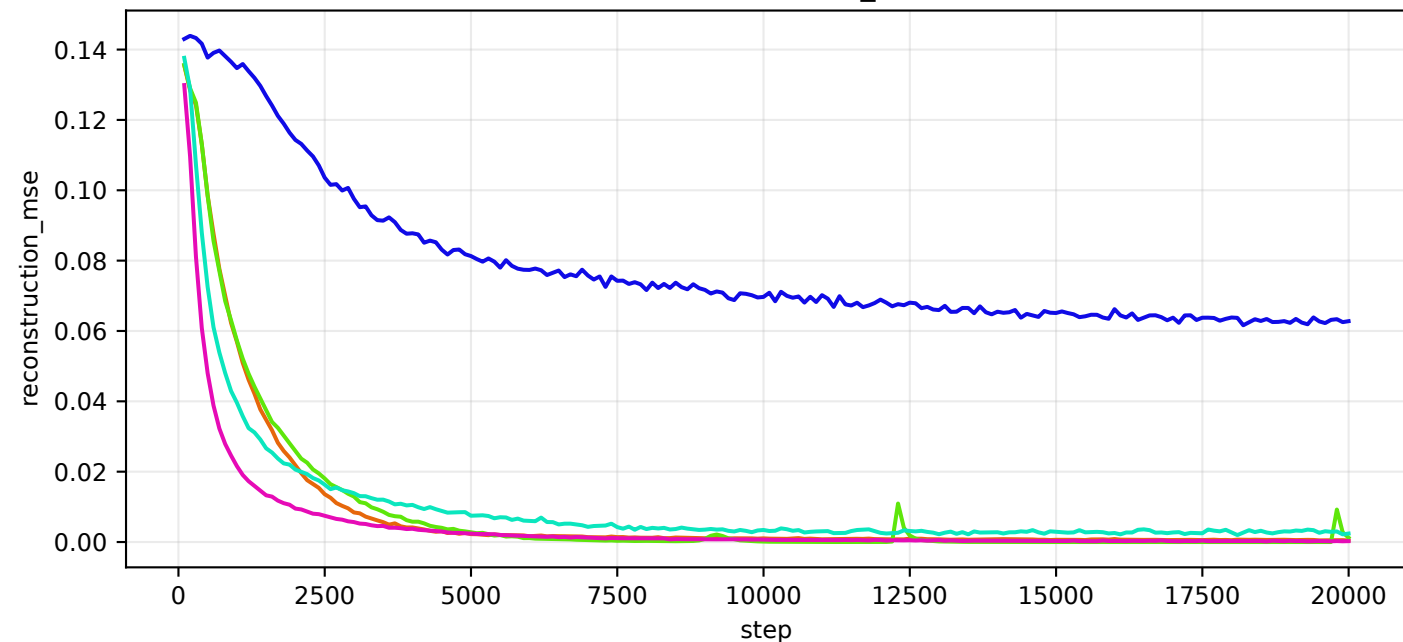

run	min	max	end	step
■ bpaee_baseline/mask00p-5000.0400.2000-00r	0.000462	0.1355	0.000462	19999
■ bpaee_singlepass/mask00p-5000.0400.2000-00r	6.83e-08	0.1356	0.001259	19999
■ dfaee_singlepass/mask00p-5000.0400.2000-00r	0.001984	0.1376	0.00241	19999
■ drtpae_singlepass/mask00p-5000.0400.2000-00r	0.06163	0.1439	0.06278	19999
■ hytaee_singlepass/mask00p-5000.0400.2000-00r	0.0001752	0.1299	0.0002563	19999