


train/mse_reconstruction_step

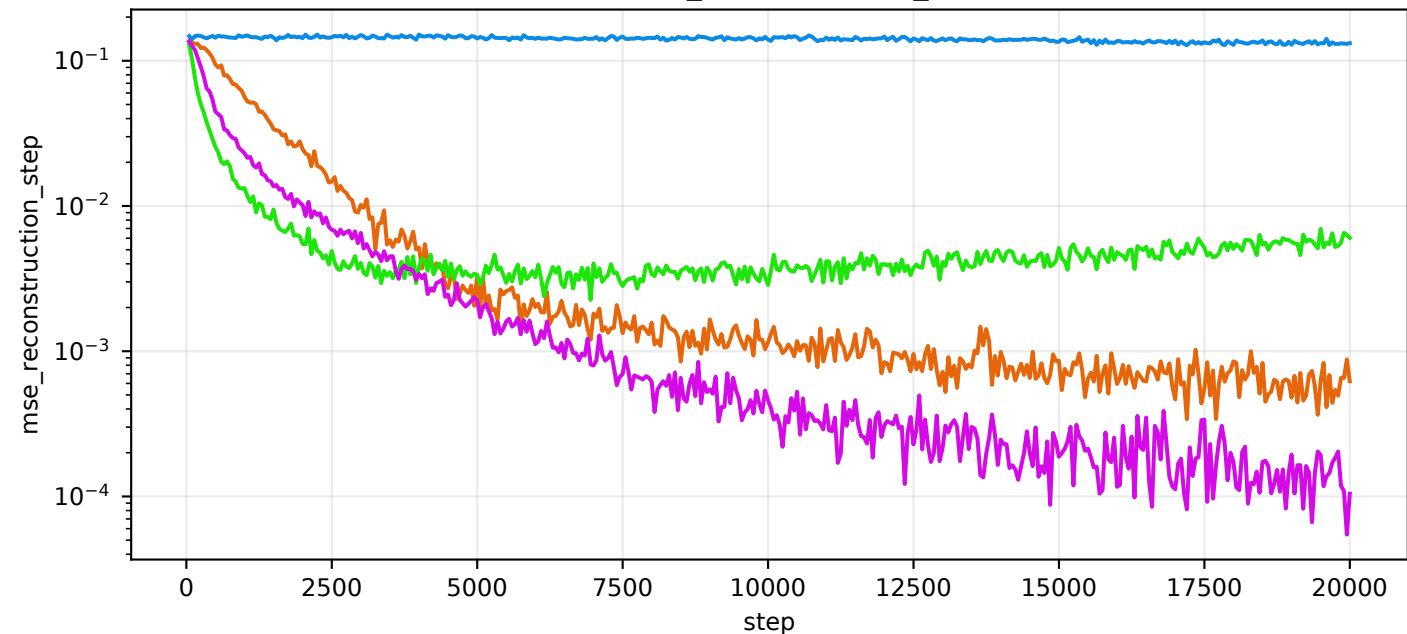

run	min	max	end	step
 bpaе_baseline/mask00p_5000.0400.2000_r00	0.0003408	0.1371	0.0006219	19999
 dfaаe_training/mask00p_5000.0400.2000_r00	0.002254	0.1288	0.006042	19999
 drtpae_training/mask00p_5000.0400.2000_r00	0.1279	0.1516	0.1323	19999
 hytaae_training/mask00p_5000.0400.2000_s20	5.466e-05	0.1354	0.0001043	19999