


train/mse_reconstruction_step

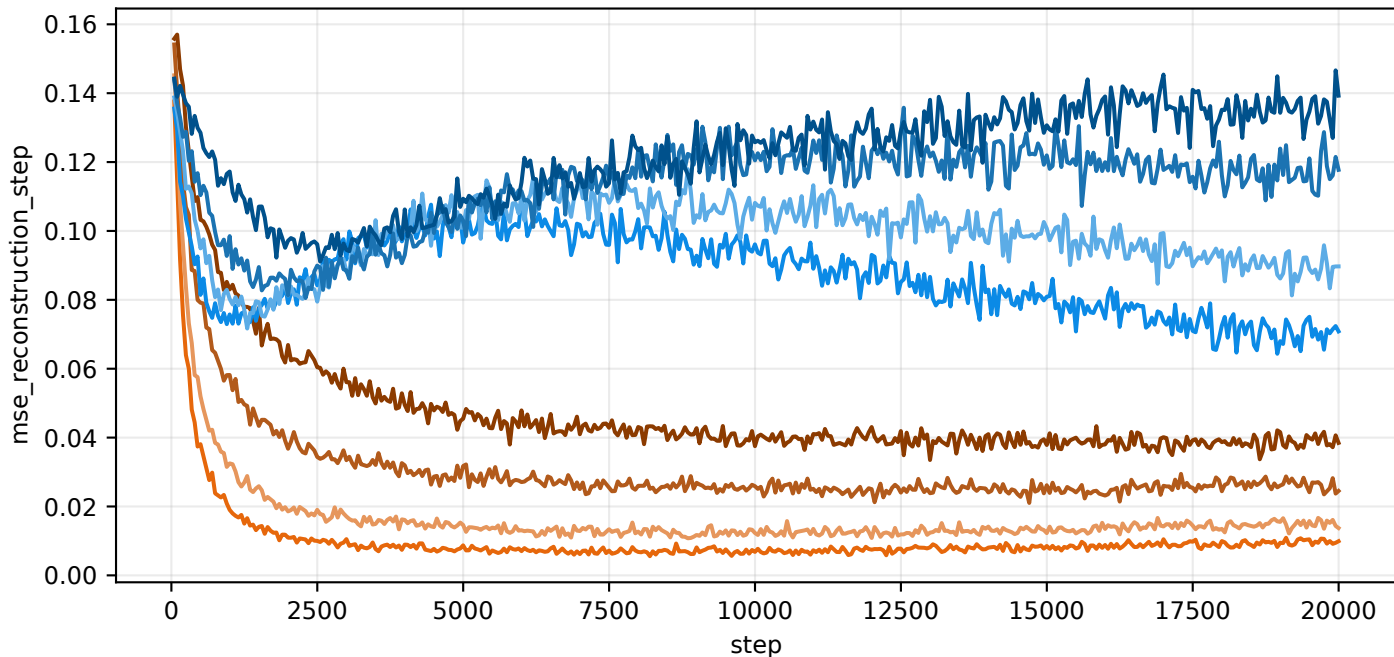

run	min	max	end	step
dfaae_group1/mask50p_5000.0400.2000_r00	0.005562	0.1376	0.009912	19999
dfaae_group1/mask75p_5000.0400.2000_r00	0.01076	0.1452	0.01373	19999
dfaae_group1/mask90p_5000.0400.2000_r00	0.02103	0.1541	0.02451	19999
dfaae_group1/mask95p_5000.0400.2000_r00	0.03349	0.157	0.03846	19999
dfaae_group2/mask50p_5000.0400.0064_r00	0.06434	0.1356	0.07084	19999
dfaae_group2/mask75p_5000.0400.0064_r00	0.07167	0.1388	0.08971	19999
dfaae_group2/mask90p_5000.0400.0064_r00	0.08052	0.1438	0.1177	19999
dfaae_group2/mask95p_5000.0400.0064_r00	0.09112	0.1466	0.1393	19999