


train/latent_post_active_rate

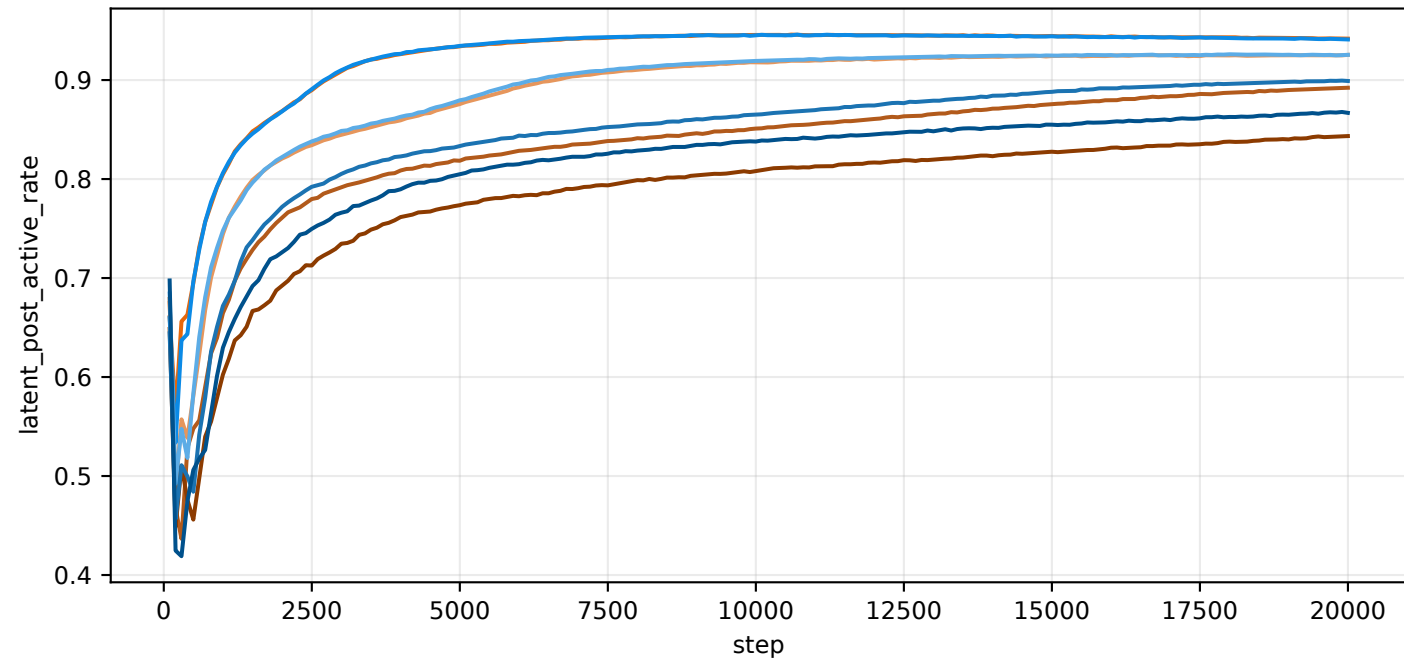

run	min	max	end	step
bpae_group1/mask50p_5000.0400.2000_r00	0.5643	0.9459	0.9419	19999
bpae_group1/mask75p_5000.0400.2000_r00	0.4866	0.9254	0.9254	19999
bpae_group1/mask90p_5000.0400.2000_r00	0.4366	0.8922	0.8922	19999
bpae_group1/mask95p_5000.0400.2000_r00	0.4486	0.8435	0.8434	19999
bpae_group2/mask50p_5000.0400.2000_r05	0.5338	0.9459	0.941	19999
bpae_group2/mask75p_5000.0400.2000_r05	0.4922	0.9261	0.9255	19999
bpae_group2/mask90p_5000.0400.2000_r05	0.4565	0.8995	0.8991	19999
bpae_group2/mask95p_5000.0400.2000_r05	0.419	0.8678	0.8668	19999