


train/mse_reconstruction_step

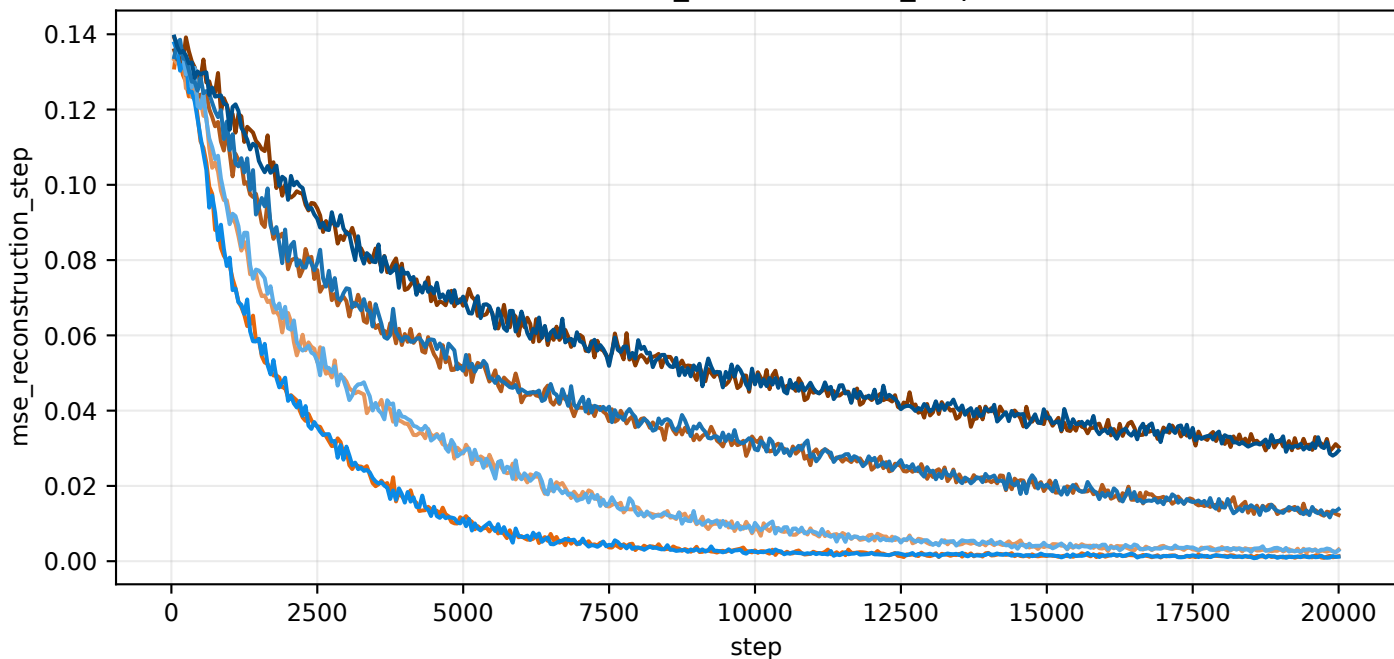

run	min	max	end	step
 bpae_group1/mask50p_5000.0400.2000_r00	0.0008902	0.1378	0.001316	19999
 bpae_group1/mask75p_5000.0400.2000_r00	0.002185	0.1344	0.003109	19999
 bpae_group1/mask90p_5000.0400.2000_r00	0.01208	0.1391	0.01228	19999
 bpae_group1/mask95p_5000.0400.2000_r00	0.02926	0.1392	0.03035	19999
 bpae_group2/mask50p_5000.0400.2000_r05	0.0007958	0.1376	0.001182	19999
 bpae_group2/mask75p_5000.0400.2000_r05	0.00237	0.1361	0.002909	19999
 bpae_group2/mask90p_5000.0400.2000_r05	0.01163	0.1386	0.01385	19999
 bpae_group2/mask95p_5000.0400.2000_r05	0.02804	0.1394	0.02936	19999