


val/reconstruction_bce

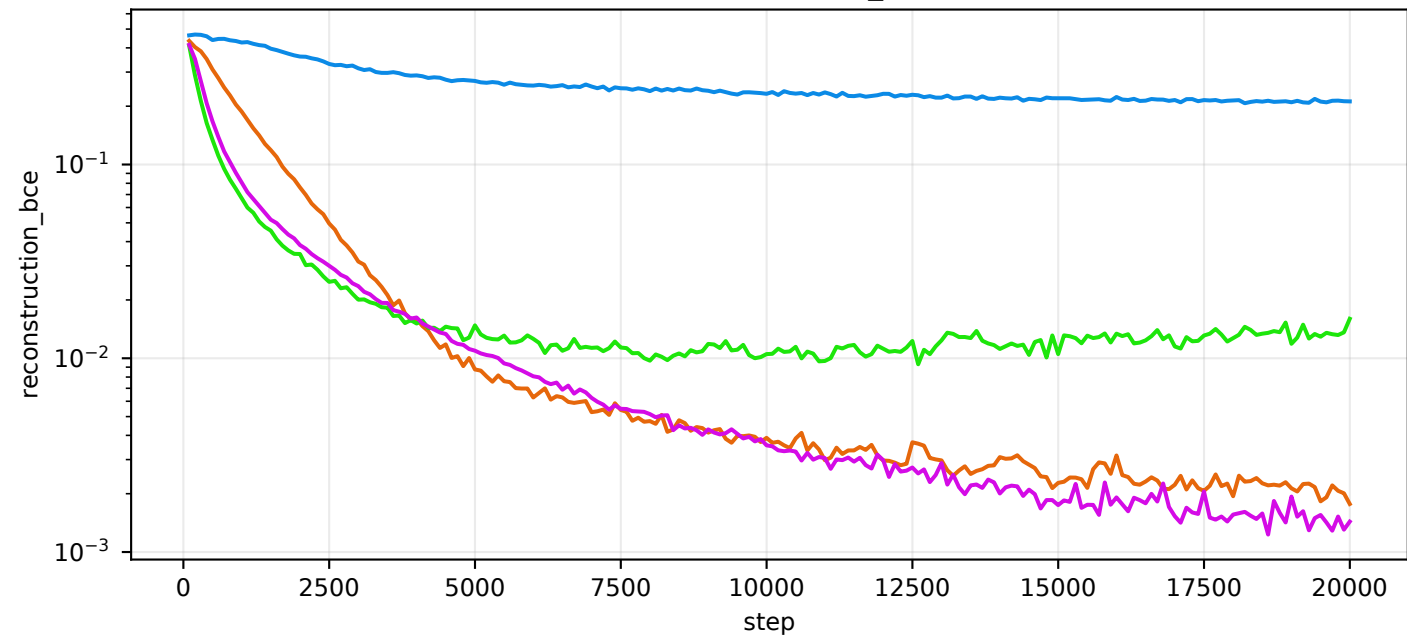

run	min	max	end	step
bpae_baseline/mask00p-5000.0400.2000-00r	0.00177	0.4346	0.00177	19999
dfaee_singlepass/version_0	0.009314	0.4116	0.01598	19999
drtpae_singlepass/mask00p-5000.0400.2000-00r	0.2072	0.4687	0.2118	19999
hytaae_singlepass/mask00p-5000.0400.2000-00r	0.001231	0.4147	0.001435	19999