


val/reconstruction_mse

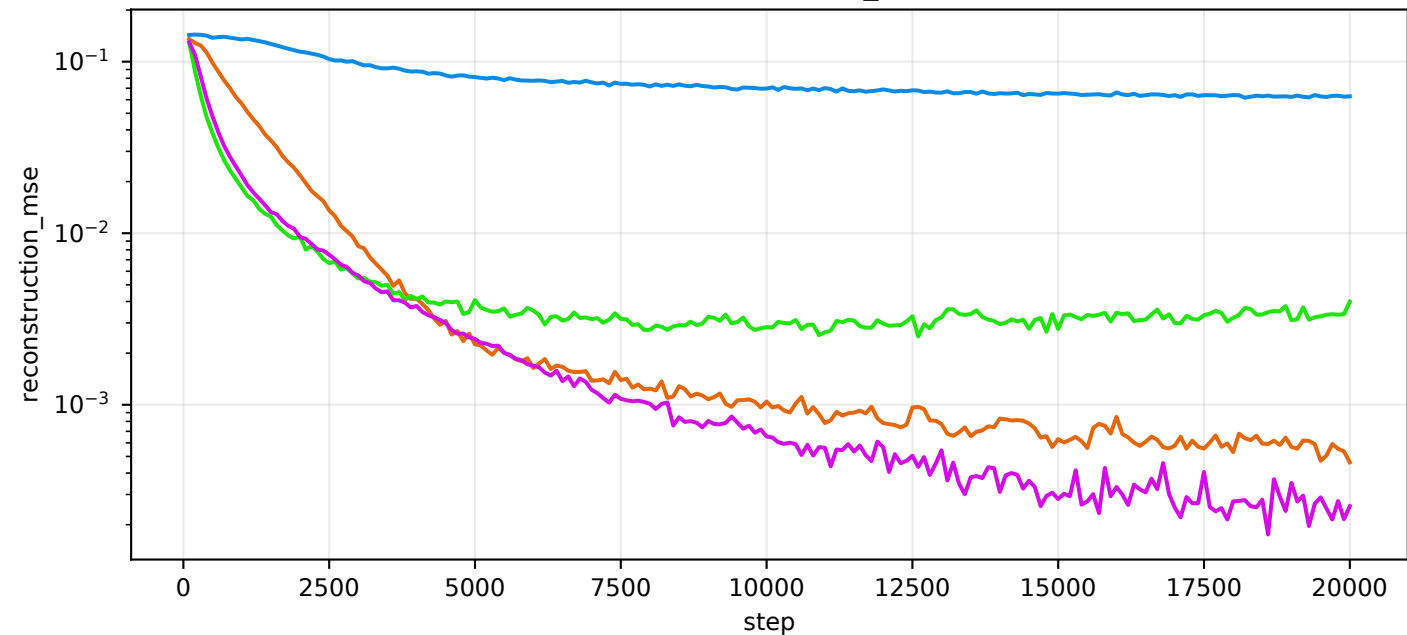

run	min	max	end	step
 bpae_baseline/mask00p-5000.0400.2000-00r	0.000462	0.1355	0.000462	19999
 dfaae_singlepass/version_0	0.002504	0.1298	0.003991	19999
 drtpae_singlepass/mask00p-5000.0400.2000-00r	0.06163	0.1439	0.06278	19999
 hytaae_singlepass/mask00p-5000.0400.2000-00r	0.0001752	0.1299	0.0002563	19999