


train/mse_reconstruction_step

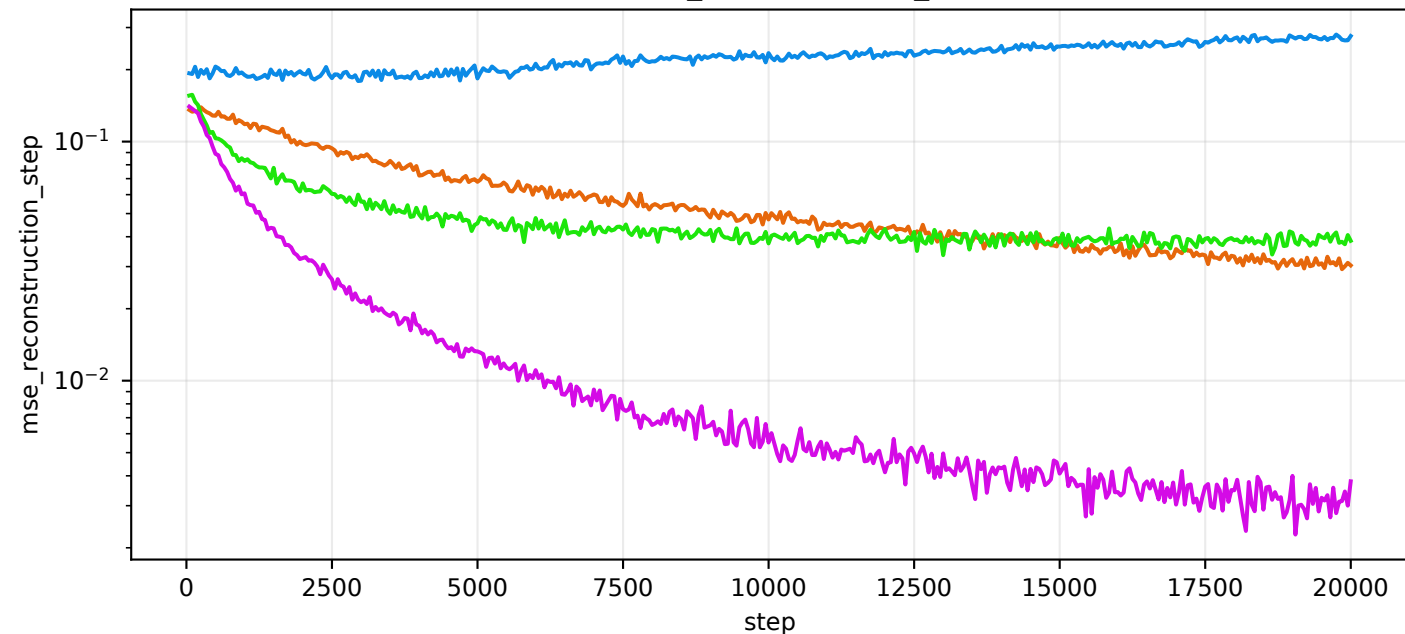

run	min	max	end	step
 bpaе_baseline/mask95p_5000.0400.2000_r00	0.02926	0.1392	0.03035	19999
 dfaе_training/mask95p_5000.0400.2000_r00	0.03349	0.157	0.03846	19999
 drtpae_training/mask95p_5000.0400.2000_r00	0.1792	0.2804	0.2764	19999
 hytaae_training/mask95p_5000.0400.2000_s20	0.002272	0.1401	0.003793	19999