


train/mse_reconstruction_step

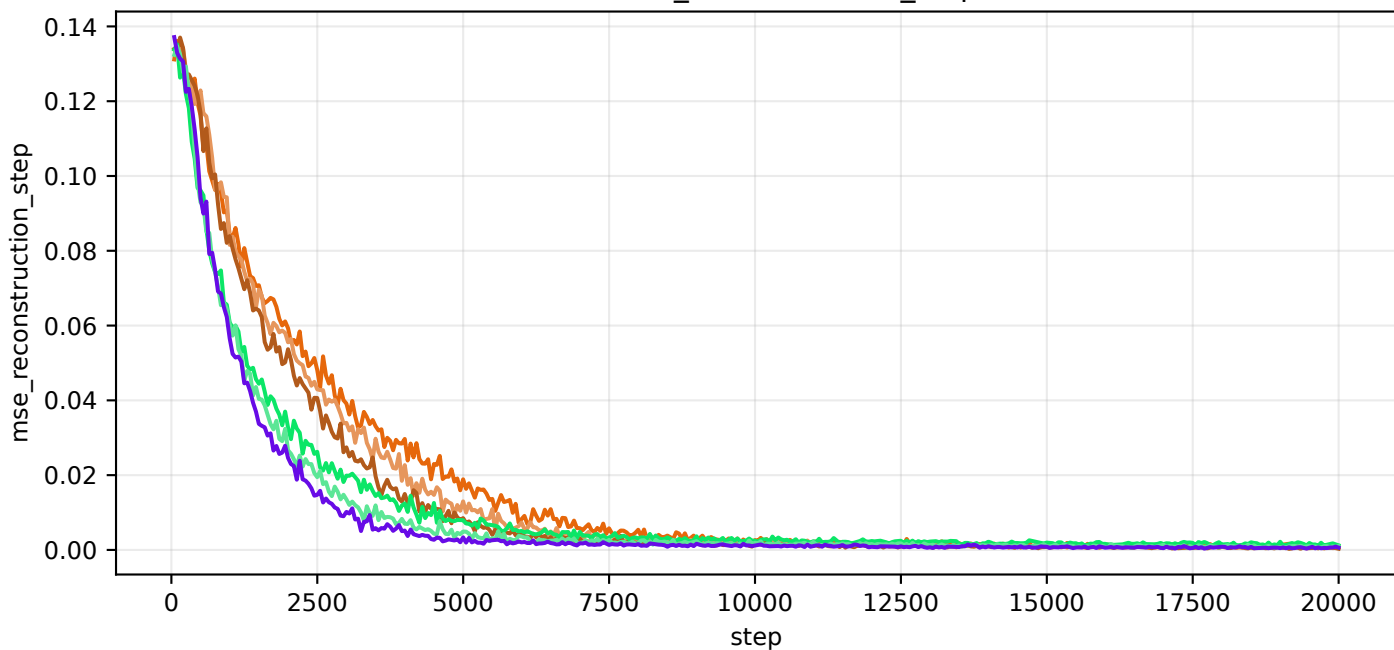

run	min	max	end	step
 bpae_group1/mask00p_5000.0400.0064_r00	0.0004879	0.1361	0.0006869	19999
 bpae_group1/mask00p_5000.0400.0128_r00	0.0004415	0.1343	0.0006763	19999
 bpae_group1/mask00p_5000.0400.0250_r00	0.0002723	0.137	0.0003181	19999
 bpae_group2/mask00p_5000.0100.2000_r00	0.001099	0.1352	0.001225	19999
 bpae_group2/mask00p_5000.0200.2000_r00	0.0005865	0.1347	0.00103	19999
 bpae_training/mask00p_5000.0400.2000_r00	0.0003408	0.1371	0.0006219	19999