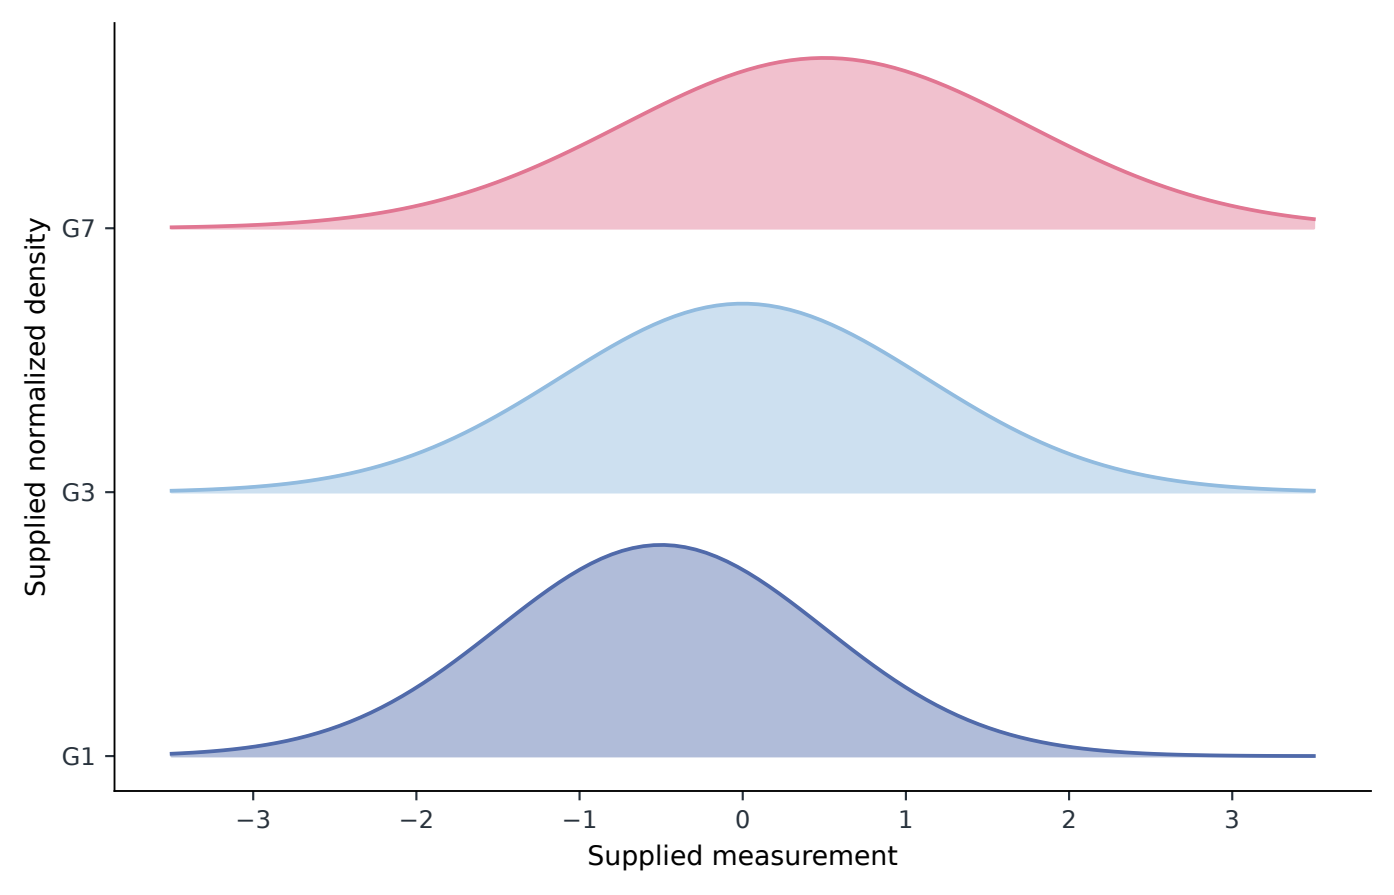
Supplied normalized density
G7
G3
G1
−3
−2
−1
0
1
2
3
Supplied measurement