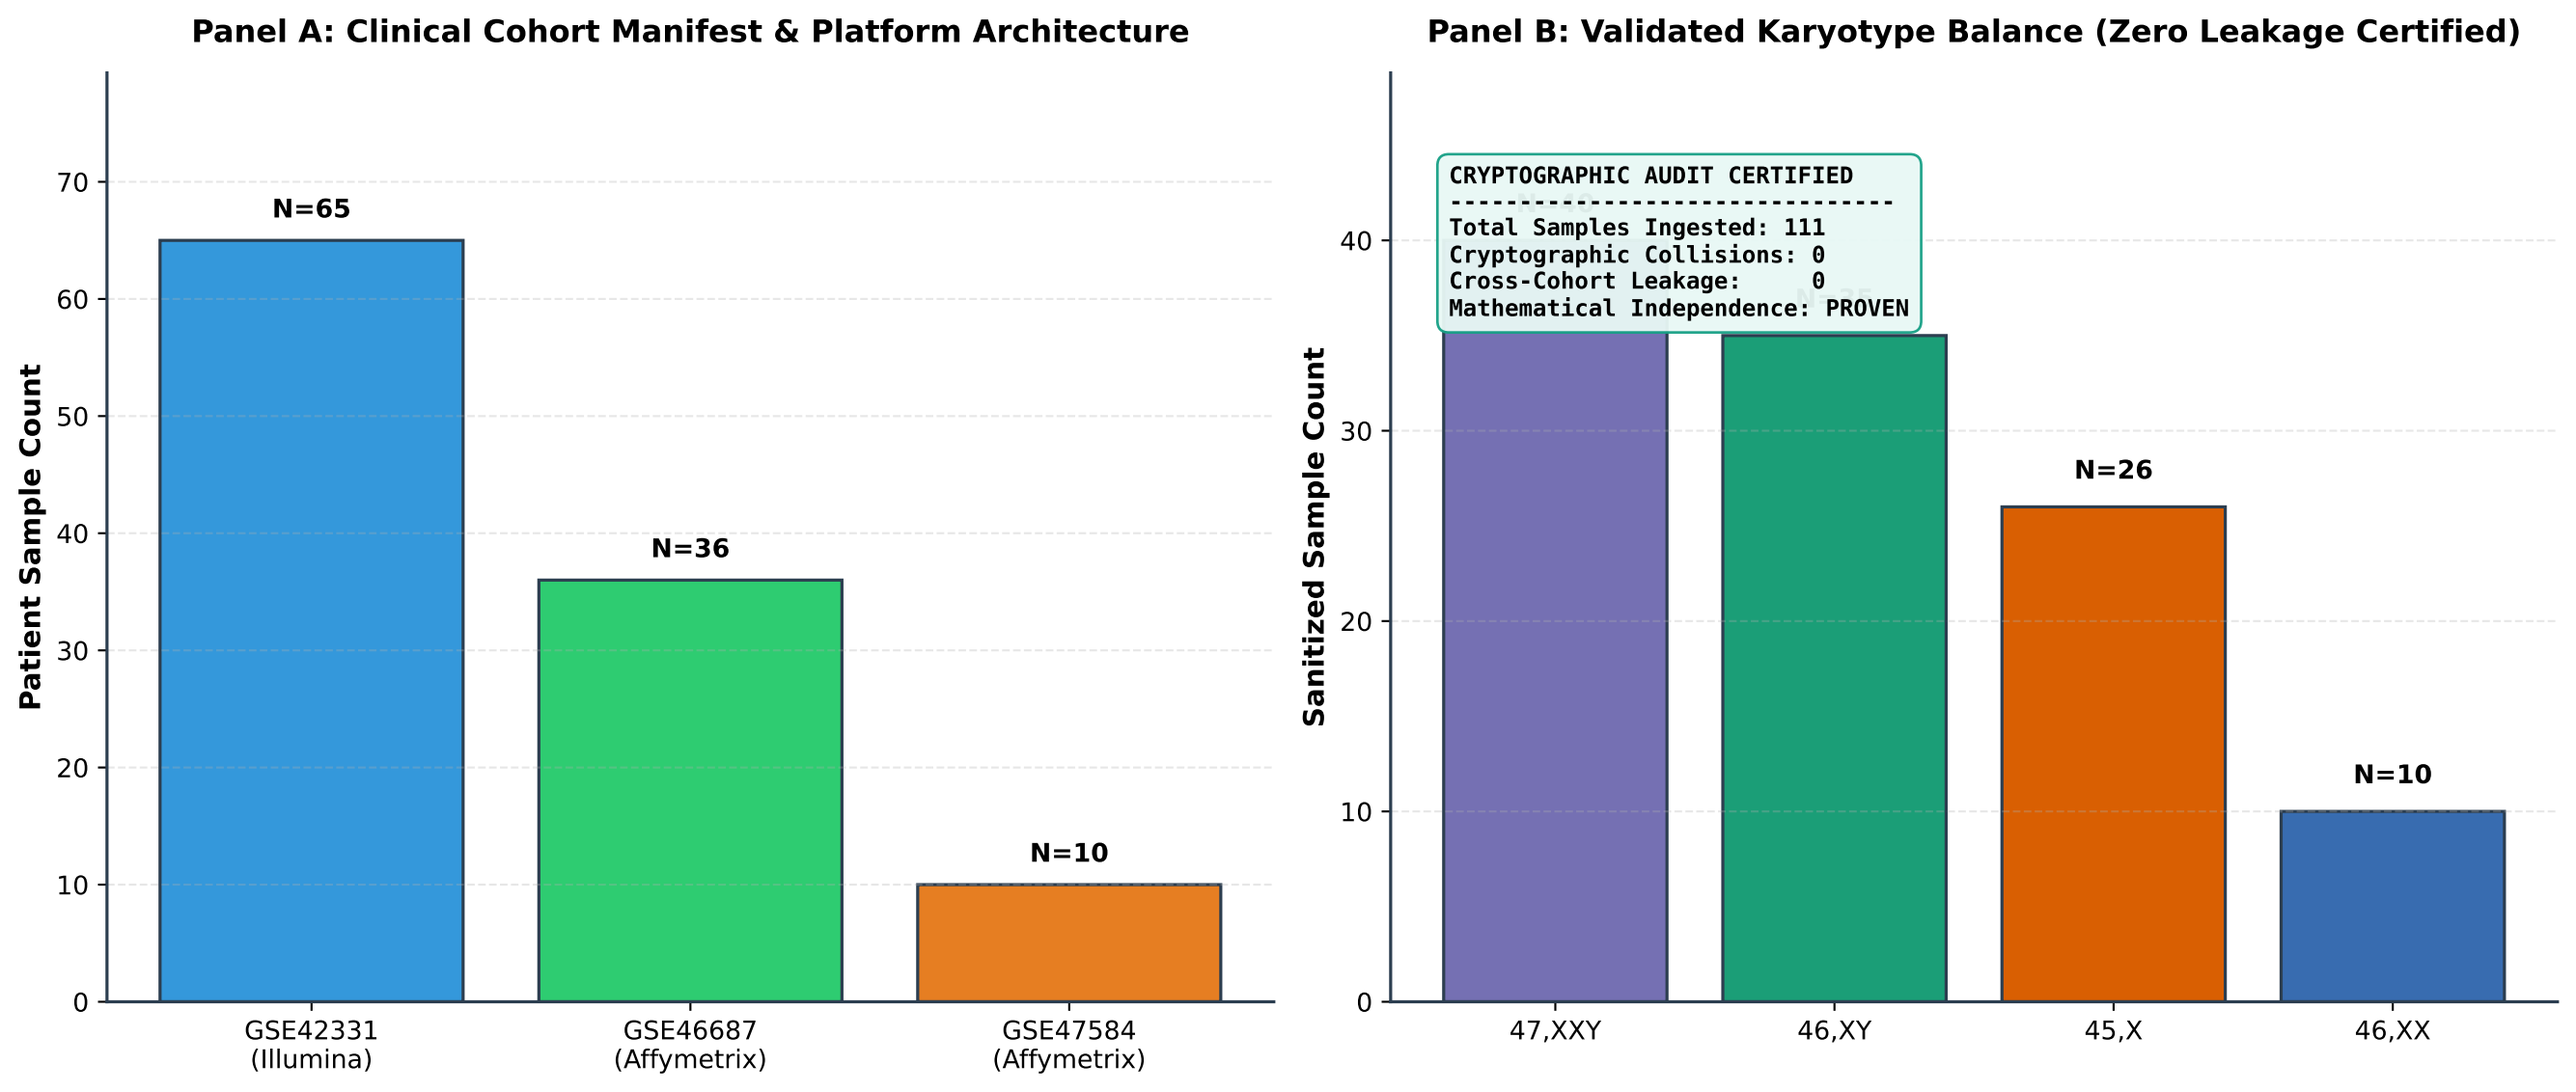
Panel A: Clinical Cohort Manifest & Platform Architecture
Patient Sample Count
0
10
20
30
40
50
60
70
N=65
N=36
N=10
GSE42331
(Illumina)
GSE46687
(Affymetrix)
GSE47584
(Affymetrix)
Panel B: Validated Karyotype Balance (Zero Leakage Certified)
Sanitized Sample Count
0
10
20
30
40
CRYPTOGRAPHIC AUDIT CERTIFIED
Total Samples Ingested: 111
Cryptographic Collisions: 0
Cross-Cohort Leakage: 0
Mathematical Independence: PROVEN
N=26
N=10
47,XXY
46,XY
45,X
46,XX