

Retention-index calibration report

22,314

Features
calibrated

13/15

Standards
samples · panel 15/15

0.0–23.9

RT range
samples min · panel 0.0–23.9

5–100

iRT range
dimensionless


0.03

RT offset
median lobs–refl (min)


81%

Coverage
features with an RI

Quality fingerprint

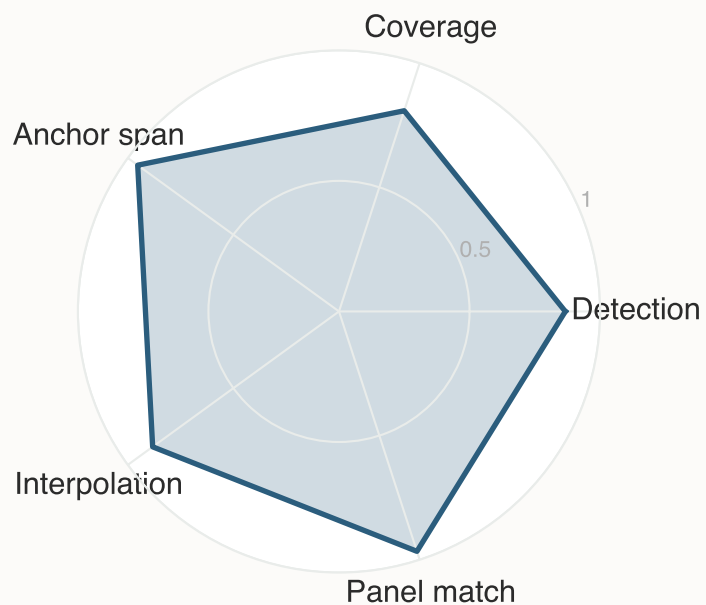


Standard detection — reference vs panel vs samples

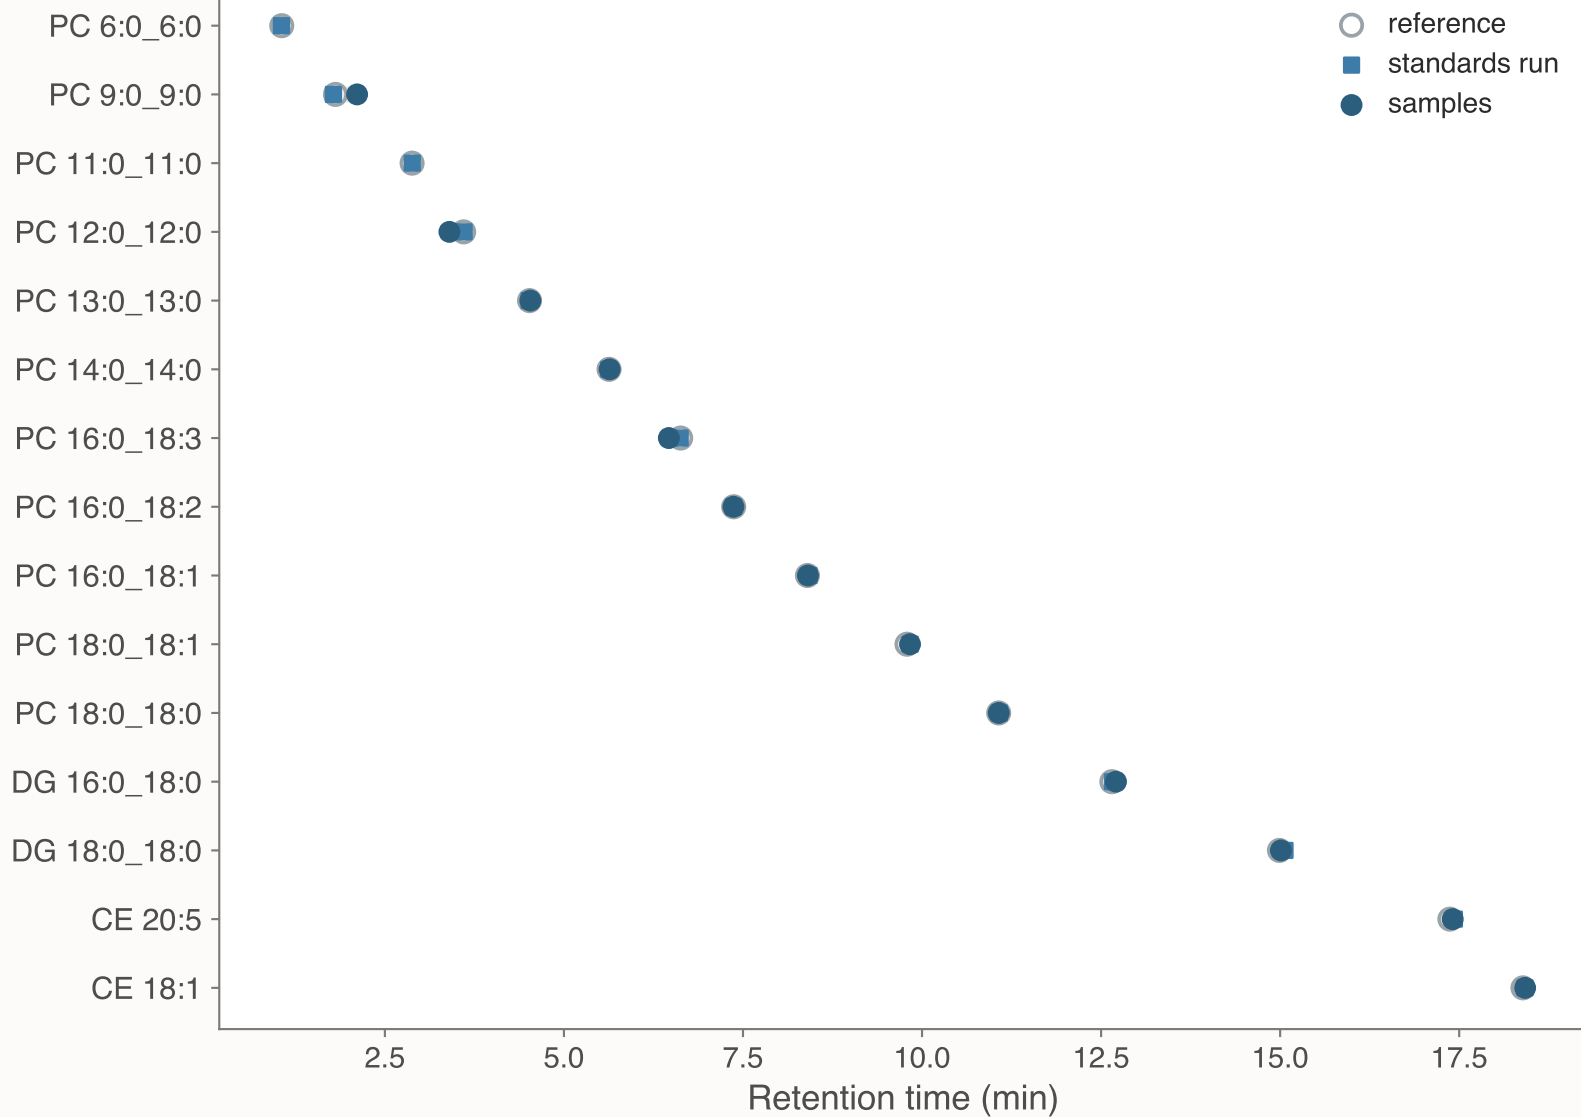

Reconstructed feature-intensity profile · before vs after calibration

standards highlighted & connected — line slant = RT offset · reconstructed from the feature table (binned intensity)

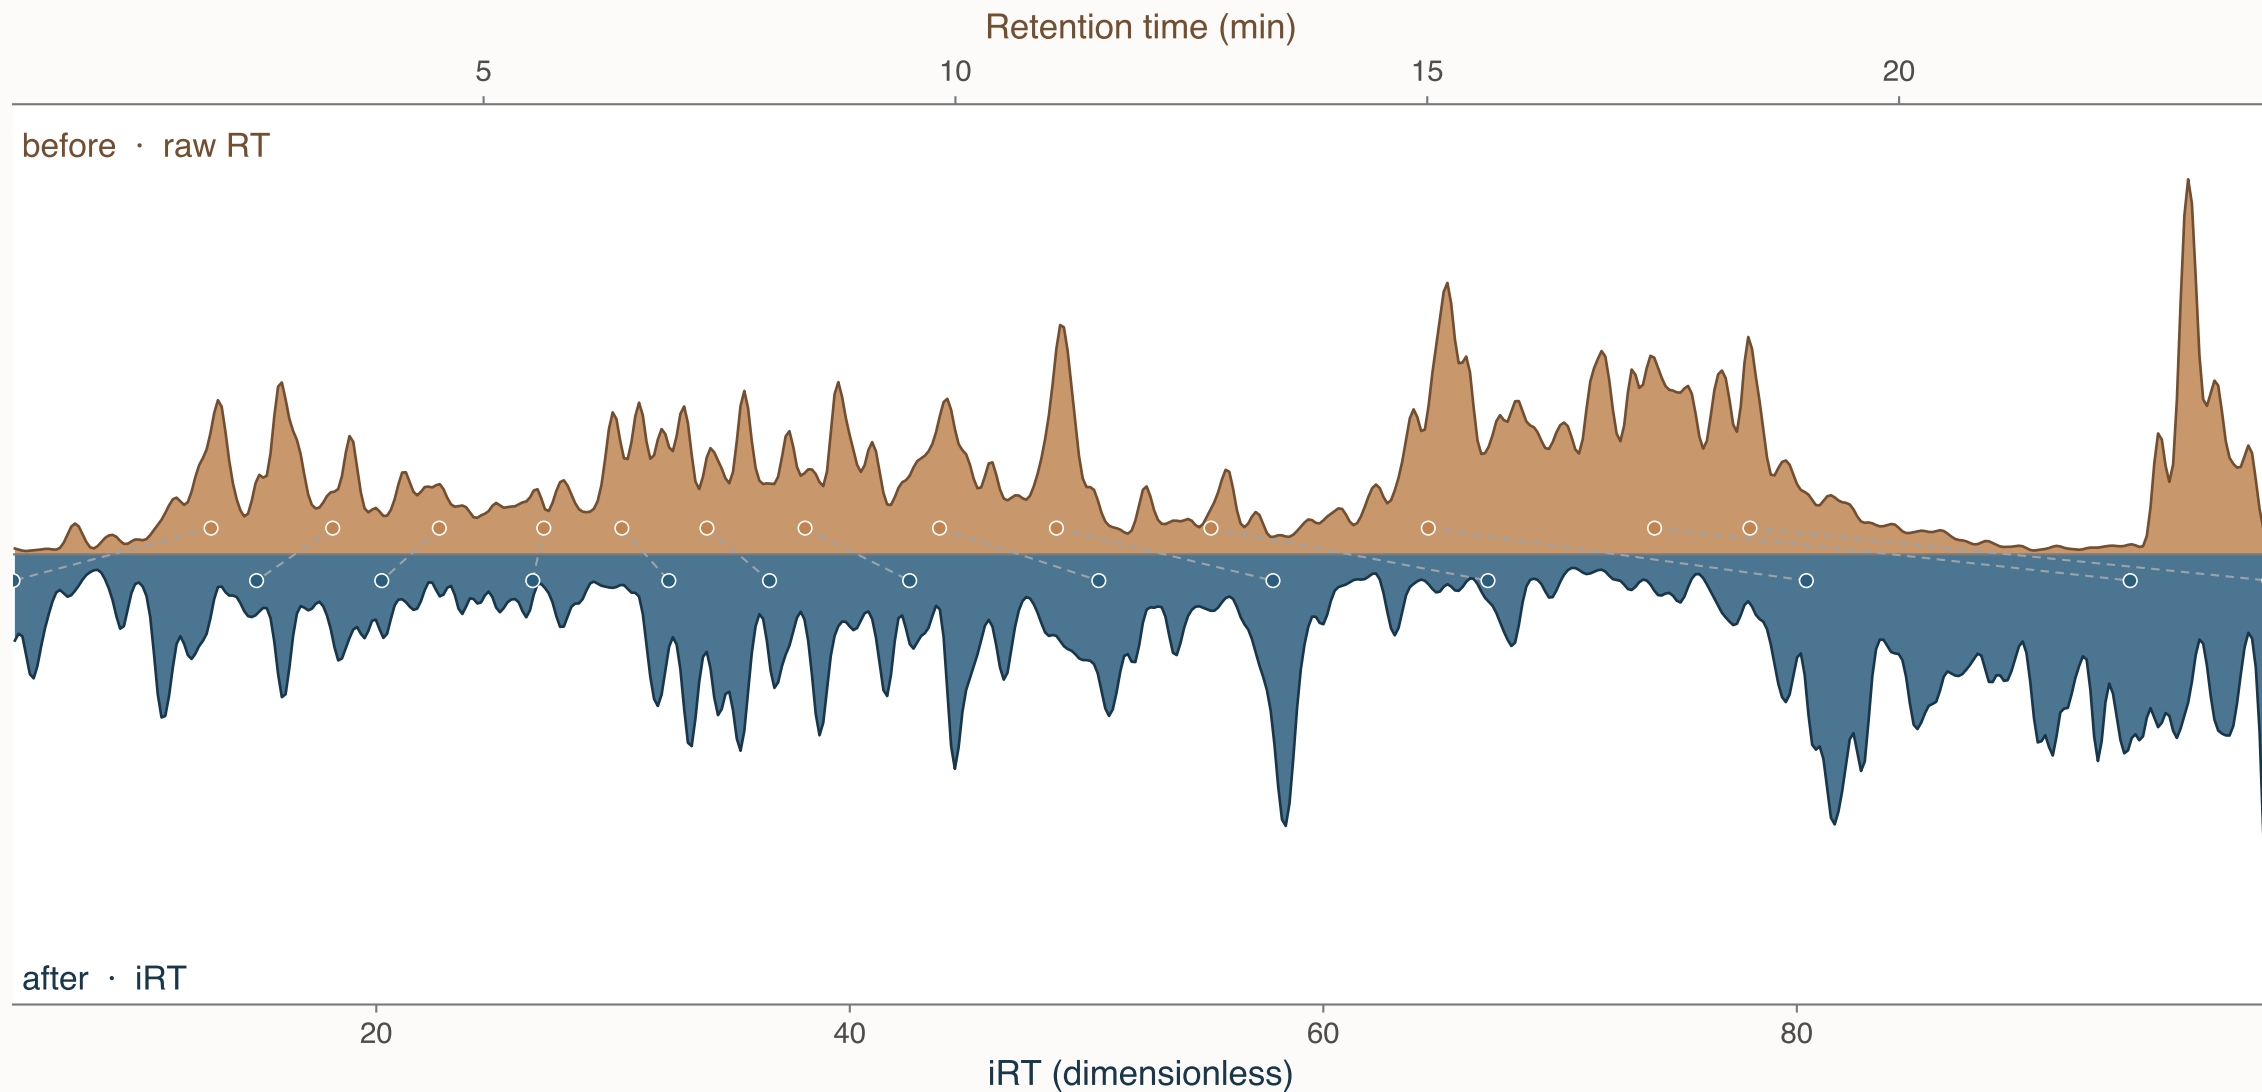

Calibration warp — RT → iRT

