



2026

Absolute Quantification and Identification of RNA from RNA-Lipid Nanoparticles using High Resolution Mass Spectrometry

Jason C. Funderburk
Virginia Commonwealth University

Follow this and additional works at: <https://scholarscompass.vcu.edu/etd>

 Part of the [Analytical Chemistry Commons](#), [Biochemistry Commons](#), [Biological and Chemical Physics Commons](#), [Investigative Techniques Commons](#), [Lipids Commons](#), [Medicinal Chemistry and Pharmaceutics Commons](#), [Nanomedicine Commons](#), [Nucleic Acids, Nucleotides, and Nucleosides Commons](#), [Other Pharmacy and Pharmaceutical Sciences Commons](#), and the [Pharmaceutical Preparations Commons](#)

© Jason C. Funderburk

Downloaded from

<https://scholarscompass.vcu.edu/etd/8315>

This Thesis is brought to you for free and open access by the Graduate School at VCU Scholars Compass. It has been accepted for inclusion in Theses and Dissertations by an authorized administrator of VCU Scholars Compass. We are committed to making our research accessible to all users and ensuring that materials conform to accessibility standards. If you encounter an accessibility barrier and need material remediated, please contact us at libcompass@vcu.edu.

Absolute Quantification and Identification of RNA from RNA-Lipid Nanoparticles using High Resolution Mass Spectrometry

©2026 Jason C. Funderburk

Absolute Quantification and Identification of RNA from RNA-Lipid Nanoparticles using High
Resolution Mass Spectrometry

A Thesis submitted in partial fulfillment of the requirements for the degree of Master of Science,
Pharmaceutical Sciences at Virginia Commonwealth University

By
Jason C. Funderburk,
B.S., Virginia Commonwealth University, 2022

Directors:
Matthew S. Halquist, PhD
Sandro R. P. da Rocha, PhD
Department of Pharmaceutics

Virginia Commonwealth University
Richmond, Virginia
April 2026

Acknowledgments

I would like to express my sincere gratitude to my parents and family for their unwavering support throughout my academic journey. Their guidance has been the cornerstone in my life, building my abilities to complete this accomplishment. I am forever grateful for their encouragement and unlimited support. I also extend my heartfelt thanks to my family for their patience and understanding through difficult times of my academic journey. Their love and support have always been a core part of my life and has greatly affected this work.

I am deeply indebted to my academic advisors for their invaluable guidance, expertise, and unwavering support throughout the course of my graduate school experience. Their insightful feedback and mentorship have been instrumental in shaping and guiding this thesis and my overall professional growth. Furthermore, I would like to acknowledge the support from fellow students and graduate faculty. Their assistance and feedback have enriched my research experience and contributed to the success of this project.

This thesis is a culmination of collective efforts and support from all those mentioned above, and I am truly grateful for all their contributions.

Table of Contents

Acknowledgments.....	iv
Table of Contents.....	v
List of Figures	vii
List of Tables	ix
Abstract	x
Chapter 1: Literature Review	1
Mass Spectrometry Based Characterization of RNA Encapsulated Lipid Nanoparticles: Current Approaches and Future Potential.....	2
RNA Based Therapeutics.....	2
Lipid Nanoparticle Delivered RNA: Overview	3
Stability of RNA Therapeutics.....	19
Current Quality Characterization Methods and Challenges of RNA Lipid Nanoparticle Drugs ..	25
Current Mass Spectrometry Approaches for Characterization of RNA-LNP Therapeutics.....	30
Conclusion	41
Chapter 2: Hypothesis and Specific Aims.....	43
1. Introduction and Research Problem.....	44
2. Hypothesis.....	46
3. Specific Aims.....	47
4. Clinical Relevance and Innovation	47
Chapter 3: Experimental	49
Absolute Quantification and Identification of RNA from RNA-Lipid Nanoparticles using High Resolution Mass Spectrometry	50
1. Introduction:.....	50
2. Materials and Methods:	53
2.1. Materials.....	53
2.2. Preparation and Characterization of RNA-LNPs.....	54
2.3. RNA Extraction from RNA-LNP	57

2.4. LC-MS Conditions for RNA Absolute Quantification and Identification	59
2.5. Data Processing.....	59
2.6. Statistical Analysis	60
3. Results and Discussion:	60
3.1. LC-MS Identification of Intact RNA extracted from RNA-LNP.....	60
3.2. LC-MS Absolute Quantification of Extracted RNA	66
4. Conclusion	68
Chapter 4: Overall conclusion and future directions	71
Chapter 5: Bibliography.....	74
Chapter 6: Appendix.....	85

List of Figures

Figure 1.1: Illustration of the evolution of liposome (A), lipoplex (B), SPLP (C) to LNP (D) for nucleic acid delivery. Created with BioRender.com.	7
Figure 1.2: Simplistic illustration of LNP structure and components with typical lipid compositions. Created with BioRender.com.	8
Figure 1.3: Chemical structures, cLogP, and cpKa of the FDA approved ionizable lipids for LNPs. Created with ChewDraw.	9
Figure 1.4: Examples of helper lipids in LNP formulations. Created with ChewDraw.	12
Figure 3.1: Preparation of RNA-Based LNPs by the Ethanol Injection Method: The preparation of RNA-based lipid nanoparticles via the ethanol injection method involves four steps followed by characterization. First, the lipid components are dissolved in ethanol (100 μ l), and the nucleic acids are dissolved in the aqueous phase (300 μ l) containing citrate buffer (pH 4.0). Secondly, the organic phase is rapidly injected dropwise into the aqueous phase under chaotic stirring conditions (900 rpm), promoting lipid nanoparticle formation stirring continues for 5-minutes after injecting. Thirdly, post-stirring a 5-minute resting period with no stirring is observed. Next, the purification and ethanol removal steps are performed with 100 μ l of PBS added. Lastly, the prepared LNPs undergo characterization for hydrodynamic diameter (HD), surface charge, content, and encapsulation efficiency (EE%) before storage under appropriate conditions. The HD and polydispersity index (PDI) are determined by diluting the sample a hundredfold in PBS and measured using dynamic light scattering (DLS). Content and EE% are quantified using the fluorescent RiboGreen [®] assay. Created with BioRender.com.	55
Figure 3.2: Extraction of RNA from LNPs by Isopropanol Precipitation Method: The extraction of RNA from RNA-LNPs via the isopropanol precipitation method involves six steps followed by measuring the resuspended RNA concentration. First, the RNA-LNP formulation (100 μ l) is diluted tenfold in 60 mM ammonium acetate in isopropanol (IPA) (900 μ l). Secondly, the solution is briefly vortexed then centrifuged (14,000 g, 4°C) for 15-minutes. Thirdly, the supernatant containing the lipids is collected and removed. Next to wash, IPA (1 mL) is added with mixing to disturb the RNA pellet then centrifuged (14,000 g, 4°C), followed by removal of the IPA. The wash step is repeated with the use of chilled 70% ethanol (1 mL). Lastly, the RNA pellet is dissolved in water and the concentration measured by LC-MS. All steps were performed on ice. Created with BioRender.com.	58
Figure 3. 3: XIC of RNA constructs: (a) XIC of guanine (150.0421 m/z) CAD fragment from the 60-mer RNA -28 charged precursor with a 1.02 ± 0.01 min retention time (rt). (b) XIC of adenine (134.0470 m/z) CAD fragment from the antisense FLuc-S1 dsRNA construct -11 charged precursor with a 1.01 ± 0.01 min rt. Created with SCIEX OS Analytics.	62
Figure 3.4: Raw TIC and MRM Spectrums of RNA constructs: (a) TIC spectrum of 60-mer RNA and (b) CAD MRM spectrum from the -28 charged precursor with a 1.02 ± 0.01 min retention time (rt). (c) TIC spectrum of the FLuc-S1 dsRNA and (d) CAD MRM spectrum from the -11 charged precursor with a 1.01 ± 0.01 min rt. Created with SCIEX Explorer.	65

Figure S1: Calibration Curve of 60-mer RNA: To perform absolute quantification an external calibration curve with the 60-mer RNA construct was prepared between 50 – 1500 ng/mL and measured n = 3. The assay was validated using ICH m10 bioanalytical method development guidance.86

Figure S2: Calibration Curve of Antisense FLuc-S1 dsRNA construct: To perform absolute quantification an external calibration curve with the FLuc-S1 RNA construct was prepared between 5 – 1500 ng/mL and measured n = 3. The assay was validated using ICH m10 bioanalytical method development guidance.87

List of Tables

Table 1.1: Current Recommended Critical Quality Attributes (CQAs) and Analytical Methods for mRNA-LNP Drug Products: The draft quality attributes (QA), and corresponding analytical methods proposed for RNA-LNP drug products, followed by the regulatory agencies that recommend the method for the quality and attribute. QA methods without an established method from USP chapters are still in draft ^{87,88}	28
Table 3.1: Parameters of LNP Formulation.....	54
Table 3.2: Physiochemical Properties of LNP Formulations: The lipid nanoparticle formulations were composed of ionizable lipid, sterol, phospholipid, and PEG lipid in a molar ratio of 50:38.5:10:1.5, respectively. n = 6.....	57
Table 3.3: List of m/z Values for Charge Range of Intact RNA Precursor Ions: The double-stranded FLuc-S1 dsRNA was composed of sense (S) and antisense (AS) RNA constructs.	63
Table 3.4: List of m/z values for MRM RNA Construct Product Ions: The monitored RNA sequence products include the negative CAD product ions of adenine (A), cytosine (C), guanine (G), uracil (U), phosphate backbone (p), phosphoribose (RbP), Adenosine-5'-monophosphate (AMP), adenosine 3',5'-cyclic monophosphate (cAMP).	66
Table 3.5: Results Comparison of RNA Quantification Techniques: The results for the theoretical RNA concentration were calculated using a dilution formula accounting for formulation (100x), RNA extraction (10x) and MS assay dilutions (10x) from the original UV-Vis measurements. Each quantification method has been converted to ng/mL to facilitate comparison. Each quantification result was measured at n = 6 for UV-Vis, n = 3 for fluorescence, and for LC-MS n = 4 (60-mer) and n = 3 (Antisense FLuc-S1 dsRNA).	67
Table 6.1: List of Abbreviations	85
Table S1: Regression equation and calibration curve report of 60-mer RNA construct: MRM scans were used to perform quantification monitoring the negative CAD product ion of guanine (150.0416 m/z) from the 60-mer constructs intact precursor ion at a -28-charge state (695.40 m/z).	86
Table S2: Regression Equation and Calibration Curve Report of Antisense FLuc-S1 dsRNA construct: MRM scans were used to perform quantification monitoring the negative CAD product ion of adenine (134.0470 m/z) from the antisense FLuc-S1 dsRNA constructs intact precursor ion at a -11-charge state (786.55 m/z).....	87

Abstract

ABSOLUTE QUANTIFICATION AND IDENTIFICATION OF RNA FROM RNA-LIPID NANOPARTICLES USING HIGH RESOLUTION MASS SPECTROMETRY

By Jason C. Funderburk, M.S.

A Thesis submitted in partial fulfillment of the requirements for the degree of Master of Science,
Pharmaceutical Sciences at Virginia Commonwealth University

Virginia Commonwealth University, 2026.

Directors:

Matthew S. Halquist, PhD
Sandro R. P. da Rocha, PhD
Department of Pharmaceutics

RNA therapeutics are a rising field of drugs with potential use for a range of conditions encompassing infectious disease immunization to therapies for cancer, diseases, and genetic disorders. RNA-lipid nanoparticles (RNA-LNPs) are the prominent delivery method for these therapeutics notable approved products include mRNA vaccines and polyneuropathy treatments. The emergency use authorizations and orphan drug status of current RNA-LNP and RNA-based drugs has allowed for their approval before finalization of regulatory developed analytical guidelines for the quality monitoring of identified critical quality attributes (CQAs). The development of mass spectrometry (MS) based approaches for characterization of RNA drug substance (DS) and critical excipients from RNA-LNPs drug products (DP) is critical for deeper assessment of quality and performance for these RNA-based drugs, from the complex nature of their stability stemming from the concurrent properties of high physiochemical instability and large biologic size. Despite recent advances in bottom-up and top-down MS RNA approach and high-resolution mass spectrometry (HRMS) capabilities, there is still a significant unmet need in development of multiple encompassing assays to monitor the many DS, DP, and critical excipient

identified CQAs. Our study aims to develop a liquid chromatography mass spectrometry (LC-MS) assay to characterize intact RNA extracted from RNA-LNPs, recognizing that RNA-based drugs is essential and growing role in disease treatment, and the potential to improve quality monitoring methods for this range of drugs.

We initiated our study by selecting a therapeutically relevant single and double-stranded RNA-construct with a benchmark LNP formulation and formulated at a desired quality target product profile (QTPP) consistent with DPs at a nitrogen to phosphorus ratio (N:P) of 6. We optimized the selected RNA extraction technique for LC-MS analysis. We systematically screened a range of LC-MS conditions to find the optimal settings for RNA identification and quantification and investigated the capability to simultaneously measure both CQAs of both extracted intact RNA constructs with MRM^{hr} scans. The range of the LC-MS quantification assay was investigated for both RNA constructs. The LC-MS quantification results of the single-stranded RNA constructs were compared for a significant difference from the concentration measured with the standardized fluorescent assay from the RNA-LNP QTPP characterization procedures.

We demonstrated simultaneous identification and absolute quantification of intact single and double-stranded RNA constructs extracted from RNA-LNPs were successfully performed with LC-MS, and quantification was validated in accordance with ICH m10 guidance. To further compare the quantification results, the mean single-stranded RNA concentration measurements from both techniques were compared with no significant difference found. Moreover, we showcased characterization of double-stranded RNA constructs demonstrating the ability to characterize more than single-stranded oligonucleotide constructs with this LC-MS assay approach.

This investigation showcases the usefulness of LC-HRMS as a simultaneous identity and

concentration quality monitoring tool for intact RNA extracted from RNA-LNPs, laying the framework for further efforts to expand CQAs monitored by this approach. This LC-MS assay, notably enhances quality and performance monitoring for RNA-LNPs, representing a promising strategy for MS-based characterization approaches for RNA-based drug products.

Chapter 1: Literature Review

Mass Spectrometry Based Characterization of RNA Encapsulated Lipid Nanoparticles: Current Approaches and Future Potential

1. RNA Based Therapeutics

RNA therapeutics first large-scale success was during the introduction of the two messenger RNA (mRNA) COVID-19 vaccines in 2020 from Pfizer-BioNTech and Moderna with both vaccine's rapid development and production of billions of doses being successfully delivered¹⁻⁵. Despite the common perception of RNA therapeutics as a brand-new technology, research in the field has been ongoing for more than 45 years with the first therapeutic demonstration in 1978^{1,6}. The first therapeutic demonstration used an antisense oligonucleotide (ASO) to target the promotor of Rous sarcoma virus (RSV) RNA to inhibit viral replication^{1,6}. The first therapeutic RNA, an ASO for the treatment of cytomegalovirus retinitis, was approved by the Food and Drug Administration (FDA) in 1998^{1,7}. Another landmark in RNA science was the expression of exogenous mRNA, which was successfully demonstrated in mice for the first time in 1990, following vaccines for cancer, infectious disease and diabetes treatments which were tested in mice during the 1990s¹⁻⁵. The first clinical trials for mRNA therapeutics were for cancer and infectious disease vaccines in 2008 for metastatic melanoma and in 2013 for rabies virus^{1,3,5}. The next breakthrough in the field was RNA interference (RNAi), which was demonstrated in 1998 through administration of ASOs and sense oligonucleotides leading to targeted inhibition of endogenous mRNA in *Caenorhabditis elegans* embryos^{1,8}. In 2018 the first RNAi therapy Patirisan (Onpattro) was approved by the FDA for the treatment of polyneuropathy caused by hereditary Transthyretin-mediated (TTR)-mediated amyloidosis^{1,2,9}.

The wide range of conditions RNA therapeutics can be applied for include infectious disease immunization, and therapies for cancer, diseases, and genetic disorders^{2-5,9}. The three

mechanisms of RNA therapeutics are RNAi, in-situ expression of antigen/protein, and disease pathway receptor/signal transduction^{2,9,10}. The RNAi nucleic acid modalities are small interfering RNA (siRNA), microRNA (miRNA), and ASOs^{2,9}. The RNAi modalities inhibit expression or promote degradation of a targeted mRNA sequence preventing endogenous expression of mRNA^{2,9}. The nucleic acid modalities that amplify/express in-situ protein/antigen are mRNA, self-activating RNA (saRNA), self-amplifying mRNA (smRNA), and splicing modulating ASOs^{2,9-11}. These nucleic acid modalities amplify protein production by pre-mRNA correction or delivery of a protein/antigen producing RNA sequence^{2,9}. RNA aptamers are nucleic acid modalities that use their tertiary structure to bind and interfere with the receptor/signal pathway of a disease². The therapeutic mechanism of RNA aptamers is unique because it does not utilize the typical biological function of oligonucleotides for therapeutic action^{2,12}. The first FDA approved RNA aptamer drug was in 2004, pegaptanib (Macugen) a 27 base-pair (bp) RNA sequence that inhibits VEGF for the treatment of wet neovascular age-related macular degeneration (AMD)^{2,12}. Recently in 2023 the second RNA aptamer drug was approved by the FDA avacincaptad pegol (Izervay) for the treatment of geographic atrophy (GA) an advanced stage of AMD¹². There is a large range of sizes for therapeutic RNA drugs ranging, between 10 to ~12,000 nucleobases, and molar masses ranging from kilodaltons to megadaltons^{2,9,11}. The many therapeutic mechanisms, nucleic acid modalities, and wide range of potential new treatments for many conditions shows the limitless potential for future development of therapeutic RNA.

2. Lipid Nanoparticle Delivered RNA: Overview

The concept of intentional manipulation of materials at nanoscale was first introduced in 1959 by Feynman¹³⁻¹⁵. This concept evolved and was later termed nanotechnology and has created a breakthrough in new capabilities and developments in virtually all fields of technology¹³⁻¹⁵. The

general definition of nanotechnology is that which relies on structures with at least one size in the range from 1 nm to 100 nm, leading to novel biological, chemical, or physical properties unique to nanoscale size¹³⁻¹⁵. Through the concepts of nanotechnology applied to medicine, the nanomedicine field was created and has led to many innovative approaches in the areas of diagnosis, screening, and treatment of disease¹³⁻¹⁵. Despite nanomedicines large scale application to medical technology there still is a lack of a uniform internationally accepted definition, however the European Medicinal Agencies (EMA) and FDA both have issued regulatory documents involving nanomedicine and nanotechnology and both are in general agreement on the definition and purpose of nanomedicine¹⁶⁻¹⁸. The FDA issues industry guidance providing the agencies interpretation of nanomedicine and provide recommendations for regulatory policy¹⁷. The EMA in a scanning report categorizes all currently authorized nanotechnology-based drug products as lipid nanoparticles (LNPs), protein/albumin-bound nanoparticles, inorganic nanoparticles/colloids, nanocrystals, and polymeric nanoparticles^{17,18}.

2.1. Development of Lipid Nanoparticles (LNPs)

Nanoparticles (NPs) have become an increasingly important technology for medical diagnosis and drug delivery^{4,13,14,19}. Medical diagnosis can be enhanced with NPs use in vivo combined with IR or NMR imaging techniques to increase resolution and sensitivity of disease detection¹³. Similarly, NPs can improve the delivery of drugs by increasing circulation and stability of the encapsulated drug (pharmacokinetics (PK) and biodistribution), with potential for organ, cellular and even intracellular targeting^{4,19}. To classify NPs the types can be grouped into three broad classes inorganic, polymeric, and lipid-based^{4,19}. The most investigated inorganic NPs are gold, iron oxide, silica, and quantum dots^{4,19}. Classes of polymeric NPs include dendrimers, nanospheres, polymersomes, and polymer micelles^{4,19}. Lipid-based NPs include liposomes, LNPs,

and nanoemulsions¹⁹. The most abundant nano drug product in the market are lipid-based NPs, with the first approved drug product in this class being Doxil in 1995. Doxil is a liposomal formulation for the delivery of doxorubicin, a chemotherapy for cancer treatment^{19,20}. Doxil provided the benefits of significantly reduced toxicity, increased circulation time, and passive tumor targeting compared to the free doxorubicin drug²⁰. Liposomes can encapsulate and deliver hydrophilic, hydrophobic and lipophilic drugs, with the ability to deliver hydrophilic and lipophilic drugs simultaneously in the same NP¹⁹. In 1977 it was discovered that liposomes could carry mRNA, with the discovery leading to the beginning of research in lipid-based delivery of nucleic acids^{5,19,21,22}.

The first encapsulation and release of an oligonucleotide from NPs was reported in 1976 using polymeric NPs to deliver thymidine-labelled DNA in an artificial matrix^{23,24}. Following the demonstration that liposomes could carry mRNA, in 1978 the first in vitro transfection and expression of liposomal mRNA with the sequence for globulin protein was demonstrated^{22,24}. The first attempts at liposomal delivery of nucleic acids used liposomes composed of cholesterol, phosphatidylcholine, phosphatidylserine (**Figure 1.1A**) and were formulated using the ether vaporization method^{22,25}. The early liposomes successfully delivered mRNA and DNA in vitro but suffered from low RNA loading, non-scalability, and poor transfection efficiency²². It was first theorized in 1987 that the addition of a positively charged lipid to liposomes could increase loading of negatively charged nucleic acids, and this led to the development of cationic lipids N-[1-(2,3-Dioleoyloxy)propyl]-N,N,N-trimethylammonium (DOTMA) and 1,2-dioleoyl-3-trimethylammonium-propane (DOTAP)^{22,24}. Cationic Lipids were combined with helper lipids and nucleic acids to form lipoplexes (**Figure 1.1B**)^{22,24}. Lipoplexes can take two major forms the non-bilayer stacked hexagonal (H_{II}) phase with aqueous cores or the membrane bilayer phase with

aqueous vesicles, the former phase favors encapsulation and delivery of nucleic acids^{22,26}. The helper lipid mixed with cationic lipid influences which phase the lipoplex would take, 1,2-Dioleoyl-sn-glycero-3-phosphoethanolamine (DOPE) lipoplexes formed the H_{II} phase and 1,2-Distearoyl-sn-glycero-3-phosphocholine (DSPC) lipoplexes formed the membrane bilayer phase^{22,26}. In 1994 it was discovered that inclusion of the ionizable lipid 1,2-dioleoyl-3-dimethylammonium-propane (DODAP) would result lipid asymmetry and facilitate membrane fusion in response to changes at biological pH gradients, which enhanced cytosolic release and reduces mRNA degradation in the lysosomal compartment as they are trafficked inside the cell²². In 1999, stabilized plasmid lipid particles (SPLP) (**Figure 1.1C**) were developed to create a nucleic acid delivery system with longer circulation times required for certain diseases due to cationic lipid-based systems rapid clearance^{22,27}. The SPLP was composed of cationic lipid, phospholipid, sterol lipid, and PEG lipid, instead of replacing the cationic lipid the solution was to use smaller amounts (6 mol%)^{22,27}. The SPLP demonstrated that incorporation of shorter chain PEG lipids significantly increased circulation time and reduced toxicity for nucleic acid delivery systems, but was ultimately unsuccessful due to an unscalable formulation process^{22,27}. These key developments in oligonucleotide delivery were all necessary for the realization of LNPs for RNA delivery. By 2010, lipid-based formulations containing ionizable lipids, phospholipids, sterol lipids, and polyethylene glycol (PEG)-functionalized lipids (PEG-lipids) became universally recognized as LNPs (**Figure 1.2**)²².

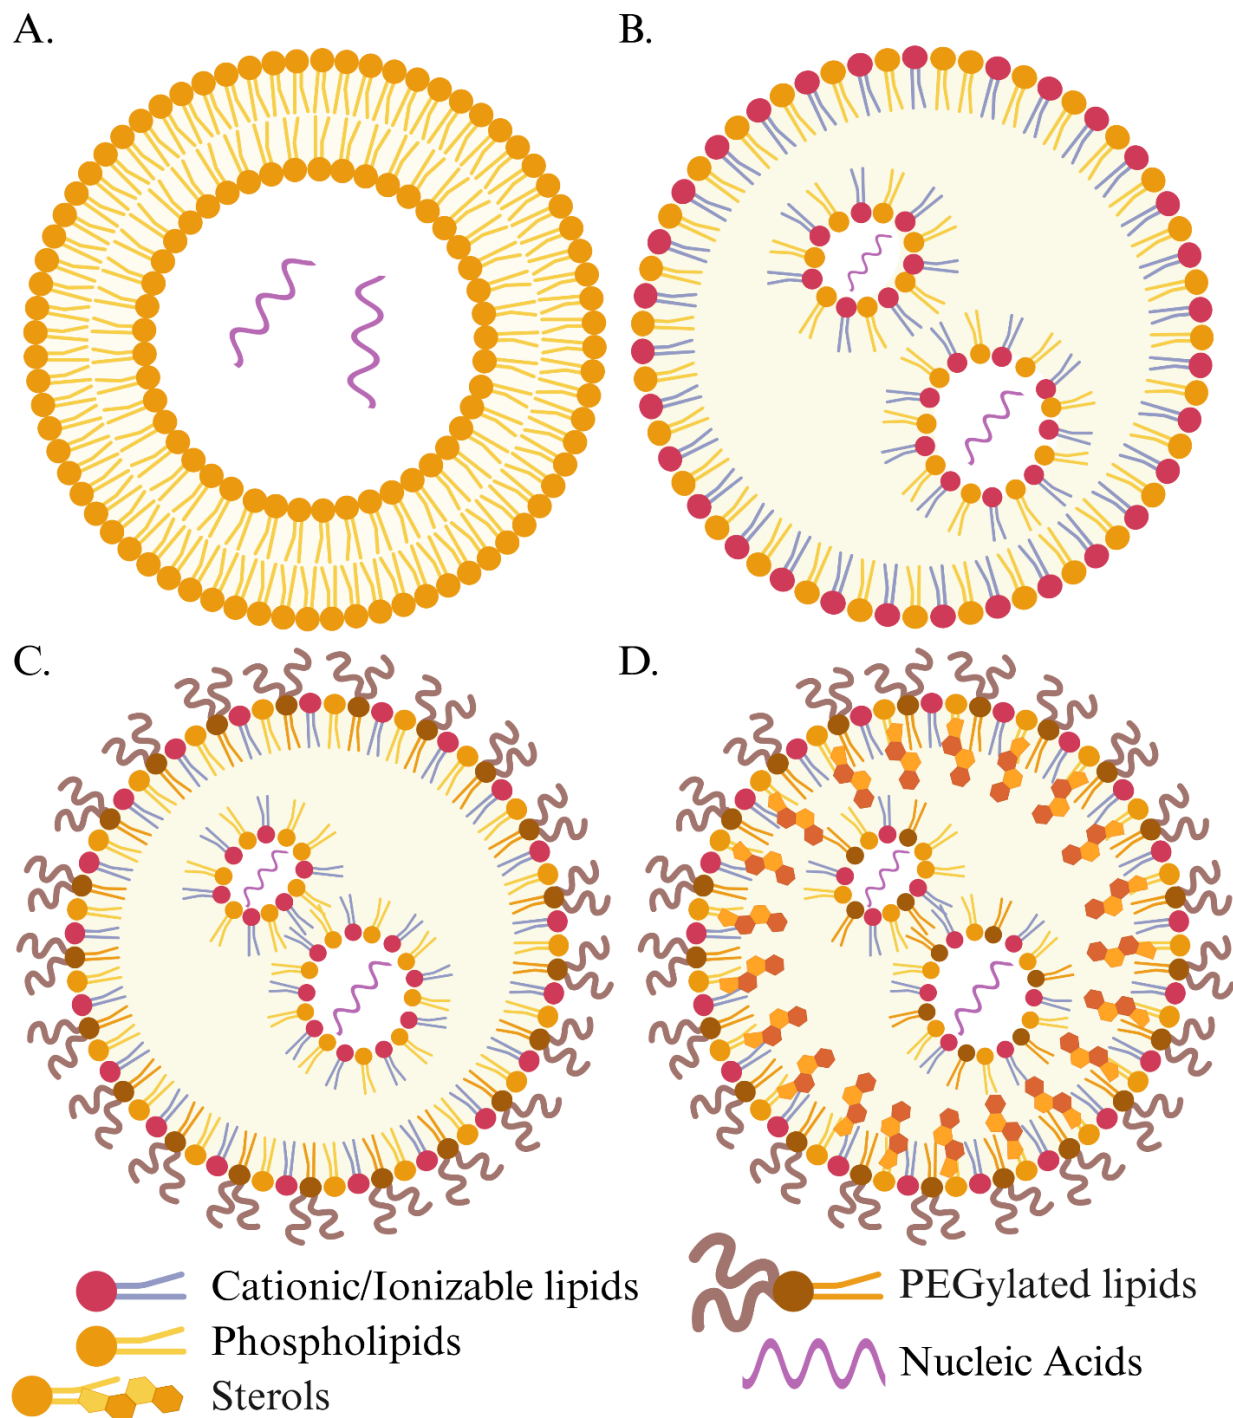


Figure 1.1: Illustration of the evolution of liposome (A), lipoplex (B), SPLP (C) to LNP (D) for nucleic acid delivery. Created with BioRender.com.

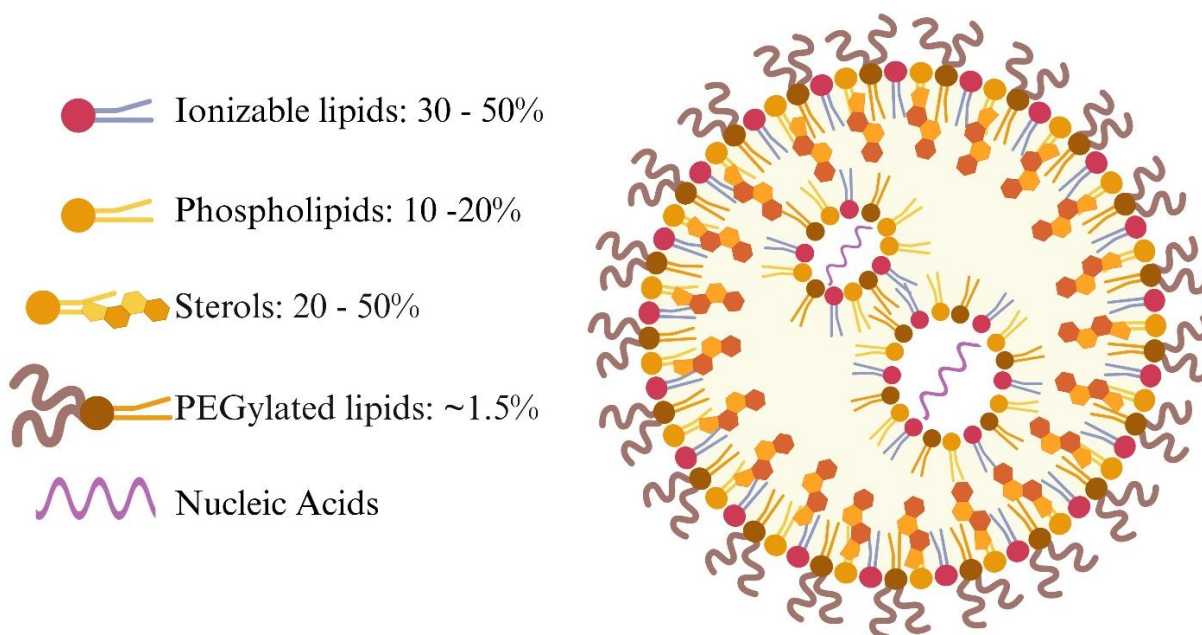


Figure 1.2: Simplistic illustration of LNP structure and components with typical lipid compositions. Created with BioRender.com.

2.2. Ionizable Lipids

Ionizable lipids are a crucial element in LNPs due to their pH-dependent ionization state^{24,26,28,29}. The lipids are designed to become positively charged at acidic pH and neutrally charged at physiological pH^{24,26,28,29}. This property has a key role in both encapsulation during formulation stages and endosomal escape during delivery for oligonucleotides to the cell cytosol^{24,26,28}. The pH-dependent ionizability of these lipids overall results in improved efficacy and safety profiles over cationic lipids²⁶. The ionizable lipids currently in FDA approved products for RNA delivery are Dlin-DMA-MC3 (MC3) for Onpattro (Patisiran®), SM-102 for the Moderna mRNA covid vaccine (mRNA-1273), and ALC-0315 for the Pfizer-BioNTech mRNA covid vaccine (BNT162b2) (**Figure 1.3**)^{26,28,29}. The amount of ionizable lipids in an LNP formulation usually varies between 30% to 50% of all lipids²⁶. Ionizable lipids are commonly classified based on their (1) headgroup, (2) linker, and (3) tail each region, which can be designed to fine tune the

properties of the ionizable lipid^{26,28-30}.

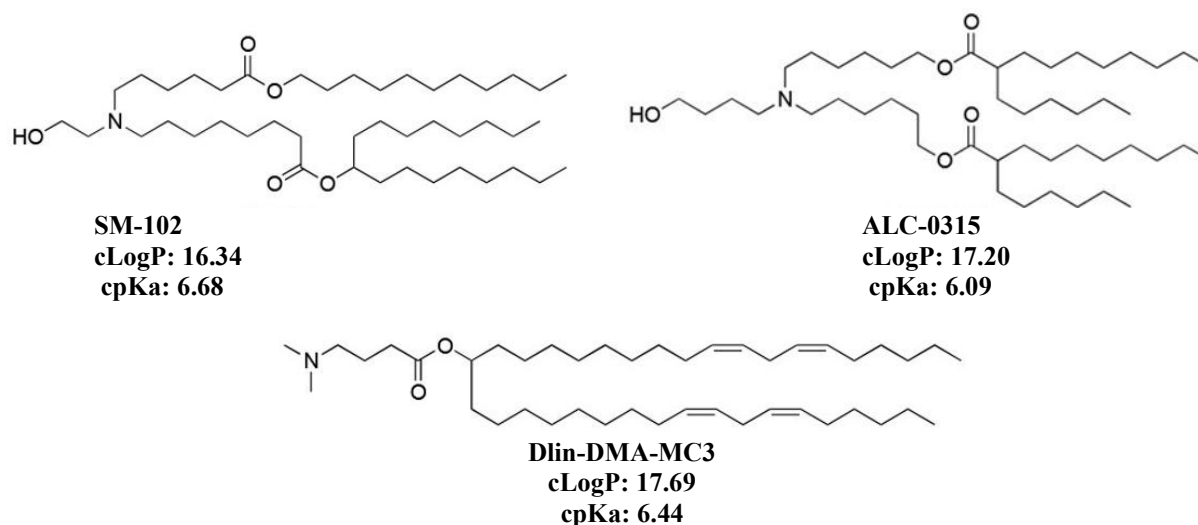


Figure 1.3: Chemical structures, cLogP, and cpKa of the FDA approved ionizable lipids for LNPs. Created with ChewDraw.

The headgroups of ionizable lipids are the region designed to assume a positive charge and exhibit pH-dependent ionization^{26,28,29}. The ionizable group of the headgroup is protonated and has positive charge at acidic pHs, and this is essential to initiate self-assembly through electrostatic forces with the negatively charged phosphodiester bond linking the ribose sugars in mRNA during formulation and endosome disruption during delivery^{26,28,29}. At physiological pH the ionizable group is unprotonated and has neutral charge, which results in improved circulation half-life, efficacy, and toxicity profiles of the LNP delivery system^{26,28,29}. The types of functional groups present in headgroups range from guanidine, heterocyclic compounds, and amines (primary, secondary, tertiary, and quaternary)^{26,28}. The charge density and spatial configuration of the headgroup are essential for LNP performance in oligonucleotide encapsulation, LNP stability, cellular membrane interaction, and endosomal escape^{26,28,29}. The ionizable headgroups in the FDA approved ionizable lipids (MC3, SM-102, ALC-0315) all have a single tertiary amine^{26,28}. The

headgroups of SM-102 and ALC-0315 also contain a hydroxyl alkyl group^{26,28}. The hydroxyl alkyl groups both increase interactions with nucleic acids and the cellular membrane, resulting in improved transfection^{26,28,29}.

The linkers of ionizable lipids role serve to connect the headgroup and tail regions^{26,28,29}. The chosen linker affects safety, stability, and transfection efficiency of the LNP^{26,28,29}. Linkers are classified into biodegradable- (esters, amides, and thiols) and non-biodegradable- containing (ethers and carbamates) groups^{26,30}. The overall charge length and steric hindrance of the linkers affect conformational flexibility of the ionizable lipid²⁹. The linkers of all the FDA approved ionizable lipids are esters with MC3 having one linker and ALC-0135 and SM-102 having two^{26,28,30}.

The tail of the ionizable lipid is the hydrophobic region designed to fine tune the lipophilicity and pKa of the lipid, impacting fluidity and fusogenicity of the LNP, overall influencing the LNP formation and potency^{26,28,29}. Most tail regions of ionizable lipids contain one to four branching tails composed of eight to twenty carbon atom chains that can be saturated or unsaturated^{26,28,29}. The tail regions of the FDA approved ionizable lipids are composed of two linoleyl -tails (MC3) or two branched saturated tails (ALC-0135, SM-102)^{26,29,30}. The spatial configuration of the tails of ALC-0135 and SM-102 creates a cone shaped geometry that increases destabilization of the endosome increasing cytosolic delivery of the nucleic acid^{26,30}.

2.3. Helper Lipids


The other lipids in LNP formulations for oligonucleotide delivery are classified as helper lipids. There are three classes of helper lipids: phospholipids, sterols, and PEGylated lipids^{28,30-34}. The helper lipids increase LNP delivery of nucleic acids by improving circulation stability, internalization, and endosomal escape^{26,28,31-34}. Helper lipids influence LNPs performance with

their lipid structures and the molar ratio in a formulation impacting cellular internalization and protein translation³¹⁻³⁵.


2.3.1. Phospholipids

The purpose of phospholipids in LNP formulations is to act as structural lipids that influence fluidity, stabilize the LNP, and package nucleic acids^{26,31,32,34,35}. Saturated phospholipids (phosphatidylcholine, phosphatidylserine, DSPC) decrease fluidity and have high phase transition temperatures that favor LNP stability^{26,32}. In the typical structure of a LNP the cylindrical-shaped phospholipids (phosphatidylcholine, phosphatidylserine, DSPC, DOPC) are mostly located in the outer membrane of the LNP^{26,32}. The unsaturated phospholipids (DOPC, DOPE) increase fluidity increasing fusogenicity of the LNP^{35,36}. Inverted cone-shaped phospholipids (DOPE) help package and deliver nucleic acids by favoring the H_{II} phase^{26,32,34,35}. The most common phospholipids used in LNP formulations are DSPC and DOPE with FDA approved LNP systems only containing DSPC (**Figure 1.4**)^{26,34}. The addition of an H_{II} phase forming helper lipid is not required for FDA approved LNP systems because the approved ionizable lipids (MC3, ALC-0135, SM-102) favor the formation H_{II} phase³⁴. Phospholipids typically consist of 10% to 20% of the total lipids in LNP formulations²⁶.

Phospholipids:

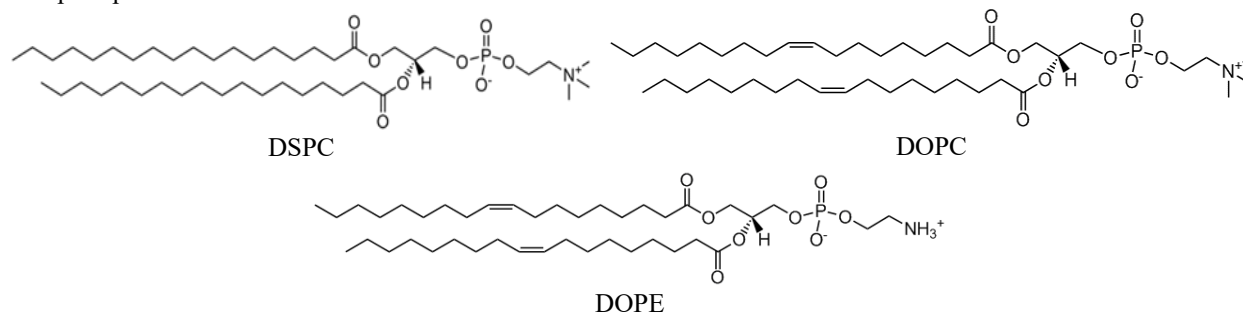

Sterol Lipids:

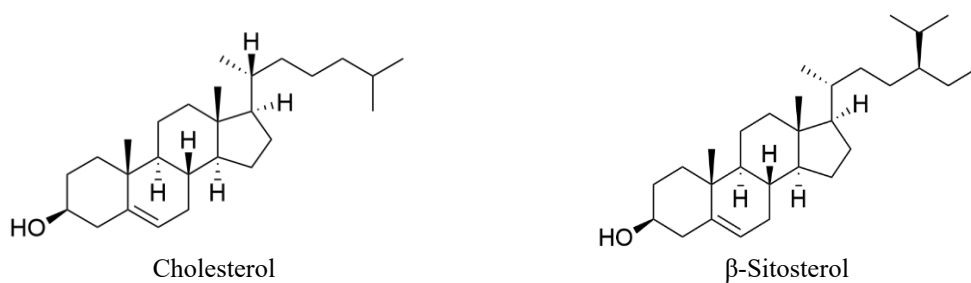

PEGylated Lipids:

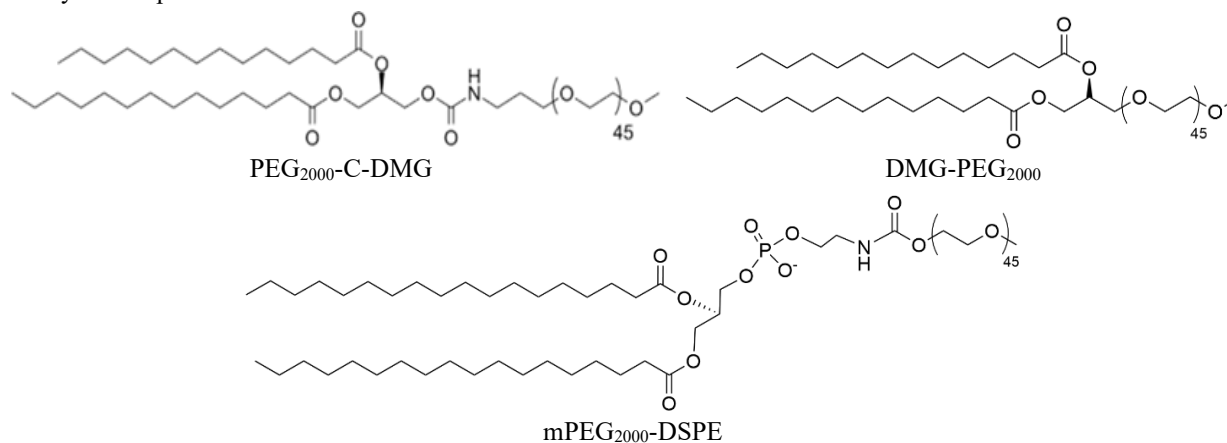


Figure 1.4: Examples of helper lipids in LNP formulations. Created with ChewDraw.

2.3.2. Sterol Lipids

Sterol lipids are structural lipids that fill the gaps between phospholipids in the hydrophobic section of LNPs³¹. The role of sterol lipids is to increase LNP stability and promote fusogenicity^{26,31,34}. LNP stability is increased with the addition of sterol lipids through stabilization

of the lipid bilayer, reduced serum protein opsonization, and lowered nucleic acid leakage^{31,34}. Sterol lipids can promote membrane fusion by influencing the fluidity of LNPs^{31,34}. Sterol Lipids are a class of lipids that contain four fused cyclic carbon rings with a hydroxyl group^{26,37}. The most common used sterol lipids are naturally occurring cholesterol and the phytosterol β -sitosterol (**Figure 1.4**)^{26,37}. Animal cellular membranes contain cholesterol and use it as vital component and precursor for synthesis³⁷. Current FDA approved LNP formulations all use cholesterol as the sterol lipid³⁴. In LNP formulations these lipids typically consist of 20% to 50% of all the lipids²⁶.

2.3.3. PEG-Lipids

PEG-lipids are the structural lipids that use PEG chains to form the hydrophilic outer shell of LNPs^{26,37}. PEG-lipids and PEG functionalized (PEGylated) lipids are included in this category^{26,34,37}. The role of PEG-lipids in LNPs are to influence size, stability, distribution, and transfection efficiency^{26,31,33,34,37,38}. The inclusion of PEG-lipids leads to LNPs with homogenous size. Increasing the amount of PEG-lipids lipids generally leads to smaller particle sizes^{33,34,38}. The presence of the PEGylated lipids also increases colloidal stability in vivo, by decreasing serum-protein opsonization^{26,31,33}. PEG-lipids affect distribution by increasing the circulation half-life and the potential for organ/tissue passive targeting due to particle size or active targeting by incorporation of targeting moieties^{34,37}. The amount of PEG-lipids can influence transfection efficiency by increasing the uptake of LNPs, but can make membrane disruption less efficient during delivery both due to increased stability^{34,37}. The most common PEGylated lipid used in LNP and liposomal formulations is mPEG₂₀₀₀-DSPE (**Figure 1.4**)³⁴. The PEG-lipids used in FDA approved LNP formulations are PEG₂₀₀₀-C-DMG for Onpattro and DMG-PEG₂₀₀₀ for the mRNA-1273 and BNT162b2 COVID-19 vaccines (**Figure 1.4**)^{34,37}. The shared components of the PEGylated lipids used in approved LNP formulations are the hydrophilic mPEG₂₀₀₀ chains and

two hydrophobic alkyl chains 14 carbons in length³⁷. The molecular weight of PEG and length of the alkyl chain affect the size and membrane fusion performance of LNPs, and these chemical structures can be designed to influence these characteristics³⁷. The amount of PEG-lipids and PEGylated lipids in LNP formulations is the smallest component, usually around ~1.5% of all the lipids^{26,34}.

2.4. Formulation of Lipid Nanoparticles

LNPs for nucleic acid delivery can be produced using a variety of methods classified as conventional and microfluidic mixing methods. Regardless of the manufacturing strategy, the formation of LNPs relies on the electrostatic association between the anionic nucleic acids and ionized lipids, followed by LNP structure formation via hydrophobic and van der Waals interactions with the helper lipid components^{26,39,40}. The conventional methods include: nanoprecipitation, single/double/nonsolvent emulsification, thin film hydration, and the ethanol injection methods^{39,40}. The microfluidic mixing methods are considered advanced forms of the ethanol injection method include: microchannel chip-based platforms, microfluidic hydrodynamic focusing (MHF), and staggered herringbone mixer (SHM), bifurcating mixer, and impingement jet mixer (IJM) methods^{39,40}. The manufacture method selected for an LNP formulation directly influences their quality attributes (QAs) including their physicochemical properties, drug loading efficiency, and stability⁴⁰.

An additional important consideration in the design of a LNP formulation is the ratio of elemental nitrogen to phosphate (N/P ratio)^{39,41}. The N/P ratio expresses the charge interaction between the cationic ionizable amino group on the ionizable lipid and the anionic phosphate backbone of nucleic acids^{39,41}. This interaction is the basis of the complexation of nucleic with ionizable lipids³⁹. A higher N/P ratio results in increased encapsulation efficiency and increased

LNP surface charge, but overall decreases LNP potency due to increased LNP protonation resistance during endosomal escape⁴¹. LNPs with lower N/P ratios have decreased surface charge and increased off target expression⁴¹. The structural dynamics of LNPs have been shown to be affected by the N/P ratio and pH during formulation⁴¹. The N/P ratios of FDA approved LNPs for RNA are 3 (Onpattro) and 6 (mRNA-1273, BNT162b2)^{39,42}.

2.4.1. Conventional Formulation Methods

The conventional formulation methods are used for small-scale laboratory and industrial production of LNPs^{39,40}. All these methods share the common steps of dissolving lipids in the organic phase and nucleic acids in the aqueous phase with mixing followed by size reduction techniques^{39,40}. The nanoprecipitation method uses precipitation as the LNP formulation mechanism involves mixing an organic phase containing the lipids with an aqueous phase containing nucleic acids without specialized mixing (magnetic stirring), followed by a method to reduce the amount organic solvent and/or particle size (dialysis, freeze-drying, rotary evaporation, or ultracentrifugation)⁴⁰. The single emulsification method is used for encapsulation of hydrophobic payloads, the double emulsification method for hydrophilic payloads, and nonsolvent emulsification method for avoidance of organic solvents^{40,43,44}. The single/double emulsification method formulated LNPs using an oil-in-water (w/o) emulsion or water-in-oil-in-water (w/o/w) emulsion, followed by an organic solvent reduction and extrusion method⁴⁰. The emulsification methods are not commonly used for nucleic acid encapsulated LNPs, they were developed for the delivery of multiple chemically diverse drugs, peptide-based biologics, and low-energy manufacturing, but this method offers the unique advantage of not requiring the use of toxic organic solvents^{40,43,44}. The thin film hydration method involves dissolving the lipids in an organic solvent followed by removal of the organic solvent in vacuum forming a homogenous lipid film

within the vessel, the film is then rehydrated with aqueous solution containing nucleic acids resulting in the formation of heterogenous sized LNPs^{39,40,43}. After rehydration the particles undergo multiple size reduction steps including extrusion, high-pressure homogenization, or sonication to achieve smaller, more homogeneous LNP size distribution^{39,40,43}. The thin film hydration method offers the formulation advantages of small risk of contamination, low energy requirements, but increases the potential to produce heterogenous sized particles^{39,40,43}. The ethanol (solvent) injection method involves dissolving the nucleic acids in an aqueous phase and lipids into an organic phase rapidly injecting small amounts of one phase into the other under stirring, followed by purification^{39,40,43,45}. The advantages of the method include the ability to produce smaller particles than other conventional methods with identical formulations, method simplicity, and rapid production^{39,45}. Drawbacks of the ethanol injection method include low scalability, reproducibility, and larger contamination risks^{39,45}. Ethanol injection method was first described as an improved thin-film hydration method, improved versions of ethanol injection include methods described as cross-flow and modified ethanol injection method^{39,46,47}.

2.4.2. Microfluidic Mixing Methods

The microfluidic mixing methods are used for production of LNPs designed to improve the solvent injection method through precise control of different aspects of the micro-mixing process and with the potential for scalability to large-scale industrial production^{5,26,39,40,47}. Microfluidic microchannel chip-based platforms are the simplest microfluidic mixing method utilizing in-line T or Y shaped microchannels to rapidly mix (40-60 ml/min) and produce LNPs at large scale (>100 μ L)^{39,40,47}. The aqueous phase and organic phase are added at the inlets and LNPs form at the liquid interface through diffusion-based organic solvent dilution^{39,40,48}. Microfluidic hydrodynamic focusing (MHF) is an advanced form of microfluidic mixing that relies on passive

mixing to generate laminar flow. The two types of MHF are 2D hydrodynamic flow focusing (HFF) and 3D HFF^{39,40,45}. 2D HFF consists of a chip with 3 inlets with the organic phase injected in the central inlet and aqueous in the outer two inlets with the flow of both phases perpendicular at the interface where LNP formation occurs^{39,40}. 3D HFF consists of a multicapillary-arrayed device with seven inlets that combine at the interface with the organic phase injected into the central inlet^{39,40}. The advantage of 2D HFF are the production of small particles (<150 nm) with the downside of low-scalability due to low flowrates (<10 mL/min) and low particle size uniformity due to lipid aggregation in the system^{39,40}. The advantage of 3D HFF is the production of uniform sized particles with four-times the throughput of 2D HFF with the disadvantages of complex setup requirements and price of the system³⁹. The staggered herringbone mixing (SHM) method is an advanced microfluidic method named for the asymmetric groove pattern of the microchannel^{39,40}. The groove pattern allows for the disruption of laminar flow creating controlled, chaotic micro-mixing resulting in highly reproducible, homogeneous small LNPs (30 nm) with the downside of low throughput due to flowrates (<100 mL/h)^{39,40}. The bifurcating mixer is a chip platform designed to overcome reproducibility and scalability of other mixers sold under the name NxGenTM mixer from NanoAssemblr^{40,50}. The bifurcating mixer offers the formulation advantages of reproducibility and large scalability through its precise control of chaotic mixing at high flowrates (≤ 200 mL/min)^{40,50}. The impinging jet mixer (IJM) is a method that utilizes the impact of two to four high velocity streams of fluid to create controlled shearing and mixing forces under high pressure^{40,48,51}. This mixer can change the properties of the produced LNPs by adjusting the flowrate and pressure mixing parameters, the design facilitates the translation of small-scale to large-scale production of LNPs^{40,48,51}. The advantages of all the microfluidic methods over the conventional methods for LNP production are the enhanced control of physicochemical properties,

improved encapsulation efficiencies, and improved scalability³⁹. An important aspect of LNP formulation design is that they can be optimized to a specific micro-mixing method, or a method is selected to achieve desired formulation outcomes. Microfluidic methods are used for industrial production of Onpattro and the mRNA-1273 vaccine and IJM systems developed by Knauer are used to manufacture the BNT162b2 vaccine^{40,49,51}.

2.5. Advantages of LNP for Nucleic Acid Delivery

The greatest challenge in the field of therapeutic nucleic acids is its delivery to the cell cytosol^{4,5,26,39,52,53}. Delivery of individual, naked oligonucleotides is possible, but expression is extremely inefficient and higher doses result in increased immunogenic response in vivo^{26,52,53}. The greatest challenges faced in nucleic acid delivery are degradation of the payload and challenges in crossing the cellular membrane due to its (large) size and (negative) surface charge^{26,42,52,53}. The main degradation forces nucleic acids experience are environmental from inherent high instability and endogenous immune responses, a single break in the sequence can result in a non-expressible sequence^{26,42,52,53}. Various methods have been developed for the delivery of nucleic acids and can broadly be classified as viral and non-viral delivery systems both are used in vivo and in vitro^{4,5,19,52,53}. The viral delivery system mechanism uses contemporary viruses (adenoviruses, adeno-associated viruses, lentiviruses, and Sendai virus) as viral vectors with the viral genetic material replaced with a therapeutic nucleic acid sequence^{4,5,19,39}. Viral delivery systems are not commonly used outside research settings due to their high manufacturing costs, small payload capacity, and large potential for biosafety issues^{4,5,19,39}. The non-viral delivery systems are classified into two additional groups mechanical and nucleic acids encapsulated in lipid or various polymeric NP delivery systems^{4,52,53}. The mechanical delivery systems include electroporation, high-pressure injection, gene guns, and ultrasound⁵³. Nucleic acid carrying NPs

consist of lipid-based vectors, polymer-based vectors, hybrid vectors, and inorganic nanoparticle-based delivery vectors^{4,5,52,53}.

LNPs are categorized under lipid-based vectors, and are the most successful, commonly used delivery platform for therapeutic RNA^{52,53}. Since LNPs are the most accepted system for RNA delivery, currently most research in formulation development focusses on the main four areas of LNP lipid content optimization, LNP surface targeting modification, co-delivery of oligonucleotides/drugs, and the developments of new NPs^{4,5,53,54}. LNP lipid content research focuses on optimization of the lipids through chemical structure modification or formulation contents to improve encapsulation, stability, and targeting^{4,5,53}. LNP surface targeting research focuses on the development of targeting moieties for receptor-mediated endocytosis mechanism to enhance LNP uptake in targeted cell populations^{4,5,53,54}. Research in co-delivery focuses on LNP delivery of more than one nucleic acid sequence or biologic/drug as a treatment strategies^{5,53,54}. The development of NPs focuses on new nanomaterials, NPs, and methods to formulate NPs⁵.

3. Stability of RNA Therapeutics

One of the greatest challenges in the therapeutic nucleic acid field is the high inherent instability property of oligonucleotides due to high rates of chemical degradation and physical instability requiring special storage conditions, overall, negatively affecting shelf-life and translation efficiency^{26,42,43,55-62}. Chemical degradation occurs when modifications on the oligonucleotide structure occur via bond formation or cleavage primarily through the mechanisms of hydrolysis and oxidation, as both can lead to strand breaks^{42,61-63}. Hydrolysis mainly affects the structural backbone phosphodiester bonds and the *N*-glycosidic bonds of nucleic acids^{42,61-63}. The common sources hydrolytic degradation reactions occur from are acid/base-catalysis, the presence

of metal cations, thermal induction, and nucleophilic attack from other nucleic acids, water, or other nucleophiles present in solution^{42,61-63}. Oxidation of nucleic acids occurs mainly from reactions with reactive oxygen species (ROS) which are formed from decomposition of peroxides, ionizing radiation, metal-catalyzed reduction of oxygen, and photolysis^{42,61-63}. The common ROS species include hydroxyl radicals, peroxides, and singlet oxygen species^{42,62,63}. Each individual reaction between a ROS and a nucleobase can yield a unique reaction with a distinct mechanism dependent on the ROS species, pH, nucleobases, and solution composition, but nucleobases containing purine and pyrimidine structures are most susceptible to oxidation^{62,63}. The results from any chemical degradation can alter the higher order of the overall oligonucleotides structure is referred to as physical instability^{42,60-63}.

One strategy to increase physical stability of nucleic acids is to decrease the structures predisposition to chemical and enzymatic degradation through sequence and structure design^{9,42,53,62,63}. The structure of nucleic acids determines its ability for molecular interactions, which greatly impacts RNA inherent stability. The main structural stability factors include: single/double-stranded, the nucleobase content (DNA, RNA, and modified), the structural configuration, and the length or size in nucleobases^{9,42,53,56,57,60-63}. Single-stranded nucleic acids are significantly less stable than double-stranded for both DNA and RNA^{58,62,64}. Modified nucleobases are the most stable followed by DNA nucleobases with RNA nucleobases being the least stable^{9,42,53,62}. The higher chemical instability of RNA compared to DNA stems mainly from the additional hydroxyl group in the 2'-ribose position, resulting in the phosphodiester bond between DNA nucleobases being around 200 times stronger than a similar RNA counterpart^{61,62}. Chemical modifications to increase stability and functionality of nucleotides are placed on the base, the phosphate backbone, and the ribose moieties^{9,62}. The mRNA-1273 and BNT162b2

vaccines both use N1-methylpseudouridine, and Onpattro uses methylation and fluorination chemical modifications on the 2'-ribose position of select nucleotides^{9,53,62}. The purpose of the methylation modification in all three approved RNA-LNP products is to block the interaction with ribonucleases reducing enzymatic hydrolytic degradation^{9,53,62}. The ribose fluorination chemical modification in Onpattro makes the siRNA less susceptible to enzymatic and chemically induced hydrolysis, through blocking ribonuclease interaction and creating a stabilizing electronic effect on the entire structure, increasing physiochemical stability^{9,62}. The structural configuration can be manipulated at the primary, secondary, and tertiary level to increase nucleic acid stability^{42,53,56,61,62,64,65}. The primary structure is the sequence of nucleotide monomers and stability modifications include nucleotide chemical modifications and control over the nucleic acid sequence^{61,62,64}. The secondary structure consists of the two-dimensional nucleotide sequence configuration that forms the foundation of the three-dimensional oligonucleotide structure^{61,62,65}. The function of nucleic acids are derived from their secondary structures, but secondary structures can also be exploited to enhance stability^{62,65}. Secondary structures of RNA can both increase or decrease physiochemical stability through various interactions that maintain biochemical processes. These structures include bulged loop, hairpin loop, H-type pseudoknot, internal loop, kissing hairpin pseudoknot, multi loop, and stacks^{62,65}. The tertiary structure of nucleic acids is the three-dimensional arrangement formed by interactions between nucleotide bases, the phosphodiester chains, and ions that are recognized by proteins, ligands, and other oligonucleotides^{62,66}. The tertiary structural elements significantly impact stability common structures include helical duplexes, loops, quadruplex groups, triple-stranded structures, and trunks^{62,66}. The length of the nucleic acid sequence drastically affects stability with a negative correlation between increasing length and stability^{42,57,62}. The increasing instability with RNA

length is thought to originate from the increase in putative sites for physiochemical degradation occurrence⁵⁷. The inherent stability of RNA from the sequence configuration is a huge consideration when developing a therapeutic oligonucleotide for a drug product^{9,42,53}.

Another major degradation pathway of nucleic acids is nuclease catalyzed cleavage^{56,62,67-72}. Nucleases are an integral part of biological processes and are classified as endonucleases or exonucleases, deoxyribonucleases (DNase) or ribonucleases (RNase), topoisomerases, recombinases, ribozymes, or RNA splicing enzymes^{67,68,70,71}. Nucleases are a very diverse group of proteins and are commonly classified into superfamilies based on substrate preference, cleavage mechanism, and evolutionary relationship^{67,68,70}. Common ribonucleases that oligonucleotides are modified to inhibit cleavage include ribonucleases A, H, P, T1, and T2^{56,62,72,73}. Alternatively, certain approved oligonucleotide therapeutics can rely on the recruitment of specific ribonucleases to fulfil their targeting mechanism for therapeutic action, with approved products using guide oligonucleotides recruit RNase H or AGO2^{9,69}. The three approved products that recruit RNase H to silence mRNA associated with the intended disease reducing the production of harmful proteins as a treatment include Inotersen (Tegsedi), Volanesorsen (Waylivra), and Tofersen (Qalsody)^{9,69}. The six approved siRNA products that recruit RNase AGO2 to cleave the double stranded include Onpattro, Givosiran (Givlaari), Lumasiran (Oxlumo), Inclisiran (Leqvio), Vutrisiran (Amvuttra), and Nedosiran (Rivfloza)^{9,69}. Among all the current approved RNase recruiting oligonucleotides drug products Onpattro is the only product that utilizes LNPs⁶⁹. The ability for specific or various RNase to recognize substrate sites on an RNA sequence greatly impacts the stability and function of the sequence^{9,64,69}.

Lipid-based encapsulating drug delivery systems were not solely developed for efficient delivery of nucleic acids. Other benefits include improved in vivo and storage stability, but this

introduces physicochemical instability of LNPS as a factor in the system^{42,56,59-63,74}. The three common forms of LNP physical instability that occur during storage are aggregation, fusion and leakage^{42,56,74,75}. LNP aggregation occurs when individual nanoparticles cluster together and fusion occurs when individual nanoparticles lipid membranes merge, both result in larger particle sizes over time⁵⁶. LNP leakage occurs when there is any undesirable release of encapsulated drug, usually during storage⁵⁶. The main mechanism behind the changes in lipid crystalline structure is the transition from high to low energy states and an increasing order of lattice energy^{56,76}. LNP chemical instability occurs primarily when hydrolysis or oxidation occurs on the lipids of the LNP^{56,74}. The common sources of lipid chemical instability in LNP formulations are light, temperature, storage buffer type and pH^{56,63}. The lipids that are most susceptible to chemical degradation contain unsaturated acyl chains⁵⁶. The most common method used to retain LNP stability is frozen storage. During freeze thaw cycle is when LNPs are most susceptible to instability^{42,56,74,75}. The use of PEG-lipids in LNPs improves colloidal and storage stability but its use/mole fraction must be limited to not decrease transfection efficiency⁷⁴. This necessitates the use of other strategies to retain LNP stability, including cryoprotectants and stabilizers that are added to the formulations^{74,75,76}. Sucrose and trehalose are commonly added to LNP formulations as a cryoprotectant and stabilizer to reduce aggregation and fusion^{56,74,75,76}. The lipid composition plays an important role in stability of the LNP but stability data from approved RNA-LNPs indicates the stability of the nucleic acids is the largest factor in the overall stability^{42,60,62}.

Both the mRNA-1273 and BNT162b2 COVID-19 vaccines suffer from high instability and were only successful due to logistics infrastructure developed for RNA therapeutics transportation and storage at subzero temperatures^{26,42,60,63,74}. The reported storage conditions of the two current approved Moderna vaccines (Moderna COVID-19, SPIKEVAX®) is between -50 to -15 °C with

a shelf life of 10 months, 60 days under refrigerated conditions, and 12 hours under room temperature⁷⁷. The storage conditions of the two approved Pfizer vaccines (COMIRNATY®, Pfizer-BioNTech COVID-19) is between -90 to -60 °C with a 18 month stability, under refrigerated conditions the shelf life is 8-months, and 4 hours under room temperature^{78,79}. All the current COVID-19 vaccines cannot be refrozen once thawed and all Pfizer vaccines must be used within 4 hours of opening⁷⁷⁻⁷⁹. The long-term subzero storage requirements for all current mRNA-based COVID-19 vaccines is a large barrier for distribution in less developed regions making vaccine distribution with the current storage control requirements less feasible^{26,42}. Unlike the four approved COVID-19 vaccines, Onpattro is never frozen during storage, under refrigeration the approved shelf life is 3 years, and 14 days under room temperature^{42,80}. Onpattro is more stable in general due to the higher inherent stability of the shorter, double-stranded siRNA cargo, despite using the same or similar lipids as the covid vaccines seen through longer shelf life and refrigerated storage conditions⁴².

LNPs must encapsulate, protect, and deliver active RNA and have the potential for site-specific targeting. Control of these properties has been demonstrated through manipulatable LNP structural factors: encapsulation efficiency (EE%), particle size, PEGylation, surface charge, and targeting ligands modification⁴³. Specific structural factors are critical to the indicated performance of therapeutic RNA drug products^{42,43}. Particle size is a critical structural factor many formulations utilize to enhance uptake in desired site-specific cellular targets^{43,81}. The amount of time and storage conditions an RNA-LNP formulation can maintain desired ranges of the specified structural factors is the general method used to determine stability⁴³. Stability studies on RNA-LNP formulations have demonstrated the advanced nature of formulation stability and the need to monitor all specified structural factors to achieve desired formulation performance^{58,59,63}. Stability

studies of mRNA-LNP stored under nonfrozen conditions (4 to 25 °C) demonstrated the formulations maintained the same size, surface charge, and EE%, but nonfrozen conditions lead to decreasing protein expression^{58,63}. Establishing and monitoring structural factors is critical to RNA-LNP formulation stability since a change in the structural factors or encapsulated cargo degradation overall leads to a loss of function^{43,63}.

4. Current Quality Characterization Methods and Challenges of RNA Lipid Nanoparticle Drugs

Characterization of RNA-LNP formulations is essential for understanding the preparation, stability, and predicted performance of formulations between batches, manufacturers, and any other production variability^{43,82-85}. The performance of RNA-LNP formulations (stability, in vivo distribution, cellular uptake, and protein expression) are impacted significantly by LNP physiochemical structural factors including size, surface charge, and morphology^{43,85}. Currently, multiple published protocols exist for the characterization of RNA-LNP formulations; however, the protocols are all not in agreement with the amount and exact characterization methods for each LNP physiochemical factor. What is agreed is that EE%, particle size, polydispersity index (PDI), zeta potential, and either expression or integrity of extracted RNA are the minimal required characteristics required to be assessed to understand/predict formulation performance^{43,82-86}.

Regulatory agencies classify the critical physiochemical factors that indicate performance of RNA-LNPs as critical quality attributes (CQAs)^{55,85,87,88}. Identified CQAs must be assessed via comprehensive analytical methods performed at each stage of manufacture that ensure a consistent finished drug product^{55,85}. The regulatory framework for RNA-LNP based therapeutics is currently rapidly evolving with each new issue and update of guidelines⁸⁵. The FDA classifies RNA-LNPs under nanotechnology that utilize nanomaterials as active and inactive ingredients including

biologics with two industry guidance documents issued in 2017 and 2022^{17,91}. This broad classification covers many more drug products types than RNA loaded LNPs and recommends general characterization guidance for each manufacture stage^{17,85,91}. In April of 2022, the United States Pharmacopeia (USP) published draft guidelines for the analytical methods for characterization of mRNA vaccines and therapeutics. This document is currently in draft 3rd edition⁸⁷. The EMA published a similar document relating the quality aspects of mRNA vaccines in 2023 with the goal of setting RNA-LNP CQA standards for European Union members⁸⁸. The EMA and USP nearly simultaneously issued guidelines that are in general agreement solely for quality characterization of therapeutic RNA-LNPs; this highlights the importance of quality monitoring for this specific nanotechnology platform for public safety and confidence from rapid widespread adoption. At this time, the regulatory framework categorizes all RNA-based drugs on the basis of the therapeutic indication, either as vaccines for infectious and non-infectious disease or as therapeutic drug product^{87,88,90,91}.

The FDA, EMA, and USP guidelines all recommend characterizing mRNA-LNP vaccine drug products in two different stages of manufacture of the drug substance (DS), and drug product (DP)^{87,88,91}. The DS stage, characterization is performed at two crucial manufacturing steps: the one on the materials used for the production of the RNA construct and at the final RNA product before LNP encapsulation^{87,88}. The CQAs that are recommended to be monitored in the first DS stage align with plasmid DNA QAs in USP Chapter <1040>^{87,88}. The final DS identified CQAs include content, identity, integrity, purity, potency, safety, among others^{87,88}. The qualities content, identity, integrity, and potency only have one corresponding attribute for characterization that is concentration, identity confirmation, intactness, and RNA expression, respectively^{87,88}. The DS quality “purity” has ten identified attributes for characterization: RNA purity, 5’ capping efficiency,

3' poly(A) tail length, two product related impurities, and four process related impurities^{87,88}. The DS quality safety includes endotoxin and bioburden as CQAs and the other category contains appearance, residual solvent, and pH^{87,88}. The DP's CQAs are assessed to ensure the RNA-LNP final product quality. The identified CQAs for DP RNA-LNP with the corresponding analytical methods and relevant regulatory agencies are listed in detail in **Table 1.1**. The USP and EMA are nearly in harmony with mRNA-LNP DP CQAs and analytical methods, the difference being the EMA recommending additional alternative analytical methods, identifying the CQA functionality, and definition of potency^{87,88}. The EMA recommends the CQA potency should be calculated as a score from three DP CQA results (LNP uptake, endosomal escape, and expression) and cell-based assays should measure the additional CQA functionality, while USP recommends cell-based assay for potency characterization^{87,88}.

Table 1.1: Current Recommended Critical Quality Attributes (CQAs) and Analytical Methods for mRNA-LNP Drug Products: The draft quality attributes (QA), and corresponding analytical methods proposed for RNA-LNP drug products, followed by the regulatory agencies that recommend the method for the quality and attribute. QA methods without an established method from USP chapters are still in draft^{87,88}.

Quality	Attribute	Method	Agencies
Identity	mRNA Sequence Identity	Sanger Sequencing	USP, EMA
	Confirmation	Reverse Transcriptase-PCR (RT-PCR)	USP, EMA
	Identity of Lipids	RP-HPLC-CAD	USP, EMA
Content	RNA Concentration / RNA Encapsulation Efficiency	Fluorescence-based Assay	USP, EMA
		AEX-HPLC or SEC-HPLC	EMA
	Lipid Content	RP-HPLC-CAD	USP, EMA
Integrity	LNP Size and Polydispersity	Dynamic Light Scattering (DLS)	USP, EMA
	RNA Size and Integrity	Capillary Gel Electrophoresis (CGE)	USP, EMA
		IP-RP-HPLC	EMA
Purity	Product Related Impurities - Aggregate Quantitation	SEC-HPLC	USP
		RP-HPLC-CAD	EMA
	Product Related Impurities - Percentage of Fragment mRNA	IP-RP-HPLC	USP, EMA
Potency	Expression of Target Protein	Cell-based Assay	USP
	Determination of Potency	Evaluation of Content, Integrity, and Encapsulation Efficiency of RNA	EMA
Functionality	LNP Uptake, Endosomal Escape and Expression	Antigen-specific Cell-based Functionality Assay	EMA
Safety	Endotoxin	USP <85>	USP, EMA
	Sterility	USP <71>	USP, EMA
Other	Appearance	USP <790>	USP, EMA
	Residual Solvents	USP <467>	USP, EMA
	Osmolality	USP <785>	USP, EMA
	Subvisible Particles	USP <787>	USP, EMA
	Extractable Volume	USP <1>, <698>	USP, EMA
	Container Closure Integrity	USP <1207>	USP, EMA
	pH	USP <791>	USP, EMA

RNA loaded LNPs without the indication as a vaccine or that utilize non-coding RNA structures fall into a much grayer area regarding published regulatory framework⁹⁰. The regulatory classification of short length RNA-based drugs without nanoparticle carriers are small molecule drugs or biologics dependent on the synthesis method of the active substance^{90,92}. The only current approved RNA-LNP drug product without vaccine indication is Onpattro^{69,80}. The FDA and EMA

both designated Onpattro as an orphan drug, this allowed for facilitated approval without public disclosure of the CQAs as protected trade secrets^{80,92}. The product quality review and product specific guidance documents for Onpattro from the FDA show the identified DP CQAs are content, identity, physical parameters, and required compendial testing^{80,88}. Onpattro's content and identity DP CQAs require confirmation of the identity, quantification, the ratio of the siRNA duplex to each lipid, with the analytical techniques size exclusion chromatography retention time, melting point, and molecular mass confirmation for the drug substance, and the lipid methods are not disclosed^{80,88}. The DP CQAs physical parameters include EE%, particle size, and in-vitro release without the characterization techniques disclosed^{80,88}. The purity CQAs technique is not disclosed but is used to characterize percentage of the siRNA duplex to total impurities⁸⁰. The required compendial testing DP CQA characterization are appearance, bioburden, elemental impurities, endotoxins, residual solvents, pH, sodium content, and water content the required techniques for these attributes are established⁸⁰. Onpattro's quality attributes and methods are critical providing the initial framework as the first LNP product and represents the sole approved RNA-LNP therapeutic.

The overall evolving regulatory environment and classification of RNA-based drugs is extremely complex and lacks absolute regional harmonization^{85,90}. mRNA-based vaccines are the current RNA-LNP delivery systems with the most harmonized regulatory framework due to widespread forced emergency adoption⁸⁵. The rapid advancement of therapeutic RNA uses, and delivery systems creates the need for regulatory guidelines that encompass a wide-range of RNA-based drugs^{90,93}. There is currently a significant need for the identification and development of CQA methods with complimentary techniques for the active and inactive ingredients of RNA-LNP drugs^{85,93}. The establishment of future robust regulatory guidelines for RNA-LNPs delivery

systems is crucial for ensuring the safety, efficacy, quality, and streamlined development of future LNP-based RNA delivery systems for all indications^{85,93}.

5. Current Mass Spectrometry Approaches for Characterization of RNA-LNP Therapeutics

5.1. Mass Spectrometry

Mass spectrometry is a highly sensitive, rapid, and reproducible analytical technique used for characterization of complex mixtures through measuring the mass to charge (m/z) ratio of ions under vacuum⁹⁴⁻⁹⁷. The basic principle of a mass spectrometer is an instrument composed of the three core components an ion source, mass analyzer, and detector used to ionize, separate, and measure the m/z of gas-phase ions^{94,95,97}. Mass spectrometers output a mass spectrum displaying the measured m/z value on the x axis and the abundance on the y axis^{94,95}. The molecular mass, quantitative, and structural information of the ions can be derived from different mass analyzer ion sorting techniques and the measured m/z values on the outputted mass spectrum⁹⁴⁻⁹⁶. Numerous mass spectrometry related techniques for ionization and instrumentation exist for producing, resolving, and measuring the m/z of ions, creating an assortment of individual mass spectrometer types⁹⁴⁻⁹⁷.

Many different ionization methods have been developed for mass spectrometry over the years to increase the amount and complexity of ionizable compounds⁹⁴⁻⁹⁹. All ionization methods are classified as hard or soft ionization based on the intactness of the generated ion^{95,100,101}. All hard ionization techniques confer excess energy resulting in in-source ion fragmentation resulting in loss of generated ions with the intact molecular mass^{100,101}. The most common hard ionization method is electron impact (EI) ionization often with gas chromatography-MS (GC-MS), and the other commonly utilized hard ionization technique is inductively coupled plasma (ICP) torch¹⁰⁰⁻

¹⁰². EI and ICP ionization are still routinely used because the former allows for highly reproducible identification of volatile, low molecular weight (>1000 Da) compounds from established spectral libraries, and the latter allows for ionization of metalloids compounds¹⁰⁰⁻¹⁰². Soft ionization techniques result in the generation of intact molecular ions with minimal in-source fragmentation^{95,99-101}. Commonly utilized soft ionization techniques operate under ambient conditions making them highly compatible with high performance liquid chromatography (HPLC) and ultra-performance liquid chromatography (UPLC) systems, these include atmospheric pressure chemical ionization (APCI), atmospheric pressure photoionization (APPI), electrospray ionization (ESI), and matrix-assisted laser desorption/ionization (MALDI)¹⁰¹. ESI and MALDI are the most utilized soft ionization techniques for large biological molecule characterization^{94,97-101}.

ESI and MALDI both offer unique advantages when used for ionization of large biological molecules^{94,95,98-101}. Ionization in an ESI mass spectrometer occurs by the injection of a volatile, dilute analyte solution at low flow rates (1-20 $\mu\text{L}/\text{min}$) through a capillary spray needle with high voltage (0.5-6 kV) applied at the tip (<250 μm Internal Diameter (ID)) under ambient pressure conditions^{94,99}. Sheath gas (typically N_2) flows coaxially around the needle to assist nebulization and the solution forms a cone shape at the needle tip releasing the charged droplets⁹⁹. The cone shape formed, famously known as a Taylor cone, occurs from the high voltage difference causing deformation of analyte solutions meniscus towards the direction of the counter electrode⁹⁹. The other side of the ESI chamber contains the counter electrode heated capillary (usually 100-300°C, 0.2 mm ID, and 60 mm length) with an opening called source sampling cone located 1-3 cm from the source needle tip^{94,99}. The combined effects of sheath gas and the heated capillary results in near complete desolvation of ions that enter the mass spectrometer increasing ionization robustness⁹⁹. ESI can generate ions in positive or negative mode dependent on the polarity of the

applied voltage mainly through the mechanisms of protonation/deprotonation^{94,99}. The distinguishing feature of ESI is the ability for soft ionization generating ions with multiple charged states offering numerous unique ionization advantages^{95,98-100}. ESI theoretically appears to have no upper molecular mass limit for ionization due to generation of multiple charged states allowing intact large molecule characterization^{94,95}. The multiple charged states of an identical ion observed in ESI mass spectrum allows for increased mass accuracy from the averaged mass measurement from different charges, and high compatibility with mass deconvolution software^{94,99}. The major disadvantage of ESI is ion suppression creating the need for samples with salt concentrations (generally >1 mM) require desalting to prevent analyte ion suppression⁹⁴. Nanospray is the most common modification of ESI that uses a smaller spray capillary (1-10 μm ID) with a lower flowrate (<100 nL/min) with the purpose of generating smaller droplets (<200 nm diameter) than standard ESI droplets (1-2 μm diameter)^{95,100}. The two main advantages provided by nanospray ionization are increased ionization tolerance to higher aqueous and salt concentrations and slower consumption of sample solution compared to the standard ESI configuration^{99,100}.

MALDI produces ions through pulsed-laser irradiation of a co-crystallized sample matrix that absorbs the emitted wavelength (usually 337 nm) from the laser^{94,95,98}. After the pulsed-laser irradiation gas-phase ions are desorbed from the solid phase and directed into the mass spectrometer^{94,95}. To direct ions into the mass spectrometer the sample matrix is placed on a probe inserted in the vacuum or MALDI ionization can occur under ambient pressure and gas-phase ions are directed into the instrument in a manner similar to ESI^{94,103}. MALDI mass spectrometers that operate under ambient pressure have the highly advantageous ability to readily interchange with ESI¹⁰³. Only single charged gas-phase ions are generated from MALDI this allows for rapid molecular mass confirmation and creates a less complicated mass spectrum^{95,98}. The sensitivity of

MALDI is often greater than ESI allowing detection at sub-femtomole concentrations and has a high tolerance to buffer and salt sample contamination^{94,95}. The main disadvantage of MALDI is high background noise below 500 m/z due to the use of sample matrix and lower compatibility with mass analyzers⁹⁴. ESI and MALDI are both highly important soft ionization techniques for large molecule MS characterization.

Mass analyzer performance is measured by mass measurement accuracy and precision^{94,96}. Mass accuracy is expressed as the root mean square (rms) difference between the measured and theoretical mass and mass precision is derived from the rms error of repeated measurements both expressed in units of parts per million (ppm) or milliDalton (mDa)⁹⁶. The performance of a mass analyzer is most often expressed through mass resolving power⁹⁶. Mass resolution is the minimum mass difference between two peaks power is calculated⁹⁶. High mass resolution is required to resolve different compounds with similar m/z but different elemental compositions^{96,100}. High resolution mass spectrometry (HRMS) is a term used to indicate a mass analyzer with resolving power greater than 10,000, generally quadrupole, triple quadrupole (QQQ), and ion traps mass analyzers cannot achieve HRMS^{96,100}.

The mass analyzer is the mass spectrometer component where ions are separated based on the m/z under vacuum^{94-96,100,104,105}. There are six principal types of mass analyzers commonly utilized and are divided into two categories: magnetic and electrostatic field dependent on the field forces directing ion separation^{94,95}. Mass analyzers are also categorized as beam analyzers or trapping analyzers⁹⁴. Ions are ejected from the source, pass through an analyzing field, and reach a detector in beam analyzers and for trapping analyzers ions are trapped in the analyzing field⁹⁴. Magnetic sectors are the most traditional mass analyzers common between 1950-1980, this beam analyzer disperses ions in magnetic field based on their momentum and focuses ions with similar

momentum through a slit in a process called directional focusing^{94,104}. Electronic sectors are usually paired with magnetic sector mass spectrometers to correct for ion kinetic energy differences, the combination allows for ions with identical m/z and slightly different velocities to be focused to a single point^{94,104}. Magnetic sector analyzers can achieve high resolution ($>10,000$) with a m/z range up to 10,000 when coupled with an electronic sector¹⁰⁴. The other common type of magnetic field mass analyzer is the Fourier-transform ion-cyclotron resonance (FT-ICR)⁹⁴⁻⁹⁶. This analyzer contains ions in a multipole electric ion trap then pulses them to the ICR section, where electrostatic and magnetic fields maintain ion spatial coherence and m/z is measured from the ion cyclotron frequency^{96,105,106}. FT-ICR analyzers have routinely achieved mass resolutions in the hundreds of thousands and resolutions in the millions have been demonstrated, the mass range usually 50 to 20000 m/z ^{94,105,106}. The main advantage of FT-ICR is the extremely high resolving power and mass accuracy that enables resolving complex isobaric mixtures other mass analyzers cannot achieve, and the disadvantage is high operating cost greatly limits application¹⁰⁵⁻¹⁰⁷.

The electrostatic field mass analyzers commonly used include quadrupole, time-of-flight (TOF), ion trap, and orbital ion trap (orbitrap) mass analyzers. Quadrupoles and TOF are beam mass analyzers and the trapping mass analyzers are ion traps and orbitraps⁹⁴. Quadrupoles consist of four cylindrical or hyperbolic parallel rods with a dynamic electric field (radio frequency (RF) and direct current (DC)) that sort and transfer ions in motion based on m/z ^{95,107}. The two modes quadrupole analyzers operate in are ion guide and mass filter mode^{95,107}. Ion guide mode is used to transfer ions over a wide range of m/z using only RF voltage^{95,107}. Mass filter mode is used to select m/z can pass through controlled by applied DC and RF voltage to each opposite pair of electrodes to generate a quadrupole field^{95,107}. The m/z range for is usually less than 4000 and usually achieve unit resolution over the analysis mass range^{94,95}. The most widely used mass

analyzer is the quadrupole the advantages are low cost, small size, and low voltage (2-50 V) requirements⁹⁴. The TOF mass analyzer determines m/z by separating ions based on time to reach the detector^{94-96,107}. Ions are accelerated with a constant kinetic potential, resulting in equally charged ions receiving the same kinetic energy, through the TOF drift tube⁹⁴⁻⁹⁶. Orthogonal TOF mass analyzers have theoretically unlimited mass range but as ion mass increases variability in kinetic energy and spatial distribution rise reducing mass accuracy and resolution, resulting in most analyzers with operating ranges from 10 to 10000 m/z with resolution around 8000^{108,109}. To correct ion energy variability in the TOF drift region electrostatic ion mirrors called reflectrons are added to reflectron and multipass TOF analyzers^{96,110-112}. The reflectron is a spatially quadratic potential region where ions with the same m/z but slightly different velocities travel through are reflected with harmonized velocities^{96,110-112}. The common reflectron TOF drift region geometries are the “V”, “N”, and “W” ion flight trajectories^{96,111}. The reflectron has the other benefit of increased flight path in the TOF drift region, multipass TOF analyzers are designed to maximize the ion flight path distance and are configured in closed and open loop flight paths^{96,107}. Most commercial grade TOF analyzers with dual stage reflectron can reach resolving power greater than 40,000, and commercial grade multipass TOF analyzers can achieve greater than 200,000^{96,110,111}. Reflectron TOF analyzers have restricted m/z range from the reflectron field strength not having enough power to reflect larger m/z ions, usually at 10000 m/z and routinely operate below 5000 m/z , with closed loop multipass TOF have further restricted range from ions with lower m/z overtaking higher m/z ^{96,110}. The ion trap is a mass analyzer like the quadrupole with an electrode system to trap and filters ions with an addition electrostatic field in the perpendicular z direction^{94,95,107}. Unlike the quadrupoles, ion traps use RF voltage to destabilize and trap ions in a mass selective manner^{94,107}. The ion trap offers the advantage of providing true MS^n capabilities,

increased sensitivity at higher m/z , and ease of use (simple structure, small size, low cost, and vacuum requirements)^{94,107}. Commercial grade ion traps have similar m/z ranges and resolution as quadrupoles⁹⁴. The most recently invented (1999) mass analyzer is the orbitrap with commercialization in 2005^{96,113}. The analyzer is composed of a C-trap and orbitrap analyzer. The C-trap is a curved linear electrode that traps ions using RF voltage and ejects ion packets of the same m/z with DC voltage to the analyzer^{96,107,113}. The C-trap can also function as collision cell using high RF voltage^{107,113}. The orbitrap analyzer is three electrodes with two in the shape of a hollow cylinder cut in half perpendicularly and the third central electrode as a parallel rod through the cylinder^{96,113}. The ions that enter the orbitrap analyzer are pushed toward the center and oscillate axially around the central electrode forming ion rings of identical m/z producing image current that is interpreted using FT processing^{96,113}. Commercial grade orbitraps typically have a range of 50 to 8000 m/z and can achieve resolving powers in the hundreds of thousands^{96,113,114}. The orbitrap offers the advantages of ultra-high resolving power over a wide mass range, high-throughput tandem mass analysis, and small analyzer size^{96,113,114}.

The combination of two or more mass analyzers in an instrument is referred to as a tandem mass analyzer^{94-97,107,115}. Tandem mass analyzers increase performance and reduce the disadvantages of an individual mass analyzer, often mass analyzers that correct each other's disadvantages are combined^{107,115}. The principle of tandem mass spectroscopy (MS/MS) is m/z is measured before and after a mass changing reaction within a mass spectrometer, the repetition of this process is referred to as MS^n with n indicating the number of stages^{94,95,115}. The ion that is selected in the first scan is referred to as the parent or precursor ion, the post-reaction charged ions are daughter or product ions, and neutral species^{94,114}. Usually MS/MS reactions increase the ions internal energy resulting in dissociation, collision-induced dissociation (CID) or collision-activated

dissociation (CAD) is the most universal dissociation technique and others include electron-capture dissociation (ECD), electron-transfer dissociation (ETD), surface-induced dissociation (SID), and infrared multiphoton photodissociation (IRMPD)^{94,97,115,116}. CAD occurs in a collision cell and occurs from ion collision with inert gas (argon, helium, nitrogen, or xenon) resulting in ion kinetic energy converting into internal energy inducing dissociation⁹⁴⁻⁹⁷. Each dissociation technique can fragment ions in unique reproducible ways providing structural information of compounds^{115,116}. This technique allows for elucidation of structural information, significant selectivity increase, and background noise reduction^{94,95,107,115}. The most utilized tandem mass analyzer is the QQQ analyzer, but MS/MS is highly utilized in all six mentioned mass spectrometer types¹¹⁵.

The pairing of additional separation techniques with MS is often required and increases performance of rapid and sensitive investigation of complex mixtures^{94,95,100}. The most common separation techniques that are coupled with MS are gas chromatography (GC), HPLC/UPLC, and capillary electrophoresis (CE)^{100,117-120}. GC is the choice technique for separation of volatile and semi-volatile compounds with low molecular weights (≤ 1000 Da)^{100,117}. Liquid chromatography (LC) and CE techniques are not restrained by volatility and molecular weight^{100,118-120}. Both techniques improve resolution, selectivity and sensitivity, but CE is generally more sensitive, and LC techniques have significantly higher throughput¹¹⁸⁻¹²⁰.

5.2. Mass Spectrometry of Nucleic Acids

Mass Spectrometry has been recognized as rising analytical tool with potential use for wide range of quantitative and qualitative characterization for larger sized nucleic acids^{97,121-125}. Unlike the other established traditional analytical techniques for nucleic acids, MS directly analyzes the mass and structural information, this makes it an ideal technique for post-translation covalent

modification characterization¹²⁴⁻¹²⁶. Numerous mass analyzer advancements within the last 30 years resulted in analyzers with the capabilities to characterize these massive biological molecules^{121,125}. The first MS based analysis of nucleic acids was performed in 1962 using electron impact (EI) and chemical ionization (CI) with gas chromatography-MS (GC-MS)^{121-123,125,127}. This method suffered from in-source fragmentation only generating intact ions two nucleotides in length at most^{125,126}. The next two major advancements occurred in the 1980's when it was discovered that negative mode ionization was optimal and intact sequencing of short (<10) oligonucleotides by tandem MS was achieved^{123,125}. By the 1990s ESI, MALDI, and modern HRMS analyzers were introduced enabling large intact molecular weight determination and highly detailed structural characterization¹²⁵.

The two major approaches of MS-based workflows for nucleic acid characterization are classified as bottom-up and top-down approaches^{84,97,124}. These approaches originated from MS proteomics workflows but are less advanced due to the higher analysis difficulty¹²⁴. The bottom-up workflows begin with enzymatic degradation to yield nucleotides or short oligonucleotides then typically undergo liquid chromatography mass spectroscopy (LC-MS) analysis^{84,94,124}. This approach facilitates characterization of large nucleic acids, nucleobase modifications, and relative abundance of modifications, but each digestion product is removed from the overall context of the intact structure¹²⁴. The top-down approach aims for direct MS characterization of intact nucleic acids^{84,97,121,124}. Top-down approaches have proven successful for oligonucleotides less than 200 bp (~65 kDa) in length and offer the advantages of isoform observation, nucleobase modification characterization with structural context, and the ability to preserve secondary and tertiary nucleic acid structures^{84,124,128}. Bottom-up and top-down approaches are useful complimentary techniques for oligonucleotide structural characterization.

Many common and specific challenges arise in MS-based analysis of oligonucleotides⁸⁴. The common challenges are shared by most analytical techniques for nucleic acids and include the prevention of unintended nuclease or physio-chemical degradation⁸⁴. To minimize common challenges all reagents, laboratory consumables, and workspace are nuclease-free and work should be performed on ice with minimal light exposure⁸⁴. MS specific instrumentation challenges include high ionization difficulty, large molecular size, and homogeneous monomer population¹²³⁻¹²⁵. Unlike other biological molecules, oligonucleotides are primarily restricted to negative polarity ionization due to positive polarity generating high amounts of cationized ions¹²³. Many oligonucleotides of intact analysis interest are within kilodalton size range requiring increasing mass analyzer resolving power and mass limits with size^{84,123}. The oligonucleotide nucleobase monomer population consists of only five canonical nucleobases this further complicates bottom-up approaches and tandem MS analysis compared to proteomics (18 amino acids)¹²⁴.

5.3. Mass Spectrometry Characterization of RNA-LNP

MS has recently been identified as a useful tool for characterization of lipids and RNA from RNA-LNPs^{84,97,126,129-138}. Current chromatographic and instrumentation limitations require RNA extraction and separate lipid and RNA analysis due to megadalton size range and physiochemical complexity of RNA-LNPs^{87,139}. MS based lipidomic techniques have been widely established and applications for characterization of extracted lipid components of RNA-LNPs have been demonstrated^{129,137,138}. Currently various new MS based approaches for quality characterization of extracted RNA are being developed to work around limitations of commercial grade mass spectrometers^{84,126,129-136}.

The ideal LC-MS based approach for RNA-LNP DP characterization would be to chromatographically separate the intact therapeutic RNA and impurities making more consistent

methods with traditional DPs⁸⁴. Top-down LC-MS analysis of intact RNA less than 200 bp has widely been demonstrated^{84,124,128}. Ideally, this style of top-down LC-MS analysis could be applied to RNA and RNA nanoparticle or pegylated drug products within that size range to harmonize and confirm DP quality methods. Moderna demonstrated a Hydrophilic Interaction Liquid Chromatography (HILIC) LC-MS method with intact analysis of mRNA up to 2228 bp (~0.75 mDa) with mass errors less than 50 ppm in 2021 at the American Society for Mass Spectrometry conference^{84,140,141}. Charge detection MS (CDMS) performed with certain orbitrap and quadrupole time-of-flight (QToF) mass analyzers is being investigated for large intact RNA characterization for structures around one megadalton; however, the only QA information the two novel techniques can currently measure is the intact mass confirmation, the presence of an mRNA tail structure, and are being developed to access intact large RNA purity^{84,140-144}.

Simultaneously, many bottom-up MS based approaches for large RNA are currently being developed; broadly based around utilizing different RNA degradation and digestion methods to increase and control the amount and types of oligonucleotide products generated for characterization^{126,129-136}. T1 RNase is the most utilized and commercially available bottom-up sample preparation ribonuclease but suffers from the problem of lower sequence coverage with increased size¹³¹⁻¹³³. Under normal conditions, T1 RNase completely cleaves all the Guanine 3' sides resulting in identical and isomeric digestion products, commercial RNase kits can usually only measure capping and tailing efficiency of mRNA with LC-MS^{84,129,131}. The developmental digestion approaches utilize different and/or multiple ribonucleases and partial digestion strategies to increase MS sequence coverage¹³¹⁻¹³⁶. One unique bottom-up LC-MS mRNA from mRNA-LNP absolute quantification method published in 2024 utilized acid hydrolysis to degrade mRNA-LNPs into nucleobases with quantification performed on each¹²⁶. Bottom-up MS approaches for RNA

are important techniques for sequence identification and mRNA capping and tailing purity⁸⁴.

6. Conclusion

This literature review covers the rapidly advancing landscapes of RNA therapeutics, nanoparticle delivery, regulatory environments, and corresponding MS characterization approaches, with specific focus on the potential application of MS for certain approved and the likely many future RNA and RNA-LNP DPs. The significant advancements in RNA therapeutics and delivery necessitate numerous corresponding analytical techniques that remain fit only for specific purposes; this underscores the need for the development of MS based techniques for deeper structural analysis of all components and as confirmatory methods.

The wide range of RNA therapeutics with the classifications are covered to highlight RNA therapeutics increasing relevance beyond mRNA-LNP vaccines. The development of LNPs for drug delivery is reviewed to present each lipid component's crucial role due to the platform's relevance from widespread adoption for RNA therapeutics. Stability of RNA therapeutics is reviewed to cover the complex physiochemical stability of oligonucleotides and the further complication with LNP introduction emphasizing the need for advanced QA methods.

The rapidly evolving regulatory environment and MS approaches are highlighted to show increasing importance as more RNA therapeutics are approved and utilized. The variety of therapeutic indications and mechanisms driving regulatory classification of RNA therapeutics makes QAs and corresponding analytical method harmonization extremely difficult.

Despite the promise shown by MS there is still much progress to be made in oligonucleotide analysis. The need for this progress increases as more RNA therapeutics arise for many disease conditions. The only widely established RNA QA MS method is enzymatic digestion

for DS characterization of capping and tailing efficiency of mRNA. Many approved smaller RNA therapeutics have RNA DS that fall within the size range for intact HRMS characterization; the development of MS methods would benefit multiple classes of RNA and RNA nanoparticle delivered drugs dependent on the RNA size.

Chapter 2: Hypothesis and Specific Aims

1. Introduction and Research Problem

Oligonucleotide therapeutics are a promising and rising class of biologic drugs with high potential for use in a wide range of conditions encompassing infectious disease to therapies for cancer, and genetic disorders^{1-5,9}. RNA encapsulated within lipid nanoparticles (LNPs) is a prominent delivery method for currently approved oligonucleotide therapeutic products including the mRNA vaccines and polyneuropathy treatments^{77-80,92}. The emergency use authorizations (EUA) and orphan drug status allowed the approval of RNA-LNP drug products without finalization and harmonization of the analytical procedures for quality assurance^{1,92}. This leads to research and industry not having standard critical quality attributes (CQAs) and corresponding analytical procedures for this class of biologic drug products^{82,83}.

CQAs are identified physiochemical attributes that are monitored to indicate the performance of a drug^{55,85}. Widespread adoption of mRNA-LNP vaccines has prompted regulatory agencies to publish guidelines with CQAs and methods to assess those attributes that are still in draft and the only other approved RNA-LNP product's (Onpattro) quality methods are industry created⁸⁷⁻⁸⁹. Despite carrying different RNA payloads, the identified CQAs for RNA-LNP products and quality monitoring at the drug substance (DS) and drug product (DP) manufacture stage are nearly identical but certain attributes are characterized with different analytical techniques^{87-89,91}. The shared CQAs for RNA-LNP final DP include content, identity, integrity, potency, and purity of the lipids, RNA and RNA-LNP, and require compendial product testing. Examples of different RNA-LNP DP CQA methods include RNA content with HPLC-UV or fluorescent-based assay, and RNA identity, which has HPLC-UV or RT-PCR sequencing-based techniques being recommended depending on the therapeutic payload^{87-89,91}. The DP CQA RNA-LNP integrity all use dynamic light scattering (DLS) to access the hydrodynamic diameter and size distribution of LNPs^{87-89,91}. Additionally, regulatory agencies suggest a potency (functionality) RNA-LNP DP

CQA that requires a product specific in-vitro release assay^{87-89,91}. The DS and DP CQAs and corresponding analytical techniques for RNA-LNPs are numerous and fit for specific purposes¹²⁶. The establishment of future enhanced regulatory guidelines for RNA-LNPs delivery systems are crucial for ensuring the quality, safety, efficacy, and streamlined development of RNA and RNA nanocarrier based delivery systems for all indications^{85,90,93}.

Mass spectrometry (MS) has the unique capability to cover many identified RNA-LNP DP CQAs for both lipids and RNA^{129,141}. With the current Liquid Chromatography (LC) and MS limitations RNA-LNPs must be disassembled with lipids and RNA separate for LC-MS analysis using different chromatographic conditions and instrumentation settings^{87,129,138}. LC-MS has already been utilized for LNP lipid component characterization with both quantitative and qualitative structural approaches demonstrated^{136,137}. Most developments in LC-MS approaches for RNA DS analysis focus on bottom-up sample preparation centered approaches, this results in overall loss of structural context and information required for CQA monitoring beyond RNA identification and mRNA capping and tailing efficiencies¹²⁸⁻¹³⁶.

Intact RNA analysis provides unique insights into the CQAs absolute quantification (RNA content), identity, integrity and purity of an RNA sample from specificity only MS can achieve^{97,141}. Characterization of the unestablished RNA-LNP DP CQAs for quality monitoring in accordance with current regulatory guidance requires 7-8 different instruments and 8-9 individual methods^{87-89,91}. Furthermore, the unestablished CQA monitoring at the DS manufacture stage for RNA requires up to 9 instruments with a total of 24 methods^{87-89,91}. Commercial grade high resolution mass spectrometers have proven capable of routine analysis of RNA oligonucleotides up to 200 base pairs (bp) in length^{84,124,128}. This capability could be utilized for quality monitoring analysis of 20 current FDA approved RNA based drugs that fall within that size range. The future

holds untold increasing emergences of novel mass analyzer technologies and refinements of current HRMS techniques making routine MS analysis of high kilo to megadalton sized oligonucleotides eventually inevitably become feasible, furthermore resulting in use for RNA-based drug performance and quality monitoring.

Developing high resolution mass spectrometry (HRMS) based approaches for characterization of RNA from RNA-LNPs may prove critical for deeper assessment of drug product quality due to the complexity of oligonucleotide stability stemming from high physiochemical instability and very large molecular size of biologic molecules^{126,128-130}. LC-MS offers unique benefits from the ability to directly analyze the mass of each formulation component providing specificity and structural elucidation capabilities through tandem MS analysis exclusive to this technique^{97,123-125}. As nanoparticle design for therapeutic delivery increases in sophistication (targeting ligand modification, formulation complexity, oligonucleotide payload) LC-MS will become an even more ideal tool for analysis of the nanoparticle payload and components to investigate performance and monitor quality¹²⁸⁻¹³⁰.

2. Hypothesis

Building on the idea that LC-MS could be an ideal tool for characterization of RNA and lipid component of RNA-LNPs, we explore the potential of extracted intact RNA analysis by LC-MS through RNA-LNP drug quality assurance method development perspective. Utilizing a LC-MS compatible RNA extraction, we hypothesize that absolute quantification and identification of extracted intact RNA can be performed by LC-MS. This hypothesis will provide valuable insights into the development and potential for MS based characterization of RNA from RNA-LNPs.

3. Specific Aims

3.1. Aim 1: Develop LC-HRMS-based methods for the characterization of RNA-LNPs for the CQAs identity and content of extracted intact RNA.

To achieve this, RNA-LNPs will be formulated using a similar formula as the Moderna mRNA vaccine, with like lipid composition. That will serve as a benchmark LNP formulation loaded with two therapeutically relevant forms of RNA. RNA-LNP formulations will be assessed by DLS for the CQAs LNP size, polydispersity index (PDI), and zeta potential, and the standardized fluorescent assay to measure encapsulation efficiency (EE%) and RNA concentration to create the desired quality target product profile (QTPP) consistent with therapeutic RNA-LNP formulations. Isopropanol precipitation for extracted RNA and lipid separation will be performed on RNA-LNPs before LC-MS analysis. Optimal LC-MS conditions for absolute quantification and identification of extracted RNA will be investigated.

3.2. Aim 2: Compare and validate the LC-HRMS method with USP standards for content of therapeutic RNA-LNPs and verify RNA identity.

We will compare and validate the QA “RNA content” with the standardized fluorescent RNA quantification assay using ICH M10 bioanalytical method validation guidelines. Identification of RNA will be confirmed by the measured intact mass with the theoretical mass.

4. Clinical Relevance and Innovation

Advancing LC-MS for characterization of intact RNA from RNA-LNP and RNA-based drug products would benefit quality assurance monitoring methods for potentially twenty currently approved and many potential future relevant drugs in clinical trials. By utilizing LC-MS for quality

monitoring of RNA and other components, we can potentially reduce the amount of required instrumentation and provide more in-depth direct analysis compared to the vast array of other commonly utilized analytical techniques. Additionally, LC-MS characterization could be a confirmatory tool for applicable characterizable attributes. Furthermore, demonstration of LC-MS characterization of intact RNA extracted from lipid nanocarriers offers the ability for absolute quantification and identification of RNA. Investigating LC-MS methods for RNA-LNPs enriches literature on MS characterization of oligonucleotides extracted from lipid nanocarriers and drives clinical innovation in the realm of drug product quality monitoring for small interfering RNA (siRNA), antisense oligonucleotides (ASO), RNA aptamers and beyond.

Chapter 3: Experimental

Absolute Quantification and Identification of RNA from RNA-Lipid Nanoparticles using High Resolution Mass Spectrometry

1. Introduction:

RNA-based therapeutics are a rapidly rising class of biologic drugs with promising potential use in a spectrum of conditions ranging from infectious disease to therapies for cancer, and genetic disorders^{1-5,9}. Lipid nanoparticles (LNPs) are a prominent delivery method for RNA-containing therapeutics that are current approved drug products including mRNA vaccines and RNA polyneuropathy treatments^{77-80,92}. EUA and the orphan drug status of current approved RNA-LNP drugs has allowed approval before regulatory finalization and harmonization of the analytical procedures for quality monitoring^{1,90,92}. This leads to research and industry not having standardized critical quality attributes (CQAs) for those RNA-LNP drug products from identified physiochemical performance indicating factors and corresponding analytical procedures for these biologic drugs^{82,83}.

The rapid widespread adoption of mRNA vaccines prompted regulatory bodies to publish guidelines on quality monitoring of mRNA-LNP vaccines and therapeutics⁸⁷⁻⁸⁹. These guidelines are filled with numerous drug substance (DS), drug product (DP), and critical excipient CQAs with analytical procedures requiring a vast array of instrumentation^{87-88,97,126}. However, these guidelines do not encompass other approved RNA or RNA nanomaterial-delivered drugs^{17,18,89-91}. Liquid chromatography mass spectrometry (LC-MS) based analysis has emerged as promising alternative and confirmatory technique to monitor the quality of certain RNA and RNA-LNP drugs^{126,129,140}.

Despite the promise, LC-MS characterization of RNA based drugs faces many challenges, including the instrumentation capabilities limitations of LC and MS systems, and large biomolecule analysis specifically regarding oligonucleotides^{84,97,128}. In the similar fashion to the

recommended CQA approaches, RNA-LNPs must be separated into critical lipid excipient and RNA DS components with separate analysis using different mobile phases, stationary phases, and MS conditions to be compatible with current LC-MS systems^{87,128,129,139}. The most significant current limitation for MS analysis of RNA is the mass limit of the mass analyzer; most commercial grade high resolution mass spectrometry (HRMS) analyzers can achieve intact RNA analysis of RNA sized at and below 200 base pairs (bp)^{84,124,128}. Specific microbiological sample preparation techniques must be used to avoid oligonucleotide physiochemical degradation and ion adduct formation before and during LC-MS analysis^{84,97,128}. These sample preparation techniques range from the use of RNase free solvents with minimal dissolved ions, reduction of stainless-steel tubing with PEEK, and washing the LC and MS source all done with the purpose of minimizing ion-adduct formation during ionization^{84,97,128}.

LC-MS has been recognized as an ideal tool for RNA and LNP lipid component analysis due to MS ability directly characterize compounds in complex mixtures with high specificity and unique structural elution capabilities^{97,121-125,141}. Lipid components analysis from LNPs by LC-MS has been demonstrated; therefore, most LC-MS method development research focus on RNA characterization investigating bottom-up and top-down approaches^{126,128-138,140-144}. The majority of research uses bottom-up method development approaches; however, this approach results in the loss of all RNA structural context making this approach incompatible with many regulatory identified RNA CQAs^{126,128-136}. In recent years, developments in top-down approaches are becoming more frequent as availability and capabilities of commercial grade HRMS increase¹⁴⁰⁻¹⁴⁴. These approaches largely focus on pushing the intact RNA size limitation for analysis with MS based techniques¹⁴⁰⁻¹⁴⁴. Developments in both approaches are crucial to advance MS characterization for oligonucleotides and RNA drugs; however, MS method development for multiple regulatory identified CQAs for RNA based drugs is a less explored perspective¹²⁹. Method

development from this perspective is necessary for the adoption of LC-MS for RNA and RNA-LNP drug quality and performance monitoring¹²⁹.

The ideal approach to LC-MS analysis of RNA based drugs would be to separate the RNA and other components with an extraction technique that preserves the structural integrity of all critical formulation components⁸⁴. This creates more consistent methods with small molecule active pharmaceutical ingredient (API) quality monitoring and allows for direct multiple CQA characterization of RNA concentration, identity, integrity, and purity for these biologic drugs⁸⁴. The four techniques that are commonly implemented to disrupt or separate RNA-LNPs for analysis are organic precipitation, magnetic particle extraction, spin column extraction, and surfactant disruption^{87,139}. Among these RNA extraction techniques, the organic extraction options are considered the gold-standard due to yielding the highest RNA recovery and integrity preservation¹³⁹. The two common RNA-LNP organic extraction techniques are isopropanol precipitation and phenol-chloroform extraction^{87,139}. Isopropanol precipitation is the ideal technique due to direct compatibility with LC-MS as it separates lipids into an organic phase, RNA into aqueous phase, and desalts the components; without use of surfactants or highly toxic solvents requiring additional sample cleanup^{87,129,139}.

Building on the idea that LC-MS could be an ideal tool for characterization of RNA and LNP lipid component MS procedures are established, we explored the potential of extracted intact RNA analysis by LC-MS through RNA-LNP drug quality assurance method development perspective. Utilizing compatible RNA extraction, we hypothesized that intact RNA can be extracted for absolute quantification and identification to be assessed by LC-MS. To test this hypothesis, RNA-LNPs were formulated with a moderna mRNA vaccine like lipid composition as a benchmark LNP formulation and loaded with two therapeutically relevant forms of RNA. The hydrodynamic diameter (HD) of the RNA-LNP formulations were accessed by DLS and the standardized

fluorescent assay was determined for the prepared RNA-LNPs. Isopropanol precipitation for intact RNA extraction and lipid separation was utilized on RNA-LNPs to investigate compatibility with LC-MS analysis. We evaluated optimal LC-MS conditions for absolute quantification and identification of extracted RNA. The performance of the LC-MS assay was assessed using ICH M10 bioanalytical method validation, with absolute quantification of RNA compared to the standardized fluorescent (RiboGreen[®]) assay and RNA identity confirmed with the intact measured mass. Our work is scientifically relevant and innovative as it will be the first to directly address LC-MS characterization of intact RNA extracted from LNPs. The work is clinically relevant as it may lead to the development of quality monitoring techniques for many approved and future compatible RNA-based drug products.

2. Materials and Methods:

2.1. Materials

The ionizable lipid SM-102 and pegylated lipid DMG-PEG2k were sourced from MedKoo Biosciences, North Carolina, USA. Cholesterol and DSPC structural lipids were purchased from Avanti Polar Lipids, Alabama, USA. Custom synthesized single stranded RNA (60 bp, 19500.7 Da) and FLuc-S1 DsiRNA (sense: MW = 7968.73, antisense: MW = 8664.28) constructs were sourced from Integrated DNA Technologies, Iowa, USA. The Quant-iT RiboGreen[®] RNA assay kit was purchased from Thermo Fisher Scientific, Oregon, USA. 2-propanol, acetonitrile, ammonium acetate, Amicon[®] Ultra-0.5 mL centrifugal filter units (10 kDa MWCO), citrate buffer, ethanol, methanol, Nalgene mobile phase bottles (125 mL), N,N-Diisopropylethylamine (DIPEA), and phosphate buffered saline were purchased from Sigma-Aldrich, Wisconsin, USA. 1,1,1,3,3,3-Hexafluoro-2-propanol (HFIP) was purchased from Tokyo Chemical Industry, Oregon, USA. Molecular biology grade water (Ultrapure type 1) was purchased from Quality

Biologic, Maryland, USA. Glacial acetic acid was purchased from Thermo Fischer Scientific, New Jersey, USA. The ACQUITY™ Premier Oligonucleotide C18 Column, (130Å, 1.7 µm, 2.1 mm x 50 mm) was purchased from Waters Corporation, USA.

2.2. Preparation and Characterization of RNA-LNPs

RNA-LNPs were formulated with two therapeutically relevant sized forms of RNA (60-mer RNA or FLuc S1 DsiRNA) at a nitrogen to phosphate (N:P) ratio of 6, using a moderna vaccine like formulation as a benchmark detailed in **Table 3.1**.

Table 3.1: Parameters of LNP Formulation

Parameter	Lipid	Ratio (%)
Ionizable lipid	SM-102	50
Phospholipid	DSPC	10
Sterol Lipid	Cholesterol	38.5
PEG Lipid	DMG-PEG ₂₀₀₀	1.5

To efficiently prepare the two RNA-LNP formulations at small-scale the ethanol injection method was utilized (**Figure 3.1**). With the objective of therapeutically relevant RNA-LNP design, LNPs were formulated with the following quality target product profile (QTPP): hydrodynamic diameter (HD) < 200 nm, a polydispersity index (PDI) < 0.2, a negative surface charge, and an RNA encapsulation efficiency (EE%) exceeding 80%. These critical quality attributes (CQA) are essential for consistent biological performance and reproducibility across batches. The QTPP results of the formulated RNA-LNPs are listed below in **Table 3.2**.

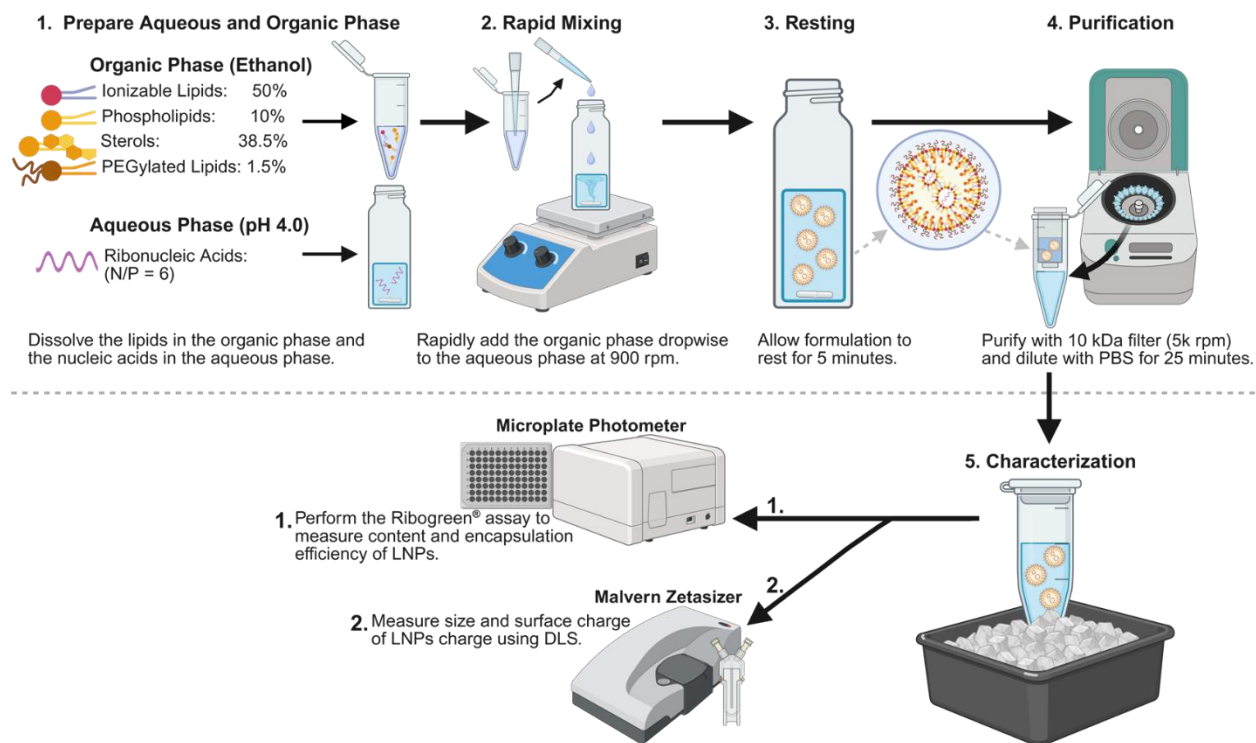


Figure 3.1: Preparation of RNA-Based LNPs by the Ethanol Injection Method: The preparation of RNA-based lipid nanoparticles via the ethanol injection method involves four steps followed by characterization. First, the lipid components are dissolved in ethanol (100 μ l), and the nucleic acids are dissolved in the aqueous phase (300 μ l) containing citrate buffer (pH 4.0). Secondly, the organic phase is rapidly injected dropwise into the aqueous phase under chaotic stirring conditions (900 rpm), promoting lipid nanoparticle formation stirring continues for 5-minutes after injecting. Thirdly, post-stirring a 5-minute resting period with no stirring is observed. Next, the purification and ethanol removal steps are performed with 100 μ l of PBS added. Lastly, the prepared LNPs undergo characterization for hydrodynamic diameter (HD), surface charge, content, and encapsulation efficiency (EE%) before storage under appropriate conditions. The HD and polydispersity index (PDI) are determined by diluting the sample a hundredfold in PBS and measured using dynamic light scattering (DLS). Content and EE% are quantified using the fluorescent RiboGreen® assay. Created with BioRender.com.

RNA-LNPs were formulated with ethanol injection technique (**Figure 3.1**). RNA in water was added to 50 mM citrate buffer at pH 4.0, and the LNP lipid components to ethanol. The ethanol-lipid solution was added using drop-wise technique to the RNA solution under continuous stirring (900 rpm), ensuring an aqueous to organic volume ratio of 3:1. After a 5 minute period, the RNA-LNP mixture was purified with an Amicon® Ultra Centrifugal Filter, and diluted with 1x phosphate-buffered saline (PBS) at pH 7.4. The lipid nanoparticle formulation was composed of an ionizable, sterol, phospholipid, and PEGylated lipid in a molar ratio of 50:38.5:10:1.5, at an N:P ratio of 6 (**Table 3.1**).

Particle size and polydispersity index (PDI) of the prepared RNA-LNPs was measured with dynamic light scattering (DLS) at 25°C under 100x dilution using a Zetasizer from Malvern Instruments. The Zetasizer was used to measure the zeta potential of RNA-LNPs with electrophoretic mobility analysis (**Figure 3.1**).

The Quant-iT RiboGreen® RNA Assay Kit was used to measure the concentration and EE% of RNA within the LNPs¹⁴⁵ (**Figure 3.1**). LNPs were added to 2% Triton X-100 in TE buffer (RNase-free) to disrupt the LNP, and total RNA concentration was quantified with RiboGreen® fluorescent dye. Non-encapsulated RNA was quantified and assessed with the LNPs diluted in 1x TE buffer with the fluorescent dye. Samples are prepared on a 96-well plate kit specific setup, both sample preparation types measured in duplicate on a plate reader. The samples were prepared in triplicate, and the plate was blanked in duplicate. The percentage of RNA encapsulation efficiency (EE%) was calculated with the formula: $[(F_{\text{total RNA}} - F_{\text{free RNA}}) / F_{\text{total RNA}}] \times 100\%$, where $F_{\text{total RNA}}$ represents the fluorescence of total RNA, and $F_{\text{free RNA}}$ represents the fluorescence of free RNA not encapsulated within LNPs¹⁴⁵.

Table 3.2: Physiochemical Properties of LNP Formulations: The lipid nanoparticle formulations were composed of ionizable lipid, sterol, phospholipid, and PEG lipid in a molar ratio of 50:38.5:10:1.5, respectively. n = 6.

RNA	HD (nm)	(PDI)	(mV)	EE%
60-mer	101 ± 3	0.20 ± 0.02	-6 ± 1	93 ± 2
FLuc DsiRNA	95 ± 3	0.20 ± 0.02	-6 ± 1	95 ± 1

2.3. RNA Extraction from RNA-LNP

To extract and preserve integrity of the intact RNA and separate the lipids from the LNP in a non-harsh and LC-MS compatible fashion the isopropanol precipitation technique (**Figure 3.2**) was utilized. The specific steps chosen for the RNA extraction technique for the assay were selected to optimize preservation of intact RNA integrity and minimize generation of MS source adducts. This was achieved through performing all steps on ice and removing pellet drying in vacuo for maximum intact RNA integrity preservation, and the addition of the 70% ethanol wash step to desalt RNA samples shown below in **Figure 3.2**.

RNA was extracted using isopropanol precipitation^{87,139} (**Figure 3.2**). RNA-LNP samples (100 µL) were diluted 10-fold in isopropanol 60 mM ammonium acetate (900 µL), briefly vortexed, then centrifuged (14,000 g, 4°C) for 15 minutes. The lipid containing supernatant was collected and discarded. The RNA pellet was washed with isopropanol (1 mL) and centrifuged (14,000 g, 4°C) for 15 minutes. The isopropanol was removed, the pellet was washed with chilled 70% ethanol (1 mL) and centrifuged (14,000 g, 4°C) for 15 minutes. The chilled 70% ethanol was removed, and the RNA pellet was resuspended in RNase free water (100 µL). All steps were performed on ice.

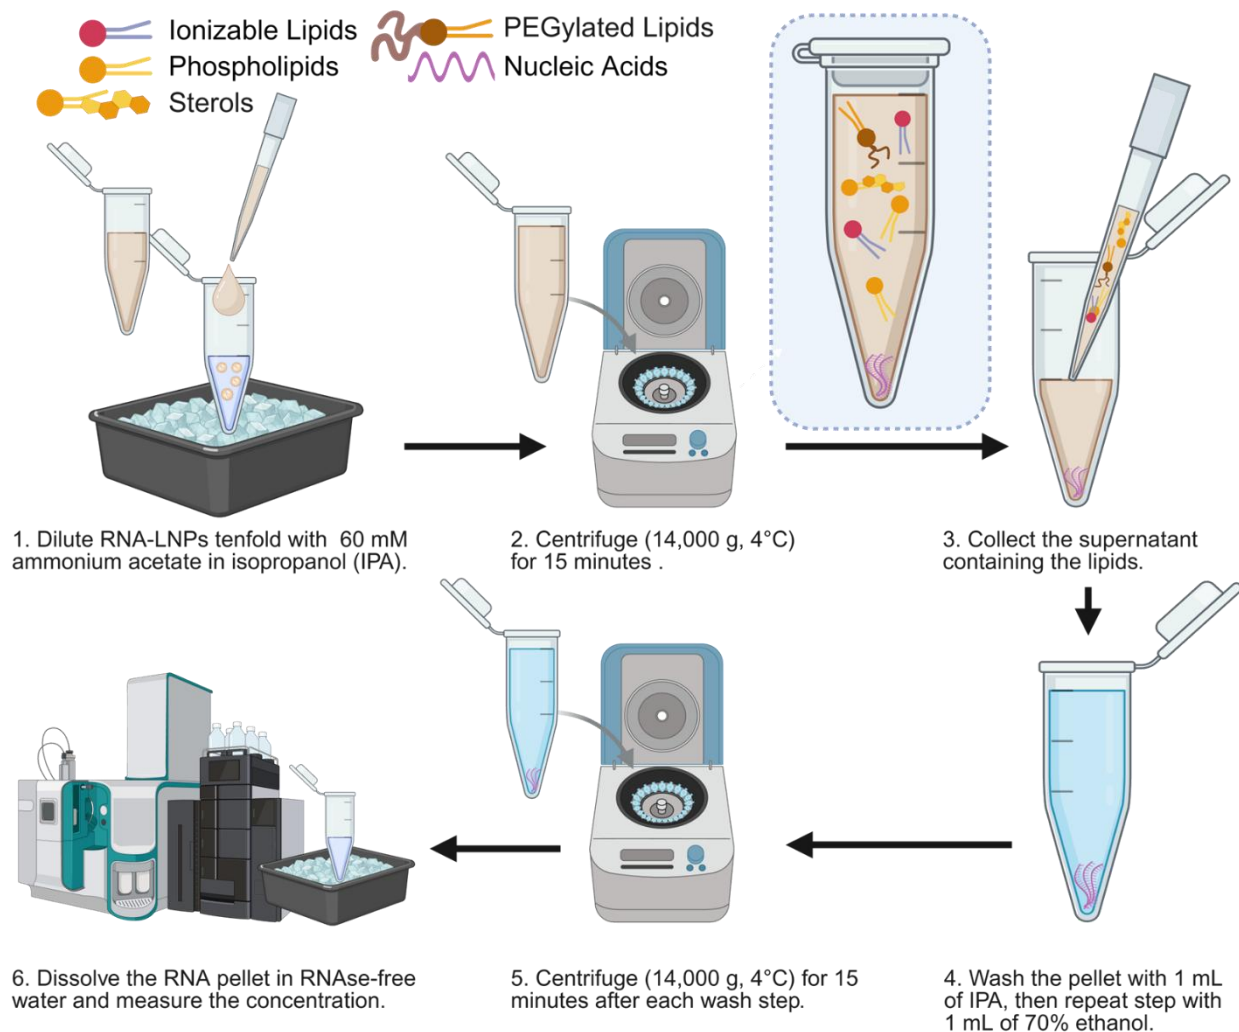


Figure 3.2: Extraction of RNA from LNPs by Isopropanol Precipitation Method: The extraction of RNA from RNA-LNPs via the isopropanol precipitation method involves six steps followed by measuring the resuspended RNA concentration. First, the RNA-LNP formulation (100 μ l) is diluted tenfold in 60 mM ammonium acetate in isopropanol (IPA) (900 μ l). Secondly, the solution is briefly vortexed then centrifuged (14,000 g, 4°C) for 15-minutes. Thirdly, the supernatant containing the lipids is collected and removed. Next to wash, IPA (1 mL) is added with mixing to disturb the RNA pellet then centrifuged (14,000 g, 4°C), followed by removal of the IPA. The wash step is repeated with the use of chilled 70% ethanol (1 mL). Lastly, the RNA pellet is dissolved in water and the concentration measured by LC-MS. All steps were performed on ice. Created with BioRender.com.

2.4. LC-MS Conditions for RNA Absolute Quantification and Identification

RNA samples were separated using ACQUITY™ Premier Oligonucleotide C18 Column, (130Å, 1.7 µm, 2.1 mm x 50 mm) with Ion-Pairing Reversed Phase Liquid Chromatography (IP-RP-LC) using a 5 minute gradient from 1.0% to 70.0% B at 2.50 minutes, maintain until 2.80 minutes, and 70.0% to 1.0% B at 2.81 minutes, and remained 1% B until 5 minutes (Solvent A: 95:5, methanol: water, 1% HFIP, 0.5% DIPEA) (Solvent B: 95:5, water: methanol, 1% HFIP, 0.5% DIPEA) at 0.2 mL/min, 60 °C, using a 20.0 µL injection volume on a Shimadzu Nexera 40 series UPLC system. The UPLC system was coupled to a SCIEX X500R QToF operated in negative mode. The source conditions were spray capillary voltage: -4.2 kV; DP: -80 V; DP spread: 0 V; cone gas: -50 psi; desolvation gas: 60 psi; curtain gas: 35 psi; CAD gas: 12 psi; source temperature: 450°C. The ToF scan mass range was 600 – 3000 Da, accumulation time was 0.1 s, CE set to -10 V, and CE spread set to 0 V. The MRM scan mass range was 100 – 1500 Da, accumulation time was 0.1 s, CE set to -55 V, CE spread set to 0 V, and DP at -80 V.

Prior to analysis to clean and minimize ion suppression the LC system and MS source prior were flushed with wash A (Wash A: 1:1:1:1, acetonitrile: methanol: isopropanol: 10% acetic acid in water) for 4 – 12 hours followed by wash B (Wash B: 1:1, methanol: water) for 2 – 8 hours at 0.4 mL/min, 40°C. The sample capillary was washed with Wash B followed by Wash A. All Nalgene mobile phase bottles were soaked in 10% acetic for 4 – 24 hours acid prior to washing or analysis and thoroughly rinsed more than 10x with water. All water used was ultrapure type 1 and all other solvents used were LC-MS grade.

2.5. Data Processing

All theoretical RNA construct masses and ions were calculated using SCIEX OS Explorer. MS data processing was performed using SCIEX OS Analyst and Explorer for RNA identification and

absolute quantification. Identification was performed by matching a minimum of two precursor ions from the intact RNA constructs measured m/z with an external standards and theoretical m/z. Absolute quantification analysis was performed by preparing 7 and 9-point external calibration curves (60-mer: 50 – 1500 ng/mL, FLuc-S1 dsRNA: 5 – 1500 ng/mL) to determine the concentration of extracted RNA with the assays validated with ICH M10 bioanalytical method validation guidelines.

2.6. Statistical Analysis

Quantitative data is presented as mean $\pm$ standard deviation (SD). Statistical data processing and analysis were conducted using GNU R (version 4.5.3). To compare the two different quantification techniques RNA measurement means a one-way ANOVA was utilized. Statistical significance was set at an α -value less than 0.05.

3. Results and Discussion:

3.1. LC-MS Identification of Intact RNA extracted from RNA-LNP

This study aimed to investigate the potential of LC-MS as a tool for characterization of extracted intact RNA from RNA-LNPs. This approach was expected to lead to the absolute quantification and identification of RNA. To confirm the capability of this top-down methodology we selected two therapeutically relevant sized RNA constructs of custom synthesized single and double-stranded RNA (60-mer, FLuc-S1 dsRNA) with the following sequences (ribonucleotide (r), deoxyribonucleotide (d)):

60-mer: rAUGGU rGAGCA rAGGGC rGAGGA rGCUGU rUCACC rGGGGU rGGUGC

rCCAUC rCUGGU rCGAGC rUGGAC

FLuc-S1 dsRNA

Sense: /5Phosphate/rGGUUC rCUGGA rACAAU rUGCUU rUUAAdCdA

Antisense: rUGUAA rAAGCA rAUUGU rUCCAG rGAACC rAG

The LC conditions were optimized to increase throughput with 5-minute runtimes. The screened conditions include with ranges include flowrate between 0.1 – 0.4 mL/min with 0.2 mL/min selected, and doubling the gradient time (1.0% to 70.0% B at 2.50 min, maintained until 2.80 min, and 70.0% to 1.0% B at 2.81 min, and remained 1% B until 5 min) and runtime (5 – 10 min). It was found the 5-minute gradient and runtime produced the best chromatographic results shown below in **Figure 3.3** and **Figure 3.4**. The MS conditions that were found to be optimal and the range of conditions for observing the ions of interest included capillary spray voltage: -4.2 kV and -4.0 – -4.5 kV; CAD gas: 12 psi and 9 – 12 psi; CE: -10 V and -5 – 10 V; ToF scan DP: -80 V and -60 – -250 V; MRM CE: -55 V and -30 – -60 V; and MRM DP: -80 V and -60 – -250 V.

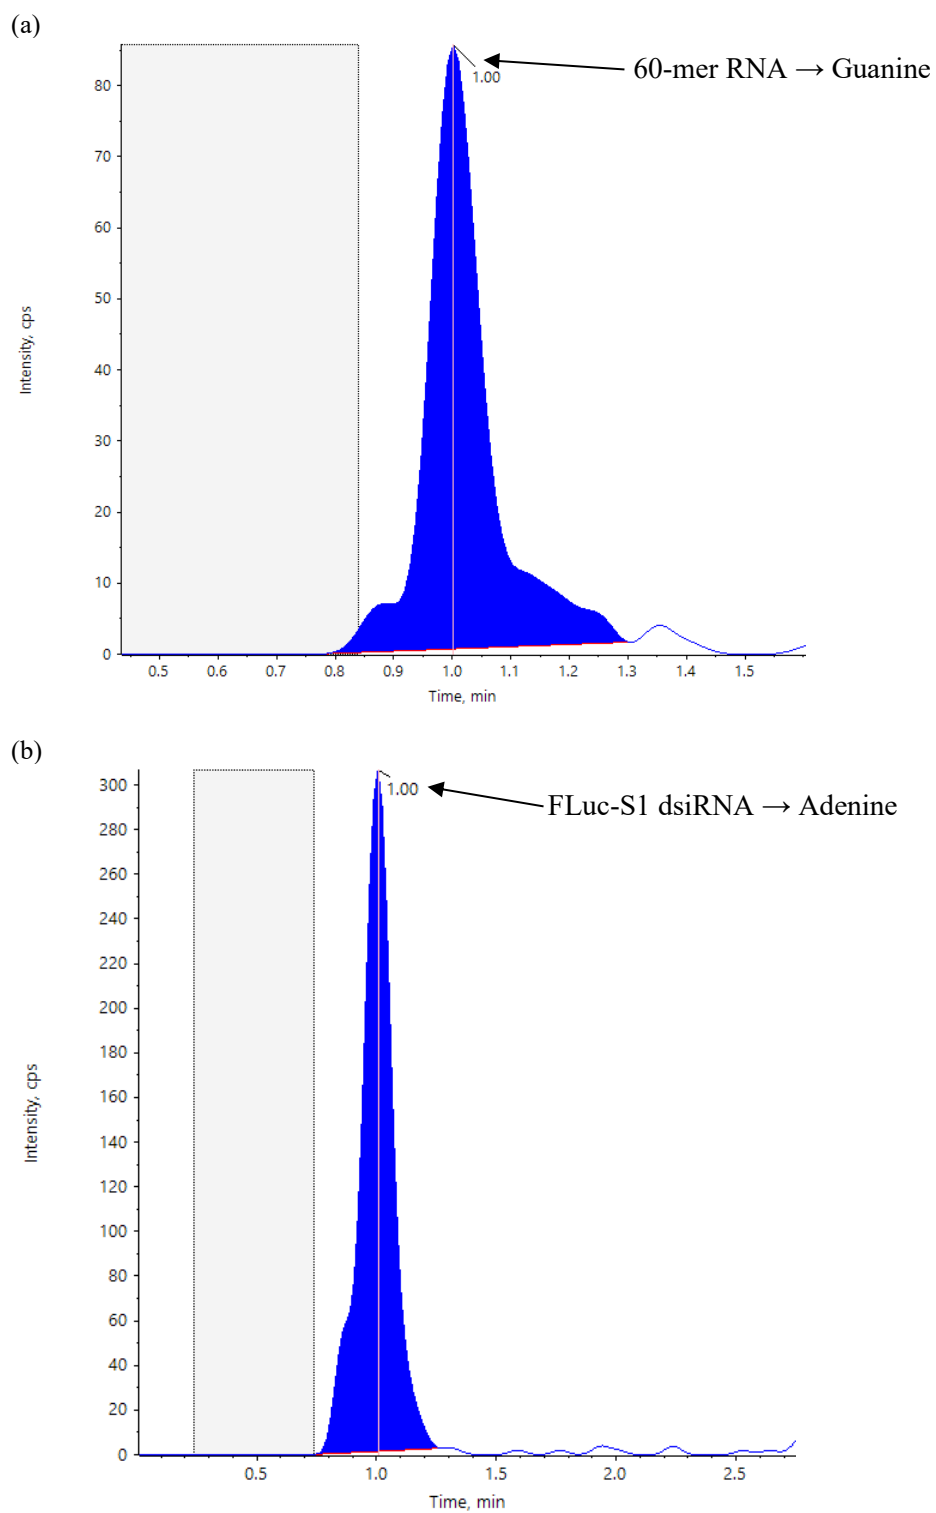


Figure 3. 3: XIC of RNA constructs: (a) XIC of guanine (150.0421 m/z) CAD fragment from the 60-mer RNA -28 charged precursor with a 1.02 ± 0.01 min retention time (rt). (b) XIC of adenine (134.0470 m/z) CAD fragment from the antisense FLuc-S1 dsRNA construct -11 charged precursor with a 1.01 ± 0.01 min rt. Created with SCIEX OS Analytics.

To confirm the identity of the RNA constructs a minimum of two intact precursor ion charge states for each RNA construct with MRM ion fragmentation patterns consistent with RNA were observed in the mass spectrum. The intact RNA precursor ions from the total ion chromatogram (TIC) selected for monitoring from the 60-mer were between -28 to -24 and -11 to -10 for both FLuc-S1 dsRNA antisense and sense constructs, the measured m/z are listed below in **Table 3.3** the intact RNA precursor ions were measured with a mass accuracy within ± 15 ppm except for -24 charged monoisotopic 60-mer precursor ion which couldn't be resolved due to low abundance.


Table 3.3: List of m/z Values for Charge Range of Intact RNA Precursor Ions: The double-stranded FLuc-S1 dsRNA was composed of sense (S) and antisense (AS) RNA constructs.

RNA	Charge	Measured Monoisotopic	Theoretical Monoisotopic	PPM	Measured Most Abundant	Theoretical Most Abundant	PPM
60-mer	-28	695.1148	695.1091	8.20	695.4015	695.4082	-9.63
60-mer	-27	720.8955	720.9043	-12.21	721.2077	721.2013	8.87
60-mer	-26	748.6717	748.6701	2.14	748.9503	748.9400	13.75
60-mer	-25	778.6590	778.6572	2.31	778.9739	778.9780	13.22
60-mer	-24	811.1683	811.1432	30.95	811.5155	811.5192	-4.56
S FLuc DsiRNA	-11	723.0801	723.0843	-5.81	723.3487	723.3577	-12.43
AS FLuc DsiRNA	-11	786.2840	786.2848	-1.02	786.5543	786.5582	-4.96
S FLuc DsiRNA	-10	795.5174	795.5186	-1.51	795.8937	795.8945	-1.01
AS FLuc DsiRNA	-10	865.0076	865.0140	-7.40	865.3126	865.3147	-2.43


MRM scans were used to confirm RNA identity with the selected ions in **Table 3.3** undergone CAD with the selection of precursor ions that produce oligonucleotide associated fragmentation. The selected oligonucleotide product ions for monitoring and their associated compound are listed below in **Table 3.4**. Numerous RNA associated CAD product ions could be observed to verify the

identity of the precursor ions shown below in **Figure 3.4**. The selected MRM oligonucleotide product ions in **Table 3.4** all had mass accuracy within ± 5 ppm.


(a)

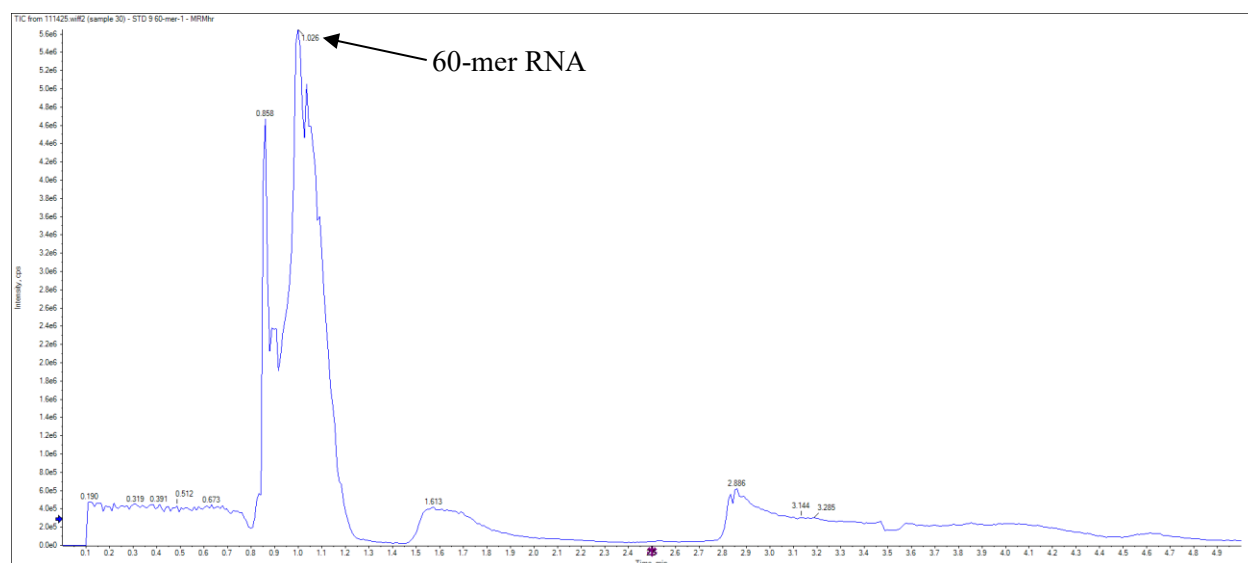

(b)

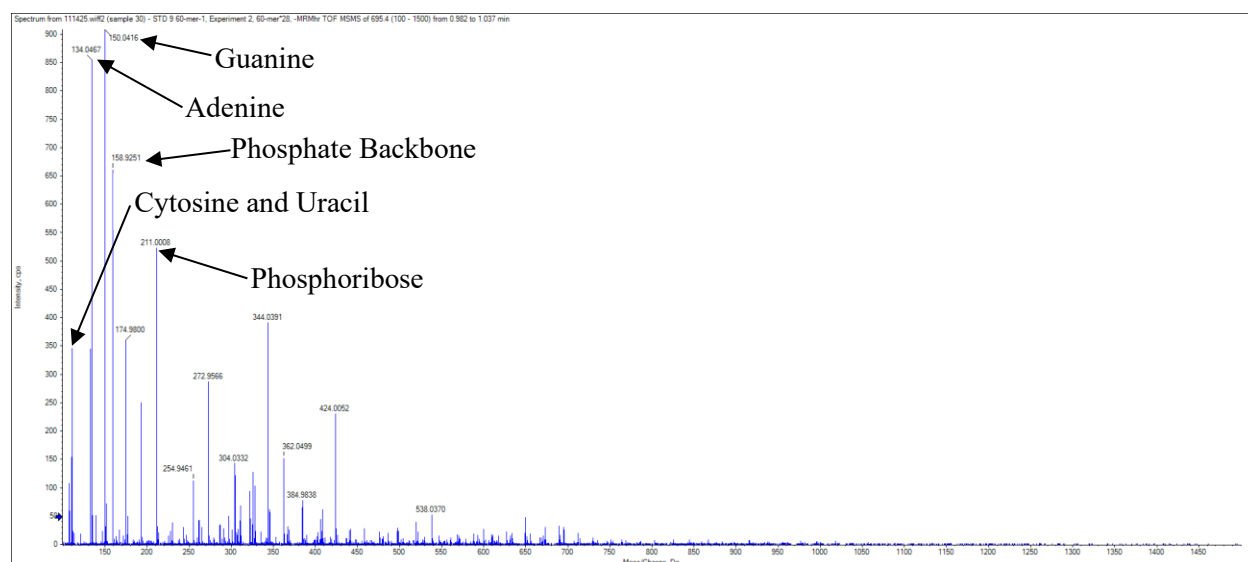

(c)

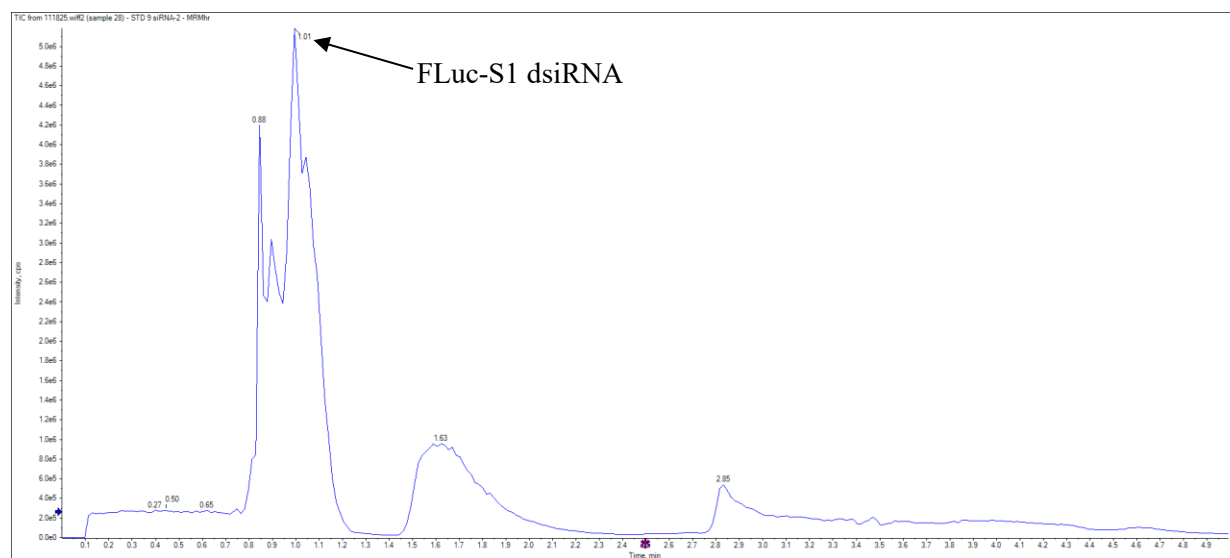

(d)

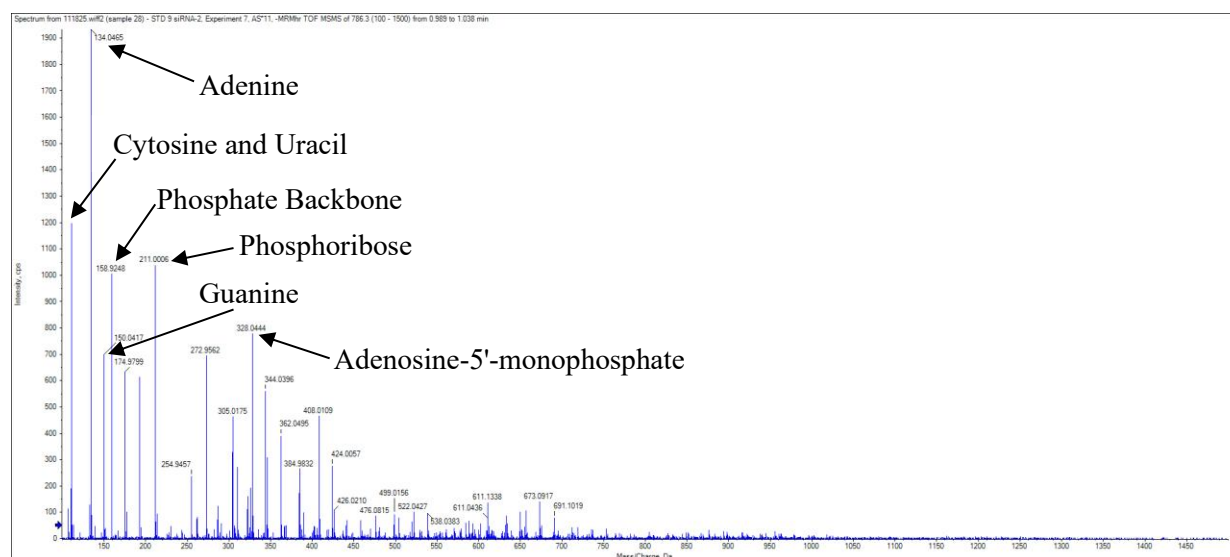


Figure 3.4: Raw TIC and MRM Spectrums of RNA constructs: (a) TIC spectrum of 60-mer RNA and (b) CAD MRM spectrum from the -28 charged precursor with a 1.02 ± 0.01 min retention time (rt). (c) TIC spectrum of the FLuc-S1 dsRNA and (d) CAD MRM spectrum from the -11 charged precursor with a 1.01 ± 0.01 min rt. Created with SCIEX Explorer.

Table 3.4: List of m/z values for MRM RNA Construct Product Ions: The monitored RNA sequence products include the negative CAD product ions of adenine (A), cytosine (C), guanine (G), uracil (U), phosphate backbone (p), phosphoribose (RbP), Adenosine-5'-monophosphate (AMP), adenosine 3',5'-cyclic monophosphate (cAMP).

RNA	Sequence Product	Measured Mass	Expected	ppm
60-mer	C	110.0356	110.0360	-3.64
60-mer	U	111.0199	111.0195	3.60
60-mer	A	134.0467	134.0470	-2.24
60-mer	G	150.0416	150.0421	-3.33
60-mer	p	158.9251	158.9252	-0.63
60-mer	RbP	211.0008	211.0002	2.84
60-mer	AMP	328.0437	328.0447	-3.05
FLuc DsiRNA	C	110.0355	110.0360	-4.54
FLuc DsiRNA	U	111.0193	111.0195	-1.80
FLuc DsiRNA	A	134.0465	134.0470	-3.73
FLuc DsiRNA	G	150.0417	150.0421	-2.67
FLuc DsiRNA	p	158.9249	158.9252	-1.89
FLuc DsiRNA	RbP	211.0004	211.0002	0.95
FLuc DsiRNA	AMP	328.0444	328.0447	-0.61
FLuc DsiRNA	cAMP	346.0551	346.0553	-0.58

3.2. LC-MS Absolute Quantification of Extracted RNA

Prior to LC-MS quantification of LNP, extracted intact RNA was performed to compare RNA concentration with the LC-MS assay. The results normalized with the LC-MS assay are below in **Table 3.5**. The measured concentration of the reconstituted 60-mer RNA was 1131 ± 13 ng/ μ L and the FLuc dsiRNA was 1035 ± 11 ng/ μ L by UV-Vis. This was done to have a starting concentration to account for the dilutions performed during the formulation and RNA extraction steps. This should not be expected to directly represent the extracted RNA concentrations. After RNA-LNP formulation, the total RNA concentration 9.21 ± 0.69 ng/ μ L for the 60-mer RNA-LNP measured by the fluorescent RiboGreen[®] assay (**Figure 3.1**), fluorescent concentrations were not reported for the FLuc-S1 dsiRNA due to validation of quantification with this specific dye and assay only applicable to single stranded RNA constructs (**Table 3.5**).

To perform LC-MS absolute quantification on the extracted RNA constructs external calibration curves were prepared using identical RNA constructs (Supplementary Figure S1, S2, Supplementary Table S1, S2). The 60-mer and FLuc-S1 dsRNA precursor ion charge states -28 and -11 for the antisense dsRNA constructs (**Figure 3.3, Table 3.4**) using the product ion associated with guanine (150.0421 m/z) for the 60-mer and adenine (134.0470 m/z) for the FLuc-S1 dsRNA the CAD products were found to be the most optimal ions for MRM absolute quantification with the MS conditions. To facilitate fluorescent and LC-MS comparison, RNA concentrations from RNA-LNPs were measured from the same prepared formulation with a simple hundred-fold dilution for LC-MS. The optimal quantification range was found to be 50 – 1500 ng/mL for the 60-mer and 5 – 1500 ng/mL for the FLuc-S1 dsRNA and the measured total concentration between the standardized assay (Ribogreen®) and the LC-MS assay were within 95% and consistent with ICH M10 bioanalytical method validation guidelines (**Table 3.5**, Supplementary Figure S1, S2, Supplementary Table S1, S2).

Table 3.5: Results Comparison of RNA Quantification Techniques: The results for the theoretical RNA concentration were calculated using a dilution formula accounting for formulation (100x), RNA extraction (10x) and MS assay dilutions (10x) from the original UV-Vis measurements. Each quantification method has been converted to ng/mL to facilitate comparison. Each quantification result was measured at n = 6 for UV-Vis, n = 3 for fluorescence, and for LC-MS n = 4 (60-mer) and n = 3 (Antisense FLuc-S1 dsRNA).

RNA Construct	Theoretical (UV-Vis, ng/mL)	Ribogreen® (ng/mL)	LC-MS (ng/mL)	LC-MS Range (ng/mL)
60-mer	~100	92.10 ± 6.90	92.46 ± 7.77	50 – 1500
Antisense FLuc DsiRNA	~100	N/A	77.75 ± 14.90	5 – 1500

It was anticipated that the LC-MS assay would measure a lower RNA concentration than the RiboGreen® due to having higher specificity for the exact RNA construct of interest unlike the fluorescent dye. Interestingly, the mean 60-mer RNA quantification results for both the fluorescent and LC-MS assay were nearly identical at 92.10 ± 6.90 and 92.46 ± 7.77 ng/mL (**Table 3.5**). A

one-way Anova test was used to test for a significant difference between the quantification results means of the LC-MS and standard fluorescent assays and found there was no significant difference ($df = 1$, F -value = 0.005, $p = 0.944$). The Quant-iT RiboGreen[®] RNA assay kit has two standard curve configurations a high-range (20 – 1000 ng/mL) and low-range (1 – 50 ng/mL) for single stranded RNA quantification¹⁴⁵. The LC-MS assay demonstrated a greater dynamic range with the ability to quantify higher RNA concentrations up to 1500 ng/mL (**Table 3.5**); furthermore, future use of tandem mass analyzers with ion transmission loss correction features has the potential to make this LC-MS assay significantly more sensitive than the Quant-iT RiboGreen[®] RNA assay kit.

LC-MS quantification of the antisense FLuc-S1 dsRNA was demonstrated to showcase the capabilities of the assay to characterize therapeutically relevant RNA beyond single-stranded constructs. The quantification results of the antisense construct were reported consistent with standard pharmaceutical practice as it is considered the therapeutically active RNA construct for interfering RNA^{146,147}. The assay has the full capability to simultaneously monitor both sense and antisense for double-stranded constructs demonstrated for the identification attribute in section 2.2. Despite not demonstrating a direct quantification comparison method for the FLuc-S1 dsRNA this showcases the LC-MS assay compatibility potential for quality monitoring with many current smaller sized approved RNA drugs.

4. Conclusion

The ability to characterize intact RNA with commercial grade high resolution mass spectrometer (HRMS) capabilities has greatly increased in recent years. From an industry and regulatory perspective, Liquid chromatography mass spectrometry (LC-MS) presents a useful tool and confirmatory method for critical quality attribute (CQAs) monitoring of RNA identity and

content for certain RNA-LNP and many RNA based drugs. However, many critical challenges exist when using LC-MS for characterization of intact RNA extracted from RNA-lipid nanoparticles (RNA-LNPs), largely stemming from instrumentation limitations and large oligonucleotide analysis. In this study, we focused on developing LC-HRMS assay to identify and measure concentration of intact RNA extracted from LNPs. This study was driven by the facts that LC-MS quality monitoring of critical lipid excipients of LNPs are established, intact extracted RNA LC-MS method development has the potential to fulfil many regulatory identified RNA CQAs, and the currently 20 FDA approved smaller RNA (<200 bp) based drugs that fall within size range compatibility.

To achieve this goal in the most efficient manner the attributes that we must demonstrate LC-MS characterization are absolute quantification and identification of intact RNA from RNA-LNPs. Demonstrations of these two attributes are the key hurdle to this approach, unlocking the future potential to fulfill other related regulatory identified RNA and critical excipient CQAs with assay expansion. Thus, we selected two therapeutically relevant RNA constructs, a benchmark therapeutic LNP formulation with relevant quality target product profile (QTPP), and an LC-MS compatible, non-harsh RNA extraction technique. Our findings showcase that the developed LC-MS assay can measure identity and quantify single and double-stranded intact RNA constructs extracted from LNPs. Our results indicated that for the same formulation, LC-MS could measure the same concentration of single-stranded RNA extracted from LNPs as the fluorescent RiboGreen[®] assay with no significant statistical differences in measurements.

This investigation highlights the usefulness of LC-HRMS as a tool for CQA monitoring of RNA and RNA-LNPs drugs and represents a foundational step for MS method development for nanocarrier extracted intact RNA characterization. Future directions could include expanding the assay to measure RNA integrity and purity CQAs using commercial comprehensive

biopharmaceutical characterization software, the addition of a sample preparation purification step to incorporate the CQA RNA encapsulation efficiency (EE%), investigating LC and MS source modifications to increase the intact RNA mass range for analysis, or demonstration of LNP critical lipid excipient characterization. While this study did not explore the use of commercial comprehensive biopharmaceutical characterization software for mass deconvolution due to available computation hardware limitations, it represents a promising avenue for future research, potentially offering this characterization approach to become truly RNA-LNP multiple regulatory CQA encompassing through measuring RNA integrity and purity with relative quantification by mass deconvolution software; alongside monitoring RNA EE% and the LNP critical lipid excipient CQAs.

Chapter 4: Overall conclusion and future directions

In this work, we set out to design an LC-HRMS assay to characterize identity and concentration of RNA constructs extracted from therapeutically relevant RNA-LNP formulations. Our research demonstrates that LC-MS can simultaneously measure identity and concentration of intact single and double-stranded RNA constructs from LNPs disrupted and separated from lipid components with organic extraction. The LC-MS assay conditions were optimized for the RNA constructs, validated using ICH m10 bioanalytical method validation guidelines, and compared to the standardized fluorescent assay with no significant difference was found between the measured concentrations for the single-stranded RNA construct for the two quantification techniques. We also demonstrated the LC-MS assays compatibility with double-stranded RNA, thus suggesting the potential advantage for the LC-MS approach to be compatible with more than single-stranded RNA constructs and oligonucleotide mixtures.

In our future studies, we seek to employ this approach to demonstrate additional regulatory identified RNA and other critical excipient CQA to expand the LC-MS assay. One approach to achieve this for an additional regulatory RNA CQAs would be to include a purification procedure before organic extraction of the RNA-LNP, this would allow for separation of encapsulated and unencapsulated of RNA allowing this assay to measure EE%, and the result could simply be compared with the standardized fluorescent assay. A second approach would be to incorporate critical excipient CQA, such as the lipid components for RNA-LNPs. This could be achieved through collection of the lipids during the organic extraction procedure for separate LC-MS analysis. A third modification to this approach to achieve additional CQAs would be to utilize commercial comprehensive biopharmaceutical mass deconvolution software with the data processing procedures of the assay. This additional data processing with the LC-MS results could measure the RNA and critical lipid CQAs identity, integrity, and purity with automated sequence

mapping and relative quantification. The fourth modification to the assay could include utilizing LC-MS to characterize the effect RNA-based drugs have on sequence specific quality monitoring cellular assays for the regulatory CQA potency. This could be achieved through creating an LC-MS assay to characterize the specific cellular target for expression or silencing associated with the RNA sequence. The combination of all these approaches for RNA-LNPs could lead to a vast reduction of the individual instrumentation required for quality monitoring and create confirmatory techniques for the listed potential CQAs, with LC-MS based approaches utilizing superior structural elution capabilities required to assess biological performance.

In addition to the application to RNA-LNPs, the LC-MS assay may have broader implications for the quality monitoring of other approved RNA-based drugs within the compatible size range, such as the pegylated RNA aptamers Macugen (pegaptanib sodium) and Izervay (avacincaptad pegol). Exploring the potential for this assay approach to characterize other RNA-based products could unveil new insights into performance and quality for a wider range of RNA drug products and their critical excipients.

Overall, further advancing research in these areas could accelerate the development and utilization of LC-MS as a tool for quality monitoring of RNA-LNP and RNA-based drugs, enhancing quality monitoring and performance assessment, and harmonizing approaches for many current and future drug products.

Chapter 5: Bibliography

References:

- (1) Kim, Y.-K. RNA Therapy: Rich History, Various Applications and Unlimited Future Prospects. *Exp Mol Med* **2022**, *54* (4), 455–465. <https://doi.org/10.1038/s12276-022-00757-5>.
- (2) Damase, T. R.; Sukhovshin, R.; Boada, C.; Taraballi, F.; Pettigrew, R. I.; Cooke, J. P. The Limitless Future of RNA Therapeutics. *Front. Bioeng. Biotechnol.* **2021**, *9*. <https://doi.org/10.3389/fbioe.2021.628137>.
- (3) Shi, Y.; Shi, M.; Wang, Y.; You, J. Progress and Prospects of mRNA-Based Drugs in Pre-Clinical and Clinical Applications. *Sig Transduct Target Ther* **2024**, *9* (1), 1–43. <https://doi.org/10.1038/s41392-024-02002-z>.
- (4) Rohner, E.; Yang, R.; Foo, K. S.; Goedel, A.; Chien, K. R. Unlocking the Promise of mRNA Therapeutics. *Nat Biotechnol* **2022**, *40* (11), 1586–1600. <https://doi.org/10.1038/s41587-022-01491-z>.
- (5) Sun, B.; Wu, W.; Narasipura, E. A.; Ma, Y.; Yu, C.; Fenton, O. S.; Song, H. Engineering Nanoparticle Toolkits for mRNA Delivery. *Advanced Drug Delivery Reviews* **2023**, *200*, 115042. <https://doi.org/10.1016/j.addr.2023.115042>.
- (6) Zamecnik, P. C.; Stephenson, M. L. Inhibition of Rous Sarcoma Virus Replication and Cell Transformation by a Specific Oligodeoxynucleotide. *Proc. Natl. Acad. Sci. U.S.A.* **1978**, *75* (1), 280–284. <https://doi.org/10.1073/pnas.75.1.280>.
- (7) Fomivirsen Approved for CMV Retinitis: First Antisense Drug. *AIDS Treat News* **1998**, No. 302, 7.
- (8) Fire, A.; Xu, S.; Montgomery, M. K.; Kostas, S. A.; Driver, S. E.; Mello, C. C. Potent and Specific Genetic Interference by Double-Stranded RNA in *Caenorhabditis Elegans*. *Nature* **1998**, *391* (6669), 806–811. <https://doi.org/10.1038/35888>.
- (9) Hu, B.; Zhong, L.; Weng, Y.; Peng, L.; Huang, Y.; Zhao, Y.; Liang, X.-J. Therapeutic SiRNA: State of the Art. *Sig Transduct Target Ther* **2020**, *5* (1), 1–25. <https://doi.org/10.1038/s41392-020-0207-x>.
- (10) Dong, Y.; Dorkin, J. R.; Wang, W.; Chang, P. H.; Webber, M. J.; Tang, B. C.; Yang, J.; Abutbul-Ionita, I.; Danino, D.; DeRosa, F.; Heartlein, M.; Langer, R.; Anderson, D. G. Poly(Glycoamidoamine) Brushes Formulated Nanomaterials for Systemic SiRNA and mRNA Delivery in Vivo. *Nano Lett.* **2016**, *16* (2), 842–848. <https://doi.org/10.1021/acs.nanolett.5b02428>.
- (11) Bloom, K.; van den Berg, F.; Arbuthnot, P. Self-Amplifying RNA Vaccines for Infectious Diseases. *Gene Ther* **2021**, *28* (3), 117–129. <https://doi.org/10.1038/s41434-020-00204-y>.
- (12) Mullard, A. FDA Approves Second RNA Aptamer. *Nature Reviews Drug Discovery* **2023**, *22* (10), 774–774. <https://doi.org/10.1038/d41573-023-00148-z>.
- (13) Riehemann, K.; Schneider, S. W.; Luger, T. A.; Godin, B.; Ferrari, M.; Fuchs, H. Nanomedicine—Challenge and Perspectives. *Angew Chem Int Ed* **2009**, *48* (5), 872–897. <https://doi.org/10.1002/anie.200802585>.
- (14) Afzal, O.; Altamimi, A. S. A.; Nadeem, M. S.; Alzarea, S. I.; Almalki, W. H.; Tariq, A.; Mubeen, B.; Murtaza, B. N.; Iftikhar, S.; Riaz, N.; Kazmi, I. Nanoparticles in Drug Delivery: From History to Therapeutic Applications. *Nanomaterials (Basel)* **2022**, *12* (24), 4494. <https://doi.org/10.3390/nano12244494>.

- (15) Boulaiz, H.; Alvarez, P. J.; Ramirez, A.; Marchal, J. A.; Prados, J.; Rodríguez-Serrano, F.; Perán, M.; Melguizo, C.; Aranega, A. Nanomedicine: Application Areas and Development Prospects. *IJMS* **2011**, *12* (5), 3303–3321. <https://doi.org/10.3390/ijms12053303>.
- (16) Webster, T. J. Nanomedicine: What's in a Definition? *Int J Nanomedicine* **2006**, *1* (2), 115–116. <https://doi.org/10.2147/nano.2006.1.2.115>.
- (17) FDA. *Drug Products, Including Biological Products, that Contain Nanomaterials*; FDA-2017-D-0759; Food and Drug Administration (FDA): **2022**; 1-29, <https://www.fda.gov/media/157812/download> (accessed 2025-06-19).
- (18) EMA. *Nanotechnology-based medicinal products for human use*; EMA/20989/2025; European Medicines Agency (EMA): **2025**; 5-29, https://www.ema.europa.eu/en/documents/report/nanotechnology-based-medicinal-products-human-use-eu-horizon-scanning-report_en.pdf (accessed 2025-06-19).
- (19) Mitchell, M. J.; Billingsley, M. M.; Haley, R. M.; Wechsler, M. E.; Peppas, N. A.; Langer, R. Engineering Precision Nanoparticles for Drug Delivery. *Nat Rev Drug Discov* **2021**, *20* (2), 101–124. <https://doi.org/10.1038/s41573-020-0090-8>.
- (20) Xu, L.; Wang, X.; Liu, Y.; Yang, G.; Falconer, R. J.; Zhao, C.-X. Lipid Nanoparticles for Drug Delivery. *Advanced NanoBiomed Research* **2022**, *2* (2), 2100109. <https://doi.org/10.1002/anbr.202100109>.
- (21) Ostro, M. J.; Giacomoni, D.; Dray, S. Incorporation of High Molecular Weight RNA into Large Artificial Lipid Vesicles. *Biochemical and Biophysical Research Communications* **1977**, *76* (3), 836–842. [https://doi.org/10.1016/0006-291X\(77\)91576-5](https://doi.org/10.1016/0006-291X(77)91576-5).
- (22) Cullis, P. R.; Felgner, P. L. The 60-Year Evolution of Lipid Nanoparticles for Nucleic Acid Delivery. *Nat Rev Drug Discov* **2024**, *23* (9), 709–722. <https://doi.org/10.1038/s41573-024-00977-6>.
- (23) Langer, R.; Folkman, J. Polymers for the Sustained Release of Proteins and Other Macromolecules. *Nature* **1976**, *263* (5580), 797–800. <https://doi.org/10.1038/263797a0>.
- (24) Hou, X.; Zaks, T.; Langer, R.; Dong, Y. Lipid Nanoparticles for mRNA Delivery. *Nat Rev Mater* **2021**, *6* (12), 1078–1094. <https://doi.org/10.1038/s41578-021-00358-0>.
- (25) Deamer, D.; Bangham, A. D. Large Volume Liposomes by an Ether Vaporization Method. *Biochimica et Biophysica Acta (BBA) - Nucleic Acids and Protein Synthesis* **1976**, *443* (3), 629–634. [https://doi.org/10.1016/0005-2787\(76\)90527-X](https://doi.org/10.1016/0005-2787(76)90527-X).
- (26) Eygeris, Y.; Gupta, M.; Kim, J.; Sahay, G. Chemistry of Lipid Nanoparticles for RNA Delivery. *Acc. Chem. Res.* **2022**, *55* (1), 2–12. <https://doi.org/10.1021/acs.accounts.1c00544>.
- (27) Wheeler, J. J.; Palmer, L.; Ossanlou, M.; MacLachlan, I.; Graham, R. W.; Zhang, Y. P.; Hope, M. J.; Scherrer, P.; Cullis, P. R. Stabilized Plasmid-Lipid Particles: Construction and Characterization. *Gene Ther* **1999**, *6* (2), 271–281. <https://doi.org/10.1038/sj.gt.3300821>.
- (28) Sun, D.; Lu, Z.-R. Structure and Function of Cationic and Ionizable Lipids for Nucleic Acid Delivery. *Pharm Res* **2023**, *40* (1), 27–46. <https://doi.org/10.1007/s11095-022-03460-2>.
- (29) Ponti, F.; Campolungo, M.; Melchiori, C.; Bono, N.; Candiani, G. Cationic Lipids for Gene Delivery: Many Players, One Goal. *Chemistry and Physics of Lipids* **2021**, *235*, 105032. <https://doi.org/10.1016/j.chemphyslip.2020.105032>.
- (30) Buschmann, M. D.; Carrasco, M. J.; Alishetty, S.; Paige, M.; Alameh, M. G.; Weissman, D. Nanomaterial Delivery Systems for mRNA Vaccines. *Vaccines* **2021**, *9* (1), 65. <https://doi.org/10.3390/vaccines9010065>.

- (31) Cheng, X.; Lee, R. J. The Role of Helper Lipids in Lipid Nanoparticles (LNPs) Designed for Oligonucleotide Delivery. *Adv Drug Deliv Rev* **2016**, *99* (Pt A), 129–137. <https://doi.org/10.1016/j.addr.2016.01.022>.
- (32) Kulkarni, J. A.; Witzigmann, D.; Leung, J.; Tam, Y. Y. C.; Cullis, P. R. On the Role of Helper Lipids in Lipid Nanoparticle Formulations of SiRNA. *Nanoscale* **2019**, *11* (45), 21733–21739. <https://doi.org/10.1039/C9NR09347H>.
- (33) Ma, X.; Wu, F.; Peng, C.; Chen, H.; Zhang, D.; Han, T. Exploration of mRNA Nanoparticles Based on DOTAP through Optimization of the Helper Lipids. *Biotechnology Journal* **2023**, *18* (11), 2300123. <https://doi.org/10.1002/biot.202300123>.
- (34) Hald Albertsen, C.; Kulkarni, J. A.; Witzigmann, D.; Lind, M.; Petersson, K.; Simonsen, J. B. The Role of Lipid Components in Lipid Nanoparticles for Vaccines and Gene Therapy. *Advanced Drug Delivery Reviews* **2022**, *188*, 114416. <https://doi.org/10.1016/j.addr.2022.114416>.
- (35) Álvarez-Benedicto, E.; Farbiak, L.; Ramírez, M. M.; Wang, X.; T. Johnson, L.; Mian, O.; D. Guerrero, E.; J. Siegwart, D. Optimization of Phospholipid Chemistry for Improved Lipid Nanoparticle (LNP) Delivery of Messenger RNA (mRNA). *Biomaterials Science* **2022**, *10* (2), 549–559. <https://doi.org/10.1039/D1BM01454D>.
- (36) Zhigaltsev, I. V.; Cullis, P. R. Morphological Behavior of Liposomes and Lipid Nanoparticles. *Langmuir* **2023**, *39* (9), 3185–3193. <https://doi.org/10.1021/acs.langmuir.2c02794>.
- (37) Zhang, Y.; Sun, C.; Wang, C.; Jankovic, K. E.; Dong, Y. Lipids and Lipid Derivatives for RNA Delivery. *Chem. Rev.* **2021**, *121* (20), 12181–12277. <https://doi.org/10.1021/acs.chemrev.1c00244>.
- (38) Li, S.; Hu, Y.; Li, A.; Lin, J.; Hsieh, K.; Schneiderman, Z.; Zhang, P.; Zhu, Y.; Qiu, C.; Kokkoli, E.; Wang, T.-H.; Mao, H.-Q. Payload Distribution and Capacity of mRNA Lipid Nanoparticles. *Nat Commun* **2022**, *13*, 5561. <https://doi.org/10.1038/s41467-022-33157-4>.
- (39) Evers, M. J. W.; Kulkarni, J. A.; Van Der Meel, R.; Cullis, P. R.; Vader, P.; Schiffelers, R. M. State-of-the-Art Design and Rapid-Mixing Production Techniques of Lipid Nanoparticles for Nucleic Acid Delivery. *Small Methods* **2018**, *2* (9), 1700375. <https://doi.org/10.1002/smt.201700375>.
- (40) Mehta, M.; Bui, T. A.; Yang, X.; Aksoy, Y.; Goldys, E. M.; Deng, W. Lipid-Based Nanoparticles for Drug/Gene Delivery: An Overview of the Production Techniques and Difficulties Encountered in Their Industrial Development. *ACS Mater. Au* **2023**, *3* (6), 600–619. <https://doi.org/10.1021/acsmaterialsau.3c00032>.
- (41) Catenacci, L.; Rossi, R.; Sechi, F.; Buonocore, D.; Sorrenti, M.; Perteghella, S.; Peviani, M.; Bonferoni, M. C. Effect of Lipid Nanoparticle Physico-Chemical Properties and Composition on Their Interaction with the Immune System. *Pharmaceutics* **2024**, *16* (12), 1521. <https://doi.org/10.3390/pharmaceutics16121521>.
- (42) Schoenmaker, L.; Witzigmann, D.; Kulkarni, J. A.; Verbeke, R.; Kersten, G.; Jiskoot, W.; Crommelin, D. J. A. mRNA-Lipid Nanoparticle COVID-19 Vaccines: Structure and Stability. *International Journal of Pharmaceutics* **2021**, *601*, 120586. <https://doi.org/10.1016/j.ijpharm.2021.120586>.
- (43) John, R.; Monpara, J.; Swaminathan, S.; Kalhapure, R. Chemistry and Art of Developing Lipid Nanoparticles for Biologics Delivery: Focus on Development and Scale-Up. *Pharmaceutics* **2024**, *16* (1), 131. <https://doi.org/10.3390/pharmaceutics16010131>.
- (44) Ma, Y.; Li, S.; Lin, X.; Chen, Y. A Perspective of Lipid Nanoparticles for RNA Delivery. *Exploration* **2024**, *4* (6), 20230147. <https://doi.org/10.1002/EXP.20230147>.

- (45) Kulkarni, J. A.; Witzigmann, D.; Chen, S.; Cullis, P. R.; Van Der Meel, R. Lipid Nanoparticle Technology for Clinical Translation of SiRNA Therapeutics. *Acc. Chem. Res.* **2019**, *52* (9), 2435–2444. <https://doi.org/10.1021/acs.accounts.9b00368>.
- (46) Tang, M.; Sagawa, A.; Inoue, N.; Torii, S.; Tomita, K.; Hattori, Y. Efficient mRNA Delivery with mRNA Lipoplexes Prepared Using a Modified Ethanol Injection Method. *Pharmaceutics* **2023**, *15* (4), 1141. <https://doi.org/10.3390/pharmaceutics15041141>.
- (47) Hattori, Y.; Tang, M.; Sato, J.; Tsuiji, M.; Kawano, K. Evaluation of mRNA Lipoplexes Prepared Using Modified Ethanol Injection Method as a Tumour Vaccine. *Journal of Drug Targeting* **2024**, *32* (10), 1267–1277. <https://doi.org/10.1080/1061186X.2024.2384074>.
- (48) Shepherd, S. J.; Issadore, D.; Mitchell, M. J. Microfluidic Formulation of Nanoparticles for Biomedical Applications. *Biomaterials* **2021**, *274*, 120826. <https://doi.org/10.1016/j.biomaterials.2021.120826>.
- (49) Maeki, M.; Uno, S.; Niwa, A.; Okada, Y.; Tokeshi, M. Microfluidic Technologies and Devices for Lipid Nanoparticle-Based RNA Delivery. *Journal of Controlled Release* **2022**, *344*, 80–96. <https://doi.org/10.1016/j.jconrel.2022.02.017>.
- (50) Precision Nanosystems. NxGen TM - A Disruptive Technology Enabling Transformative Medicine. <https://www.precisionnanosystems.com/platform-technologies/nxgen> (accessed 4 Aug 2025).
- (51) Knauer. Impingement Jets Mixing Skids for high-flow production of nanoparticles (LNP, microemulsions, etc.), **2022**. https://www.knauer.net/en/Systems-Solutions/LNP_lipid_nanoparticles/impingement-jets-mixing-skids-for-high-flow-production-of-nanoparticles (accessed 4 Aug 2025).
- (52) Qin, M.; Du, G.; Sun, X. Recent Advances in the Noninvasive Delivery of mRNA. *Acc. Chem. Res.* **2021**, *54* (23), 4262–4271. <https://doi.org/10.1021/acs.accounts.1c00493>.
- (53) Litvinova, V. R.; Rudometov, A. P.; Karpenko, L. I.; Ilyichev, A. A. mRNA Vaccine Platform: mRNA Production and Delivery. *Russ J Bioorg Chem* **2023**, *49* (2), 220–235. <https://doi.org/10.1134/S1068162023020152>.
- (54) Wang, Y.; Zhang, L.; Xu, Z.; Miao, L.; Huang, L. mRNA Vaccine with Antigen-Specific Checkpoint Blockade Induces an Enhanced Immune Response against Established Melanoma. *Molecular Therapy* **2018**, *26* (2), 420–434. <https://doi.org/10.1016/j.ymthe.2017.11.009>.
- (55) Oude Blenke, E.; Örnkvist, E.; Schöneich, C.; Nilsson, G. A.; Volkin, D. B.; Mastrobattista, E.; Almarsson, Ö.; Crommelin, D. J. A. The Storage and In-Use Stability of mRNA Vaccines and Therapeutics: Not A Cold Case. *Journal of Pharmaceutical Sciences* **2023**, *112* (2), 386–403. <https://doi.org/10.1016/j.xphs.2022.11.001>.
- (56) Liu, T.; Tian, Y.; Zheng, A.; Cui, C. Design Strategies for and Stability of mRNA–Lipid Nanoparticle COVID-19 Vaccines. *Polymers* **2022**, *14* (19), 4195. <https://doi.org/10.3390/polym14194195>.
- (57) Chheda, U.; Pradeepan, S.; Esposito, E.; Strezsak, S.; Fernandez-Delgado, O.; Kranz, J. Factors Affecting Stability of RNA – Temperature, Length, Concentration, pH, and Buffering Species. *Journal of Pharmaceutical Sciences* **2024**, *113* (2), 377–385. <https://doi.org/10.1016/j.xphs.2023.11.023>.
- (58) Reinhart, A.-G.; Osterwald, A.; Ringler, P.; Leiser, Y.; Lauer, M. E.; Martin, R. E.; Ullmer, C.; Schumacher, F.; Korn, C.; Keller, M. Investigations into mRNA Lipid Nanoparticles Shelf-Life

- Stability under Nonfrozen Conditions. *Mol. Pharmaceutics* **2023**, *20* (12), 6492–6503. <https://doi.org/10.1021/acs.molpharmaceut.3c00956>.
- (59) Zhang, H.; Barz, M. Investigating the Stability of RNA-Lipid Nanoparticles in Biological Fluids: Unveiling Its Crucial Role for Understanding LNP Performance. *Journal of Controlled Release* **2025**, *381*, 113559. <https://doi.org/10.1016/j.jconrel.2025.02.055>.
 - (60) Arte, K. S.; Chen, M.; Patil, C. D.; Huang, Y.; Qu, L.; Zhou, Q. Recent Advances in Drying and Development of Solid Formulations for Stable mRNA and siRNA Lipid Nanoparticles. *Journal of Pharmaceutical Sciences* **2025**, *114* (2), 805–815. <https://doi.org/10.1016/j.xphs.2024.12.013>.
 - (61) Pogocki, D.; Schöneich, C. Chemical Stability of Nucleic Acid-Derived Drugs. *Journal of Pharmaceutical Sciences* **2000**, *89* (4), 443–456. [https://doi.org/10.1002/\(SICI\)1520-6017\(200004\)89:4%3C443::AID-JPS2%3E3.0.CO;2-W](https://doi.org/10.1002/(SICI)1520-6017(200004)89:4%3C443::AID-JPS2%3E3.0.CO;2-W).
 - (62) Kornienko, I. V.; Aramova, O. Yu.; Tishchenko, A. A.; Rudoy, D. V.; Chikindas, M. L. RNA Stability: A Review of the Role of Structural Features and Environmental Conditions. *Molecules* **2024**, *29* (24), 5978. <https://doi.org/10.3390/molecules29245978>.
 - (63) Kamiya, M.; Matsumoto, M.; Yamashita, K.; Izumi, T.; Kawaguchi, M.; Mizukami, S.; Tsurumaru, M.; Mukai, H.; Kawakami, S. Stability Study of mRNA-Lipid Nanoparticles Exposed to Various Conditions Based on the Evaluation between Physicochemical Properties and Their Relation with Protein Expression Ability. *Pharmaceutics* **2022**, *14* (11), 2357. <https://doi.org/10.3390/pharmaceutics14112357>.
 - (64) Zhang, K.; Hodge, J.; Chatterjee, A.; Moon, T. S.; Parker, K. M. Duplex Structure of Double-Stranded RNA Provides Stability against Hydrolysis Relative to Single-Stranded RNA. *Environ. Sci. Technol.* **2021**, *55* (12), 8045–8053. <https://doi.org/10.1021/acs.est.1c01255>.
 - (65) Kai, Z.; Yuting, W.; Yulin, L.; Jun, L.; Juanjuan, H. An Efficient Simulated Annealing Algorithm for the RNA Secondary Structure Prediction with Pseudoknots. *BMC Genomics* **2019**, *20* (13), 979. <https://doi.org/10.1186/s12864-019-6300-2>.
 - (66) Butcher, S. E.; Pyle, A. M. The Molecular Interactions That Stabilize RNA Tertiary Structure: RNA Motifs, Patterns, and Networks. *Acc. Chem. Res.* **2011**, *44* (12), 1302–1311. <https://doi.org/10.1021/ar200098t>.
 - (67) Houseley, J.; Tollervey, D. The Many Pathways of RNA Degradation. *Cell* **2009**, *136* (4), 763–776. <https://doi.org/10.1016/j.cell.2009.01.019>.
 - (68) Yang, W. Nucleases: Diversity of Structure, Function and Mechanism. *Quart. Rev. Biophys.* **2011**, *44* (1), 1–93. <https://doi.org/10.1017/S0033583510000181>.
 - (69) Mikutis, S.; Bernardes, G. J. L. Technologies for Targeted RNA Degradation and Induced RNA Decay. *Chem. Rev.* **2024**, *124* (23), 13301–13330. <https://doi.org/10.1021/acs.chemrev.4c00472>.
 - (70) Tatosyan, K. A.; Ustyantsev, I. G.; Kramerov, D. A. RNA Degradation in Eukaryotic Cells. *Mol Biol* **2020**, *54* (4), 485–502. <https://doi.org/10.1134/S0026893320040159>.
 - (71) Sorrentino, S. The Eight Human “Canonical” Ribonucleases: Molecular Diversity, Catalytic Properties, and Special Biological Actions of the Enzyme Proteins. *FEBS Letters* **2010**, *584* (11), 2194–2200. <https://doi.org/10.1016/j.febslet.2010.04.018>.
 - (72) Sorrentino, S.; Libonati, M. Structure–Function Relationships in Human Ribonucleases: Main Distinctive Features of the Major RNase Types. *FEBS Letters* **1997**, *404* (1), 1–5. [https://doi.org/10.1016/S0014-5793\(97\)00086-0](https://doi.org/10.1016/S0014-5793(97)00086-0).
 - (73) Luhtala, N.; Parker, R. T2 Family Ribonucleases: Ancient Enzymes with Diverse Roles. *Trends Biochem Sci* **2010**, *35* (5), 253–259. <https://doi.org/10.1016/j.tibs.2010.02.002>.
 - (74) Sarvepalli, S.; Pasika, S. R.; Verma, V.; Thumma, A.; Bolla, S.; Nukala, P. K.; Butreddy, A.; Bolla, P. K. A Review on the Stability Challenges of Advanced Biologic Therapeutics. *Pharmaceutics* **2025**, *17* (5), 550. <https://doi.org/10.3390/pharmaceutics17050550>.
 - (75) Ball, R. L.; Bajaj, P.; Whitehead, K. A. Achieving Long-Term Stability of Lipid Nanoparticles: Examining the Effect of pH, Temperature, and Lyophilization. *Int J Nanomedicine* **2017**, *12*, 305–

315. <https://doi.org/10.2147/IJN.S123062>.
- (76) Ayat, N. R.; Sun, Z.; Sun, D.; Yin, M.; Hall, R. C.; Vaidya, A. M.; Liu, X.; Schilb, A. L.; Scheidt, J. H.; Lu, Z.-R. Formulation of Biocompatible Targeted ECO/siRNA Nanoparticles with Long-Term Stability for Clinical Translation of RNAi. *Nucleic Acid Therapeutics* **2019**, 29 (4), 195–207. <https://doi.org/10.1089/nat.2019.0784>.
 - (77) CDC. *Moderna COVID-19 Vaccine Summary*. Vaccines & Immunizations. <https://www.cdc.gov/vaccines/php/info-by-product/moderna-covid-19-summary.html> (accessed 2025-07-02).
 - (78) CDC. *Pfizer COVID-19 Vaccine Summary*. Vaccines & Immunizations. <https://www.cdc.gov/vaccines/php/info-by-product/pfizer-covid-19-summary.html> (accessed 2025-08-25).
 - (79) Pfizer Medical, COMIRNATY® (COVID-19 Vaccine, mRNA) (2025-2026 Formula) How Supplied/Storage and Handling. <https://www.pfizermedical.com/pfizer-biontech-covid-19-vaccine/storage-handling> (accessed 2025-12-26).
 - (80) Center for Drug Evaluation and Research. *ONPATTRO (patisiran) Lipid Complex Injection Addendum to Drug Product Quality Review*. 4305519; FDA, 2017. https://www.accessdata.fda.gov/drugsatfda_docs/nda/2018/210922Orig1s000ChemR.pdf (accessed 2025-08-25).
 - (81) Veiga, N.; Diesendruck, Y.; Peer, D. Targeted Lipid Nanoparticles for RNA Therapeutics and Immunomodulation in Leukocytes. *Advanced Drug Delivery Reviews* **2020**, 159, 364–376. <https://doi.org/10.1016/j.addr.2020.04.002>.
 - (82) Ma, Y.; VanKeulen-Miller, R.; Fenton, O. S. mRNA Lipid Nanoparticle Formulation, Characterization and Evaluation. *Nat Protoc* **2025**, 20 (9), 2618–2651. <https://doi.org/10.1038/s41596-024-01134-4>.
 - (83) McKenzie, R. E.; Minnell, J. J.; Ganley, M.; Painter, G. F.; Draper, S. L. mRNA Synthesis and Encapsulation in Ionizable Lipid Nanoparticles. *Current Protocols* **2023**, 3 (9), e898. <https://doi.org/10.1002/cpz1.898>.
 - (84) Guimaraes, G. J.; Kim, J.; Bartlett, M. G. Characterization of mRNA Therapeutics. *Mass Spectrometry Reviews* **2024**, 43 (5), 1066–1090. <https://doi.org/10.1002/mas.21856>.
 - (85) Nogueira, S. S.; Samaridou, E.; Simon, J.; Frank, S.; Beck-Broichsitter, M.; Mehta, A. Analytical Techniques for the Characterization of Nanoparticles for mRNA Delivery. *European Journal of Pharmaceutics and Biopharmaceutics* **2024**, 198, 114235. <https://doi.org/10.1016/j.ejpb.2024.114235>.
 - (86) Leighton, L. J.; Chaudhary, N.; Tompkins, H. T.; Kulkarni, A.; Carroddus, N. L.; Budzinska, M. A.; Lakshman Das, S.; Cheetham, S. W.; Mercer, T. R. The Design, Manufacture and LNP Formulation of MRNA for Research Use. *Nat Protoc* **2025**, 1–30. <https://doi.org/10.1038/s41596-025-01174-4>.
 - (87) Pharmacopeia, U. S. *Analytical Procedures for mRNA Vaccine Quality - Draft Guidelines*, 3rd ed. USP, 2024. <https://go.usp.org/mRNAVaccineQuality> (accessed 2025-07-02).
 - (88) EMA. *Guideline on the quality aspects of mRNA vaccine*. EMA/CHMP/BWP/82416/2025; https://www.ema.europa.eu/en/documents/scientific-guideline/draft-guideline-quality-aspects-mrna-vaccines_en.pdf (accessed 2025-12-28)
 - (89) Alnylam Pharmaceuticals. *Patisiran Product Specific Guidance (PSG_210922) Product-Specific Guidances; Draft and Revised Draft Guidances for Industry*. FDA-2007-D-0369; FDA, 2023. (accessed 2025-12-28)
 - (90) Guerriaud, M.; Kohli, E. RNA-Based Drugs and Regulation: Toward a Necessary Evolution of the Definitions Issued from the European Union Legislation. *Front. Med.* **2022**, 9.

- <https://doi.org/10.3389/fmed.2022.1012497>.
- (91) FDA, *Drug Products, Including Biological Products, that Contain Nanomaterials - Guidance for Industry*. FDA-2017-D-0759; 2022. <https://www.fda.gov/regulatory-information/search-fda-guidance-documents/drug-products-including-biological-products-contain-nanomaterials-guidance-industry> (accessed 2025-12-29)
 - (92) EMA, *Orphan Maintenance Assessment Report Onpattro (Synthetic double-stranded siRNA oligonucleotide directed against transthyretin mRNA) Treatment of transthyretin-mediated amyloidosis*. EMA/564536/2018; EMA, 2018. https://www.ema.europa.eu/en/documents/orphan-maintenance-report/onpattro-orphan-maintenance-assessment-report-initial-authorisation_en.pdf (accessed 2025-12-30)
 - (93) Somara, S.; Heidaran, M. Lipid Nanoparticle – Points to Consider in Assessing Materials Quality for RNA-Based Therapeutics. *Cytotherapy* **2025**, 102044. <https://doi.org/10.1016/j.jcyt.2025.102044>.
 - (94) Glush, G. L.; Vachet, R. W. The Basics of Mass Spectrometry in the Twenty-First Century. *Nat Rev Drug Discov* **2003**, 2 (2), 140–150. <https://doi.org/10.1038/nrd1011>.
 - (95) El-Aneel, A.; Cohen, A.; Banoub, J. Mass Spectrometry, Review of the Basics: Electrospray, MALDI, and Commonly Used Mass Analyzers. *Applied Spectroscopy Reviews* **2009**, 44 (3), 210–230. <https://doi.org/10.1080/05704920902717872>.
 - (96) Xian, F.; Hendrickson, C. L.; Marshall, A. G. High Resolution Mass Spectrometry. *Anal. Chem.* **2012**, 84 (2), 708–719. <https://doi.org/10.1021/ac203191t>.
 - (97) Thomas, B.; Akoulitchiev, A. V. Mass Spectrometry of RNA. *Trends in Biochemical Sciences* **2006**, 31 (3), 173–181. <https://doi.org/10.1016/j.tibs.2006.01.004>.
 - (98) Trimpin, S. “Magic” Ionization Mass Spectrometry. *J. Am. Soc. Mass Spectrom.* **2016**, 27 (1), 4–21. <https://doi.org/10.1007/s13361-015-1253-4>.
 - (99) Banerjee, S.; Mazumdar, S. Electrospray Ionization Mass Spectrometry: A Technique to Access the Information beyond the Molecular Weight of the Analyte. *International Journal of Analytical Chemistry* **2012**, 2012, 1–40. <https://doi.org/10.1155/2012/282574>.
 - (100) Kind, T.; Fiehn, O. Advances in Structure Elucidation of Small Molecules Using Mass Spectrometry. *Bioanal Rev* **2010**, 2 (1), 23–60. <https://doi.org/10.1007/s12566-010-0015-9>.
 - (101) Ma, X. Recent Advances in Mass Spectrometry-Based Structural Elucidation Techniques. *Molecules* **2022**, 27 (19), 6466. <https://doi.org/10.3390/molecules27196466>.
 - (102) Michalski, R.; Jabłonska, M.; Szopa, S.; Łyko, A. Application of Ion Chromatography with ICP-MS or MS Detection to the Determination of Selected Halides and Metal/Metalloids Species. *Critical Reviews in Analytical Chemistry* **2011**, 41 (2), 133–150. <https://doi.org/10.1080/10408347.2011.559438>.
 - (103) Laiko, V. V.; Baldwin, M. A.; Burlingame, A. L. Atmospheric Pressure Matrix-Assisted Laser Desorption/Ionization Mass Spectrometry. *Anal. Chem.* **2000**, 72 (4), 652–657. <https://doi.org/10.1021/ac990998k>.
 - (104) Jakubowski, N.; Moens, L.; Vanhaecke, F. Sector Field Mass Spectrometers in ICP-MS. *Spectrochimica Acta Part B: Atomic Spectroscopy* **1998**, 53 (13), 1739–1763. [https://doi.org/10.1016/S0584-8547\(98\)00222-5](https://doi.org/10.1016/S0584-8547(98)00222-5).
 - (105) Bahureksa, W.; Borch, T.; Young, R. B.; Weisbrod, C. R.; Blakney, G. T.; McKenna, A. M. Improved Dynamic Range, Resolving Power, and Sensitivity Achievable with FT-ICR Mass Spectrometry at 21 T Reveals the Hidden Complexity of Natural Organic Matter. *Anal Chem* **2022**, 94 (32), 11382–11389. <https://doi.org/10.1021/acs.analchem.2c02377>.
 - (106) Adams, F.; Barbante, C. History and Present Status of Micro- and Nano-Imaging Analysis. In *Comprehensive Analytical Chemistry*; Elsevier, 2015; Vol. 69, pp 67–124. <https://doi.org/10.1016/B978-0-444-63439-9.00003-7>.
 - (107) Li, C.; Chu, S.; Tan, S.; Yin, X.; Jiang, Y.; Dai, X.; Gong, X.; Fang, X.; Tian, D. Towards Higher Sensitivity of Mass Spectrometry: A Perspective From the Mass Analyzers. *Front. Chem.* **2021**, 9.

- <https://doi.org/10.3389/fchem.2021.813359>.
- (108) Selby, D. S.; Mlynski, V.; Guilhaus, M. A 20 kV Orthogonal Acceleration Time-of-Flight Mass Spectrometer for Matrix-Assisted Laser Desorption/Ionization1. *International Journal of Mass Spectrometry* **2001**, 210–211, 89–100. [https://doi.org/10.1016/S1387-3806\(01\)00438-9](https://doi.org/10.1016/S1387-3806(01)00438-9).
 - (109) Lee, J.; Chen, H.; Liu, T.; Berkman, C. E.; Reilly, P. T. A. High Resolution Time-of-Flight Mass Analysis of the Entire Range of Intact Singly-Charged Proteins. *Anal Chem* **2011**, 83 (24), 9406–9412. <https://doi.org/10.1021/ac202001z>.
 - (110) Verenchikov, A. N.; Kirillov, S. N.; Vorobyev, A. V.; Makarov, V. V.; Yavor, M. I.; Tonge, R. P.; Langridge, J. I. Multi Reflecting TOF MS Approaching Resolution of 1,000,000 in a Wide Mass Range. *International Journal of Mass Spectrometry* **2025**, 508, 117395. <https://doi.org/10.1016/j.ijms.2024.117395>.
 - (111) Cooper-Shepherd, D. A.; Wildgoose, J.; Kozlov, B.; Johnson, W. J.; Tyldesley-Worster, R.; Palmer, M. E.; Hoyes, J. B.; McCullagh, M.; Jones, E.; Tonge, R.; Marsden-Edwards, E.; Nixon, P.; Verenchikov, A.; Langridge, J. I. Novel Hybrid Quadrupole-Multireflecting Time-of-Flight Mass Spectrometry System. *J. Am. Soc. Mass Spectrom.* **2023**, 34 (2), 264–272. <https://doi.org/10.1021/jasms.2c00281>.
 - (112) Czerwieniec, G. A.; Russell, S. C.; Lebrilla, C. B.; Coffee, K. R.; Riot, V.; Steele, P. T.; Frank, M.; Gard, E. E. Improved Sensitivity and Mass Range in Time-of-Flight Bioaerosol Mass Spectrometry Using an Electrostatic Ion Guide. *Journal of the American Society for Mass Spectrometry* **2005**, 16 (11), 1866–1875. <https://doi.org/10.1016/j.jasms.2005.06.013>.
 - (113) Zubarev, R. A.; Makarov, A. Orbitrap Mass Spectrometry. *Anal. Chem.* **2013**, 85 (11), 5288–5296. <https://doi.org/10.1021/ac4001223>.
 - (114) Orbitrap Mass Spectrometry: Evolution and Applicability. In *Comprehensive Analytical Chemistry*; Elsevier, 2016; Vol. 71, pp 3–18. <https://doi.org/10.1016/bs.coac.2016.01.001>.
 - (115) Niessen, W. M. A. MS–MS and MSn. In *Encyclopedia of Spectroscopy and Spectrometry*; Elsevier, 1999; pp 1675–1681. <https://doi.org/10.1016/B978-0-12-374413-5.00215-3>.
 - (116) Qi, Y.; Volmer, D. A. Electron-based Fragmentation Methods in Mass Spectrometry: An Overview. *Mass Spectrometry Reviews* **2017**, 36 (1), 4–15. <https://doi.org/10.1002/mas.21482>.
 - (117) Špánik, I.; Machyňáková, A. Recent Applications of Gas Chromatography with High-resolution Mass Spectrometry. *J of Separation Science* **2018**, 41 (1), 163–179. <https://doi.org/10.1002/jssc.201701016>.
 - (118) Rodriguez-Aller, M.; Gurny, R.; Veuthey, J.-L.; Guillaume, D. Coupling Ultra High-Pressure Liquid Chromatography with Mass Spectrometry: Constraints and Possible Applications. *Journal of Chromatography A* **2013**, 1292, 2–18. <https://doi.org/10.1016/j.chroma.2012.09.061>.
 - (119) Guillaume, D.; Schappler, J.; Rudaz, S.; Veuthey, J.-L. Coupling Ultra-High-Pressure Liquid Chromatography with Mass Spectrometry. *TrAC Trends in Analytical Chemistry* **2010**, 29 (1), 15–27. <https://doi.org/10.1016/j.trac.2009.09.008>.
 - (120) Týčová, A.; Ledvina, V.; Klepárník, K. Recent Advances in CE-MS Coupling: Instrumentation, Methodology, and Applications. *Electrophoresis* **2017**, 38 (1), 115–134. <https://doi.org/10.1002/elps.201600366>.
 - (121) Xie, Y.; Brás-Costa, C.; Lin, Z.; Garcia, B. A. Mass Spectrometry Analysis of Nucleic Acid Modifications: From Beginning to Future. *Mass Spectrometry Reviews* **2024**, mas.21907. <https://doi.org/10.1002/mas.21907>.
 - (122) Oberacher, H. Frontiers of Mass Spectrometry in Nucleic Acids Analysis. *Eur J Mass Spectrom (Chichester)* **2010**, 16 (3), 351–365. <https://doi.org/10.1255/ejms.1045>.
 - (123) Nordhoff, E.; Kirpekar, F.; Roepstorff, P. Mass Spectrometry of Nucleic Acids. *Mass Spectrom. Rev.* **1996**, 15 (2), 67–138. [https://doi.org/10.1002/\(SICI\)1098-2787\(1996\)15:2%253C67::AID-MAS1%253E3.0.CO;2-8](https://doi.org/10.1002/(SICI)1098-2787(1996)15:2%253C67::AID-MAS1%253E3.0.CO;2-8).
 - (124) Lanzillotti, M. B.; Brodbelt, J. S. Progress in Tandem Mass Spectrometry Data Analysis for Nucleic Acids. *Mass Spectrometry Reviews* **2025**, mas.21923. <https://doi.org/10.1002/mas.21923>.
 - (125) Schürch, S. Characterization of Nucleic Acids by Tandem Mass Spectrometry - The Second

- Decade (2004–2013): From DNA to RNA and Modified Sequences. *Mass Spectrometry Reviews* **2016**, 35 (4), 483–523. <https://doi.org/10.1002/mas.21442>.
- (126) Lowenthal, M. S.; Antonishek, A. S.; Phinney, K. W. Quantification of mRNA in Lipid Nanoparticles Using Mass Spectrometry. *Anal. Chem.* **2024**, 96 (3), 1214–1222. <https://doi.org/10.1021/acs.analchem.3c04406>.
- (127) Biemann, K.; McCloskey, J. A. **Application of Mass Spectrometry to Structure Problems.**¹ **VI. Nucleosides**². *J. Am. Chem. Soc.* **1962**, 84 (10), 2005–2007. <https://doi.org/10.1021/ja00869a048>.
- (128) Fekete, S.; Doneanu, C.; Addepalli, B.; Gaye, M.; Nguyen, J.; Alden, B.; Birdsall, R.; Han, D.; Isaac, G.; Lauber, M. Challenges and Emerging Trends in Liquid Chromatography-Based Analyses of mRNA Pharmaceuticals. *J Pharm Biomed Anal* **2023**, 224, 115174. <https://doi.org/10.1016/j.jpba.2022.115174>.
- (129) Menneteau, T.; Butré, C. I.; Mouvet, D.; Delobel, A. Multi-Attribute Monitoring of Therapeutic mRNA by Liquid Chromatography–Mass Spectrometry. *LCGC Eur.* **2023**, 18–24. <https://doi.org/10.56530/lcgc.eu.fd3584v4>.
- (130) Camperi, J.; Lippold, S.; Ayalew, L.; Roper, B.; Shao, S.; Freund, E.; Nissenbaum, A.; Galan, C.; Cao, Q.; Yang, F.; Yu, C.; Guilbaud, A. Comprehensive Impurity Profiling of mRNA: Evaluating Current Technologies and Advanced Analytical Techniques. *Anal. Chem.* **2024**, 96 (9), 3886–3897. <https://doi.org/10.1021/acs.analchem.3c05539>.
- (131) Jiang, T.; Yu, N.; Kim, J.; Murgo, J.-R.; Kissai, M.; Ravichandran, K.; Miracco, E. J.; Presnyak, V.; Hua, S. Oligonucleotide Sequence Mapping of Large Therapeutic mRNAs via Parallel Ribonuclease Digestions and LC-MS/MS. *Anal. Chem.* **2019**, 91 (13), 8500–8506. <https://doi.org/10.1021/acs.analchem.9b01664>.
- (132) Tang, S.; Liu, G.-Y.; Yan, Y.; Wang, S.; Li, N. Development of a Flow Through-Based Limited Digestion Approach for High-Throughput and High-Sequence Coverage Mapping of Therapeutic mRNAs. *Anal. Chem.* **2024**, 96 (42), 16994–17003. <https://doi.org/10.1021/acs.analchem.4c04384>.
- (133) Strupat, K.; Busse-Patel, F.; Hartmer, R. Concept for High-Throughput mRNA Sequence Confirmation by Atmospheric Pressure MALDI Technique Applied to RNA Digestion Products. *International Journal of Mass Spectrometry* **2025**, 518, 117510. <https://doi.org/10.1016/j.ijms.2025.117510>.
- (134) N. Welbourne, E.; J. Copley, R.; R. Owen, G.; A. Evans, C.; Isoko, K.; Cook, K.; Cordiner, J.; Kis, Z.; Z. Moghadam, P.; J. Dickman, M. Mass Spectrometry-Based mRNA Sequence Mapping via Complementary RNase Digests and Bespoke Visualisation Tools. *Analyst* **2025**, 150 (5), 1012–1021. <https://doi.org/10.1039/D5AN00033E>.
- (135) Jones, J. D.; Grassmyer, K. T.; Kennedy, R. T.; Koutmou, K. S.; Maloney, T. D. Nuclease P1 Digestion for Bottom-Up RNA Sequencing of Modified siRNA Therapeutics. *Anal. Chem.* **2023**, 95 (9), 4404–4411. <https://doi.org/10.1021/acs.analchem.2c04902>.
- (136) You, X.-J.; Yuan, B.-F. Detecting Internal N7-Methylguanosine mRNA Modifications by Differential Enzymatic Digestion Coupled with Mass Spectrometry Analysis. In *RNA Modifications: Methods and Protocols*; McMahon, M., Ed.; Springer US: New York, NY, 2021; pp 247–259. https://doi.org/10.1007/978-1-0716-1374-0_16.
- (137) Kinsey, C.; Lu, T.; Deiss, A.; Vuolo, K.; Klein, L.; Rustandi, R. R.; Loughney, J. W. Determination of Lipid Content and Stability in Lipid Nanoparticles Using Ultra High-performance Liquid Chromatography in Combination with a Corona Charged Aerosol Detector. *Electrophoresis* **2022**, 43 (9–10), 1091–1100. <https://doi.org/10.1002/elps.202100244>.
- (138) Crowe A.; Jain N.; Higgins R.; Proos R.; Stone M.; Pohl K. Distinguishing Oxidative Impurities from Ionizable Lipids Used in LNP Formulations Using Electron Activated Dissociation Achieving Structural Elucidation and Distinction of Oxidative Isomer Impurities of Lipids with Electron-Activated Dissociation (EAD) and the ZenoTOF 7600 System. 2022. https://sciex.com/content/dam/SCIEX/tech-notes/biopharma/ruo-mkt-02-14983-a/RUO-MKT-02-14983-A_Lipid%20impurity%20structural%20elucidation%20with%20EAD.pdf (accessed 2026-01-29)

- (139) Malburet, C.; Carboni, A.; Guinamand, S.; Naik, H.; Fertier-Prizzon, S. mRNA Extraction from Lipid Nanoparticles. *Journal of Chromatography A* **2024**, *1714*, 464545. <https://doi.org/10.1016/j.chroma.2023.464545>.
- (140) Schneeberger E.; Jiang T. Expanding the Horizon: LC-MS approaches for intact mass spectrometry of pharmaceutical mRNA up to 2000-nt long. *ASMS Conference*. **2021**.
- (141) Camperi, J.; Chatla, K.; Freund, E.; Galan, C.; Lippold, S.; Guilbaud, A. Current Analytical Strategies for mRNA-Based Therapeutics. *Molecules* **2025**, *30* (7), 1629. <https://doi.org/10.3390/molecules30071629>.
- (142) Brophy P.; Shion H.; Doneanu C.; H Yang BD.; Botamanenko D.; Abbatiello S.; Jarrell A.; Koza S.; Yu Y.; Giles K.; Jarrold M. Characterization of intact mRNA using IP-RP-TOF-MS, SEC MALS and CDMS. *ASMS Conference*. Poster. **2022**. <https://www.waters.com/content/dam/waters/fr/library/posters/2022/waters-poster-CharacterizationofIntactmRNAUsingIonPairReversedPhaseTimeofFlightMS-PSTR135098898.pdf> (accessed 2026-01-30)
- (143) Deslignière, E.; Barnes, L. F.; Powers, T. W.; Friese, O. V.; Heck, A. J. R. Characterization of Intact mRNA-Based Therapeutics by Charge Detection Mass Spectrometry and Mass Photometry. *Molecular Therapy Methods & Clinical Development* **2025**, *33* (2), 101454. <https://doi.org/10.1016/j.omtm.2025.101454>.
- (144) Afroz, R.; Bowen, K.; Liu, W.; Gadkari, V. Native Charge Detection Mass Spectrometry of Kilobase-Scale Messenger RNAs. January 13, 2026. <https://doi.org/10.26434/chemrxiv-2026-1w4ct-v2>.
- (145) ThermoFisher Scientific. *Quant-iT™ RiboGreen™ RNA Reagent and Kit User Guide*. Pub. No. MAN0002073; 2022. <https://documents.thermofisher.com/TFS-Assets/LSG/manuals/mp11490.pdf> (accessed 2026-04-25).
- (146) Agrawal, K.; Ji, S.; Jian, W. Simultaneous Quantification of siRNA Antisense and Sense Strands by Hybrid Liquid Chromatography-Mass Spectrometry. *Bioanalysis* **2025**, *17* (4), 249–259. <https://doi.org/10.1080/17576180.2025.2457894>.
- (147) Song, Z.; Yuan, L. A Novel Hybrid LC-MS/MS Methodology for the Quantitative Bioanalysis of Antibody-siRNA Conjugates. *Anal. Chem.* **2025**, *97* (36), 19570–19577. <https://doi.org/10.1021/acs.analchem.5c02727>.

Chapter 6: Appendix

Table 6.1: List of Abbreviations

Abbreviation	Meaning
VEGF	Vascular endothelial growth factor
IR	Infrared
NMR	Nuclear magnetic resonance
DLin-MC3-DMA	(6Z,9Z,28Z,31Z)-heptatriaconta-6,9,28,31-tetraen-19-yl 4-(dimethylamino) butanoate
SM-102	heptadecan-9-yl 8-((2-hydroxyethyl)(6-oxo-6-(undecyloxy)hexyl)amino) octanoate
ALC-0315	(4-hydroxybutyl)azanediyl)bis(hexane-6,1-diyl) bis(2-hexyldecanoate)
DOPC	1,2-dioleoyl-sn-glycero-3-phosphocholine
mPEG ₂₀₀₀ -DSPE	methoxy-polyethylene glycol (M.W. 2000)-distearoylphosphatidylethanolamine
PEG ₂₀₀₀ -C-DMG	N,N-dimethylglycine-C-methyl polyethylene glycol (M.W. 2000)
DMG-PEG ₂₀₀₀	1,2-dimyristoyl-rac-glycero-3-methoxypolyethylene glycol (M.W. 2000)
RT-PCR	Reverse transcription polymerase chain reaction
RP-HPLC-CAD	Reversed-phase high-performance liquid chromatography with charged aerosol detector
SEC-HPLC	Size exclusion-high-performance liquid chromatography
IP-RP-HPLC	Ion pair reversed-phase high-performance liquid chromatography
HPLC-UV	High-performance liquid chromatography with ultraviolet detector
MW	Molecular Weight
DP	Decluster Potential
CAD	Collision Associated Dissociation gas
CE	Collision Energy
MRM	Multiple Reaction Monitoring
XIC	Extracted Ion Chromatogram
QToF	Quadrupole Time-of-Flight mass spectrometer

Table S1: Regression equation and calibration curve report of 60-mer RNA construct: MRM scans were used to perform quantification monitoring the negative CAD product ion of guanine (150.0416 m/z) from the 60-mer constructs intact precursor ion at a -28-charge state (695.40 m/z).

Regression Equation: $y = 10.75652 x + -475.23574$ ($r = 0.99095$, $r^2 = 0.98198$) (weighting: $1 / y$)

Expected (ng/mL)	Number of Values	Mean Calculated Concentration (ng/mL)	Average Accuracy across Replicates	Std. Deviation	%CV
50.27	2 of 3	58.082	115.6	8.84	15.2
100.53	1 of 3	99.700	99.2	N/A	N/A
150.80	2 of 3	128.247	85.0	16.57	12.9
301.60	3 of 3	281.053	93.2	40.22	14.3
504.27	2 of 3	458.513	90.9	36.75	8.0
1017.90	3 of 3	1108.934	108.9	55.89	5.0
1508.00	2 of 3	1528.529	101.4	217.42	14.2

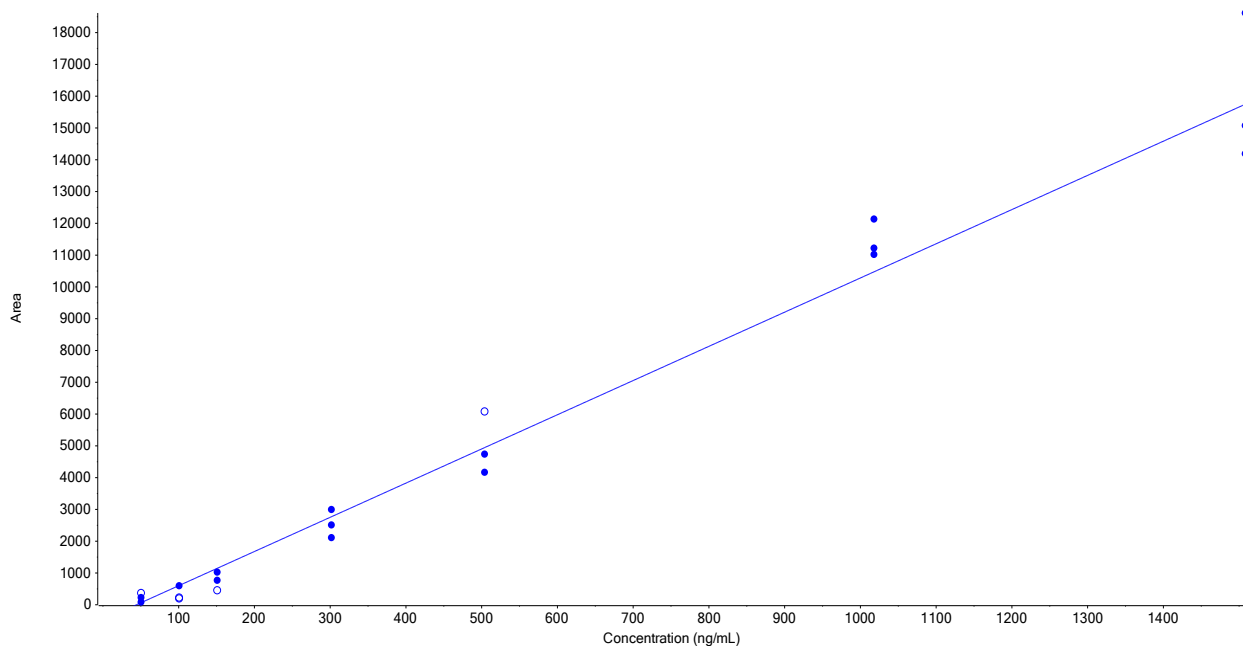


Figure S1: Calibration Curve of 60-mer RNA: To perform absolute quantification an external calibration curve with the 60-mer RNA construct was prepared between 50 – 1500 ng/mL and measured $n = 3$. The assay was validated using ICH m10 bioanalytical method development guidance.

Table S2: Regression Equation and Calibration Curve Report of Antisense FLuc-S1 dsRNA construct: MRM scans were used to perform quantification monitoring the negative CAD product ion of adenine (134.0470 m/z) from the antisense FLuc-S1 dsRNA constructs intact precursor ion at a -11-charge state (786.55 m/z).

Regression Equation: $y = 32.90147x - 87.52353$ ($r = 0.99693$, $r^2 = 0.99387$) (weighting: $1/x$)

Expected (ng/mL)	Number of Values	Mean Calculated Concentration (ng/mL)	Average Accuracy across Replicates	Std. Deviation	%CV
5.17	3 of 3	6.138	118.7	0.79	12.9
25.24	3 of 3	21.538	85.3	2.88	13.4
50.49	2 of 3	56.090	111.1	6.21	11.1
100.98	3 of 3	88.709	87.9	4.60	5.2
151.46	3 of 3	152.338	100.6	17.46	11.5
302.93	3 of 3	292.201	96.5	18.25	6.2
500.81	2 of 3	511.285	102.1	6.47	1.3
1001.61	2 of 3	1064.216	106.3	99.72	9.4
1502.42	2 of 3	1461.022	97.2	99.66	6.8

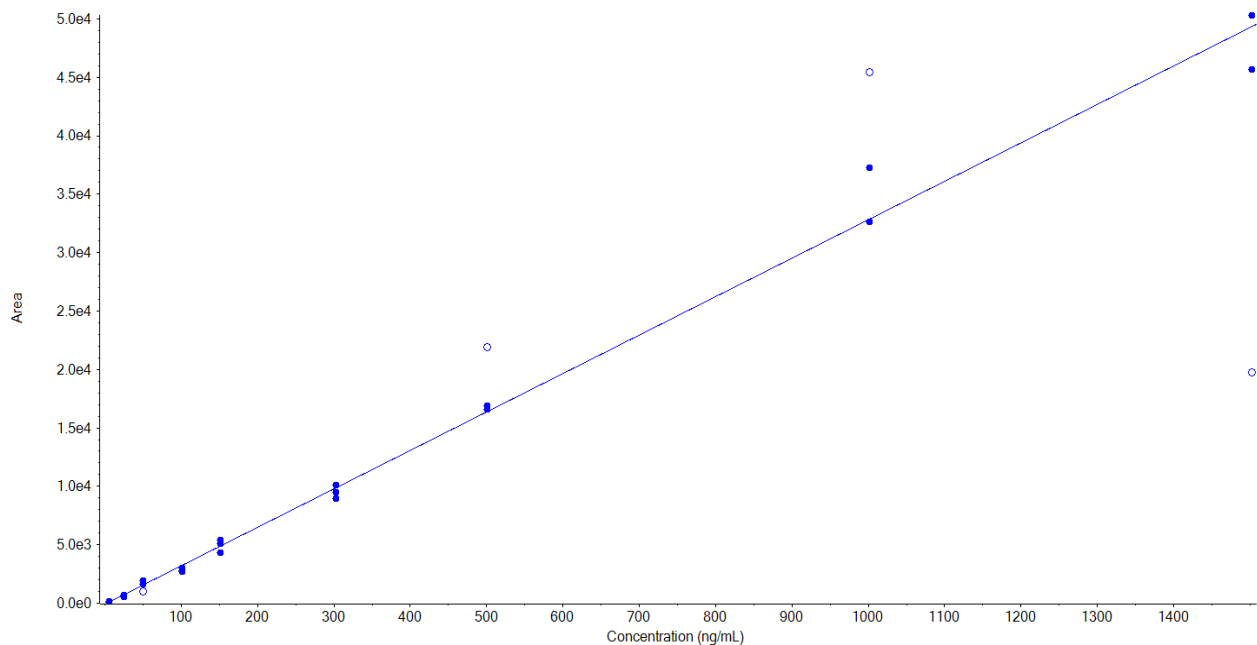


Figure S2: Calibration Curve of Antisense FLuc-S1 dsRNA construct: To perform absolute quantification an external calibration curve with the FLuc-S1 RNA construct was prepared between 5 – 1500 ng/mL and measured $n = 3$. The assay was validated using ICH m10 bioanalytical method development guidance.

