


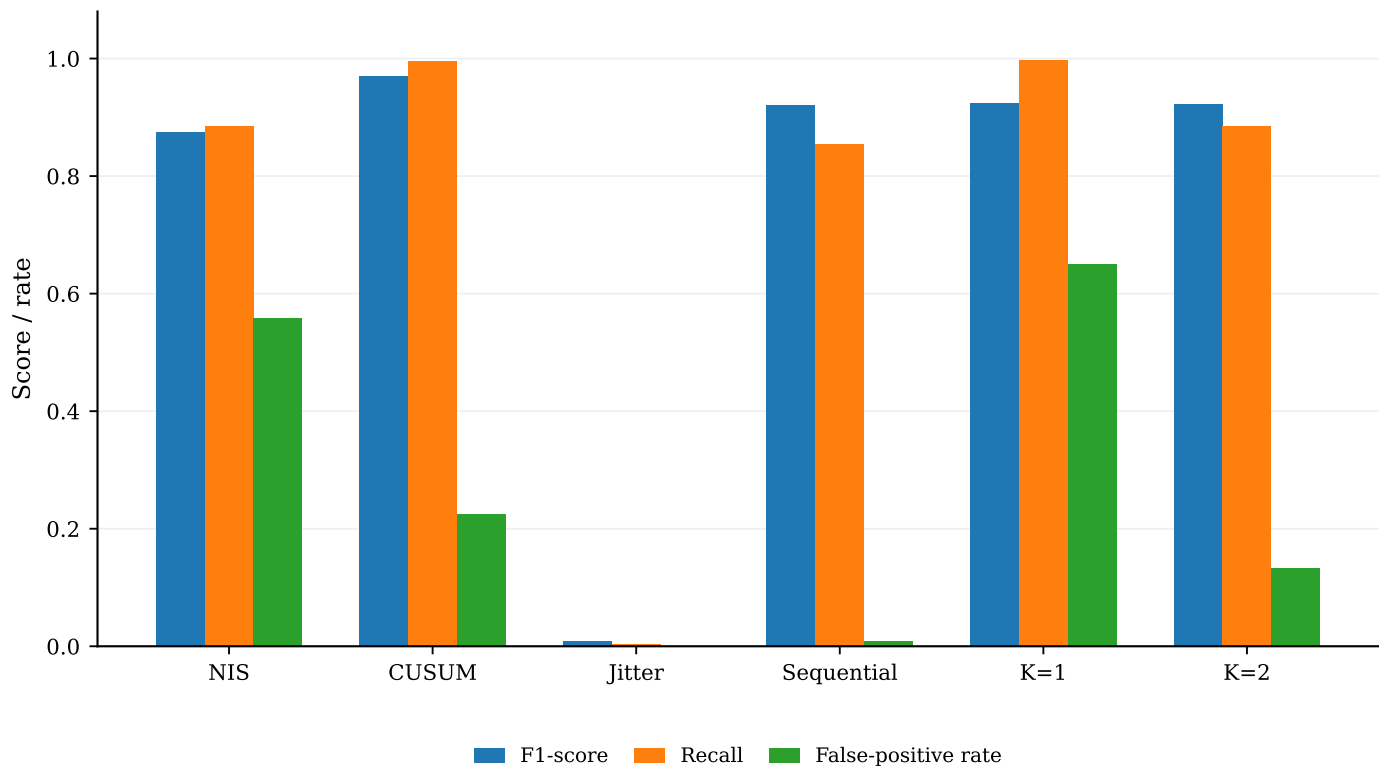

Authoritative detector trace: N=1,200 (960 positive; 240 negative)