KINETIX

User Testing Briefing

Physiotherapist Protocol

Patient Protocol

Today's Briefing

What we'll cover — and what happens after

Physiotherapist

- Retrieve & position device
- Log in to Kinetix UI
- View & select appointment
- Edit treatment plan
- Run warm-up cycle
- Start treatment
- Stop & Help buttons
- View results
- Wipe down device

After the guided run-through, you'll complete the task solo. A questionnaire will follow.

Patient

- Arrive & be seated
- Leg placement (assisted)
- Experience warm-up cycle
- Experience treatment
- Stop & Help buttons
- Leg removal (assisted)

PHYSIOTHERAPIST

Step 1 — Retrieve the Device

The device is stored 5 metres from the treatment area

1. Locate the device at the designated storage point (~5 m from treatment area)
2. Unlock any storage latch or cable lock before moving
3. Grip the handle firmly and wheel or carry the device to the treatment chair
4. Position the device at the foot of the patient's bed — flat, stable surface
5. Confirm device is powered off before connecting to power outlet

PHYSIOTHERAPIST

Step 1 — Retrieve the Device

IMAGE OF DEVICE LOCATION

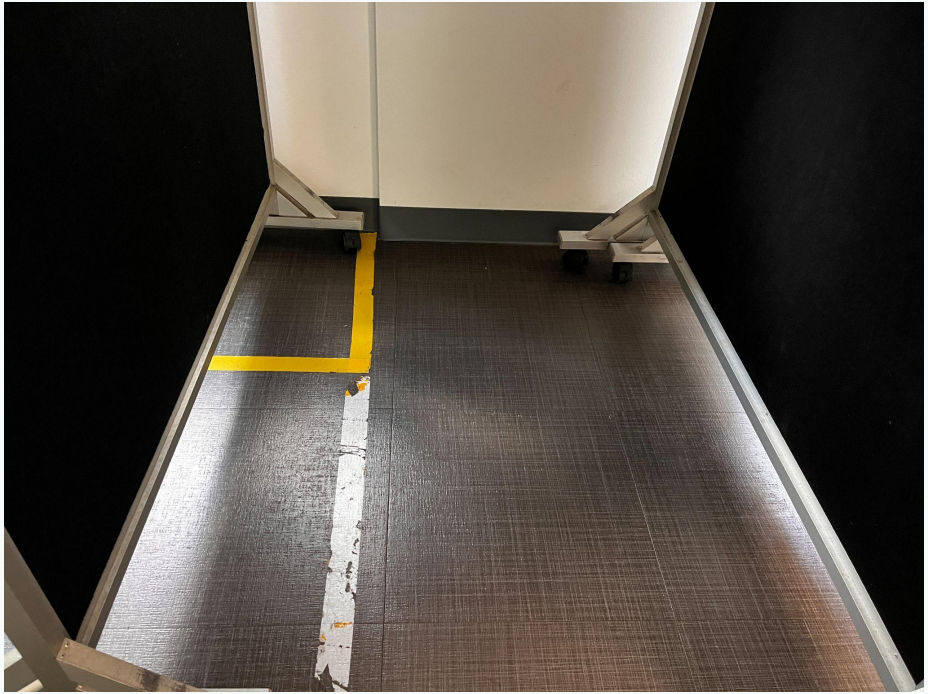

PHYSIOTHERAPIST

Step 2 — Log In to the Kinetix UI

1. Plug in the device
2. Wait for the Kinetix app home screen to load on the tablet (~15 seconds)
3. Enter your staff credentials (username + password)
4. Tap Log In — confirm your name appears in the top-right corner

! Note that the app will automatically connect to the device via bluetooth without further action from you.

PHYSIOTHERAPIST

Step 3 — View & Select Appointment

1. From the dashboard, tap 'Appointments' in the left-hand navigation
2. Confirm today's appointments are available selected in the sidebar
3. Find the patient matching your physical referral.
4. Tap the patient's name to open their appointment record
5. Verify patient name to match the physical referral and tap to edit the treatment plan according to the provided plan.

PHYSIOTHERAPIST

Step 4 — Edit Treatment Plan

1. Inside the appointment, tap 'Edit Treatment'
2. Review pre-loaded parameters: exercise mode, range of motion, duration, etc.
3. Save the details.

PHYSIOTHERAPIST

Steps 5 & 6 — Warm-Up + Treatment

The device runs automatically once started

Automatic Warm-Up Cycle	Start Treatment
Assist patient in placing leg on the device	Confirm patient is comfortable and ready
Tap 'Start Warm-Up' on the session screen	Tap 'Start Treatment' on the UI
Device runs a gentle auto-cycle of one rep (~30 seconds)	Device executes the programmed treatment plan
Ensure tablet is within reach for patient to press stop/help	Ensure tablet is within reach for patient to press stop/help
Warm-up ends automatically	Session ends automatically per plan parameters

PHYSIOTHERAPIST

Step 7 — Responding to Stop & Help

Our actors will press stop and help

STOP BUTTON

Patient or device halts immediately.
Check patient, address issue, resume or abort session.

HELP BUTTON

Patient requests assistance.
Approach calmly, assess situation, provide support.

Physiotherapist Response Protocol

1. Stay calm and approach the patient immediately
2. Press STOP on the UI if the device has not already halted
3. Ask the patient to describe their experience / discomfort

PHYSIOTHERAPIST

Steps 8 & 9 — Results & Device Wipe Down

View Session Results

1. After session ends, tap 'View Results'
2. Review force output, range-of-motion & session log
3. Add clinical notes if required
4. Tap 'Complete Session' to finalise the record
5. Log out of the UI

Wipe Down Device

1. Power off the device using the power button
2. Use approved disinfectant wipes on all contact surfaces
3. Pay attention to the leg cradle and handgrip areas
4. Allow to air-dry for 60 seconds before storage
5. Return device to storage point — lock in place

PATIENT

What to expect from your Kinetix session

- Leg placement & comfort
- Warm-up & treatment cycles
- Stop & Help buttons

This section is for patients only

PATIENT

Step 1 — Arrival & Leg Placement

Your physiotherapist will assist you throughout this step

1. Enter the treatment room and take a seat in the designated treatment chair
2. Your physiotherapist will position the Kinetix device at your feet
3. With assistance, rest your affected leg gently into the device's leg cradle
4. The device will be adjusted to fit your leg comfortably. Speak up if anything feels uncomfortable

PATIENT

Steps 2 & 3 — Warm-Up then Treatment

The device moves your leg gently and automatically

Warm-Up Cycle	Treatment Cycle
The device will begin a gentle warm-up	Your physiotherapist will start the treatment
Complete the first rep and look out for any discomfort	Movements may be slightly more pronounced.
Breathe steadily and try to relax your leg	Follow the instructions on the Ui to complete the exercise
Warm-up lasts approximately 30 seconds	Duration varies per treatment plan
It will stop automatically when complete	Session ends automatically and view your score

PATIENT

Step 4 — The Stop & Help Buttons

You are in control — use these if you need to

STOP BUTTON

Immediately halts the device.
Press if you feel pain or discomfort.

HELP BUTTON

Calls your physiotherapist.
Press if you need assistance or feel uncertain.

You are always in control

- Both buttons are within easy reach on the device at all times
- Your physiotherapist will always be in the room or nearby
- There are no wrong answers. Press Stop or Help whenever you need to

PATIENT

Step 5 — Completing Your Session

Your physiotherapist will assist with removal

1. When treatment ends, the device will slow and stop. Remain still.
2. Your physiotherapist will signal that the session is complete
3. With assistance, carefully lift your leg out of the cradle
4. With assistance, return to your personal mobility device.

What Happens Next

After this briefing, you'll complete the task on your own.

01

Solo Run-Through

Complete your respective protocol independently. Our team will observe but not intervene unless safety requires it.

02

Questionnaire

After completing the task, you'll receive a written questionnaire. Answer honestly — all feedback is valuable.

03

Debrief

We'll gather as a group to discuss findings, challenges, and next steps for the Kinetix development.

Thank you for participating in Kinetix User Testing