

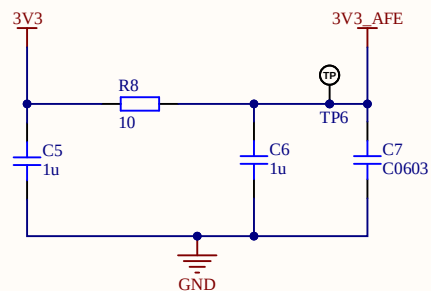


SomniLink — Respiratory Inductance Plethysmography (RIP) Analog Front End — Rev A

3.3 V discrete Colpitts oscillator | Frequency output to SomniMate nRF54L20A

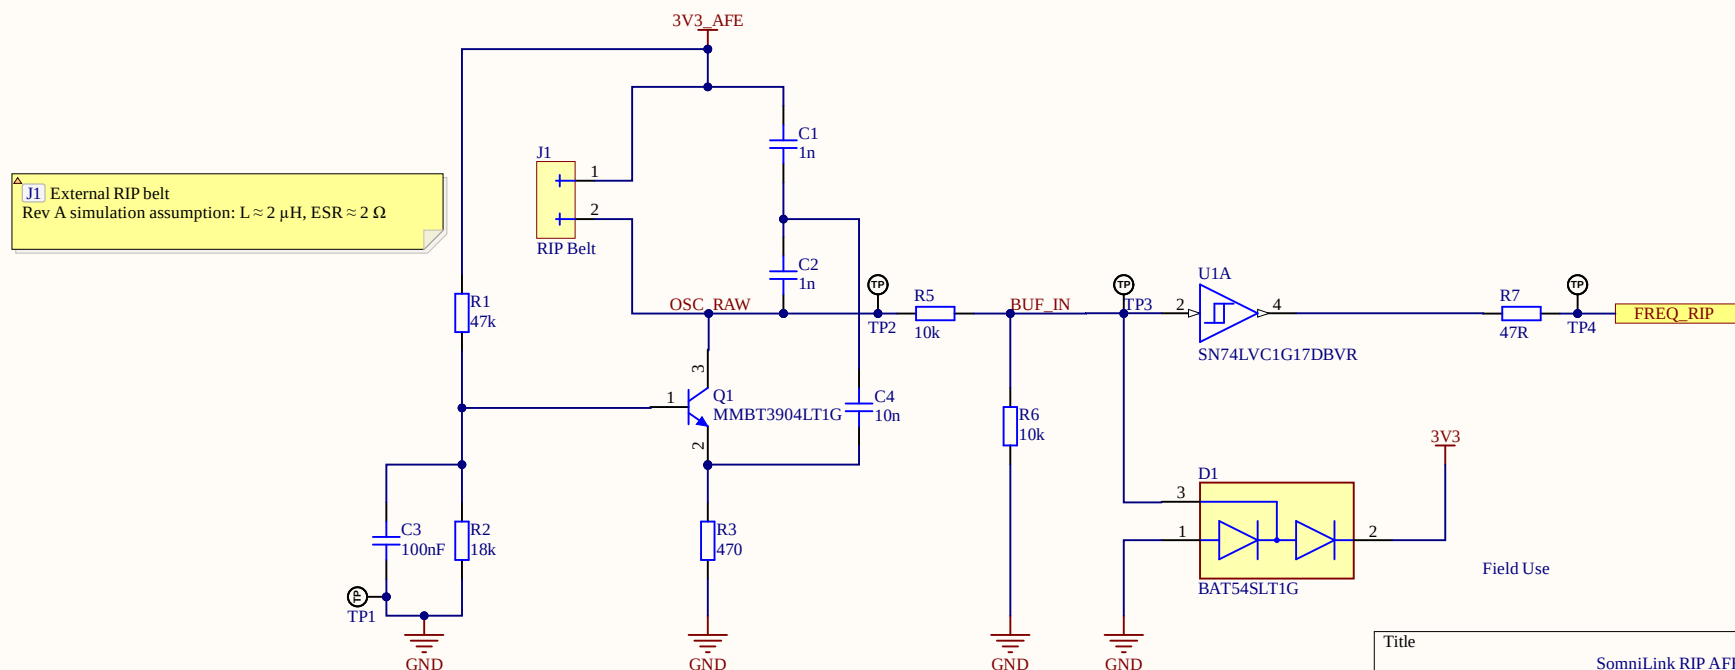

3V3_AFE C-R-C supply isolation
1 μ F / 10 Ω / 1 μ F + 100 nF

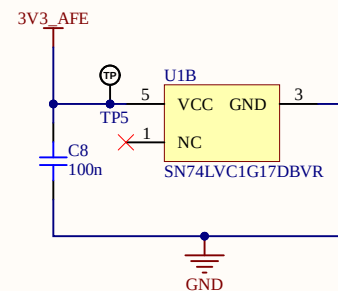

Title				SomniLink RIP AFE – Rev A		
Size	Number			Revision		
A4	SM-RIP-AFE-001			A		
Date:	8/21/2026			Sheet 1 of	1	
File:	C:\Users\A\RIP_AFE.SchDoc			Drawn By:	Caoilte Donohoe	