CMS *ETL ETROC Charge Injection*
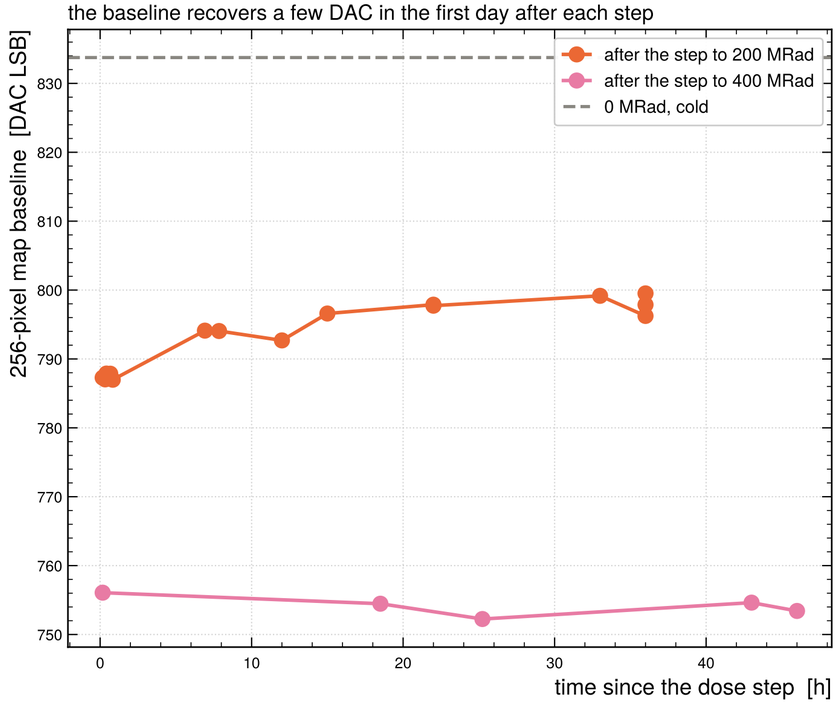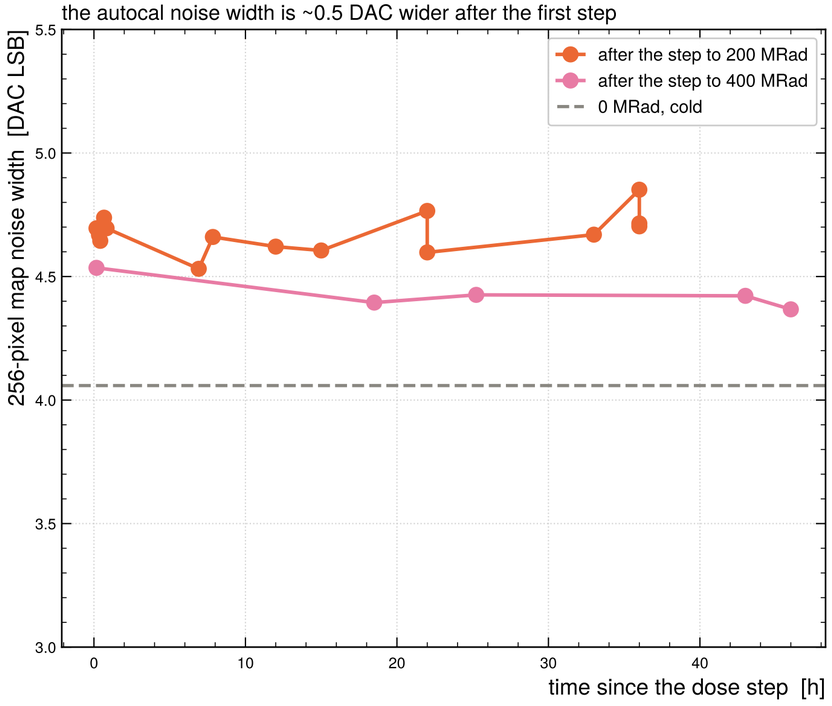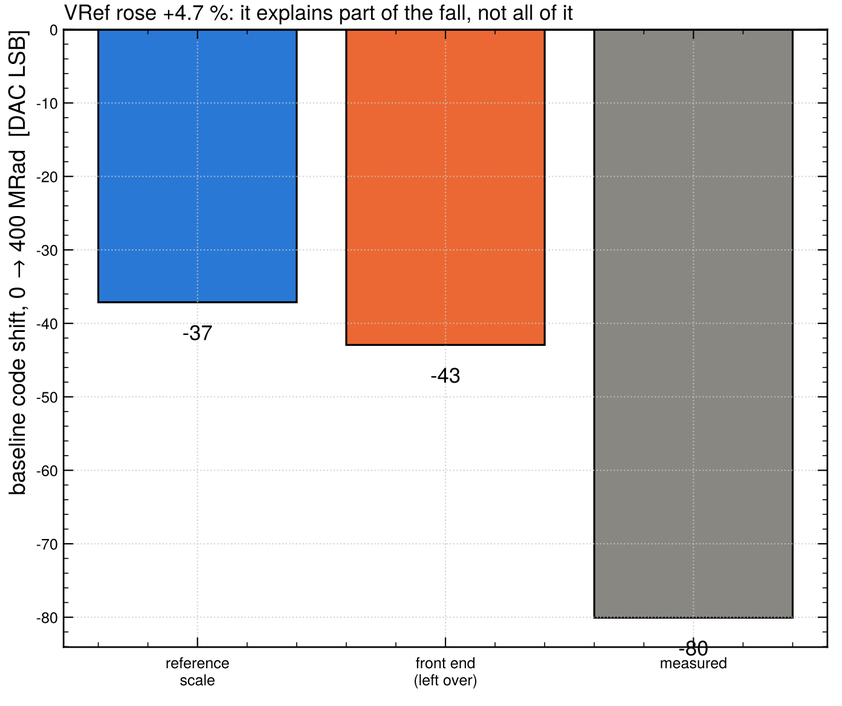
Cooling down after each dose step, and the reference-scale decomposition
ET2p03_BARE9, 256-pixel autocalibration maps at A 1.2 / D 1.2 V (supply), plate −23 to −24 °C; decomposition assumes DAC full scale proportional to VRef
CERN X-ray TID campaign, August 2024