Baseline against dose on two chip revisions and two ET2.03 dies
ET2p01_W36_6 (external VRef) against ET2p03_BARE9 and ET2p03_BARE7 (internal VRef); shifts are paired per pixel
ET2.01 and ET2.03, January and August 2024

absolute baselines — the scales are not comparable

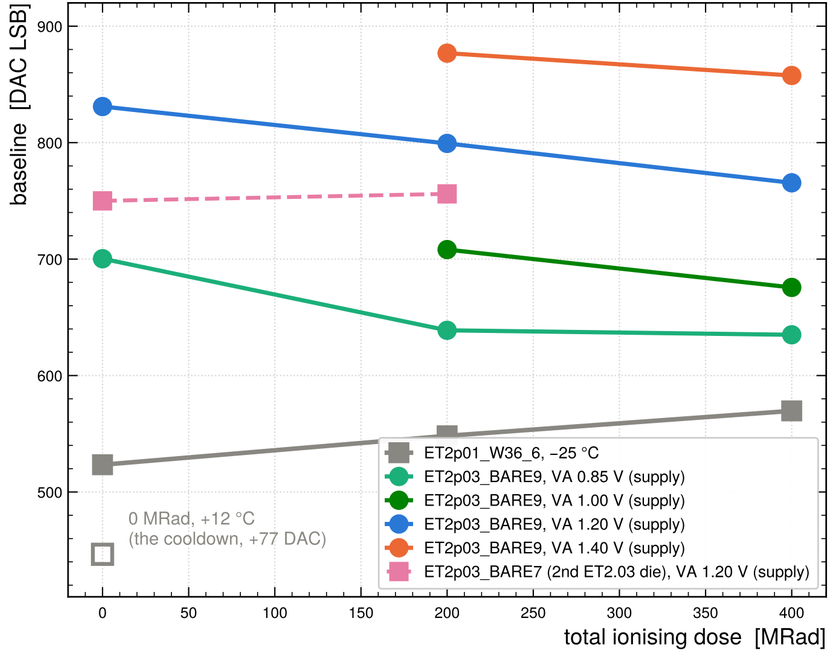

the shift: BARE9 falls on every rail; the second ET2.03 die BARE7 does not

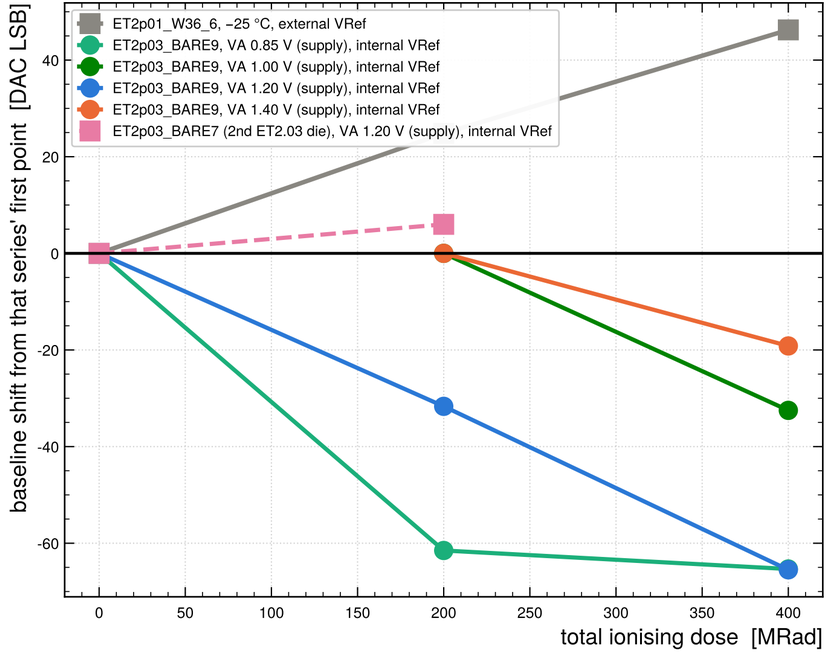
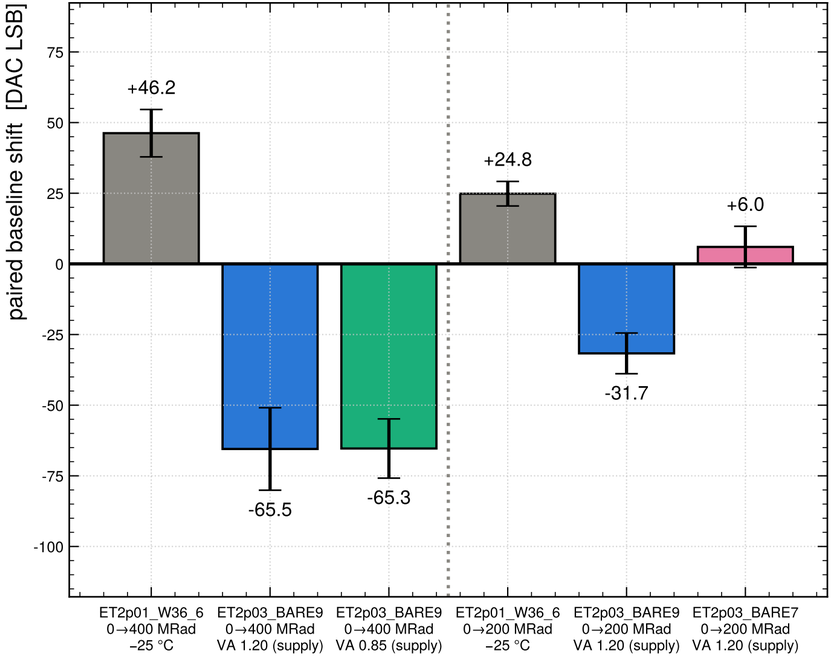
right of the dotted line: the SAME dose step on both ET2.03 dies —
BARE9 falls, BARE7 does not (error bars are the per-pixel s.e.m.)