Tech Support

Software version:	2.5.1K5
User name:	seal
Time and Date:	2025-03-05 19:18:21
Tray number:	5
Tray name:	Compass_Box7_MonMon_NUTR_Feb2023_JB

Sulfate

Calibration data

ID	Absorbance	Calc mg SO4/L	Target mg SO4/L	% Error
S1	0.0020	0.40	0.00	
*90	0.0224	3.71	5.00	-25.8058
S91	0.0545	9.31	10.00	-6.9269
S92	0.0826	14.61	15.00	-2.5840
S93	0.1109	20.34	20.00	1.7250
S94	0.1591	31.00	30.00	3.3181
S95	0.1938	39.34	40.00	-1.6472
S0	0.0022	0.44	0.00	

Calibration status

Polynomial order	2
Correlation coefficient	0.9989
RSE (%)	5.97
Carryover(%)	0.1
Calibration equation	y = cx^2 + bx + a
y =	Concentration mg SO4/L
x =	Measured absorbance
a =	8.697209E-02
b =	1.562034E+02
c =	2.393096E+02
Original Date & Time	2025-03-05 12:58:31 (2025-03-05 12:32:12)

Calibration graph

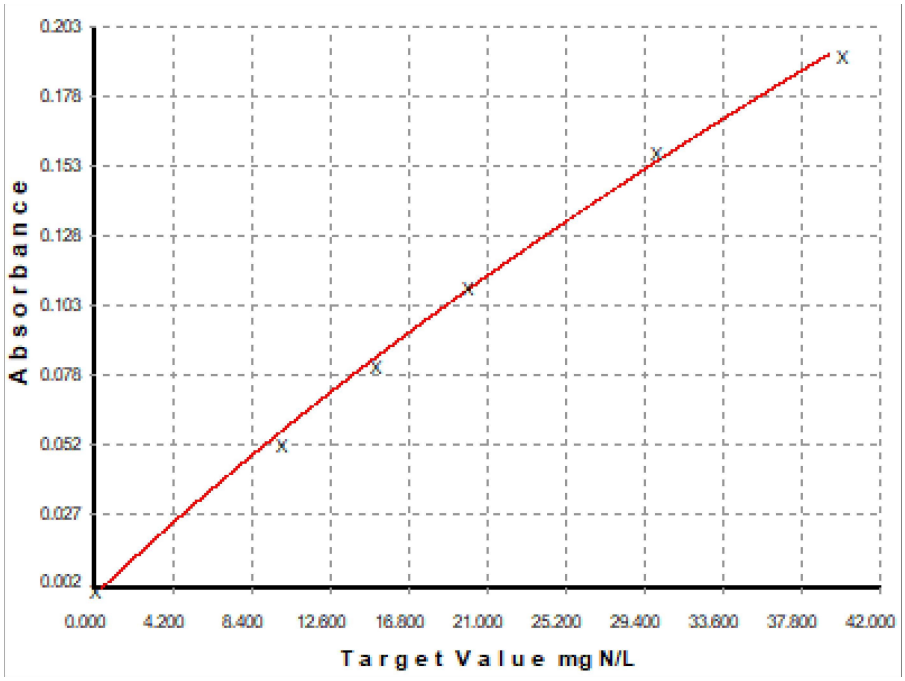

Reagents

Number	Reagent name	Batch number	User	Expiry date
4	Turbidimetric reagent (sulfate)		seal	
39	DI Water (Blank)		UTESE	

Tech Support

Test results

Cup	Type	ID	Details	Result	Units	Raw data	QC Pro	Auto dil.	Man dil.	User	Time &
	CCV	CCV		20.57	mg SO4/L	0.111932				seal	2025-03-05
	CCB	CCB		0.60	mg SO4/L	0.003286				seal	2025-03-05
4	U1	2 ppm SO4		1.52	mg SO4/L	0.009041				seal	2025-03-05
5	U2	2 ppm SO4		1.99	mg SO4/L	0.011986				seal	2025-03-05
6	U3	2 ppm SO4		1.54	mg SO4/L	0.009145				seal	2025-03-05
7	U4	385	7_1_385_44967_OWC_OWC_W_PW_	80.48 ELH	mg SO4/L	0.338793				seal	2025-03-05
8	U5	386	7_2_386_44967_OWC_OWC_W_PW_	5.65 _20	mg SO4/L	0.033869				seal	2025-03-05
9	U6	387	7_3_387_44967_OWC_OWC_W_PW_	10.16 45	mg SO4/L	0.059134				seal	2025-03-05
10	U7	388	7_4_388_44967_OWC_OWC_W_PW_	10.17 10	mg SO4/L	0.059160				seal	2025-03-05
11	U8	389	7_5_389_44967_OWC_OWC_W_PW_	9.19 _20	mg SO4/L	0.053811				seal	2025-03-05
12	U9	390	7_6_390_44967_OWC_OWC_W_PW_	7.83 _45	mg SO4/L	0.046266				seal	2025-03-05
13	U10	391	7_7_391_44967_OWC_OWC_W_PW_	8.88 _10	mg SO4/L	0.052105				seal	2025-03-05
	CCV	CCV		18.83	mg SO4/L	0.103561				seal	2025-03-05
	CCB	CCB		0.50	mg SO4/L	0.002618				seal	2025-03-05
14	U11	392	7_8_392_44967_OWC_OWC_W_PW_	11.98 20	mg SO4/L	0.068864				seal	2025-03-05
15	U12	393	7_9_393_44967_OWC_OWC_W_PW_	7.71 _45	mg SO4/L	0.045595				seal	2025-03-05
16	U13	394	7_11_394_44967_OWC_OWC_TR_PW	2.05 A_10	mg SO4/L	0.012358				seal	2025-03-05
17	U14	395	7_12_395_44967_OWC_OWC_TR_PW	67.45 ELH	mg SO4/L	0.296531				seal	2025-03-05
18	U15	396	7_13_396_44967_OWC_OWC_TR_PW	76.85 ELH	mg SO4/L	0.327298				seal	2025-03-05
19	U16	397	7_14_397_44967_OWC_OWC_TR_PW	2.06 B_10	mg SO4/L	0.012379				seal	2025-03-05
20	U17	398	7_15_398_44967_OWC_OWC_TR_PW	15.09 B_20	mg SO4/L	0.084973				seal	2025-03-05
21	U18	399	7_16_399_44967_OWC_OWC_TR_PW	76.83 ELH	mg SO4/L	0.327228				seal	2025-03-05
22	U19	400	7_17_400_44967_OWC_OWC_TR_PW	1.81 C_10	mg SO4/L	0.010846				seal	2025-03-05
23	U20	401	7_18_401_44967_OWC_OWC_TR_PW	1.64 C_20	mg SO4/L	0.009787				seal	2025-03-05
	CCV	CCV		16.45	mg SO4/L	0.091810				seal	2025-03-05
	CCB	CCB		0.46	mg SO4/L	0.002396				seal	2025-03-05
24	U21	402	7_19_402_44967_OWC_OWC_TR_PW	82.04 ELH	mg SO4/L	0.343685				seal	2025-03-05
25	U22	403	7_21_403_44967_OWC_OWC_UP_PW	2.56 A_10	mg SO4/L	0.015484				seal	2025-03-05
26	U23	404	7_23_404_44967_OWC_OWC_UP_PW	2.75 A_45	mg SO4/L	0.016621				seal	2025-03-05
27	U24	405	7_24_405_44967_OWC_OWC_UP_PW	1.15 B_10	mg SO4/L	0.006729				seal	2025-03-05
28	U25	406	7_25_406_44967_OWC_OWC_UP_PW	6.52 B_20	mg SO4/L	0.038883				seal	2025-03-05
29	U26	407	7_27_407_44967_OWC_OWC_UP_PW	58.77 ELH	mg SO4/L	0.266713				seal	2025-03-05
30	U27	408	7_28_408_44967_OWC_OWC_UP_PW	2.69 C_20	mg SO4/L	0.016259				seal	2025-03-05
31	U28	409	7_29_409_44967_OWC_OWC_UP_PW	632.29 ELH	mg SO4/L	1.331435				seal	2025-03-05
32	U29	410	7_31_410_44967_OWC_OWC_TR_RZ	2.51 _	mg SO4/L	0.015151				seal	2025-03-05
33	U30	411	7_32_411_44967_OWC_OWC_TR_RZ	1.72 _	mg SO4/L	0.010306				seal	2025-03-05
	CCV	CCV		16.85	mg SO4/L	0.093841				seal	2025-03-05
	CCB	CCB		0.48	mg SO4/L	0.002516				seal	2025-03-05
34	U31	412	7_33_412_44967_OWC_OWC_TR_RZ	7.31 _	mg SO4/L	0.043384				seal	2025-03-05
35	U32	413	7_34_413_44967_OWC_OWC_TR_RZ	6.22 _	mg SO4/L	0.037171				seal	2025-03-05
36	U33	414	7_35_414_44967_OWC_OWC_TR_RZ	1.69 _	mg SO4/L	0.010103				seal	2025-03-05
37	U34	415	7_36_415_44967_OWC_OWC_TR_RZ	2.08 _	mg SO4/L	0.012496				seal	2025-03-05
38	U35	416	7_37_416_44967_OWC_OWC_TR_RZ	1.52 _	mg SO4/L	0.009018				seal	2025-03-05
39	U36	417	7_38_417_44967_OWC_OWC_TR_RZ	8.76 _	mg SO4/L	0.051440				seal	2025-03-05
40	U37	418	7_41_418_44967_OWC_OWC_UP_RZ	23.15 _	mg SO4/L	0.124082				seal	2025-03-05
41	U38	419	7_42_419_44967_OWC_OWC_UP_RZ	46.90 ELH	mg SO4/L	0.223308				seal	2025-03-05
42	U39	420	7_43_420_44967_OWC_OWC_UP_RZ	24.34 _	mg SO4/L	0.129563				seal	2025-03-05
43	U40	421	7_44_421_44967_OWC_OWC_UP_RZ	49.86 ELH	mg SO4/L	0.234436				seal	2025-03-05
	CCV	CCV		21.42	mg SO4/L	0.115950				seal	2025-03-05
	CCB	CCB		0.56	mg SO4/L	0.003031				seal	2025-03-05

Tech Support

Cup	Type	ID	Details	Result	Units	Raw data	QC Pro	Auto dil.	Man dil.	User	Time &
47	U44	425	7_49_425_44967_OWC_OWC__Strean	2.02	mg SO4/L	0.012132				seal	2025-03-05
48	U45	426	7_51_426_44978_CRC_CRC_W_PW_	232.81 ELH	mg SO4/L	0.712373				seal	2025-03-05
49	U46	427	7_52_427_44978_CRC_CRC_W_PW_	273.02 ELH	mg SO4/L	0.790329				seal	2025-03-05
50	U47	428	7_53_428_44978_CRC_CRC_W_PW_	336.43 ELH	mg SO4/L	0.903257				seal	2025-03-05
51	U48	429	7_54_429_44978_CRC_CRC_W_PW_	234.98 ELH	mg SO4/L	0.716739				seal	2025-03-05
52	U49	430	7_55_430_44978_CRC_CRC_W_PW_	248.74 ELH	mg SO4/L	0.743949				seal	2025-03-05
53	U50	431	7_56_431_44978_CRC_CRC_W_PW_	267.94 ELH	mg SO4/L	0.780785				seal	2025-03-05
	CCV	CCV		14.21	mg SO4/L	0.080480				seal	2025-03-05
	CCB	CCB		0.49	mg SO4/L	0.002578				seal	2025-03-05
54	U51	432	7_57_432_44978_CRC_CRC_W_PW_	277.11 ELH	mg SO4/L	0.797969				seal	2025-03-05
55	U52	433	7_58_433_44978_CRC_CRC_W_PW_	252.90 ELH	mg SO4/L	0.752026				seal	2025-03-05
56	U53	434	7_59_434_44978_CRC_CRC_W_PW_	277.13 ELH	mg SO4/L	0.797993				seal	2025-03-05
57	U54	435	7_61_435_44978_CRC_CRC_TR_PW_	199.09 ELH	mg SO4/L	0.642186				seal	2025-03-05
58	U55	436	7_62_436_44978_CRC_CRC_TR_PW_	242.34 ELH	mg SO4/L	0.731385				seal	2025-03-05
59	U56	437	7_63_437_44978_CRC_CRC_TR_PW_	122.33 ELH	mg SO4/L	0.459328				seal	2025-03-05
60	U57	438	7_64_438_44978_CRC_CRC_TR_PW_	229.15 ELH	mg SO4/L	0.704992				seal	2025-03-05
61	U58	439	7_65_439_44978_CRC_CRC_TR_PW_	227.13 ELH	mg SO4/L	0.700890				seal	2025-03-05
62	U59	440	7_66_440_44978_CRC_CRC_TR_PW_	154.23 ELH	mg SO4/L	0.540017				seal	2025-03-05
63	U60	441	7_67_441_44978_CRC_CRC_TR_PW_	167.93 ELH	mg SO4/L	0.572459				seal	2025-03-05
	CCV	CCV		12.97	mg SO4/L	0.074064				seal	2025-03-05
	CCB	CCB		0.50	mg SO4/L	0.002623				seal	2025-03-05
64	U61	442	7_68_442_44978_CRC_CRC_TR_PW_	200.59 ELH	mg SO4/L	0.645407				seal	2025-03-05
65	U62	443	7_69_443_44978_CRC_CRC_TR_PW_	133.64 ELH	mg SO4/L	0.488868				seal	2025-03-05
66	U63	444	7_71_444_44978_CRC_CRC_UP_PW_	6.54 _10	mg SO4/L	0.038997				seal	2025-03-05
67	U64	445	7_72_445_44978_CRC_CRC_UP_PW_	37.27 _20	mg SO4/L	0.185373				seal	2025-03-05
68	U65	446	7_74_446_44978_CRC_CRC_UP_PW_	6.34 _10	mg SO4/L	0.037823				seal	2025-03-05
69	U66	447	7_77_447_44978_CRC_CRC_UP_PW_	4.80 _10	mg SO4/L	0.028872				seal	2025-03-05
70	U67	448	7_78_448_44978_CRC_CRC__Open__	96.89 ELH	mg SO4/L	0.388501				seal	2025-03-05
71	U68	449	7_79_449_44978_CRC_CRC__Open__	77.19 ELH	mg SO4/L	0.328382				seal	2025-03-05
72	U69	450	7_80_450_44978_CRC_CRC__Open__	75.44 ELH	mg SO4/L	0.322780				seal	2025-03-05
73	U70	451	7_80_451_44978_CRC_CRC_TR_RZ_	111.97 ELH	mg SO4/L	0.431288				seal	2025-03-05
	CCV	CCV		13.75	mg SO4/L	0.078119				seal	2025-03-05
	CCB	CCB		0.50	mg SO4/L	0.002624				seal	2025-03-05
74	U71	452	7_81_452_44978_CRC_CRC_TR_RZ_	155.30 ELH	mg SO4/L	0.542591				seal	2025-03-05
75	U72	453	7_83_453_44978_CRC_CRC_TR_RZ_	145.61 ELH	mg SO4/L	0.518972				seal	2025-03-05
76	U73	454	7_85_454_44978_CRC_CRC_TR_RZ_	141.93 ELH	mg SO4/L	0.509847				seal	2025-03-05
77	U74	455	7_86_455_44978_CRC_CRC_TR_RZ_	190.81 ELH	mg SO4/L	0.624159				seal	2025-03-05
78	U75	456	7_87_456_44978_CRC_CRC_TR_RZ_	232.10 ELH	mg SO4/L	0.710959				seal	2025-03-05
79	U76	457	7_88_457_44978_CRC_CRC_TR_RZ_	57.57 ELH	mg SO4/L	0.262466				seal	2025-03-05
80	U77	458	7_91_458_44978_CRC_CRC_UP_RZ_	5.99	mg SO4/L	0.035803				seal	2025-03-05
81	U78	459	7_92_459_44978_CRC_CRC_UP_RZ_	8.64	mg SO4/L	0.050782				seal	2025-03-05
82	U79	460	7_93_460_44978_CRC_CRC_UP_RZ_	4.96	mg SO4/L	0.029858				seal	2025-03-05
83	U80	461	7_94_461_44978_CRC_CRC_UP_RZ_	13.48	mg SO4/L	0.076742				seal	2025-03-05
	CCV	CCV		20.13	mg SO4/L	0.109856				seal	2025-03-05
	CCB	CCB		0.48	mg SO4/L	0.002525				seal	2025-03-05
84	U81	462	7_95_462_44978_CRC_CRC_UP_RZ_	16.07	mg SO4/L	0.089934				seal	2025-03-05
85	U82	463	7_96_463_44978_CRC_CRC_UP_RZ_	6.31	mg SO4/L	0.037650				seal	2025-03-05
86	U83	464	7_97_464_44978_CRC_CRC_UP_RZ_	9.96	mg SO4/L	0.058030				seal	2025-03-05
87	U84	465	7_98_465_44978_CRC_CRC_UP_RZ_	4.33	mg SO4/L	0.026107				seal	2025-03-05
88	U85	Field Blank		34.32	mg SO4/L	0.173218				seal	2025-03-05
89	U86	Field Blank		31.07	mg SO4/L	0.159408				seal	2025-03-05
90	U87	Field Blank		135.64 ELH	mg SO4/L	0.493974				seal	2025-03-05

Tech Support

Cup	Type	ID	Details	Result	Units	Raw data	QC Pro	Auto dil.	Man dil.	User	Time &
	CCB	CCB		0.00	mg SO4/L	0.000000				seal	
	CCV	CCV		0.00	mg SO4/L	0.000000				seal	
	CCB	CCB		0.00	mg SO4/L	0.000000				seal	
	CCV	CCV		0.00	mg SO4/L	0.000000				seal	
	CCB	CCB		0.00	mg SO4/L	0.000000				seal	
	CCV	CCV		0.00	mg SO4/L	0.000000				seal	
	CCB	CCB		0.00	mg SO4/L	0.000000				seal	

Test parameters Sulfate

Test number	2		
Long test name	Sulfate	**Short test name**	SO4
Units	mg SO4/L	**Decimal places**	2
Test type	End Point		

Main parameters

Sample volume	400	**Water volume**	0	**Number of mixes**	2
Cuvette primes	2	**Cuvette washes**	2	**Baseline on wash**	Yes
Cadmium volume	0	**Reduction time**	0	**Diluent location**	Reagent 24

Math parameters

Reaction time	270	**Wavelength**	405nm	**Polynomial order**	2
Repeat delta check	0.250	**Auto dilution factor**	10.000	**Manual dilution factor**	0.000
Linearity Low	0.0020	**Linearity High**	0.1938	**Latest Slope**	1.0000
Alert Low	0.000	**Alert High**	0.000	**Latest Intercept**	0.0000

Reagent parameters

Number of reagents 1

Reagent	Name	Volume	Delay	Replaced in blank
1	Turbidimetric reagent (sul	200	0	Yes

Tech Support

Standards

Auto Std. Number	6	**Auto Std. Concentration**	40.0000	**Exclude the Blank**	No
Auto Std. Position	Cup 5	**Standard 1 (Blank) Position**	Reagent 24	**Correlation limit**	0.9900

Standard	Value	Standard	Value	Auto Standard	Percentage	Value
1	0.0000			S90	12.5000	5.0000
				S91	25.0000	10.0000
				S92	37.5000	15.0000
				S93	50.0000	20.0000
				S94	75.0000	30.0000
				S95	100.0000	40.0000

QC PRO

Control	Low value	High value	Location	Frequency	Start before
CCV	16.0000	24.0000	Reagent 11	10	1
CCB	-0.8000	0.8000	Reagent 24	10	1

Control	%% (+ \ -)	Stock Conc.	Spike added	Location
DUP	0.0000			
SPKA	0.0000	0.0000	0.0000	Cup 105
SPKM	0.0000		0.0000	
SPKD	0.0000			

Advanced parameters

Set diagnostic slope & intercept	No	**Extra debubble action**	Yes
Eliminate air from transfer	No	**Eliminate air from cuvette wash**	No
Extra aspiration steps	0	**Smart dilution**	No

Diagnostics

Cup	Type	Result	Absorbance	T	W
1		20.57	0.111932	0.115935	0.004003
2		0.60	0.003286	0.007111	0.003826
3		1.52	0.009041	0.012849	0.003808
4	U1	1.99	0.011986	0.015671	0.003685
5	U2	1.54	0.009145	0.012747	0.003602
6	U3	80.48 ELH	0.338793	0.342491	0.003698
7	U4	5.65	0.033869	0.037597	0.003728
8	U5	10.16	0.059134	0.062882	0.003747
9	U6	10.17	0.059160	0.062784	0.003624
10	U7	9.19	0.053811	0.057489	0.003678
11	U8	7.83	0.046266	0.049841	0.003575
12	U9	8.88	0.052105	0.055719	0.003613
13	U10	18.83	0.103561	0.107221	0.003660
14	U11	0.50	0.002618	0.006281	0.003663
15	U12	11.98	0.068864	0.072510	0.003646
16	U13	7.71	0.045595	0.049204	0.003609
17	U14	2.05	0.012358	0.016011	0.003653
20	U17	67.45 ELH	0.296531	0.300173	0.003643
21	U18	76.85 ELH	0.327298	0.331150	0.003852
22	U19	2.06	0.012379	0.016152	0.003772
23	U20	15.09	0.084973	0.088939	0.003966

Tech Support

Cup	Type	Result	Absorbance	T	W
24	U21	76.83 ELH	0.327228	0.331301	0.004073
25	U22	1.81	0.010846	0.014820	0.003974
26	U23	1.64	0.009787	0.013806	0.004019
27	U24	16.45	0.091810	0.095753	0.003943
28	U25	0.46	0.002396	0.006338	0.003942
29	U26	82.04 ELH	0.343685	0.347675	0.003989
30	U27	2.56	0.015484	0.019491	0.004007
31	U28	2.75	0.016621	0.020682	0.004061
34	U31	1.15	0.006729	0.010723	0.003994
35	U32	6.52	0.038883	0.043182	0.004299
36	U33	58.77 ELH	0.266713	0.270997	0.004285
37	U34	2.69	0.016259	0.020527	0.004268
38	U35	632.29 ELH	1.331435	1.335695	0.004260
39	U36	2.51	0.015151	0.019407	0.004255
40	U37	1.72	0.010306	0.014493	0.004187
41	U38	16.85	0.093841	0.098058	0.004217
42	U39	0.48	0.002516	0.006740	0.004224
43	U40	7.31	0.043384	0.047616	0.004232
44	U41	6.22	0.037171	0.041632	0.004461
45	U42	1.69	0.010103	0.014367	0.004264
48	U45	2.08	0.012496	0.016804	0.004308
49	U46	1.52	0.009018	0.013241	0.004223
50	U47	8.76	0.051440	0.055718	0.004278
51	U48	23.15	0.124082	0.128438	0.004357
52	U49	46.90 ELH	0.223308	0.227755	0.004447
53	U50	24.34	0.129563	0.134072	0.004509
54	U51	49.86 ELH	0.234436	0.238908	0.004472
55	U52	21.42	0.115950	0.120435	0.004485
56	U53	0.56	0.003031	0.007444	0.004413
57	U54	67.79 ELH	0.297673	0.302281	0.004609
58	U55	10.17	0.059198	0.063723	0.004524
59	U56	48.51 ELH	0.229369	0.233911	0.004541
62	U59	2.02	0.012132	0.016594	0.004462
63	U60	232.81 ELH	0.712373	0.717109	0.004736
64	U61	273.02 ELH	0.790329	0.795434	0.005105
65	U62	336.43 ELH	0.903257	0.909078	0.005821
66	U63	234.98 ELH	0.716739	0.722701	0.005962
67	U64	248.74 ELH	0.743949	0.750076	0.006128
68	U65	267.94 ELH	0.780785	0.787180	0.006395
69	U66	14.21	0.080480	0.086866	0.006386
70	U67	0.49	0.002578	0.008854	0.006276
71	U68	277.11 ELH	0.797969	0.804529	0.006560
72	U69	252.90 ELH	0.752026	0.758630	0.006604
73	U70	277.13 ELH	0.797993	0.804833	0.006840
76	U73	199.09 ELH	0.642186	0.649170	0.006984
77	U74	242.34 ELH	0.731385	0.738735	0.007350
78	U75	122.33 ELH	0.459328	0.466748	0.007420
79	U76	229.15 ELH	0.704992	0.712574	0.007581
80	U77	227.13 ELH	0.700890	0.708918	0.008027
81	U78	154.23 ELH	0.540017	0.548018	0.008002
82	U79	167.93 ELH	0.572459	0.580731	0.008273
83	U80	12.97	0.074064	0.082136	0.008072

Tech Support

Cup	Type	Result	Absorbance	T	W
91	U88	6.34	0.037823	0.046355	0.008532
91	U89	4.80	0.028872	0.037289	0.008417
91	U90	96.89 ELH	0.388501	0.397054	0.008553
91	U91	77.19 ELH	0.328382	0.337035	0.008653
91	U92	75.44 ELH	0.322780	0.331324	0.008544
91	U93	111.97 ELH	0.431288	0.439875	0.008587
92		13.75	0.078119	0.086580	0.008461
93		0.50	0.002624	0.011157	0.008533
94		155.30 ELH	0.542591	0.551086	0.008495
95		145.61 ELH	0.518972	0.527557	0.008586
96		141.93 ELH	0.509847	0.518505	0.008658
99		190.81 ELH	0.624159	0.632833	0.008674
100		232.10 ELH	0.710959	0.719908	0.008949
101		57.57 ELH	0.262466	0.271481	0.009015
102		5.99	0.035803	0.044814	0.009011
103		8.64	0.050782	0.059696	0.008914
104		4.96	0.029858	0.038840	0.008982
105		13.48	0.076742	0.085725	0.008983
106		20.13	0.109856	0.118836	0.008980
0		0.48	0.002525	0.011523	0.008998
0		16.07	0.089934	0.098984	0.009049
0		6.31	0.037650	0.046659	0.009009
0		9.96	0.058030	0.066986	0.008957
0		4.33	0.026107	0.035120	0.009013
0		34.32	0.173218	0.182334	0.009116
0		31.07	0.159408	0.168519	0.009111
0		135.64 ELH	0.493974	0.503083	0.009110
0		13.83	0.078514	0.087647	0.009133
0		0.50	0.002646	0.011827	0.009182
0		0.00	0.000000	0.000000	0.000000
0		0.00	0.000000	0.000000	0.000000
0		0.00	0.000000	0.000000	0.000000
0		0.00	0.000000	0.000000	0.000000
0		0.00	0.000000	0.000000	0.000000
0		0.00	0.000000	0.000000	0.000000
0		0.00	0.000000	0.000000	0.000000
0		0.00	0.000000	0.000000	0.000000
0		0.00	0.000000	0.000000	0.000000
0		0.00	0.000000	0.000000	0.000000

Tech Support

Tech Support

Nitrate (NOx)

Calibration data

ID	Absorbance	Calc mg N/L	Target mg N/L	% Error
S1	0.1040	-0.0096	0.0000	
S90	0.1452	0.0450	0.0500	-9.9795
S91	0.1926	0.1079	0.1000	7.9235
S92	0.3030	0.2545	0.2500	1.7893
S93	0.4962	0.5108	0.5000	2.1682
S94	0.6718	0.7438	0.7500	-0.8277
S95	0.8630	0.9976	1.0000	-0.2426
S0	0.1093	-0.0026	0.0000	

Calibration status

Polynomial order	1
Correlation coefficient	0.9998
RSE (%)	6.54
Carryover(%)	0.7
Calibration equation	y = bx + a
y =	Concentration mg N/L
x =	Measured absorbance
a =	-1.476768E-01
b =	1.327068E+00
Original Date & Time	2025-03-05 11:48:19

Calibration graph

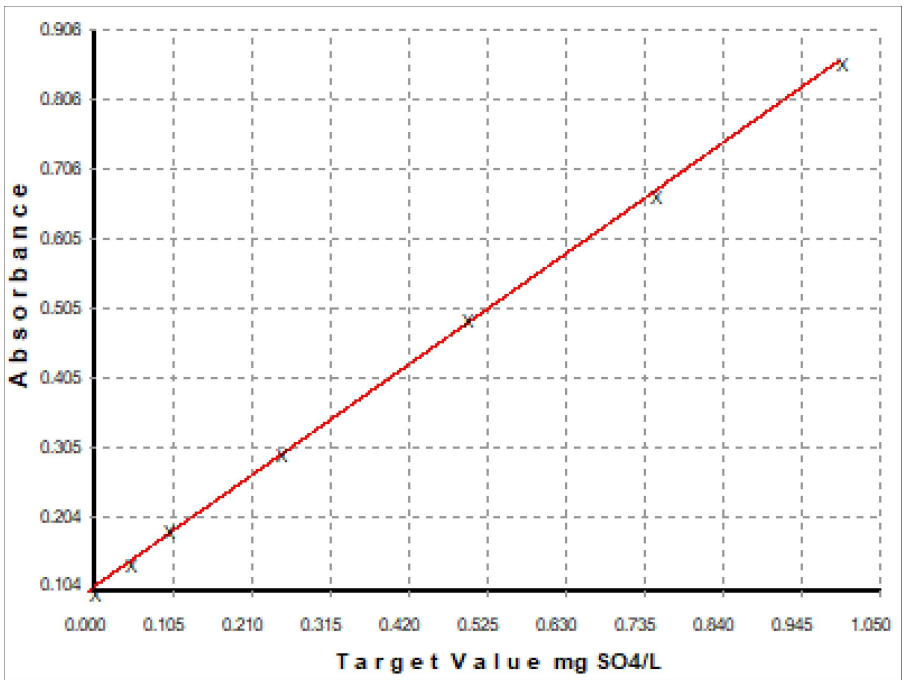

Reagents

Number	Reagent name	Batch number	User	Expiry date
13	DI Water 2			
5	Working color reagent (nitrate)			
39	DI Water (Blank)		UTESE	

Test results

Cup	Type	ID	Details	Result	Units	Raw data	QC Pro	Auto dil.	Man dil.	User	Ti
	CCV	CCV		0.4659	mg N/L	0.462363				seal	202
	CCB	CCB		-0.0176	mg N/L	0.097990				seal	202
7	U4	385	7_1_385_44967_OWC_OWC_W_PW_	0.049710	mg N/L	0.148745				seal	202
8	U5	386	7_2_386_44967_OWC_OWC_W_PW_	0.009420	mg N/L	0.118328				seal	202
9	U6	387	7_3_387_44967_OWC_OWC_W_PW_	-0.002315	mg N/L	0.109528				seal	202

Tech Support

Cup	Type	ID	Details	Result	Units	Raw data	QC Pro	Auto dil.	Man dil.	User	Ti
11	U8	389	7_5_389_44967_OWC_OWC_W_PW_	0.0320 20	mg N/L	0.135398				seal	202
12	U9	390	7_6_390_44967_OWC_OWC_W_PW_	0.3086 45	mg N/L	0.343826				seal	202
13	U10	391	7_7_391_44967_OWC_OWC_W_PW_	0.0142 10	mg N/L	0.122010				seal	202
14	U11	392	7_8_392_44967_OWC_OWC_W_PW_	0.0247 20	mg N/L	0.129897				seal	202
15	U12	393	7_9_393_44967_OWC_OWC_W_PW_	0.0042 45	mg N/L	0.114447				seal	202
16	U13	394	7_11_394_44967_OWC_OWC_TR_PW	0.1362 _10	mg N/L	0.213942				seal	202
	CCV	CCV		0.4844	mg N/L	0.476264				seal	202
	CCB	CCB		-0.0105	mg N/L	0.103402				seal	202
17	U14	395	7_12_395_44967_OWC_OWC_TR_PW	0.0058 _20	mg N/L	0.115672				seal	202
18	U15	396	7_13_396_44967_OWC_OWC_TR_PW	0.0172 _45	mg N/L	0.124227				seal	202
19	U16	397	7_14_397_44967_OWC_OWC_TR_PW	0.0122 3_10	mg N/L	0.120464				seal	202
20	U17	398	7_15_398_44967_OWC_OWC_TR_PW	0.0108 3_20	mg N/L	0.119406				seal	202
21	U18	399	7_16_399_44967_OWC_OWC_TR_PW	0.0138 3_45	mg N/L	0.121680				seal	202
22	U19	400	7_17_400_44967_OWC_OWC_TR_PW	0.1654 _10	mg N/L	0.235893				seal	202
23	U20	401	7_18_401_44967_OWC_OWC_TR_PW	0.1365 _20	mg N/L	0.214166				seal	202
24	U21	402	7_19_402_44967_OWC_OWC_TR_PW	0.0623 _45	mg N/L	0.158228				seal	202
25	U22	403	7_21_403_44967_OWC_OWC_UP_PW	0.0233 _10	mg N/L	0.128850				seal	202
26	U23	404	7_23_404_44967_OWC_OWC_UP_PW	-0.0012 _45	mg N/L	0.110371				seal	202
	CCV	CCV		0.4898	mg N/L	0.480363				seal	202
	CCB	CCB		-0.0009	mg N/L	0.110615				seal	202
27	U24	405	7_24_405_44967_OWC_OWC_UP_PW	0.0124 3_10	mg N/L	0.120592				seal	202
28	U25	406	7_25_406_44967_OWC_OWC_UP_PW	0.0405 3_20	mg N/L	0.141774				seal	202
29	U26	407	7_27_407_44967_OWC_OWC_UP_PW	0.0453 _10	mg N/L	0.145450				seal	202
30	U27	408	7_28_408_44967_OWC_OWC_UP_PW	-0.0039 _20	mg N/L	0.108370				seal	202
31	U28	409	7_29_409_44967_OWC_OWC_UP_PW	0.0929 _45	mg N/L	0.181306				seal	202
32	U29	410	7_31_410_44967_OWC_OWC_TR_RZ	0.2867	mg N/L	0.132884		x10.0000		seal	202
33	U30	411	7_32_411_44967_OWC_OWC_TR_RZ	3.0872	mg N/L	0.343911		x10.0000		seal	202
34	U31	412	7_33_412_44967_OWC_OWC_TR_RZ	2.1436	mg N/L	0.272811		x10.0000		seal	202
35	U32	413	7_34_413_44967_OWC_OWC_TR_RZ	-0.0591	mg N/L	0.106827		x10.0000		seal	202
36	U33	414	7_35_414_44967_OWC_OWC_TR_RZ	0.0642	mg N/L	0.116120		x10.0000		seal	202
	CCV	CCV		0.4748	mg N/L	0.469086				seal	202
	CCB	CCB		-0.0000	mg N/L	0.111268				seal	202
37	U34	415	7_36_415_44967_OWC_OWC_TR_RZ	1.2152	mg N/L	0.202849		x10.0000		seal	202
38	U35	416	7_37_416_44967_OWC_OWC_TR_RZ	5.9561	mg N/L	0.560100		x10.0000		seal	202
39	U36	417	7_38_417_44967_OWC_OWC_TR_RZ	1.8211	mg N/L	0.248504		x10.0000		seal	202
40	U37	418	7_41_418_44967_OWC_OWC_UP_RZ	-0.0392	mg N/L	0.108326		x10.0000		seal	202
41	U38	419	7_42_419_44967_OWC_OWC_UP_RZ	0.1847	mg N/L	0.125198		x10.0000		seal	202
42	U39	420	7_43_420_44967_OWC_OWC_UP_RZ	0.0339	mg N/L	0.113835		x10.0000		seal	202
43	U40	421	7_44_421_44967_OWC_OWC_UP_RZ	0.7269	mg N/L	0.166052		x10.0000		seal	202
44	U41	422	7_45_422_44967_OWC_OWC_UP_RZ	-0.0425	mg N/L	0.108080		x10.0000		seal	202
45	U42	423	7_46_423_44967_OWC_OWC_UP_RZ	-0.0972 ELL	mg N/L	0.103954		x10.0000		seal	202
46	U43	424	7_48_424_44967_OWC_OWC_UP_RZ	0.0124	mg N/L	0.112212		x10.0000		seal	202
	CCV	CCV		0.4769	mg N/L	0.470631				seal	202
	CCB	CCB		-0.0062	mg N/L	0.106575				seal	202
47	U44	425	7_49_425_44967_OWC_OWC__Strear	8.0615 ELH	mg N/L	6.185928				seal	202
48	U45	426	7_51_426_44978_CRC_CRC_W_PW_	0.0935 0	mg N/L	0.181755				seal	202
49	U46	427	7_52_427_44978_CRC_CRC_W_PW_	0.0017 0	mg N/L	0.112532				seal	202
50	U47	428	7_53_428_44978_CRC_CRC_W_PW_	-0.0011 5	mg N/L	0.110457				seal	202
51	U48	429	7_54_429_44978_CRC_CRC_W_PW_	0.0088 0	mg N/L	0.117878				seal	202
52	U49	430	7_55_430_44978_CRC_CRC_W_PW_	0.0023 0	mg N/L	0.113050				seal	202
53	U50	431	7_56_431_44978_CRC_CRC_W_PW_	-0.0018 5	mg N/L	0.109953				seal	202
54	U51	432	7_57_432_44978_CRC_CRC_W_PW_	0.0320 0	mg N/L	0.135363				seal	202

Tech Support

Cup	Type	ID	Details	Result	Units	Raw data	QC Pro	Auto dil.	Man dil.	User	Ti
58	U55	436	7_62_436_44978_CRC_CRC_TR_PW_	-0.0000 20	mg N/L	0.111247				seal	202
59	U56	437	7_63_437_44978_CRC_CRC_TR_PW_	0.0411 45	mg N/L	0.142244				seal	202
60	U57	438	7_64_438_44978_CRC_CRC_TR_PW_	0.0141 10	mg N/L	0.121877				seal	202
61	U58	439	7_65_439_44978_CRC_CRC_TR_PW_	0.0002 20	mg N/L	0.111406				seal	202
62	U59	440	7_66_440_44978_CRC_CRC_TR_PW_	0.0073 45	mg N/L	0.116811				seal	202
63	U60	441	7_67_441_44978_CRC_CRC_TR_PW_	-0.0034 10	mg N/L	0.108716				seal	202
64	U61	442	7_68_442_44978_CRC_CRC_TR_PW_	0.0227 20	mg N/L	0.128371				seal	202
65	U62	443	7_69_443_44978_CRC_CRC_TR_PW_	0.4744 45	mg N/L	0.468797				seal	202
66	U63	444	7_71_444_44978_CRC_CRC_UP_PW_	8.0212 ELH	mg N/L	6.155607				seal	202
	CCV	CCV		0.5215	mg N/L	0.504272				seal	202
	CCB	CCB		-0.0030	mg N/L	0.108983				seal	202
67	U64	445	7_72_445_44978_CRC_CRC_UP_PW_	7.0184 ELH	mg N/L	5.399904				seal	202
68	U65	446	7_74_446_44978_CRC_CRC_UP_PW_	6.9219 ELH	mg N/L	5.327227				seal	202
69	U66	447	7_77_447_44978_CRC_CRC_UP_PW_	7.9763 ELH	mg N/L	6.121781				seal	202
70	U67	448	7_78_448_44978_CRC_CRC__Open__	2.5777 ELH	mg N/L	2.053665				seal	202
71	U68	449	7_79_449_44978_CRC_CRC__Open__	2.5454 ELH	mg N/L	2.029311				seal	202
72	U69	450	7_80_450_44978_CRC_CRC__Open__	2.7477 ELH	mg N/L	2.181816				seal	202
73	U70	451	7_80_451_44978_CRC_CRC_TR_RZ_	0.3879	mg N/L	0.140509		x10.0000		seal	202
74	U71	452	7_81_452_44978_CRC_CRC_TR_RZ_	1.1306	mg N/L	0.196474		x10.0000		seal	202
75	U72	453	7_83_453_44978_CRC_CRC_TR_RZ_	0.6603	mg N/L	0.161036		x10.0000		seal	202
76	U73	454	7_85_454_44978_CRC_CRC_TR_RZ_	-0.0707	mg N/L	0.105950		x10.0000		seal	202
	CCV	CCV		0.4739	mg N/L	0.468380				seal	202
	CCB	CCB		-0.0146	mg N/L	0.100294				seal	202
77	U74	455	7_86_455_44978_CRC_CRC_TR_RZ_	-0.0585	mg N/L	0.106874		x10.0000		seal	202
78	U75	456	7_87_456_44978_CRC_CRC_TR_RZ_	-0.1346 ELL	mg N/L	0.101141		x10.0000		seal	202
79	U76	457	7_88_457_44978_CRC_CRC_TR_RZ_	0.1809	mg N/L	0.124910		x10.0000		seal	202
80	U77	458	7_91_458_44978_CRC_CRC_UP_RZ_	14.9336 ELH	mg N/L	1.236590		x10.0000		seal	202
81	U78	459	7_92_459_44978_CRC_CRC_UP_RZ_	22.2693 ELH	mg N/L	1.789364		x10.0000		seal	202
82	U79	460	7_93_460_44978_CRC_CRC_UP_RZ_	26.8404 ELH	mg N/L	2.133816		x10.0000		seal	202
83	U80	461	7_94_461_44978_CRC_CRC_UP_RZ_	13.6280 ELH	mg N/L	1.138207		x10.0000		seal	202
84	U81	462	7_95_462_44978_CRC_CRC_UP_RZ_	3.9237	mg N/L	0.406948		x10.0000		seal	202
85	U82	463	7_96_463_44978_CRC_CRC_UP_RZ_	6.0441	mg N/L	0.566731		x10.0000		seal	202
86	U83	464	7_97_464_44978_CRC_CRC_UP_RZ_	15.4614 ELH	mg N/L	1.276361		x10.0000		seal	202
	CCV	CCV		0.4874	mg N/L	0.478554				seal	202
	CCB	CCB		-0.0059	mg N/L	0.106816				seal	202
87	U84	465	7_98_465_44978_CRC_CRC_UP_RZ_	22.6988 ELH	mg N/L	1.821724		x10.0000		seal	202
88	U85	Field Blank		0.0932	mg N/L	0.181538				seal	202
89	U86	Field Blank		0.0844	mg N/L	0.174904				seal	202
90	U87	Field Blank		0.9517	mg N/L	0.828454				seal	202
91	U88	1 ppm NOx Standarno dilution		1.0293 ELH	mg N/L	0.886912				seal	202
91	U89	1 ppm NOx Standarx2 dilution		1.0577 ELH	mg N/L	0.908285				seal	202
91	U90	1 ppm NOx Standarx5 dilution		1.0410 ELH	mg N/L	0.895680				seal	202
91	U91	1 ppm NOx Standarx10 dilution		1.0625 ELH	mg N/L	0.911896				seal	202
91	U92	1 ppm NOx Standarx20 dilution		1.0368 ELH	mg N/L	0.892570				seal	202
91	U93	1 ppm NOx Standarx50 dilution		1.0749 ELH	mg N/L	0.921277				seal	202
	CCV	CCV		0.4783	mg N/L	0.471667				seal	202
	CCB	CCB		-0.0112	mg N/L	0.102821				seal	202

Tech Support

Cup	Type	ID	Details	Result	Units	Raw data	QC Pro	Auto dil.	Man dil.	User	Ti

Test parameters Nitrate (NOx)

Test number	3		
Long test name	Nitrate (NOx)	**Short test name**	NOx_NO3
Units	mg N/L	**Decimal places**	4
Test type	End Point		

Main parameters

Sample volume	180	**Water volume**	0	**Number of mixes**	1
Cuvette primes	2	**Cuvette washes**	2	**Baseline on wash**	Yes
Cadmium volume	0	**Reduction time**	0	**Diluent location**	Reagent 24

Math parameters

Reaction time	1825	**Wavelength**	520nm	**Polynomial order**	1
Repeat delta check	0.250	**Auto dilution factor**	1.000	**Manual dilution factor**	0.000
Linearity Low	0.1040	**Linearity High**	0.8630	**Latest Slope**	1.3271
Alert Low	0.000	**Alert High**	0.000	**Latest Intercept**	-0.1477

Reagent parameters

Number of reagents 2

Reagent	Name	Volume	Delay	Replaced in blank
1	DI Water 2	10	0	No
2	Working color reagent (nit310)		27	No

Standards

Auto Std. Number	6	**Auto Std. Concentration**	1.0000	**Exclude the Blank**	No
Auto Std. Position	Cup 3	**Standard 1 (Blank) Position**	Reagent 24	**Correlation limit**	0.9900

Standard	Value	Standard	Value	Auto Standard	Percentage	Value
1	0.0000			S90	5.0000	0.0500
				S91	10.0000	0.1000
				S92	25.0000	0.2500
				S93	50.0000	0.5000
				S94	75.0000	0.7500
				S95	100.0000	1.0000

Tech Support

QC PRO

Control	Low value	High value	Location	Frequency	Start before
CCV	0.4000	0.6000	Reagent 12	10	1
CCB	-0.0200	0.0200	Reagent 24	10	1
Control	**%% (+ \ -)**	**Stock Conc.**	**Spike added**	**Location**	
DUP	0.0000				
SPKA	0.0000	3.0000	0.2500	Cup 103	
SPKM	0.0000		0.0000		
SPKD	0.0000				

Advanced parameters

Set diagnostic slope & intercept	No	**Extra debubble action**	No
Eliminate air from transfer	No	**Eliminate air from cuvette wash**	No
Extra aspiration steps	0	**Smart dilution**	No

Diagnostics

Cup	Type	Result	Absorbance	T	W
1		0.4659	0.462363	0.460876	-0.001487
2		-0.0176	0.097990	0.096484	-0.001506
6	U3	0.0497	0.148745	0.147099	-0.001646
7	U4	0.0094	0.118328	0.116640	-0.001687
8	U5	-0.0023	0.109528	0.107898	-0.001630
9	U6	0.0611	0.157330	0.155591	-0.001739
10	U7	0.0320	0.135398	0.133689	-0.001708
11	U8	0.3086	0.343826	0.342174	-0.001652
12	U9	0.0142	0.122010	0.120211	-0.001799
15	U12	0.0247	0.129897	0.128182	-0.001715
16	U13	0.0042	0.114447	0.112764	-0.001682
17	U14	0.1362	0.213942	0.212277	-0.001665
18	U15	0.4844	0.476264	0.474613	-0.001651
19	U16	-0.0105	0.103402	0.101727	-0.001675
20	U17	0.0058	0.115672	0.113999	-0.001674
21	U18	0.0172	0.124227	0.122626	-0.001601
22	U19	0.0122	0.120464	0.118910	-0.001555
23	U20	0.0108	0.119406	0.117911	-0.001495
24	U21	0.0138	0.121680	0.120105	-0.001574
25	U22	0.1654	0.235893	0.234391	-0.001501
26	U23	0.1365	0.214166	0.212647	-0.001520
29	U26	0.0623	0.158228	0.156674	-0.001554
30	U27	0.0233	0.128850	0.127345	-0.001505
31	U28	-0.0012	0.110371	0.108771	-0.001601
32	U29	0.4898	0.480363	0.478950	-0.001413
33	U30	-0.0009	0.110615	0.109243	-0.001372
34	U31	0.0124	0.120592	0.119207	-0.001385
35	U32	0.0405	0.141774	0.140324	-0.001450
36	U33	0.0453	0.145450	0.144209	-0.001241
37	U34	-0.0039	0.108370	0.107043	-0.001327
38	U35	0.0929	0.181306	0.179957	-0.001350
39	U36	0.2867	0.132884	0.131627	-0.001257
40	U37	3.0872	0.343911	0.342753	-0.001158
43	U40	2.1436	0.272811	0.271612	-0.001199
44	U41	0.0591	0.106827	0.105637	-0.001190

Tech Support

Cup	Type	Result	Absorbance	T	W
48	U45	1.2152	0.202849	0.201837	-0.001012
49	U46	5.9561	0.560100	0.559076	-0.001024
50	U47	1.8211	0.248504	0.247554	-0.000950
51	U48	-0.0392	0.108326	0.107364	-0.000962
52	U49	0.1847	0.125198	0.124192	-0.001006
53	U50	0.0339	0.113835	0.112877	-0.000959
54	U51	0.7269	0.166052	0.165148	-0.000903
57	U54	-0.0425	0.108080	0.107088	-0.000992
58	U55	-0.0972 ELL	0.103954	0.103042	-0.000912
59	U56	0.0124	0.112212	0.111344	-0.000868
60	U57	0.4769	0.470631	0.469825	-0.000806
61	U58	-0.0062	0.106575	0.105784	-0.000791
62	U59	8.0615 ELH	6.185928	6.185424	-0.000505
63	U60	0.0935	0.181755	0.180984	-0.000771
64	U61	0.0017	0.112532	0.111760	-0.000771
65	U62	-0.0011	0.110457	0.109758	-0.000700
66	U63	0.0088	0.117878	0.117166	-0.000712
67	U64	0.0023	0.113050	0.112295	-0.000755
68	U65	-0.0018	0.109953	0.109297	-0.000656
71	U68	0.0320	0.135363	0.134701	-0.000663
72	U69	0.0399	0.141363	0.140654	-0.000708
73	U70	0.0162	0.123495	0.122861	-0.000634
74	U71	0.4693	0.464895	0.464308	-0.000588
75	U72	-0.0090	0.104480	0.103909	-0.000571
76	U73	0.1946	0.257909	0.257455	-0.000454
77	U74	-0.0000	0.111247	0.110748	-0.000499
78	U75	0.0411	0.142244	0.141772	-0.000472
79	U76	0.0141	0.121877	0.121426	-0.000452
80	U77	0.0002	0.111406	0.110921	-0.000485
81	U78	0.0073	0.116811	0.116322	-0.000489
82	U79	-0.0034	0.108716	0.108285	-0.000431
85	U82	0.0227	0.128371	0.128022	-0.000349
86	U83	0.4744	0.468797	0.468357	-0.000440
87	U84	8.0212 ELH	6.155607	6.155816	0.000209
88	U85	0.5215	0.504272	0.504067	-0.000205
89	U86	-0.0030	0.108983	0.108704	-0.000279
90	U87	7.0184 ELH	5.399904	5.400225	0.000321
91	U88	6.9219 ELH	5.327227	5.327573	0.000346
91	U89	7.9763 ELH	6.121781	6.122300	0.000518
91	U90	2.5777 ELH	2.053665	2.053656	-0.000009
91	U91	2.5454 ELH	2.029311	2.029250	-0.000060
91	U92	2.7477 ELH	2.181816	2.181643	-0.000173
91	U93	0.3879	0.140509	0.140304	-0.000205
94		1.1306	0.196474	0.196267	-0.000207
95		0.6603	0.161036	0.160787	-0.000249
96		-0.0707	0.105950	0.105659	-0.000290
97		0.4739	0.468380	0.468274	-0.000106
98		-0.0146	0.100294	0.100101	-0.000194
99		-0.0585	0.106874	0.106696	-0.000178
100		-0.1346 ELL	0.101141	0.100986	-0.000155
101		0.1809	0.124910	0.124734	-0.000175
102		14.9336 ELH	1.236590	1.236470	-0.000120

Tech Support

Cup	Type	Result	Absorbance	T	W
0		15.4614 ELH	1.276361	1.276271	-0.000090
0		0.4874	0.478554	0.478500	-0.000054
0		-0.0059	0.106816	0.106716	-0.000100
0		22.6988 ELH	1.821724	1.821681	-0.000043
0		0.0932	0.181538	0.181506	-0.000032
0		0.0844	0.174904	0.174863	-0.000041
0		0.9517	0.828454	0.828457	0.000004
0		1.0293 ELH	0.886912	0.887010	0.000098
0		1.0577 ELH	0.908285	0.908336	0.000051
0		1.0410 ELH	0.895680	0.895732	0.000051
0		1.0625 ELH	0.911896	0.912049	0.000153
0		1.0368 ELH	0.892570	0.892747	0.000177
0		1.0749 ELH	0.921277	0.921438	0.000160
0		0.4783	0.471667	0.471808	0.000141
0		-0.0112	0.102821	0.102862	0.000041

Tech Support

Nitrite

Calibration data

ID	Absorbance	Calc ug N/L	Target ug N/L	% Error
S1	0.0010	-0.58	0.00	
S90	0.0026	0.20	0.89	-77.8220
S91	0.0045	1.09	1.78	-38.5900
S92	0.0114	4.50	4.89	-8.0550
S93	0.0222	9.74	10.22	-4.6687
S94	0.0537	25.10	24.89	0.8568
S95	0.1064	50.79	50.22	1.1343
S96	0.1614	77.63	75.11	3.3534
S97	0.3151	152.63	150.22	1.6015
S98	0.4063	197.12	200.00	-1.4397
S0	0.0059	1.80	0.00	

Calibration status

Polynomial order	1
Correlation coefficient	0.9997
RSE (%)	33.06
Carryover(%)	1.2
Calibration equation	y = bx + a
y =	Concentration ug N/L
x =	Measured absorbance
a =	-1.087518E+00
b =	4.878107E+02
Original Date & Time	2025-03-05 11:38:28

Calibration graph

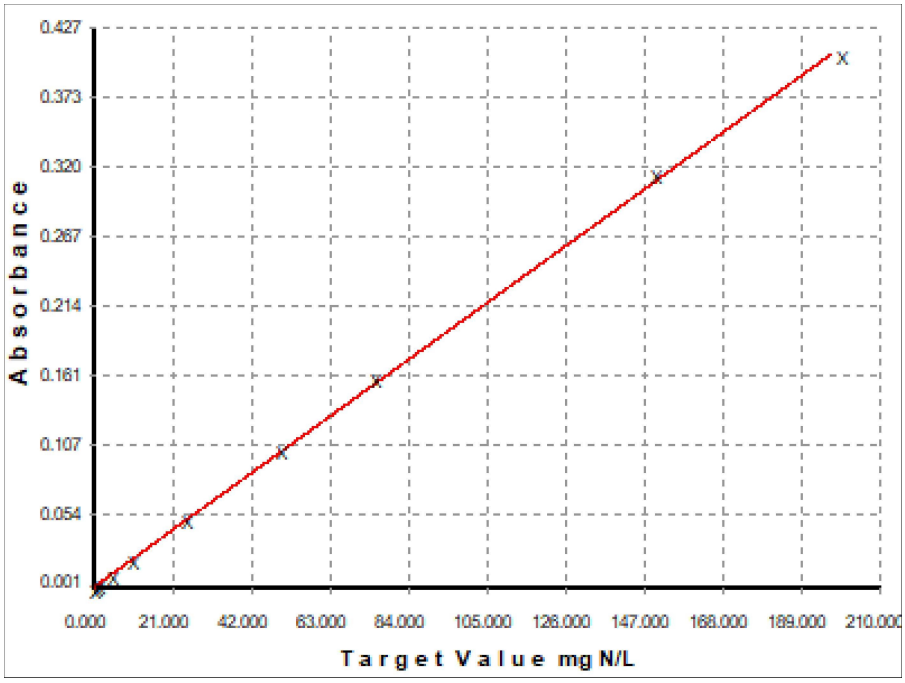

Reagents

Number	Reagent name	Batch number	User	Expiry date
14	Sulfa-NEDD (NO2)			

Test results

Cup	Type	ID	Details	Result	Units	Raw data	QC Pro	Auto dil.	Man dil.	User	Time &
	CCV	CCV		93.93	ug N/L	0.194779				seal	2025-03-05
	CCB	CCB		0.57	ug N/L	0.003393				seal	2025-03-05
7	U4	385	7_1_385_44967_OWC_OWC_W_PW_	6.51 _10	ug N/L	0.015579				seal	2025-03-05
8	U5	386	7_2_386_44967_OWC_OWC_W_PW_	4.34 _20	ug N/L	0.011117				seal	2025-03-05
9	U6	387	7_3_387_44967_OWC_OWC_W_PW_	2.75 _45	ug N/L	0.007870				seal	2025-03-05

Tech Support

Cup	Type	ID	Details	Result	Units	Raw data	QC Pro	Auto dil.	Man dil.	User	Time &
11	U8	389	7_5_389_44967_OWC_OWC_W_PW_	7.35 _20	ug N/L	0.017306				seal	2025-03-05
12	U9	390	7_6_390_44967_OWC_OWC_W_PW_	3.35 _45	ug N/L	0.009100				seal	2025-03-05
13	U10	391	7_7_391_44967_OWC_OWC_W_PW_	12.60 10	ug N/L	0.028049				seal	2025-03-05
14	U11	392	7_8_392_44967_OWC_OWC_W_PW_	7.05 _20	ug N/L	0.016690				seal	2025-03-05
15	U12	393	7_9_393_44967_OWC_OWC_W_PW_	3.46 _45	ug N/L	0.009329				seal	2025-03-05
16	U13	394	7_11_394_44967_OWC_OWC_TR_PW	1.87 A_10	ug N/L	0.006073				seal	2025-03-05
	CCV	CCV		95.32	ug N/L	0.197629				seal	2025-03-05
	CCB	CCB		0.57	ug N/L	0.003399				seal	2025-03-05
17	U14	395	7_12_395_44967_OWC_OWC_TR_PW	2.73 A_20	ug N/L	0.007824				seal	2025-03-05
18	U15	396	7_13_396_44967_OWC_OWC_TR_PW	2.50 A_45	ug N/L	0.007345				seal	2025-03-05
19	U16	397	7_14_397_44967_OWC_OWC_TR_PW	2.10 B_10	ug N/L	0.006535				seal	2025-03-05
20	U17	398	7_15_398_44967_OWC_OWC_TR_PW	2.40 B_20	ug N/L	0.007145				seal	2025-03-05
21	U18	399	7_16_399_44967_OWC_OWC_TR_PW	2.19 B_45	ug N/L	0.006719				seal	2025-03-05
22	U19	400	7_17_400_44967_OWC_OWC_TR_PW	2.25 C_10	ug N/L	0.006846				seal	2025-03-05
23	U20	401	7_18_401_44967_OWC_OWC_TR_PW	7.57 C_20	ug N/L	0.017745				seal	2025-03-05
24	U21	402	7_19_402_44967_OWC_OWC_TR_PW	4.11 C_45	ug N/L	0.010650				seal	2025-03-05
25	U22	403	7_21_403_44967_OWC_OWC_UP_PW	3.70 A_10	ug N/L	0.009823				seal	2025-03-05
26	U23	404	7_23_404_44967_OWC_OWC_UP_PW	3.26 A_45	ug N/L	0.008902				seal	2025-03-05
	CCV	CCV		95.73	ug N/L	0.198473				seal	2025-03-05
	CCB	CCB		0.73	ug N/L	0.003725				seal	2025-03-05
27	U24	405	7_24_405_44967_OWC_OWC_UP_PW	3.75 B_10	ug N/L	0.009926				seal	2025-03-05
28	U25	406	7_25_406_44967_OWC_OWC_UP_PW	1.53 B_20	ug N/L	0.005369				seal	2025-03-05
29	U26	407	7_27_407_44967_OWC_OWC_UP_PW	34.09 C_10	ug N/L	0.072113				seal	2025-03-05
30	U27	408	7_28_408_44967_OWC_OWC_UP_PW	2.73 C_20	ug N/L	0.007826				seal	2025-03-05
31	U28	409	7_29_409_44967_OWC_OWC_UP_PW	3.61 C_45	ug N/L	0.009624				seal	2025-03-05
32	U29	410	7_31_410_44967_OWC_OWC_TR_RZ	2.05 _	ug N/L	0.006434				seal	2025-03-05
33	U30	411	7_32_411_44967_OWC_OWC_TR_RZ	2.42 _	ug N/L	0.007196				seal	2025-03-05
34	U31	412	7_33_412_44967_OWC_OWC_TR_RZ	3.97 _	ug N/L	0.010366				seal	2025-03-05
35	U32	413	7_34_413_44967_OWC_OWC_TR_RZ	3.46 _	ug N/L	0.009325				seal	2025-03-05
36	U33	414	7_35_414_44967_OWC_OWC_TR_RZ	2.85 _	ug N/L	0.008070				seal	2025-03-05
	CCV	CCV		94.98	ug N/L	0.196941				seal	2025-03-05
	CCB	CCB		1.22	ug N/L	0.004733				seal	2025-03-05
37	U34	415	7_36_415_44967_OWC_OWC_TR_RZ	5.94 _	ug N/L	0.014401				seal	2025-03-05
38	U35	416	7_37_416_44967_OWC_OWC_TR_RZ	6.36 _	ug N/L	0.015261				seal	2025-03-05
39	U36	417	7_38_417_44967_OWC_OWC_TR_RZ	4.88 _	ug N/L	0.012238				seal	2025-03-05
40	U37	418	7_41_418_44967_OWC_OWC_UP_RZ	12.21 _	ug N/L	0.027251				seal	2025-03-05
41	U38	419	7_42_419_44967_OWC_OWC_UP_RZ	19.19 _	ug N/L	0.041569				seal	2025-03-05
42	U39	420	7_43_420_44967_OWC_OWC_UP_RZ	12.06 _	ug N/L	0.026945				seal	2025-03-05
43	U40	421	7_44_421_44967_OWC_OWC_UP_RZ	18.56 _	ug N/L	0.040274				seal	2025-03-05
44	U41	422	7_45_422_44967_OWC_OWC_UP_RZ	23.46 _	ug N/L	0.050325				seal	2025-03-05
45	U42	423	7_46_423_44967_OWC_OWC_UP_RZ	5.56 _	ug N/L	0.013628				seal	2025-03-05
46	U43	424	7_48_424_44967_OWC_OWC_UP_RZ	20.21 _	ug N/L	0.043653				seal	2025-03-05
	CCV	CCV		89.59	ug N/L	0.185886				seal	2025-03-05
	CCB	CCB		2.53	ug N/L	0.007425				seal	2025-03-05
47	U44	425	7_49_425_44967_OWC_OWC__Strear	18.47	ug N/L	0.040100				seal	2025-03-05
48	U45	426	7_51_426_44978_CRC_CRC_W_PW_S	3.34 10	ug N/L	0.009073				seal	2025-03-05
49	U46	427	7_52_427_44978_CRC_CRC_W_PW_S	2.23 20	ug N/L	0.006798				seal	2025-03-05
50	U47	428	7_53_428_44978_CRC_CRC_W_PW_S	1.78 45	ug N/L	0.005880				seal	2025-03-05
51	U48	429	7_54_429_44978_CRC_CRC_W_PW_S	2.31 10	ug N/L	0.006957				seal	2025-03-05
52	U49	430	7_55_430_44978_CRC_CRC_W_PW_S	2.09 20	ug N/L	0.006511				seal	2025-03-05
53	U50	431	7_56_431_44978_CRC_CRC_W_PW_S	2.08 45	ug N/L	0.006493				seal	2025-03-05
54	U51	432	7_57_432_44978_CRC_CRC_W_PW_S	2.86 10	ug N/L	0.008089				seal	2025-03-05

Tech Support

Cup	Type	ID	Details	Result	Units	Raw data	QC Pro	Auto dil.	Man dil.	User	Time &
58	U55	436	7_62_436_44978_CRC_CRC_TR_PW_	1.74 _20	ug N/L	0.005804				seal	2025-03-05
59	U56	437	7_63_437_44978_CRC_CRC_TR_PW_	2.16 _45	ug N/L	0.006657				seal	2025-03-05
60	U57	438	7_64_438_44978_CRC_CRC_TR_PW_	1.92 _10	ug N/L	0.006172				seal	2025-03-05
61	U58	439	7_65_439_44978_CRC_CRC_TR_PW_	1.21 _20	ug N/L	0.004705				seal	2025-03-05
62	U59	440	7_66_440_44978_CRC_CRC_TR_PW_	1.96 _45	ug N/L	0.006254				seal	2025-03-05
63	U60	441	7_67_441_44978_CRC_CRC_TR_PW_	1.58 _10	ug N/L	0.005475				seal	2025-03-05
64	U61	442	7_68_442_44978_CRC_CRC_TR_PW_	2.46 _20	ug N/L	0.007279				seal	2025-03-05
65	U62	443	7_69_443_44978_CRC_CRC_TR_PW_	2.20 _45	ug N/L	0.006749				seal	2025-03-05
66	U63	444	7_71_444_44978_CRC_CRC_UP_PW_	16.38 _10	ug N/L	0.035816				seal	2025-03-05
	CCV	CCV		94.40	ug N/L	0.195755				seal	2025-03-05
	CCB	CCB		1.76	ug N/L	0.005831				seal	2025-03-05
67	U64	445	7_72_445_44978_CRC_CRC_UP_PW_	12.19 _20	ug N/L	0.027217				seal	2025-03-05
68	U65	446	7_74_446_44978_CRC_CRC_UP_PW_	4.83 _10	ug N/L	0.012130				seal	2025-03-05
69	U66	447	7_77_447_44978_CRC_CRC_UP_PW_	9.46 _10	ug N/L	0.021629				seal	2025-03-05
70	U67	448	7_78_448_44978_CRC_CRC__Open__	15.61	ug N/L	0.034222				seal	2025-03-05
71	U68	449	7_79_449_44978_CRC_CRC__Open__	17.01	ug N/L	0.037097				seal	2025-03-05
72	U69	450	7_80_450_44978_CRC_CRC__Open__	16.78	ug N/L	0.036621				seal	2025-03-05
73	U70	451	7_80_451_44978_CRC_CRC_TR_RZ_	2.86	ug N/L	0.008099				seal	2025-03-05
74	U71	452	7_81_452_44978_CRC_CRC_TR_RZ_	3.51	ug N/L	0.009425				seal	2025-03-05
75	U72	453	7_83_453_44978_CRC_CRC_TR_RZ_	4.78	ug N/L	0.012033				seal	2025-03-05
76	U73	454	7_85_454_44978_CRC_CRC_TR_RZ_	2.23	ug N/L	0.006809				seal	2025-03-05
	CCV	CCV		94.64	ug N/L	0.196230				seal	2025-03-05
	CCB	CCB		1.61	ug N/L	0.005531				seal	2025-03-05
77	U74	455	7_86_455_44978_CRC_CRC_TR_RZ_	2.66	ug N/L	0.007675				seal	2025-03-05
78	U75	456	7_87_456_44978_CRC_CRC_TR_RZ_	3.64	ug N/L	0.009684				seal	2025-03-05
79	U76	457	7_88_457_44978_CRC_CRC_TR_RZ_	2.47	ug N/L	0.007303				seal	2025-03-05
80	U77	458	7_91_458_44978_CRC_CRC_UP_RZ_	6.92	ug N/L	0.016418				seal	2025-03-05
81	U78	459	7_92_459_44978_CRC_CRC_UP_RZ_	9.79	ug N/L	0.022301				seal	2025-03-05
82	U79	460	7_93_460_44978_CRC_CRC_UP_RZ_	6.29	ug N/L	0.015124				seal	2025-03-05
83	U80	461	7_94_461_44978_CRC_CRC_UP_RZ_	9.64	ug N/L	0.021982				seal	2025-03-05
84	U81	462	7_95_462_44978_CRC_CRC_UP_RZ_	6.71	ug N/L	0.015979				seal	2025-03-05
85	U82	463	7_96_463_44978_CRC_CRC_UP_RZ_	7.35	ug N/L	0.017297				seal	2025-03-05
86	U83	464	7_97_464_44978_CRC_CRC_UP_RZ_	9.98	ug N/L	0.022690				seal	2025-03-05
	CCV	CCV		93.62	ug N/L	0.194155				seal	2025-03-05
	CCB	CCB		1.91	ug N/L	0.006148				seal	2025-03-05
87	U84	465	7_98_465_44978_CRC_CRC_UP_RZ_	14.43	ug N/L	0.031814				seal	2025-03-05
88	U85	Field Blank		1.95	ug N/L	0.006233				seal	2025-03-05
89	U86	Field Blank		1.46	ug N/L	0.005222				seal	2025-03-05
90	U87	Field Blank		2.33	ug N/L	0.007015				seal	2025-03-05
	CCV	CCV		94.12	ug N/L	0.195177				seal	2025-03-05
	CCB	CCB		1.92	ug N/L	0.006160				seal	2025-03-05

Tech Support

Cup	Type	ID	Details	Result	Units	Raw data	QC Pro	Auto dil.	Man dil.	User	Time &

Test parameters Nitrite

Test number	8		
Long test name	Nitrite	**Short test name**	NO2
Units	ug N/L	**Decimal places**	2
Test type	End Point		

Main parameters

Sample volume	450	**Water volume**	0	**Number of mixes**	2
Cuvette primes	1	**Cuvette washes**	2	**Baseline on wash**	Yes
Cadmium volume	0	**Reduction time**	0	**Diluent location**	Reagent 24

Math parameters

Reaction time	360	**Wavelength**	520nm	**Polynomial order**	1
Repeat delta check	0.250	**Auto dilution factor**	1.000	**Manual dilution factor**	0.000
Linearity Low	0.0010	**Linearity High**	0.4063	**Latest Slope**	487.8107
Alert Low	0.000	**Alert High**	0.000	**Latest Intercept**	-1.0875

Reagent parameters

Number of reagents 1

Reagent	Name	Volume	Delay	Replaced in blank
1	Sulfa-NEDD (NO2)	50	0	No

Standards

Auto Std. Number	9	**Auto Std. Concentration**	200.0000	**Exclude the Blank**	No
Auto Std. Position	Cup 2	**Standard 1 (Blank) Position**	Reagent 24	**Correlation limit**	0.9950

Standard	Value	Standard	Value	Auto Standard	Percentage	Value
1	0.0000			S90	0.4444	0.8889
				S91	0.8889	1.7778
				S92	2.4444	4.8889
				S93	5.1111	10.2222
				S94	12.4444	24.8889
				S95	25.1111	50.2222
				S96	37.5556	75.1111
				S97	75.1111	150.2222
				S98	100.0000	200.0000

Tech Support

QC PRO

Control	Low value	High value	Location	Frequency	Start before
CCV	80.0000	120.0000	Reagent 17	10	1
CCB	-4.0000	4.0000	Reagent 24	10	1
Control	**%% (+ \ -)**	**Stock Conc.**	**Spike added**	**Location**	
DUP	0.0000				
SPKA	0.0000	0.0000	0.0000	Cup 102	
SPKM	0.0000		0.0000		
SPKD	0.0000				

Advanced parameters

Set diagnostic slope & intercept	No	**Extra debubble action**	Yes
Eliminate air from transfer	Yes	**Eliminate air from cuvette wash**	No
Extra aspiration steps	0	**Smart dilution**	No

Diagnostics

Cup	Type	Result	Absorbance	T	W
1		93.93	0.194779	0.193569	-0.001210
2		0.57	0.003393	0.002265	-0.001128
6	U3	6.51	0.015579	0.014547	-0.001033
7	U4	4.34	0.011117	0.010064	-0.001053
8	U5	2.75	0.007870	0.006932	-0.000938
9	U6	12.36	0.027576	0.026624	-0.000952
10	U7	7.35	0.017306	0.016377	-0.000929
11	U8	3.35	0.009100	0.008157	-0.000943
12	U9	12.60	0.028049	0.027169	-0.000880
15	U12	7.05	0.016690	0.015824	-0.000866
16	U13	3.46	0.009329	0.008513	-0.000817
17	U14	1.87	0.006073	0.005295	-0.000778
18	U15	95.32	0.197629	0.196822	-0.000807
19	U16	0.57	0.003399	0.002584	-0.000815
20	U17	2.73	0.007824	0.006994	-0.000831
21	U18	2.50	0.007345	0.006466	-0.000878
22	U19	2.10	0.006535	0.005688	-0.000848
23	U20	2.40	0.007145	0.006269	-0.000875
24	U21	2.19	0.006719	0.005863	-0.000857
25	U22	2.25	0.006846	0.006010	-0.000836
26	U23	7.57	0.017745	0.016902	-0.000843
29	U26	4.11	0.010650	0.009856	-0.000794
30	U27	3.70	0.009823	0.008974	-0.000849
31	U28	3.26	0.008902	0.008074	-0.000828
32	U29	95.73	0.198473	0.197652	-0.000821
33	U30	0.73	0.003725	0.002800	-0.000925
34	U31	3.75	0.009926	0.009022	-0.000904
35	U32	1.53	0.005369	0.004430	-0.000939
36	U33	34.09	0.072113	0.071399	-0.000714
37	U34	2.73	0.007826	0.007021	-0.000805
38	U35	3.61	0.009624	0.008773	-0.000851
39	U36	2.05	0.006434	0.005584	-0.000850
40	U37	2.42	0.007196	0.006347	-0.000849
43	U40	3.97	0.010366	0.009523	-0.000843
44	U41	3.46	0.009325	0.008492	-0.000833

Tech Support

Cup	Type	Result	Absorbance	T	W
48	U45	5.94	0.014401	0.013608	-0.000793
49	U46	6.36	0.015261	0.014324	-0.000937
50	U47	4.88	0.012238	0.011303	-0.000935
51	U48	12.21	0.027251	0.026434	-0.000816
52	U49	19.19	0.041569	0.040817	-0.000752
53	U50	12.06	0.026945	0.026193	-0.000752
54	U51	18.56	0.040274	0.039587	-0.000688
57	U54	23.46	0.050325	0.049743	-0.000582
58	U55	5.56	0.013628	0.012939	-0.000688
59	U56	20.21	0.043653	0.042994	-0.000659
60	U57	89.59	0.185886	0.185442	-0.000443
61	U58	2.53	0.007425	0.006771	-0.000654
62	U59	18.47	0.040100	0.039481	-0.000619
63	U60	3.34	0.009073	0.008342	-0.000731
64	U61	2.23	0.006798	0.006023	-0.000775
65	U62	1.78	0.005880	0.005043	-0.000838
66	U63	2.31	0.006957	0.006132	-0.000825
67	U64	2.09	0.006511	0.005638	-0.000873
68	U65	2.08	0.006493	0.005596	-0.000897
71	U68	2.86	0.008089	0.007232	-0.000856
72	U69	3.71	0.009827	0.008932	-0.000895
73	U70	2.44	0.007234	0.006297	-0.000937
74	U71	93.61	0.194119	0.193414	-0.000705
75	U72	1.77	0.005865	0.005007	-0.000858
76	U73	2.50	0.007348	0.006472	-0.000876
77	U74	1.74	0.005804	0.004860	-0.000944
78	U75	2.16	0.006657	0.005708	-0.000949
79	U76	1.92	0.006172	0.005185	-0.000987
80	U77	1.21	0.004705	0.003706	-0.000999
81	U78	1.96	0.006254	0.005230	-0.001024
82	U79	1.58	0.005475	0.004432	-0.001043
85	U82	2.46	0.007279	0.006240	-0.001040
86	U83	2.20	0.006749	0.005703	-0.001047
87	U84	16.38	0.035816	0.034858	-0.000958
88	U85	94.40	0.195755	0.194871	-0.000884
89	U86	1.76	0.005831	0.004812	-0.001019
90	U87	12.19	0.027217	0.026229	-0.000988
91	U88	4.83	0.012130	0.011128	-0.001002
91	U89	9.46	0.021629	0.020661	-0.000968
91	U90	15.61	0.034222	0.033151	-0.001071
91	U91	17.01	0.037097	0.036050	-0.001047
91	U92	16.78	0.036621	0.035572	-0.001048
91	U93	2.86	0.008099	0.006952	-0.001147
94		3.51	0.009425	0.008327	-0.001098
95		4.78	0.012033	0.010938	-0.001095
96		2.23	0.006809	0.005690	-0.001119
97		94.64	0.196230	0.195253	-0.000977
98		1.61	0.005531	0.004498	-0.001033
99		2.66	0.007675	0.006580	-0.001096
100		3.64	0.009684	0.008615	-0.001069
101		2.47	0.007303	0.006486	-0.000817
102		6.92	0.016418	0.015340	-0.001077

Tech Support

Cup	Type	Result	Absorbance	T	W
0		9.98	0.022690	0.021557	-0.001134
0		93.62	0.194155	0.193099	-0.001055
0		1.91	0.006148	0.004957	-0.001191
0		14.43	0.031814	0.030728	-0.001086
0		1.95	0.006233	0.005089	-0.001144
0		1.46	0.005222	0.004065	-0.001156
0		2.33	0.007015	0.005852	-0.001163
0		94.12	0.195177	0.194070	-0.001108
0		1.92	0.006160	0.005044	-0.001116

Tech Support

Ammonia (PPS)

Calibration data

ID	Absorbance	Calc mg N/L	Target mg N/L	% Error
S1	0.0057	-0.0070	0.0000	
S90	0.0315	0.1161	0.1200	-3.2718
S91	0.0623	0.2623	0.2600	0.8960
S92	0.1170	0.5227	0.5200	0.5146
S93	0.1649	0.7508	0.7400	1.4660
S94	0.2181	1.0040	1.0000	0.4019
S95	0.3246	1.5111	1.5200	-0.5875
*96	0.3914	1.8292	2.0000	-8.5414
S0	0.0077	0.0024	0.0000	

Calibration status

Polynomial order	1
Correlation coefficient	0.9999
RSE (%)	1.90
Carryover(%)	0.0
Calibration equation	y = bx + a
y =	Concentration mg N/L
x =	Measured absorbance
a =	-3.403773E-02
b =	4.760067E+00
Original Date & Time	2025-03-05 12:16:38
	(2025-03-05 11:30:52)

Calibration graph

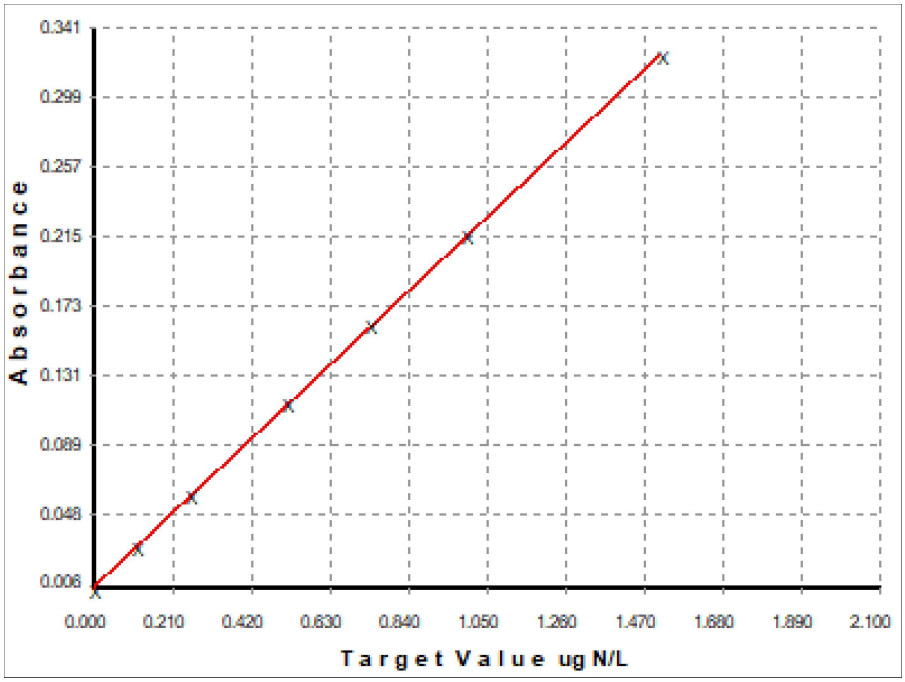

Reagents

Number	Reagent name	Batch number	User	Expiry date
1	Citrate reagent (NH4)		seal	
2	PPS (NH4)			
3	Hypochorite reagent (NH4)			
39	DI Water (Blank)		UTESE	

Tech Support

Test results

Cup	Type	ID	Details	Result	Units	Raw data	QC Pro	Auto dil.	Man dil.	User	Time &
	CCV	CCV		0.5214	mg N/L	0.116693				seal	2025-03-05
	CCB	CCB		-0.0028	mg N/L	0.006570				seal	2025-03-05
7	U4	385	7_1_385_44967_OWC_OWC_W_PW_	0.4693 10	mg N/L	0.105739				seal	2025-03-05
8	U5	386	7_2_386_44967_OWC_OWC_W_PW_	0.8795 20	mg N/L	0.191916				seal	2025-03-05
9	U6	387	7_3_387_44967_OWC_OWC_W_PW_	1.1276 45	mg N/L	0.244034				seal	2025-03-05
10	U7	388	7_4_388_44967_OWC_OWC_W_PW_	0.7552 10	mg N/L	0.165802				seal	2025-03-05
11	U8	389	7_5_389_44967_OWC_OWC_W_PW_	0.5685 20	mg N/L	0.126576				seal	2025-03-05
12	U9	390	7_6_390_44967_OWC_OWC_W_PW_	1.0547 45	mg N/L	0.228725				seal	2025-03-05
13	U10	391	7_7_391_44967_OWC_OWC_W_PW_	0.9577 10	mg N/L	0.208349				seal	2025-03-05
14	U11	392	7_8_392_44967_OWC_OWC_W_PW_	0.7538 20	mg N/L	0.165515				seal	2025-03-05
15	U12	393	7_9_393_44967_OWC_OWC_W_PW_	1.0754 45	mg N/L	0.233064				seal	2025-03-05
16	U13	394	7_11_394_44967_OWC_OWC_TR_PW	0.0407 A_10	mg N/L	0.015703				seal	2025-03-05
	CCV	CCV		0.5251	mg N/L	0.117467				seal	2025-03-05
	CCB	CCB		-0.0028	mg N/L	0.006566				seal	2025-03-05
17	U14	395	7_12_395_44967_OWC_OWC_TR_PW	0.1111 A_20	mg N/L	0.030491				seal	2025-03-05
18	U15	396	7_13_396_44967_OWC_OWC_TR_PW	0.0400 A_45	mg N/L	0.015564				seal	2025-03-05
19	U16	397	7_14_397_44967_OWC_OWC_TR_PW	0.0844 B_10	mg N/L	0.024887				seal	2025-03-05
20	U17	398	7_15_398_44967_OWC_OWC_TR_PW	0.0572 B_20	mg N/L	0.019166				seal	2025-03-05
21	U18	399	7_16_399_44967_OWC_OWC_TR_PW	0.0968 B_45	mg N/L	0.027483				seal	2025-03-05
22	U19	400	7_17_400_44967_OWC_OWC_TR_PW	0.0763 C_10	mg N/L	0.023177				seal	2025-03-05
23	U20	401	7_18_401_44967_OWC_OWC_TR_PW	0.0752 C_20	mg N/L	0.022953				seal	2025-03-05
24	U21	402	7_19_402_44967_OWC_OWC_TR_PW	0.0589 C_45	mg N/L	0.019517				seal	2025-03-05
25	U22	403	7_21_403_44967_OWC_OWC_UP_PW	0.0680 A_10	mg N/L	0.021439				seal	2025-03-05
26	U23	404	7_23_404_44967_OWC_OWC_UP_PW	0.0308 A_45	mg N/L	0.013611				seal	2025-03-05
	CCV	CCV		0.5082	mg N/L	0.113912				seal	2025-03-05
	CCB	CCB		-0.0042	mg N/L	0.006270				seal	2025-03-05
27	U24	405	7_24_405_44967_OWC_OWC_UP_PW	0.1117 B_10	mg N/L	0.030617				seal	2025-03-05
28	U25	406	7_25_406_44967_OWC_OWC_UP_PW	0.1788 B_20	mg N/L	0.044721				seal	2025-03-05
29	U26	407	7_27_407_44967_OWC_OWC_UP_PW	0.0903 C_10	mg N/L	0.026127				seal	2025-03-05
30	U27	408	7_28_408_44967_OWC_OWC_UP_PW	0.0263 C_20	mg N/L	0.012669				seal	2025-03-05
31	U28	409	7_29_409_44967_OWC_OWC_UP_PW	0.4744 C_45	mg N/L	0.106808				seal	2025-03-05
32	U29	410	7_31_410_44967_OWC_OWC_TR_RZ	0.0758	mg N/L	0.023078				seal	2025-03-05
33	U30	411	7_32_411_44967_OWC_OWC_TR_RZ	0.0747	mg N/L	0.022840				seal	2025-03-05
34	U31	412	7_33_412_44967_OWC_OWC_TR_RZ	0.0290	mg N/L	0.013245				seal	2025-03-05
35	U32	413	7_34_413_44967_OWC_OWC_TR_RZ	0.0521	mg N/L	0.018102				seal	2025-03-05
36	U33	414	7_35_414_44967_OWC_OWC_TR_RZ	0.0790	mg N/L	0.023749				seal	2025-03-05
	CCV	CCV		0.4979	mg N/L	0.111746				seal	2025-03-05
	CCB	CCB		-0.0026	mg N/L	0.006609				seal	2025-03-05
37	U34	415	7_36_415_44967_OWC_OWC_TR_RZ	0.0719	mg N/L	0.022263				seal	2025-03-05
38	U35	416	7_37_416_44967_OWC_OWC_TR_RZ	0.0866	mg N/L	0.025338				seal	2025-03-05
39	U36	417	7_38_417_44967_OWC_OWC_TR_RZ	0.0451	mg N/L	0.016624				seal	2025-03-05
40	U37	418	7_41_418_44967_OWC_OWC_UP_RZ	0.0446	mg N/L	0.016516				seal	2025-03-05
41	U38	419	7_42_419_44967_OWC_OWC_UP_RZ	0.0381	mg N/L	0.015154				seal	2025-03-05
42	U39	420	7_43_420_44967_OWC_OWC_UP_RZ	0.0359	mg N/L	0.014689				seal	2025-03-05
43	U40	421	7_44_421_44967_OWC_OWC_UP_RZ	0.0393	mg N/L	0.015411				seal	2025-03-05
44	U41	422	7_45_422_44967_OWC_OWC_UP_RZ	0.0985	mg N/L	0.027840				seal	2025-03-05
45	U42	423	7_46_423_44967_OWC_OWC_UP_RZ	0.0340	mg N/L	0.014295				seal	2025-03-05
46	U43	424	7_48_424_44967_OWC_OWC_UP_RZ	0.0457	mg N/L	0.016756				seal	2025-03-05
	CCV	CCV		0.4834	mg N/L	0.108706				seal	2025-03-05
	CCB	CCB		-0.0023	mg N/L	0.006671				seal	2025-03-05

Tech Support

Cup	Type	ID	Details	Result	Units	Raw data	QC Pro	Auto dil.	Man dil.	User	Time &
55	U52	433	7_58_433_44978_CRC_CRC_W_PW_	0.3302 0	mg N/L	0.076513				seal	2025-03-05
56	U53	434	7_59_434_44978_CRC_CRC_W_PW_	0.2327 5	mg N/L	0.056032				seal	2025-03-05
	CCV	CCV		0.5224	mg N/L	0.116896				seal	2025-03-05
	CCB	CCB		-0.0019	mg N/L	0.006748				seal	2025-03-05
57	U54	435	7_61_435_44978_CRC_CRC_TR_PW_	0.1483 10	mg N/L	0.038306				seal	2025-03-05
58	U55	436	7_62_436_44978_CRC_CRC_TR_PW_	0.1504 20	mg N/L	0.038738				seal	2025-03-05
59	U56	437	7_63_437_44978_CRC_CRC_TR_PW_	0.0863 45	mg N/L	0.025278				seal	2025-03-05
60	U57	438	7_64_438_44978_CRC_CRC_TR_PW_	0.1688 10	mg N/L	0.042608				seal	2025-03-05
61	U58	439	7_65_439_44978_CRC_CRC_TR_PW_	0.1577 20	mg N/L	0.040291				seal	2025-03-05
62	U59	440	7_66_440_44978_CRC_CRC_TR_PW_	0.1280 45	mg N/L	0.034042				seal	2025-03-05
63	U60	441	7_67_441_44978_CRC_CRC_TR_PW_	0.1670 10	mg N/L	0.042235				seal	2025-03-05
64	U61	442	7_68_442_44978_CRC_CRC_TR_PW_	0.1617 20	mg N/L	0.041118				seal	2025-03-05
65	U62	443	7_69_443_44978_CRC_CRC_TR_PW_	0.0932 45	mg N/L	0.026734				seal	2025-03-05
66	U63	444	7_71_444_44978_CRC_CRC_UP_PW_	0.1775 10	mg N/L	0.044435				seal	2025-03-05
	CCV	CCV		0.5004	mg N/L	0.112281				seal	2025-03-05
	CCB	CCB		-0.0025	mg N/L	0.006621				seal	2025-03-05
67	U64	445	7_72_445_44978_CRC_CRC_UP_PW_	0.1195 20	mg N/L	0.032252				seal	2025-03-05
68	U65	446	7_74_446_44978_CRC_CRC_UP_PW_	0.1841 10	mg N/L	0.045829				seal	2025-03-05
69	U66	447	7_77_447_44978_CRC_CRC_UP_PW_	0.1158 10	mg N/L	0.031486				seal	2025-03-05
70	U67	448	7_78_448_44978_CRC_CRC__Open__	0.1464	mg N/L	0.037901				seal	2025-03-05
71	U68	449	7_79_449_44978_CRC_CRC__Open__	0.1037	mg N/L	0.028931				seal	2025-03-05
72	U69	450	7_80_450_44978_CRC_CRC__Open__	0.0862	mg N/L	0.025257				seal	2025-03-05
73	U70	451	7_80_451_44978_CRC_CRC_TR_RZ_	0.1106	mg N/L	0.030395				seal	2025-03-05
74	U71	452	7_81_452_44978_CRC_CRC_TR_RZ_	0.1386	mg N/L	0.036260				seal	2025-03-05
75	U72	453	7_83_453_44978_CRC_CRC_TR_RZ_	0.1071	mg N/L	0.029654				seal	2025-03-05
76	U73	454	7_85_454_44978_CRC_CRC_TR_RZ_	0.1089	mg N/L	0.030030				seal	2025-03-05
	CCV	CCV		0.4868	mg N/L	0.109426				seal	2025-03-05
	CCB	CCB		-0.0037	mg N/L	0.006379				seal	2025-03-05
77	U74	455	7_86_455_44978_CRC_CRC_TR_RZ_	0.1455	mg N/L	0.037709				seal	2025-03-05
78	U75	456	7_87_456_44978_CRC_CRC_TR_RZ_	0.1959	mg N/L	0.048314				seal	2025-03-05
79	U76	457	7_88_457_44978_CRC_CRC_TR_RZ_	0.0626	mg N/L	0.020300				seal	2025-03-05
80	U77	458	7_91_458_44978_CRC_CRC_UP_RZ_	0.0514	mg N/L	0.017950				seal	2025-03-05
81	U78	459	7_92_459_44978_CRC_CRC_UP_RZ_	0.0645	mg N/L	0.020695				seal	2025-03-05
82	U79	460	7_93_460_44978_CRC_CRC_UP_RZ_	0.0891	mg N/L	0.025875				seal	2025-03-05
83	U80	461	7_94_461_44978_CRC_CRC_UP_RZ_	0.1177	mg N/L	0.031877				seal	2025-03-05
84	U81	462	7_95_462_44978_CRC_CRC_UP_RZ_	0.0459	mg N/L	0.016803				seal	2025-03-05
85	U82	463	7_96_463_44978_CRC_CRC_UP_RZ_	0.1216	mg N/L	0.032705				seal	2025-03-05
86	U83	464	7_97_464_44978_CRC_CRC_UP_RZ_	0.0601	mg N/L	0.019783				seal	2025-03-05
	CCV	CCV		0.4929	mg N/L	0.110705				seal	2025-03-05
	CCB	CCB		-0.0048	mg N/L	0.006140				seal	2025-03-05
87	U84	465	7_98_465_44978_CRC_CRC_UP_RZ_	0.0826	mg N/L	0.024510				seal	2025-03-05
88	U85	Field Blank		0.0336	mg N/L	0.014215				seal	2025-03-05
89	U86	Field Blank		0.0356	mg N/L	0.014635				seal	2025-03-05
90	U87	Field Blank		0.1015	mg N/L	0.028475				seal	2025-03-05
	CCV	CCV		0.4747	mg N/L	0.106871				seal	2025-03-05
	CCB	CCB		-0.0036	mg N/L	0.006390				seal	2025-03-05

Tech Support

Cup	Type	ID	Details	Result	Units	Raw data	QC Pro	Auto dil.	Man dil.	User	Time &

Test parameters Ammonia (PPS)

Test number	9		
Long test name	Ammonia (PPS)	**Short test name**	NH3_PPS
Units	mg N/L	**Decimal places**	4
Test type	End Point		

Main parameters

Sample volume	300	**Water volume**	0	**Number of mixes**	2
Cuvette primes	2	**Cuvette washes**	2	**Baseline on wash**	Yes
Cadmium volume	0	**Reduction time**	0	**Diluent location**	Reagent 24

Math parameters

Reaction time	1200	**Wavelength**	660nm	**Polynomial order**	1
Repeat delta check	0.250	**Auto dilution factor**	1.000	**Manual dilution factor**	0.000
Linearity Low	0.0057	**Linearity High**	0.3246	**Latest Slope**	4.7601
Alert Low	0.000	**Alert High**	0.000	**Latest Intercept**	-0.0340

Reagent parameters

Number of reagents 3

Reagent	Name	Volume	Delay	Replaced in blank
1	Citrate reagent (NH4)	100	0	No
2	PPS (NH4)	100	300	No
3	Hypochorite reagent (NH450		321	No

Standards

Auto Std. Number	7	**Auto Std. Concentration**	2.0000	**Exclude the Blank**	No
Auto Std. Position	Cup 1	**Standard 1 (Blank) Position**	Reagent 24	**Correlation limit**	0.9900

Standard	Value	Standard	Value	Auto Standard	Percentage	Value
1	0.0000			S90	6.0000	0.1200
				S91	13.0000	0.2600
				S92	26.0000	0.5200
				S93	37.0000	0.7400
				S94	50.0000	1.0000
				S95	76.0000	1.5200
				S96	100.0000	2.0000

Tech Support

QC PRO

Control	Low value	High value	Location	Frequency	Start before
CCV	0.3000	0.7000	Reagent 10	10	1
CCB	-0.0400	0.0400	Reagent 24	10	1
Control	**%% (+ \ -)**	**Stock Conc.**	**Spike added**	**Location**	
DUP	0.0000				
SPKA	10.0000	10.0000	0.5000	Cup 101	
SPKM	0.0000		0.0000		
SPKD	0.0000				

Advanced parameters

Set diagnostic slope & intercept	No	**Extra debubble action**	Yes
Eliminate air from transfer	Yes	**Eliminate air from cuvette wash**	No
Extra aspiration steps	0	**Smart dilution**	No

Diagnostics

Cup	Type	Result	Absorbance	T	W
1		0.5214	0.116693	0.115082	-0.001611
2		-0.0028	0.006570	0.004947	-0.001623
6	U3	0.4693	0.105739	0.103970	-0.001769
7	U4	0.8795	0.191916	0.190130	-0.001786
8	U5	1.1276	0.244034	0.242314	-0.001720
9	U6	0.7552	0.165802	0.164072	-0.001729
10	U7	0.5685	0.126576	0.124897	-0.001680
11	U8	1.0547	0.228725	0.227032	-0.001694
12	U9	0.9577	0.208349	0.206734	-0.001614
15	U12	0.7538	0.165515	0.163944	-0.001571
16	U13	1.0754	0.233064	0.231461	-0.001603
17	U14	0.0407	0.015703	0.014097	-0.001605
18	U15	0.5251	0.117467	0.115939	-0.001529
19	U16	-0.0028	0.006566	0.005047	-0.001519
20	U17	0.1111	0.030491	0.028929	-0.001562
21	U18	0.0400	0.015564	0.014056	-0.001508
22	U19	0.0844	0.024887	0.023298	-0.001589
23	U20	0.0572	0.019166	0.017589	-0.001577
24	U21	0.0968	0.027483	0.025962	-0.001521
25	U22	0.0763	0.023177	0.021597	-0.001580
26	U23	0.0752	0.022953	0.021390	-0.001563
29	U26	0.0589	0.019517	0.017968	-0.001549
30	U27	0.0680	0.021439	0.020351	-0.001088
31	U28	0.0308	0.013611	0.012168	-0.001443
32	U29	0.5082	0.113912	0.112523	-0.001389
33	U30	-0.0042	0.006270	0.004902	-0.001368
34	U31	0.1117	0.030617	0.029054	-0.001563
35	U32	0.1788	0.044721	0.043083	-0.001638
36	U33	0.0903	0.026127	0.024461	-0.001666
37	U34	0.0263	0.012669	0.011026	-0.001643
38	U35	0.4744	0.106808	0.105147	-0.001660
39	U36	0.0758	0.023078	0.021414	-0.001664
40	U37	0.0747	0.022840	0.021199	-0.001641
43	U40	0.0290	0.013245	0.011572	-0.001673
44	U41	0.0521	0.018102	0.016400	-0.001701

Tech Support

Cup	Type	Result	Absorbance	T	W
48	U45	0.0719	0.022263	0.020658	-0.001605
49	U46	0.0866	0.025338	0.023707	-0.001631
50	U47	0.0451	0.016624	0.014978	-0.001645
51	U48	0.0446	0.016516	0.014823	-0.001693
52	U49	0.0381	0.015154	0.013518	-0.001636
53	U50	0.0359	0.014689	0.012997	-0.001692
54	U51	0.0393	0.015411	0.013729	-0.001681
57	U54	0.0985	0.027840	0.026131	-0.001709
58	U55	0.0340	0.014295	0.012587	-0.001708
59	U56	0.0457	0.016756	0.015100	-0.001657
60	U57	0.4834	0.108706	0.107114	-0.001592
61	U58	-0.0023	0.006671	0.005108	-0.001563
62	U59	0.0693	0.021699	0.020087	-0.001613
63	U60	0.1884	0.046725	0.045050	-0.001675
64	U61	0.1666	0.042158	0.040483	-0.001675
65	U62	0.1774	0.044417	0.042671	-0.001746
66	U63	0.2047	0.050154	0.048461	-0.001692
67	U64	0.1423	0.037053	0.035312	-0.001741
68	U65	0.1233	0.033044	0.031352	-0.001693
71	U68	0.1480	0.038243	0.036484	-0.001760
72	U69	0.3302	0.076513	0.074731	-0.001782
73	U70	0.2327	0.056032	0.054262	-0.001770
74	U71	0.5224	0.116896	0.115250	-0.001646
75	U72	-0.0019	0.006748	0.005111	-0.001636
76	U73	0.1483	0.038306	0.036601	-0.001705
77	U74	0.1504	0.038738	0.037014	-0.001724
78	U75	0.0863	0.025278	0.023538	-0.001740
79	U76	0.1688	0.042608	0.040793	-0.001815
80	U77	0.1577	0.040291	0.038555	-0.001735
81	U78	0.1280	0.034042	0.032272	-0.001770
82	U79	0.1670	0.042235	0.040437	-0.001798
85	U82	0.1617	0.041118	0.039283	-0.001836
86	U83	0.0932	0.026734	0.024902	-0.001832
87	U84	0.1775	0.044435	0.042583	-0.001852
88	U85	0.5004	0.112281	0.110503	-0.001777
89	U86	-0.0025	0.006621	0.004887	-0.001735
90	U87	0.1195	0.032252	0.030407	-0.001845
91	U88	0.1841	0.045829	0.043933	-0.001896
91	U89	0.1158	0.031486	0.029623	-0.001863
91	U90	0.1464	0.037901	0.036103	-0.001798
91	U91	0.1037	0.028931	0.027073	-0.001859
91	U92	0.0862	0.025257	0.023364	-0.001894
91	U93	0.1106	0.030395	0.028529	-0.001866
94		0.1386	0.036260	0.034372	-0.001888
95		0.1071	0.029654	0.027886	-0.001768
96		0.1089	0.030030	0.028088	-0.001942
97		0.4868	0.109426	0.107557	-0.001869
98		-0.0037	0.006379	0.004529	-0.001849
99		0.1455	0.037709	0.035798	-0.001911
100		0.1959	0.048314	0.046436	-0.001879
101		0.0626	0.020300	0.018453	-0.001847
102		0.0514	0.017950	0.016118	-0.001832

Tech Support

Cup	Type	Result	Absorbance	T	W
0		0.0601	0.019783	0.017916	-0.001867
0		0.4929	0.110705	0.108903	-0.001801
0		-0.0048	0.006140	0.004330	-0.001810
0		0.0826	0.024510	0.022666	-0.001844
0		0.0336	0.014215	0.012333	-0.001882
0		0.0356	0.014635	0.012753	-0.001882
0		0.1015	0.028475	0.026574	-0.001901
0		0.4747	0.106871	0.105073	-0.001799
0		-0.0036	0.006390	0.004674	-0.001716