Synoptic CB: Porewater SO4/Cl

September 2024 Samples

2025-09-22

Contents

##Add Required Packages

0.1 Run Information

```
###### Run information - PLEASE CHANGE
  Date_Run = "2025-05-29" #Date that instrument was run
  Run_by = "Zoe Read"  #Instrument user
  Script_run_by = "Zoe Read" #Code user
  run_notes = "3 samples were above the highest standard:
  2_MSM_202409_TR_LysA_10cm, 5_MSM_202409_TR_LysB_10cm, 8_MSM_202409_TR_LysC_10cm
  " #any notes from the run
  samples <- c("GCW", "GWI", "MSM", "SWH") #whatever identifies your samples within the same names
  samples_pattern <- paste(samples, collapse = "|")
    #samples_pattern <- "GCW" #use this instead of the line above if you have only one site code

###### File Names - PLEASE CHANGE
#file path and name for raw summary data file
  raw_file_name_cl = "Raw Data/COMPASS_Synoptic_CB_MonMon_202409_Cl.txt"
  raw_file_name_so4 = "Raw Data/COMPASS_Synoptic_CB_MonMon_202409_SO4.txt"

#file path and name of processed data file
  processed_file_name = "Processed Data/COMPASS_SynopticCB_PW_Processed_Cl_SO4_202409.csv"

###### Log Files - PLEASE CHECK
#downloaded metadata csv - downloaded from Google drive as csv for this year
  Raw_Metadata = "Raw Data/COMPASS_SynopticCB_PW_SampleLog_2024.csv"

#qaqc log file path for this year
  Log_path = "Raw Data/COMPASS_Synoptic_Cl_SO4_QAQClog_2024.csv"
```

##Set Up Code - constants and QAQC cutoffs

##Read in metadata and create similar sample IDs for matching to samples

##Import Sample Data

0.2 Assess Standard Curves

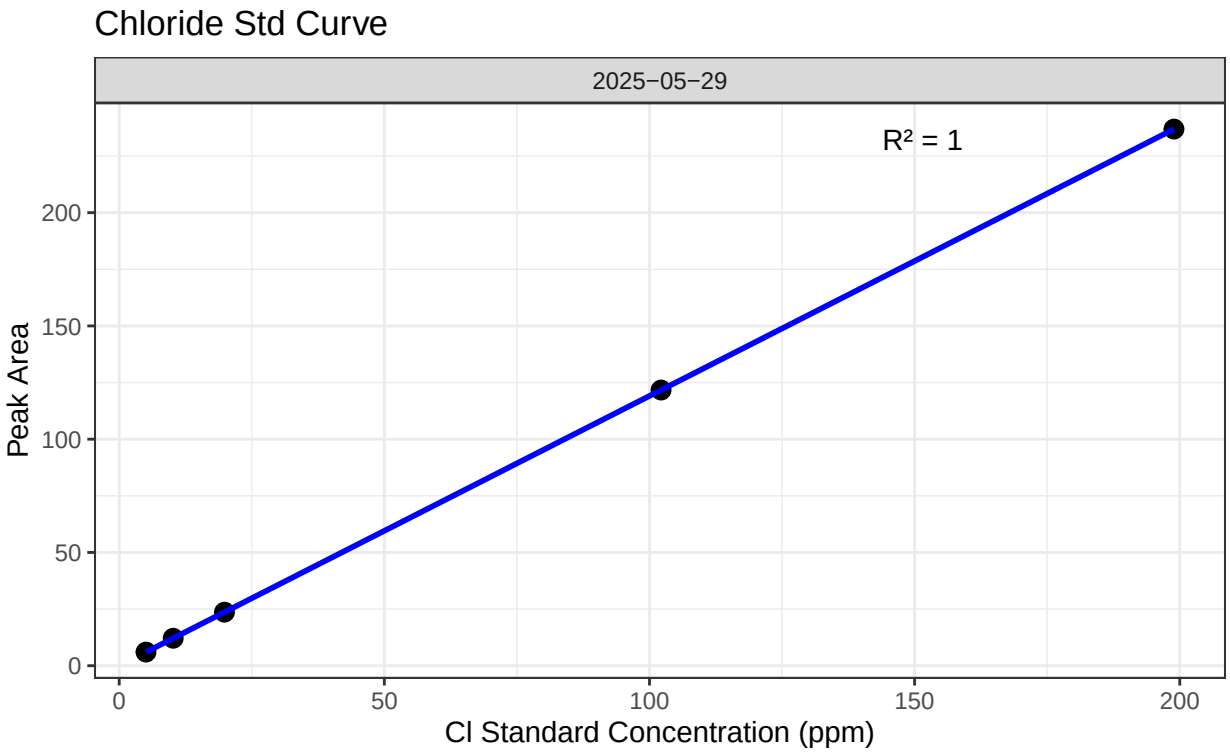

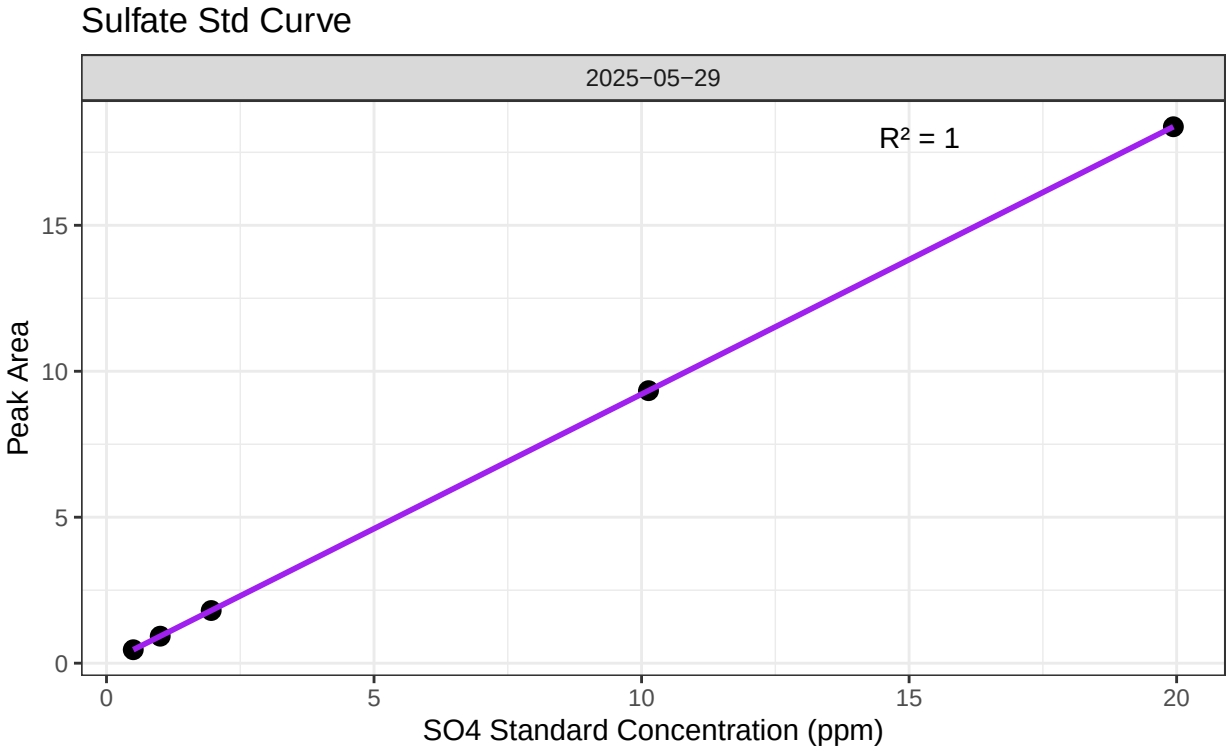


```
## [1] "QAQC log file exists and has been read into the code."
```

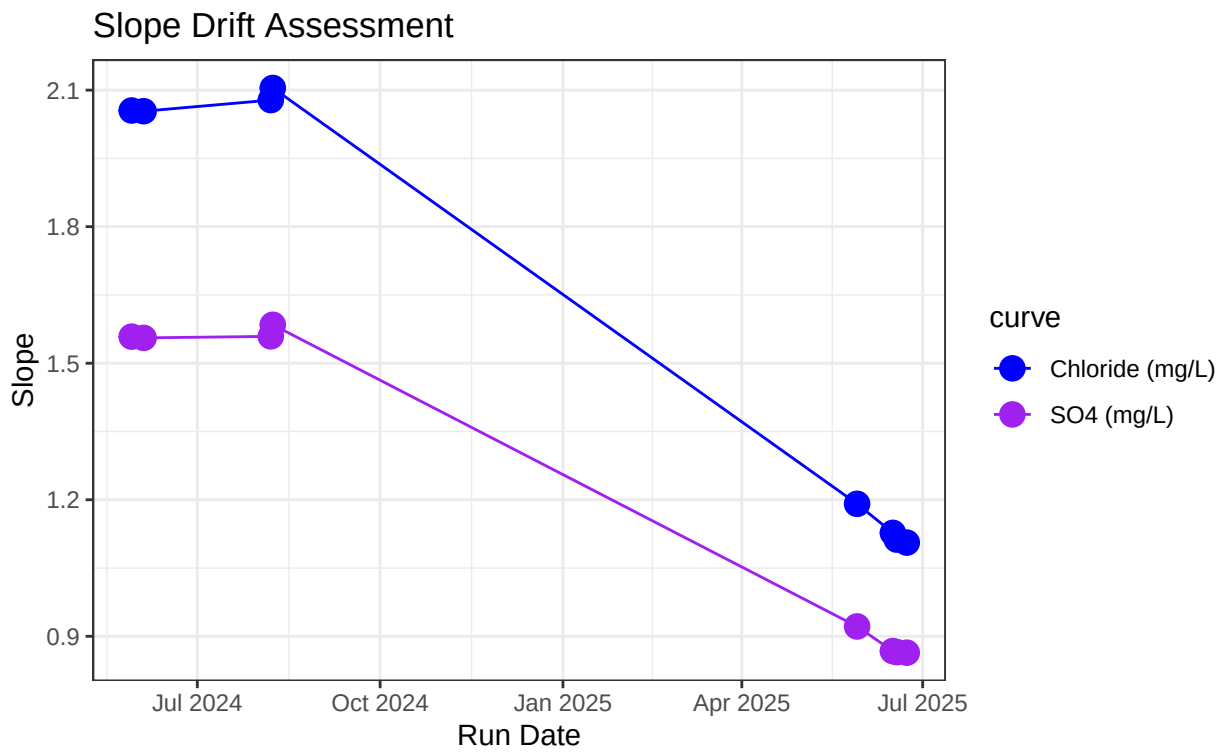


```
## [1] "Cl Curve r2 GOOD"
```

```
## [1] "SO4 Curve r2 GOOD"
```

0.3 Assess Check Standards

```
## # A tibble: 5 x 5
##   sample_ID  mean_Cl   sd_Cl    cv_Cl flag_Cl
##   <chr>        <dbl>   <dbl>    <dbl> <chr>
## 1 Standard 1    5.06 0.00247 0.000489 Chloride Check Standard RSD within Range ~
## 2 Standard 2   10.2  0.0256  0.00250  Chloride Check Standard RSD within Range ~
## 3 Standard 3   19.9  0.0950  0.00476  Chloride Check Standard RSD within Range ~
## 4 Standard 4  102.   0.153   0.00149  Chloride Check Standard RSD within Range ~
## 5 Standard 5  199.   0.172   0.000862 Chloride Check Standard RSD within Range ~
```

```
## # A tibble: 5 x 5
##   sample_ID  mean_SO4  sd_SO4   cv_SO4 flag_SO4
##   <chr>         <dbl>   <dbl>    <dbl> <chr>
## 1 Standard 1    0.501 0.00110 0.00220  Sulfate Check Standard RSD within Range ~
## 2 Standard 2    1.00  0.00149 0.00148  Sulfate Check Standard RSD within Range ~
## 3 Standard 3    1.96  0.00662 0.00337  Sulfate Check Standard RSD within Range ~
## 4 Standard 4   10.2   0.0485  0.00476  Sulfate Check Standard RSD within Range ~
## 5 Standard 5   20.0   0.0167  0.000836 Sulfate Check Standard RSD within Range ~
```

```
## [1] ">80% of Chloride Check Standards have RSD within range - PROCEED"
```

```
## [1] ">80% of Sulfate Check Standards have RSD within range - PROCEED"
```

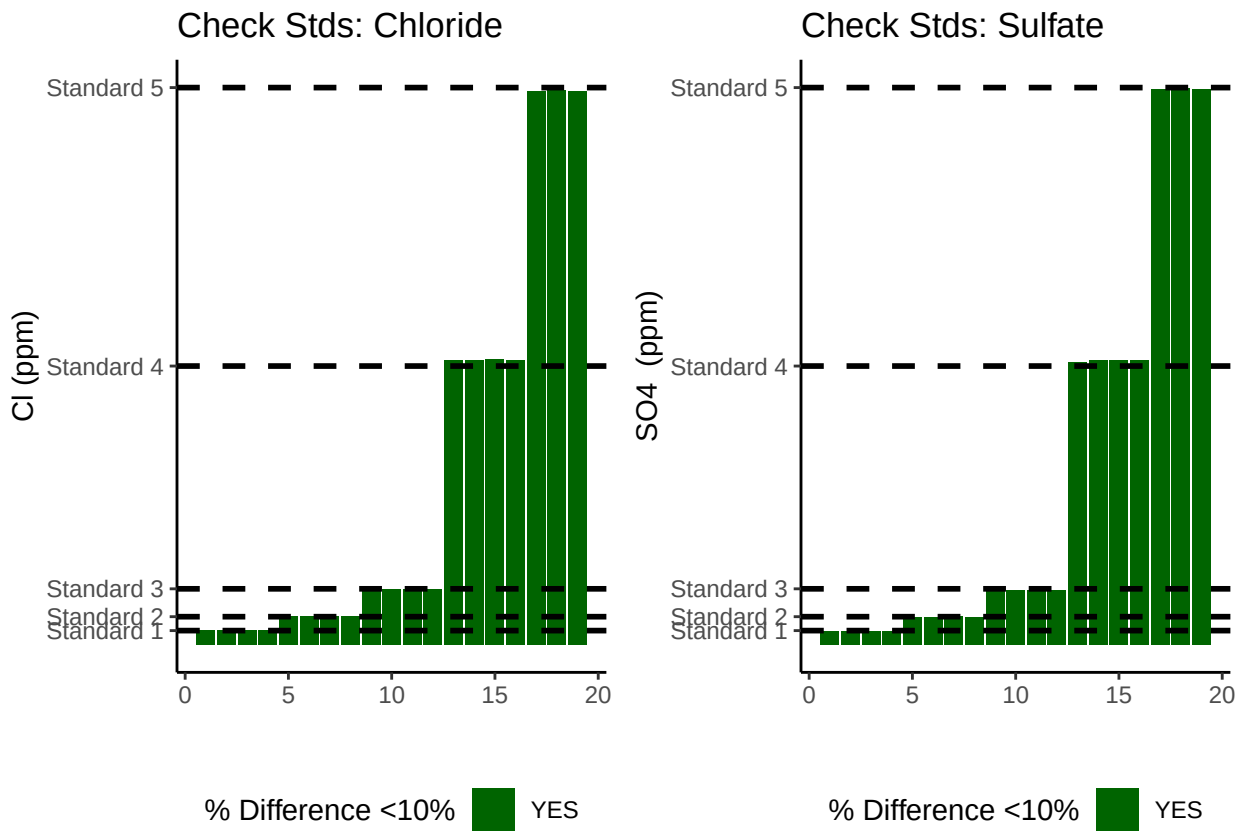


```
## [1] ">80% of Chloride Check Standards are within range of expected concentration - PROCEED"
```

```
## [1] ">80% of Sulfate Check Standards are within range of expected concentration - PROCEED"
```

0.4 Assess Blanks

```
## [1] ">80% of Chloride Blank concentrations are lower 25% quartile of samples"
```

```
## [1] ">80% of Sulfate Blank concentrations are lower 25% quartile of samples"
```

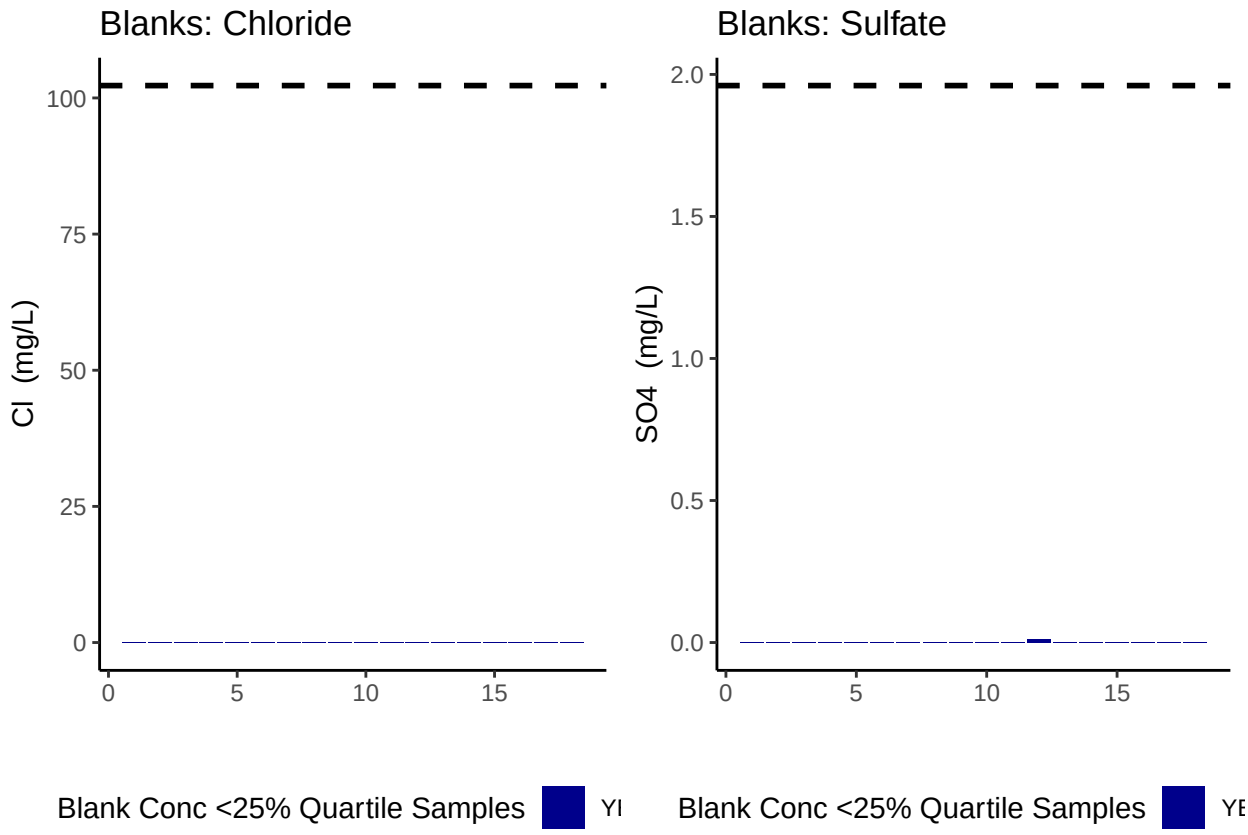


```
## Chloride blanks mean ppm:

## [1] 0.007438889

## Sulfate blanks mean ppm:

## [1] 0.0006388889
```

0.5 Assess Duplicates

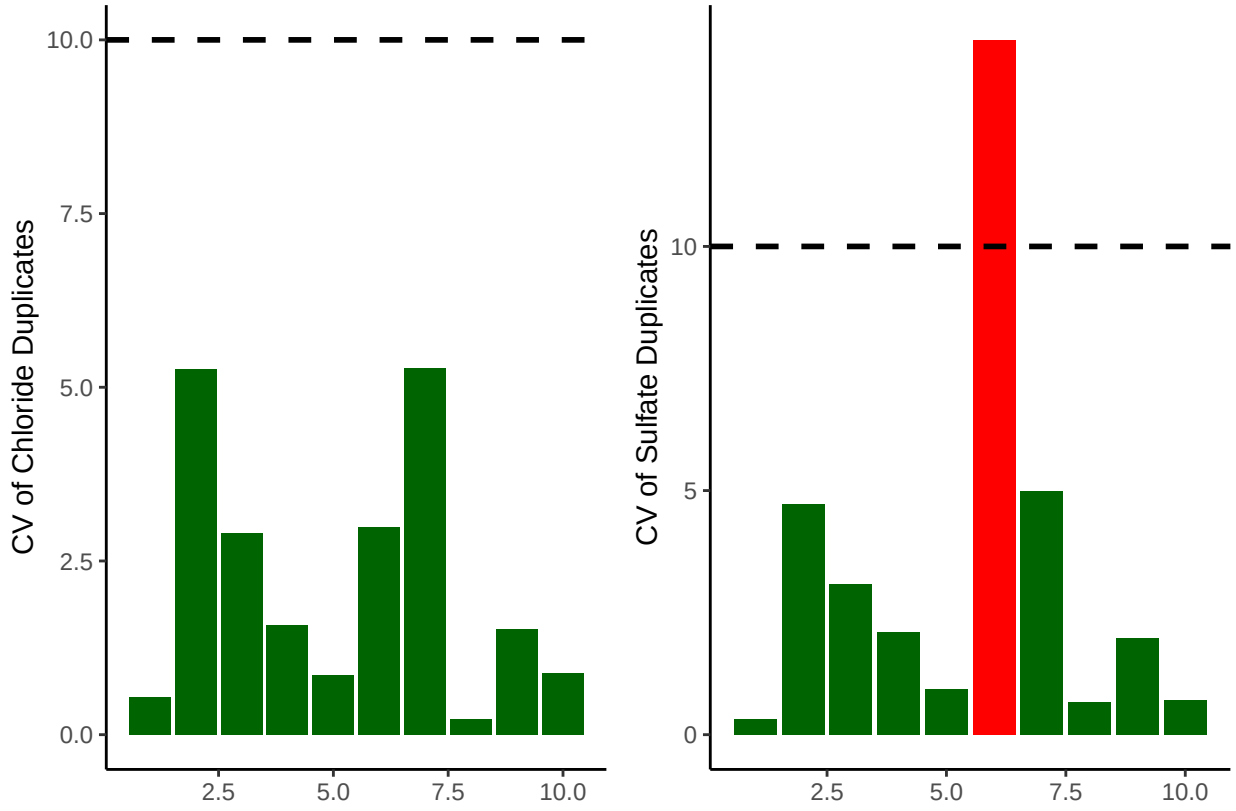


```
## [1] ">80% of Chloride Duplicates have a CV <10% - PROCEED"
```

```
## [1] ">80% of Sulfate Duplicates have a CV <10% - PROCEED"
```

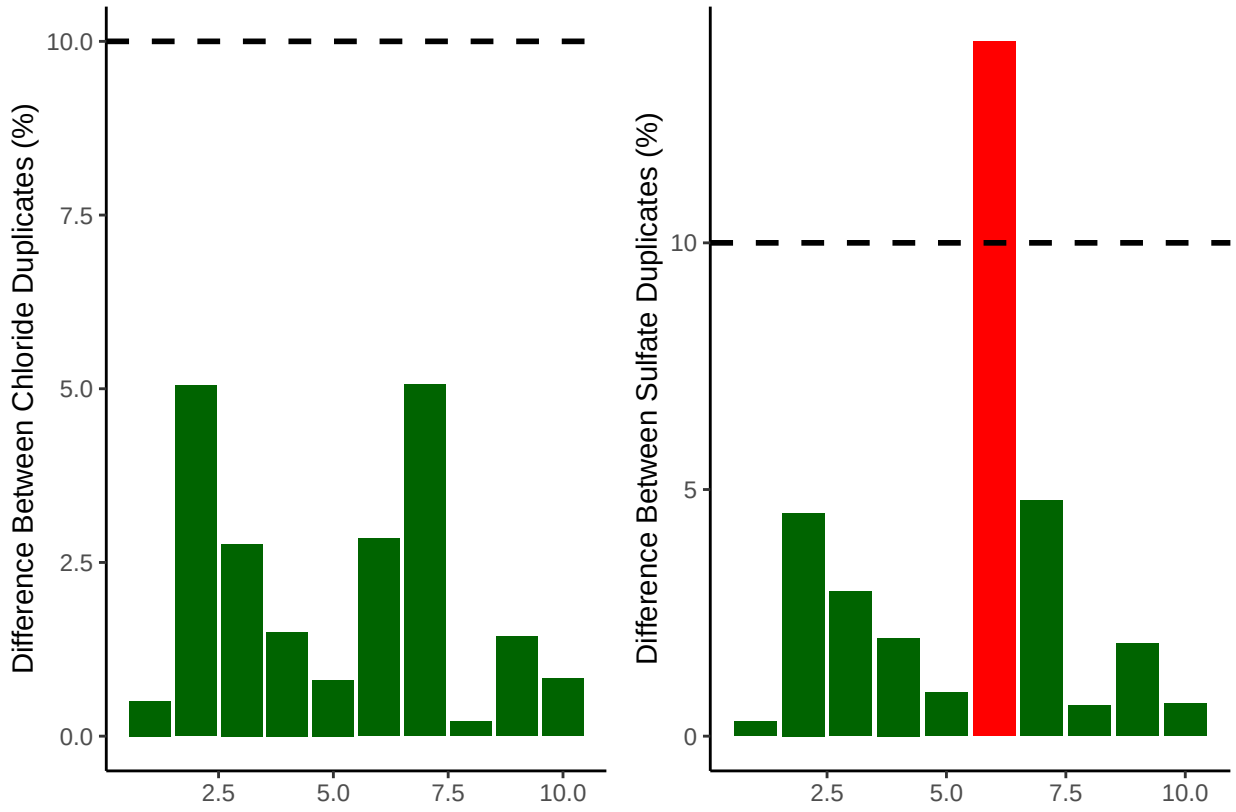


```
## [1] ">80% of Chloride Duplicates have a percent difference <10% - PROCEED"
```

```
## [1] ">80% of Sulfate Duplicates have a percent difference <10% - PROCEED"
```

0.6 Calculate mmol/L concentrations & salinity, add dilutions

```
# Convert ppm to mmol/L
all_dat$SO4_Conc_mM <- (all_dat$SO4_ppm / s_mw)
all_dat$Cl_Conc_mM <- (all_dat$Cl_ppm / cl_mw)

# Calculate Salinity
# calculated using the Knudsen equation
# Salinity = 0.03 + 1.8050 * Chlorinity
# Ref: A Practical Handbook of Seawater Analysis by Strickland & Parsons (P. 11)
# =((1.807*Cl_ppm)+0.026)/1000
all_dat$salinity <- ((1.8070 * all_dat$Cl_ppm) + 0.026) / 1000

#Need to determine dilution factors for your samples
#for Steph / COMPASS this depends on the site so...
all_dat$Dilution <- 1
all_dat$Dilution <-  ifelse(str_detect(all_dat$sample_ID, "MSM") & str_detect(all_dat$sample_ID, "UP"),
all_dat$Dilution <-  ifelse(str_detect(all_dat$sample_ID, "MSM") & str_detect(all_dat$sample_ID, "TR"),
all_dat$Dilution <-  ifelse(str_detect(all_dat$sample_ID, "MSM") & str_detect(all_dat$sample_ID, "WC"),
```

```r
all_dat$Dilution <-  ifelse(str_detect(all_dat$sample_ID, "MSM") & str_detect(all_dat$sample_ID, "SW"),

all_dat$Dilution <-  ifelse(str_detect(all_dat$sample_ID, "GCW") & str_detect(all_dat$sample_ID, "UP"),
all_dat$Dilution <-  ifelse(str_detect(all_dat$sample_ID, "GCW") & str_detect(all_dat$sample_ID, "TR"),
all_dat$Dilution <-  ifelse(str_detect(all_dat$sample_ID, "GCW") & str_detect(all_dat$sample_ID, "WC"),
all_dat$Dilution <-  ifelse(str_detect(all_dat$sample_ID, "GCW") & str_detect(all_dat$sample_ID, "SW"),

all_dat$Dilution <-  ifelse(str_detect(all_dat$sample_ID, "GWI") & str_detect(all_dat$sample_ID, "UP"),
all_dat$Dilution <-  ifelse(str_detect(all_dat$sample_ID, "GWI") & str_detect(all_dat$sample_ID, "TR"),
all_dat$Dilution <-  ifelse(str_detect(all_dat$sample_ID, "GWI") & str_detect(all_dat$sample_ID, "WC"),
all_dat$Dilution <-  ifelse(str_detect(all_dat$sample_ID, "GWI") & str_detect(all_dat$sample_ID, "SW"),

all_dat$Dilution <-  ifelse(str_detect(all_dat$sample_ID, "SWH"), 50, all_dat$Dilution)

# head(all_dat)
```

0.7 Assess Analytical Spikes

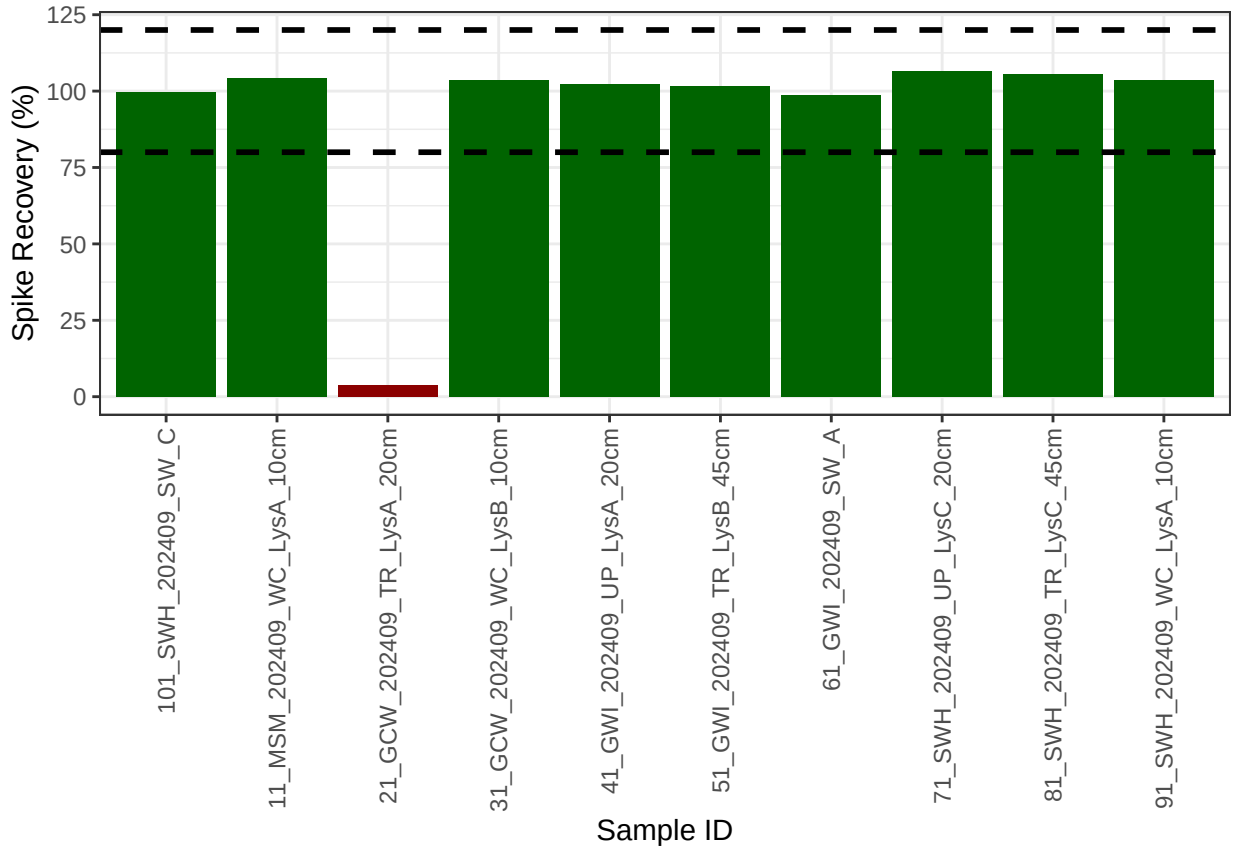


```
## [1] ">80% of SO4 spikes have a recovery between the high and low cutoff - PROCEED"
```

0.8 Check if samples within the range of the standard curve

```
## Sample Flagging
```

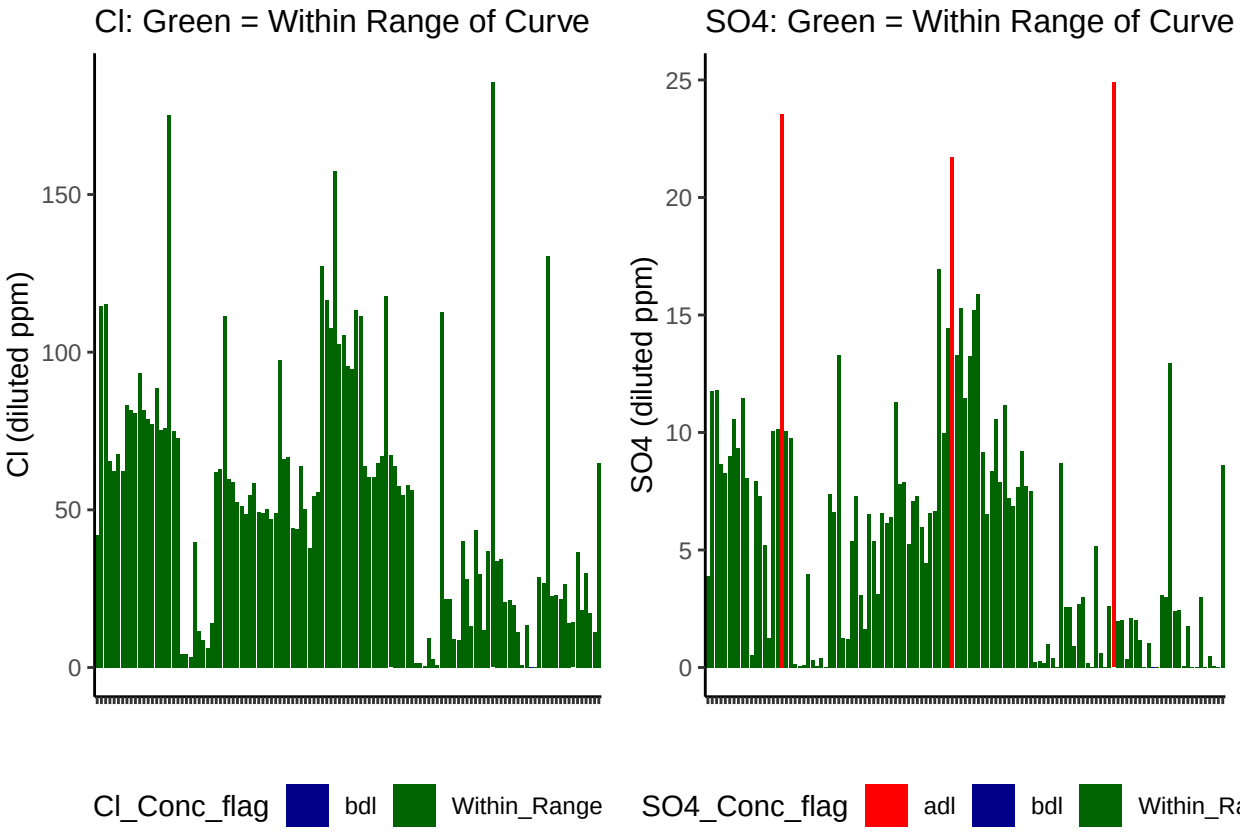

Table 1: SO4 samples

SO4_Conc_flag	Percent_samples
Within_Range	96.6386555
adl	2.5210084
bdl	0.8403361

Table 2: Cl samples

Cl_Conc_flag	Percent_samples
Within_Range	99.1596639
bdl	0.8403361

0.9 Check to see if samples run match metadata & merge info

```
## All sample IDs are present in metadata.
```

0.10 Visualize Data by Plot

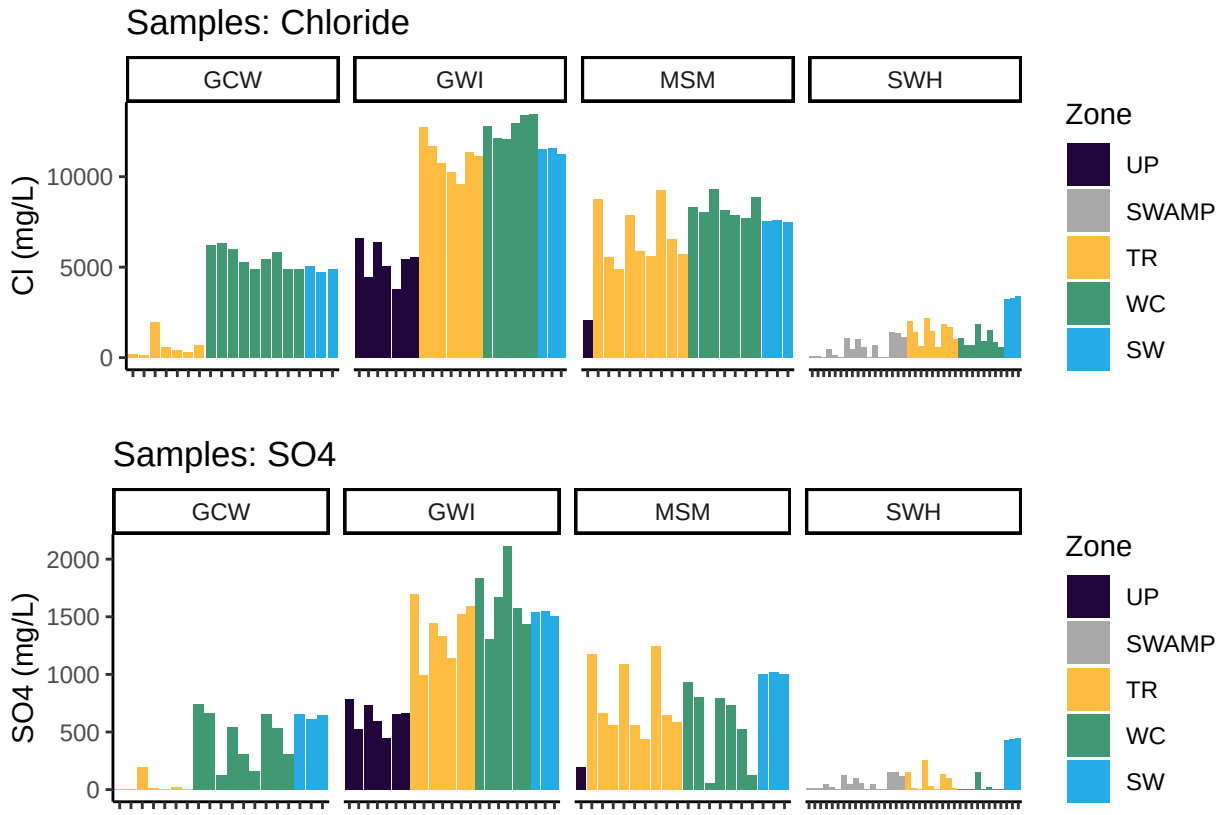

0.11 Export Processed Data

#end