



COMPASS_Iron_Reacidification_Comparison_2026


Zoe Read

2026-03-12

##Collected samples from TEMPEST and GCW TR in March 2026. Some samples were added directly to vials with 75 uL of 50% HCl in the field, some samples were added to empty vials, and then those were acidified in the lab a few weeks later using 75 uL HCl.

Mean with SD Plot Acidified vs Re-acidified Samples

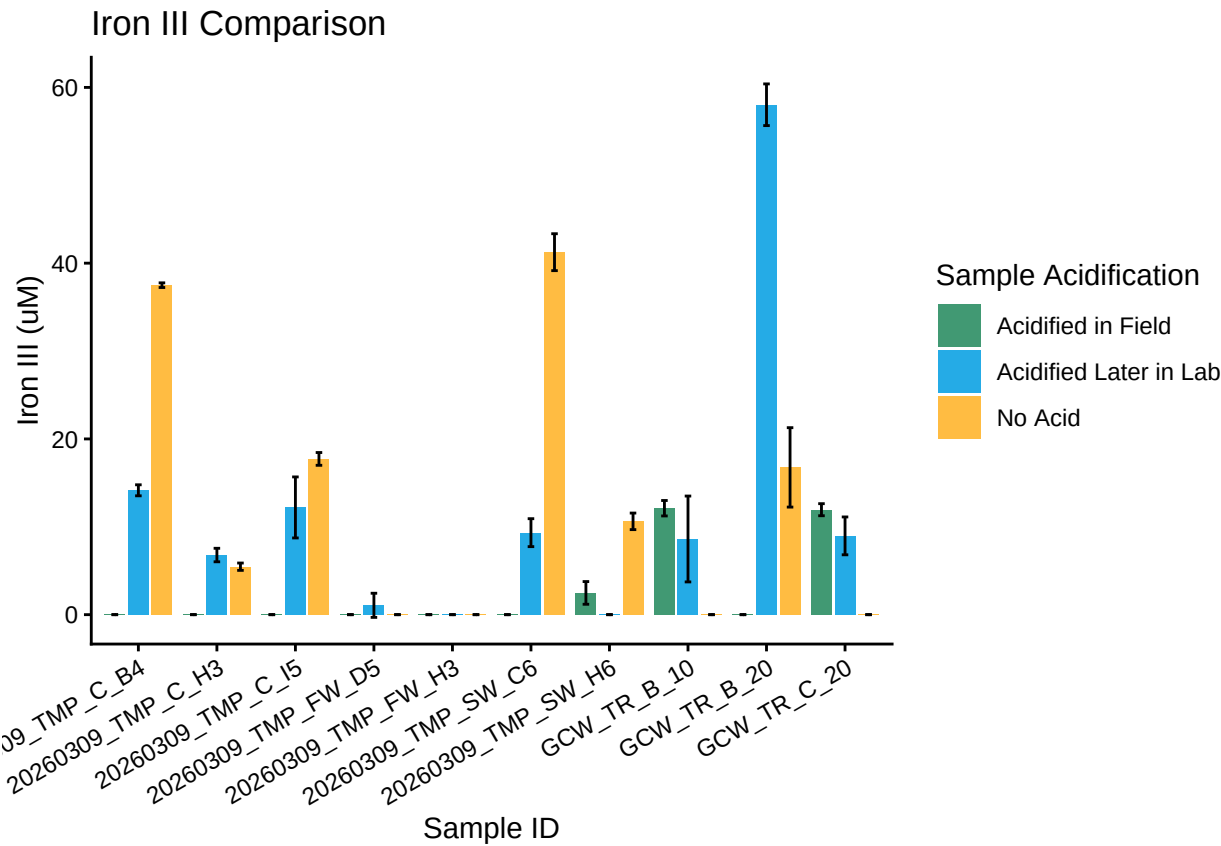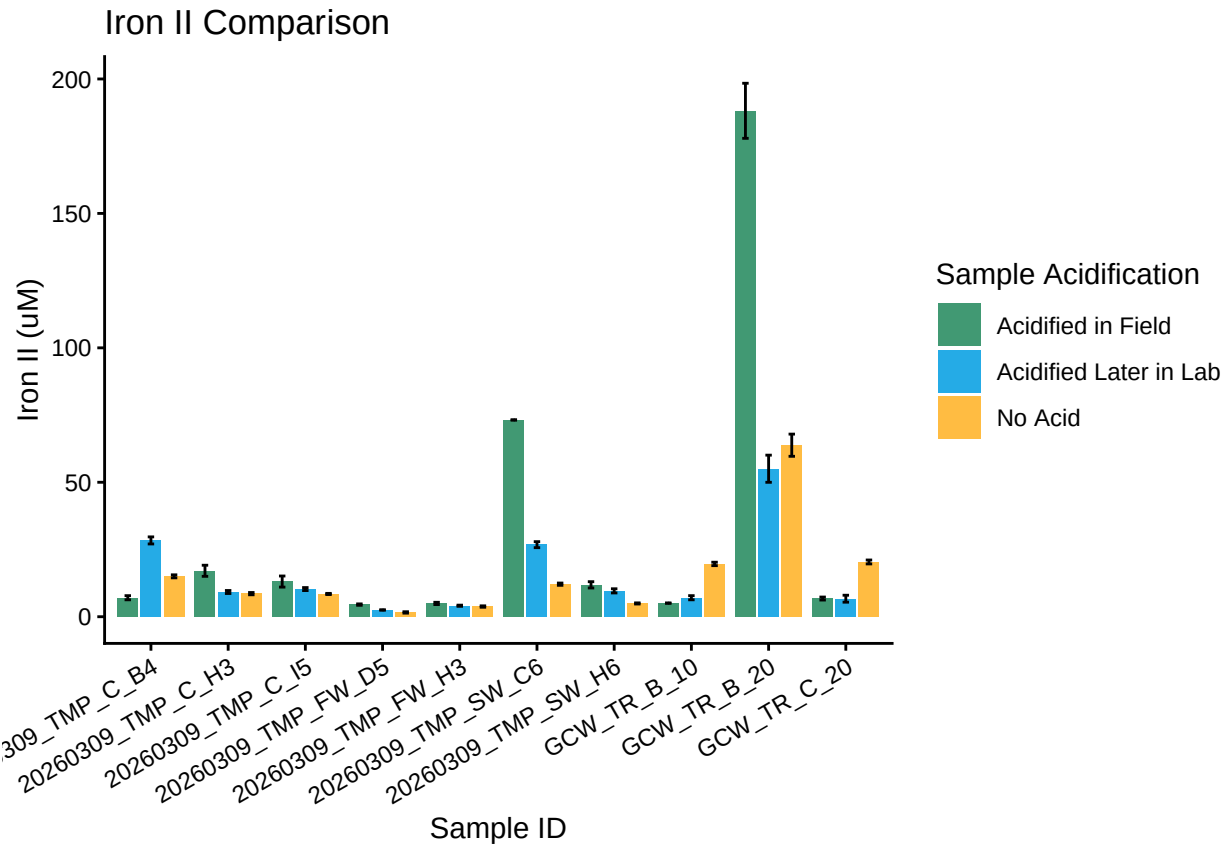


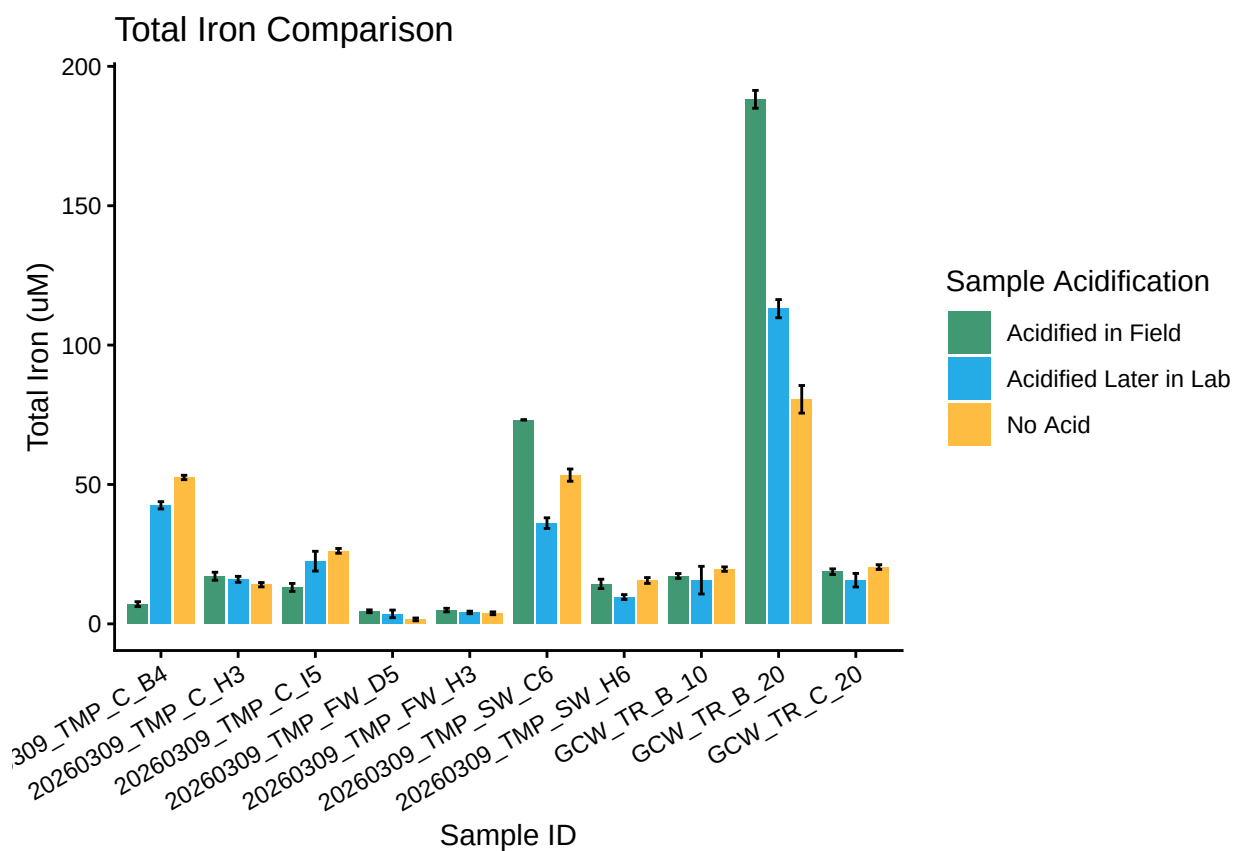

Plotting values against each other

##	Acid_state_1	FE_2_mean	FE_3_mean	FE_tot_mean	new_ID
## 1	Acidified in Field	7.062721	0.000000	7.062721	20260309_TMP_C_B4
## 2	Acidified in Field	17.083274	0.000000	17.083274	20260309_TMP_C_H3
## 3	Acidified in Field	13.075053	0.000000	13.075053	20260309_TMP_C_I5
## 4	Acidified in Field	11.860440	2.476655	14.337095	20260309_TMP_SW_H6
## 5	Acidified in Field	188.165758	0.000000	188.165758	GCW_TR_B_20
## 6	Acidified Later in Lab	28.379170	14.153648	42.532818	20260309_TMP_C_B4

1:1 Comparison of All Fe Measurements

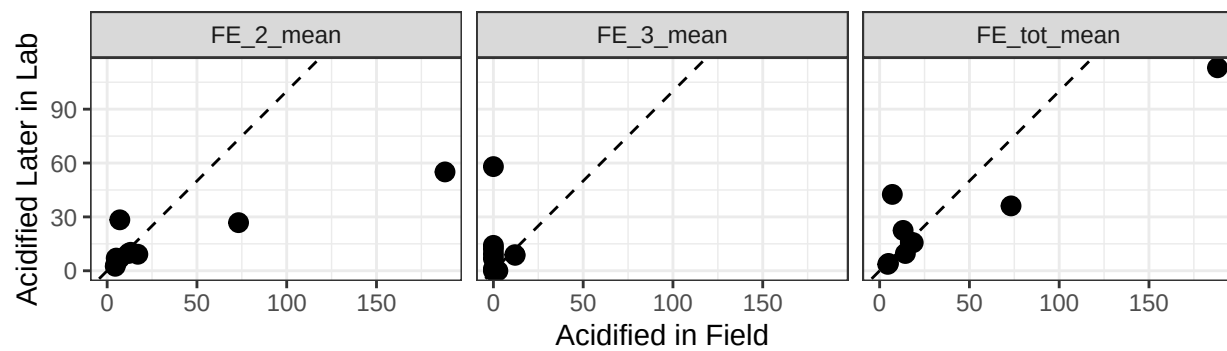

1:1 Comparison of TEMPEST Fe Measurements

