

4

3

2



1

B

B

A



A

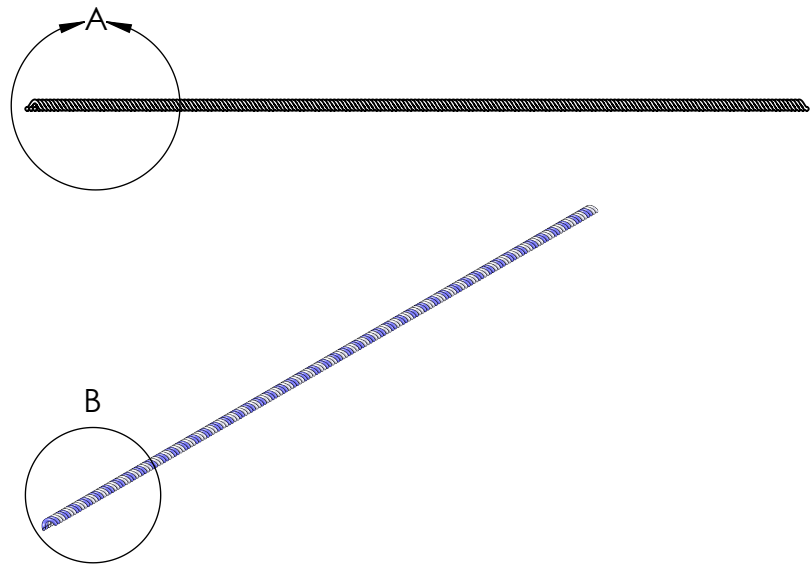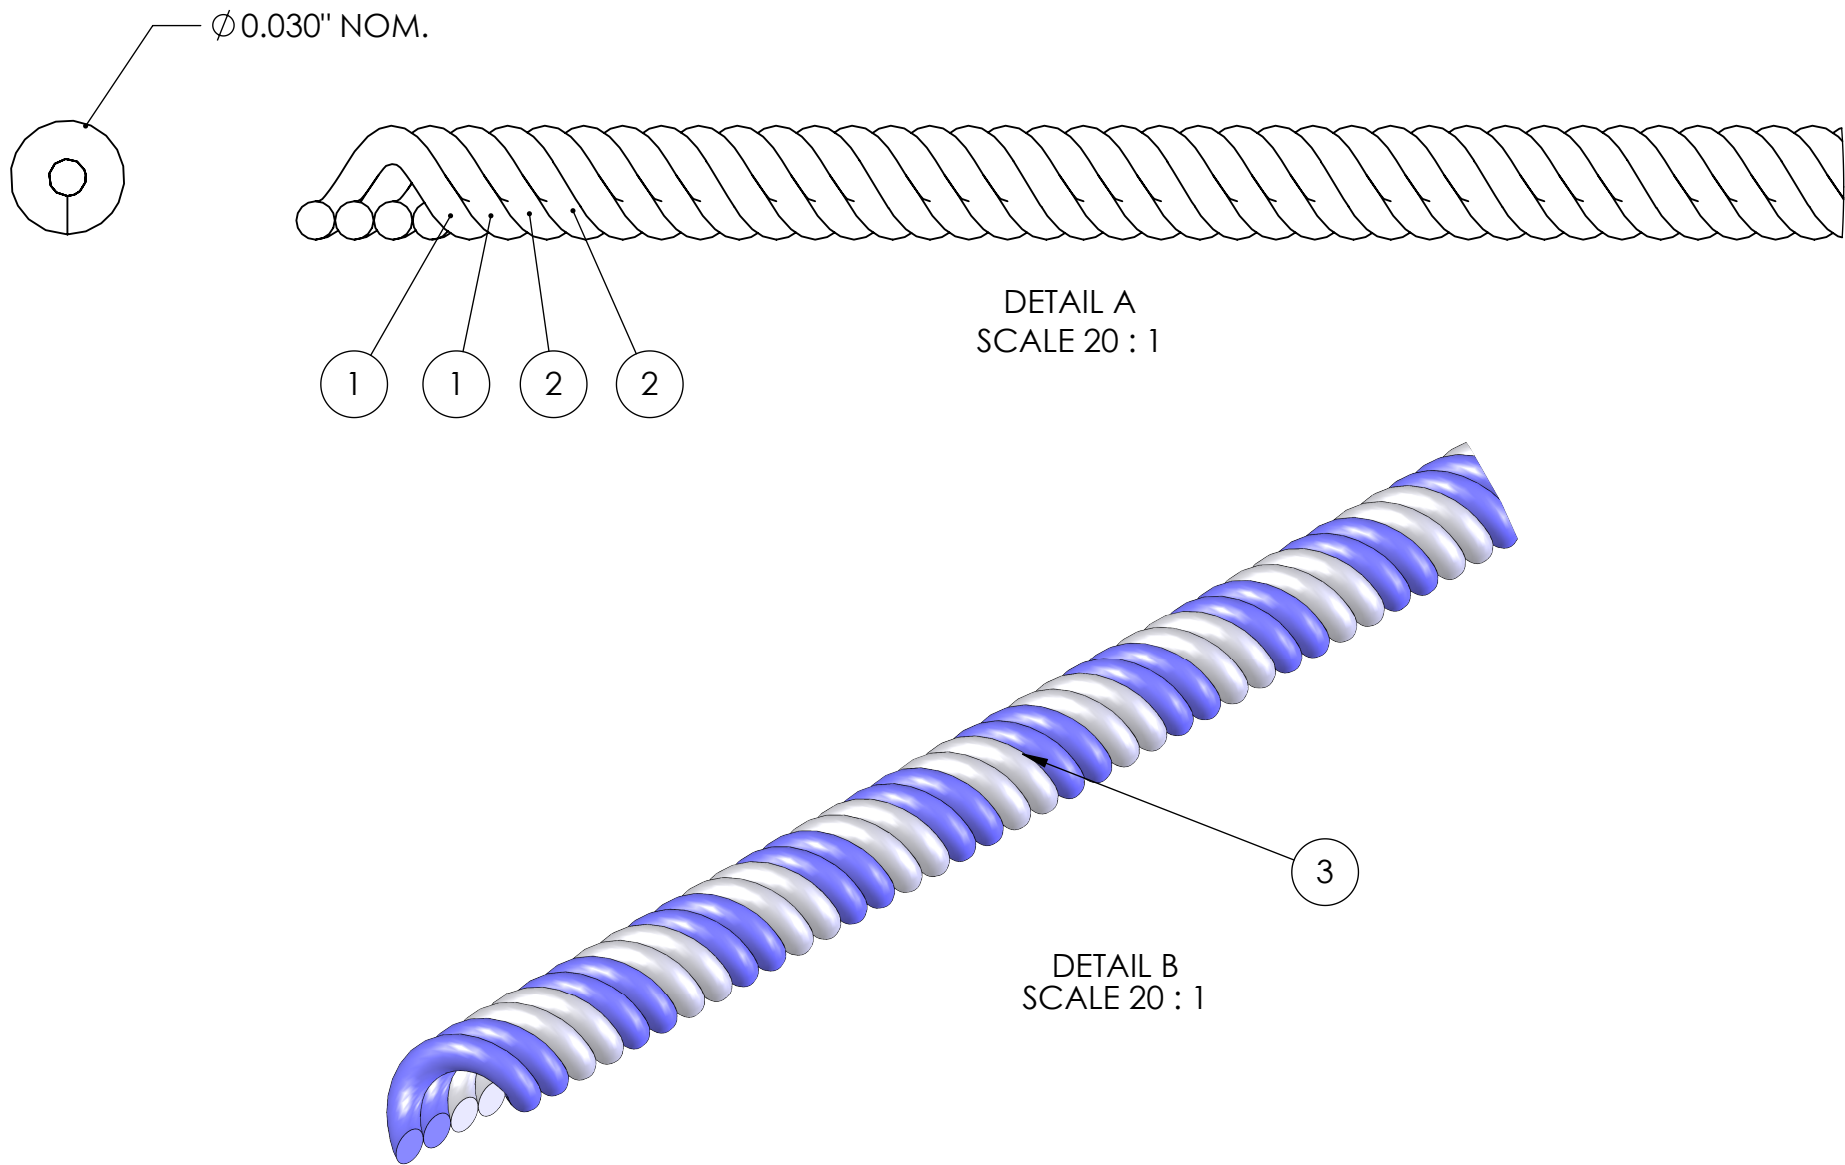

- NOTES:**
- CLOSE WOUND BIFLAR COILED CABLE. TANDEM WOUND.
 - COIL GAPS GREATER THAN 0.002" NOT ALLOWED
 - WOUND LENGTH AS NEEDED
 - WOUND LEADS MUST BE PACKAGED TO PREVENT DAMAGE OR CONTAMINATION DURING HANDLING, STORAGE, AND SHIPMENT

- WINDING PARAMETERS:**
- RIGHT-HAND WIND (Carraige feed - right; Mandrel direction - clockwise (right))
 - 0.010" MANDREL
 - MANDREL TENSION = 1/8" drop with 2.1 oz. (60 grams) center weight
 - Use opposed dual leadwire feed spools
 - Two leadwires per feed spool
 - FEEDER ANGLE = 20° from normal, both front and rear spools
 - FEEDER TENSION (combined for tandem feed)
 - INITIAL 2.1 oz. (60 grams) for first 1/4" - 1/2"
 - FINAL 18.0 oz. (510 grams) for cable body
 - FEED RATE = 37 mils per revolution
 - FEED LENGTH = 1.9 x finished length for each helix wound on mandrel
 - FEED LENGTH = (apporx.) **TBD** x finsihed length after removing from mandrel (coil relaxation)

ITEM NO.	DESCRIPTION
1	PFA coated leadwire - blue
2	PFA coated leadwire - clear
3	4 Filar cable, blu-blu-clr-clr

<div> Open source implantable devices</div>				
THE INFORMATION CONTAINED IN THIS DRAWING IS PUBLICLY RELEASED BY COSMIC UNDER AN OPEN SOURCE LICENSE. COSMIC IS NOT LIABLE FOR ANY ASPECT OF USE OF THIS DRAWING, INCLUDING EDITS, FABRICATION, AND REPRODUCTION OF THIS DESIGN.				
DO NOT SCALE DRAWING		THIRD ANGLE PROJECTION		
INTERPRET DIMENSIONS AND TOLERANCES PER ASME Y14.5M - 2018				
DIMENSIONS IN INCHES UNLESS OTHERWISE SPECIFIED				
MATERIAL	DFT		FINISH	
DOC. NAME				
Filar, DFT, Blue-Clear				
PROJECT	DATE	SIZE	DOC. NUMBER	REV
NNP	6/27/2024	B	NNP-DWG-140-010-000	1.0
SHEET	SCALE			
1 OF 1	2:1			

4

3

2

1