
MgO and NaCl-B2: published EOS and independent refits

Shen and Smith (2026), Table II and Supplemental Table S1

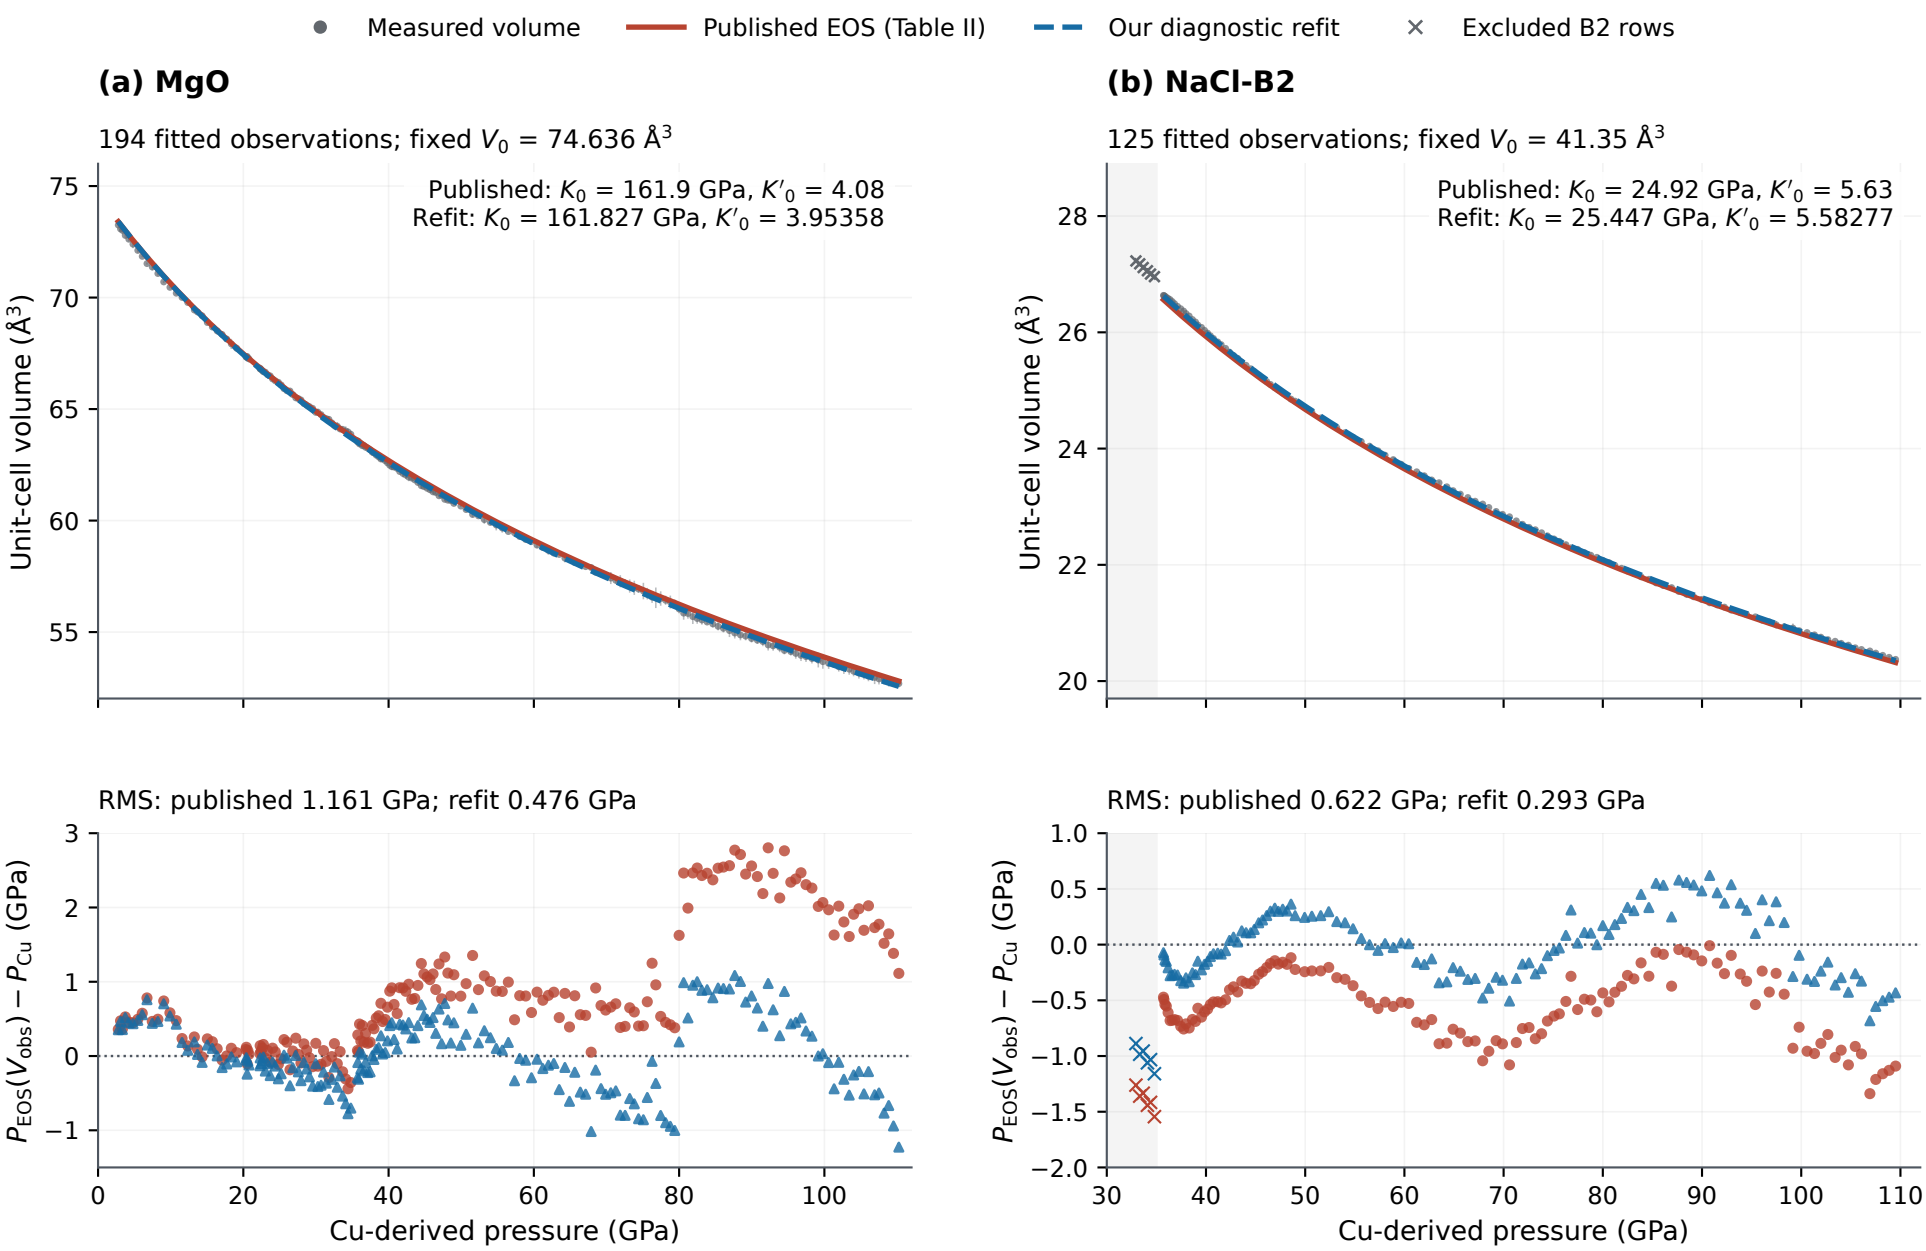

Cu pressure: Fratanduono et al. (2020), 298 K EOS; each volume paired with Cu from the same DAC and run.
Refits: ordinary Vinet, unweighted pressure residuals, fixed published V0. Error bars: reported sample-volume standard errors only.
Cu-derived pressures are held fixed in fitting. Residual RMS uses fitted rows; crosses mark six NaCl-B2 rows at P(Cu) <= 35 GPa.
Fits are shown within the fitted pressure intervals. Diagnostic refits; original author weights and exact fit inputs remain unconfirmed.
Source: Shen and Smith, Phys. Rev. B 113, 144113 (2026), doi:10.1103/fxgq-96sg; Cu: Phys. Rev. Lett. 124, 015701 (2020).