Brucite: continuous expansion refit versus Fukui et al. (2003)

Published Table 4 data
New continuous refit · curved expansion + published slopes
Published isotherms · original expansion + tabulated moduli
Original continuous reconstruction · original expansion + published slopes

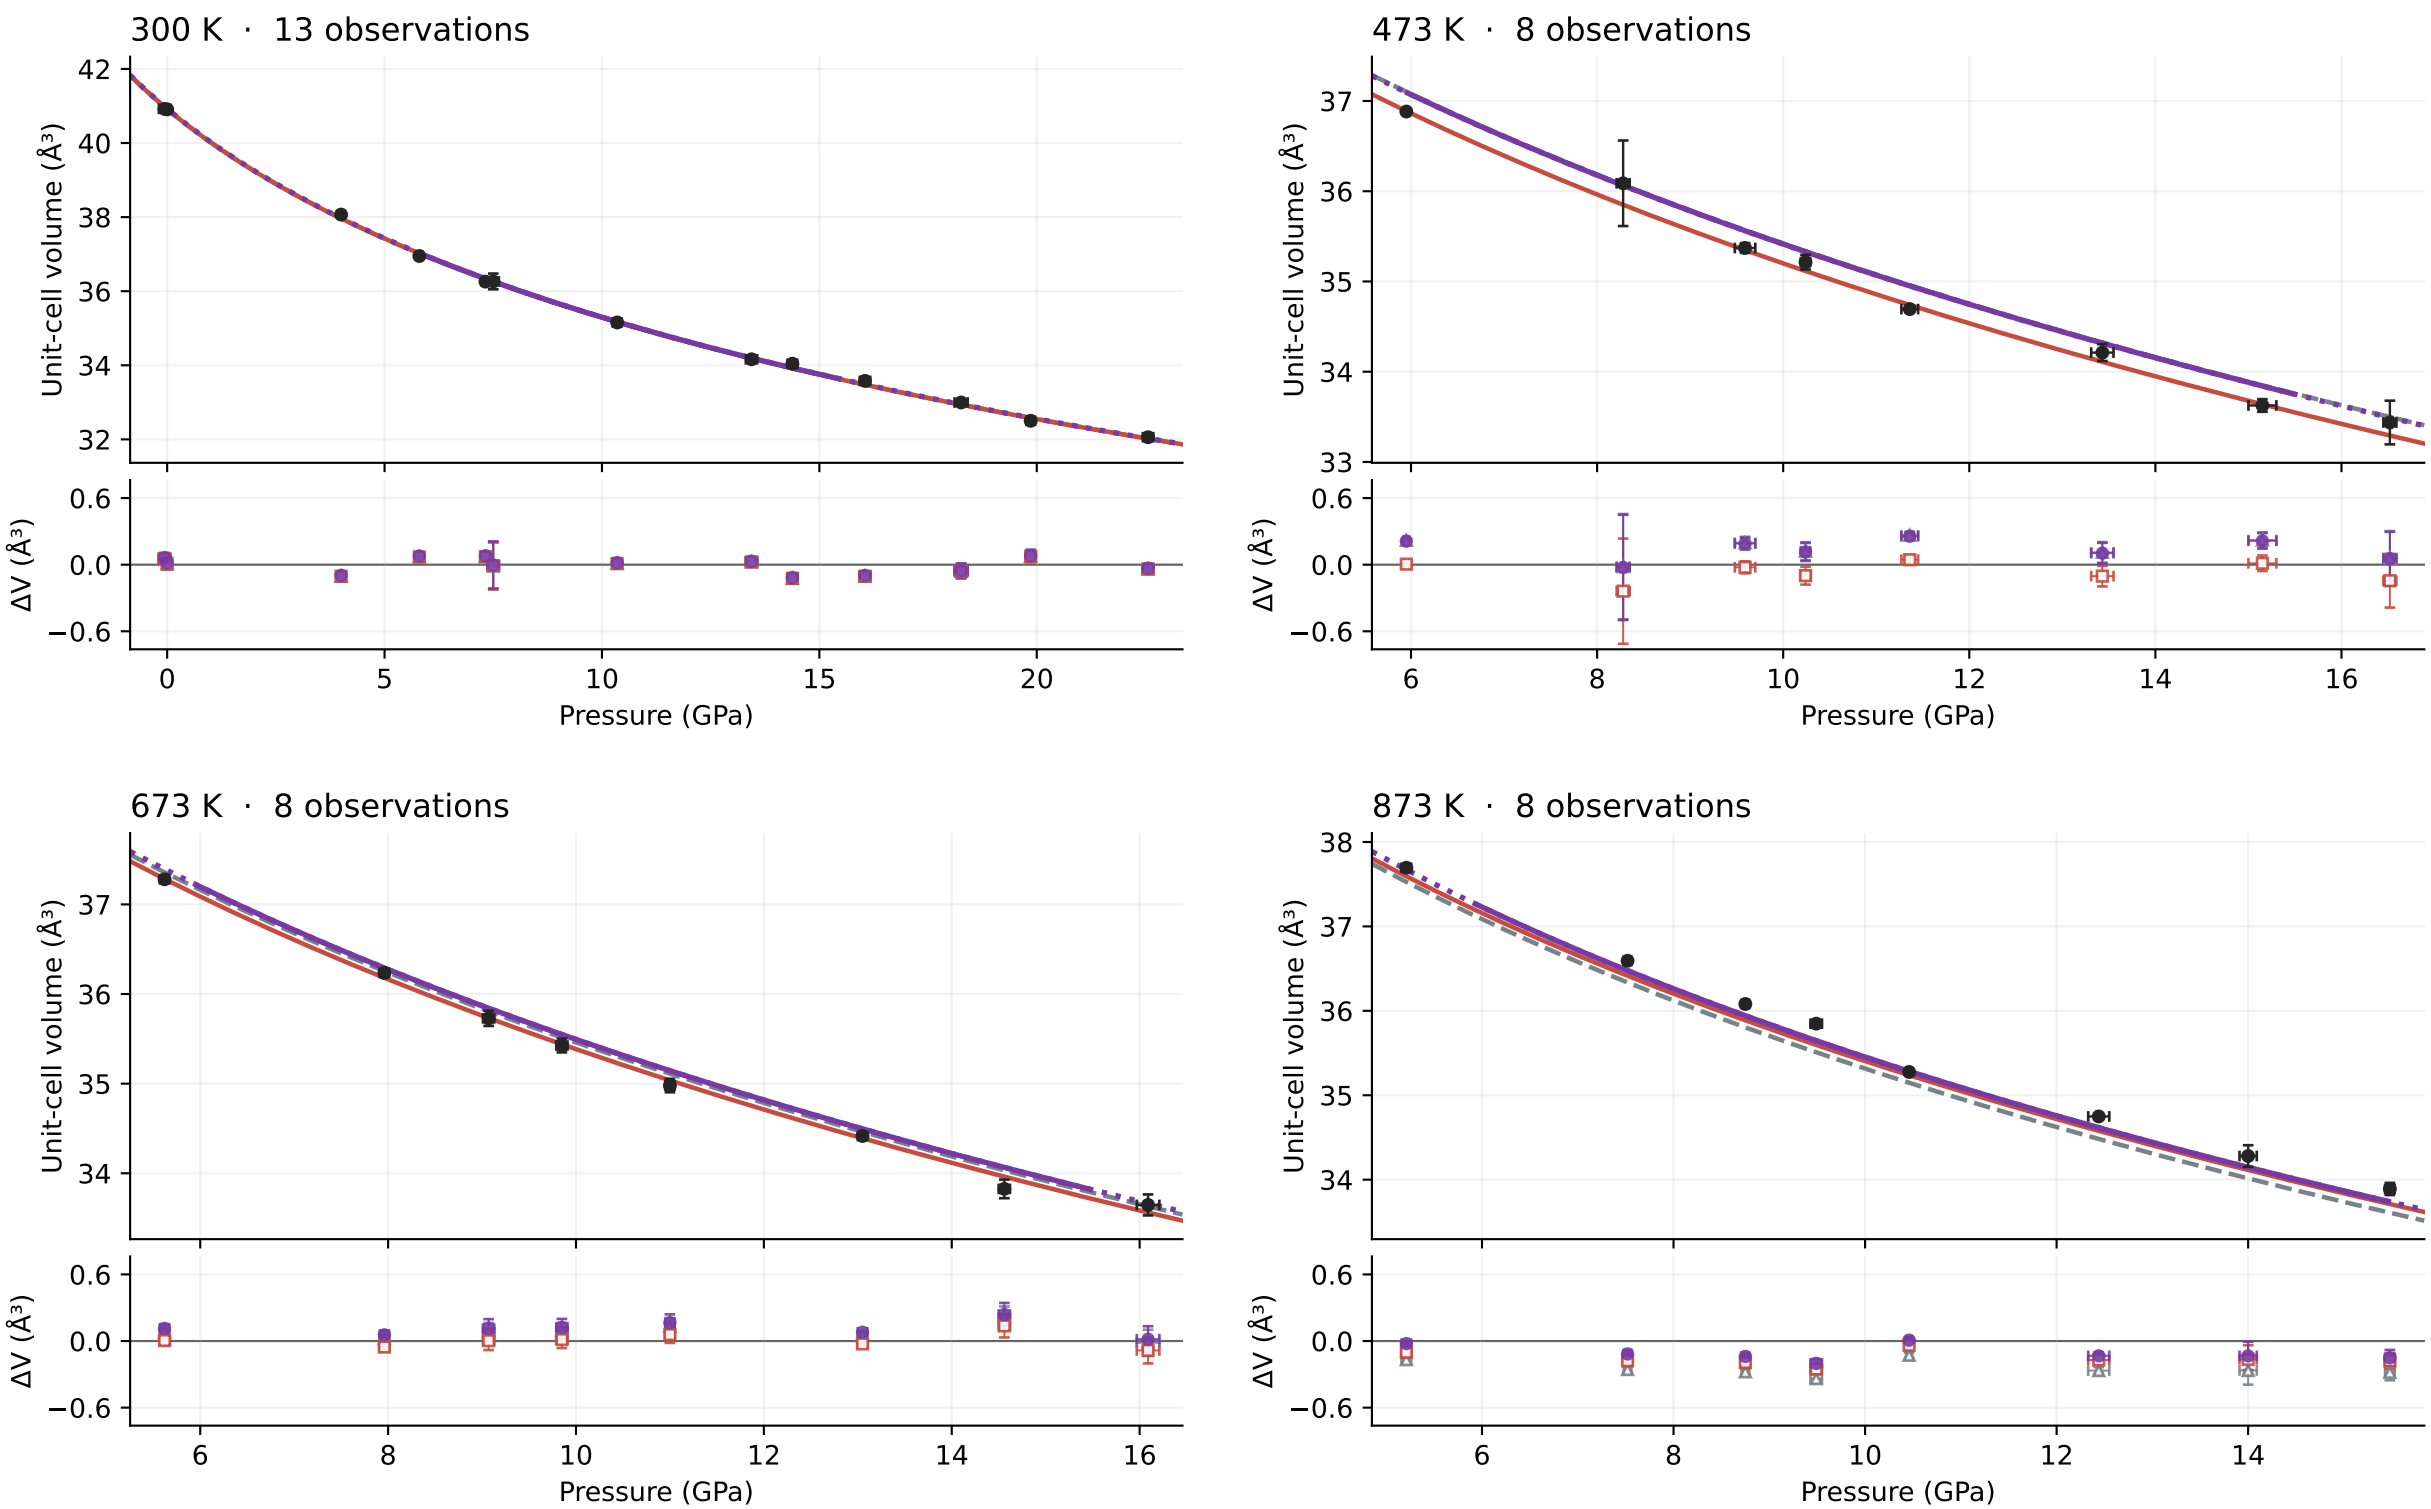

ΔV = calculated − observed volume at observed pressure; bars show reported P and V errors, excluding model uncertainty.
Purple dotted portions lie outside the continuous catalog interval (5.95–15.48 GPa).
Both continuous curves use published slopes anchored at the 300 K moduli; original fitted intercepts were not reported.
Curved expansion was fitted only to ambient data (299.3–592.9 K); higher-temperature reference volumes are extrapolated.