Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE72902186_2022-10-17_14-01-54.xad

Created: 10/17/2022 2:01:53 PM
Modified: 10/17/2022 2:34:43 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/µl] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/µl] : 125
Upper Marker Concentration [pg/µl] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4

Ladder


Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

© Copyright 2003 - 2021 Agilent, Inc.

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE72902186_2022-10-17_14-01-54.xad

Created: 10/17/2022 2:01:53 PM
Modified: 10/17/2022 2:34:43 PM

Electropherogram Summary

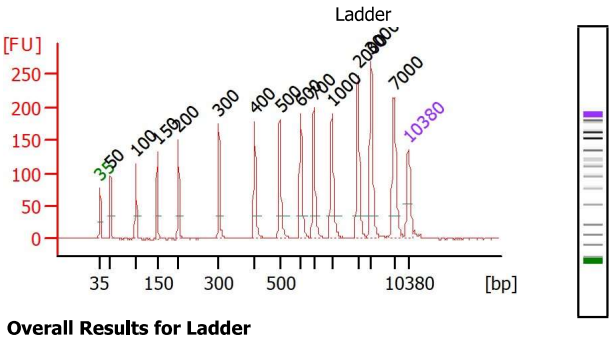


Overall Results for Ladder

Noise: 0.4

Peak table for Ladder

Peak		Size [bp]	Conc. [pg/µl]	Molarity [pmol/l]	Observations
1		35	125.00	5,411.3	Lower Marker
2		50	150.00	4,545.5	Ladder Peak
3		100	150.00	2,272.7	Ladder Peak
4		150	150.00	1,515.2	Ladder Peak
5		200	150.00	1,136.4	Ladder Peak
6		300	150.00	757.6	Ladder Peak
7		400	150.00	568.2	Ladder Peak
8		500	150.00	454.5	Ladder Peak
9		600	150.00	378.8	Ladder Peak
10		700	150.00	324.7	Ladder Peak
11		1,000	150.00	227.3	Ladder Peak
12		2,000	150.00	113.6	Ladder Peak
13		3,000	150.00	75.8	Ladder Peak

Peak		Size [bp]	Conc. [pg/µl]	Molarity [pmol/l]	Observations
14		7,000	150.00	32.5	Ladder Peak
15		10,380	75.00	10.9	Upper Marker

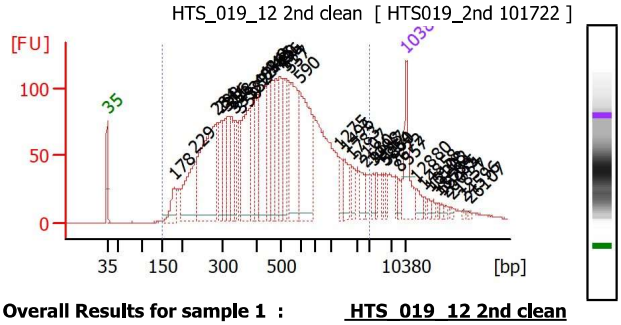

Overall Results for sample 1 : HTS_019_12 2nd clean

Number of peaks found: 41
Noise: 0.4
Corr. Area 1: 4,029.0

Region table for sample 1 : HTS_019_12 2nd clean

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/µl]	Molarity [pmol/l]	Color
150	3,000	4,029.0	92	608	79.4	2,899.76	11,398.4	

© Copyright 2003 - 2021 Agilent, Inc.


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE72902186_2022-10-17_14-01-54.xad

Created: 10/17/2022 2:01:53 PM
Modified: 10/17/2022 2:34:43 PM

Electropherogram Summary Continued ...

Peak table for sample 1 : HTS_019_12 2nd clean

Peak	Size [bp]	Conc. [pg/µl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	178	54.06	459.2	
3	229	162.64	1,074.9	
4	284	369.94	1,971.3	
5	298	76.17	387.7	
6	311	80.24	391.3	
7	316	76.35	365.9	
8	328	56.91	263.2	
9	335	62.25	281.7	
10	350	52.49	227.3	
11	382	187.69	744.6	
12	392	77.00	297.9	
13	403	62.16	233.4	
14	434	149.93	522.9	
15	449	88.63	299.0	
16	465	85.01	276.7	
17	480	76.38	241.1	
18	496	89.30	272.6	
19	514	64.89	191.2	
20	537	186.71	526.8	
21	590	218.33	561.1	
22	1,275	29.38	34.9	
23	1,496	30.89	31.3	
24	1,783	20.29	17.2	
25	2,107	29.26	21.0	
26	2,680	12.67	7.2	
27	3,398	14.24	6.4	
28	4,117	11.72	4.3	
29	5,254	13.26	3.8	
30	5,860	14.87	3.8	
31	7,672	10.61	2.1	
32	8,557	12.40	2.2	
33	10,380	75.00	10.9	Upper Marker
34	12,880	0.00	0.0	
35	14,858	0.00	0.0	
36	16,108	0.00	0.0	
37	17,202	0.00	0.0	
38	18,504	0.00	0.0	
39	19,285	0.00	0.0	
40	20,014	0.00	0.0	
41	21,837	0.00	0.0	
42	24,596	0.00	0.0	
43	26,107	0.00	0.0	

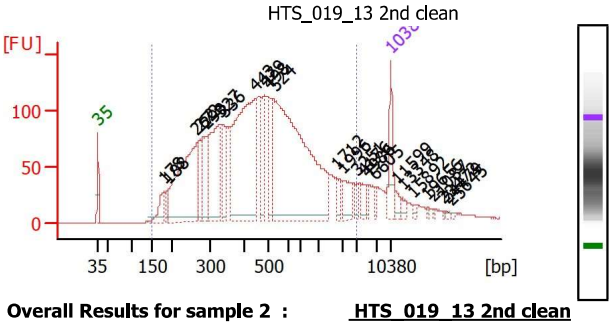

Overall Results for sample 2 : HTS_019_13 2nd clean

Number of peaks found:	25
Noise:	0.4
Corr. Area 1:	4,260.7

Region table for sample 2 : HTS_019_13 2nd clean

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/µl]	Molarity [pmol/l]	Color
150	3,000	4,260.7	92	583	80.2	3,611.62	14,680.7	

Peak table for sample 2 : HTS_019_13 2nd clean

Peak	Size [bp]	Conc. [pg/µl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	178	88.74	756.8	
3	188	32.32	261.1	
4	262	529.23	3,059.6	
5	272	94.48	525.5	
6	290	162.12	847.5	
7	327	315.77	1,462.0	
8	336	68.78	309.7	
9	443	639.03	2,183.5	
10	479	106.65	337.1	
11	498	125.86	383.1	
12	524	953.90	2,760.8	
13	1,712	21.11	18.7	
14	1,996	47.42	36.0	
15	3,251	14.18	6.6	
16	4,176	20.44	7.4	
17	4,986	11.83	3.6	
18	6,605	12.68	2.9	
19	10,380	75.00	10.9	Upper Marker
20	11,599	0.00	0.0	
21	13,348	0.00	0.0	
22	15,892	0.00	0.0	
23	19,656	0.00	0.0	
24	21,087	0.00	0.0	


© Copyright 2003 - 2021 Agilent, Inc.

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE72902186_2022-10-17_14-01-54.xad

Created: 10/17/2022 2:01:53 PM
Modified: 10/17/2022 2:34:43 PM

Electropherogram Summary Continued ...

Peak	Size [bp]	Conc. [pg/µl]	Molarity [pmol/l]	Observations
25	23,472	0.00	0.0	
26	24,479	0.00	0.0	
27	25,645	0.00	0.0	

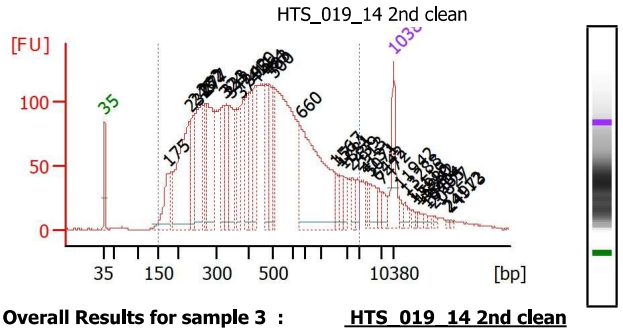

Overall Results for sample 3 : HTS_019_14 2nd clean

Number of peaks found:	36
Noise:	0.5
Corr. Area 1:	4,875.8

Region table for sample 3 : HTS_019_14 2nd clean

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/µl]	Molarity [pmol/l]	Color
150	3,000	4,875.8	92	565	84.5	3,869.89	16,831.8	

Peak table for sample 3 : HTS_019_14 2nd clean


Peak	Size [bp]	Conc. [pg/µl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	175	130.31	1,128.4	
3	232	409.05	2,672.9	
4	243	133.66	833.6	
5	262	261.09	1,508.2	
6	272	85.19	475.1	
7	277	221.69	1,211.6	
8	324	119.12	557.7	
9	333	95.57	434.9	
10	342	151.37	671.2	
11	374	85.87	347.7	
12	395	104.82	402.3	
13	411	100.85	371.6	
14	420	97.75	352.5	
15	464	96.38	314.9	
16	483	99.59	312.2	
17	500	71.44	216.4	
18	660	405.17	929.9	
19	1,567	19.53	18.9	
20	1,711	23.42	20.7	
21	1,881	20.98	16.9	
22	2,439	24.73	15.4	
23	2,913	17.89	9.3	
24	4,131	13.96	5.1	
25	5,071	30.21	9.0	
26	6,442	19.06	4.5	
27	7,472	21.80	4.4	
28	10,380	75.00	10.9	Upper Marker
29	11,942	0.00	0.0	
30	13,288	0.00	0.0	
31	15,119	0.00	0.0	
32	15,980	0.00	0.0	
33	16,842	0.00	0.0	
34	18,404	0.00	0.0	
35	19,265	0.00	0.0	
36	20,827	0.00	0.0	
37	24,112	0.00	0.0	
38	24,973	0.00	0.0	

© Copyright 2003 - 2021 Agilent, Inc.

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE72902186_2022-10-17_14-01-54.xad

Created: 10/17/2022 2:01:53 PM
Modified: 10/17/2022 2:34:43 PM

Electropherogram Summary Continued ...

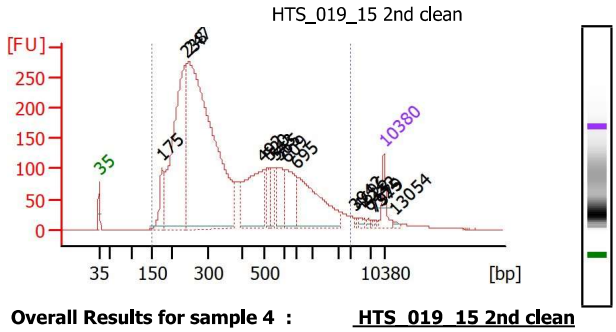

Overall Results for sample 4 : HTS_019_15 2nd clean


Number of peaks found:	15
Noise:	0.5
Corr. Area 1:	7,220.5

Region table for sample 4 : HTS_019_15 2nd clean

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/µl]	Molarity [pmol/l]	Color
150	3,000	7,220.5	97	461	85.0	6,916.91	35,017.5	

Peak table for sample 4 : HTS_019_15 2nd clean

Peak	Size [bp]	Conc. [pg/µl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	175	258.88	2,242.1	
3	238	1,630.88	10,372.9	
4	247	3,315.14	20,320.4	
5	492	532.05	1,639.8	
6	520	107.91	314.3	
7	543	105.50	294.4	
8	565	187.90	504.3	
9	609	217.52	541.2	
10	695	549.26	1,197.7	
11	3,942	7.35	2.8	
12	4,696	13.27	4.3	
13	6,442	8.60	2.0	
14	7,325	4.83	1.0	
15	7,979	5.83	1.1	
16	10,380	75.00	10.9	Upper Marker
17	13,054	0.00	0.0	

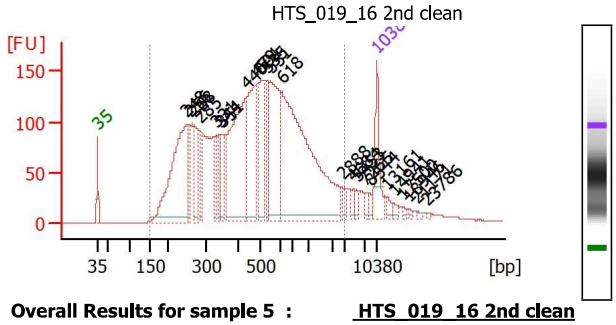

Overall Results for sample 5 : HTS_019_16 2nd clean

Number of peaks found:	24
Noise:	0.4
Corr. Area 1:	5,204.5

Region table for sample 5 : HTS_019_16 2nd clean

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/µl]	Molarity [pmol/l]	Color
150	3,000	5,204.5	93	593	76.4	3,312.72	13,163.2	

Peak table for sample 5 : HTS_019_16 2nd clean

Peak	Size [bp]	Conc. [pg/µl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	248	514.09	3,142.3	
3	256	79.14	468.6	
4	268	143.97	814.3	
5	285	63.36	336.8	
6	331	58.35	266.7	
7	344	69.47	305.7	
8	351	60.18	259.9	
9	440	427.66	1,472.2	
10	479	231.78	733.6	
11	501	112.84	341.3	
12	535	71.53	202.5	
13	551	264.27	727.3	
14	618	700.75	1,718.6	
15	2,888	16.24	8.5	
16	4,684	10.92	3.5	
17	5,453	8.78	2.4	
18	7,265	12.67	2.6	
19	8,544	8.37	1.5	
20	10,380	75.00	10.9	Upper Marker
21	13,161	0.00	0.0	
22	14,941	0.00	0.0	
23	17,500	0.00	0.0	
24	18,946	0.00	0.0	


© Copyright 2003 - 2021 Agilent, Inc.

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE72902186_2022-10-17_14-01-54.xad

Created: 10/17/2022 2:01:53 PM
Modified: 10/17/2022 2:34:43 PM

Electropherogram Summary Continued ...

Peak	Size [bp]	Conc. [pg/µl]	Molarity [pmol/l]	Observations
25	21,171	0.00	0.0	
26	23,786	0.00	0.0	

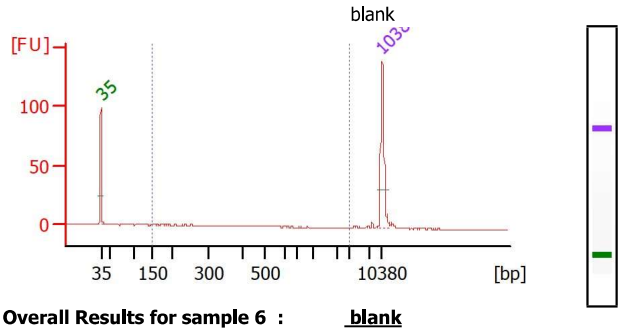

Overall Results for sample 6 : blank

Number of peaks found:	0
Noise:	0.3
Corr. Area 1:	8.4

Region table for sample 6 : blank

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/µl]	Molarity [pmol/l]	Color
150	3,000	8.4	39	418	100.0	8.34	48.2	

Peak table for sample 6 : blank


Peak	Size [bp]	Conc. [pg/µl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	10,380	75.00	10.9	Upper Marker

© Copyright 2003 - 2021 Agilent, Inc.

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE72902186_2022-10-17_14-01-54.xad

Created: 10/17/2022 2:01:53 PM
Modified: 10/17/2022 2:34:43 PM

Gel Image

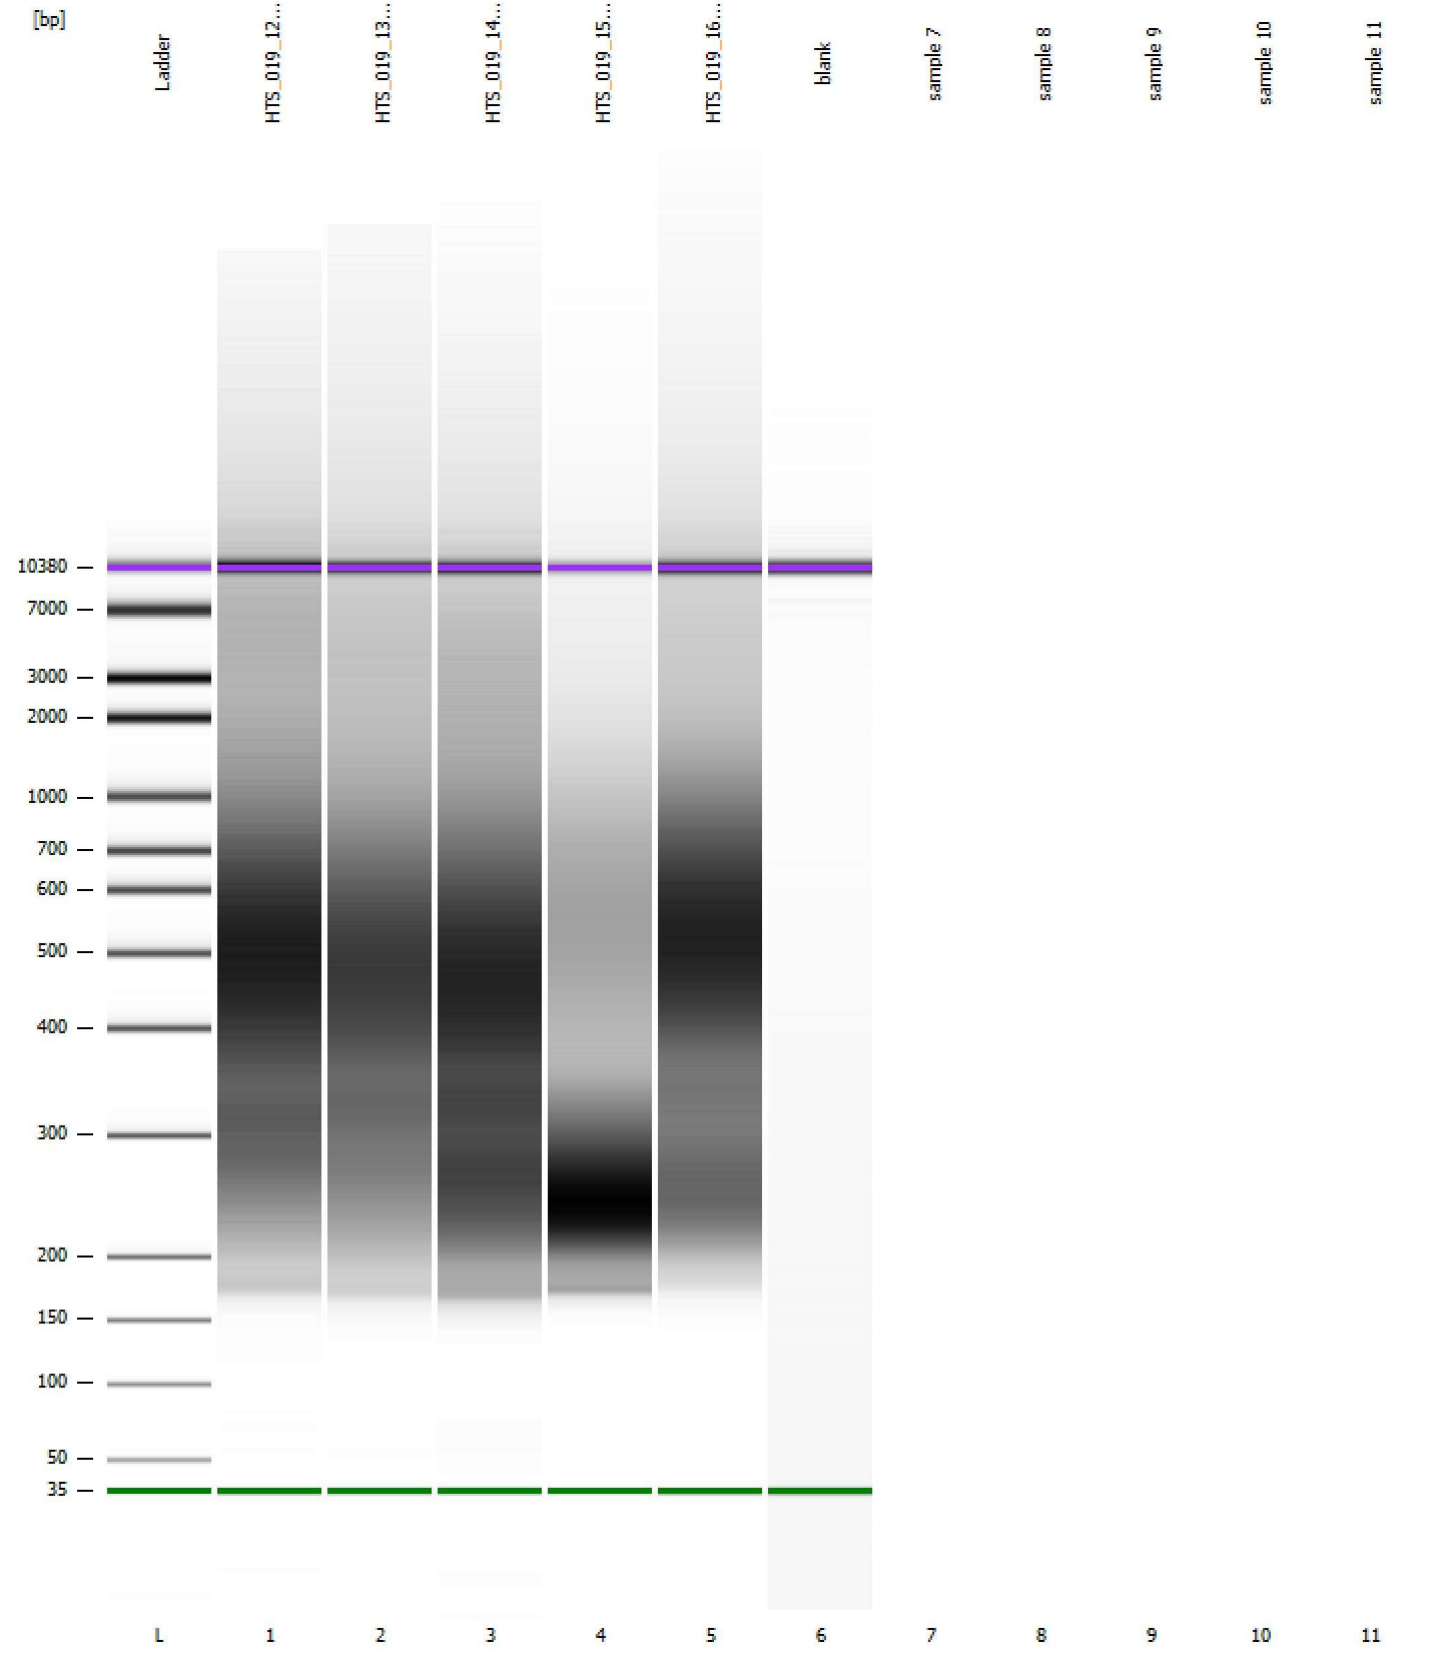

© Copyright 2003 - 2021 Agilent, Inc.

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE72902186_2022-10-17_14-01-54.xad

Created: 10/17/2022 2:01:53 PM
Modified: 10/17/2022 2:34:43 PM

Invalid Samples

Sample 7 has not been run, no results available.

Sample 8 has not been run, no results available.

Sample 9 has not been run, no results available.

Sample 10 has not been run, no results available.

Sample 11 has not been run, no results available.

© Copyright 2003 - 2021 Agilent, Inc.