

PRODUCT:

N2494A-201
PSRF Center Plate for Segmented Bridge Adapter

 N2494A
PSRF Segmented Bridge Adapter Kit

N2494A-208
PSRF Delta/Multitest/Tesec Stiffener Inlay
for Bridge Adapter

E6980DA
Stiffener Small

E6980EA
Stiffener Large

Customized DUT Board
(small or large)

PORT SCALE RF DUT BOARD SETUP FOR SEGMENTED BRIDGE ADAPTER FOR
DELTA/MULTITEST HANDLER
PRODUCT OVERVIEW AND ASSEMBLY INSTRUCTION

STEP 6
IF ITEM 13 IS USED INSTALL IT WITH
ITEM 14 ON ITEM 1

STEP 3
AFTER STEP 2
TIGHTEN BACK SCREWS M3 (2x)

STEP 1
PUT ITEM 1 ON ITEM 3.
NOTE:
ORIENTATION ON INDICATORS
MUST FACE IN THE
SAME DIRECTION.

STEP 2
TIGHTEN FRONT SCREWS M3 (2x) FIRST

STEP 7
INSTALL ITEM 15 WITH ITEM 16 ON STIFFENER ITEM 11

INSTALL ITEM 5, 6 WITH ITEM 7 FOR DELTA CASTLE HANDLER.
ITEM 5, 6 AND 7 IS PART OF THE PRODUCT N2494A-208

STEP 4
PLACE ASSEMBLY (ITEM 1 AND ITEM 3) ON ITEM
AND SCREW IT WITH ITEM 4.
NOTE: ORIENTATION ON INDICATORS MUST FACE
IN THE SAME DIRECTION.

INSTALL ITEM 8, 9 WITH ITEM 10 FOR DELTA FLEX HANDLER.
ITEM 8, 9 AND 10 IS PART OF THE PRODUCT N2494A-208

STEP 5
INSTALL ITEM 12 TO ITEM 11

7		8	
FILE NAME N2494-90112-151D.cml		ISSUED DATE 2011-08-04	ISSUED NUMBER N2494-90112-1
DATE	DESCRIPTION	ISSUED BY	DATE
A	AS ISSUED	Peter Hirschmann	2010-02-10
B	SHEET 3 AND 4 ADDED	Peter Hirschmann	2010-07-19
C	PRODUCT N2494A CHANGED	Peter Hirschmann	2011-03-30
D	NAMING ON SHEET 3 AND 4 CORRECTED	Peter Hirschmann	2011-08-04

PRODUCTS:

N2494-262 EXTRACTION TOOL FOR MULTIPOINT RF CABLE

N2393-83805 SMP SCREW DRIVER

N2494A-260 PSRF MULTI-PORT MINI-COAX CONNECTOR (MPMCC),
6 CHANNELS, SINGLE ITEM

N2494A-261 PSRF HOUSING FOR CHANNEL CABLES, MPMC,
6 CHANNELS, SINGLE ITEM

N2494A-601 PSRF DUT CABLE SET FOR MPMCC,
STRAIGHT, LENGTH 150mm, 6 CH, SINGLE ITEM

N2494A-602 PSRF DUT CABLE SET FOR MPMCC,
STRAIGHT, LENGTH 200mm, 6 CH, SINGLE ITEM

N2494A-101 PSRF DUT CABLE FOR MPMCC,
STRAIGHT, 150mm LENGTH, MALE, SINGLE ITEM

N2494A-102 PSRF DUT CABLE FOR MPMCC,
STRAIGHT, 200mm LENGTH, MALE, SINGLE ITEM

N2494A-001 PSRF DUT CABLE FOR MPMCC,
STRAIGHT, 150mm LENGTH, FEMALE, SINGLE ITEM

N2494A-002 PSRF DUT CABLE FOR MPMCC,
STRAIGHT, 200mm LENGTH, FEMALE, SINGLE ITEM

N2494A-691 PSRF DUT CABLE SET FOR MPMCC,
90 DEGREE, LENGTH 150mm, 6 CH, SINGLE ITEM

N2494A-692 PSRF DUT CABLE SET FOR MPMCC,
90 DEGREE, LENGTH 200mm, 6 CH, SINGLE ITEM

N2494A-191 PSRF DUT CABLE FOR MPMCC,
90 DEGREE, 150mm LENGTH, MALE, SINGLE ITEM

N2494A-192 PSRF DUT CABLE FOR MPMCC,
90 DEGREE, 200mm LENGTH, MALE, SINGLE ITEM.

N2494A-091 PSRF DUT CABLE FOR MPMCC,
90 DEGREE, 150mm LENGTH, FEMALE, SINGLE ITEM

N2494A-092 PSRF DUT CABLE FOR MPMCC,
90 DEGREE, 200mm LENGTH, FEMALE, SINGLE ITEM

TESTER SCALE THIS METRIC 1000 100 10 1 0.1 0.01 0.001		Peter Hirschmann 2010-02-10 Peter Hirschmann 2010-02-10 PSRF SEGMENTED BRIDGE ADAPTER DUT BOARD SETUP FOR DELTA/MULTITEST	
TESTER SCALE THIS METRIC 1000 100 10 1 0.1 0.01 0.001		PSRF SEGMENTED BRIDGE ADAPTER DUT BOARD SETUP FOR DELTA/MULTITEST	



- 

THESE AREAS CONTACT THE STIFFENER INLAY
ON BOTTOM SIDE OF PCB
SIGNAL, GND TRACES, VIAS AND PADS ARE NOT ALLOWED



THESE AREAS ARE AT A CLEARANCE HEIGHT OF 3.5mm TO THE STIFFENER INLAY
ON BOTTOM SIDE OF PCB
SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED
RECOMMENDED MAX. COMPONENT HEIGHT = 2.5mm



THESE AREAS ARE AT A CLEARANCE HEIGHT OF 5mm TO THE STIFFENER INLAY
ON BOTTOM SIDE OF PCB
SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED
RECOMMENDED MAX. COMPONENT HEIGHT = 4mm



THESE AREAS ARE AT A CLEARANCE HEIGHT OF 9.5mm TO THE STIFFENER INLAY
ON BOTTOM SIDE OF PCB
SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED
RECOMMENDED MAX. COMPONENT HEIGHT = 8.5mm



THIS AREA HAS A CLEARANCE HEIGHT OF 34.8mm TO THE CONNECTOR PLATE
ON BOTTOM SIDE OF PCB, WITHOUT TAKING CARE OF RF CABLES AND BENDING RADIUS.
SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED
RECOMMENDED MAX. COMPONENT HEIGHT = 20.0mm



COMPONENT PLACEMENT AREA ON BOTTOM SIDE OF PCB
TRACES, VIAS AND PADS ARE ALLOWED
RECOMMENDED MAX. COMPONENT HEIGHT = 20.0mm



THESE AREAS ARE AT A CLEARANCE HEIGHT OF 8mm TO THE STIFFENER INLAY
ON BOTTOM SIDE OF PCB
SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED
RECOMMENDED MAX. COMPONENT HEIGHT = 7mm




THESE AREAS ARE AT A CLEARANCE HEIGHT OF 21mm TO THE STIFFENER INLAY
ON BOTTOM SIDE OF PCB
SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED
RECOMMENDED MAX. COMPONENT HEIGHT = 20mm

NOTES:

1. USE KEEP-OUT AREA DEFINITION IN CONJUNCTION WITH GENERAL DUT BOARD DEFINITION.
SEE D-E6980-96540-1 SMALL DUT BOARD AND D-E6980-96550-1 LARGE DUT BOARD
2. ALL KEEP-OUT AREAS RELATE TO THE BOTTOM SIDE OF THE PCB

NO TEST SCHEMATIC METRIC	ONLY AVAILABLE FOR RND 100 & RND 2000	Peter Hirschmann 2010-02-10 2010-02-10	PSRF SEGMENTED BRIDGE ADAPTER KEEP OUT AREA DELTA/MULTITEST	VERIGY N2494-90112-1
		• SEGMENTED AREA IN HIGHLIGHTED • THIRD ANGLE PROJECTION • ADDITIONAL TO RND 1-2000-000 • CATEGORY 2000-000-000-000	TYPE 2 4 UNIT SEGMENTED 1:1 SCALE VIEW A1	

Port Scale RF DUT Board setup for Segmented Bridge Adapter for Delta/Multitest handler
Keep-out area definition for DUT Board design, using Purge Kit N2367A in DUT IF

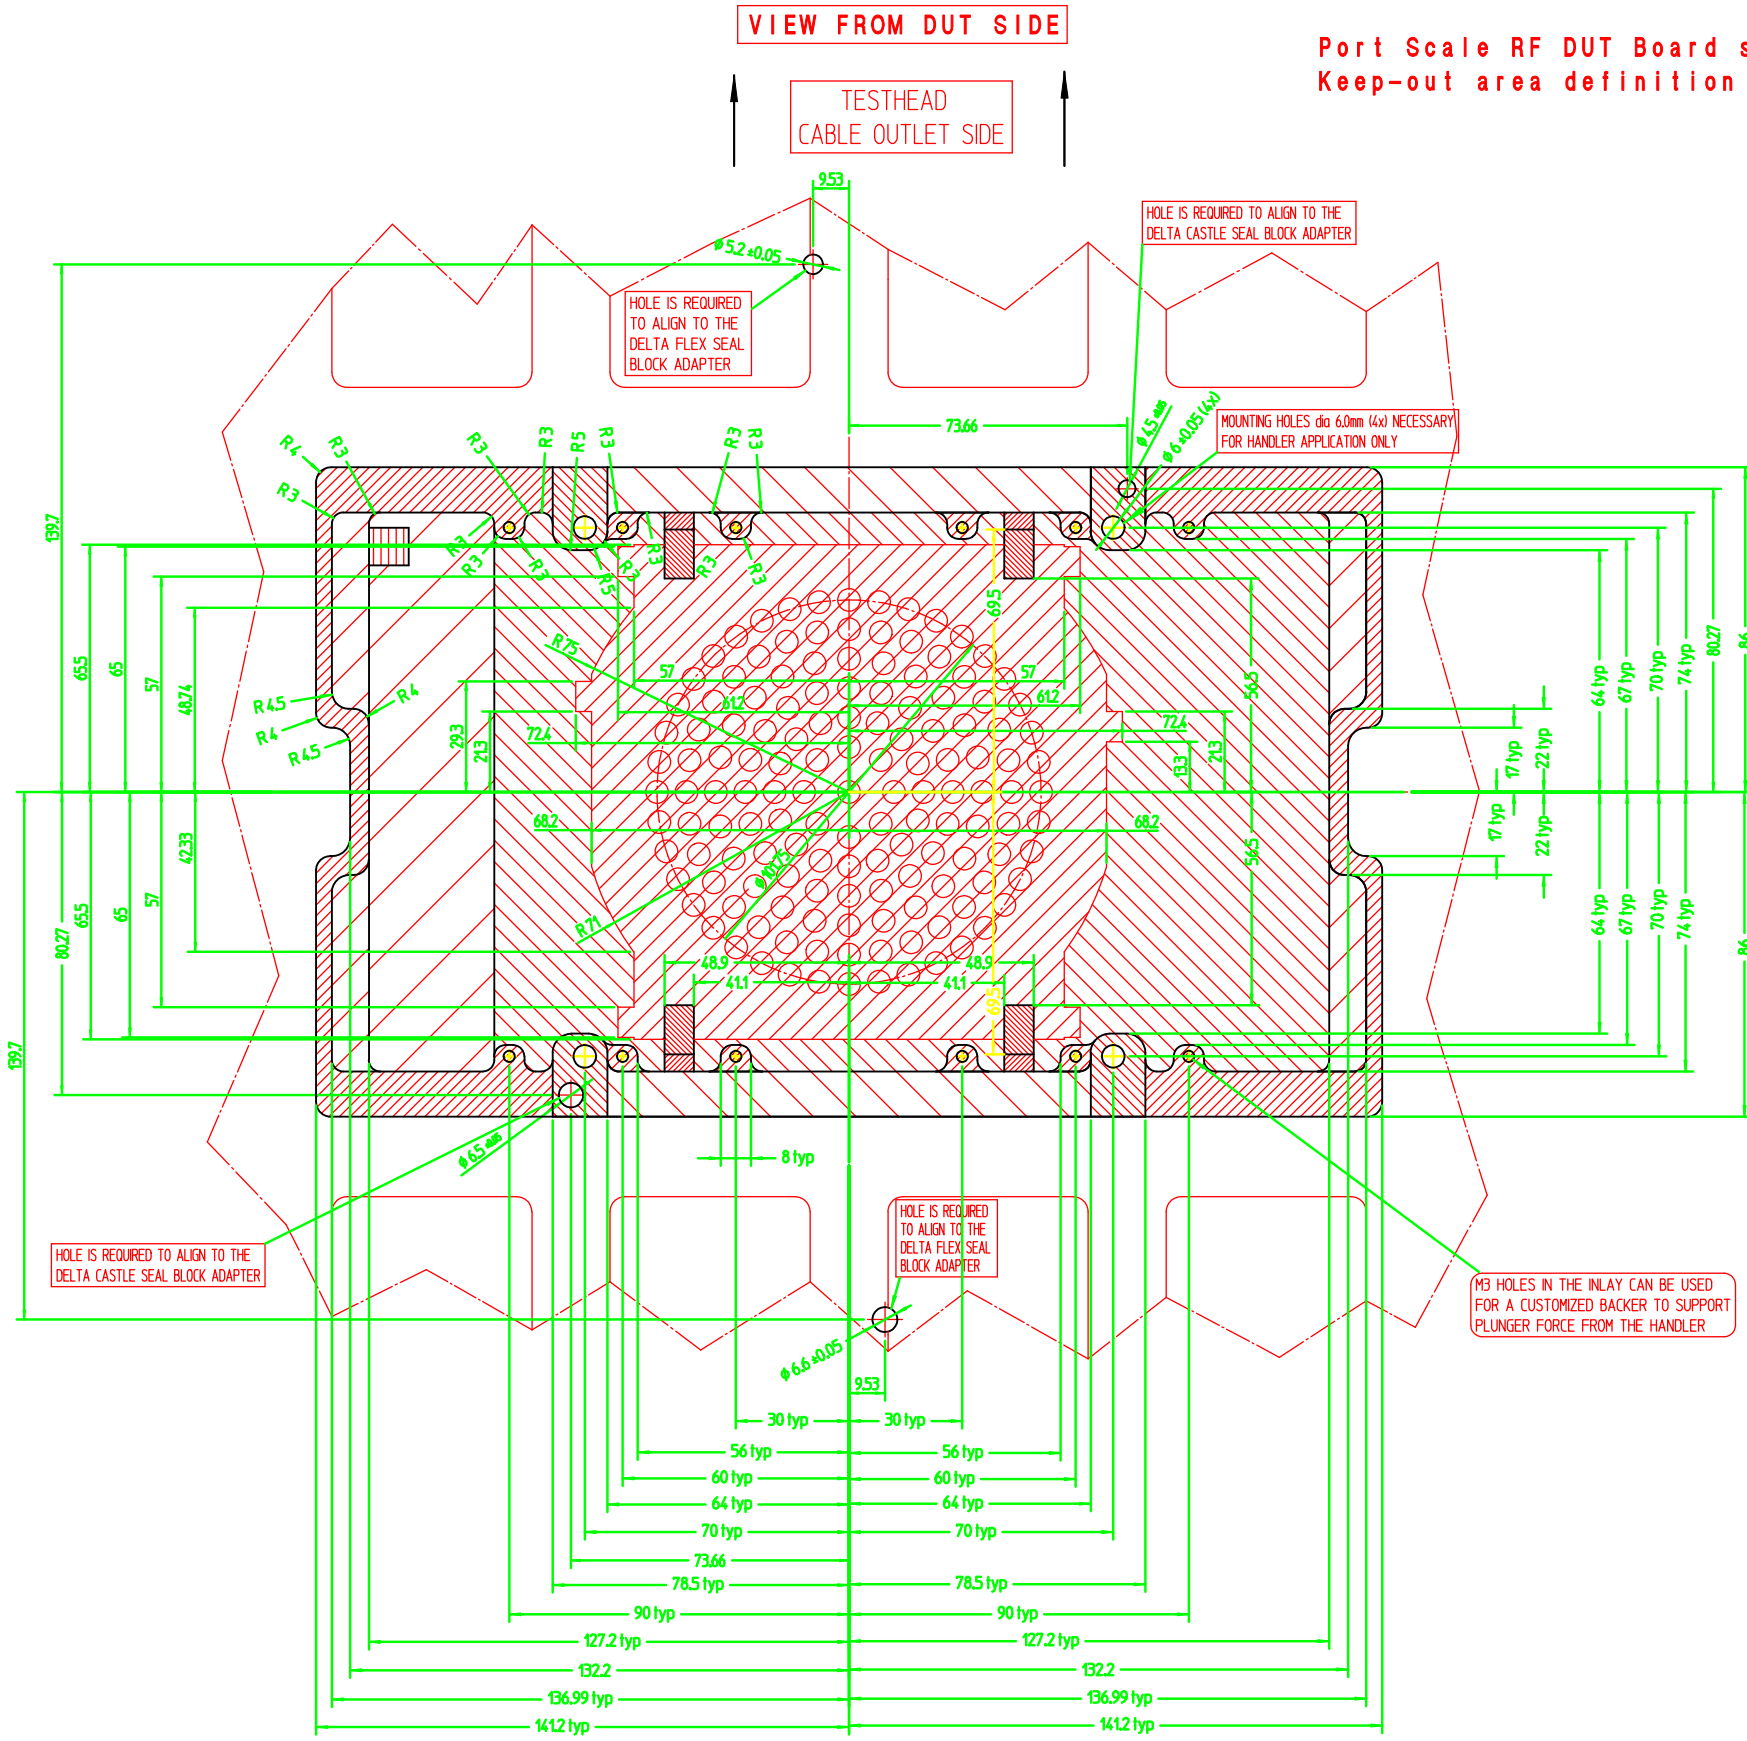


- THESE AREAS CONTACT THE STIFFENER INLAY ON BOTTOM SIDE OF PCB. SIGNAL, GND TRACES, VIAS AND PADS ARE NOT ALLOWED
- THESE AREAS ARE AT A CLEARANCE HEIGHT OF 3.5mm TO THE STIFFENER INLAY ON BOTTOM SIDE OF PCB. SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 2.5mm
- THESE AREAS ARE AT A CLEARANCE HEIGHT OF 5mm TO THE STIFFENER INLAY ON BOTTOM SIDE OF PCB. SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 4mm
- THESE AREAS ARE AT A CLEARANCE HEIGHT OF 9.5mm TO THE STIFFENER INLAY ON BOTTOM SIDE OF PCB. SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 8.5mm
- THIS AREA HAS A CLEARANCE HEIGHT OF 34.8mm TO THE CONNECTOR PLATE ON BOTTOM SIDE OF PCB, WITHOUT TAKING CARE OF RF CABLES AND BENDING RADIUS. SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 20.0mm
- THESE AREAS ARE AT A CLEARANCE HEIGHT OF 22.5mm TO THE PURGE KIT N2367A ON BOTTOM SIDE OF PCB. COMPONENT PLACEMENT AREA ON BOTTOM SIDE OF PCB. TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 20.0mm
- THESE AREAS ARE AT A CLEARANCE HEIGHT OF 8mm TO THE STIFFENER INLAY ON BOTTOM SIDE OF PCB. SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 7mm
- THESE AREAS ARE AT A CLEARANCE HEIGHT OF 21.0mm TO THE STIFFENER INLAY ON BOTTOM SIDE OF PCB. SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 20.0mm
- THIS AREA IS AT A CLEARANCE HEIGHT OF 27.0mm TO THE PURGE KIT N2367A ON BOTTOM SIDE OF PCB. COMPONENT PLACEMENT AREA ON BOTTOM SIDE OF PCB. TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 20.0mm
- THIS AREA IS AT A CLEARANCE HEIGHT OF 12.0mm TO THE PURGE KIT N2367A ON BOTTOM SIDE OF PCB. COMPONENT PLACEMENT AREA ON BOTTOM SIDE OF PCB. TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 11.0mm

NOTES:
1. USE KEEP-OUT AREA DEFINITION IN CONJUNCTION WITH GENERAL DUT BOARD DEFINITION. SEE D-E6980-96540-1 SMALL DUT BOARD AND D-E6980-96550-1 LARGE DUT BOARD
2. ALL KEEP-OUT AREAS RELATE TO THE BOTTOM SIDE OF THE PCB

VIEW FROM DUT SIDE

TESTHEAD
CABLE OUTLET SIDE

Port Scale RF DUT Board setup for Segmented Bridge Adapter for Delta/Multitest handler
Keep-out area definition for DUT Board design, using Purge Kit N2467A in DUT IF

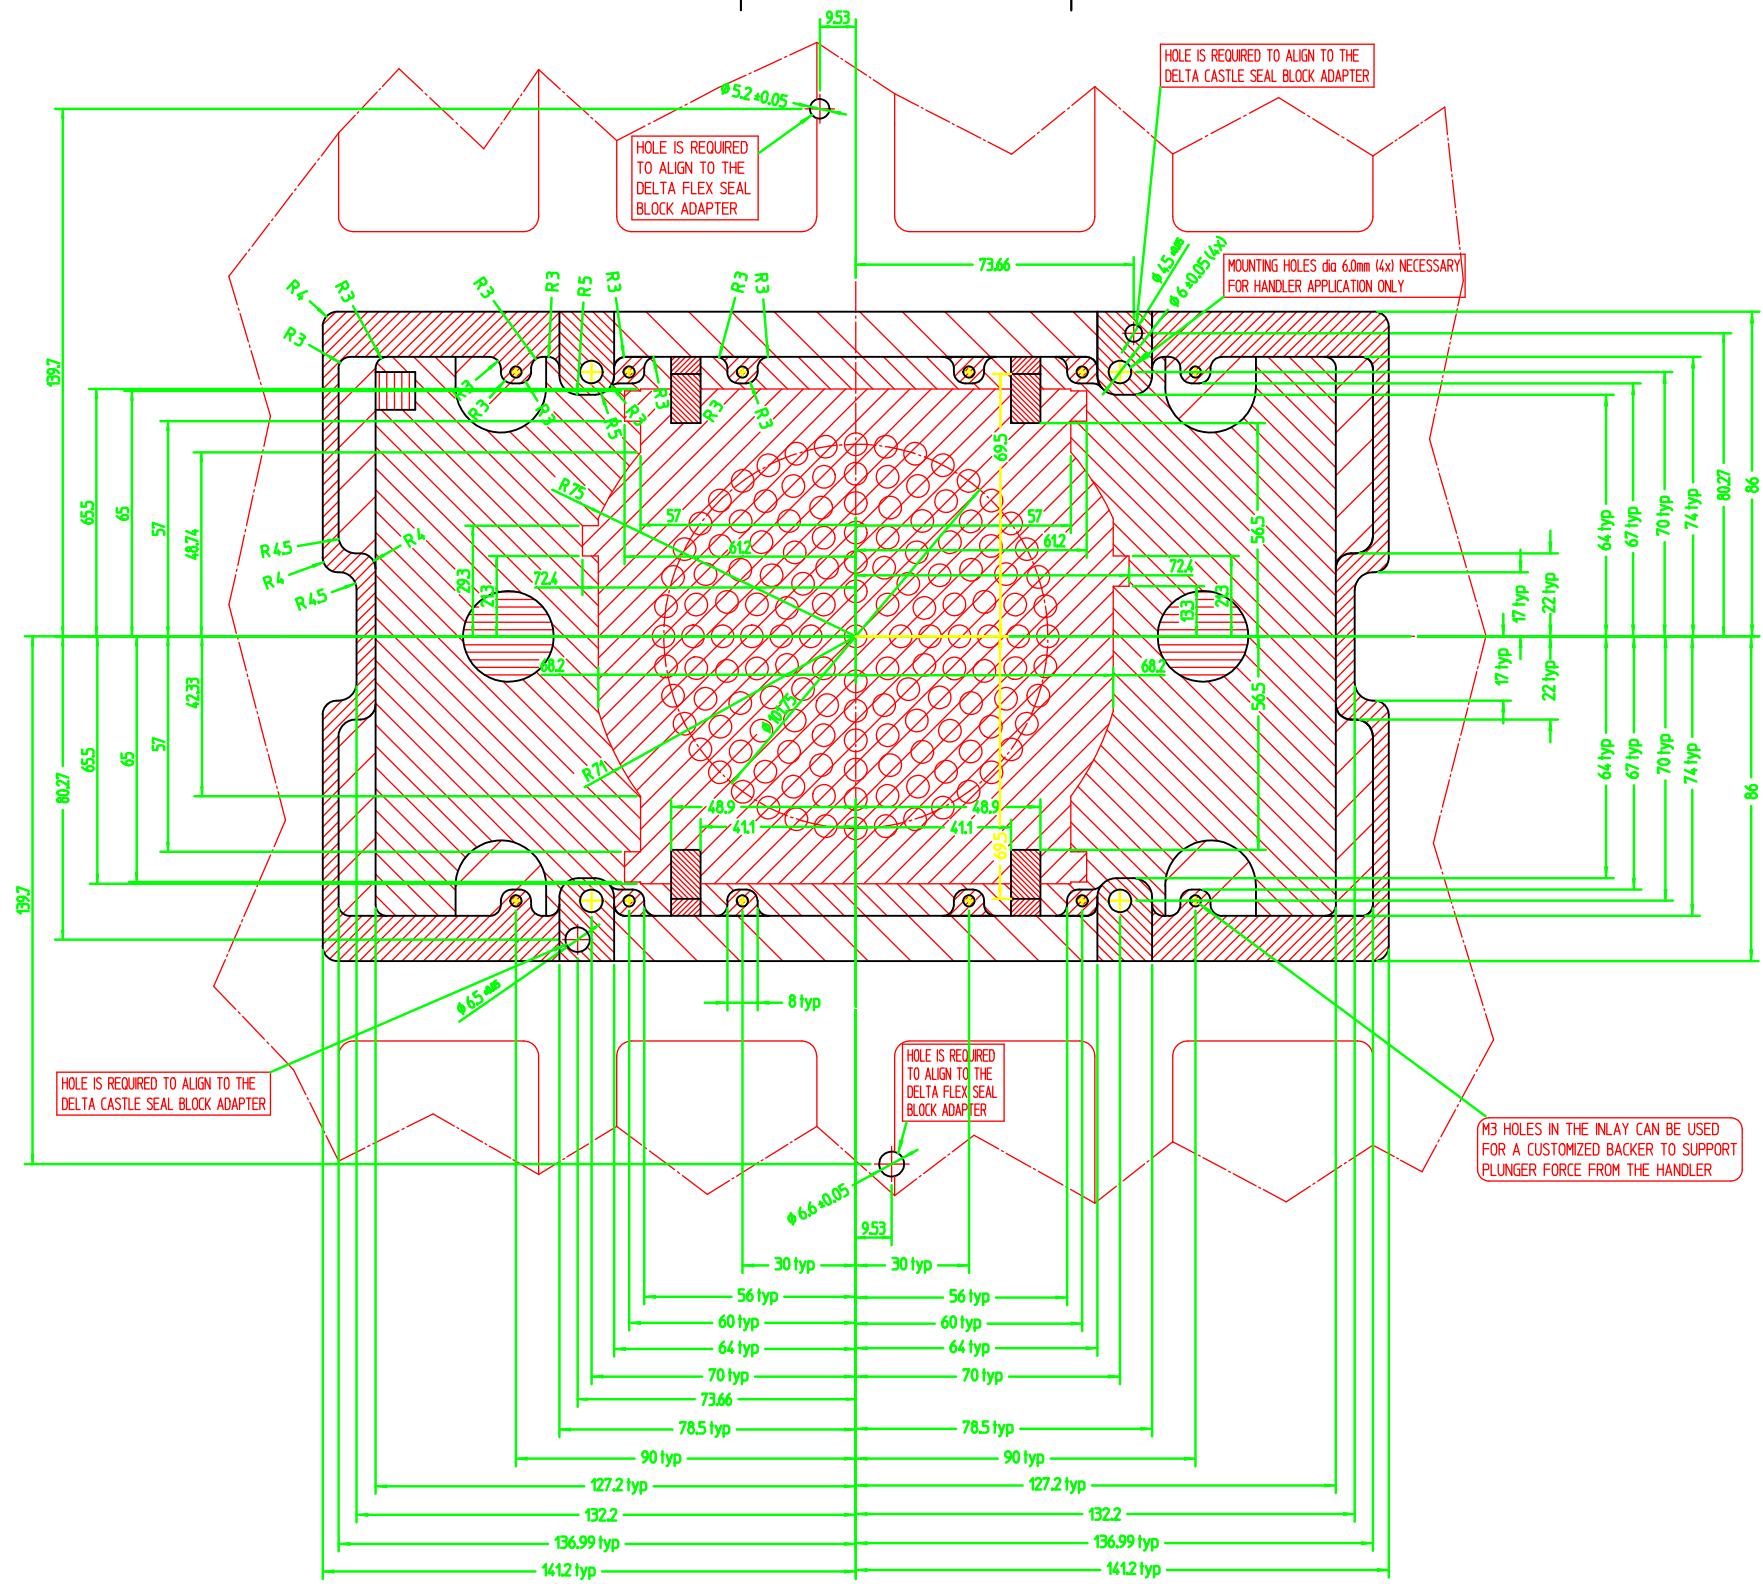

- THESE AREAS CONTACT THE STIFFENER INLAY ON BOTTOM SIDE OF PCB. SIGNAL, GND TRACES, VIAS AND PADS ARE NOT ALLOWED
- THESE AREAS ARE AT A CLEARANCE HEIGHT OF 3.5mm TO THE STIFFENER INLAY ON BOTTOM SIDE OF PCB. SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 2.5mm
- THESE AREAS ARE AT A CLEARANCE HEIGHT OF 5mm TO THE STIFFENER INLAY ON BOTTOM SIDE OF PCB. SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 4mm
- THESE AREAS ARE AT A CLEARANCE HEIGHT OF 9.5mm TO THE STIFFENER INLAY ON BOTTOM SIDE OF PCB. SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 8.5mm
- THIS AREA HAS A CLEARANCE HEIGHT OF 34.8mm TO THE CONNECTOR PLATE ON BOTTOM SIDE OF PCB, WITHOUT TAKING CARE OF RF CABLES AND BENDING RADIUS. SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 20.0mm
- THESE AREAS ARE AT A CLEARANCE HEIGHT OF 39.0mm TO THE PURGE KIT N2467A ON BOTTOM SIDE OF PCB. COMPONENT PLACEMENT AREA ON BOTTOM SIDE OF PCB. TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 20.0mm
- THESE AREAS ARE AT A CLEARANCE HEIGHT OF 8mm TO THE STIFFENER INLAY ON BOTTOM SIDE OF PCB. SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 7mm
- THESE AREAS ARE AT A CLEARANCE HEIGHT OF 21.0mm TO THE STIFFENER INLAY ON BOTTOM SIDE OF PCB. SIGNAL AND GND TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 20.0mm
- THIS AREA IS AT A CLEARANCE HEIGHT OF 28.0mm TO THE PURGE KIT N2467A ON BOTTOM SIDE OF PCB. COMPONENT PLACEMENT AREA ON BOTTOM SIDE OF PCB. TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 20.0mm
- THIS AREA IS AT A CLEARANCE HEIGHT OF 35.0mm TO THE PURGE KIT N2467A ON BOTTOM SIDE OF PCB. COMPONENT PLACEMENT AREA ON BOTTOM SIDE OF PCB. TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 20.0mm
- THIS AREA IS AT A CLEARANCE HEIGHT OF 25.0mm TO THE PURGE KIT N2467A ON BOTTOM SIDE OF PCB. COMPONENT PLACEMENT AREA ON BOTTOM SIDE OF PCB. TRACES, VIAS AND PADS ARE ALLOWED. RECOMMENDED MAX. COMPONENT HEIGHT = 20.0mm

NOTES:
1. USE KEEP-OUT AREA DEFINITION IN CONJUNCTION WITH GENERAL DUT BOARD DEFINITION. SEE D-E6980-96540-1 SMALL DUT BOARD AND D-E6980-96550-1 LARGE DUT BOARD
2. ALL KEEP-OUT AREAS RELATE TO THE BOTTOM SIDE OF THE PCB