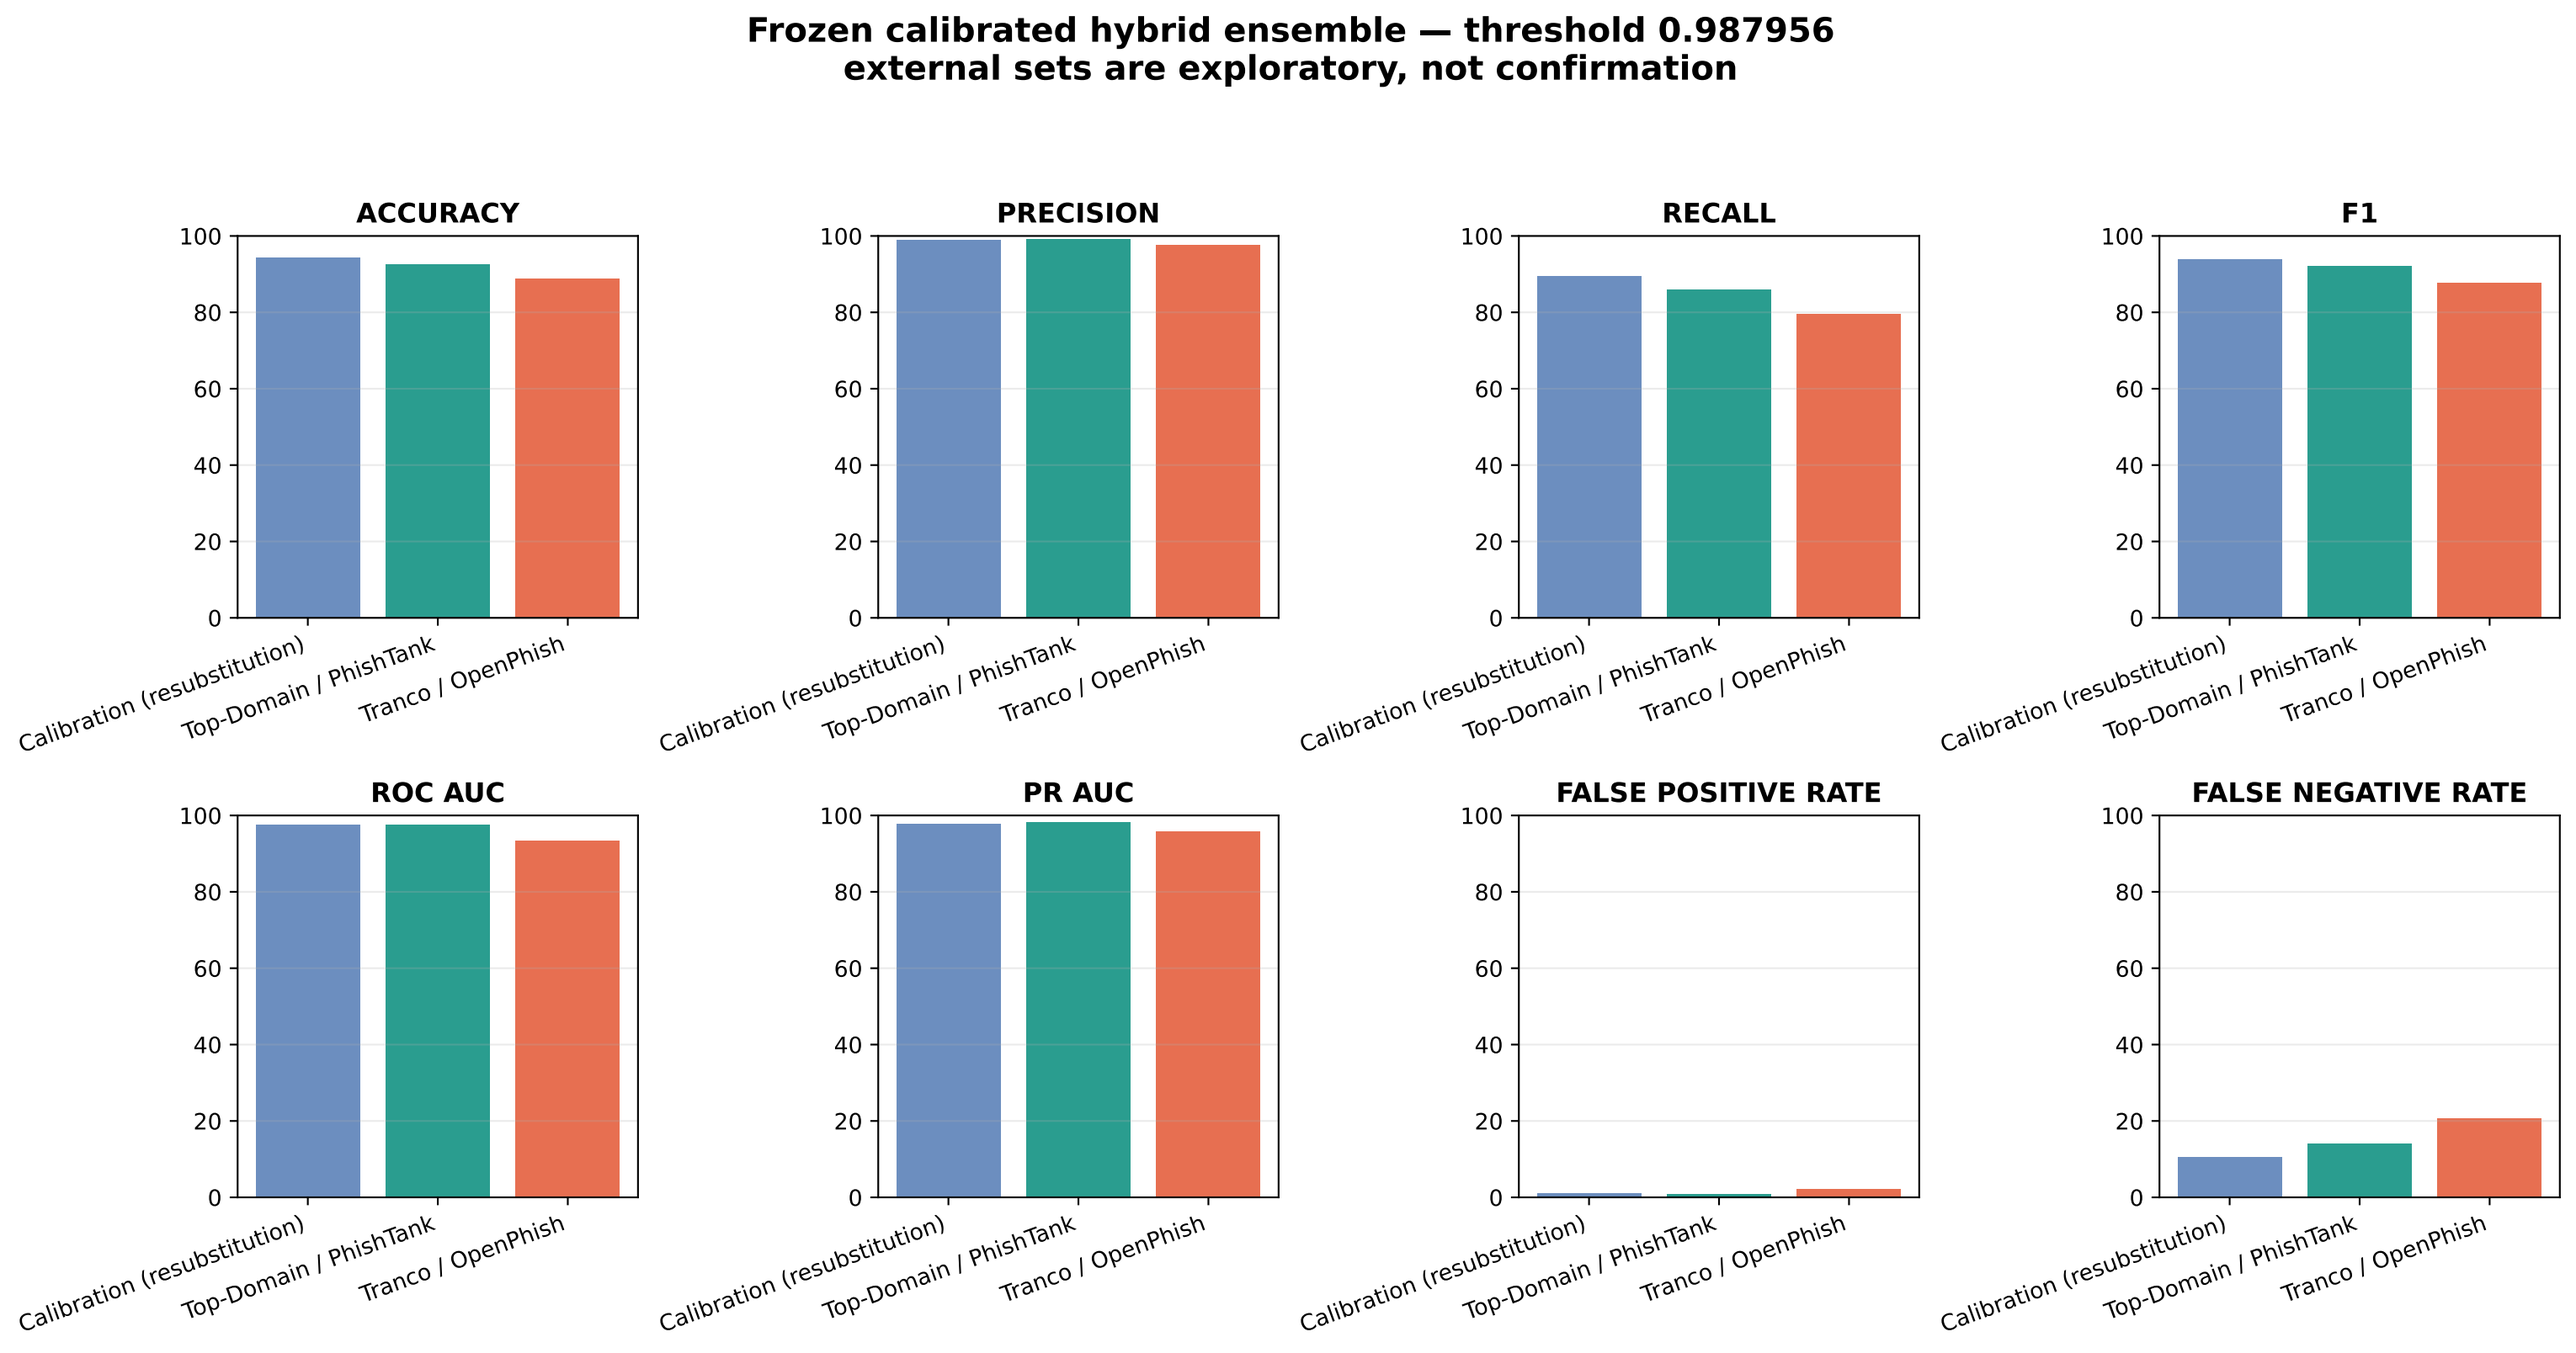
Frozen calibrated hybrid ensemble — threshold 0.987956
external sets are exploratory, not confirmation
ACCURACY
PRECISION
RECALL
F1
ROC AUC
PR AUC
FALSE POSITIVE RATE
FALSE NEGATIVE RATE
0
20
40
60
80
100
Calibration (resubstitution)
Top-Domain / PhishTank
Tranco / OpenPhish