Fictional visual-review test

Software test only. No student data or real experimental results.

Claim for review: These data prove that stationary phase starts at 180 minutes.

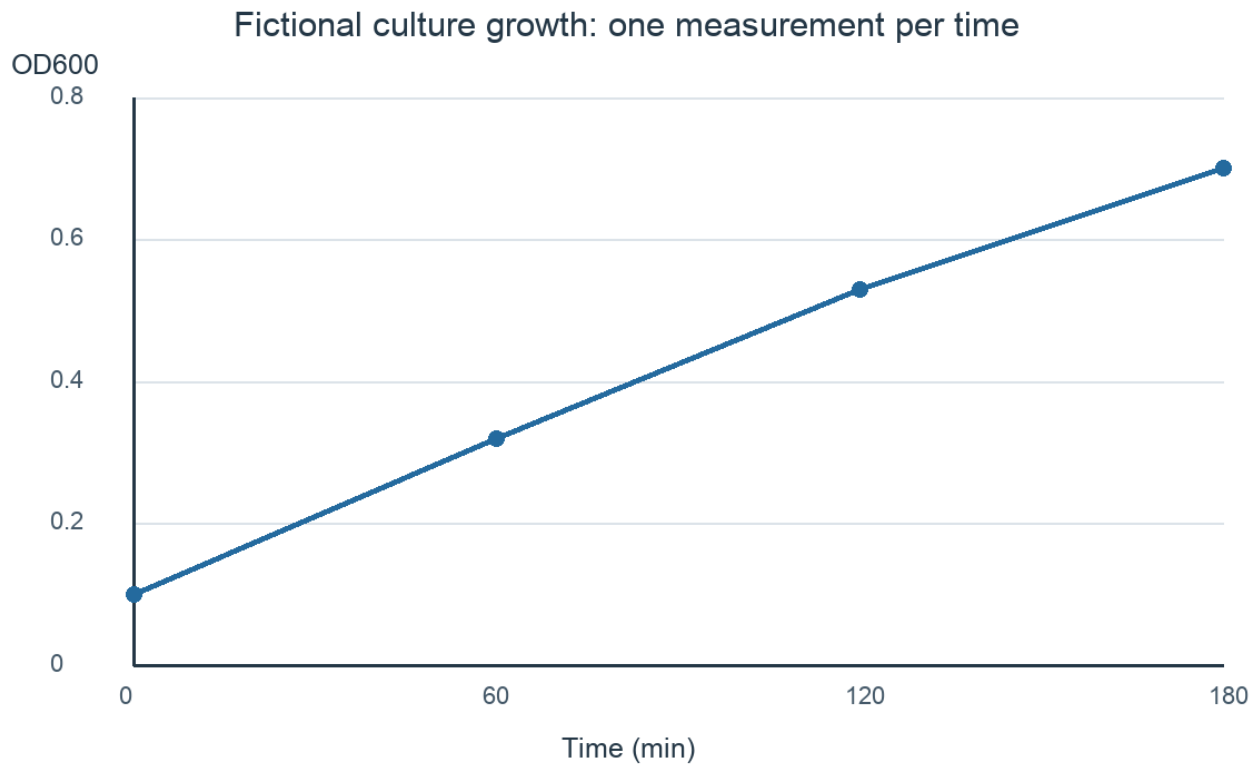

Figure 1. Single measurements; no error bars shown.

Methods: OD600 was measured once at each time point.

Results: OD600 increased from 0.10 to 0.70 over 180 minutes.

Fictional data table

Table 1. Raw values supplied for software validation.

Time (min)	OD600
0	0.10
60	0.32
120	0.53
180	0.70

No inferential statistical test is justified from this series alone.

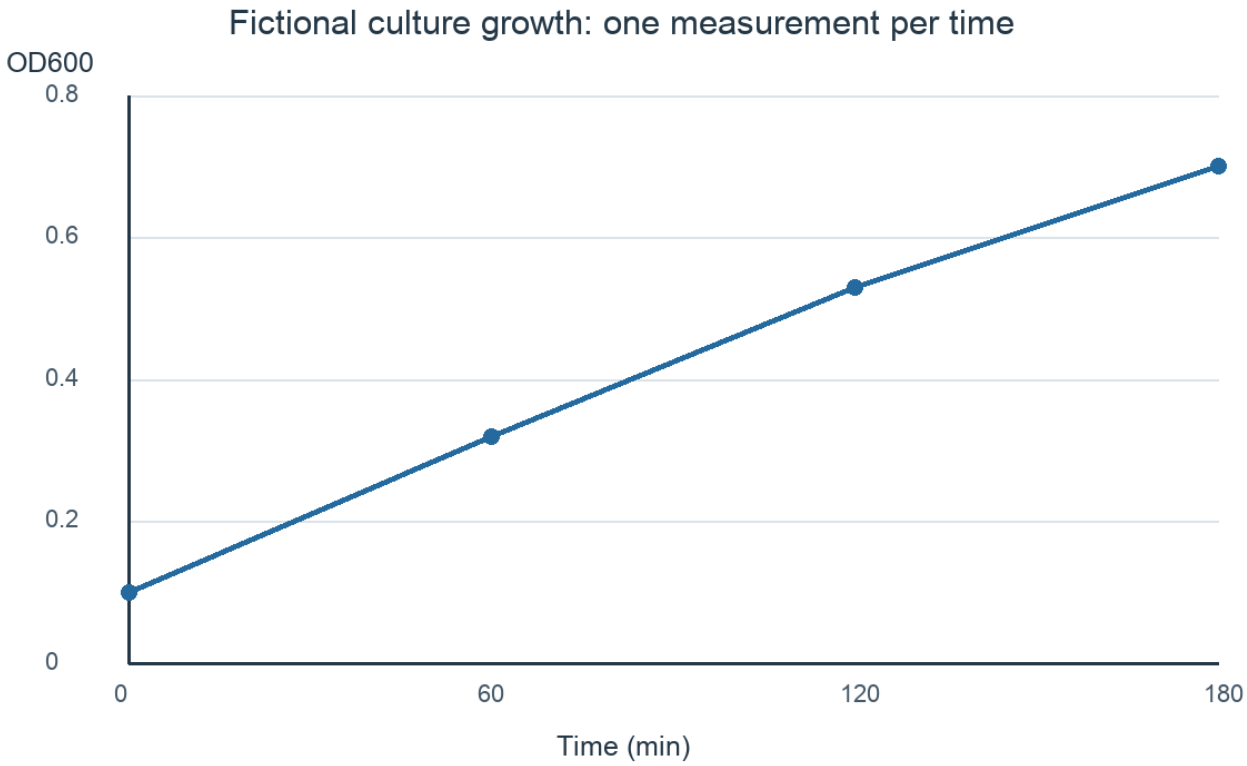

Figure 1. Single measurements; no error bars shown.