


Patient: [REDACTED]
Recorded: Monday, 2. September 2019 at 08:54:28
Heart Rate: 87 BPM
Duration: 30s

Instant Analysis: Normal
*Instant Analysis is done on Lead I.



Enhanced Filter, Mains Frequency: 50Hz Scale: 25mm/s, 10mm/mV

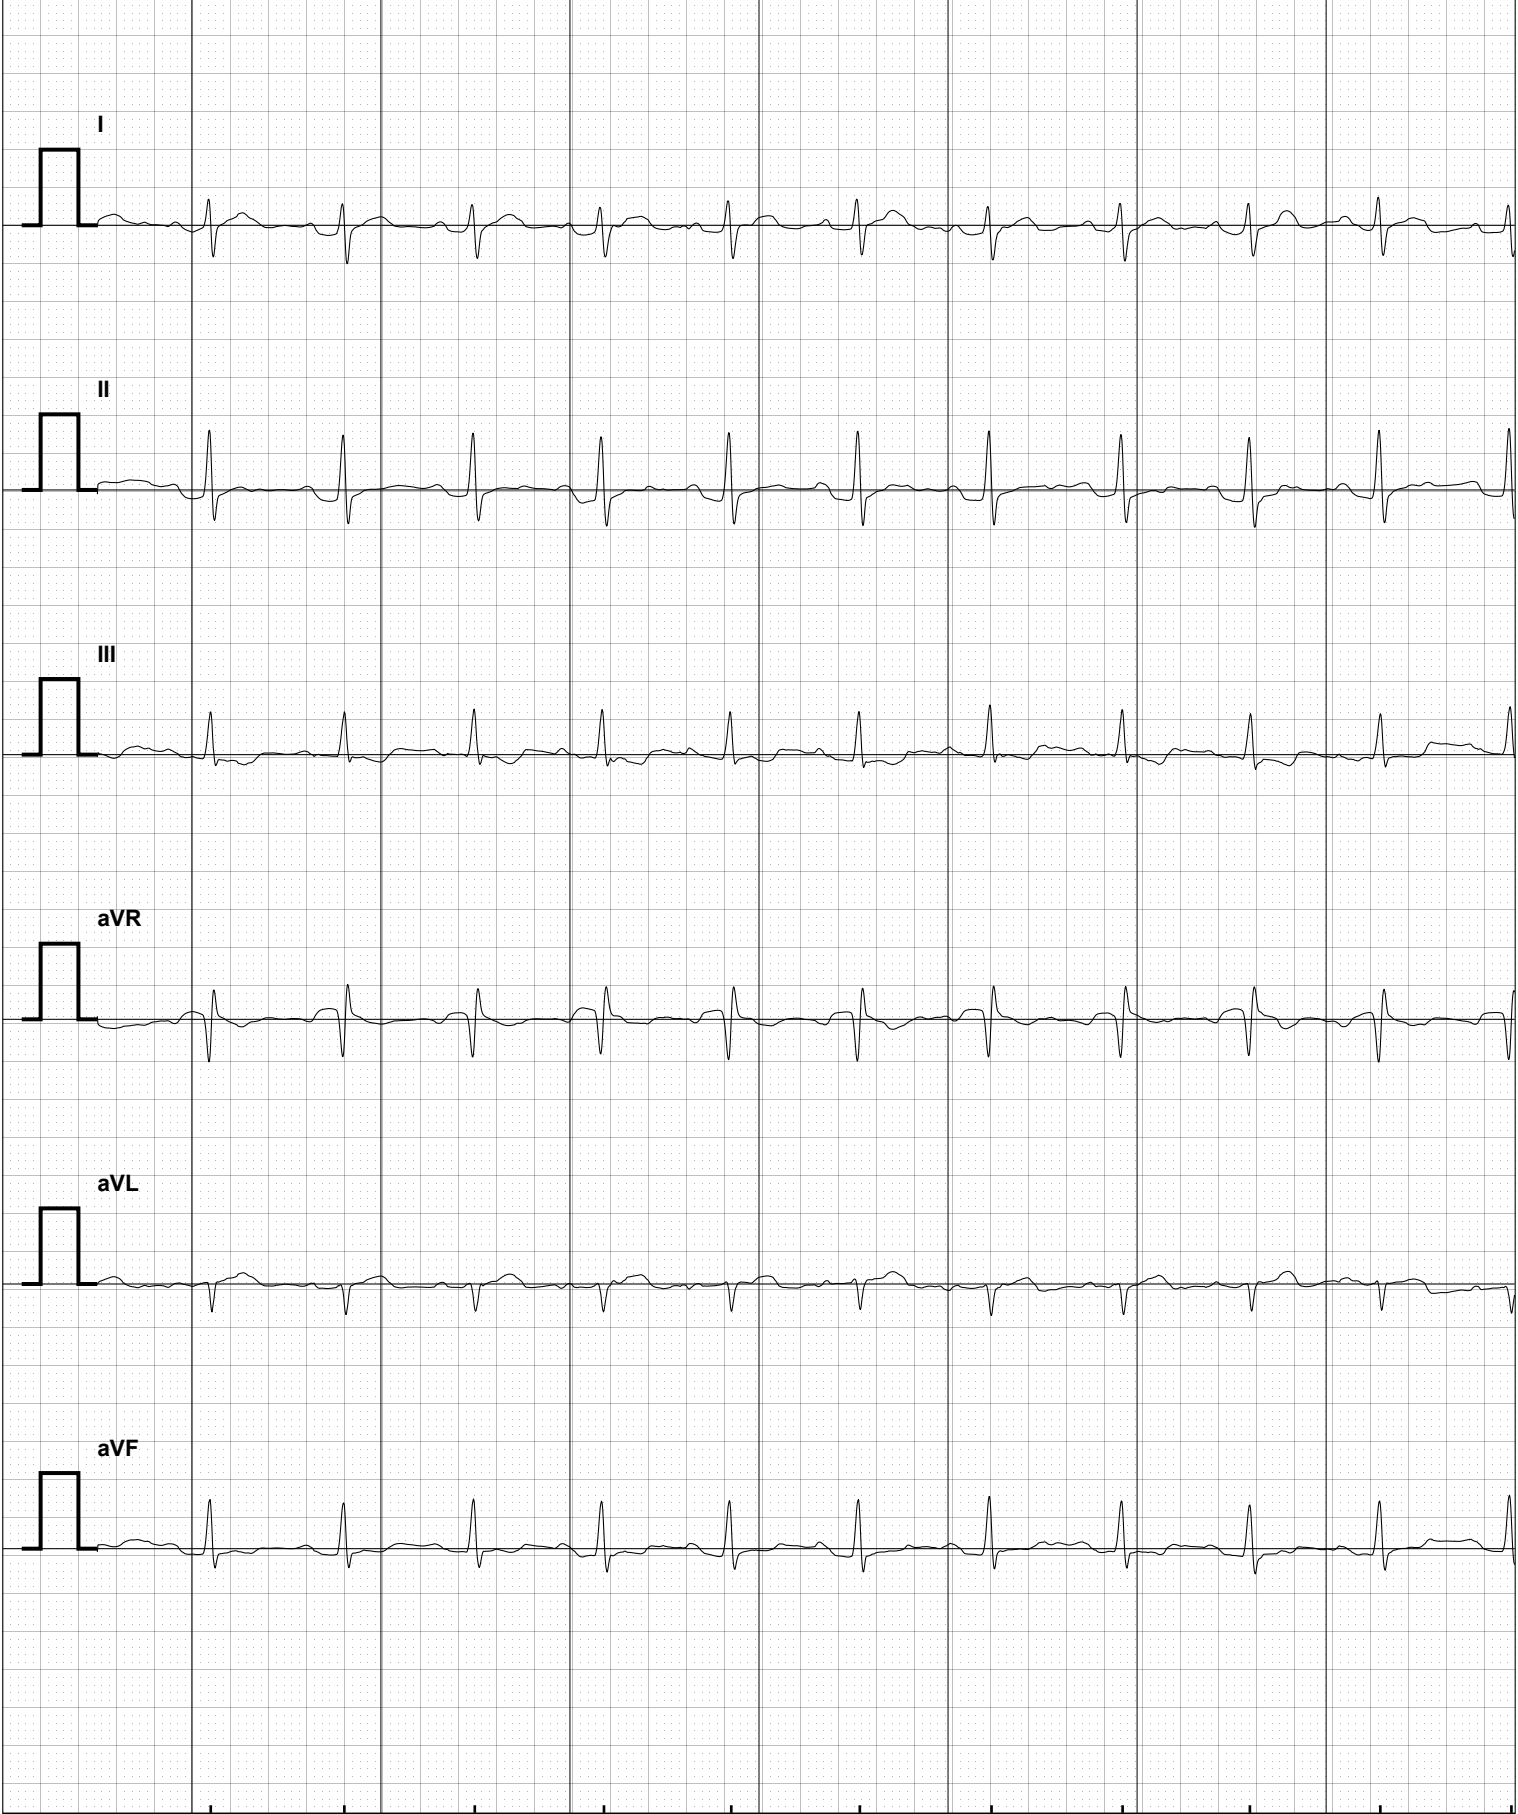


Patient: [REDACTED]
Recorded: Monday, 2. September 2019 at 08:54:28
Heart Rate: 87 BPM
Duration: 30s

Instant Analysis: Normal
*Instant Analysis is done on Lead I.



Enhanced Filter, Mains Frequency: 50Hz Scale: 25mm/s, 10mm/mV

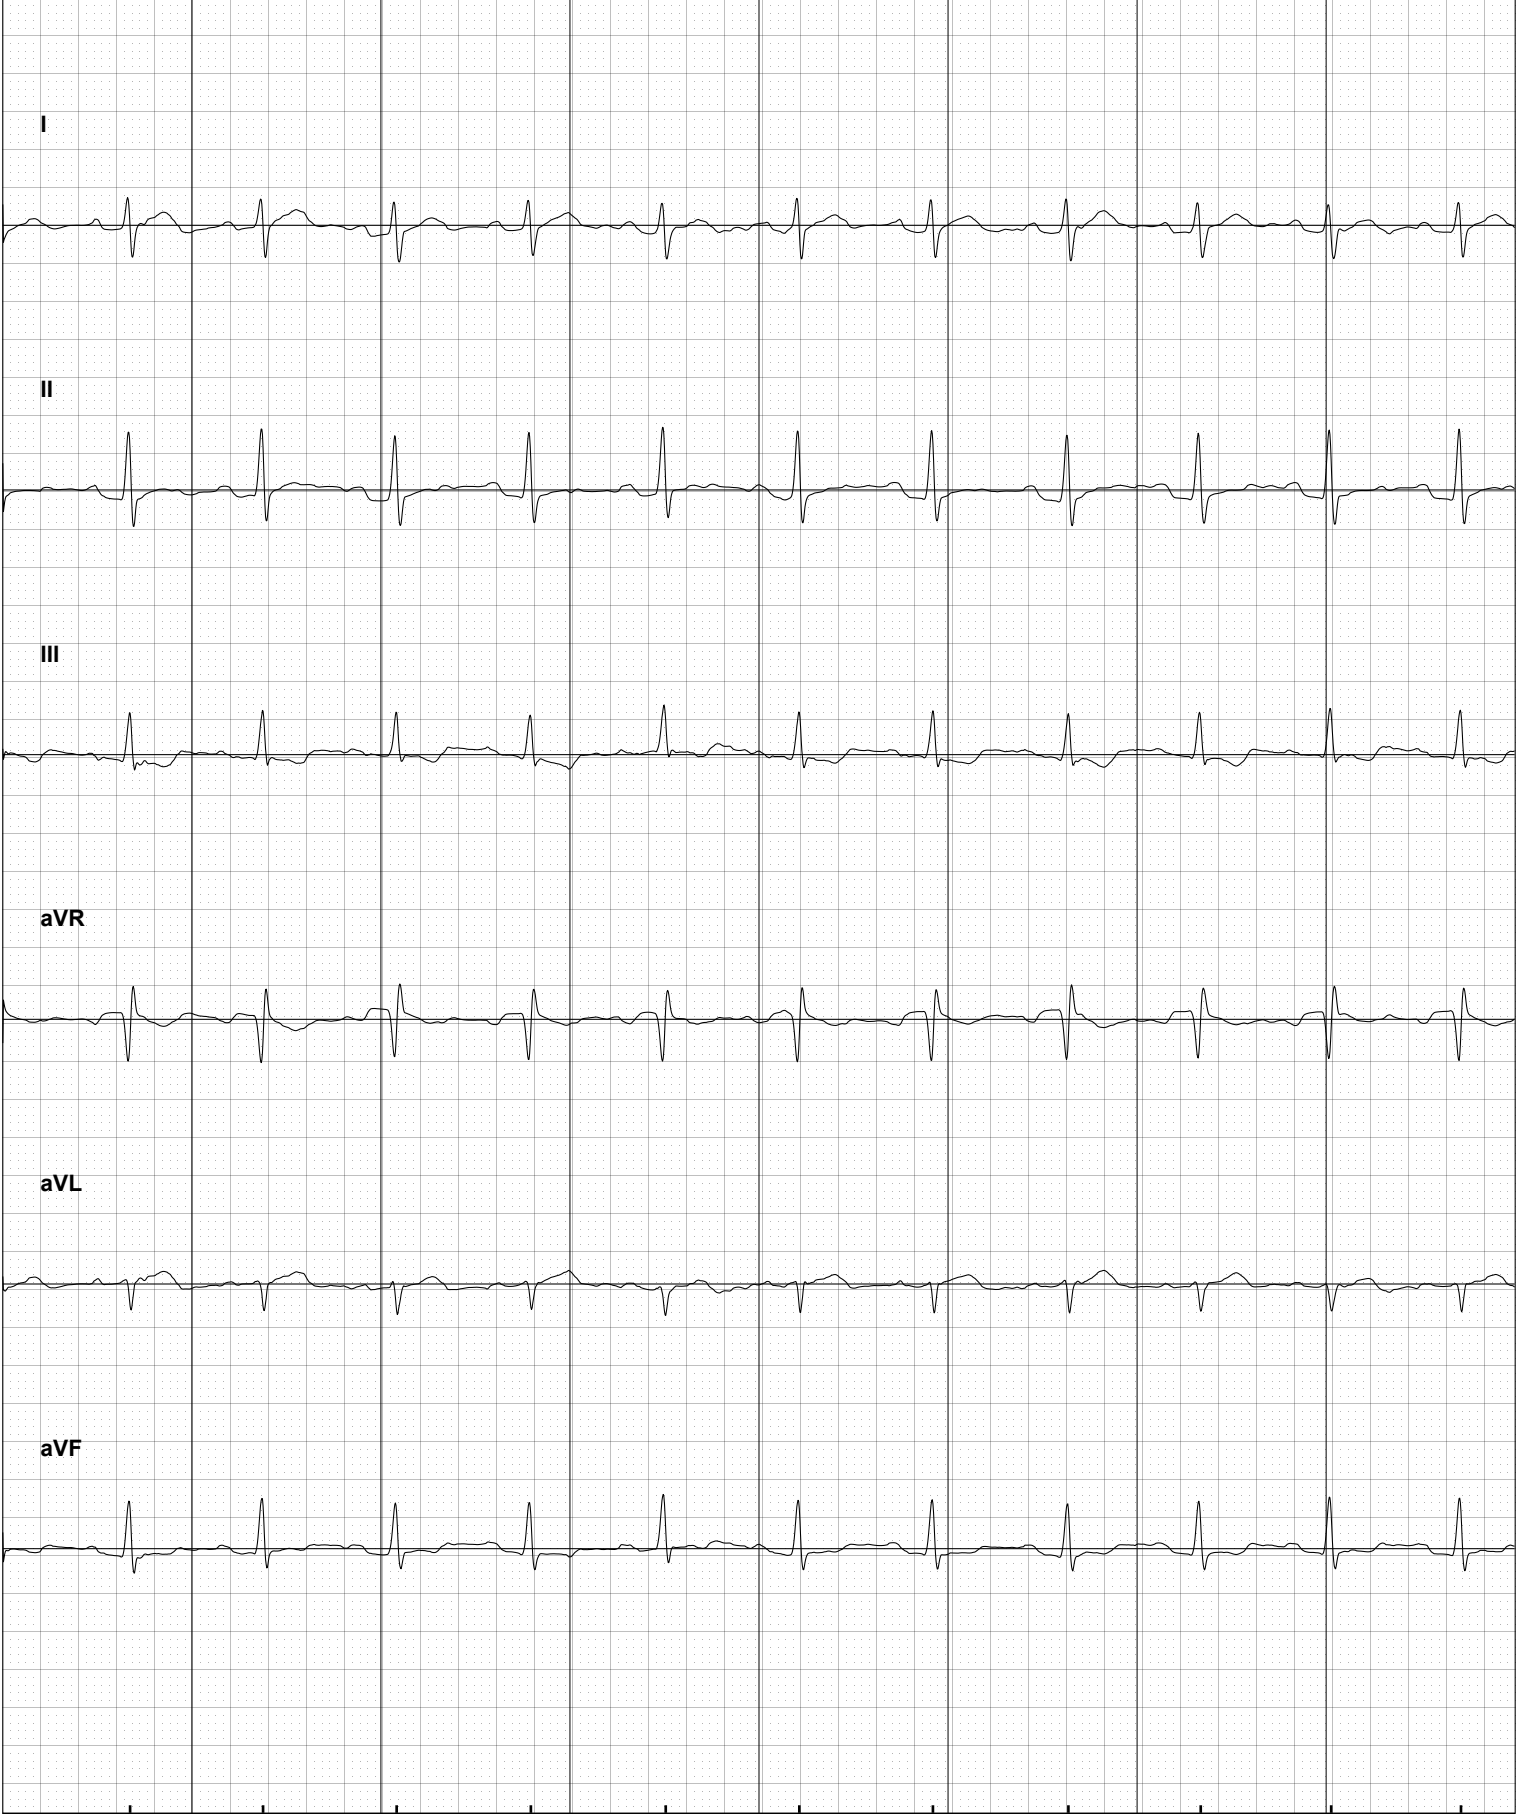


Patient: [REDACTED]
Recorded: Monday, 2. September 2019 at 08:54:28
Heart Rate: 87 BPM
Duration: 30s

Instant Analysis: Normal
*Instant Analysis is done on Lead I.



Enhanced Filter, Mains Frequency: 50Hz Scale: 25mm/s, 10mm/mV

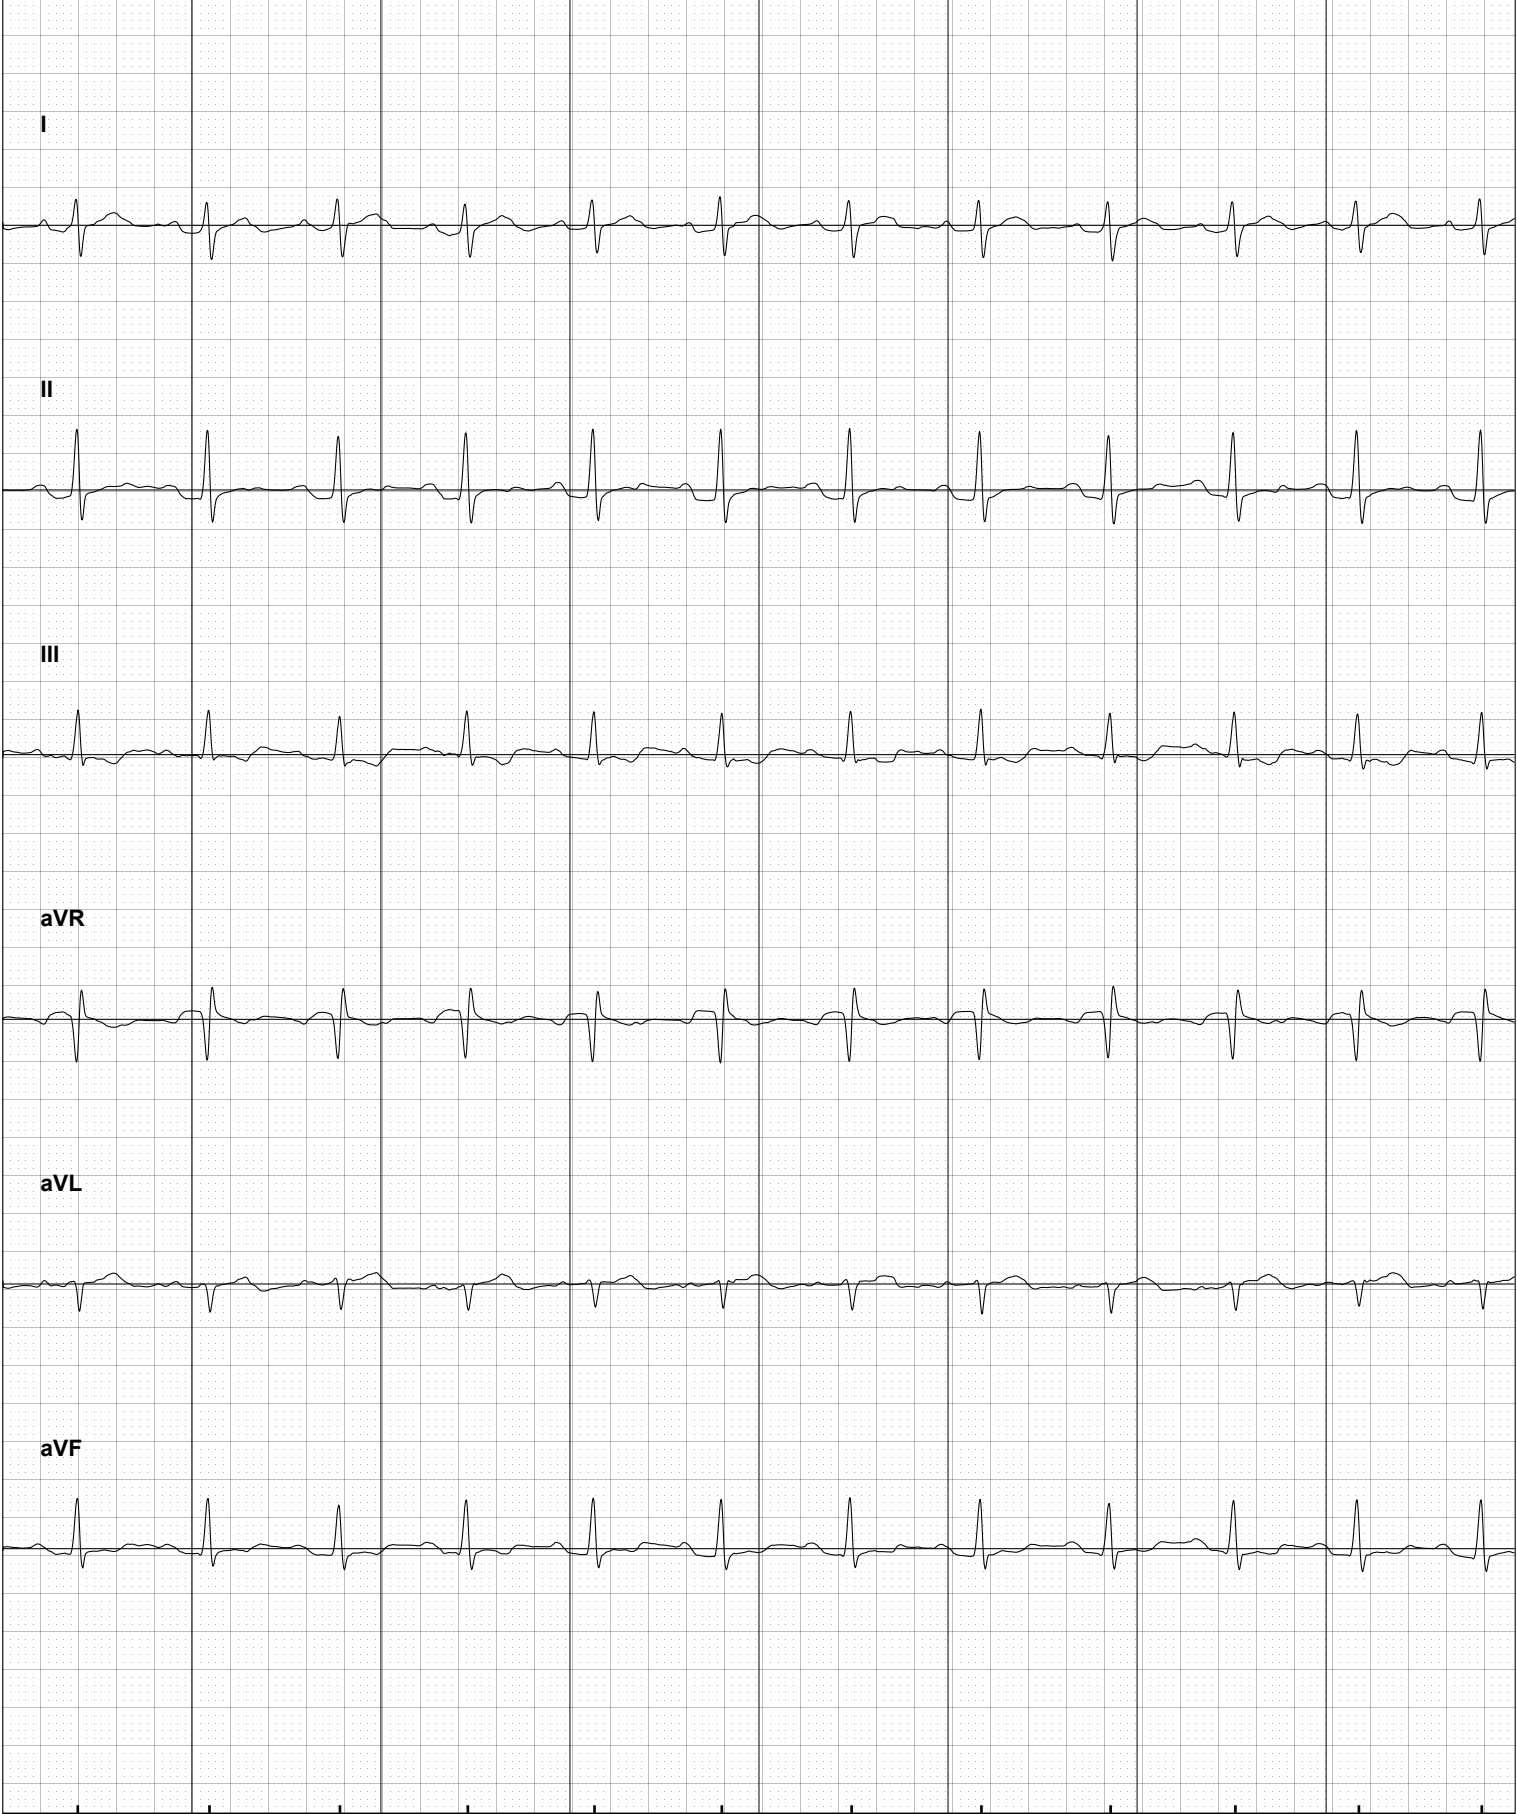

Patient: [REDACTED]
Recorded: Monday, 2. September 2019 at 08:54:28
Heart Rate: 87 BPM
Duration: 30s

Instant Analysis: Normal
*Instant Analysis is done on Lead I.



Enhanced Filter, Mains Frequency: 50Hz Scale: 25mm/s, 10mm/mV

