



Summary

Scan Name	ATEAM-908-KG_63-PRE
Date Prepared	2022-04-29 17:11:25.608572
VDP (%)	23.8
Mean Specific Ventilation (mL/mL)	0.14
Tidal Volume (mL)	253.053
Ventilation Heterogeneity (%)	76.59
Ventilation Heterogeneity - Small Scale (%)	40.01
Ventilation Heterogeneity - Large Scale (%)	46.03


Ventilation Frequency Distribution

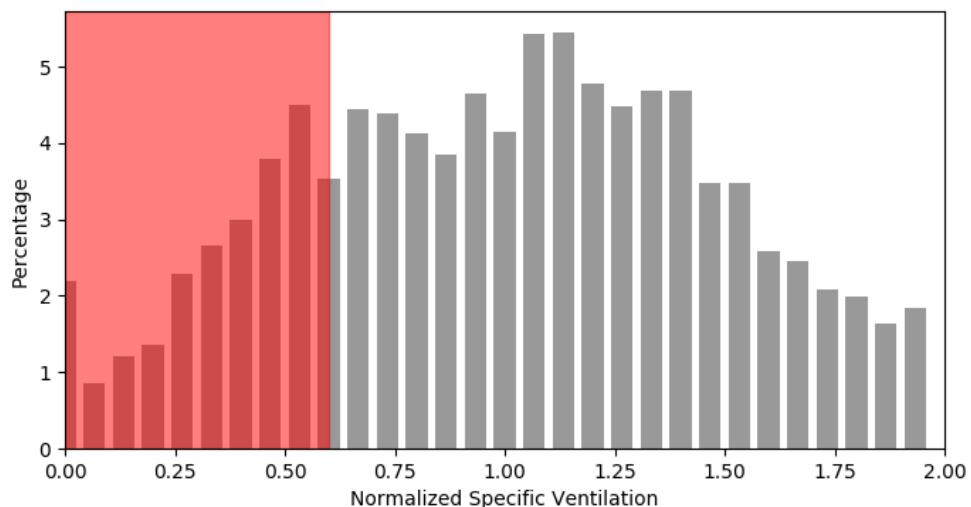

Regional Ventilation Visualization (Peak Inspiration)

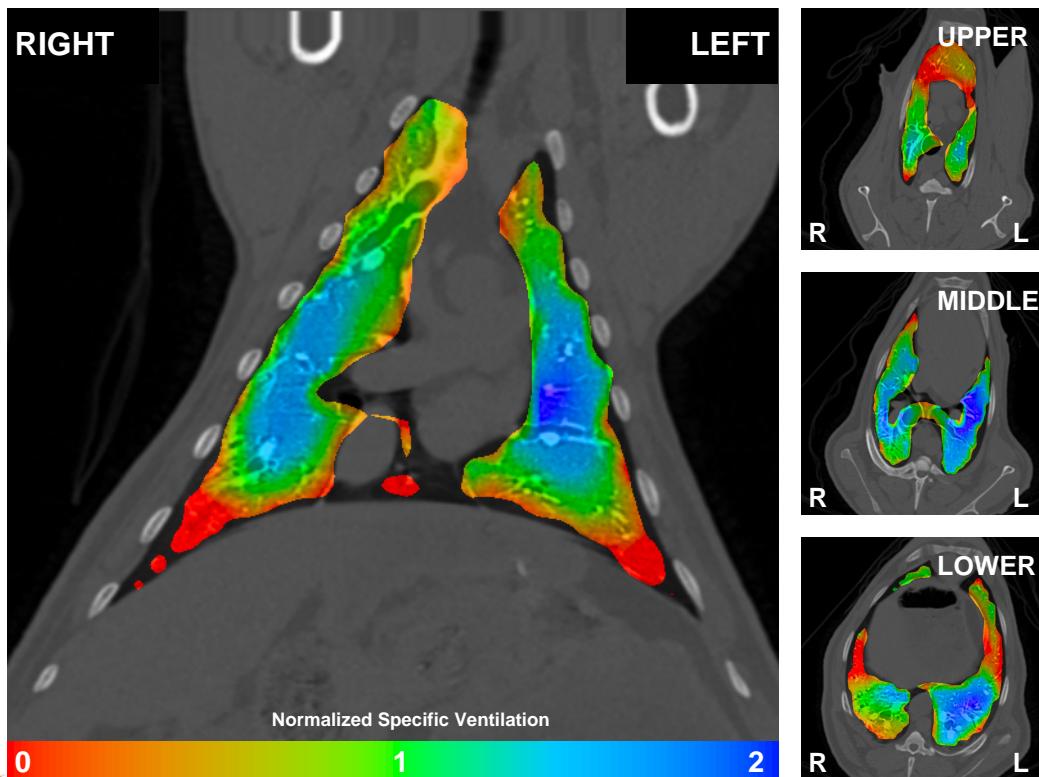


Regional Ventilation Visualization (Peak Inspiration) - Axial Slices Page 1

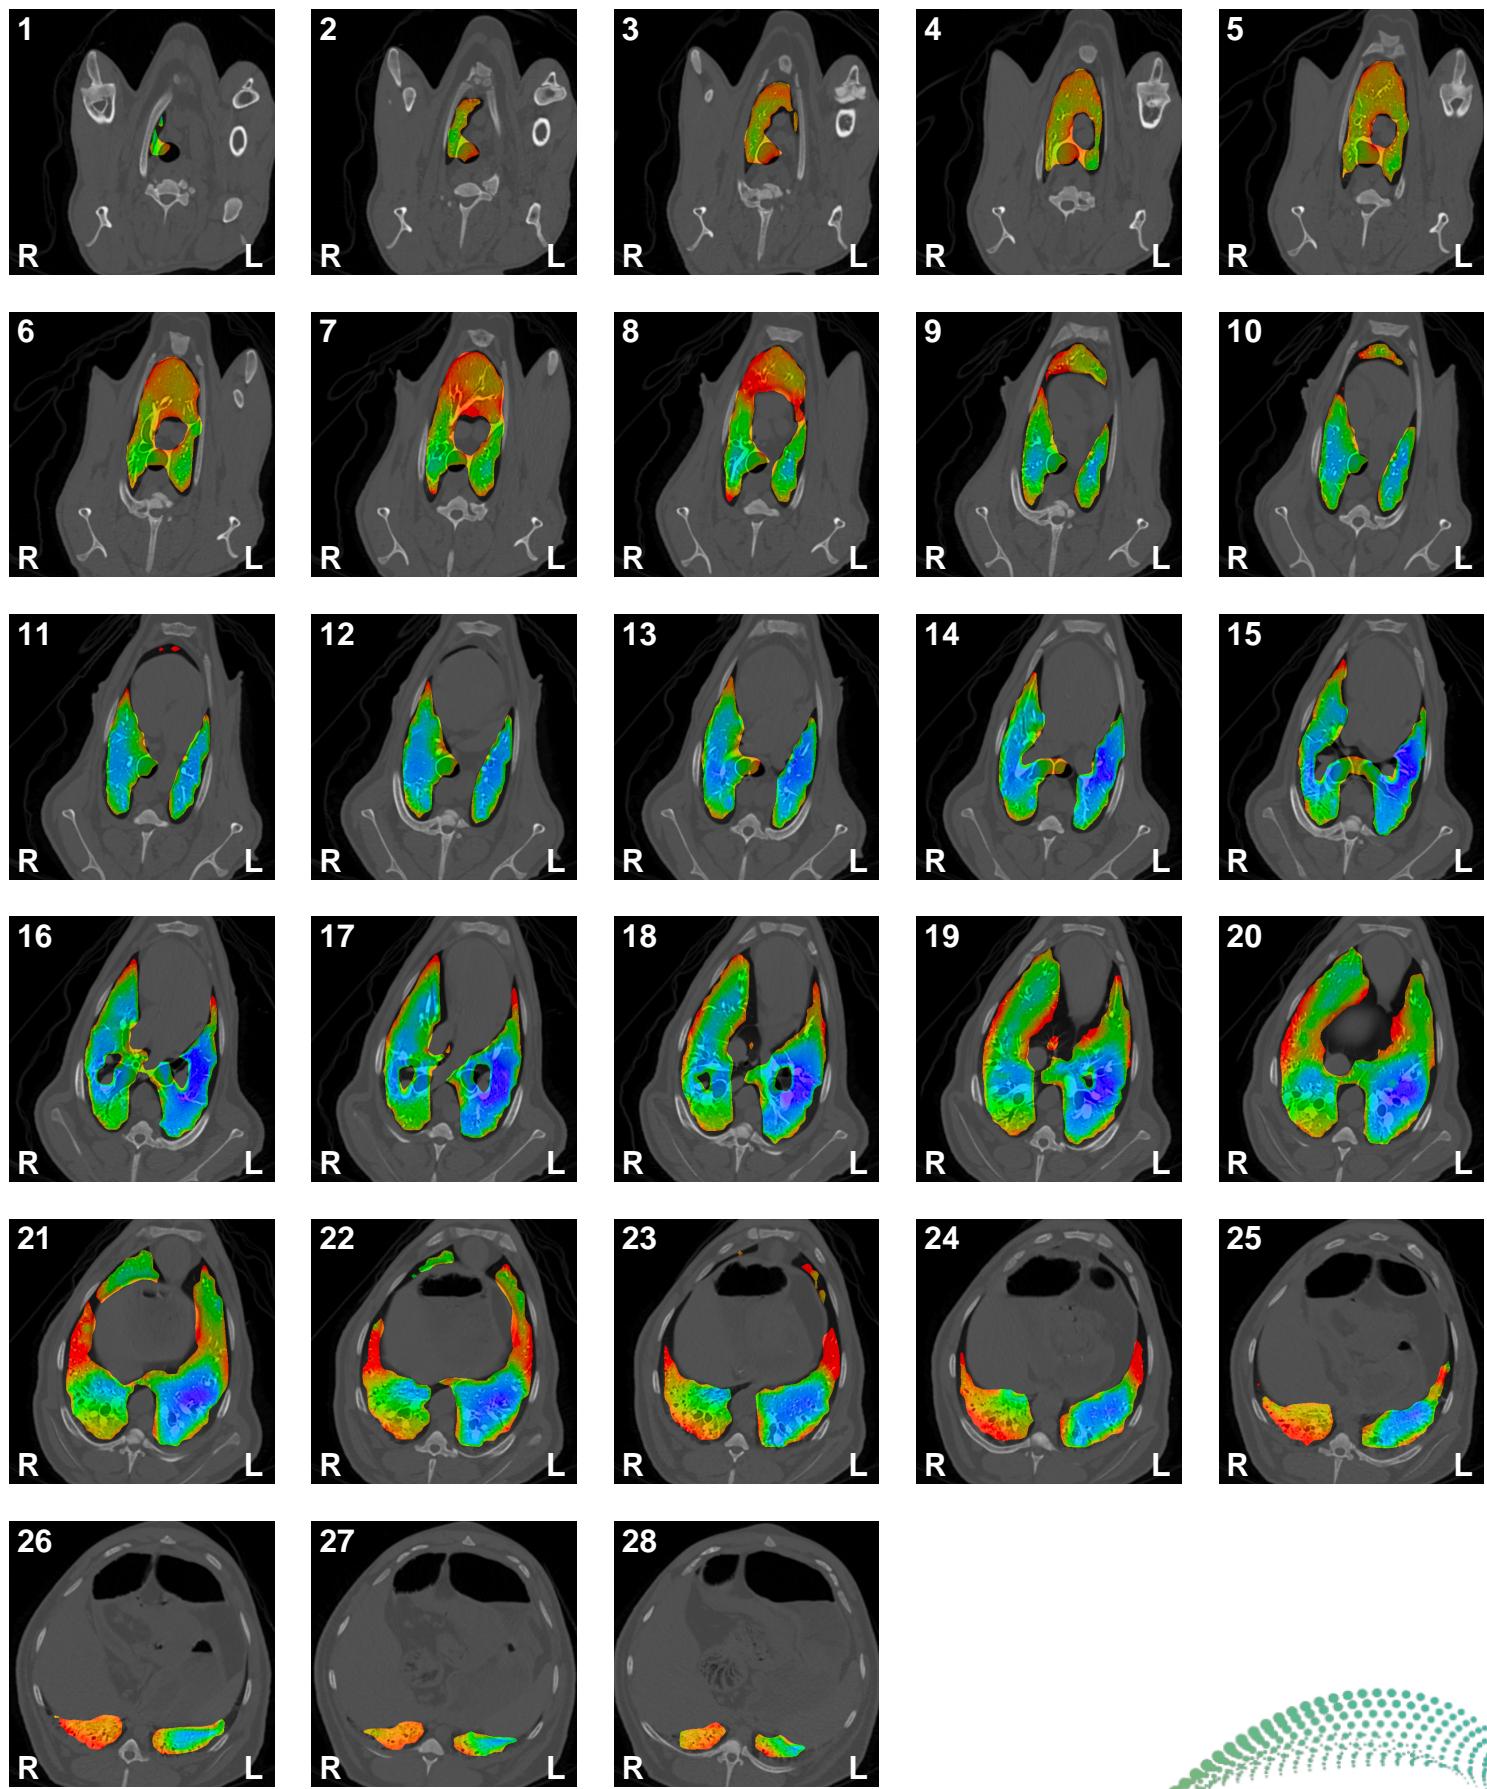









Slice Spacing = 8.0 mm

Regional Ventilation Visualization (Peak Inspiration) - Coronal Slices

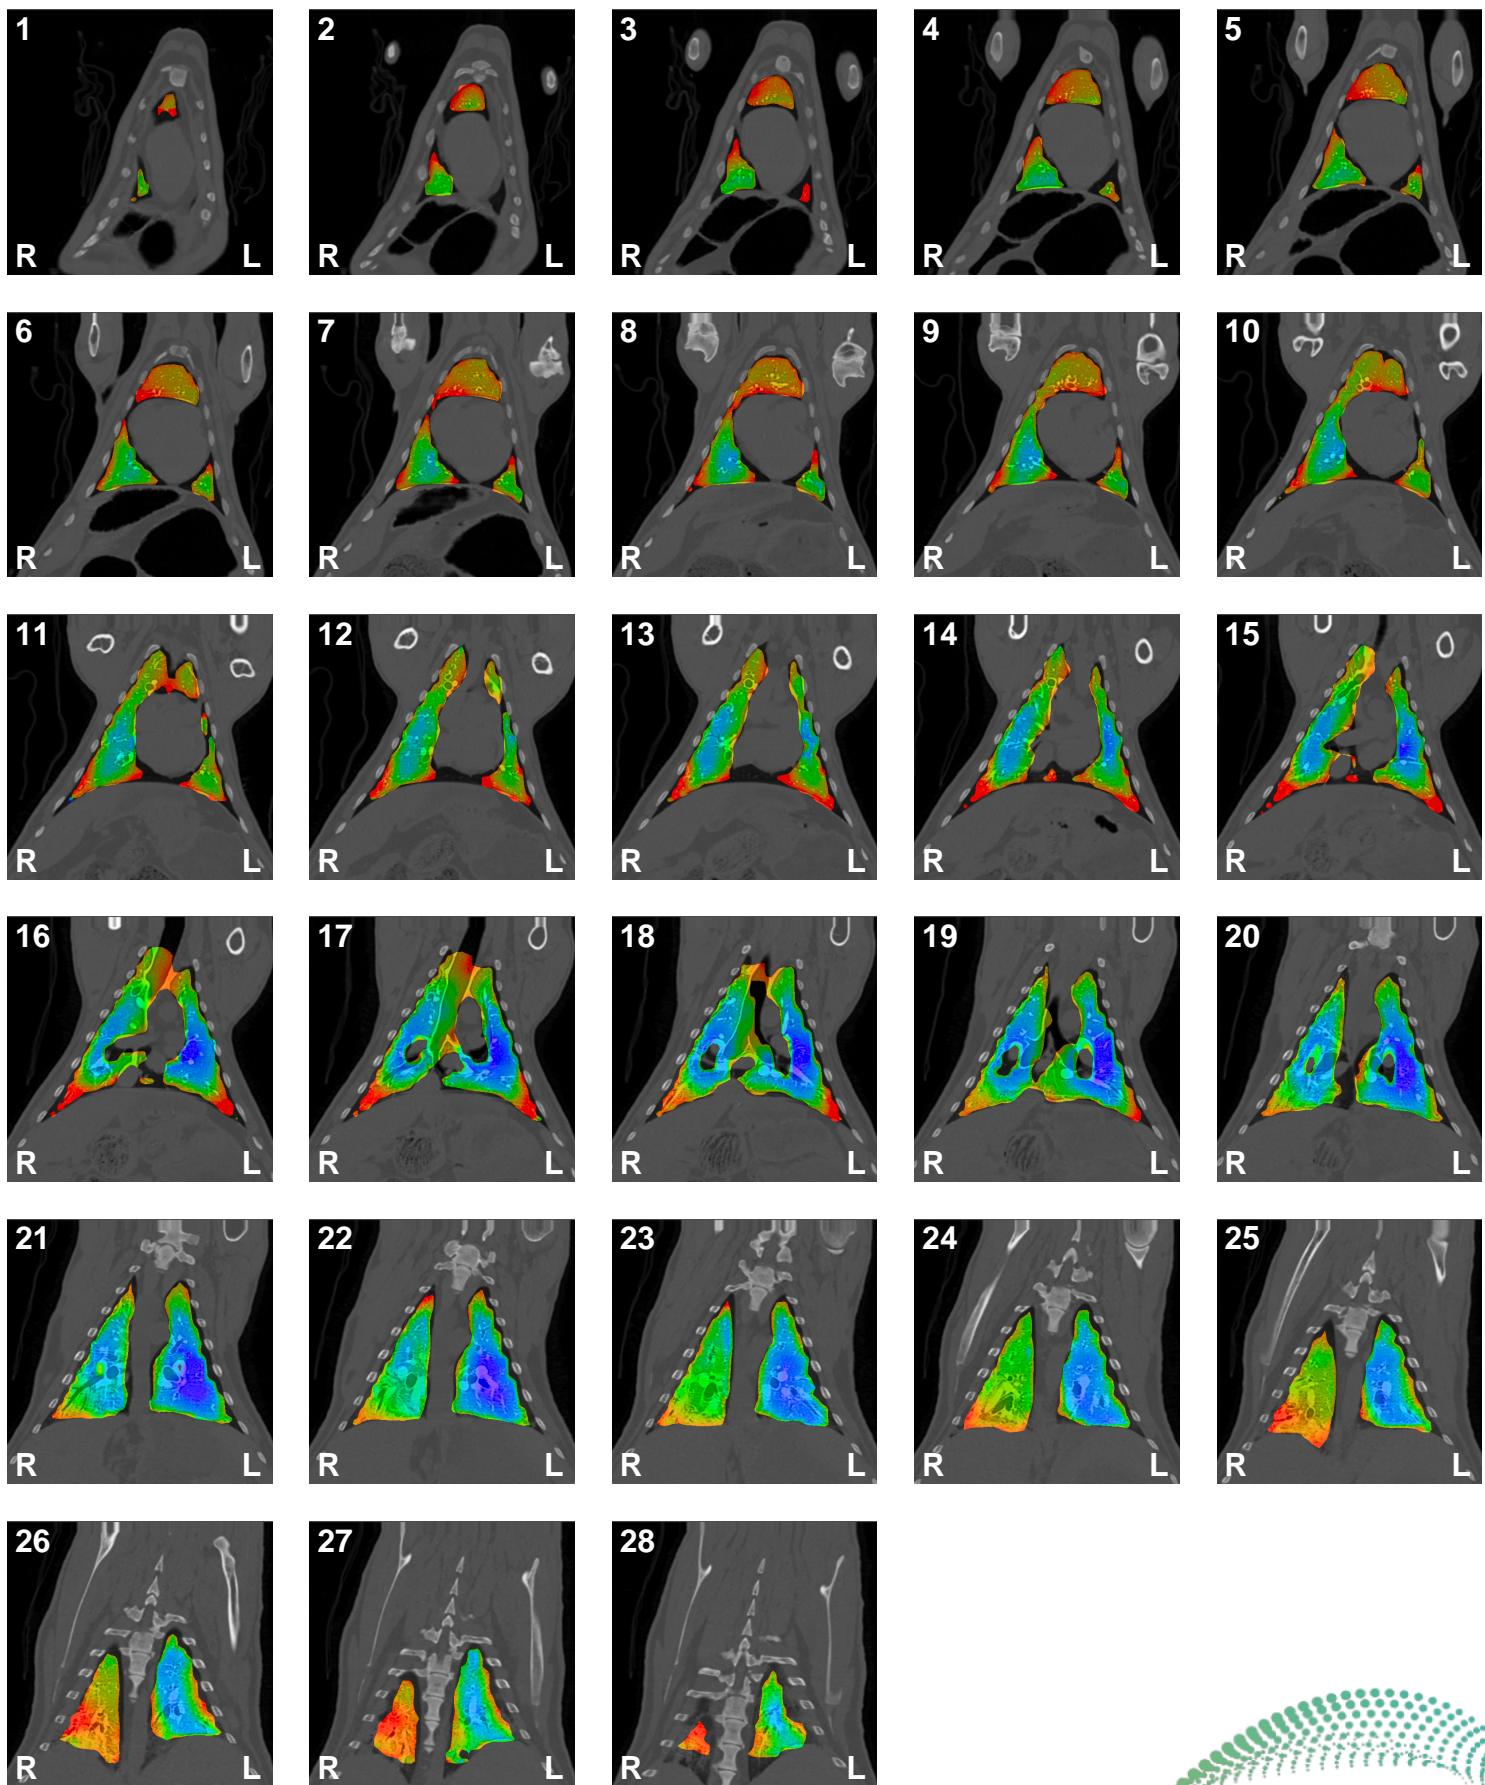

Slice Spacing = 8.0 mm

Coronal Mid-plane: Regional Ventilation Visualizations Across Phase Points (PP)

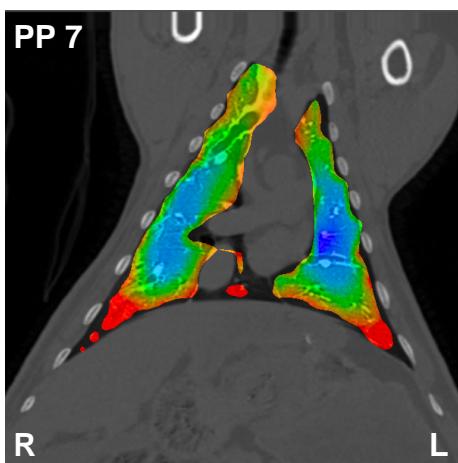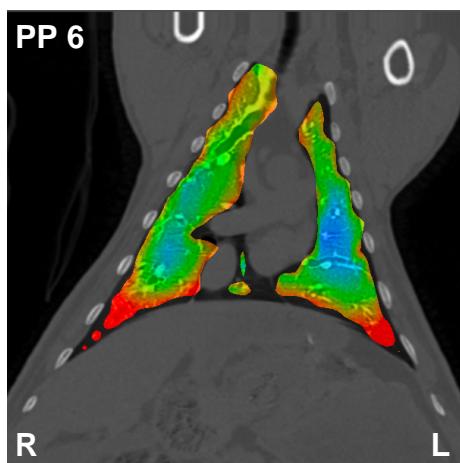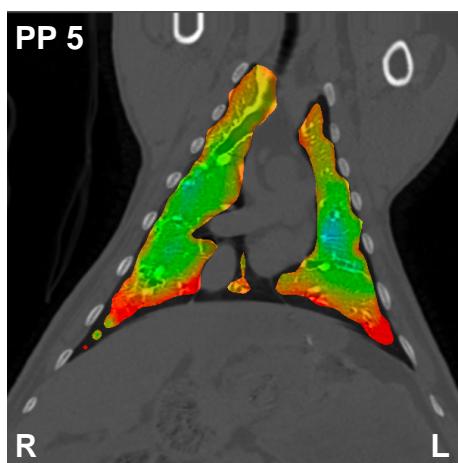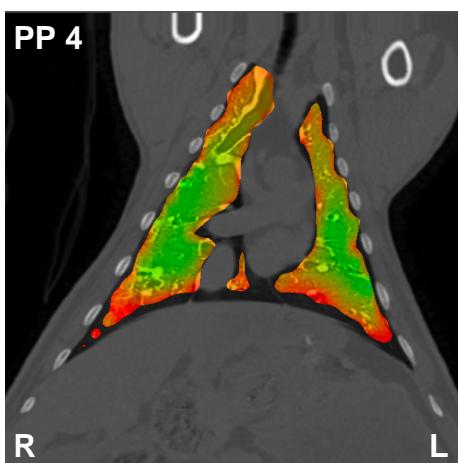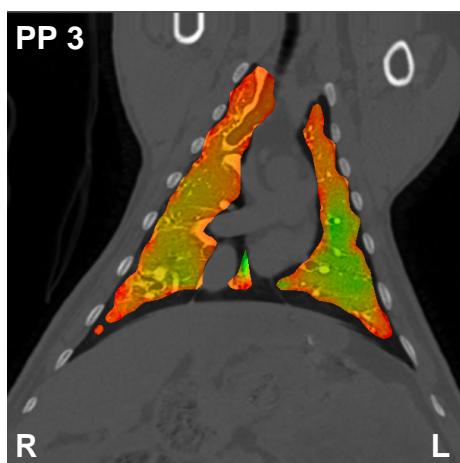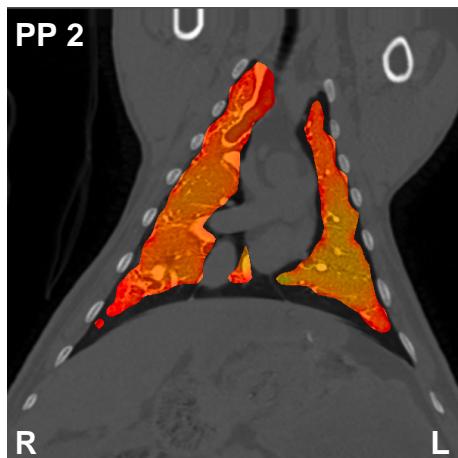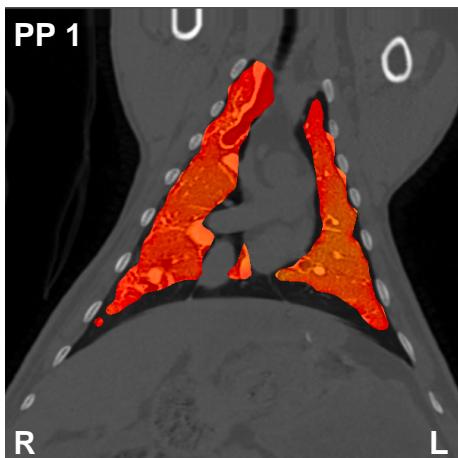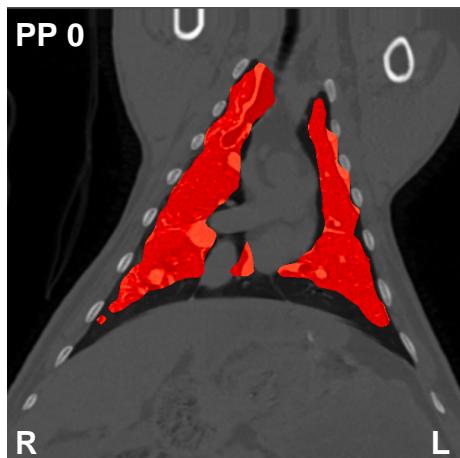

CT Acquisition Date: 20211007

Fluoro Acquisition Date: 20211007

Dataset: ATEAM-908-KG_63-PRE Build: dawson-m103 Config Version: v1.3.2