

¹ QuDAP: an Open Source Software for Quantum Materials Characterization

³ **Chunli Tang**  ³, **Skai White**¹, **Jingyu Jia**², **Masoud Mahjouri-Samani**³, and ⁴ **Wencan Jin**³

⁵ 1 Hampton University, Hampton, VA, USA 2 Great Neck South High School, Lake Success, NY, USA 3
⁶ Auburn University, Auburn, AL, USA

DOI: [10.xxxxxx/draft](https://doi.org/10.xxxxxx/draft)

Software

- [Review](#) 
- [Repository](#) 
- [Archive](#) 

Editor: Sophie Beck  

Reviewers:

- [@domna](#)
- [@lapmk](#)

Submitted: 07 August 2024

Published: unpublished

License

Authors of papers retain copyright and release the work under a ¹⁹ Creative Commons Attribution 4.0 International License ([CC BY 4.0](#))²⁰

⁷ Summary

⁸ Quantum Materials Data Acquisition and Processing (QuDAP), a Python-based and open-
⁹ source software package, is designed to control and automate material characterizations based
¹⁰ on the Physical Property Measurement System (PPMS) ([Quantum Design, 2024](#)). The software
¹¹ supports major hardware interfaces and protocols (USB, RS232, GPIB, and Ethernet), enabling
¹² communication with the measurement modules associated with the PPMS. It integrates
¹³ multiple Python libraries to realize instrument control, data acquisition, and real-time data
¹⁴ visualization. Here, we present features of QuDAP, including direct control of instruments
¹⁵ without relying on proprietary software, real-time data plotting for immediate verification
¹⁶ and analysis, full automation of data acquisition and storage, and real-time notifications of
¹⁷ experiment status and errors. These capabilities enhance experimental efficiency, reliability,
¹⁸ and reproducibility.

¹⁹ Statement of need

²⁰ The exploration of quantum materials ([Awschalom et al., 2021](#); [Azam et al., 2022](#); [Kumari et al., 2021](#); [Wei et al., 2020](#)) has gained significant interest over decades, benefiting from their unique properties at the quantum level, compact size, and low energy consumption. These materials are promising candidates for applications in future quantum computers, sensors, and memory devices. Studying the intriguing properties of quantum materials demands extreme conditions such as low temperature, high magnetic field, and ultra-high vacuum environments. Therefore, many experimental approaches have been employed to characterize quantum materials, including magnetometry ([Foner, 1956](#)), spectroscopic techniques ([Rahman et al., 2021](#); [Tang et al., 2023](#)), electrical transport ([Nagaosa et al., 2010](#); [Rojo et al., 2013](#)), thermal transport ([Goyal et al., 2023](#); [Kalantari & Zhang, 2022](#)), and advanced microscopy ([Li et al., 2018](#); [Zhang et al., 2018](#)). Among them, the Physical Property Measurement System (PPMS, Quantum Design) provides the capability to achieve those goals with precise control of temperature and magnetic field under a high vacuum environment. In this process, PPMS needs to communicate with multiple peripheral instruments through hardware interfaces, including USB, RS232, GPIB, and Ethernet. To control and automate the data acquisition, software is needed to integrate the Standard Commands for Programmable Instruments (SCPI) protocol ([Keysight Technologies, 2022](#)).

³⁷ QuDAP is a Python-based data acquisition and processing software package to control and
³⁸ automate quantum material characterization experiments. It is developed based on the
³⁹ measurement modules of Quantum Design DynaCool PPMS including magnetometry, electrical
⁴⁰ transport, and ferromagnetic resonance spectroscopy. This software package provides a graphic
⁴¹ user interface to visualize and process the experimental data in real time, giving the users a

42 more efficient way to monitor the experiment. [Figure 1](#) demonstrates the connection utility of
43 this software. All the instruments are connected through the hardware interface of USB, RS232,
44 GPIB, and ethernet. The commands for each instrument are sent using PyVISA ([Grecco et](#)
45 [al., 2023](#)) and MultiPyVu ([Damon D Jackson, 2023](#)). The software provides the benefits as
46 summarized below:

- 47 1. Provide direct Python script communication and control of PPMS and instruments
48 without using the built-in software, which improves the tunability and efficiency of the
49 experiment.
- 50 2. Built-in demagnetization process before each measurement to enhance the reliability of
51 the measurement.
- 52 3. Fully automated data acquisition and saving process with real-time plotting and progress
53 visualization.
- 54 4. Save the data with specific identifiers to avoid data overwrite and record the experiment
55 configuration of each measurement. Real-time notification on the measurement status
56 and program error through push notification allows the user to promptly identify and
57 verify the experimental and parameter setup.
- 58 5. Various post-data processing features allow to process optical, magnetic, and electrical
59 data.

60 In the following sections, we introduce the Graphic User Interface and show the experiment
61 procedure for this software.

DRAFT

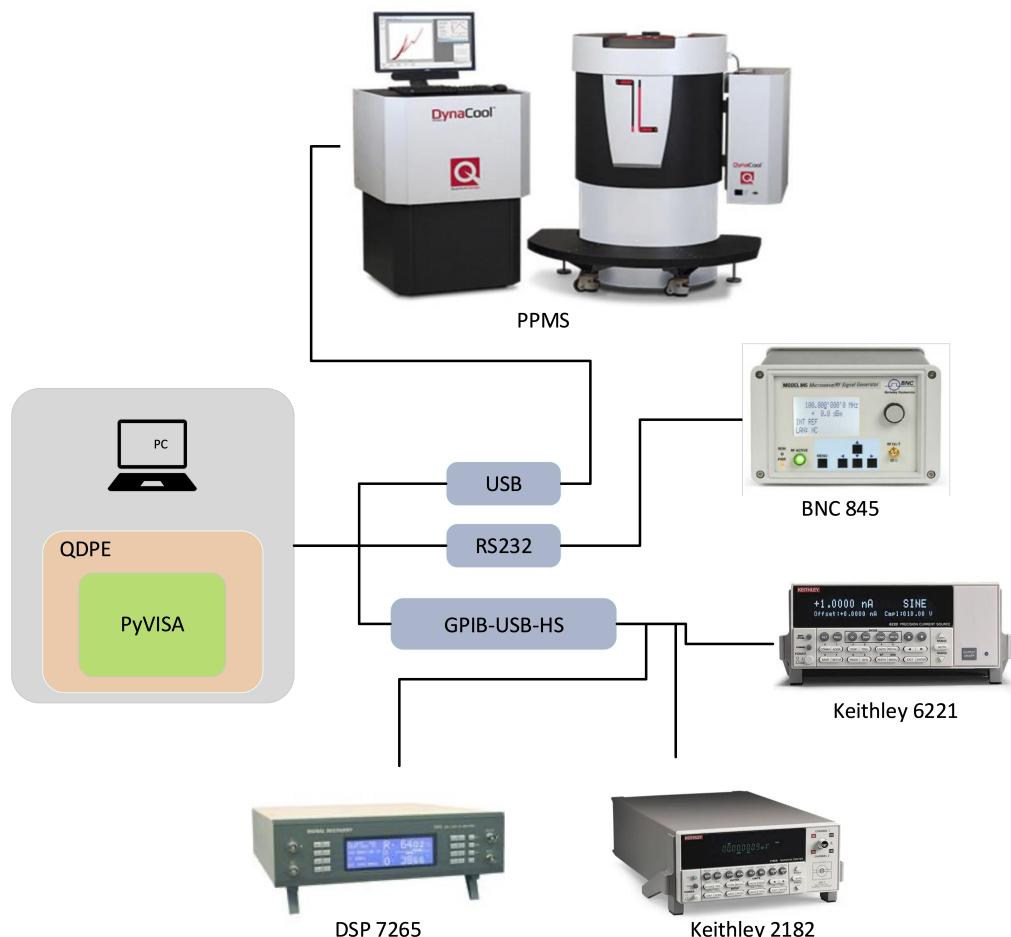


Figure 1: Block Diagram of the instrumentation of QuDAP. The QuDAP software establish the instrument communication using USB, RS232, and GPIB to control the PPMS ([Quantum Design, 2024](#)), BNC845 ([Berkeley Nucleonics, 2020](#)), Keithley 6221 ([Tektronix, 2024](#)), Keithley 2182 ([Tektronix, 2017](#)), and DSP7265 ([Signal Recovery, 2002](#)).

Experiemnt Workflow

Rotational anisotropy second harmonic generation measurements are performed using an ultrafast light source using the normal or oblique incident geometry with the fixed incident light configuration of p - or s polarization. The normal incidence geometry is when the incident light and scattered light are perpendicular to the sample surface. In contrast, the oblique incidence geometry configured both lights at an angle with respect to the normal incidence geometry. The second harmonic signal is collected by a single-photon-counting EMCCD camera. The reflected SHG intensity is recorded as a function of the azimuthal angle ϕ between the scattering plane (electric polarization) and the in-plane crystalline axis ([Gemperline et al., 2025](#)).

The static magnetization $M - H$ hysteresis loops and $M - T$ curves are collected using a Quantum Design DynaCool PPMS with the vibrating sample magnetometer option.

The transport measurements were carried out using a physical property measurement system (PPMS, Quantum Design DynaCool). The Hall resistivity is measured in a 4- or 6-terminal Hall bar device at various temperatures and magnetic fields by applying AC or DC current. The AC/DC current was supplied from a Keithley 6221 DC and AC current source, and the

⁷⁸ Hall resistivity was read by a Keithley 2182A nanovoltmeter to characterize the Hall effect of
⁷⁹ the quantum materials ([Fang et al., 2025](#)).

⁸⁰ Ferromagnetic resonance spectroscopy is measured using a coplanar waveguide (CPW) and
⁸¹ an RF diode. The microwave is injected through the CPW, and the RF diode converts the
⁸² current signal into a detectable voltage. The broadband CryoFMR option, with either field
⁸³ modulation or Amplitude modulation, was used for FMR spectroscopy acquisition, in which a
⁸⁴ locked-in amplifier records the output signal ([Tang et al., 2023](#)).

⁸⁵ Instrument Descriptions

⁸⁶ The Quantum Design PPMS Dynacool offers continuous and precise field and temperature
⁸⁷ sweeping control with the vacuum system at 10^{-4} Torr. The temperature is tunable in the
⁸⁸ range of 1.8 - 400 K and the field can sweep from -9 T to 9 T. Equipped with the internal
⁸⁹ lock-in amplifier and current source, PPMS can characterize a plethora of magnetic properties
⁹⁰ including the hysteresis loops, coercivity, and magnetic anisotropy from vibrating sample
⁹¹ magnetometer (VSM); effective magnetization, gyromagnetic ratio, and magnetic damping
⁹² from ferromagnetic resonance (FMR); Hall effect, magnetoresistance, and I-V curves from
⁹³ Electrical Transport option (ETO); heat capacity from Thermal Transport Option (TTO).

⁹⁴ As summarized in Table I, our Quantum Design PPMS Dynacool is connected to Keithley
⁹⁵ Nanovoltmeter Model 2182A, Keithley Current Source 6221 from Tektronix, Berkeley Nucleonics
⁹⁶ Corp 845 microwave and RF signal generator, and 7265 DSP Lock-in Amplifier from Signal
⁹⁷ Recovery. The instruments mentioned above can be controlled by Python. The next section
⁹⁸ will discuss the implementation of Python to establish the connection to those instruments.

TABLE I: Hardware controlled by QuDAP

Company	Instrument	Description
Quantum Design	PPMS Dynacool	It offers continuous low-temperature control and precise field and temperature sweep modes for sample measurements in a low vibration environment.
Tektronix	Keithley Nanovoltmeter Model 2182A	It provides accurate, ultra-low voltage measurements with 1 nV sensitivity.
Tektronix	Keithley Current Source 6221	It is an AC/DC current source waveform generator.
Berkeley Nucleonics Corp	Microwave and RF Signal Generator Model 845	It is a low-noise and fast-switching microwave signal generator covering from VLF to K-band, 100 kHz up to 26.5 GHz.
Signal Recovery	7265 DSP Lock-in Amplifier	It offers full-scale voltage sensitivities down to 2 nV and current sensitivities to 2 fA over an operation frequency range of 1 MHz to 250 kHz.

¹⁰⁰ Graphic User Interface

¹⁰¹ QuDAP utilizes MultiPyVu for controlling the PPMS. It is a socket-based server/client that
¹⁰² enables both readback and control of the temperature, magnetic field, and chamber operations
¹⁰³ of the sample environment. MultiPyVu also contains a wait function that allows the user
¹⁰⁴ to pause the operation until the desired stability criteria are met, while an additional class
¹⁰⁵ simplifies the writing of MultiVu-readable data files.

¹⁰⁶ The interface of the software is shown in [Figure 2](#). It contains three parts from left to right:
¹⁰⁷ main menu, options sidebar, and run window. The main menu allows users to select the
¹⁰⁸ option of the dashboard, data processing, and experiment. The detailed options are shown
¹⁰⁹ in the options sidebar once select the main option. The software starts up to the dashboard
¹¹⁰ window, which shows all the connections from VISA. The dashboard window also provides the
¹¹¹ feature of quick access to the functions and directs to the selected page. The data processing
¹¹² options feature data processing from various quantum materials characterization, including
¹¹³ magnetometry, ferromagnetic resonance, and electrical transport. The last option on the main
¹¹⁴ menu is the experiment option. Under the experiment option, there are features of individual
¹¹⁵ control for each instrument, preset experiment type, and quick test. The individual instrument

116 gives the user many options to control each feature. Besides, QuDAP allows users to customize
117 the experiment setup to link and control instruments. The preset measurements can be found
118 under the Measurement tab in the option sidebar. This feature provides the users with the
119 preset script for both ETO and FMR measurements. Once selecting the preset option, the user
120 will connect instruments and set up the parameters. A log panel will pop up when the user
121 presses the start button, and the experimental log will be recorded as a txt file. To facilitate
122 the data management, an example of the data file naming convention will be provided. After
123 the measurement starts, in the backend, the software will check all the parameters to ensure a
124 valid entry. The Quick Test option allows users to take measurements without constraining
125 the preset script. Users can select the instruments they need for specific experiments. After
126 the measurements are finished, users can find metadata as well as the recorded experimental
127 under the preselected folder and process the data under the data processing option.

128 This software is available in the format of a Python script file. The experimental features are
129 supported only on the Windows operating system due to driver dependencies, while the data
130 processing features are cross-platform and can be run on Windows, macOS, and Linux. It will
131 also pack into executable software for those who do not have experience in Python programs.

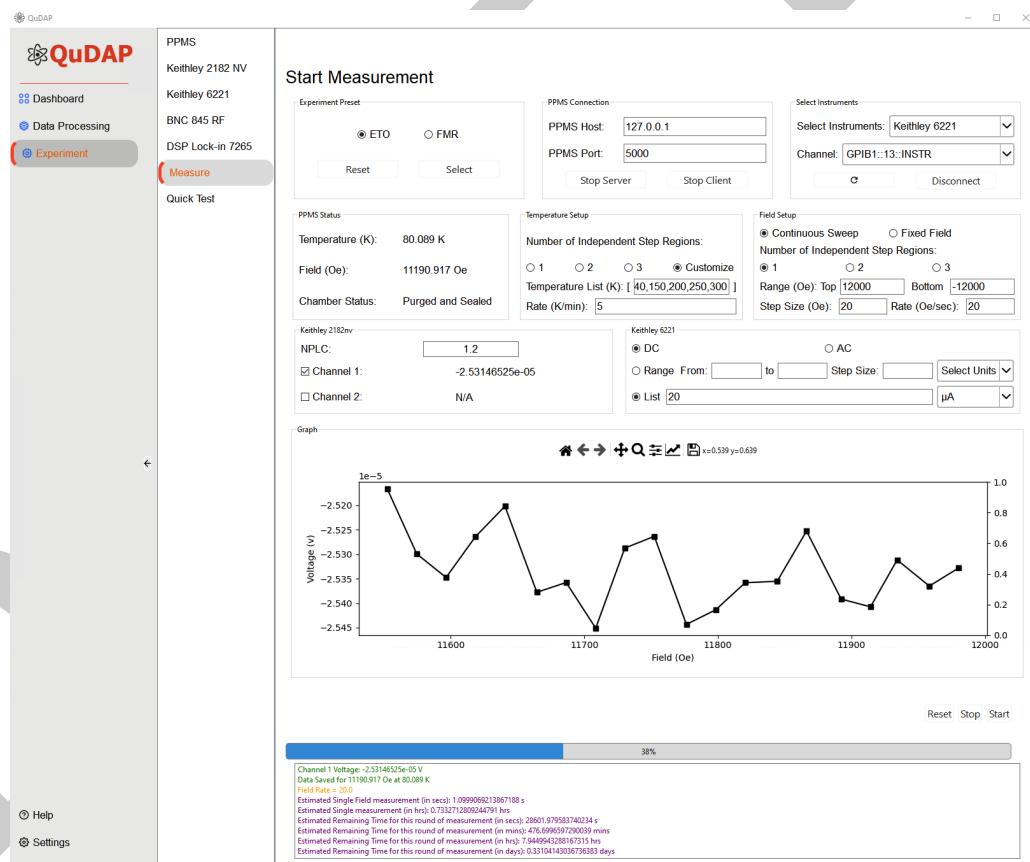


Figure 2: GUI Interface of the QuDAP. The interface shows the ETO measurement setup and real-time data visualization.

Acknowledgements

132 S. W was funded by Collaborative Approaches among Scientists and Engineers REU National
133 Science Foundation EEC Division Grant 2349639.

135 References

- 136 Awschalom, D. D., Du, C. R., He, R., Heremans, F. J., Hoffmann, A., Hou, J., Kurebayashi,
137 H., Li, Y., Liu, L., Novosad, V., & others. (2021). Quantum engineering with hybrid
138 magnonic systems and materials. *IEEE Transactions on Quantum Engineering*, 2, 1–36.
- 139 Azam, N., Boebinger, M. G., Jaiswal, S., Unocic, R. R., Fathi-Hafshejani, P., & Mahjouri-
140 Samani, M. (2022). Laser-assisted synthesis of monolayer 2D MoSe₂ crystals with tunable
141 vacancy concentrations: Implications for gas and biosensing. *ACS Applied Nano Materials*,
142 5(7), 9129–9139.
- 143 Berkeley Nucleonics. (2020). *Model 845 datasheet v2.75*. https://www.berkeleynucleonics.com/sites/default/files/products/resources/845_datasheet_v275.1.pdf
- 144 Damon D Jackson, Q. D. (2023). *MultiPyVu 2.1.4*. <https://pypi.org/project/MultiPyVu/>
- 145 Fang, M., Tang, C., Chen, S., Tang, Z., Choi, M.-Y., Jang, J. H., Chung, H.-S., Nair, M. N.,
146 Jin, W., & Yang, E.-H. (2025). Proximity-induced antisymmetric humps in hall resistivity
147 in fe-doped monolayer WSe₂. *Applied Physics Letters*, 126(10).
- 148 Foner, S. (1956). Vibrating sample magnetometer. *Review of Scientific Instruments*, 27(7),
149 548–548.
- 150 Gemperline, P. T., Thind, A. S., Tang, C., Sterbinsky, G. E., Kiefer, B., Jin, W., Klie, R. F.,
151 & Comes, R. B. (2025). Strain effects in SrHfO₃ films grown by hybrid molecular beam
152 epitaxy. *ACS Applied Electronic Materials*, 7(3), 983–996.
- 153 Goyal, H., Peek, S. E., Sellers, J. A., & Hamilton, M. C. (2023). Methodology to characterize
154 thermal properties of thin film superconductors using a DynaCool physical property
155 measurement system. *IEEE Transactions on Applied Superconductivity*, 33(5), 1–5.
- 156 Grecco, H. E., Dartailh, M. C., Thalhammer-Thurner, G., Bronger, T., & Bauer, F. (2023).
157 PyVISA: The python instrumentation package. *Journal of Open Source Software*, 8(84),
158 5304. <https://doi.org/10.21105/joss.05304>
- 159 Kalantari, M. H., & Zhang, X. (2022). Thermal transport in 2D materials. *Nanomaterials*,
160 13(1), 117.
- 161 Keysight Technologies. (2022). *Instrument automation with python*.
- 162 Kumari, S., Pradhan, D. K., Pradhan, N. R., & Rack, P. D. (2021). Recent developments on
163 2D magnetic materials: Challenges and opportunities. *Emergent Materials*, 4(4), 827–846.
- 164 Li, X., Sun, M., Shan, C., Chen, Q., & Wei, X. (2018). Mechanical properties of 2D materials
165 studied by in situ microscopy techniques. *Advanced Materials Interfaces*, 5(5), 1701246.
- 166 Nagaosa, N., Sinova, J., Onoda, S., MacDonald, A. H., & Ong, N. P. (2010). Anomalous hall
167 effect. *Reviews of Modern Physics*, 82(2), 1539–1592.
- 168 Quantum Design. (2024). *Quantum design PPMS DynaCool*. <https://www.qdusa.com/products/dynacool.html>
- 169 Rahman, S., Torres, J. F., Khan, A. R., & Lu, Y. (2021). Recent developments in van der waals
170 antiferromagnetic 2D materials: Synthesis, characterization, and device implementation.
171 *ACS Nano*, 15(11), 17175–17213.
- 172 Rojo, M. M., Calero, O. C., Lopeandia, A., Rodriguez-Viejo, J., & Martin-Gonzalez, M. (2013).
173 Review on measurement techniques of transport properties of nanowires. *Nanoscale*, 5(23),
174 11526–11544.
- 175 Signal Recovery. (2002). *Model 7265 DSP lock-in amplifier*. <https://www.atecorp.com/atecorp/media/pdfs/data-sheets/7265lockinampv7web.pdf?ext=.pdf>
- 176 Tang, C., Alahmed, L., Mahdi, M., Xiong, Y., Inman, J., McLaughlin, N. J., Zollitsch, C.,
177 7787. <https://doi.org/10.xxxxxx/draft>.

- 180 Kim, T. H., Du, C. R., Kurebayashi, H., & others. (2023). Spin dynamics in van der waals
181 magnetic systems. *Physics Reports*, 1032, 1–36.
- 182 Tektronix. (2017). *Model 2182 and 2182A nanovoltmeter user's manual*. https://download.tek.com/manual/2182A-900-01_May_2017.pdf
- 183 Tektronix. (2024). *Keithley 6220-6221*. <https://download.tek.com/datasheet/6220-6221.pdf>
- 185 Wei, S., Liao, X., Wang, C., Li, J., Zhang, H., Zeng, Y.-J., Linghu, J., Jin, H., & Wei, Y. (2020).
186 Emerging intrinsic magnetism in two-dimensional materials: Theory and applications. *2D
187 Materials*, 8(1), 012005.
- 188 Zhang, H., Huang, J., Wang, Y., Liu, R., Huai, X., Jiang, J., & Anfuso, C. (2018). Atomic
189 force microscopy for two-dimensional materials: A tutorial review. *Optics Communications*,
190 406, 3–17.

DRAFT