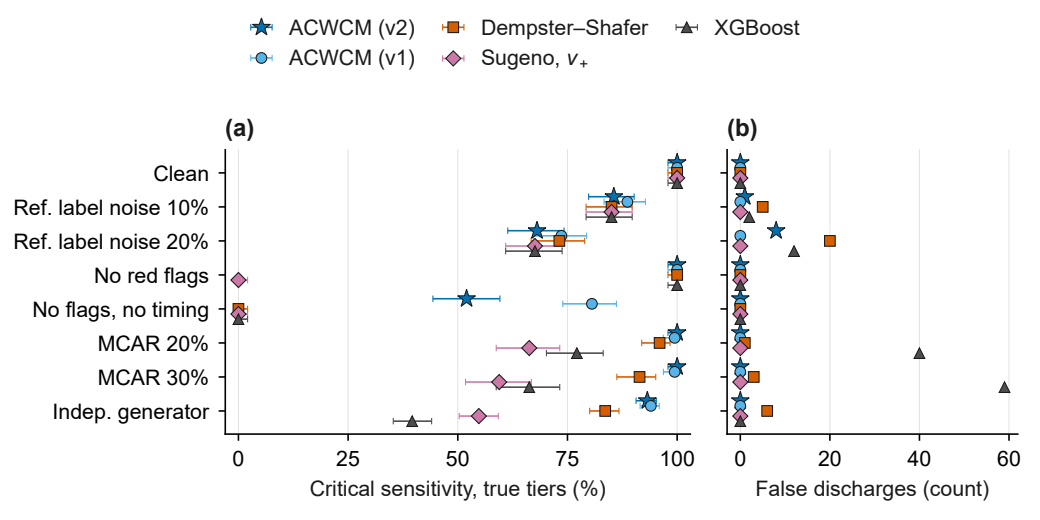

ACWCM (v2)
ACWCM (v1)
Dempster–Shafer
Sugeno, v_+
XGBoost
(a)
(b)
Clean
Ref. label noise 10%
Ref. label noise 20%
No red flags
No flags, no timing
MCAR 20%
MCAR 30%
Indep. generator
0
25
50
75
100
Critical sensitivity, true tiers (%)
0
20
40
60
False discharges (count)