



开关电源





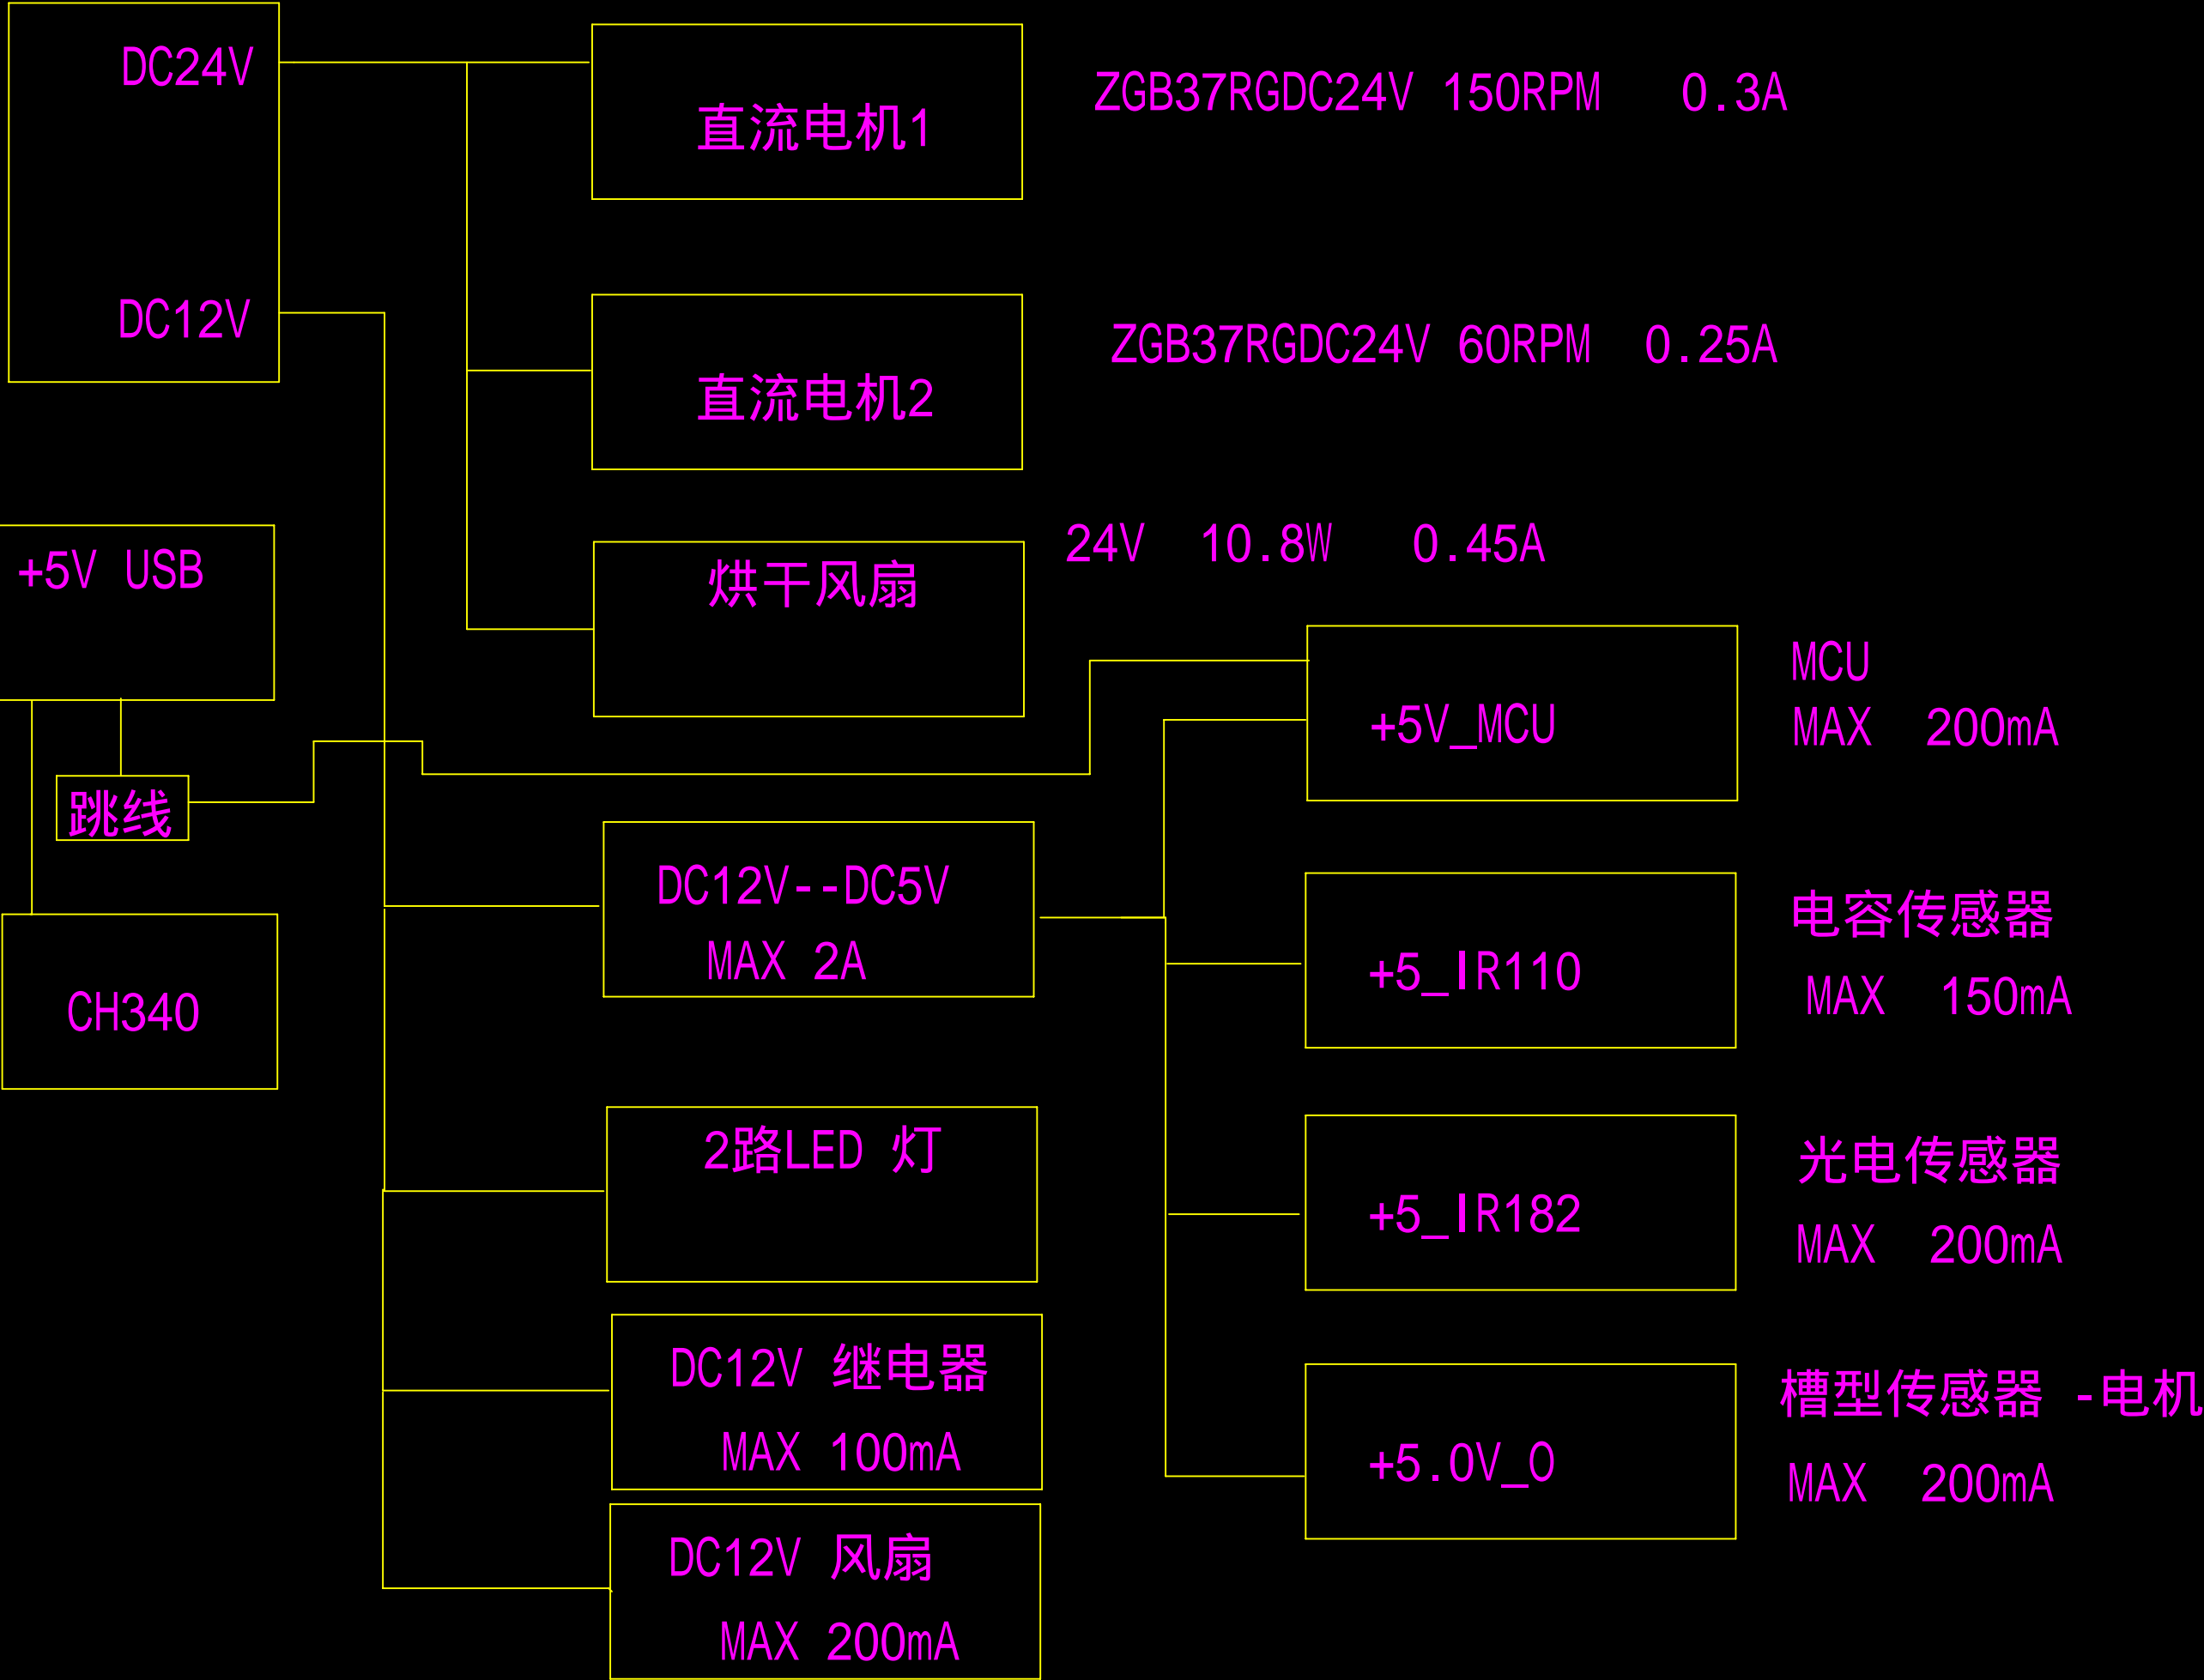

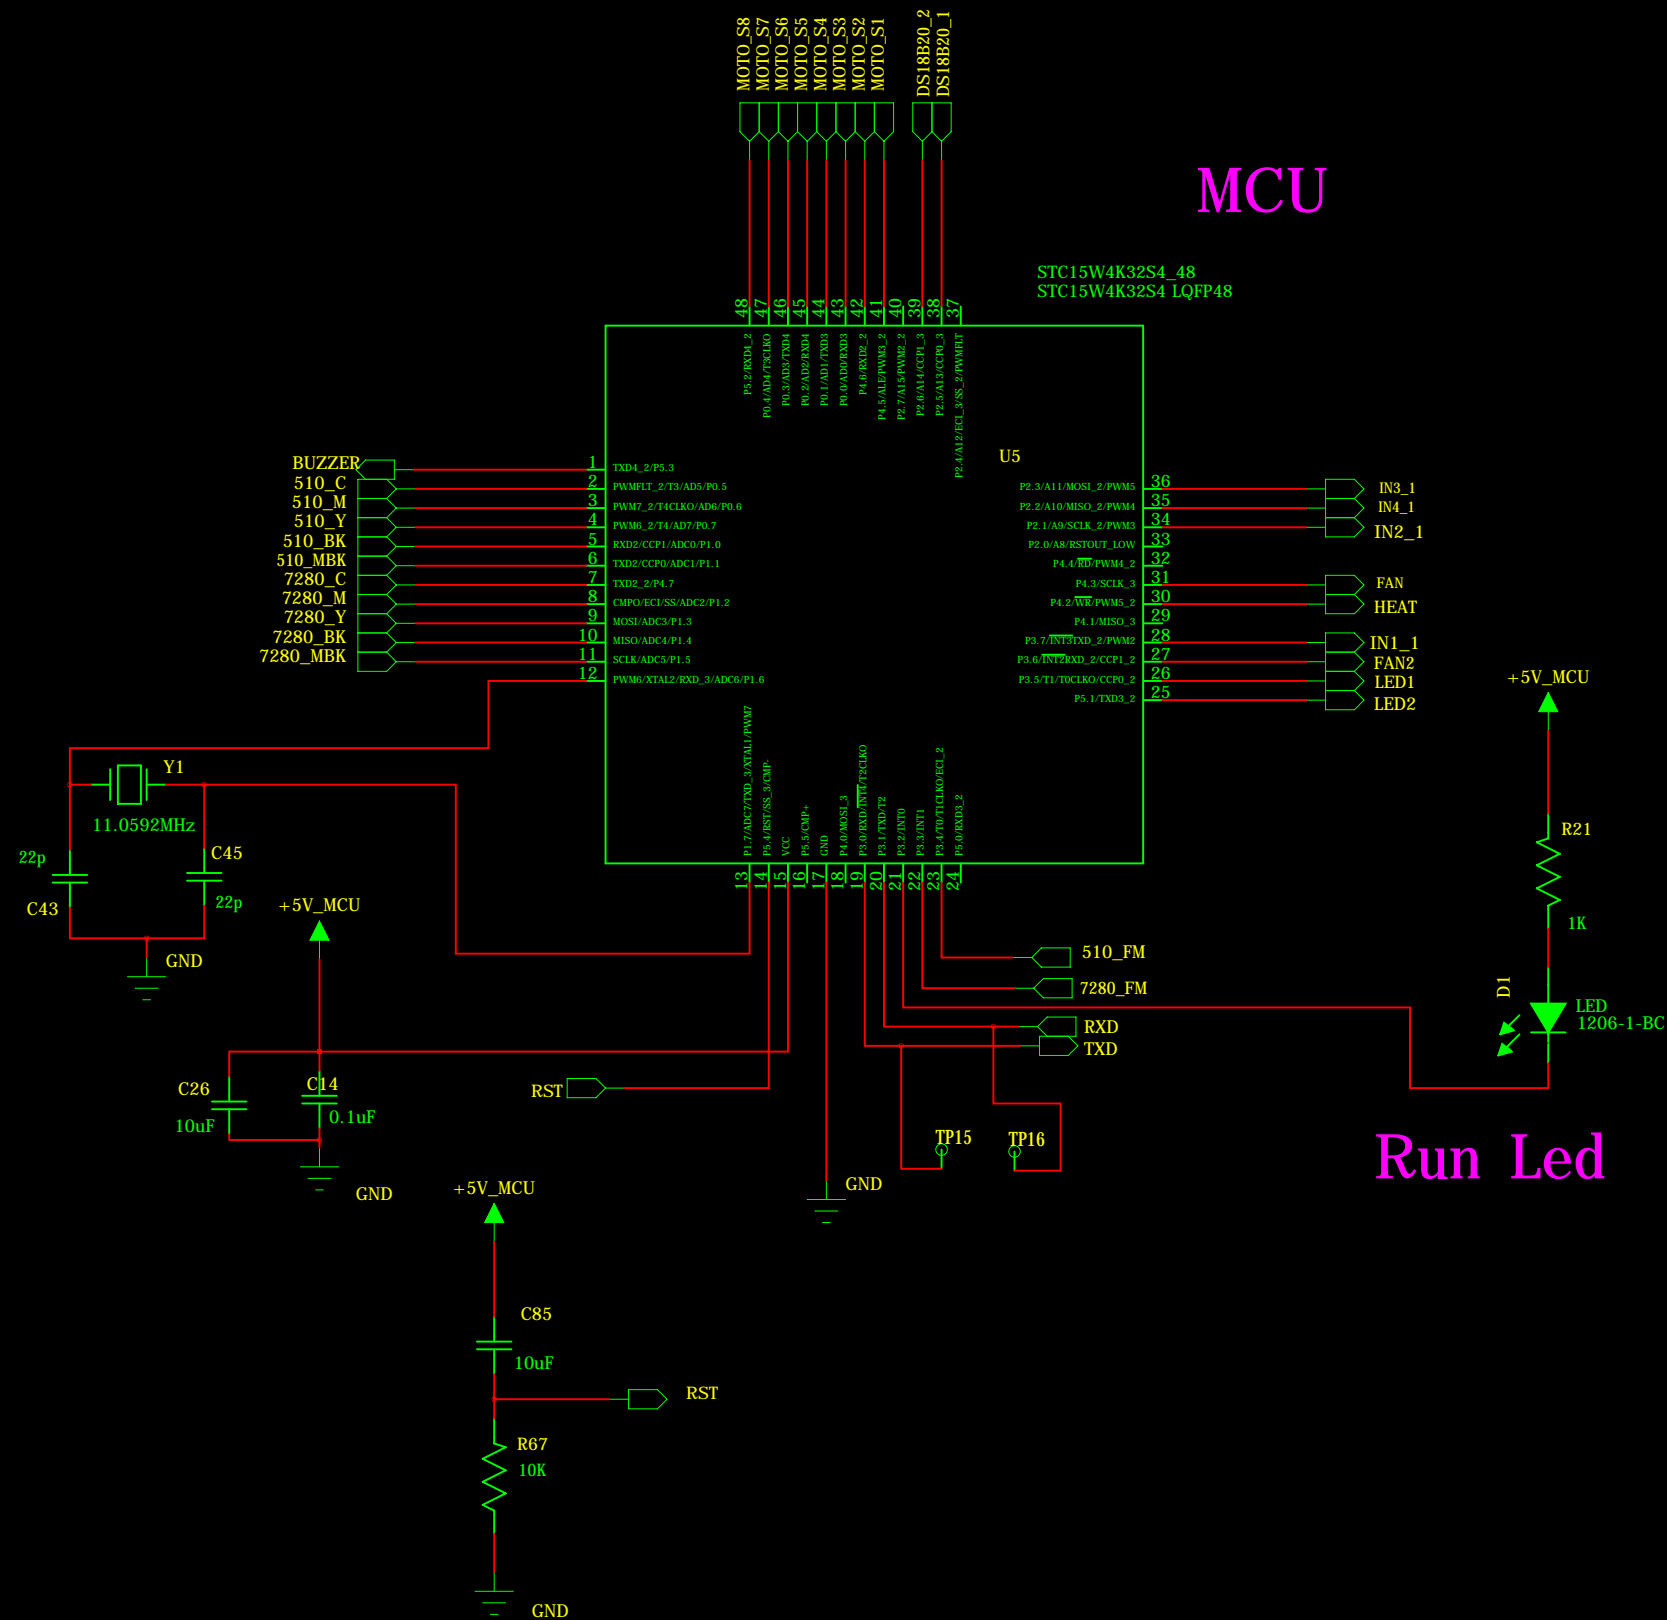

DRAWN: <b>ZB</b>	DATED: <b>2016.9.7</b>	COMPANY: <b>Shenzhen Ju Ding Medical Equipment Co., Ltd.</b>		
CHECKED: <Checked By>	DATED: <Checked Date>	TITLE: <b>SDP-2A</b>		
RELEASED: <Released By>	DATED: <Release Date>	CODE: <Code>	SIZE: <b>A3</b>	DRAWING NO: <b>CL20160322</b>
SHEET: 4 OF 9				REV: <b>V1.0</b>

DC\_Motor ZGB37RG DC24V MAX1.1A

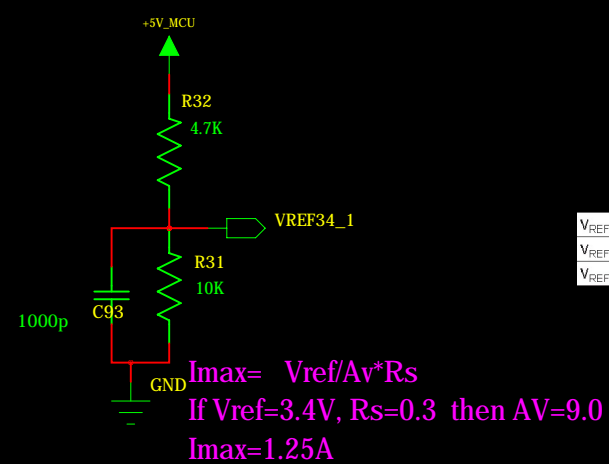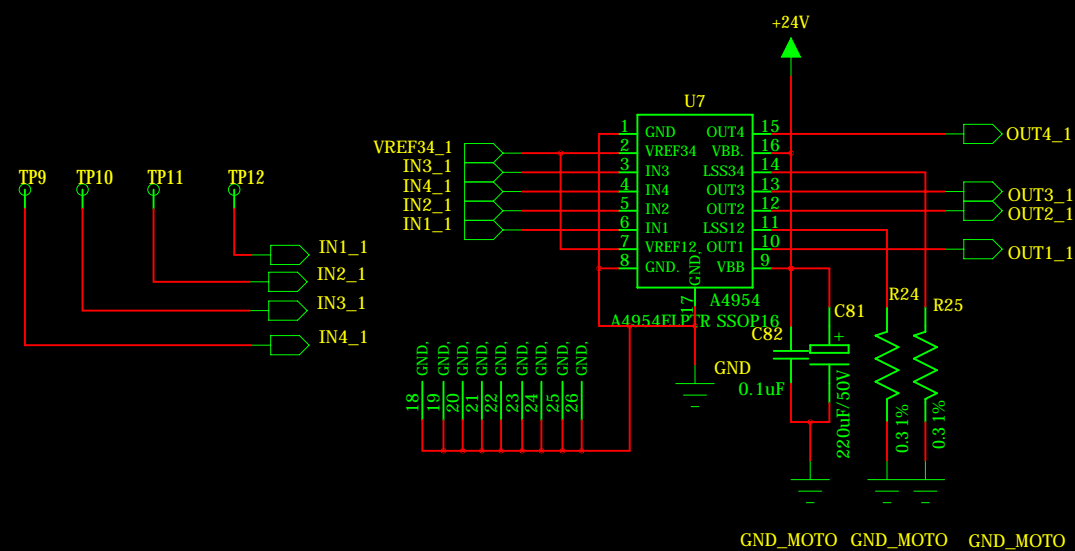


$V_{REF}/I_{SS}, V_{REF} = 5\text{ V}$	9.5	–	10.5	V/V
$V_{REF}/I_{SS}, V_{REF} = 2.5\text{ V}$	9.0	–	10.0	V/V
$V_{REF}/I_{SS}, V_{REF} = 1\text{ V}$	8.0	–	10.0	V/V


DRAWN:  ZB	DATED:  2016.9.7	COMPANY: Shenzhen Ju Ding Medical Equipment Co., Ltd.			
		TITLE: SDP-2A			
CHECKED:  <Checked By>	DATED:  <Checked Date>	CODE:  <Code>	SIZE: A3	DRAWING NO:	REV:
RELEASED:  <Released By>	DATED:  <Release Date>	SHEET: 5 OF 9			V1.0

Sensor\_5V Part

7280 FS-IR110-CA 3P 2.0 mm

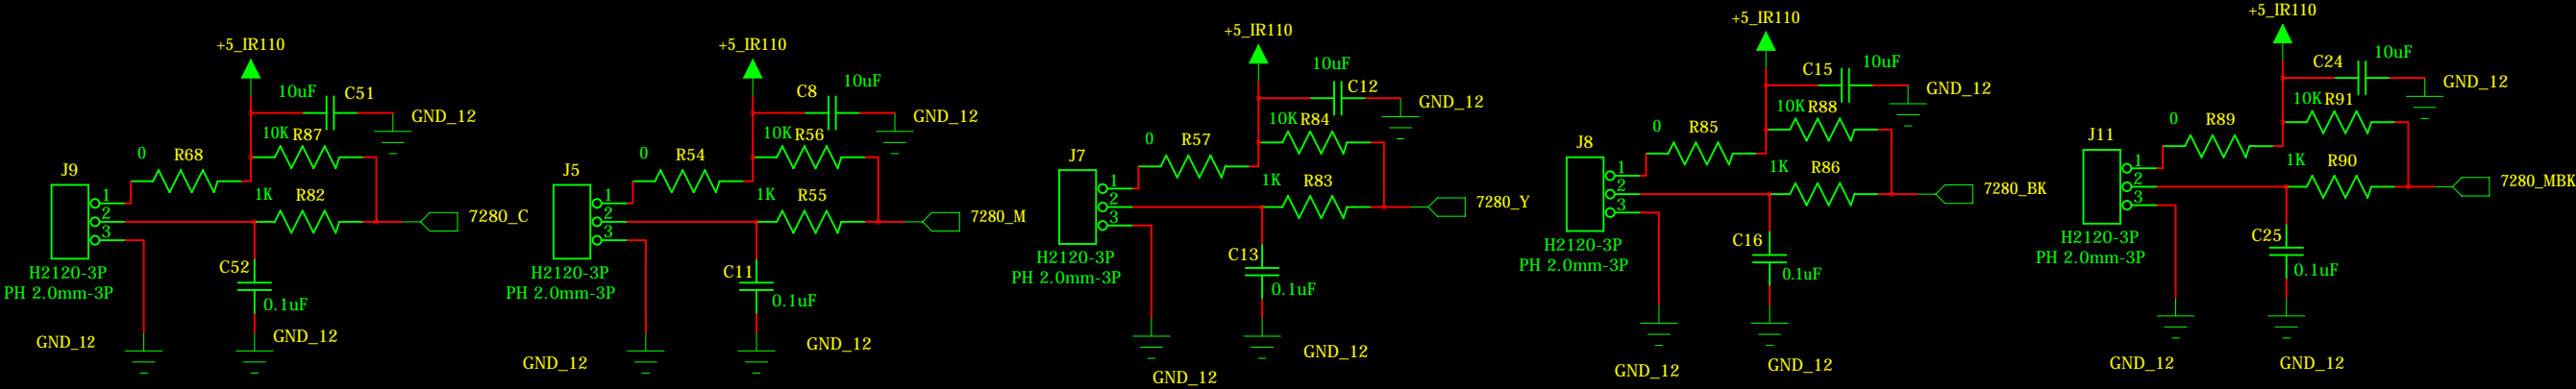









510 FS-IR82 3P 2.54 mm

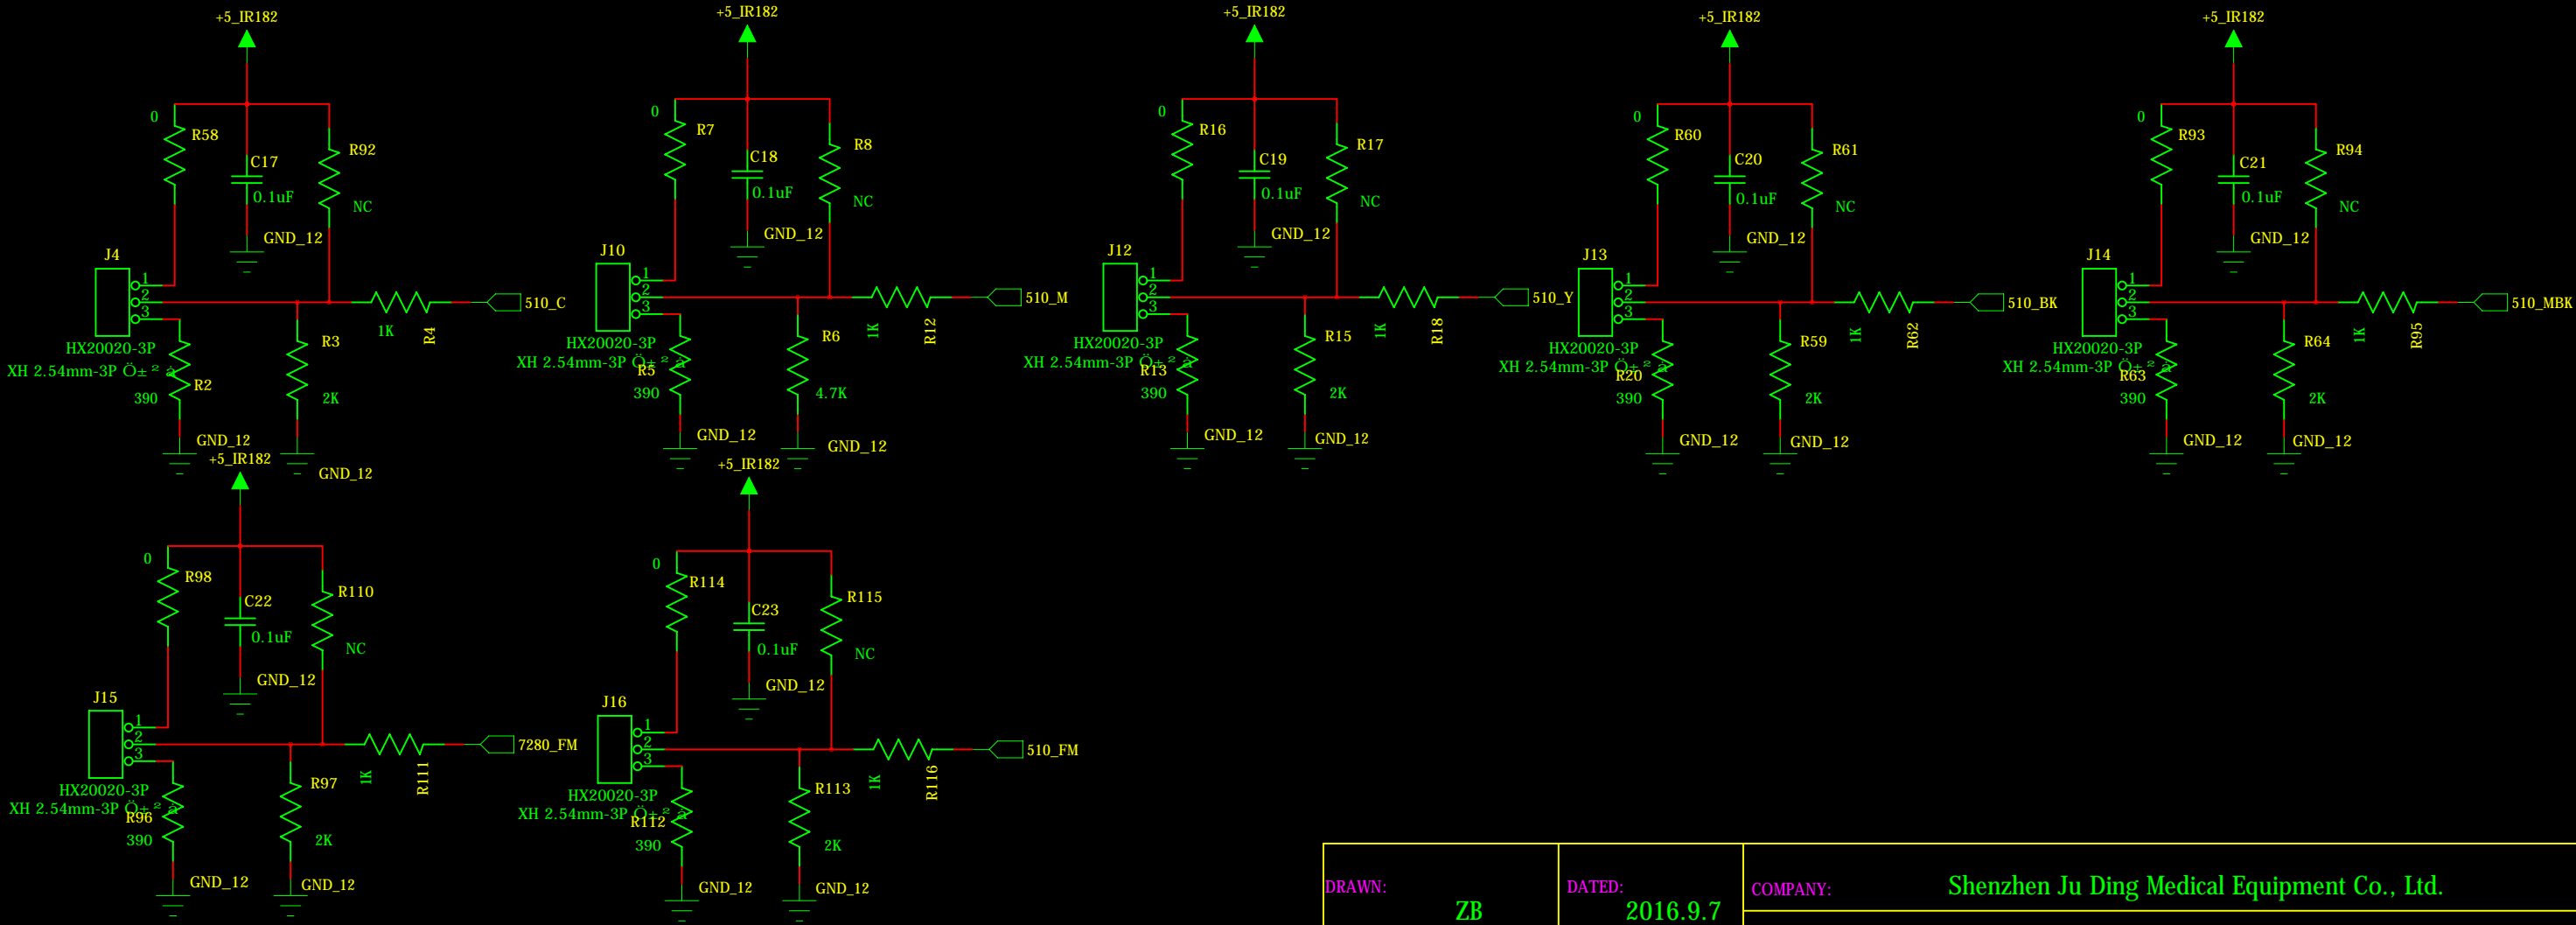

7280

510


DRAWN: ZB	DATED: 2016.9.7	COMPANY: Shenzhen Ju Ding Medical Equipment Co., Ltd.		
CHECKED: <Checked By>	DATED: <Checked Date>	TITLE: SDP-2A		
RELEASED: <Released By>	DATED: <Release Date>	CODE: <Code>	SIZE: A3	DRAWING NO: CL20160322
SHEET: 6 OF 9				REV: V1.0

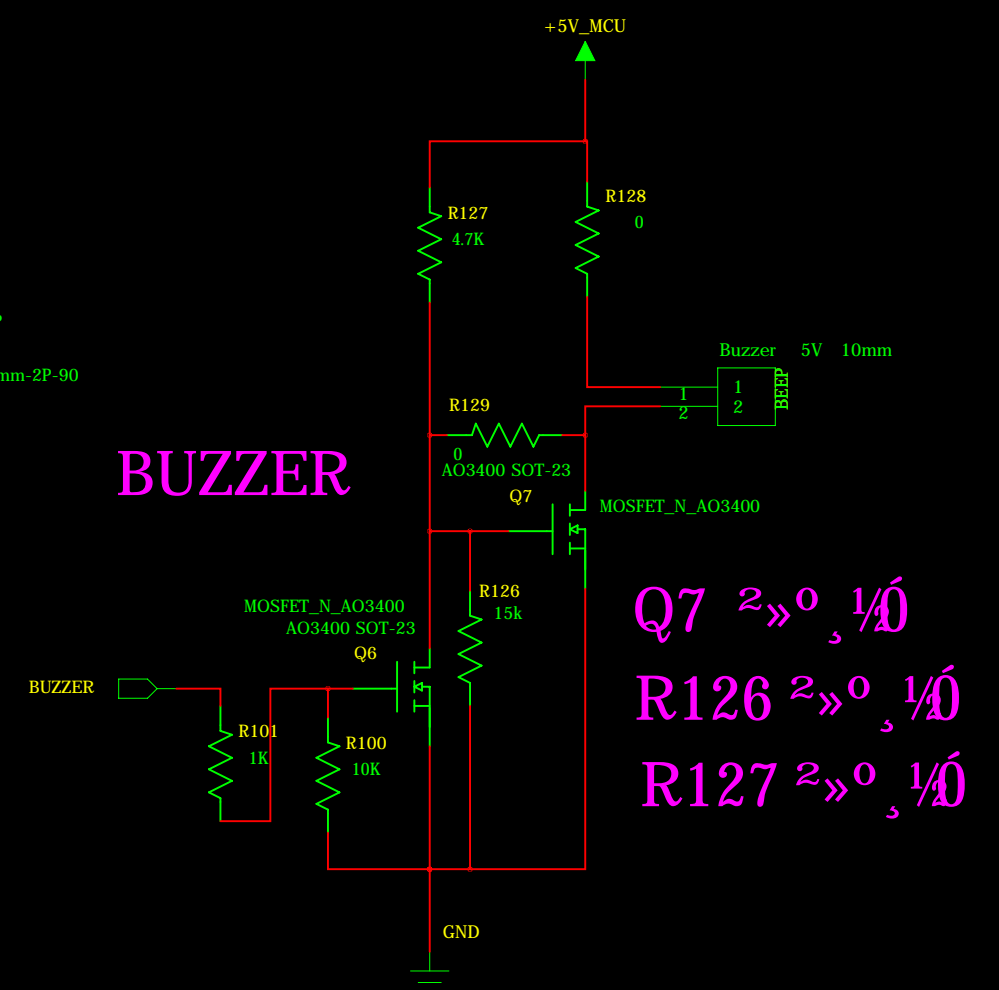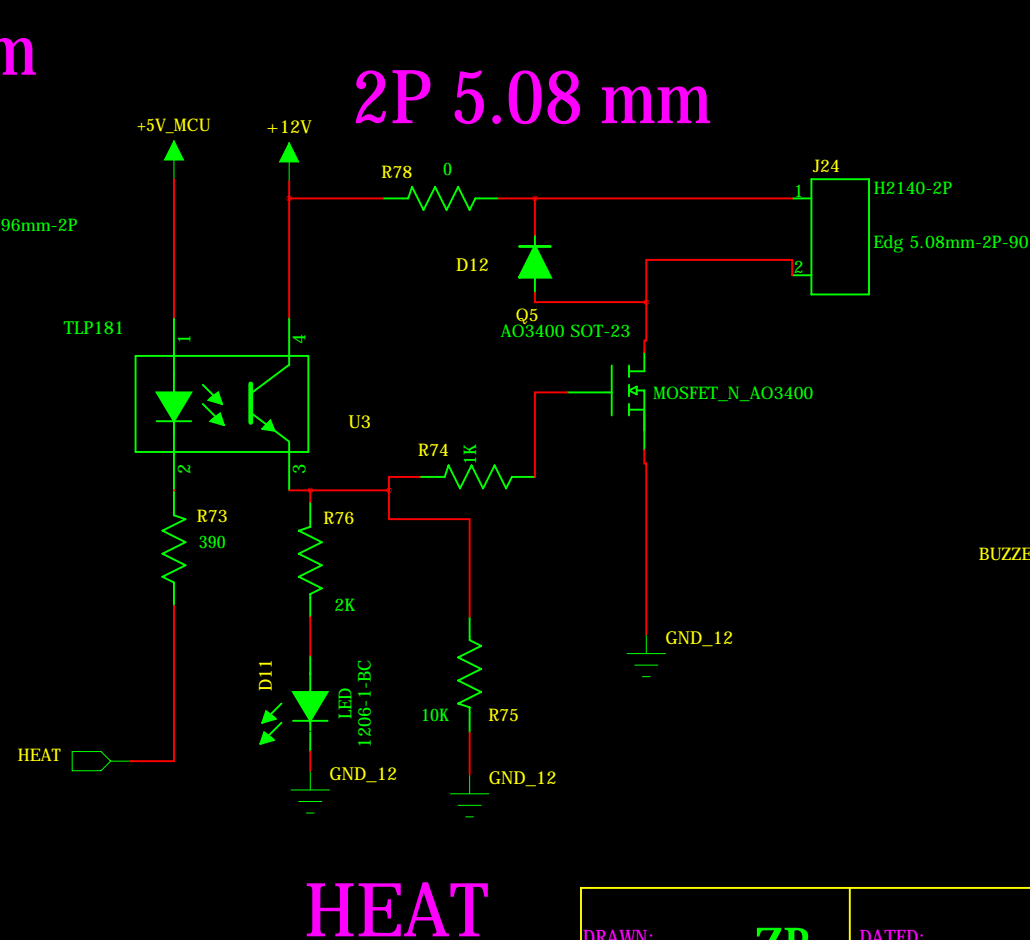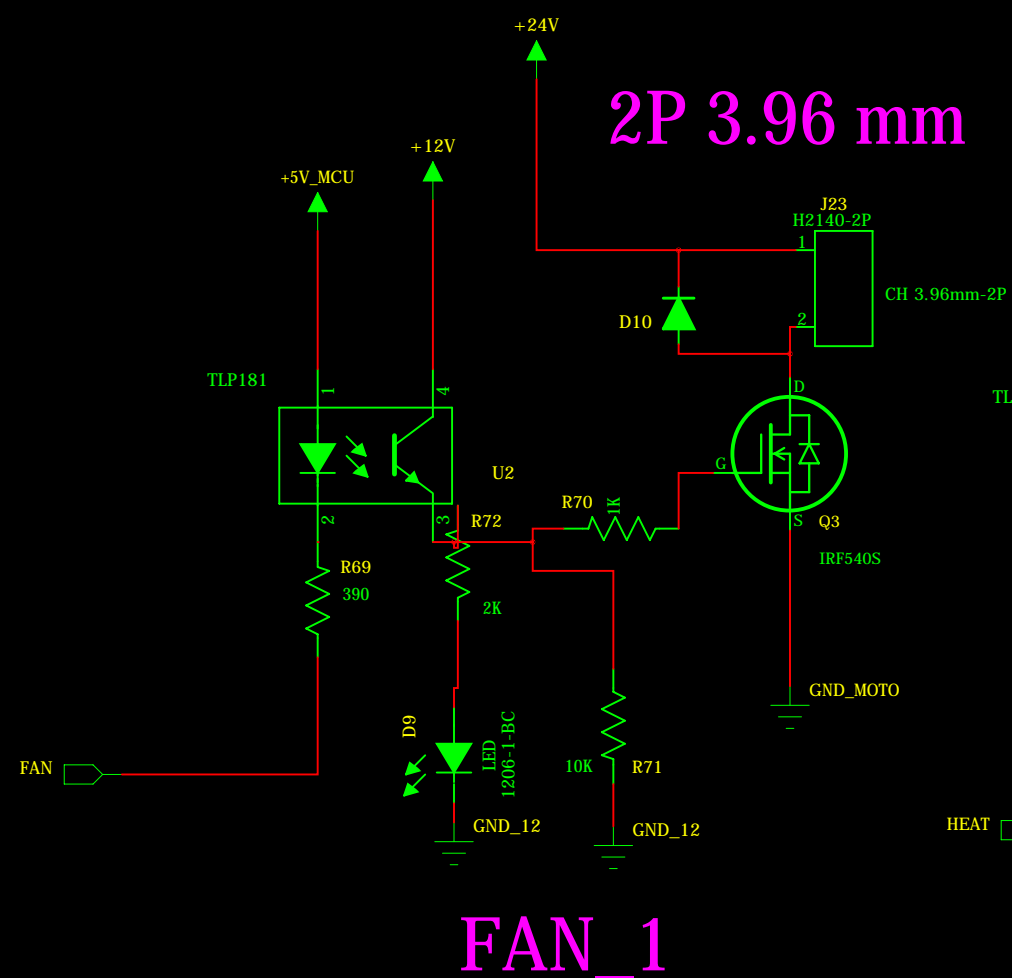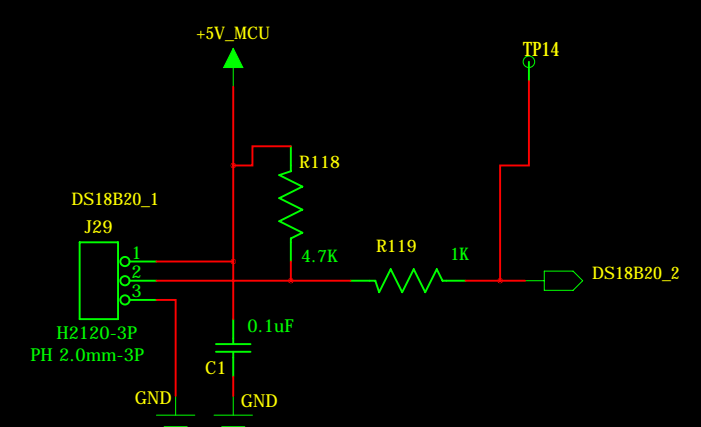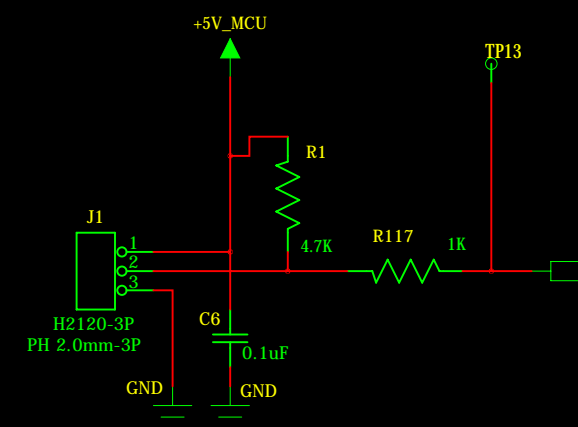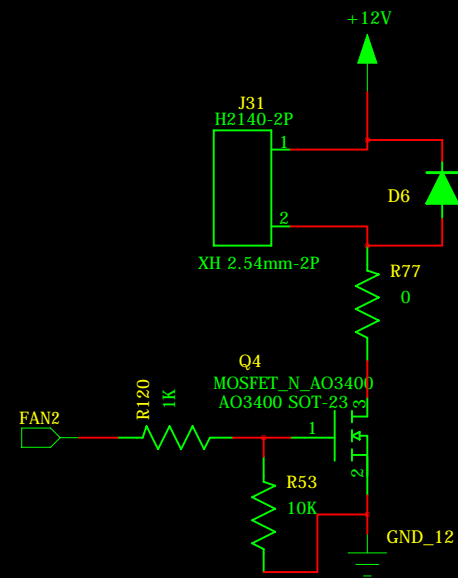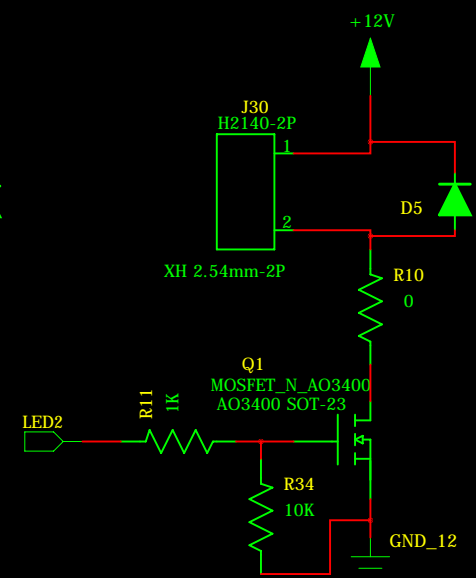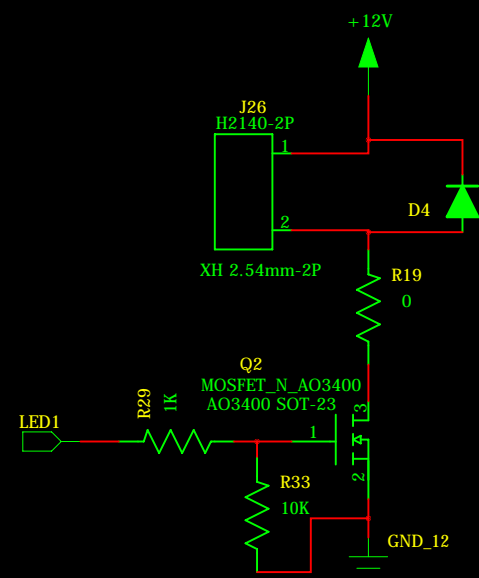

DRAWN:  <b>ZB</b>	DATED:  <b>2016.9.7</b>	COMPANY: <b>Shenzhen Ju Ding Medical Equipment Co., Ltd.</b>			
		TITLE: <b>SDP-2A</b>			
CHECKED:  <Checked By>	DATED:  <Checked Date>	CODE:  <Code>	SIZE:  <b>A3</b>	DRAWING NO:  <b>CL20160322</b>	REV:  
RELEASED:  <Released By>	DATED:  <Release Date>	SHEET: 7 OF 9			<b>V1.0</b>

USB to Serial









5P 2.0 mm

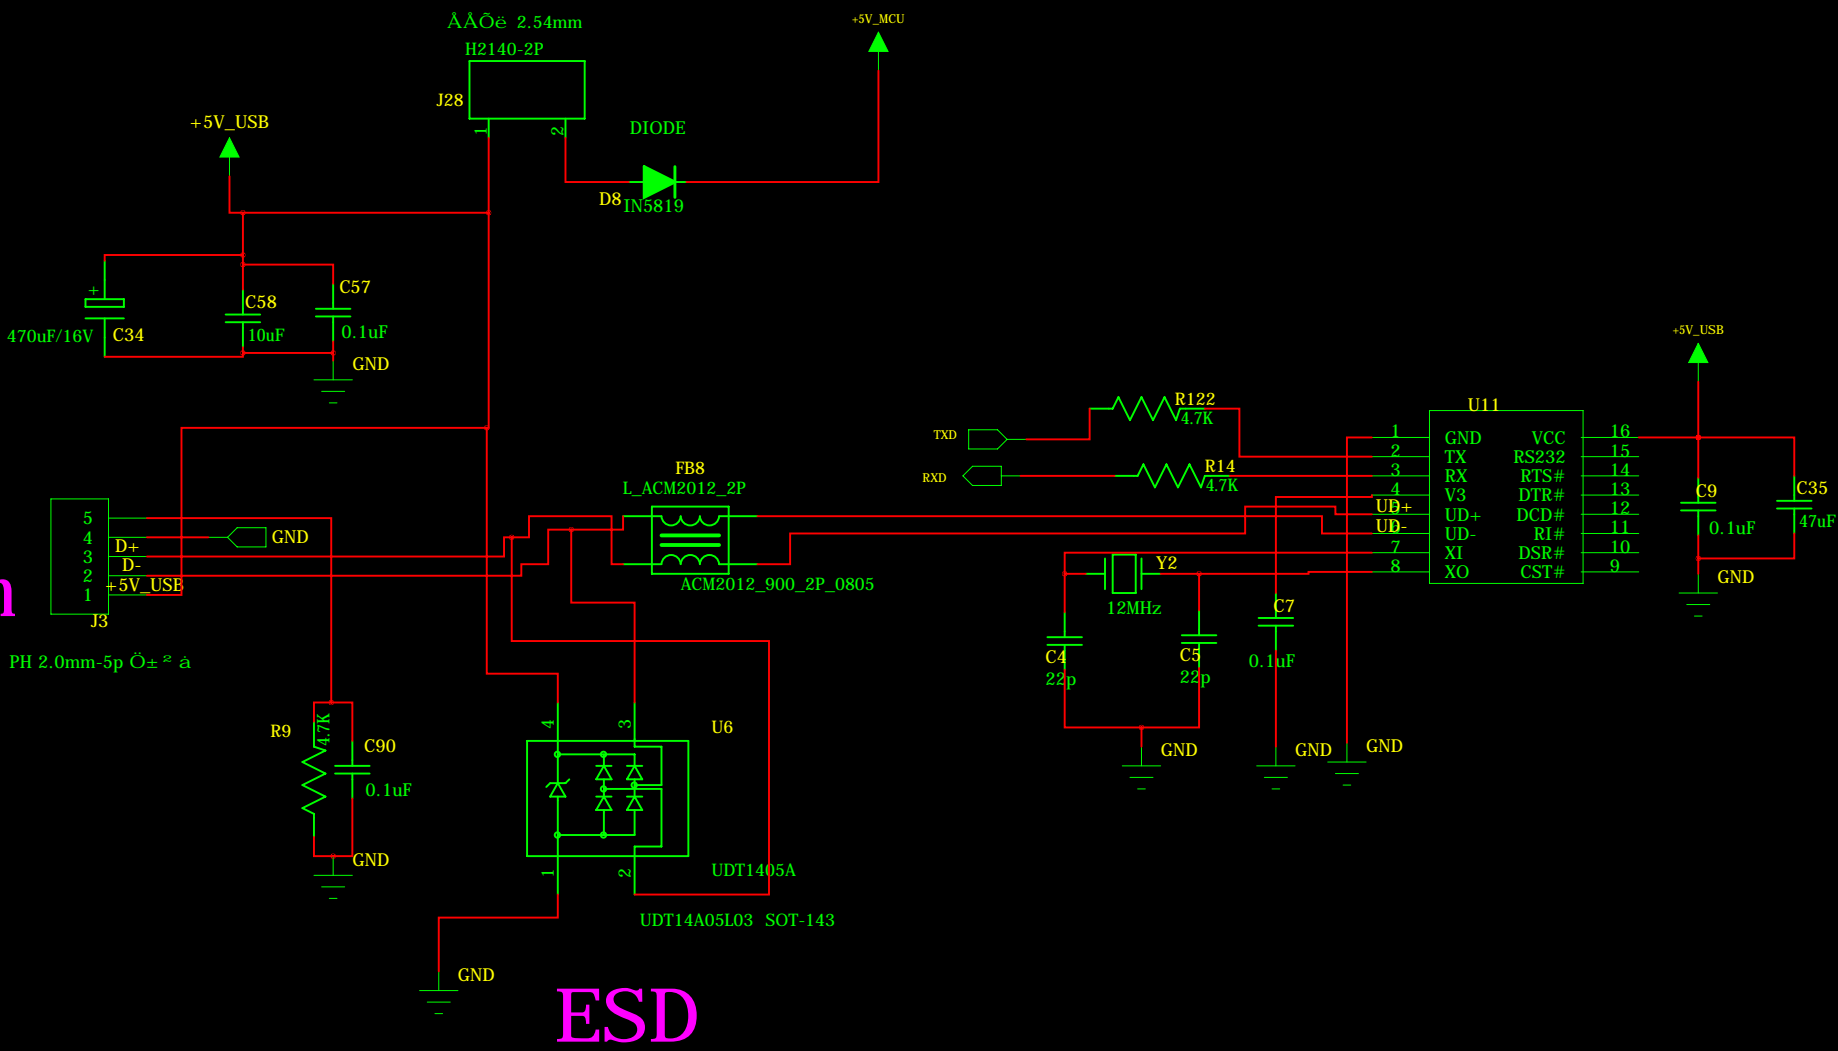

DRAWN: ZB	DATED: 2016.9.7	COMPANY: Shenzhen Ju Ding Medical Equipment Co., Ltd.		
CHECKED: <Checked By>	DATED: <Checked Date>	TITLE: SDP-2A		
RELEASED: <Released By>	DATED: <Release Date>	CODE: <Code>	SIZE: A3	DRAWING NO: CL20160322
SHEET: 8 OF 9				REV: V1.0



IF 17 mA    3P 2.0 mm  
7280 È±0½

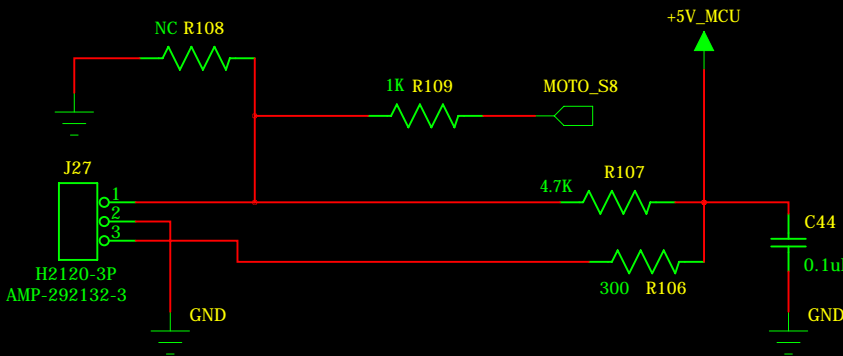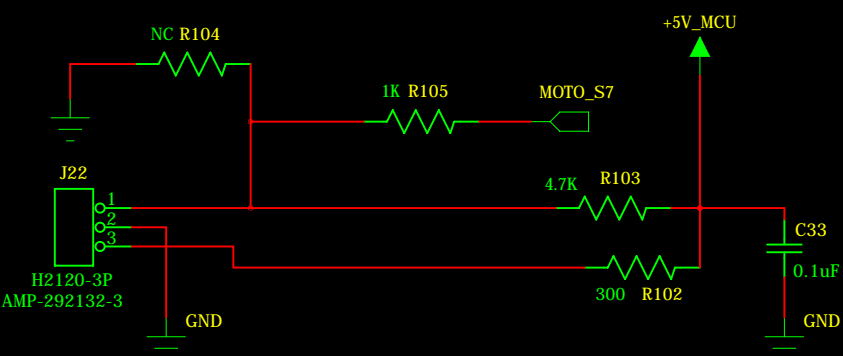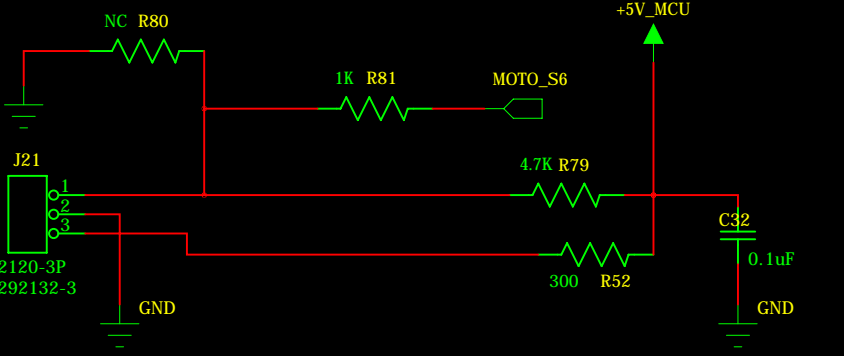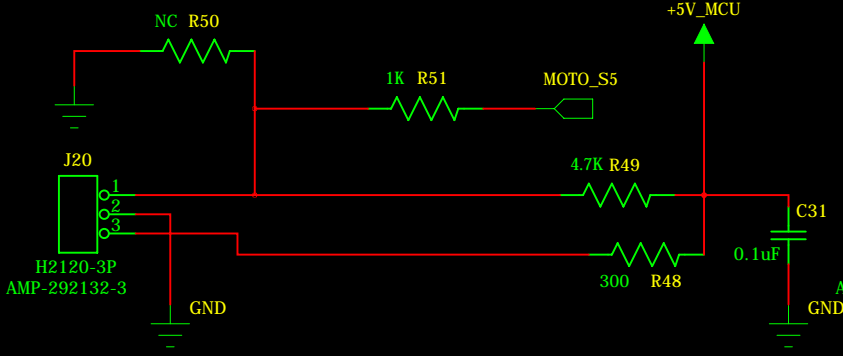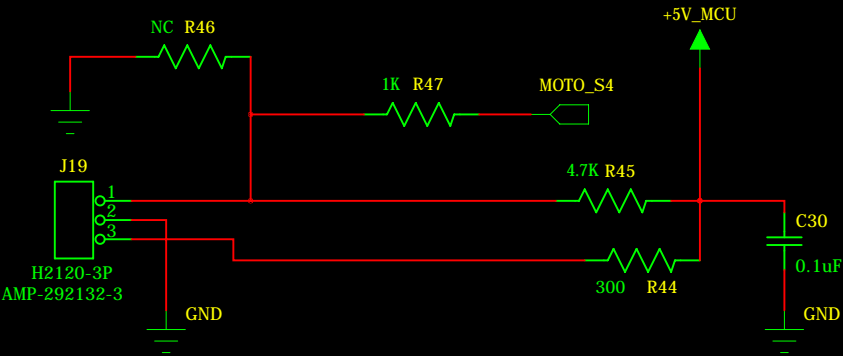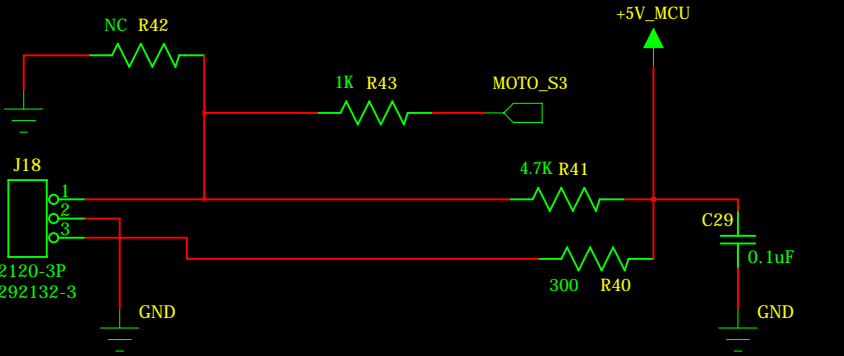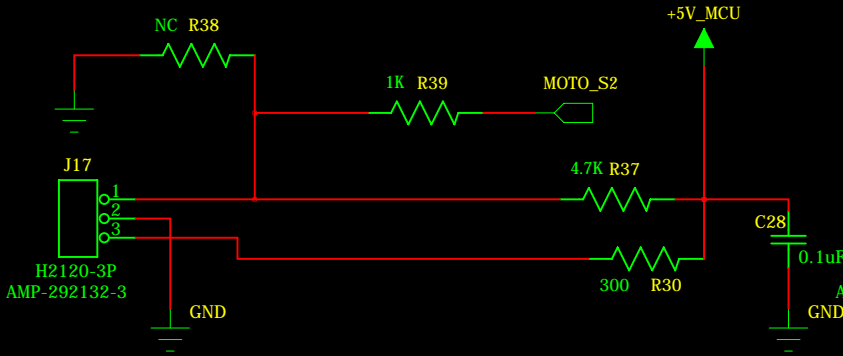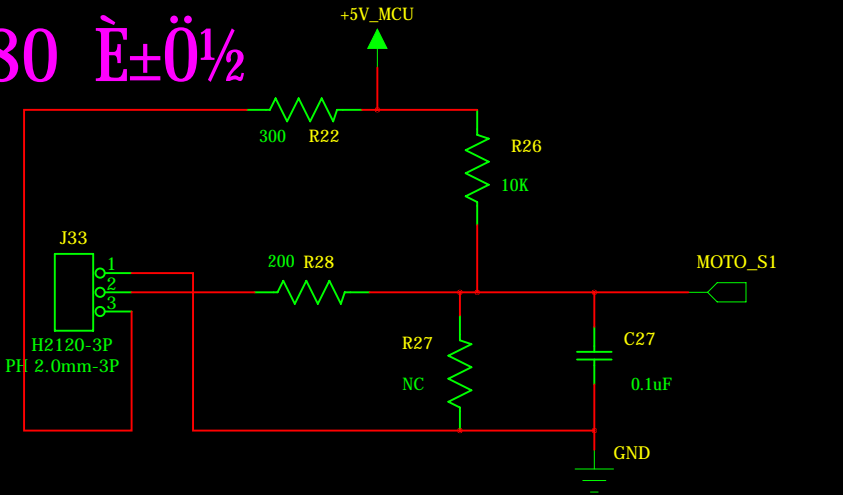

DRAWN: <b>ZB</b>	DATED: <b>2016.9.7</b>	COMPANY: <b>Shenzhen Ju Ding Medical Equipment Co., Ltd.</b>		
CHECKED: <Checked By>	DATED: <Checked Date>	TITLE: <b>SDP-2A</b>		
RELEASED: <Released By>	DATED: <Release Date>	CODE: <Code>	SIZE: <b>A3</b>	DRAWING NO: <b>CL20160322</b>
SHEET: 9 OF 9				REV: <b>V1.0</b>