



## OneAttension experiment report

Generated with OneAttension Version 3.2 (r5971) Mon May 15 15:12:44 BST 2023

Experiment info

Name	csg524 Sample 1 Measurement 2
Type	Contact angle
Date	15-May-2023 15:11

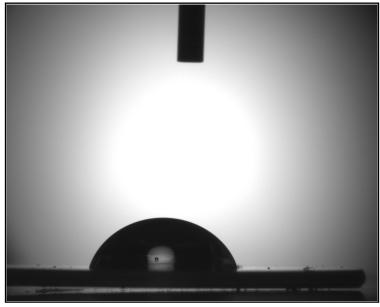

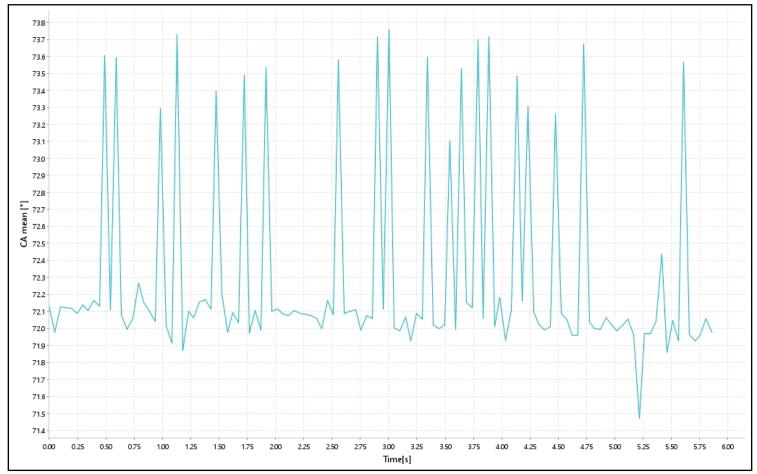



## Detailed results

Time [s]	CA left [°]	CA right [°]	CA mean [°]	Volume [µl]	Baseline [mm]
0.00	72.51	71.76	72.13	0.22	1.13
0.00	72.33	71.76	72.13	0.22	1.13
0.10	72.35	71.90	72.13	0.22	1.13
0.15	72.43	71.82	72.12	0.22	1.13
0.20	72.40	71.84	72.12	0.22	1.13
0.25	72.46	71.72	72.09	0.22	1.13
0.30	72.49	71.80	72.14	0.22	1.13
0.34	72.46	71.74	72.10	0.22	1.13
0.39	72.45	71.88	72.17	0.22	1.13
0.44	72.40 74.19	71.85	72.13	0.22	1.13
0.49	74.19	73.02 71.90	73.61 72.11	0.23 0.22	1.13 1.13
0.59	74.19	72.99	73.59	0.23	1.13
0.64	72.31	71.84	72.08	0.22	1.13
0.69	72.27	71.72	72.00	0.22	1.13
0.74	72.32	71.79	72.06	0.22	1.13
0.79	72.51	72.02	72.27	0.22	1.13
0.84	72.52	71.78	72.15	0.22	1.13
0.89	72.44	71.76	72.10	0.22	1.13
0.93	72.32 73.87	71.76 72.72	72.04 73.29	0.22 0.22	1.13 1.13
1.03	72.25	71.78	72.01	0.22	1.13
1.08	72.24	71.59	71.92	0.22	1.13
1.13	74.45	73.01	73.73	0.23	1.13
1.18	72.18	71.57	71.87	0.22	1.13
1.23	72.35	71.85	72.10	0.22	1.13
1.28	72.32	71.80	72.06	0.22	1.13
1.33	72.43	71.88	72.16	0.22	1.13
1.38	72.40 72.45	71.94 71.77	72.17 72.11	0.22 0.22	1.13
1.43	74.04	72.75	73.39	0.22	1.13 1.13
1.53	72.48	71.93	72.20	0.22	1.13
1.57	72.23	71.72	71.98	0.22	1.13
1.62	72.36	71.82	72.09	0.22	1.13
1.67	72.39	71.67	72.03	0.22	1.13
1.72	74.18	72.79	73.49	0.22	1.13
1.77	72.27	71.67	71.97	0.22	1.13
1.82	72.40	71.81	72.11	0.22	1.13
1.87 1.92	72.25 74.16	71.74 72.91	71.99 73.54	0.22 0.23	1.13 1.13
1.97	72.37	71.83	72.10	0.22	1.13
2.02	72.34	71.88	72.11	0.22	1.13
2.07	72.46	71.71	72.08	0.22	1.13
2.12	72.36	71.79	72.07	0.22	1.13
2.16	72.38	71.83	72.11	0.22	1.13
2.21	72.40	71.78	72.09	0.22	1.13
2.26	72.40	71.77	72.08	0.22	1.13
2.31 2.36	72.48 72.47	71.67 71.65	72.08 72.06	0.22 0.22	1.13 1.13
2.41	72.47	71.71	72.00	0.22	1.13
2.46	72.37	71.96	72.16	0.22	1.13
2.51	72.32	71.83	72.08	0.22	1.13
2.56	74.32	72.84	73.58	0.23	1.13
2.61	72.44	71.74	72.09	0.22	1.13
2.66	72.44	71.76	72.10	0.22	1.13
2.71	72.40	71.81	72.11	0.22	1.13
2.76 2.80	72.29	71.69 71.73	71.99	0.22 0.22	1.13
2.80	72.42 72.39	71.73 71.73	72.08 72.06	0.22	1.13 1.13
2.90	74.41	73.02	73.71	0.23	1.13
2.95	72.31	71.92	72.11	0.22	1.13
3.00	74.36	73.15	73.76	0.23	1.13
3.05	72.27	71.74	72.00	0.22	1.13
3.10	72.26	71.72	71.99	0.22	1.13
3.15	72.43	71.70	72.07	0.22	1.13
3.20	72.26	71.60	71.93	0.22	1.13
3.25	72.46 72.37	71.72 71.74	72.09 72.05	0.22 0.22	1.13 1.13
3.35	74.31	72.89	73.60	0.22	1.13
3.40	72.29	71.75	72.02	0.22	1.13
		Attension e	xperiment report		·

Attension [Together with Biolin Scientific]							
3.44	72.27	71.72	72.00	0.22	1.13		
3.49	72.25	71.79	72.02	0.22	1.13		
3.54	73.59	72.61	73.10	0.22	1.13		
3.59	72.26	71.73	72.00	0.22	1.13		
3.64	74.22	72.84	73.53	0.23	1.13		
3.69	72.47	71.84	72.15	0.22	1.13		
3.74	72.42	71.83	72.12	0.22	1.13		
3.79	74.50	72.90	73.70	0.22	1.13		
3.84	72.37	71.75	72.06	0.22	1.13		
3.89	74.43	73.00	73.71	0.23	1.13		
3.94	72.25	71.77	72.01	0.22	1.13		
3.99	72.40	71.97	72.18	0.22	1.13		
4.03	72.27	71.59	71.93	0.22	1.13		
4.08	72.44	71.78	72.11	0.22	1.13		
4.13	74.15	72.82	73.49	0.22	1.13		
4.18	72.44	71.89	72.16	0.22	1.13		
4.23	73.91	72.69	73.30	0.23	1.13		
4.28	72.34	71.85	72.10	0.22	1.13		
4.33	72.35	71.70	72.03	0.22	1.13		
4.38	72.24	71.74	71.99	0.22	1.13		
4.43	72.26	71.76	72.01	0.22	1.13		
4.48	73.88	72.64	73.26	0.23	1.13		
4.53	72.25	71.93	72.09	0.22	1.13		
4.58	72.32	71.78	72.05	0.22	1.13		
4.63	72.26	71.66	71.96	0.22	1.13		
4.67	72.35	71.57	71.96	0.22	1.13		
4.72	74.44	72.91	73.67	0.22	1.13		
4.77	72.36	71.72	72.04	0.22	1.13		
4.82	72.39	71.61	72.00	0.21	1.13		
4.87	72.31	71.68	71.99	0.21	1.13		
4.92	72.19	71.93	72.06	0.22	1.13		
4.97	72.07	71.97	72.02	0.22	1.13		
5.02	72.22	71.76	71.99	0.22	1.13		
5.07	72.39	71.65	72.02	0.21	1.13		
5.12	72.38	71.73	72.06	0.22	1.13		
5.17	72.18	71.75	71.96	0.22	1.13		
5.22	71.87	71.07	71.47	0.21	1.12		
5.26	72.37	71.57	71.97	0.22	1.13		
5.31	72.32	71.62	71.97	0.22	1.13		
5.36	72.36	71.72	72.04	0.22	1.13		
5.41	72.50	72.37	72.44	0.22	1.13		
5.46 5.51	72.22 72.35	71.50 71.74	71.86 72.05	0.22 0.22	1.13 1.13		
5.56	72.35	71.74	72.05	0.22	1.13		
5.61	74.17	72.96	73.57	0.23	1.13		
5.66	72.19	72.96	71.96	0.23	1.13		
5.71	72.19	71.74	71.98	0.22	1.13		
5.76	72.23	71.62	71.96	0.22	1.13		
5.81	72.38	71.73	72.06	0.22	1.13		
5.86	72.25	71.73	71.98	0.22	1.13		
10.00	, 2 . 2 9	, _ • , _	, = • > 0	V • Z Z	±•±9		