


a Calibration at 60 min



b Calibration at 120 min

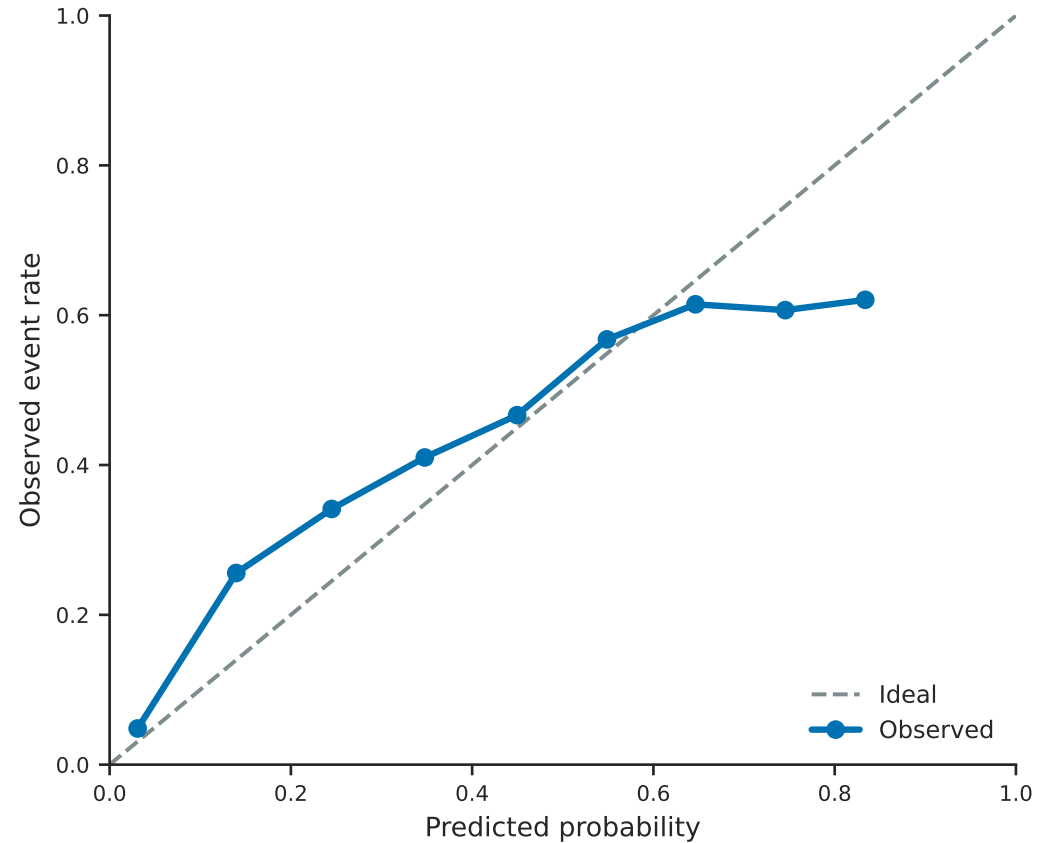