


RQ3: paired cost of zeroing each signal

Positive means removing the signal cost accuracy. 4 of 4 intervals include zero (ringed on the zero line), so no ablation is conclusive.

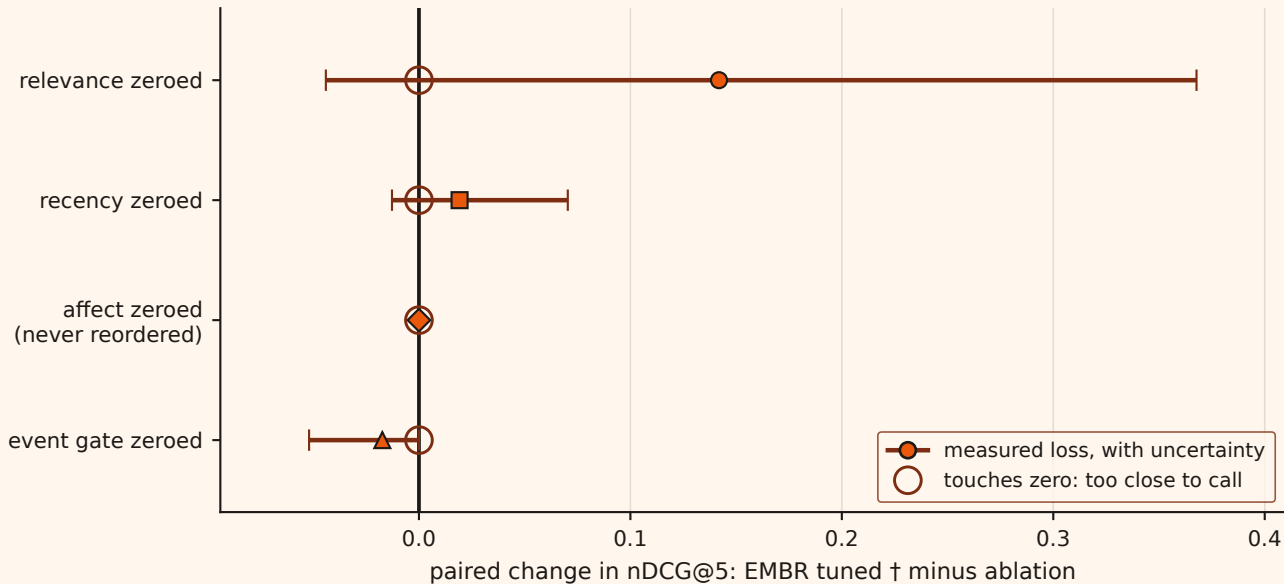

right of zero = zeroing the signal cost accuracy