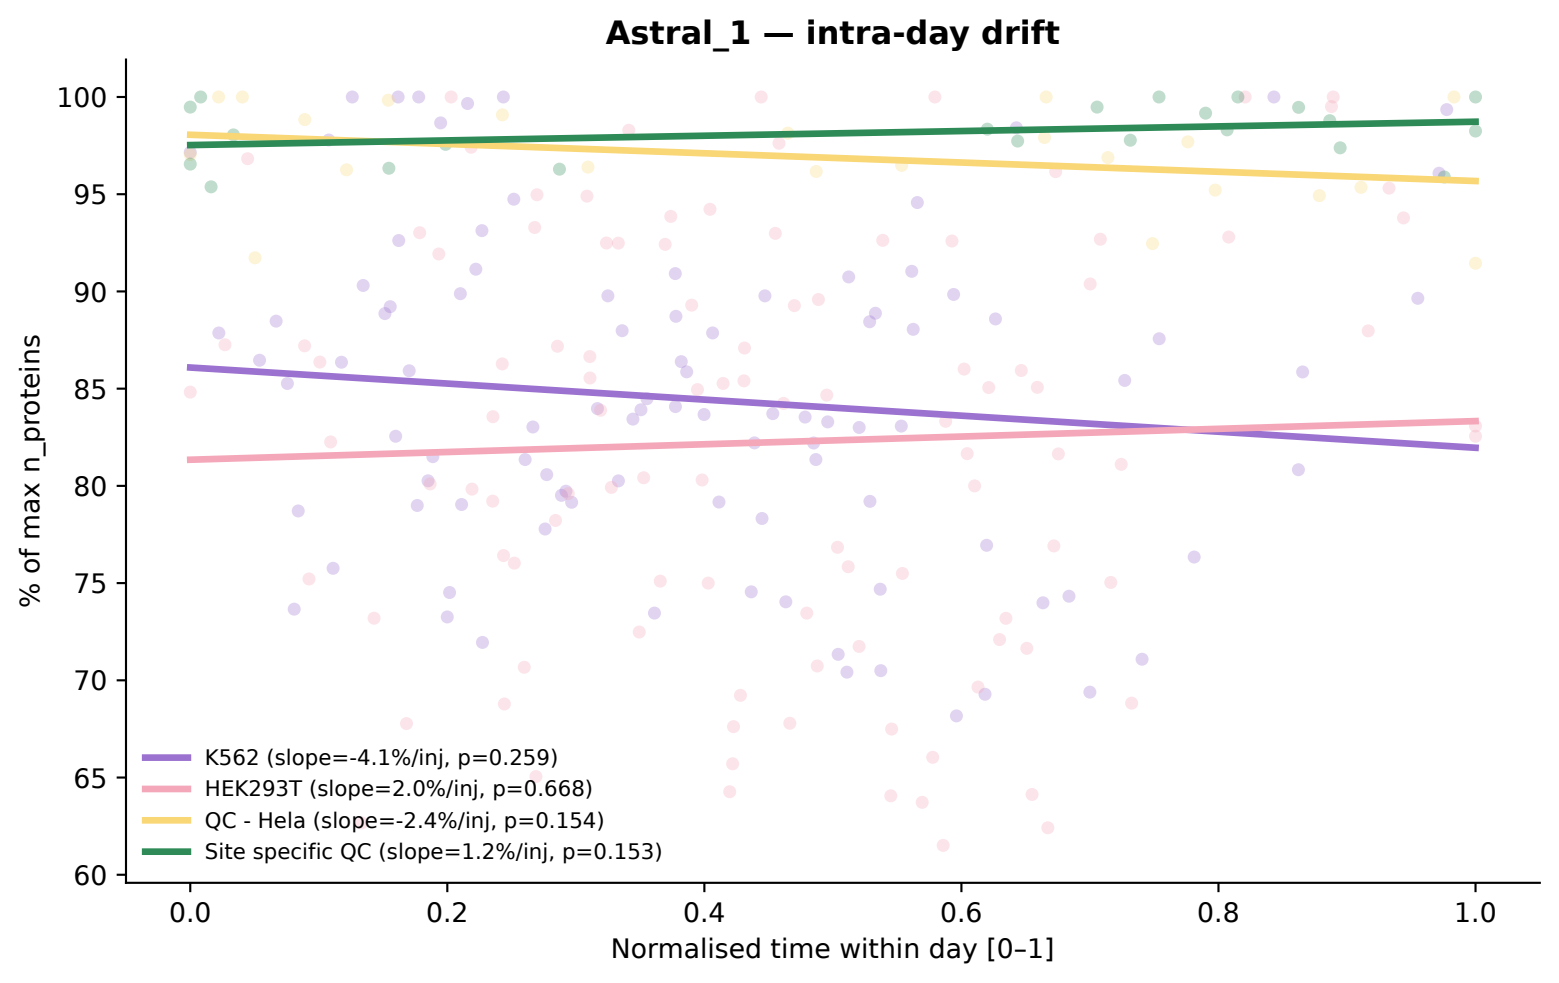
Astral_1 — intra-day drift
% of max n_proteins
Normalised time within day [0–1]
K562 (slope=-4.1%/inj, p=0.259)
HEK293T (slope=2.0%/inj, p=0.668)
QC - Hela (slope=-2.4%/inj, p=0.154)
Site specific QC (slope=1.2%/inj, p=0.153)